



BSI Standards Publication

Fine ceramics (advanced ceramics, advanced technical ceramics) — Light source for testing semiconducting photocatalytic materials used under indoor lighting environment

National foreword

This British Standard is the UK implementation of ISO 14605:2013.

The UK participation in its preparation was entrusted to Technical Committee RPI/13, Advanced technical ceramics.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2013. Published by BSI Standards Limited 2013

ISBN 978 0 580 69621 3

ICS 81.060.30

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 October 2013.

Amendments issued since publication

| Date | Text affected |
|------|---------------|
|------|---------------|

**Fine ceramics (advanced ceramics,
advanced technical ceramics) — Light
source for testing semiconducting
photocatalytic materials used under
indoor lighting environment**

*Céramiques techniques — Sources lumineuses destinées aux
essais des matériaux photocatalytiques semi-conducteurs dans un
environnement d'éclairage intérieur*





COPYRIGHT PROTECTED DOCUMENT

© ISO 2013

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

| | Page |
|---|----------|
| Foreword | iv |
| 1 Scope | 1 |
| 2 Normative references | 1 |
| 3 Terms and definitions | 1 |
| 4 Light source | 4 |
| 4.1 General | 4 |
| 4.2 Fluorescent lamps | 4 |
| 5 UV sharp cut-off filters | 5 |
| 6 Illuminance meters | 6 |
| 7 UV radiometers | 6 |
| 8 Indoor lighting conditions and selection of UV sharp cut-off filters | 6 |
| 9 Measurement and use conditions | 7 |
| 10 Test report | 7 |

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2. www.iso.org/directives

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received. www.iso.org/patents

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

The committee responsible for this document is ISO/TC 206, *Fine ceramics*.

Fine ceramics (advanced ceramics, advanced technical ceramics) — Light source for testing semiconducting photocatalytic materials used under indoor lighting environment

1 Scope

This International Standard specifies the light source and radiometer used in the performance evaluation of semiconducting photocatalytic materials used under an indoor lighting environment in a laboratory. A light source of an indoor lighting environment does not include the sunlight passing through the window glass.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 10677, *Fine ceramics (advanced ceramics, advanced technical ceramics) — Ultraviolet light source for testing semiconducting photocatalytic materials*

IEC 60081, *Double-capped fluorescent lamps — Performance specification*

CIE 13.3:1995, *Method of measuring and specifying colour rendering properties of light sources*

IEC 60050-845: 1987, *International electrotechnical vocabulary, Lighting*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

photocatalyst

substance that carries out many functions based on oxidization and reduction reactions under optical irradiation, including decomposition and removal of air and water contaminants, deodorization, and antibacterial, antifungal, self-cleaning and antifogging actions

3.2

indoor light-active photocatalyst

substance that carries out many functions based on oxidization and reduction reactions produced by artificial light sources for general lighting service, including decomposition and removal of air and water contaminants, deodorization, and antibacterial, antifungal, self-cleaning and antifogging actions

3.3

indoor lighting environment

indoor lighting environment with artificial light sources for general lighting service that does not include sunlight

3.4 **correlated colour temperature**

the temperature of the Planckian radiator whose perceived colour most closely resembles that of a given stimulus at the same brightness and under specified viewing conditions

Note 1 to entry: The correlated colour temperature is expressed in kelvins (K).

Note 2 to entry: The recommended method of calculating the correlated colour temperature of a stimulus is to determine on a chromaticity diagram the temperature corresponding to the point on the Planckian locus that is intersected by the agreed isotherm line containing the point representing the stimulus.

Note 3 to entry: Reciprocal correlated colour temperature is used rather than reciprocal colour temperature whenever correlated colour temperature is appropriate.

[SOURCE: IEC 60050-845: 1987, definition 845-03-50]

3.5 **colour rendering index**

measure of the degree to which the psychophysical colour of an object illuminated by the test illuminant conforms to that of the same object illuminated by the reference illuminant, suitable allowance having been made for the state of chromatic adaptation

[SOURCE: IEC 60050-845: 1987, definition 845-02-61]

3.6 **CIE 1974 general colour rendering index**

Ra
mean of the CIE 1974 special colour rendering indices for a specified set of eight test colour samples

[SOURCE: IEC 60050-845: 1987, definition 845-02-63]

3.7 **high transmission region**

HTR
wavelength region for which transmittance of a UV sharp cut-off filter is larger than 72 %; it is one of the performance descriptions for UV sharp cut-off filters

Note 1 to entry: See Key A in [Figure 1](#).

3.8 **threshold limit wavelength of high transmission**

TLH
wavelength for which transmittance of a UV sharp cut-off filter is 72 %; it is one of the performance descriptions for UV sharp cut-off filters

Note 1 to entry: See Key B in [Figure 1](#).

3.9 **absorption region**

AR
wavelength region for which transmittance of a UV sharp cut-off filter is less than 5 %; it is one of the performance descriptions for UV sharp cut-off filters

Note 1 to entry: See Key C in [Figure 1](#).

3.10 **threshold limit wavelength of absorption**

TLA
wavelength for which transmittance of a UV sharp cut-off filter is 5 %; it is one of the performance descriptions for UV sharp cut-off filters

Note 1 to entry: See Key D in [Figure 1](#).

3.11
range of slope
RoS


wavelength difference between the threshold limit wavelength of high transmission (TLH) and that of absorption (TLA); it is one of the performance descriptions for UV sharp cut-off filters

Note 1 to entry: See Key E in [Figure 1](#).

3.12
threshold limit wavelength of transmission
TLT

middle wavelength of the threshold limit wavelength of high transmission (TLH) and threshold limit wavelength of absorption (TLA); it is one of the performance descriptions for UV sharp cut-off filters

Note 1 to entry: See Key F in [Figure 1](#).

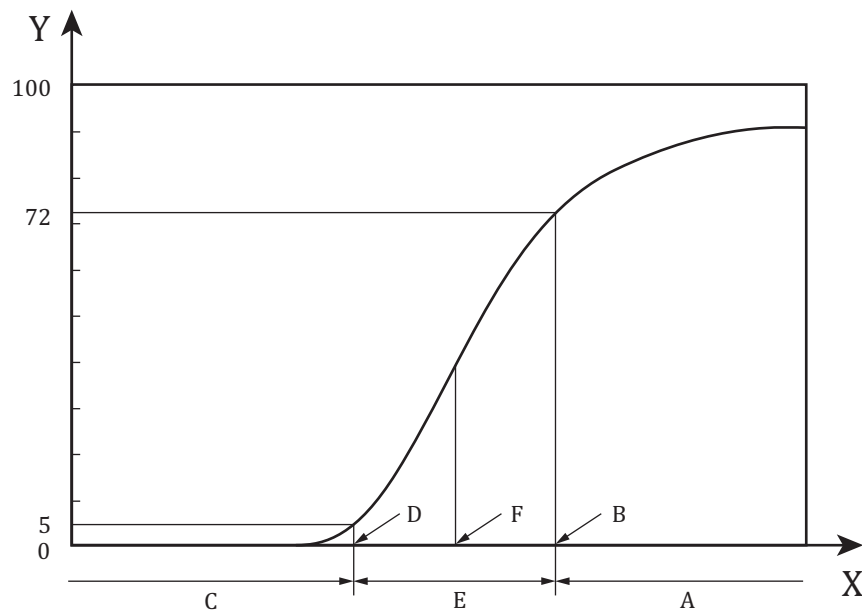

Key

- X wavelength, nm
- Y transmittance, %
- A high transmission region (HTR)
- B threshold limit wavelength of high transmission (TLH)
- C absorption region (AR)
- D threshold limit wavelength of absorption (TLA)
- E range of slope (RoS)
- F threshold limit wavelength of transmission (TLT)

Figure 1 — Definitions of UV sharp cut-off filters


4 Light source

4.1 General

For evaluation of indoor light-active photocatalysts, the light source that is a combination of one of the lamps described below and an ultraviolet (UV) sharp cut-off filter shall be used.

4.2 Fluorescent lamps


A halophosphate or triphosphor fluorescent lamp that a correlated colour temperature is between 3800 K to 4500 K (F4000) shall be used for testing of indoor light-active photocatalytic materials used under an indoor lighting environment without sunlight. The CIE 1974 general colour rendering index (Ra) defined by CIE 13.3 of halophosphate fluorescent lamp is about 60. When a triphosphor fluorescent lamp is used for testing, the fluorescent lamp which Ra is higher than 80 shall be selected. Performance specifications of fluorescent lamps are specified in IEC 60081. A typical relative spectral power distribution of the halophosphate fluorescent lamp is shown in [Figure 2](#), and triphosphor one is shown in [Figure 3](#) respectively.

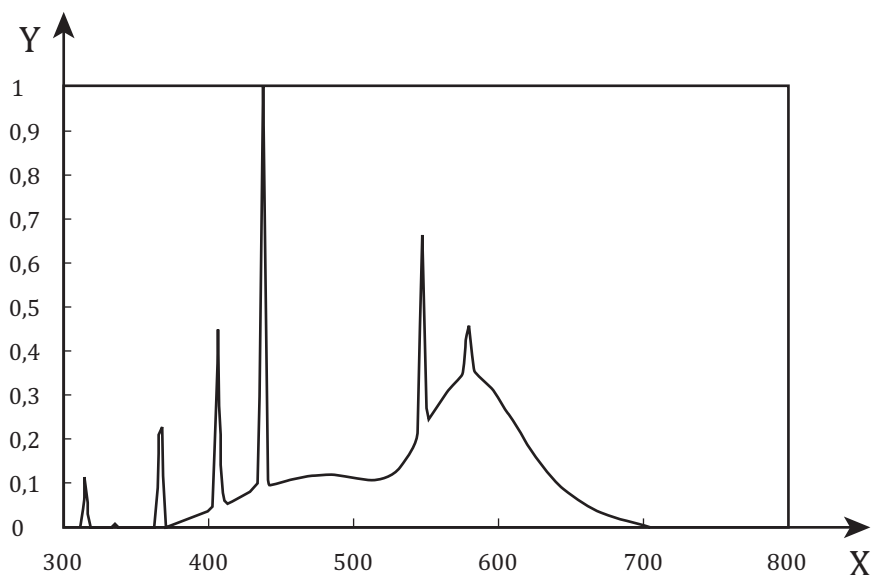

Key

- X wavelength, nm
- Y relative radiant power

Figure 2 — A typical spectral power distribution of a halophosphate fluorescent lamp in which a correlated colour temperature is 4100 K and CIE 1974 general colour rendering index is 60

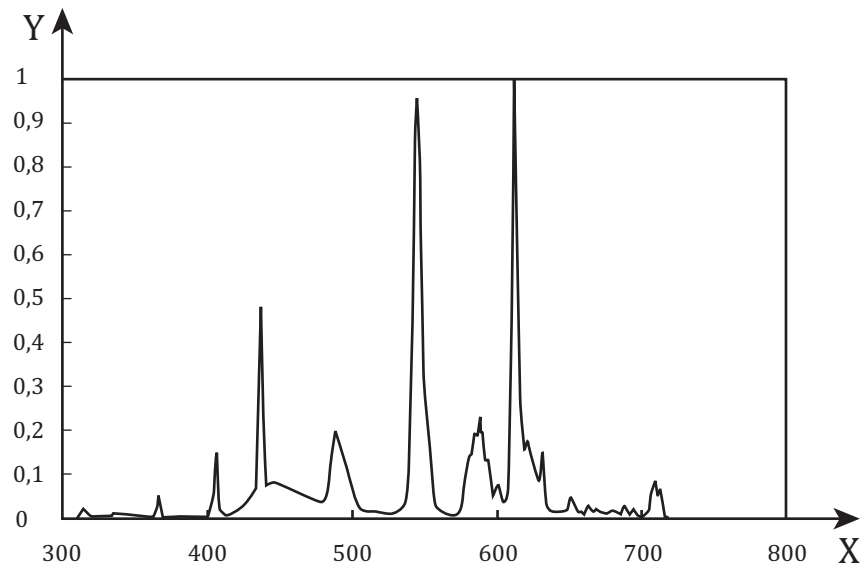

Key

X wavelength, nm


Y relative radiant power

Figure 3 — A typical spectral power distribution of a triphosphor fluorescent lamp in which a correlated colour temperature is 4288 K and CIE 1974 general colour rendering index is 80

5 UV sharp cut-off filters

Two types of UV sharp cut-off filters shall be used for testing.

A transmittance of first one is 0.1 % or less at 400 nm, threshold limit wavelength of transmission (TLT) is $416 \text{ nm} \pm 5 \text{ nm}$, range of slope (RoS) is $14 \text{ nm} \pm 5 \text{ nm}$ and average transmittance between 450 nm to 780 nm is higher than 80 % (Type A). And a transmittance of the other one is 0.1 % or less at 380 nm, threshold limit wavelength of transmission (TLT) is $392 \text{ nm} \pm 5 \text{ nm}$, range of slope (RoS) is $14 \text{ nm} \pm 5 \text{ nm}$ and average transmittance between 420 nm to 780 nm is higher than 80 % (Type B). Examples of spectral transmittance of UV sharp cut-off filters are shown in [Figure 4](#). When using the filter of different transmittance from this standard for testing, spectral transmittance shall be reported with a product name, product number, manufacturer, and thickness.

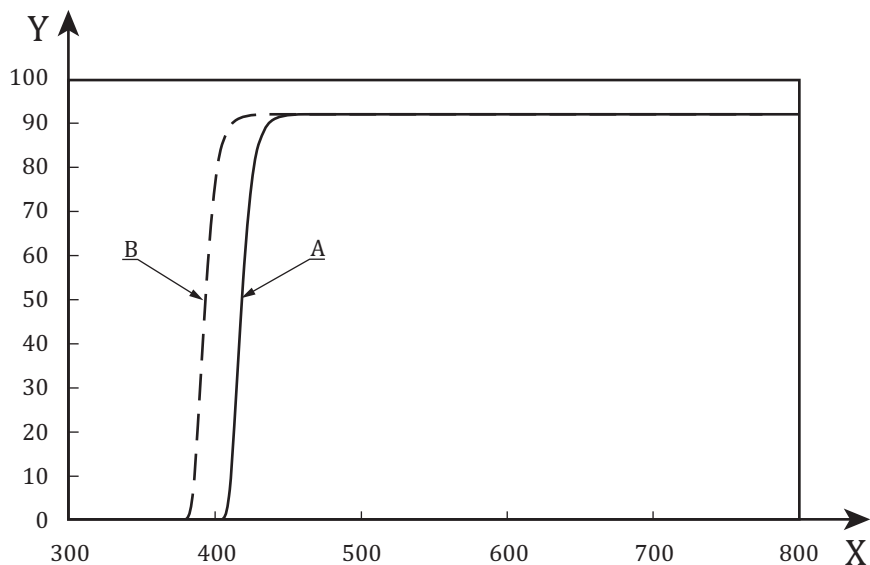

Key

- X wavelength, nm
- Y transmittance, %
- A Type A
- B Type B

Figure 4 — Examples of spectral transmittance of UV sharp cut-off filters

6 Illuminance meters

The irradiance shall be measured in illuminance (lx) by using an illuminance meter that has been calibrated by a calibration laboratory and traceability with the national standard has been maintained.

7 UV radiometers

The UV irradiance shall be measured in irradiance (W/m^2 or mW/cm^2) by using a UV radiometer specified in ISO 10677.

8 Indoor lighting conditions and selection of UV sharp cut-off filters

To set three kinds of indoor lighting conditions (condition A, condition B, condition C), the method of selecting the UV sharp cut-off filter is defined.

Condition A

Condition A is an indoor lighting condition by luminaire with cover that transmits optical radiation longer wavelength than 400 nm. In this condition, the type A filter shall be used.

Condition B

Condition B is an indoor lighting condition by luminaire with cover that transmits optical radiation longer wavelength than 380 nm. In this condition, the type B filter shall be used.

Condition C

Condition C is an indoor lighting condition by luminaire without cover. When evaluating this condition, the UV sharp cut-off filter is not needed in general. However, in general, a fluorescent lamp for general lighting service emits very small UV radiation and large amount of visible radiation, and photocatalytic responsivity in UV range is higher than that in visible range. It is necessary to separate UV effects and the visible one. Therefore, to evaluate true performance produced by only visible radiation, performance evaluation by combination of the UV sharp cut-off filter and the light source shall be done together. The type of filter is defined by each application.

9 Measurement and use conditions

- a) The illuminance shall be measured with and without a UV sharp cut-off filter, along with the UV irradiance. The illuminance for testing shall be set as a standard value specified in each standard.
- b) The illuminance and UV irradiance shall be measured at stabilized condition, which is a minimum of 15 min after the light is turned on.
- c) The illuminance and UV irradiance shall be measured at start and end of the testing. The lamp shall be replaced when the illuminance has decreased to 70 % of the initial value.
- d) If a luminaire with a reflection plate is used for testing, the reflection plate shall be shown small absorption in ultraviolet and visible radiation.
- e) The transmittance of the UV sharp cut-off filter might be changed by long time irradiation. Therefore, transmittance of the filter shall be measured periodically or the filter shall be replaced periodically.
- f) If an acrylic sharp cut-off filter is used, the shape of the filter might be transformed by the long time irradiation. In this case, before switching the lighting on, the shape of the filter shall be checked.

10 Test report

The test report shall include at least the following information:

- a) a reference to this International Standard: ISO 14605:2013;
- b) kind of lamp used (catalogue number, manufacturer, emission data of the lamp);
- c) kind of filter used (catalogue number, manufacturer, thickness, transmission data of the filter);
- d) kind of illuminance meter and UV radiometer used in the measurement (catalogue number, manufacturer);
- e) illuminance and UV irradiance with and without UV sharp cut-off filter at the samples surface.

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email bsmusales@bsigroup.com.

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

Useful Contacts:

Customer Services

Tel: +44 845 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 845 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com



...making excellence a habit.™