

BS ISO 17218:2014



BSI Standards Publication

# Sterile acupuncture needles for single use

**bsi.**

...making excellence a habit.™

**National foreword**

This British Standard is the UK implementation of ISO 17218:2014.

The UK participation in its preparation was entrusted to Technical Committee CH/100, Healthcare and medical equipment (European and International).

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2014.

Published by BSI Standards Limited 2014

ISBN 978 0 580 78013 4

ICS 11.040.25

**Compliance with a British Standard cannot confer immunity from legal obligations.**

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 May 2014.

**Amendments/corrigenda issued since publication**

Date	Text affected
------	---------------

---

INTERNATIONAL  
STANDARD

**ISO**  
**17218**

First edition  
2014-02-01

---

---

**Sterile acupuncture needles for single  
use**

*Aiguilles d'acupuncture stériles à usage unique*



Reference number  
ISO 17218:2014(E)



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2014

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

<b>Foreword</b> .....	<b>iv</b>
<b>Introduction</b> .....	<b>v</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Configuration</b> .....	<b>2</b>
4.1 Acupuncture needle configuration.....	2
4.2 Acupuncture needle types.....	2
4.3 Types of needle handles.....	3
<b>5 Requirements</b> .....	<b>5</b>
5.1 Materials.....	5
5.2 Dimensions.....	5
5.3 Performance requirements.....	7
5.4 Sterility assurance.....	9
<b>6 Package</b> .....	<b>9</b>
6.1 Primary package.....	9
6.2 Secondary package.....	10
<b>7 Labelling</b> .....	<b>10</b>
7.1 General.....	10
7.2 Primary package.....	10
7.3 Secondary package.....	10
<b>8 Transit and storage</b> .....	<b>11</b>
<b>Annex A (informative) Test methods for the intensity and sharpness of the tip of the needle</b> .....	<b>12</b>
<b>Annex B (informative) Test methods for the puncture performance of the tip of the needle</b> .....	<b>16</b>
<b>Annex C (informative) Test method for resistance to corrosion</b> .....	<b>21</b>
<b>Bibliography</b> .....	<b>23</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: Foreword - Supplementary information

The committee responsible for this document is ISO/TC 249, *Traditional Chinese medicine*.

## Introduction

This International Standard applies to sterile acupuncture needles for single use (specialized for filiform needles) used by professional acupuncturists for acupuncture treatment. Sterile acupuncture needles for single use are sterilized by the manufacturer, and the healthcare professional can open the sealed package and use the needle immediately.

In order to encourage innovation, this International Standard does not enforce the combination of the needle diameter and length. However, considering the clinical usage requirements, the standard provides the specifications for the needle diameter and length.

The sharpness and puncture performance of the needle tip are of very important clinical significance. [Annex A](#) states the guidelines and the evaluation methods for the intensity and the sharpness of the needle tip, while [Annex B](#) provides two qualitative and quantitative evaluation methods to determine the puncture performance of the needle tip.

The qualitative methods to evaluate the puncture performance of needle tip are described in [Annex B](#). The methods are simple, direct and practical. It makes them especially suitable for routine inspection and for cross-comparison of the acupuncture needles' clinical applications. They also play a very important role in the enhancement of the quality of the needle tip. The methods to evaluate the puncture performance of the needle tip can be used to further evaluate the puncture and puncture performance of the acupuncture needle. Currently, the more appropriate method is to use the needle tip to pierce through polyurethane material; however, this method has not yet been implemented internationally.

Considering the consistency of standards in the future, this standard provides the methods to evaluate the puncture performance of the needle tip and ranks [5.3.5.2](#) as recommended. The standard does not provide the sharpness index of the piercing through polyurethane material by the needle tip. This index will be added to the standard when it becomes appropriate. To improve product quality, all inspection reports should include the inspection information as well as the results of the performance evaluation.

Since every manufacturer's design, production, and sterilization methods are different, no regulations exist for the materials of the acupuncture needle handle. Still, the needle body and the needle handle of acupuncture needle should have good biocompatibility.

In order to ensure product safety and efficacy, the manufacturer should perform risk analysis and enforce risk management in addition to adhering to the requirements of local rules and regulations, the relevant background data of the medical devices and clinical practice throughout the entire duration of the product's life cycle. ISO 14971 has provided manufacturers a framework for the effective management of hazards associated with the use of medical devices.

In some countries, the requirements proposed here are subject to legal sanctions. Such rules and regulations should take precedence over the standards set forth in this document.





# Sterile acupuncture needles for single use

## 1 Scope

This International Standard specifies the requirements for the sterile acupuncture needles for single use (specialized for filiform needles).

## 2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 6507-1:2005, *Metallic materials — Vickers hardness test — Part 1: Test method*

ISO 10993-1, *Biological evaluation of medical devices — Part 1: Evaluation and testing within a risk management process*

ISO 15223-1, *Medical devices — Symbols to be used with medical device labels, labelling and information to be supplied — Part 1: General requirements*

## 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

### 3.1

#### **body of the needle**

part of the acupuncture needle that is inserted into the human body

Note 1 to entry: See [Figure 1](#).

### 3.2

#### **handle of the needle**

part of the acupuncture needle that is not inserted into the human body

Note 1 to entry: See [Figure 1](#).

### 3.3

#### **tip of the needle**

sharp apex at the end of the acupuncture needle body that is inserted into the human body

Note 1 to entry: See [Figure 1](#).

### 3.4

#### **root of the needle**

part of the acupuncture needle that connects the needle body to the needle handle

Note 1 to entry: See [Figure 1](#).

### 3.5

#### **tail of the needle**

end part of the needle handle at the opposite side of the tip of the needle

Note 1 to entry: See [Figure 1](#).

**3.6 sterile acupuncture needle**  
acupuncture needle that has been sterilized

**3.7 guide tube**  
assistant tool in the shape of a slender, long tube into which the needle is placed and used for easy insertion

**3.8 hardness of the needle body**  
measure of resistance of the acupuncture needle body to permanent deformation

**3.9 primary package**  
sealed or closed packaging system that forms a microbial barrier, directly enclosing the acupuncture needle


Note 1 to entry: The primary package is usually the smallest unit package of use and the package that is in direct contact with one or more acupuncture needles.

**3.10 secondary package**  
package containing one or more primary packages for distribution and storage

## 4 Configuration

### 4.1 Acupuncture needle configuration

The configuration of the acupuncture needle and the name of each of its parts are shown in [Figure 1](#).

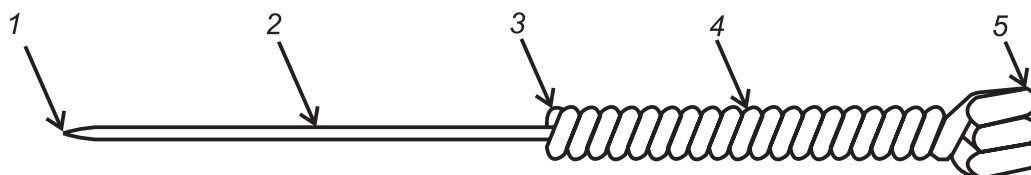

#### Key

- 1 tip of the needle
- 2 body of the needle
- 3 root of the needle
- 4 handle of the needle
- 5 tail of the needle


**Figure 1 — Example of typical structure of acupuncture needle**

### 4.2 Acupuncture needle types

The acupuncture needle includes two types:

- acupuncture needle with a guide tube; and
- acupuncture needle without a guide tube.

The acupuncture needle with guide tube is shown in [Figure 2](#). However, no uniform requirement is provided for the fixing method of the needle tube.

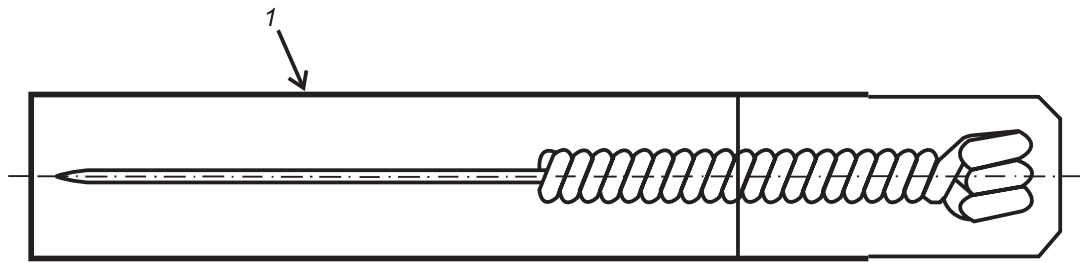


**Key**

1 guide tube

**Figure 2 — The acupuncture needle with a guide tube**

### 4.3 Types of needle handles

The types of needle handles include the ring handle, the plain handle, the flower handle, the metal tube handle, and the plastic handle, etc. The types of needle handles are not limited to those shown in the [Figure 3](#).

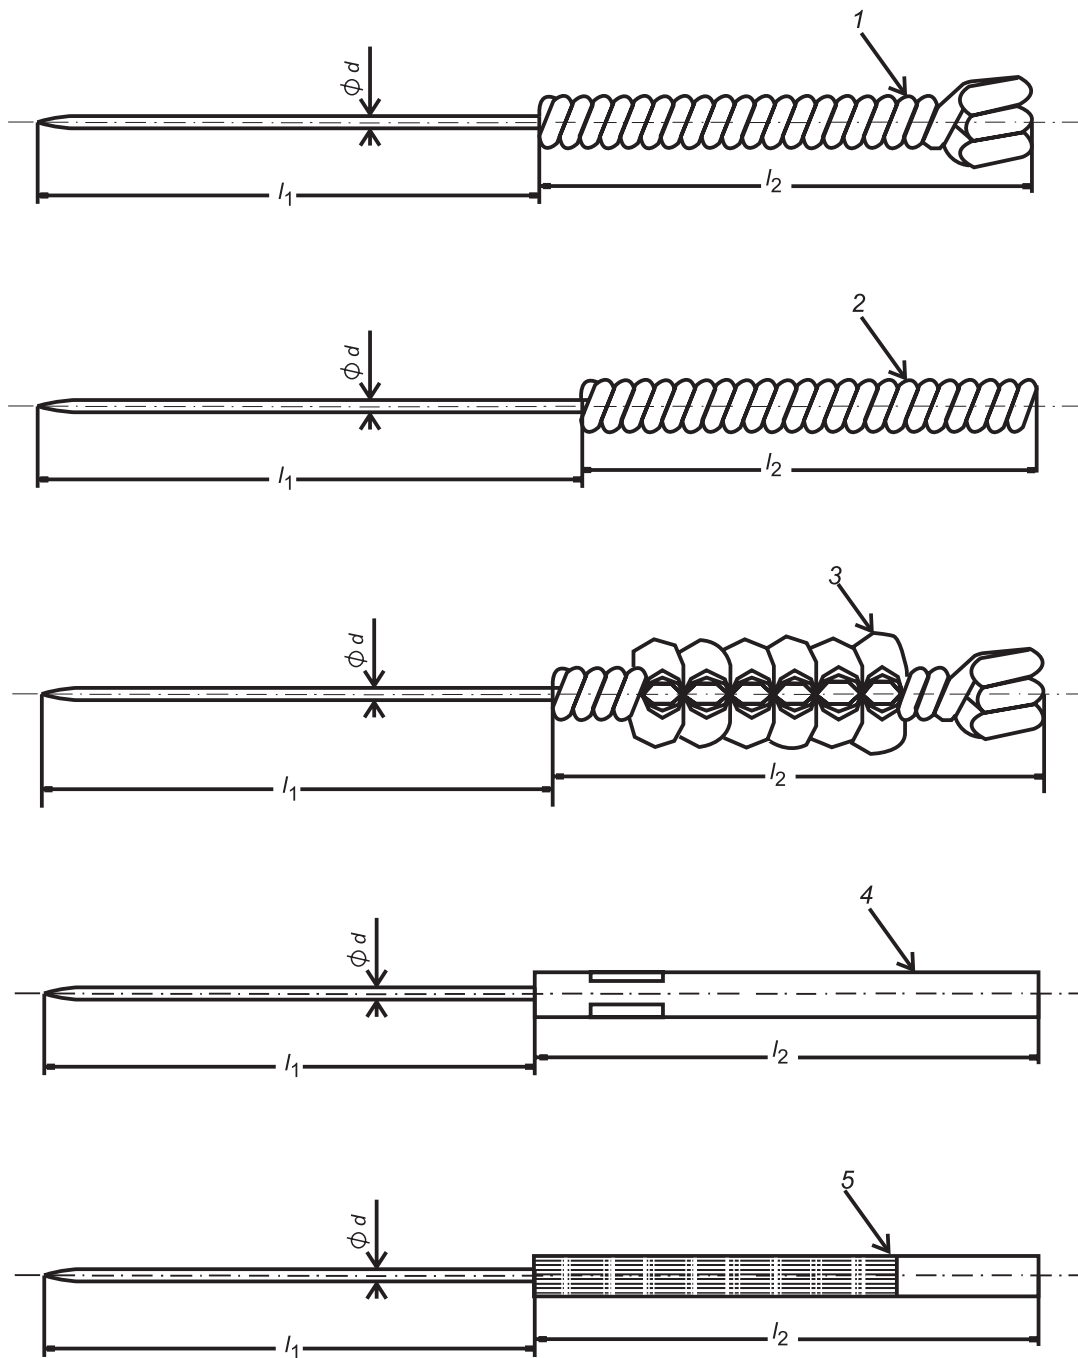

**Key**

- |   |                   |                 |                             |
|---|-------------------|-----------------|-----------------------------|
| 1 | ring handle       | $l_1$           | length of the needle body   |
| 2 | plain handle      | $l_2$           | length of the needle handle |
| 3 | flower handle     | $\varnothing d$ | diameter of the needle body |
| 4 | metal tube handle |                 |                             |
| 5 | plastic handle    |                 |                             |

**Figure 3 — Example of types of handles of acupuncture needles**

## 5 Requirements

### 5.1 Materials

The biocompatibility of the body of the needle shall be assessed and documented according to the guidance and principles given in ISO 10993-1.

Compliance is demonstrated by:

- a) analogy with published data; or
- b) the selection of materials already shown to be biocompatible by proven clinical use in a similar application; or
- c) experience with similar devices already on the market together with evidence of traceability to the materials used in the acupuncture needle; or
- d) compliance with published procedures for biological evaluation of:
  - 1) Cytotoxicity;
  - 2) Sensitization;
  - 3) Intracutaneous reactivity;
  - 4) Ethylene oxide sterilization residuals (if using EO. to sterilize).

If the material of the body of the needle is changed and/or if there is a new coating on the surface of the needle body, and if there is risk indicating that these may cause side-effects to the human body, then testing should be in accordance with ISO 10993 series.

NOTE There is no uniform regulation regarding materials of the needle handle and body. Currently, the popularly used material of the needle body is made of X5CrNi18-9, X7CrNi18-9 Austenite Stainless Steel, etc. which are given in ISO 15510:2010.

### 5.2 Dimensions

#### 5.2.1 Size designation

The size of the acupuncture needle shall be designated by the following:

- a) the nominal diameter of the body of acupuncture needle, expressed in millimetres; and
- b) the nominal length of the body of acupuncture needle, expressed in millimetres.

The size of acupuncture needle shall be referred to as “the designated metric size” and specified as the diameter of the needle body × the length of the needle body.

EXAMPLE Ø 0,30 × 40 mm

#### 5.2.2 Tolerance of dimensions

##### 5.2.2.1 Diameter of the needle body

When measured by a micrometer or similar equipment, the nominal diameter of the body of acupuncture needle shall comply with [Table 1](#).

**Table 1 — Nominal diameter of needle body**

Dimensions in millimetres

Nominal diameter of needle body <i>d</i>	Tolerance
$0,10 \leq d < 0,25$	$\pm 0,008$
$0,25 \leq d \leq 0,45$	$\pm 0,015$
$0,45 < d \leq 0,80$	$\pm 0,020$

**5.2.2.2 Length of body of the needle**

When measured by vernier calipers or similar equipment, the nominal length of the body of acupuncture needle shall comply with [Table 2](#).

**Table 2 — Nominal length of needle body**

Dimensions in millimetres

Nominal length of needle body <i>l</i> <sub>1</sub>	Tolerance
$5 \leq l_1 \leq 25$	$\pm 0,50$
$25 < l_1 \leq 60$	$\pm 1,00$
$60 < l_1 \leq 100$	$\pm 2,00$
$100 < l_1 \leq 200$	$\pm 3,00$

**5.2.3 Dimensions of needle handle**

The handle of acupuncture needles shall be of suitable diameter and length for the intended purpose or manipulation.

The length of the handle of acupuncture needles (*l*<sub>2</sub>) shall be no less than 13 mm.

The dimensions of the coiling handle wire used in the manufacturing of ring handles, plain handles and flower handles should comply with [Table 3](#). The diameter of the plastic handle and the metal tube handle should comply with [Table 4](#).

**Table 3 — Diameter of the coiling handle wire**

Dimensions in millimetres

Nominal diameter of needle body <i>d</i>	Diameter of the coiling handle wire
$0,10 \leq d < 0,20$	0,30
$0,20 \leq d < 0,30$	0,35
$0,30 \leq d < 0,40$	0,40
$0,40 \leq d < 0,50$	0,45
$0,50 \leq d \leq 0,80$	0,50

**Table 4 — Diameter of the plastic handle and the metal tube handle and coiling handle which are joined by other method than coiling around the needle body**

Dimensions in millimetres

Type of needle handle	Diameter of needle handle
Metal tube handle, Plastic handle, etc.	0,80 – 2,50
NOTE These diameters are only applicable to “Cylinder-shaped” handle.	

### 5.3 Performance requirements

#### 5.3.1 Appearance and cleanliness

5.3.1.1 When inspected by normal or corrected-to-normal vision:

- a) the surface of the acupuncture needles shall appear free from particles and extraneous matter;
- b) the body of the needle shall be straight and there shall be neither breakage nor unevenness; and
- c) the handle of needle shall not have any protuberances that could cause a scratch or cut, etc. If the handle of the needle is made of winding coils, the spiral loop should be arranged symmetrically without obvious gaps and the colour and lustre of the surface of the needle handle should be even. If the handle is plated, it shall not exhibit layering or shedding.

5.3.1.2 When examined under x 10 magnification:

- a) the body of the needle shall be straight and there shall be neither breakage nor unevenness;
- b) the body of the needle shall be smooth and clean:
  - 1) shall appear free from particles or extraneous matter produced during the metal processing course;
  - 2) shall not have any obvious defects such as ruggedness, scars, bends, grooves, rust or twist.
- c) the tip of needle shall be sharp-edged, polished sharply and has no deficiencies of scars, fringes, spikes or hooks.

If the body of the acupuncture needle is lubricated, the lubricant shall not be visible under normal or corrected-to-normal vision as droplets of fluid on the surface of the needle body.

#### 5.3.2 Drawing strength

The body of the needle shall be solidly joined to the handle of the needle at the root of the needle.

When the minimum static force given in [Table 5](#) is applied in the direction of the centre axis of the body of the needle depending on the nominal diameter of the body of the needle, it shall not be drawn out of the handle of the needle. Axial displacement of the handle of the needle from the body of the needle of more than 3 mm is not permitted.

**Table 5 — Force to test drawing strength**

Nominal diameter of needle body <i>d</i> mm	Force N
0,10	5
$0,10 < d \leq 0,16$	5,5
$0,16 < d \leq 0,20$	7
$0,20 < d \leq 0,25$	8
$0,25 < d \leq 0,35$	15
$0,35 < d \leq 0,45$	20
$0,45 < d \leq 0,55$	25
$0,55 < d \leq 0,80$	30

### 5.3.3 Hardness of the needle body

To assess the hardness test according to the requirements given in ISO 6507-1:2005 or other equivalent methods, the hardness of the body of the needle shall comply with [Table 6](#).

**Table 6 — Hardness of the needle body**

Nominal diameter of needle body <i>d</i> mm	Hardness HV <sub>0.2kg</sub>
$0,10 \leq d < 0,25$	$\geq 480, \leq 680$
$0,25 \leq d < 0,30$	$\geq 460, \leq 655$
$0,30 \leq d < 0,45$	$\geq 450, \leq 655$
$0,45 \leq d \leq 0,80$	$\geq 420, \leq 630$

The hardness can also be converted into tensile strength.

NOTE This hardness is only applicable to the stainless steel body of the needle.

### 5.3.4 Resistance to breakage of the needle body

The body of the needle shall be of sufficient resistance to breakage.

After a body of the needle is coiled tightly around a mandrel which diameter is 3 times larger than the needle body, the body of the needle shall be free from any crack, break or separation of layers. In case of a body of the needle no more than 15 mm in length, the needle body shall be tested by being coiled twice circles around the mandrel tightly and a body of the needle longer than 15 mm shall be coiled five circles.

### 5.3.5 Intensity and puncture performance of the needle tip

#### 5.3.5.1 General

The tip of the needle shall have good intensity and puncture performance.

#### 5.3.5.2 Intensity and sharpness of the needle tip

When tested in accordance with [Annex A](#), the tip of the needle shall have good intensity. The needle tips shall not have any hooks or bends after a set amount of pressure has been applied. The puncture force shall not exceed the values set forth in [Table 7](#). The other equivalent method is available.



**Table 7 — Pressure and puncture force**

Nominal diameter of needle body <i>d</i> mm	Pressure N	Puncture force N
$0,10 \leq d \leq 0,12$	0,2	0,5
$0,12 < d \leq 0,25$	0,4	0,7
$0,25 < d \leq 0,35$	0,5	0,8
$0,35 < d \leq 0,45$	0,6	0,9
$0,45 < d \leq 0,80$	0,7	1,0

### 5.3.5.3 Puncture performance of the needle tip

When tested in accordance with [Annex B](#), the tip of the needle should have good puncture performance. If the puncture force is low, this indicates that the needle tip is sharp. This can be selected for the performance of each manufacturer's needle tip.

### 5.3.6 Resistance to corrosion of the needle body

The body of the needle shall have good resistance to corrosion. If the conditions of storage have been met, there shall be no corrosion of the body of the needle before the expiry date.

When tested in accordance with [Annex C](#), the partially immersed body of the needle shall show no evidence of corrosion resulting from the test. [Annex C](#) shall be applied only to the stainless steel body of the needle.

## 5.4 Sterility assurance

Sterile acupuncture needles for single use shall be sterilized through a validated sterilization process in order to ensure that the products are sterile.

NOTE For appropriate sterilization methods, see Bibliography. The requirements for validation and routine control of a sterilization process for medical devices are provided in ISO 11135-1, ISO 11137-1 and ISO 17665-1.

## 6 Package

### 6.1 Primary package

Sterile acupuncture needle shall be sealed in a primary package. There shall be no foreign matter within the primary package under visual inspection.

The material and design of this primary package shall not have detrimental effects on the contents. The material and design of this primary package should be such as to ensure:

- a) the maintenance of sterility of the contents under dry, clean and adequately ventilated storage conditions;
- b) the minimum risk of contamination of the contents during removal from the package;
- c) adequate protection of the contents during normal handling, transit and storage; and
- d) that once opened, the package cannot be easily resealed, and it shall be obvious that the package has been opened.

NOTE The requirements of materials, sterile barrier systems and packaging systems for terminally sterilized medical devices are provided by ISO 11607-1.

## 6.2 Secondary package

One or more primary packages shall be packaged in a secondary package.

The secondary package shall be sufficiently robust to protect the contents during handling, transit and storage.

One or more secondary packages may be packaged in a storage or a transit package.

## 7 Labelling

### 7.1 General

The symbols to be used with medical device labels, labelling, and information to be supplied on the package shall comply with ISO 15223-1.

### 7.2 Primary package

The primary package shall be marked with at least the following information:

- a) the name or trade-mark or logo of the manufacturer and/or supplier;
- b) a description of the contents, including the designated metric size in accordance with [5.2](#);
- c) the lot number, prefixed by the word "LOT", and/or date of manufacture;
- d) expiry date;
- e) method of sterilization, the word "STERILE" or symbol;
- f) the words "For single use" or "Do not reuse" or symbol.

### 7.3 Secondary package

The secondary package shall be marked with at least the following information:

- a) the name, address and trademark of the manufacturer and/or supplier;
- b) description of the contents, including the designated metric size in accordance with [5.2](#), the quantity and the type;
- c) the lot number, prefixed by the word "LOT", and/or date of manufacture;
- d) expiry date;
- e) method of sterilization, the word "STERILE" or symbol;
- f) the words "For single use" or "Do not reuse" or symbol;
- g) if appropriate, the licensed certificate number according to the requirements of the regulations;
- h) information for handling, storage and transportation;
- i) a warning to check the integrity of each primary package before use, such as "Do not use if package is damaged" or symbol;
- j) a warning that excessive electrical stimulation may cause corrosion to needles;
- k) if used, the names or composition of additives (such as lubricant) used as a coating on the surface of needle body;

- l) if appropriate, indication that the needles are not for use in moxibustion if the handle of the needle cannot tolerate the heat from the burning of moxa; and
- m) if appropriate, those who are allergic to the material of the needle body should use with caution or follow the instruction of an acupuncture physician.

## **8 Transit and storage**

**8.1** The transport requirements should comply with the order contract.

**8.2** The acupuncture needles should have sufficient protection from damage. Once the acupuncture needles are packaged, they should be stored in a clean, well-ventilated and non-contaminated environment. The storage environment should have controls in place for humidity, temperature and exposure to direct sunlight.

## **Annex A** (informative)

### **Test methods for the intensity and sharpness of the tip of the needle**


#### **A.1 General**

The intensity of the tip of the needle: refers to the needle tip ability to resist breakage when thrust vertically on the steel block.

The sharpness of the tip of the needle: refers to the force required by the needle tip to vertically pierce aluminium foil.

#### **A.2 Apparatus for measuring**


**A.2.1** The typical apparatus for measuring the intensity and sharpness of the tip of the needle as shown in [Figure A.1](#) and [Figure A.2](#), they can also use the other equipment with the same performance, precision (including measuring amplifier installed on the equipment, data processing and display units, printers and floppy disks and other devices).

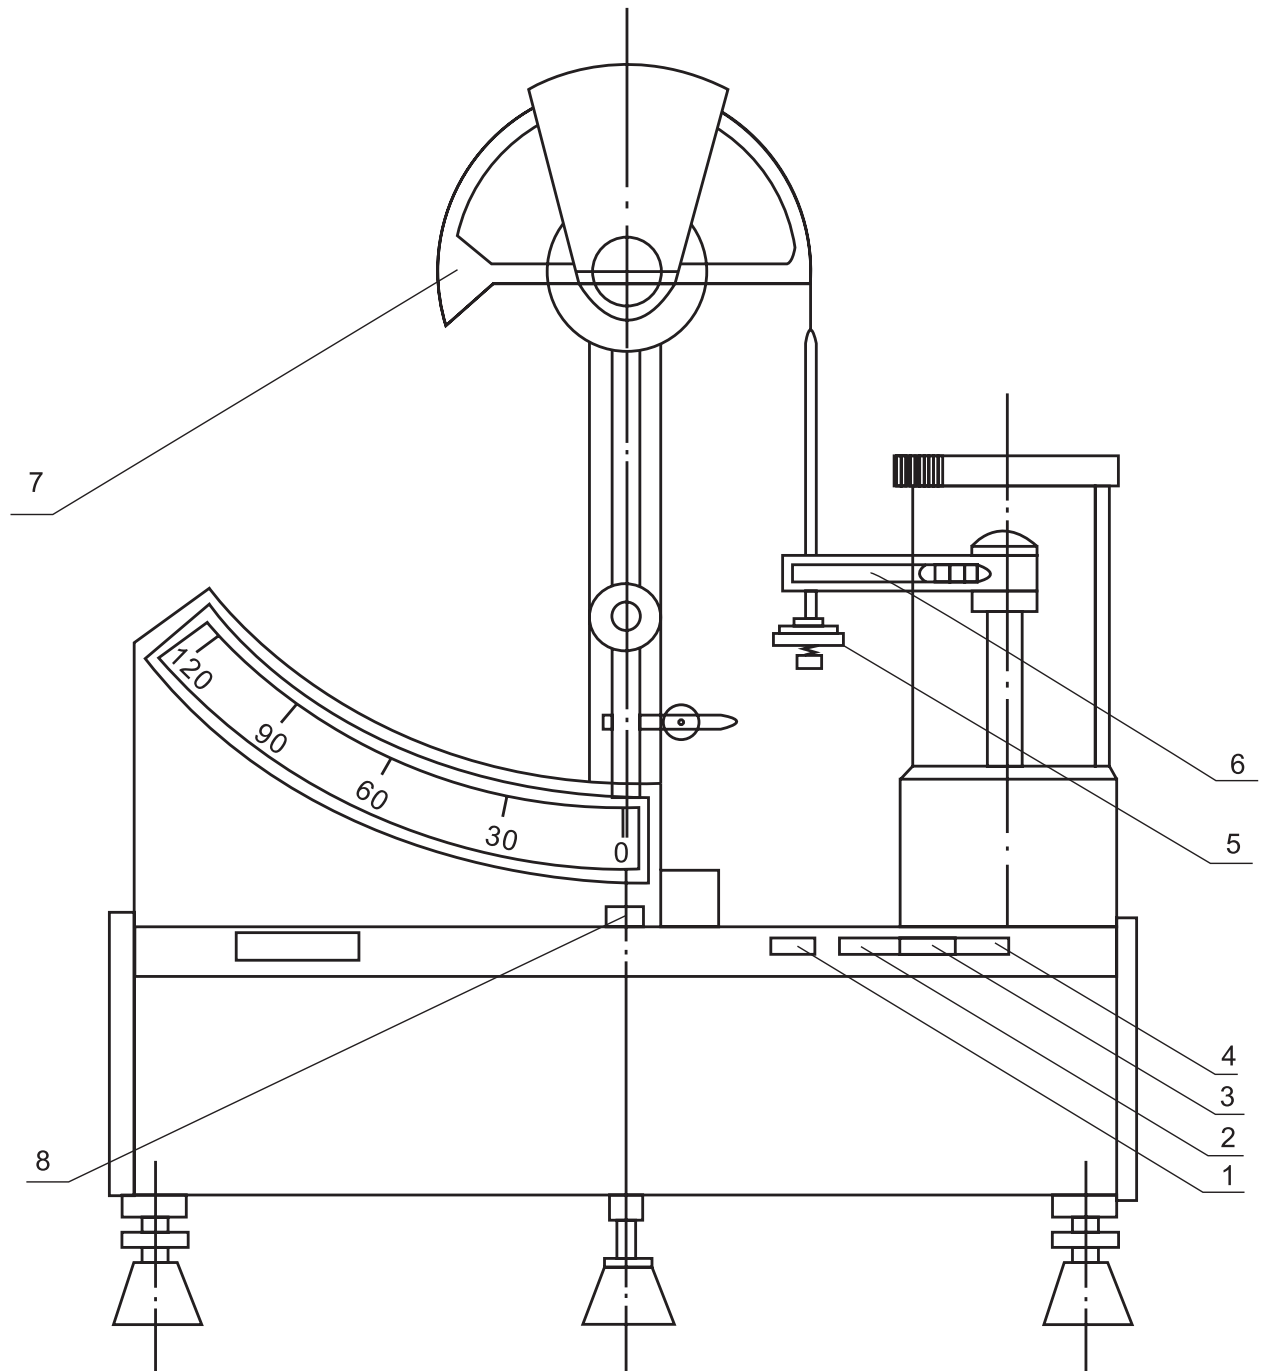

**Key**

- |   |                                      |   |                                   |
|---|--------------------------------------|---|-----------------------------------|
| 1 | power button (on and off)            | 5 | aluminium foil clamping apparatus |
| 2 | function control button (on and off) | 6 | needle clamping apparatus         |
| 3 | function control button (on and off) | 7 | adjustment rod                    |
| 4 | function control button (on and off) | 8 | (carpenter's) level               |

**Figure A.1 — Example of typical apparatus for measuring**

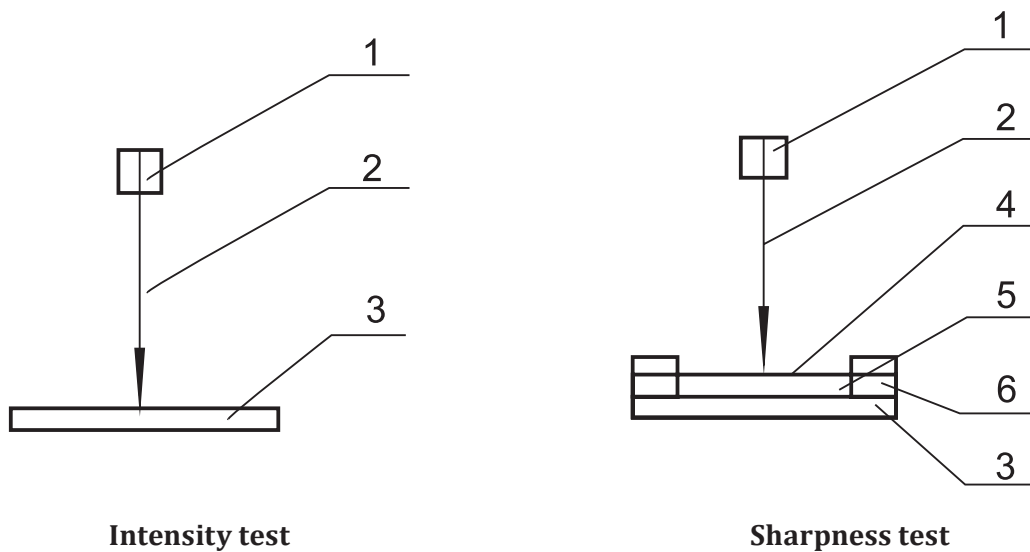

- Key**
- 1 clamped head
  - 2 needle body
  - 3 steel block
  - 4 punctured material
  - 5 gap
  - 6 plate

**Figure A.2 — Principles of testing for the intensity and sharpness of the needle tip**

**A.2.2** The full load, minimum value, and speed of the apparatus should comply with [Table A.1](#).

**Table A.1 — Hardness of the body of needle**

Items	Designation
Full load	≤ 1,2 N
Minimum value	0,01 N
Speed	≤ 0,1 mm/s

**A.2.3** The apparatus's erroneous differences in value shall be no more than 0,01 N.

**A.2.4** The apparatus should have an auto-correction capability and an antishock device. The needle clamp should be stable during use.

**A.2.5** The transmission of the apparatus should be sensitive and reliable.

**A.2.6** The starting inductive quantity of the apparatus should be no more than 0,02 N.

**A.2.7** The aperture of aluminium foil clamping apparatus is 5 mm, after clamping the Aluminium foil shall not loosen, and should be flat.

**A.2.8** The steel block surface of the strength of the sample acupuncture needle tip should be smooth and without rust.

### A.3 Aluminium foil

**A.3.1** The aluminium foil surface should be clean and smooth and without overlaps, severe wrinkles, mildew stains, or sand holes.

**A.3.2** The aluminium foil is a pliable material. The thickness should be  $(0,05 \pm 0,002)$  mm and purity of no less than 99,5 %.

**A.3.3** The strength of the pull resistance of the aluminium foil should be no less than 3 kg/mm<sup>2</sup>, and the elongation should be no less than 3 %.

### A.4 Procedure

**A.4.1** Testing for the intensity of the needle tip: After the test sample is affixed to the apparatus (with 5 mm of the tip of the needle exposed), the needle tip is thrust vertically onto the steel block. According to [A.2.2](#), increase force, speed and load until they reach the numerical values of the standard set by [5.3.5.2](#), removing the load after (5 to 10) s. Then, when examining the sample under x 5 magnification, the needle tip shall not have any bends or hooks. In addition, when the tip of the needle is dragged along the surface of cotton, it should not pull any fibres.

**A.4.2** After the intensity test, keep the sample acupuncture needle clamped in the test apparatus and allow the needle to gradually increase its force exerted on the aluminium foil (by way of the transmission); the swaying rod will react accordingly. When the force acting on the acupuncture needle exceeds the resistance of the aluminium foil, the needle tip will pierce through the aluminium foil and come into contact with the electrode. The apparatus will automatically stop increasing the force. At this time, the value indicated by the pointer on the swaying rod is the piercing force of the needle tip. For other equipment, perform equivalent procedures in accordance with the apparatus being used.

**A.4.3** Press the on-off button of the function controls to allow the swaying rod and pointer to return to their original positions. For other equipment, perform equivalent procedures in accordance with the apparatus being used.

**A.4.4** Move the aluminium foil in the clamp to allow the distance between each pierced hole to exceed three times that of the test sample.

### A.5 Test report

The test report shall contain at least the following information:

- a) the identity and designated metric size of the body of the needle;
- b) the measured values of puncture force, expressed in newtons to the nearest 0,01 N;
- c) the date of testing.

## Annex B (informative)

### Test methods for the puncture performance of the tip of the needle

#### B.1 General

The test method in this annex is exemplary. Test conditions, test materials, and value limits should be determined by criteria and reference values depending on the size and characteristics of the needle.

Therefore, concerning the setting conditions, ranges, and precision of the testing apparatus, methods suiting the testing needles should be selected.

#### B.2 Method A — Qualitative test method

Cover the mouth of a cup (diameter of 100 mm) with the membrane of a surgical rubber glove (in accordance with ISO 10282) and tighten it properly with a rubber band. Puncture the membrane perpendicularly with the acupuncture needle. During the piercing, if the dent of the membrane is small and there is little resistance, this indicates that the needle tip is sharp. Otherwise, the needle tip is blunt.

NOTE This method can be qualitatively evaluated depending on the needle's puncture performance. This method is suitable for the cross-comparison of the purchaser and the quality control of production.

#### B.3 Method B — Quantitative test method

##### B.3.1 The testing apparatus for evaluating puncture performance

The apparatus should provide the following:

- a) speed  $v = (50-250)$  mm/min; the average drive precision  $\leq$  established drive speed  $\pm 5$  %;
- b) average precision of the (0-50) sensor is  $\pm 5$  % of full range;
- c) puncture diameter of polymerized film after clamping is 10 mm.

NOTE A sketch map produced by the typical apparatus for measuring and recording puncture force as shown in [Figure B.1](#). Other apparatuses of similar performance and precision can also be used.



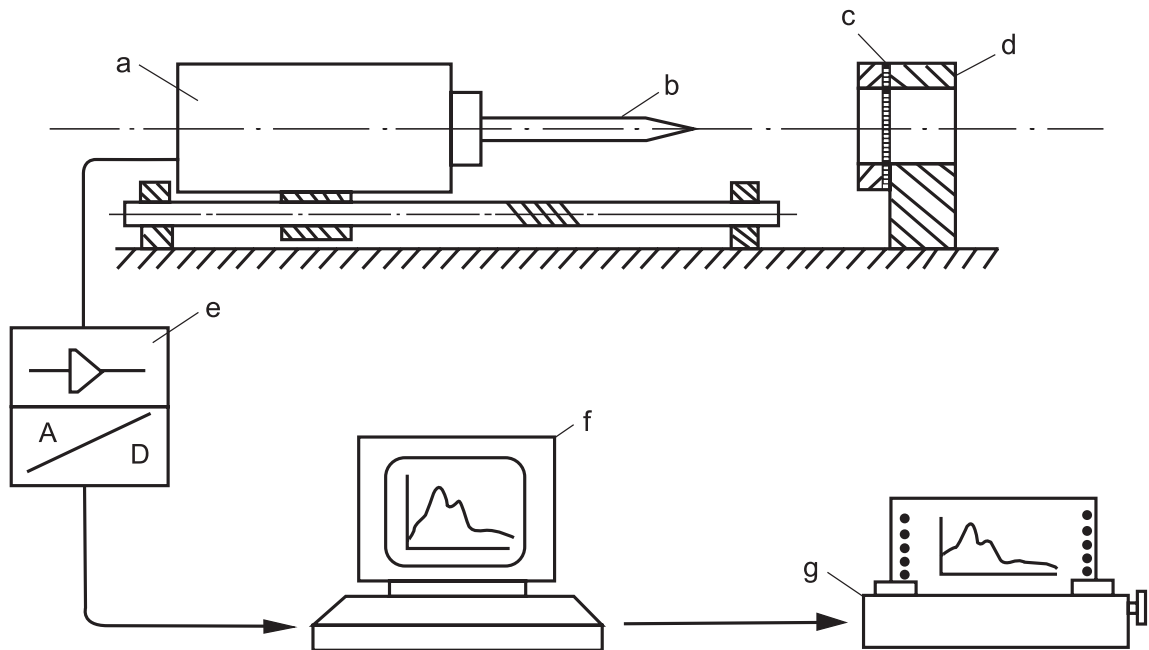


Figure B.1 — Sketch map produced by the typical testing apparatus

### B.3.2 The polymerized film materials

The polymerized wax suitable for the piercing test is elastic with a thickness of  $(0,35 \pm 0,05)$  mm. The Shore Hardness of the polyurethane film is  $(85 \pm 10)$  Shore A.

### B.3.3 Procedure

**B.3.3.1** The polymerized film is placed in  $(22 \pm 2)^\circ\text{C}$  for 24 h and tested in the same temperature.

**B.3.3.2** One part of the polymerized film of sequent length is clamped vertically on the apparatus. The polymerized film should not be tense. If the polymerized film has a refined processing surface, this surface should face the tip of the needle.

**B.3.3.3** The handle of the needle of the test acupuncture needle is installed on the fixed apparatus and the body of the needle is placed perpendicularly to the surface of the polymerized film. The tip of the needle punctures the centre of the area.

**B.3.3.4** The movement speed is 100 mm/min.

**B.3.3.5** Turn on the testing apparatus.

**B.3.3.6** Pierce the polymerized film and record the graph of force versus corresponding displacement.

**B.3.3.7** Measure the corresponding peak values ( $f_0$ ,  $f_1$ , and  $f_2$ ).

**B.3.3.8** Unused and non-punctured areas should be selected during every piercing of the polymerized film.

### B.3.4 Recording the peak values of the coordinate figures

The various force values can be identified by observing the typical peak values during the puncturing of the polymerized film by the needle.


Diagram of the typical features of the needle piercing through the film are shown in [Figure B.2](#).

Diagram of the typical puncture force of the needle ( $F_0, F_1, F_2$ ) is shown in [Figure B.3](#).

### **B.3.5 The results indicate**

Compare with the same types of needles (of known quality and performance) to evaluate the coordinate graph of differences in force and position.

Puncture performance can be viewed as the peak values of force.

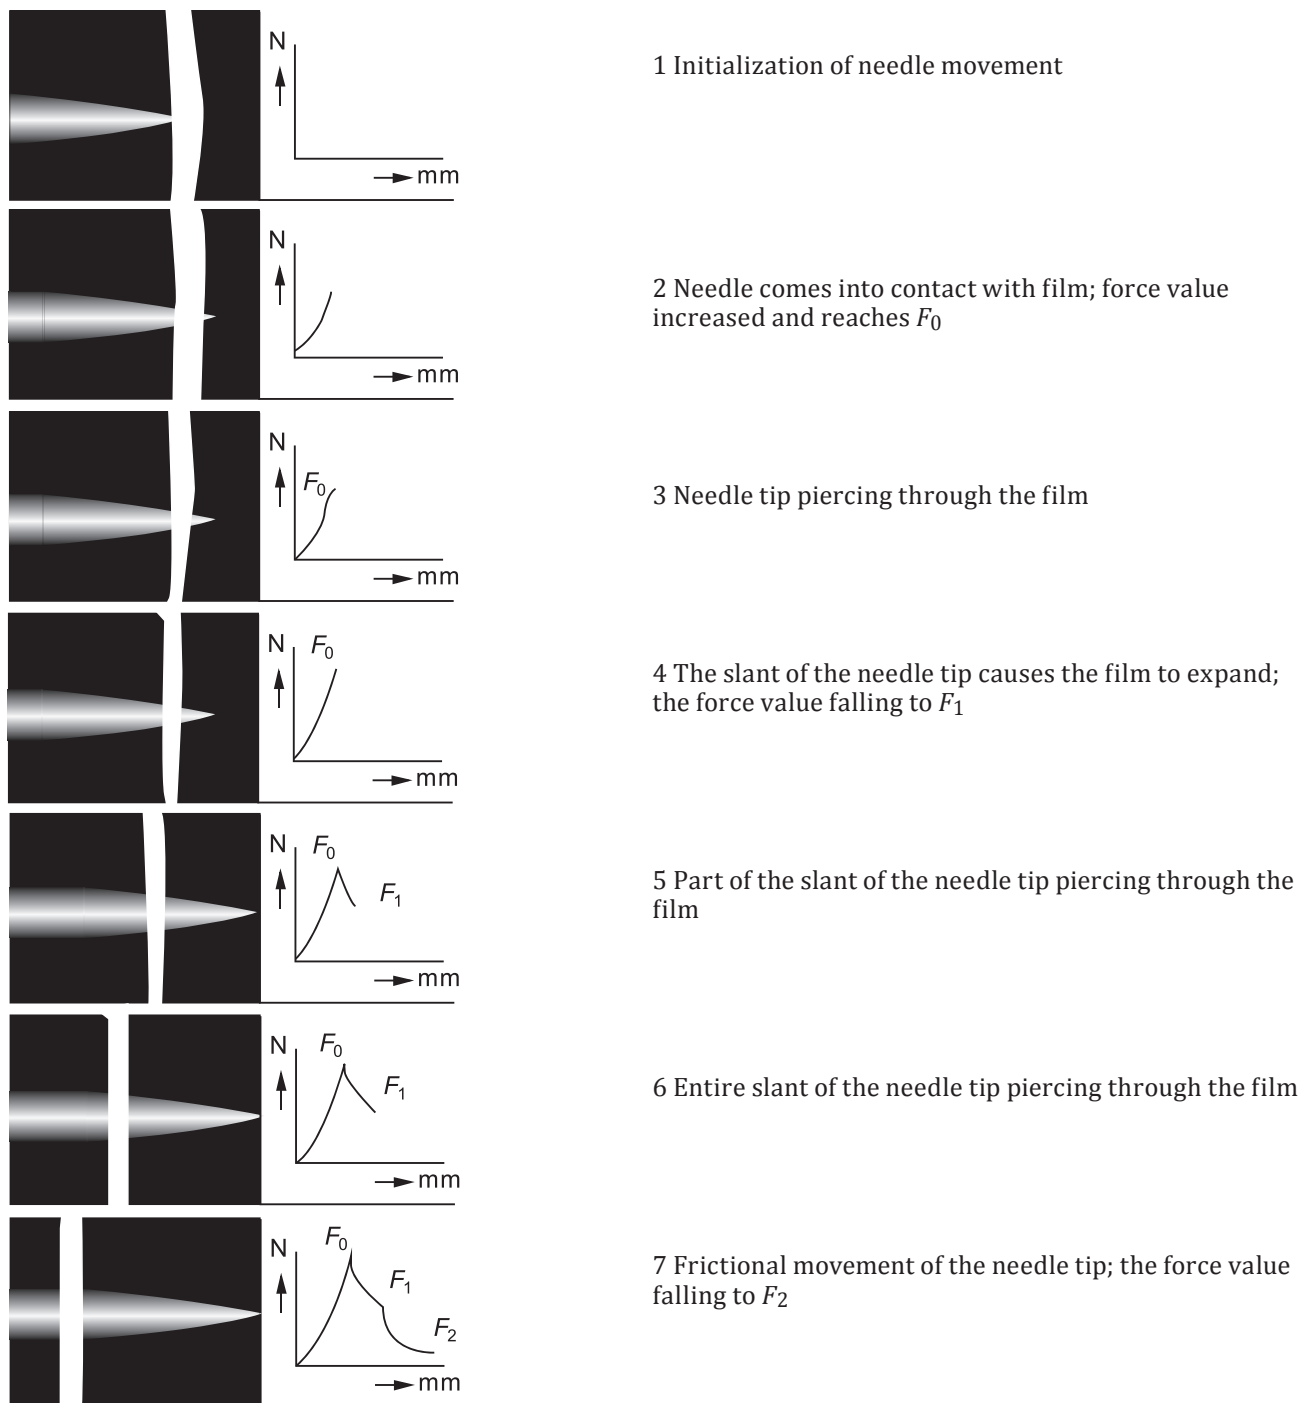


**Key**

$F_0$  the peak force of the needle tip piercing through the polymerized film

$F_1$  the peak force of the slanted surface of the needle tip cutting through the polymerized film

$F_2$  the frictional peak force of the length of the needle body piercing through the polymerized film

**Figure B.2 — Diagram of the typical features of the needle piercing through the film**

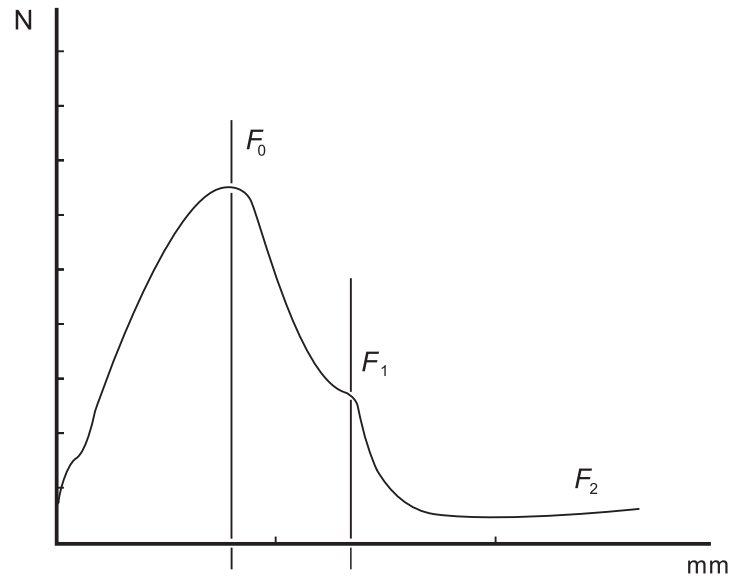

**Figure B.3 — Diagram of the typical puncture force of the needle ( $F_0$ ,  $F_1$ ,  $F_2$ )**

## Annex C (informative)

### Test method for resistance to corrosion

#### C.1 Principle

The body of the needle is partially immersed in sodium chloride solution or citric acid solution for a specified time and afterwards the immersed portion is compared visually with the non-immersed portion for signs of corrosion.

#### C.2 Method A — Testing with sodium chloride solution

##### C.2.1 Reagents and apparatus

###### C.2.1.1 Reagents

$c(\text{NaCl}) = 0,5\text{mol/l}$  (analytical grade reagent) in distilled or deionized water of grade 3 in accordance with ISO 3696.

###### C.2.1.2 Apparatus

Selection of laboratory borosilicate glassware.

##### C.2.2 Procedure

Any grease or dirt should be wiped off the Austenitic stainless steel of the body of the needle or manufactured needle body. After wiping, the test samples can be soaked in acetone or other organic solutions for further degreasing. The samples should then be washed and rinsed with the grade 3 water and set aside in preparation for later use.

Place a piece of body of the needle in a glass vessel ([C.2.1.2](#)) containing sodium chloride solution ([C.2.1.1](#)) at  $(23 \pm 2)^\circ\text{C}$ , so that approximately half the length of the body of the needle is immersed. Maintain the liquid and body of the needle at  $(23 \pm 2)^\circ\text{C}$ , for  $7\text{ h} \pm 5\text{ min}$ .

Remove the body of the needle, wipe it dry and compare the immersed and non-immersed portions under normal or corrected vision for signs of corrosion caused by the immersion. The partially immersed of the body of the needle shall show no evidence of corrosion resulting.

#### C.3 Method B — Testing with citric acid solution

##### C.3.1 Reagents and apparatus

###### C.3.1.1 Reagents

100 g/l (10 %) citric acid (chemically grade reagent) in distilled or deionized water of grade 3 in accordance with ISO 3696.

###### C.3.1.2 Apparatus

Selection of laboratory borosilicate glassware.

### C.3.2 Procedure

Any grease or dirt should be wiped off the Austenitic stainless steel of the body of the needle or manufactured needle body. After wiping, the test samples can be soaked in acetone or other organic solutions for further degreasing. The samples should then be washed and rinsed with the grade 3 water and set aside in preparation for later use.

Soak the test samples in the citric acid solution and keep them in a room-temperature environment for  $5 \text{ h} \pm 5 \text{ min}$ . Remove the articles from the solution and wash them with the water of grade 3. Place the test samples in a glass vessel with the water of grade 3 and boil for  $(30 \pm 5) \text{ min}$ , to cool and keep them in a room-temperature setting for  $(48 \pm 1) \text{ h}$ .

Remove the test samples, wipe dry and compare the immersed and non-immersed portions of the body of the needle by normal or corrected-to-normal vision under  $\times 10$  magnification. The partially immersed of the body of the needle shall show no evidence of corrosion resulting.

### C.4 Test report

The test report shall contain at least the following information:

- a) the identity and designated metric size of the body of the needle;
- b) whether corrosion occurred on the immersed half during the test;
- c) the date of testing.

## Bibliography

- [1] ISO 780:1997, *Packaging — Pictorial marking for handling of goods*
- [2] ISO 2859-1:1999, *Sampling procedures for inspection by attributes — Part 1: Sampling schemes indexed by acceptance quality limit (AQL) for lot-by-lot inspection*
- [3] ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods*
- [4] ISO 6507-2:2005, *Metallic materials — Vickers hardness test — Part 2: Verification and calibration of testing machines*
- [5] ISO 6507-3:2005, *Metallic materials — Vickers hardness test — Part 3: Calibration of reference blocks*
- [6] ISO 6507-4:2005, *Metallic materials — Vickers hardness test — Part 4: Tables of hardness values*
- [7] ISO 7864:1993, *Sterile hypodermic needles for single use*
- [8] ISO 7000:2012, *Graphical symbols for use on equipment — Registered symbols*
- [9] ISO 9626:1991, *Stainless steel needle tubing for the manufacture of medical devices (Amendment 1 published 2001)*
- [10] ISO 10282:2002, *Single-use sterile rubber surgical gloves — Specification*
- [11] ISO 10993-1:2009, *Biological evaluation of medical devices — Part 1: Evaluation and testing within a risk management process*
- [12] ISO 10993-5:2009, *Biological evaluation of medical devices — Part 5: Tests for in vitro cytotoxicity*
- [13] ISO 10993-7:2008, *Biological evaluation of medical devices — Part 7: Ethylene oxide sterilization residuals*
- [14] ISO 10993-10:2010, *Biological evaluation of medical devices — Part 10: Tests for irritation and skin sensitization*
- [15] ISO 10993-11:2006, *Biological evaluation of medical devices — Part 11: Tests for systemic toxicity*
- [16] ISO 11135-1:2007, *Sterilization of health care products — Ethylene oxide — Part 1: Requirements for development, validation and routine control of a sterilization process for medical devices*
- [17] ISO 11137-1:2006, *Sterilization of health care products — Radiation — Part 1: Requirements for development, validation and routine control of a sterilization process for medical devices*
- [18] ISO 11137-2:2013, *Sterilization of health care products — Radiation — Part 2: Establishing the sterilization dose*
- [19] ISO 11138-1:2006, *Sterilization of health care products — Biological indicators — Part 1: General requirements*
- [20] ISO 11138-2:2006, *Sterilization of health care products — Biological indicators — Part 2: Biological indicators for ethylene oxide sterilization processes*
- [21] ISO 11607-1:2006, *Packaging for terminally sterilized medical devices — Part 1: Requirements for materials, sterile barrier systems and packaging systems*
- [22] ISO 11607-2:2006, *Packaging for terminally sterilized medical devices — Part 2: Validation requirements for forming, sealing and assembly processes*

- [23] ISO 11737-1:2006, *Sterilization of medical devices — Microbiological methods — Part 1: Determination of a population of microorganisms on products*
- [24] ISO 11737-2:2007, *Sterilization of medical devices — Microbiological methods — Part 2: Tests of sterility performed in the validation of a sterilization process*
- [25] ISO 13485:2003, *Medical devices — Quality management systems — Requirements for regulatory purposes*
- [26] ISO 14971:2007, *Medical devices — Application of risk management to medical devices*
- [27] ISO 15223-1:2012, *Medical devices — Symbols to be used with medical device labels, labelling and information to be supplied — Part 1: General requirements*
- [28] ISO 15223-2:2010, *Medical devices — Symbols to be used with medical device labels, labelling, and information to be supplied — Part 2: Symbol development, selection and validation*
- [29] ISO 15510:2010, *Stainless steels — Chemical composition*
- [30] ISO 17665-1:2006, *Sterilization of health care products — Moist heat — Part 1: Requirements for the development, validation and routine control of a sterilization process for medical devices*
- [31] EN 980:2008, *Graphical symbols for use in the labelling of medical devices*
- [32] EN 1041:2008, *Information supplied by the manufacturer with medical devices*
- [33] EN 10088-1:2005, *Stainless steels*
- [34] WFAS STANDARD – 001:2012, *Acupuncture needles*
- [35] GB/T 1031-1995, *Surface roughness parameters and their values*
- [36] GB 2024-1994, *Acupuncture needles*
- [37] GB/DRT 2024-2010, *Acupuncture needles (Draft standard)*
- [38] JIS T 9301:2005, *Acupuncture needle for single use*
- [39] KS P 3007:2009, *Sterile disposable acupuncture needle*
- [40] YY 0043-2005, *Medical suture needle*
- [41] YY/T 0149-2006, *Medical instruments of stainless steel - Test methods of corrosive resistance*
- [42] YY 0666-2008, *Method for the test of sharpness and strength of needles tips*
- [43] 93/42/EEC, Council Directive 93/42/EEC of 14 June 1993 concerning medical devices
- [44] 2007/47/EC, Directive of the European Parliament and of the Council of 5 September 2007 amending Council Directive 90/385/EEC on the approximation of the laws of the Member States relating to active implantable medical devices, Council Directive 93/42/EEC concerning medical devices and Directive 98/8/EC concerning the placing of biocidal products on the market









# British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

## About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

## Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at [bsigroup.com/standards](http://bsigroup.com/standards) or contacting our Customer Services team or Knowledge Centre.

## Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at [bsigroup.com/shop](http://bsigroup.com/shop), where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

## Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to [bsigroup.com/subscriptions](http://bsigroup.com/subscriptions).

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

**PLUS** is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit [bsigroup.com/shop](http://bsigroup.com/shop).

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email [bsmusales@bsigroup.com](mailto:bsmusales@bsigroup.com).

## BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

## Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

## Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

## Useful Contacts:

### Customer Services

**Tel:** +44 845 086 9001

**Email (orders):** [orders@bsigroup.com](mailto:orders@bsigroup.com)

**Email (enquiries):** [cservices@bsigroup.com](mailto:cservices@bsigroup.com)

### Subscriptions

**Tel:** +44 845 086 9001

**Email:** [subscriptions@bsigroup.com](mailto:subscriptions@bsigroup.com)

### Knowledge Centre

**Tel:** +44 20 8996 7004

**Email:** [knowledgecentre@bsigroup.com](mailto:knowledgecentre@bsigroup.com)

### Copyright & Licensing

**Tel:** +44 20 8996 7070

**Email:** [copyright@bsigroup.com](mailto:copyright@bsigroup.com)



...making excellence a habit.™