

BS ISO 17293-2:2014



BSI Standards Publication

Surface active agents — Determination of chloroacetic acid (chloroacetate) in surfactants

Part 2: Ionic chromatographic method

bsi.

...making excellence a habit.™

National foreword

This British Standard is the UK implementation of ISO 17293-2:2014.

The UK participation in its preparation was entrusted to Technical Committee CII/34, Methods of test for surface active agents.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2014. Published by BSI Standards Limited 2014

ISBN 978 0 580 76728 9

ICS 71.100.40

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 March 2014.

Amendments issued since publication

Date	Text affected
------	---------------

**Surface active agents — Determination
of chloroacetic acid (chloroacetate) in
surfactants —**

Part 2:
Ionic chromatographic method

*Agents de surface — Détermination de l'acide chloroacétique
(chloroacétate) dans les agents tensioactifs —*

Partie 2: Méthode par chromatographie ionique





COPYRIGHT PROTECTED DOCUMENT

© ISO 2014

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Principle	1
4 Reagents	1
4.1 General	1
5 Apparatus	2
6 Procedure	3
6.1 General	3
6.2 Ion chromatographic condition	3
6.3 Calibration	3
6.4 Sampling and analysis	3
7 Results and calculation	4
7.1 General	4
7.2 Content of monochloroacetic acid	4
7.3 Content of dichloroacetic acid	4
8 Precision	4
8.1 Repeatability limit	4
8.2 Reproducible limit	5
9 Test report	5
Annex A (informative) Typical chromatograms	6

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 91, *Surface active agents*.

ISO 17293 consists of the following parts, under the general title *Surface active agents – Determination of chloroacetic acid (chloroacetate) in surfactants*:

- *Part 1: HPLC method*
- *Part 2: Ionic chromatographic method*

Surface active agents — Determination of chloroacetic acid (chloroacetate) in surfactants —

Part 2: Ionic chromatographic method

1 Scope

This part of ISO 17293 specifies a method for the determination of monochloroacetic acid (monochloroacetate) and dichloroacetic acid (dichloroacetate) in surfactants by ion chromatographic method.

The method applies for anionic surfactants such as alkyl (phenyl) ethoxylated carboxylate (AEC) or amphoteric surfactants such as alkyl imidazoline carboxylate, alkyl dimethyl betaine, and fatty acetyl propyl dimethyl betaine.

The limit of detection (LOD) is $\leq 0,01 \mu\text{g/ml}$ for monochloroacetic acid and $\leq 0,05 \mu\text{g/ml}$ for dichloroacetic acid; and the limit of quantification (LOQ) is $\leq 0,1 \mu\text{g/ml}$ for each standard (using a standard solution).

The LOD, at 1 g of sample weight, is $\leq 1 \text{ mg/kg}$ for monochloroacetic acid and $\leq 5 \text{ mg/kg}$ for dichloroacetic acid; and the LOQ is $\leq 10 \text{ mg/kg}$ for each acid.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 607, *Surface active agents and detergents — Methods of sample division*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 5725-2, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*

3 Principle

The sample solution is diluted to a proper concentration and flows through an anionic ion exchange column. The monochloroacetic acid (monochloroacetate) and dichloroacetic acid (dichloroacetate) are adsorbed in the column then eluted by the mobile phase and detected by an electrical conductivity detector.

The contents of monochloroacetic acid and dichloroacetic acid in the sample are achieved by the external calibration method.

4 Reagents

4.1 General

During the analysis, use only reagents of recognized analytical grade and the water used shall conform to grade 1 in accordance with ISO 3696, unless otherwise specified.

4.2 **Monochloroacetic acid (ClCH₂COOH), purity > 99 % (w/w)**

4.3 **Dichloroacetic acid (Cl₂CHCOOH), purity > 99 % (w/w)**

4.4 **Sulfuric acid (H₂SO₄)**

4.5 **Sodium carbonate (Na₂CO₃)**

4.6 **Sodium hydrogen carbonate (NaHCO₃)**

4.7 **Sodium hydroxide (NaOH)**

4.8 **Sodium carbonate/sodium hydrogen carbonate eluent stock solution**, containing 0,32 mol/l sodium carbonate and 0,1 mol/l sodium hydrogen carbonate.

Dissolve 3,39 g of sodium carbonate (4.5) and 0,84 g of sodium hydrogen carbonate (4.6) in 30 ml of water and swirl to mix. Quantitatively transfer the solution to a 100 ml volumetric flask (5.8), make up to the mark with water, stopper, and mix thoroughly.

4.9 **Sodium carbonate/sodium hydrogen carbonate eluent solution**, containing 3,2 mmol/l sodium carbonate and 1 mmol/l sodium hydrogen carbonate.

Quantitatively transfer 10 ml of sodium carbonate/sodium hydrogen carbonate stock solution (4.8) to a 1 000 ml volumetric flask (5.8), dilute to the mark with water, stopper, and mix thoroughly.

4.10 **Sulfuric acid solution, 50 mmol/l**

Dilute 3,0 ml of sulfuric acid (4.4) in 1 000 ml of water, mix thoroughly.

4.11 **Sodium hydroxide solution, 15 mmol/l**

Dissolve 0,6 g of sodium hydroxide (4.7) in 30 ml of water and swirl to mix. Quantitatively transfer the solution to a 1 000 ml volumetric flask (5.8), dilute to the mark with water, stopper, and mix thoroughly.

5 Apparatus

Use usual laboratory apparatus and, in particular, the following.

5.1 **Ion chromatography instrument**, equipped with pump, separator column, guard column, appropriate suppressor, data process system, and electrical conductivity detector.

5.2 **Separator column**, anionic ion exchange column, suitable for resolving monochloroacetic acid and dichloroacetic acid from sample, 4 mm × 250 mm, with appropriate guard column.

5.3 **Filter syringe**, of capacity 2 ml or 5 ml.

5.4 **Injection syringe**, of capacity 25 µl.

5.5 **Analytical balance**, accurate to 0,1 mg.

5.6 **Filters**, with suitable porosity (0,2 µm or 0,45 µm) for the filtration of reagents and sample.

5.7 **Vacuum pump**.

5.8 **Volumetric flasks**, of capacity 100 ml and 1 000 ml.

5.9 **Glass beakers**, of capacity 25 ml and 100 ml.

6 Procedure

6.1 General

The choice of chromatographic conditions depends on the apparatus in use and can be varied from those given below, provided that suitable separation of the compounds of interest is maintained. The following conditions have been found to be suitable for the column recommended.

6.2 Ion chromatographic condition

Two kinds of ion chromatographic conditions can be used in this part of ISO 17293, depending on the apparatus selected.

6.2.1 Ion chromatographic condition 1

- a) Eluent solution ([4.9](#))
- b) Flow rate: 0,70 ml/min
- c) Column temperature: room temperature
- d) Injection volume: 20 µl
- e) Regeneration solution ([4.10](#))

Based on the above conditions, a typical chromatogram can be found in [Figure A.1](#).

6.2.2 Ion chromatographic condition 2

- a) Eluent solution ([4.11](#))
- b) Flow rate: 0,85 ml/min
- c) Column temperature: room temperature
- d) Injection volume: 20 µl

Based on the above conditions, a typical chromatogram can be found in [Figure A.2](#).

6.3 Calibration

- 1) Dissolve 0,1 g of monochloroacetic acid ([4.2](#)) and 0,1 g of dichloroacetic acid ([4.3](#)), accurate to 0,1 mg, in 20 ml of water. Transfer quantitatively to a 1 000 ml volumetric flask([5.8](#)), make up to the mark with water and completely homogenize.

Store this solution in a refrigerator at (4 ± 2) °C and renew it every 7 d.

Quantitatively dilute 0,1 ml, 0,5 ml, 1,0 ml, 5,0 ml, and 10,0 ml of this solution to 100 ml with water, respectively. These standards shall be freshly prepared before analysis.

- 2) Filter ([5.6](#)) the diluted solutions and inject 20 µl each to equipment for analysis. The analysis must be done at least twice in accordance with the chromatographic conditions given in [6.2.1](#) or [6.2.2](#). The obtained linear correlation coefficient (R) shall be 0,999 or above.

6.4 Sampling and analysis

Prepare and store the test sample in accordance with ISO 607.

Add approximately 1 g of sample, accurate to 0,1 mg, in 30 ml of water, and stir until the sample is dissolved completely. Transfer into a 100 ml volumetric flask, make up to the mark with water. Filter (5.6) the solution and inject 20 µl for analysis on the appropriate chromatographic condition.

If necessary, pretreatment should be done to remove surfactant in order to protect the ion exchange column. Reversed phase ODS can be used before injection.

7 Results and calculation

7.1 General

Determine the monochloroacetic acid and dichloroacetic acid contents in the test sample using the procedure according to 6.4. Calculate the results in milligrams per kilogram (mg/kg) according to Formula (1) and Formula (2). Under given experimental conditions, no hydrolysis of chloroacetic acid has been observed.

7.2 Content of monochloroacetic acid

$$X_1(\text{mg} / \text{kg}) = \frac{A \times V}{m} \quad (1)$$

where

X_1 is the content of monochloroacetic acid, in milligrams per kilogram;

A is the calculated concentration of monochloroacetic acid in the test sample solution, in micrograms per millilitre;

V is the volume of test sample, in millilitres;

m is the mass of the test sample, in grams.

7.3 Content of dichloroacetic acid

$$X_2(\text{mg} / \text{kg}) = \frac{B \times V}{m} \quad (2)$$

where

X_2 is the content of dichloroacetic acid, in milligrams per kilogram;

B is the calculated concentration of dichloroacetic acid in the test sample solution, in micrograms per millilitre.

8 Precision

8.1 Repeatability limit

The absolute difference between two independent single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, shall not exceed the repeatability limit (r) in more than 5 % of cases.

According to ISO 5725-2, r can be expected to be:

— 10 % for contents greater than or equal to 50 mg/kg;

— 15 % for contents less than 50 mg/kg.

8.2 Reproducible limit

The absolute difference between two single test results, obtained using the same method on identical test material in different laboratories by different operators using different equipment, shall not exceed the reproducibility limit (R) in more than 5 % of cases. R can be expected to be 35 %.

9 Test report

The test report shall include the following information:

- a) the test method used, with a reference to this part of ISO 17293 (i.e. part of ISO 17293-2);
- b) all information necessary for the complete identification of the test compound;
- c) all the data (e.g. in tabular form) obtained and the calibration curve;
- d) all operating details not specified in this part of ISO 17293, or regarded as optional, together with details of any incidents which may have influenced the test result(s).

Annex A (informative)

Typical chromatograms

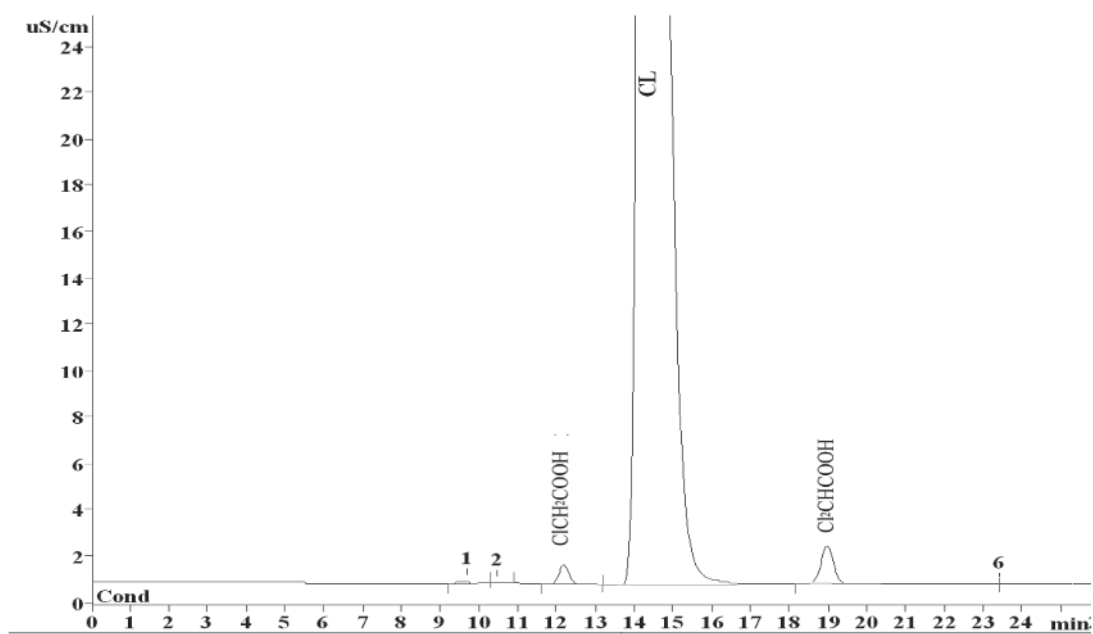


Figure A.1 — A typical IC chromatogram for monochloroacetic acid and dichloroacetic acid (on IC condition 1)

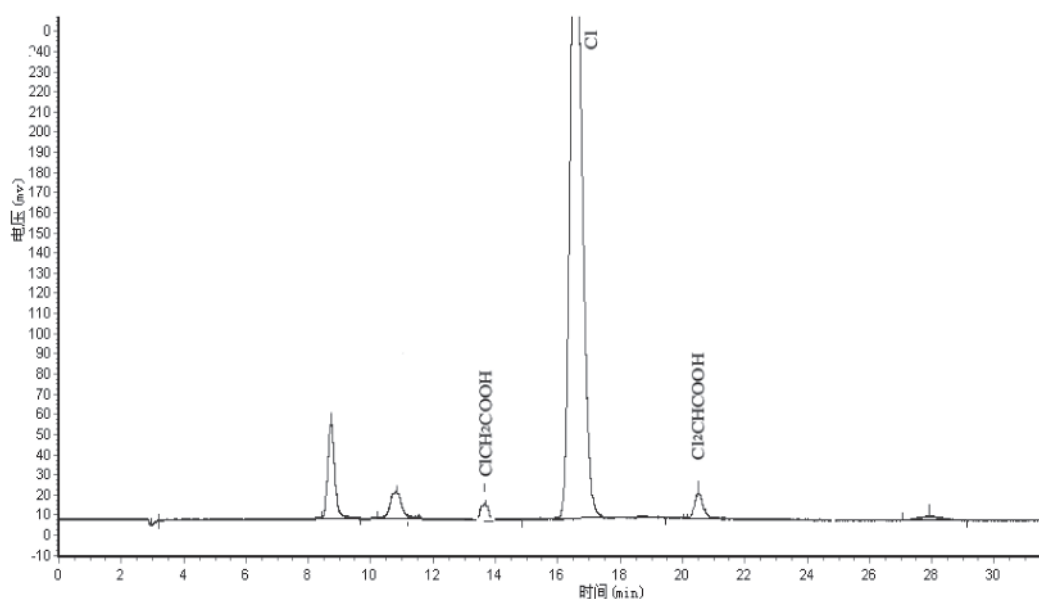


Figure A.2 — A typical IC chromatogram for monochloroacetic acid and dichloroacetic acid (on IC condition 2)

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email bsmusales@bsigroup.com.

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

Useful Contacts:

Customer Services

Tel: +44 845 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 845 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com



...making excellence a habit.™