

BS ISO 18251-1:2017



BSI Standards Publication

Non-destructive testing — Infrared thermography

Part 1: Characteristics of system and
equipment

bsi.

National foreword

This British Standard is the UK implementation of ISO 18251-1:2017.

The UK participation in its preparation was entrusted to Technical Committee WEE/46, Non-destructive testing.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2017.
Published by BSI Standards Limited 2017

ISBN 978 0 580 82616 0

ICS 19.100

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 January 2017.

Amendments/corrigenda issued since publication

Date	Text affected
------	---------------

**Non-destructive testing — Infrared
thermography —**

Part 1:
**Characteristics of system and
equipment**

*Essais non destructifs — Thermographie infrarouge —
Partie 1: Caractéristiques du système et des équipements*





COPYRIGHT PROTECTED DOCUMENT

© ISO 2017, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	v
Introduction	vi
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 IR system setup	1
5 Objective lens	2
5.1 General.....	2
5.2 Spectral response.....	2
5.3 Focal length (mm).....	2
5.4 Aperture f-number.....	2
5.5 Interchangeable object lenses.....	3
6 Detector	3
6.1 General.....	3
6.2 Detector types.....	3
6.3 Detector arrays.....	3
6.4 Scanning systems.....	3
6.5 Working wavelength range.....	3
6.6 Number of pixels.....	4
6.7 Bad/dead pixel.....	4
6.8 Detector operability.....	4
6.9 Thermal time constant.....	4
6.10 Integration time.....	4
6.11 Temperature range.....	4
7 Image processor	4
7.1 General.....	4
7.2 Image acquisition.....	4
7.2.1 Timing acquisition.....	4
7.2.2 Trigger acquisition.....	5
7.2.3 Image freeze.....	5
7.3 Image display.....	5
7.4 Image analysis.....	5
7.5 Image processing.....	5
7.5.1 General.....	5
7.5.2 Bad/dead pixel replacement.....	5
7.5.3 Non-uniformity correction.....	5
7.5.4 Image enhancement.....	5
7.5.5 Filtering.....	6
7.5.6 Time correlated processing method.....	6
7.5.7 Visible-infrared image fusion.....	6
7.6 Image recording.....	6
8 Thermal stimulation source	6
8.1 General.....	6
8.2 Optical radiation devices.....	6
8.3 Convective excitation devices.....	6
8.4 Electromagnetic induction devices.....	7
8.5 Mechanical excitation devices.....	7
8.6 Advantages and drawbacks of thermal stimulation sources.....	7
9 Integrated characteristics and functions of infrared systems and equipment	7
9.1 Integrated performance parameters.....	7
9.1.1 Noise equivalent temperature difference (NETD).....	7

9.1.2	Minimum resolvable temperature difference (MRTD).....	8
9.1.3	Minimum detectable temperature difference (MDTD).....	8
9.1.4	Field of view (FOV).....	8
9.1.5	Instantaneous field of view (IFOV).....	8
9.1.6	Minimum working distance.....	8
9.1.7	Maximum temperature measurement range.....	8
9.1.8	Temperature measurement uniformity.....	8
9.1.9	Operating temperature range.....	9
9.2	Integrated functions.....	9
9.2.1	Digital input/output interface.....	9
9.2.2	Data transfer interface.....	9
9.2.3	Video output interface.....	9
10	Accessories	9
10.1	Infrared mirror.....	9
10.2	Attenuation filter.....	9
10.3	Spectral filters.....	9
10.4	Tripod.....	9
10.5	Reference blocks.....	9
	Bibliography	10

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 135, *Non-destructive testing*, Subcommittee SC 8, *Thermographic testing*.

A list of all parts in the ISO 18251 series can be found on the ISO website.

Introduction

The industrial applications of infrared thermographic testing in non-destructive testing (NDT) are growing, along with a remarkable improvement in thermographic technologies. The effectiveness of any application of infrared thermographic testing depends upon proper and correct usage of the system and equipment. The purpose of this document is to provide the characterization description of system and equipment for infrared thermography in the field of industrial NDT. The development of this document resolves the lack of International Standards on infrared equipment and systems. The main interested parties who will benefit from this document are manufacturers and users of such equipment and systems.

Non-destructive testing — Infrared thermography —

Part 1: Characteristics of system and equipment

1 Scope

This document describes the main components, and their characteristics, constituting an infrared (IR) imaging system and related equipment used in non-destructive testing (NDT). It also aims to assist the user in the selection of an appropriate system for a particular measurement task.

The following items are specified:

- objective lens;
- detector;
- image processor;
- display;
- thermal stimulation source;
- accessories.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 10878, *Non-destructive testing — Infrared thermography — Vocabulary*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 10878 apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <http://www.iso.org/obp>

4 IR system setup

[Figure 1](#) represents an imaging arrangement including the IR system. The lens focuses an image of the object on the detector. The array of pixels in the detector produces electrical signals dependent on infrared radiation intensity. The electrical signals are processed to produce an image that is shown on a display and available for storage or further processing.

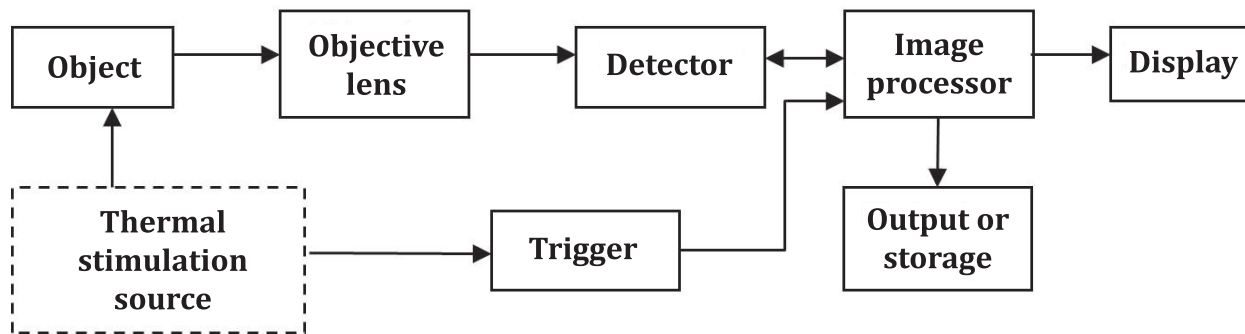


Figure 1 — IR system setup

5 Objective lens

5.1 General

The objective lens of an optical system is the element, or combination of elements, that focuses radiant energy from the object and forms the primary image.

Interchangeable lenses are used to reach a desired spatial resolution of the investigated object, or object detail.

5.2 Spectral response

IR-cameras are adapted to the transmission properties of the atmosphere for infrared radiation (atmospheric windows):

- Short Wave, SW: wavelength between approx. 0,8 μm and 2 μm ;
- Mid Wave, MW: wavelength between approx. 3 μm and 5 μm ;
- Long Wave, LW: wavelength between approx. 8 μm and 14 μm .

The spectral response of the IR-camera depends on the used detector. The transmission of the objective lens system should be adapted to the spectral response of the detector. The detector is selected according to the test problem.

5.3 Focal length (mm)

The focal length is the distance between optical centre of the lens and the focal plane point of the detector. The image of an observed object differs according to the focal length of the lens. A long focal length results in a smaller field of view and a larger image on the focal plane; this can be useful for increasing the working distance or visualizing fine details of an object.

5.4 Aperture f-number

The aperture defines the opening through which the rays come to a focus on the focal plane array. The effective size of the lens aperture affects the amount of radiant energy that passes through a lens. It is usually specified as an f-number, the ratio of the focal length to the effective aperture diameter. It strongly influences the sensitivity of the infrared detector. A larger aperture, a lower f-number, allows more radiant energy to reach the detector, increasing sensitivity of the system. These are “fast” apertures like f/1.1 or f/2. A smaller aperture, a higher f-number, allows less light that gets in. These are “slow” apertures like f/3 or f/4.5.

The lens aperture diameter needs to be greater than the detector diagonal to ensure that most of the radiant energy hitting the detector comes through the lens rather than from the internal parts of the system enclosure.

Detector aperture and lens aperture have to be carefully matched. It is beneficial to keep the lens system slightly faster than the detector in order to improve the ratio of rays accumulated by the lens system to the rays incoming from lens housing and other internal components.

5.5 Interchangeable object lenses

Interchangeable object lenses are used to adapt the camera system to special geometric requirements of measurement tasks (image section, required minimal resolution). There are typically standard object lenses, e.g. wide angle and telephoto lenses as well as accessory lenses for the measurement of large or small objects. For improved accuracy, each object lens shall be calibrated together with the camera.

6 Detector

6.1 General

The detector represents the core of the infrared camera since it senses infrared radiation and converts it to a usable electrical signal. Several characteristics affect the performance of the detector system. The type, number and arrangement of detector elements affect the sensitivity, thermal resolution, response time and spectral response of the imaging system.

6.2 Detector types

There are many different kinds of detectors available in infrared equipment, such as microbolometer, photoelectric, pyroelectric or quantum sensor, etc. These detectors are classified as two types: thermal detectors and quantum detectors. Thermal detectors, e.g. microbolometers or pyroelectric detectors, work at room temperature. Quantum detectors, e.g. photoelectric detectors or QWIP detectors, have to be cooled down to very low temperatures to reduce thermal noise. Quantum detectors have a higher sensitivity and they are easily compatible with higher frame modes of image acquisition.

6.3 Detector arrays

Infrared detectors can be single, linear arrays or two-dimensional arrays. Single element detectors require a scanning system to direct radiation from successive parts of the image at the detector in an organized two-dimensional scan that can be decoded into an image. Linear arrays can be used for producing images of moving objects, such as production lines. Two-dimensional detector arrays [focal plane array (FPA)] are capable of recording images without scanning.

6.4 Scanning systems

Mechanical scanning is achieved by moving mirrors, prisms, or polygons. Scanning cameras inherently provide homogeneous images without electronic correction mechanisms. However, the frame rate is limited due to the scanning. They are therefore less suitable to capture fast processes than FPA-cameras.

6.5 Working wavelength range

The working wavelength range depends on the detectors' material, objective lens and encapsulating window. For testing, it is selected according to the test condition and test object.

6.6 Number of pixels

A two-dimensional detector array typically consists of a rectangular array of sensors or elements. For a detector of M rows and N columns, the number of pixels is $M \times N$. The number of pixels directly affects spatial resolution of the infrared camera.

6.7 Bad/dead pixel

A bad/dead pixel is a detector element that does not respond or responds slowly to changes in radiation intensity. Imaging systems may incorporate algorithms to provide data to replace signals from bad/dead pixels.

6.8 Detector operability

Detector operability represents the percentage of individual sensors delivering a proper and usable electrical signal.

6.9 Thermal time constant

As thermal detectors have a thermal capacity, they need a distinct time to respond to changes in radiation intensity. The thermal time constant for thermal detectors is the time required to change its body temperature by 63,2 % of a specific temperature span when the measurements are made under zero-power conditions in thermally stable environments. This is especially relevant in systems where the temperature is changing with time. The thermal time constant directly affects maximum frame rate, voltage sensitivity, noise equivalent power or NETD. In some applications, e.g. windowing, the maximum frame rate is higher than the thermal constant, and thus a lesser signal-to-noise ratio (SNR) is achieved.

6.10 Integration time

The integration time is the time that the detector accumulates radiation signal. It is determined by the storage capacity of electronic charge and the intensity of incoming infrared rays. As the extension of integration time, the SNR of the infrared focal plane will be improved, but the frame rate may be reduced. For convenience of use and to expand the application range, the integration time is designed to be adjustable in modern high-end cameras.

6.11 Temperature range

The dynamic range of the detector is the interval between the lowest and highest measurable temperatures. The range shall be specified for black-body temperatures (emissivity = 1). The detector may be damaged, exceeding the dynamic range. The dynamic range depends on integration time for quantum detectors.

7 Image processor

7.1 General

Image processor performs acquisition, analysis, processing, display and storage of thermal image.

7.2 Image acquisition

7.2.1 Timing acquisition

Timing is based on the system clock so that date, time and exposure interval can be acquired.

7.2.2 Trigger acquisition

Synchronizing external equipment with the imaging system requires the imaging system to respond to external trigger signals or to generate trigger signals based on image acquisition. This function is mainly used in active thermography including, for example, pulsed thermography, lock-in thermography, laser thermography or eddy current thermography.

7.2.3 Image freeze

Image freezing is the function that allows freezing the current view without long-term storage.

7.3 Image display

A monitor (display) is used to visualize the thermal image of the viewed scene. Typically, pseudo-colour image and grey-scale image are used with single frame display mode or continuous dynamic video play mode.

7.4 Image analysis

The image analysis usually includes

- a) estimation of apparent temperature from the IR radiation intensity signal,
- b) spot measurement of the temperature,
- c) possibility of displaying the local minimum and maximum temperature in addition to the average,
- d) isotherms colour-mark ranges of the same temperature if the emissivity is the same everywhere,
- e) analysis of a time plot of a pixel or area irradiance, and
- f) visualization of selected line profiles.

7.5 Image processing

7.5.1 General

The purpose of image processing is to enhance the image to prepare it for computer or visual analysis, but any signal processing will impact the results' quality.

7.5.2 Bad/dead pixel replacement

Bad/dead pixels are replaced using an algorithm based on surrounding pixel signals to improve the usability of images.

7.5.3 Non-uniformity correction

Non-uniformity correction is used to compensate for differences in detector element responses to improve the uniformity of the detector.

7.5.4 Image enhancement

Image processing methods mainly related to histogram adjust brightness, contrast and gamma correction, which can be performed all together or individually. Various other processes can be applied to thermal images to enhance the visibility of features that the operator intends to highlight.

7.5.5 Filtering

Spatial filtering, spectral filtering and frame averaging are used to reduce image noise. It can visibly improve the SNR.

7.5.6 Time correlated processing method

For sequences of thermal images captured by, for example, pulsed thermography, lock-in thermography, laser thermography or eddy current thermography, a time correlated processing method may be used to extract more useful information.

7.5.7 Visible-infrared image fusion

A common method of enhancing location of indications is blending or “fusion” of signals from visible light and infrared detectors.

7.6 Image recording

The system should record the image as a single frame or a series of frames at a suitable frame rate for replay as a video with a full dynamic range and record related parameters of associated equipment and test conditions. A note should be added on image data compression.

8 Thermal stimulation source

8.1 General

The active thermography requires an external energy source in order to thermally stimulate the material to test. Suitable energy source and excitation principle shall be chosen according to the object and testing purpose. There exists a variety of stimulation sources, for instance, but not limited to, optical radiation, hot gas generator, induction coil, vibration probe and cooling device. Pulse, step and harmonic are examples of excitation principles.

These relevant technical data regarding the NDT purpose shall be provided by the equipment excitation source supplier. For example, the technical data of laser source should be inclusive of, but not limited to, power (W), irradiation (W/m^2), wavelength (nm), pulse duration time (s) and beam size (mm^2).

8.2 Optical radiation devices

The heating principle of optical thermal stimulation is the absorption of optical radiation at the sample surface. Conventional optical radiation devices include laser and lamps which are used for excitation of the investigated object. Laser sources can also be applied to detect surface cracks which are open toward the surface. The cracks are disturbing the lateral heat diffusion of the area heated by the laser spot and thus can be detected by generating temperature steps at the surface. There exists a variety of lamps, for instance, but not limited to, flash lamp, halogen lamp and spot light. Flash lamps heat up the surface of the investigated object with very short light pulses (pulse thermography). The selection of lamps depends on the test piece and inspection objective.

8.3 Convective excitation devices

The heating principle of convective excitation is the transfer of heat between a moving fluid (gas, liquid) and a solid testing object. Usually, there are two kinds of convective excitation source: hot and cooling device. Hot gas generator may be an air jet, steam from boilers, etc. Hot fluids are used for convective heating of the investigated object. Cooling devices, such as air jets, water jets, liquid nitrogen jets or sudden contact with ice, dry ice, etc., are employed when the temperature of the object to be tested is already higher than ambient temperature.

8.4 Electromagnetic induction devices

The heating principle of electromagnetic induction is that an alternating magnetic field generates eddy currents in an electrically conductive material. Eddy current can result in heating of the conductive testing object. In contrast to 8.2 and 8.3 and depending on the material properties, the whole volume of the test object or a surface layer with a distinct thickness is heated. Electromagnetic induction devices are used for contactless heating of electrically conductive objects. The frequency, coil dimension, coil current, distance between the coil and sample, sample and coil geometry, sample electrical conductivity and magnetic permeability are the major parameters in induction thermography.

8.5 Mechanical excitation devices

The heating principle of mechanical excitation is based on the friction between the movements of the internal object. According to the law of conservation of energy, no energy is destroyed due to friction. Energy is transformed from kinetic energy to thermal energy. Objects can be excited by mechanical excitation (e.g. by vibration sources). Certain object areas are selectively heated up because of mechanical losses. Mechanical excitation can be useful for closed cracks in materials.

8.6 Advantages and drawbacks of thermal stimulation sources

Table 1 lists the advantages and drawbacks of common thermal stimulation sources.

Table 1 — Advantages and drawbacks of different thermal stimulation sources

Thermal stimulation source	Advantages	Drawbacks
Laser	Very high, stable and controllable energy density, uniformity, fast heating	Small heating area (it is possible to perform a linear scanning by deflection of the laser beam), safety issues related to the use of high-powered lasers
Flash lamp	Fast heating, large heating area, the whole temperature history curve can be recorded	Low energy density, non-uniformity, safety issues (eye protection) are required
Halogen lamp	Stable and controllable energy density, large heating area	Low energy density, non-uniformity
Spot light	Repeatable heating, high energy density, uniformity	Small heating area
Hot gas generator	Fast heating, large heating area, uniformity	Low energy density
Electromagnetic induction devices	Large heating area, high energy density	Conductive materials only
Vibration sources	Very large heating area, high selectivity, internal heating	Low energy density, non-uniformity, coupling problems

9 Integrated characteristics and functions of infrared systems and equipment

9.1 Integrated performance parameters

9.1.1 Noise equivalent temperature difference (NETD)

The NETD characterizes the ability of an IR-camera to resolve a temperature difference of a black body. It is an equivalent temperature value corresponding to a signal-to-noise ratio of unity (1). Therefore, except if data treatment is performed, it is not possible to measure a difference equal to the NETD.

The NETD varies with the measurement setting, for instance (but not limited to):

- a) temperature of the object;
- b) measurement range;
- c) integration time (quantum detectors);
- d) data averaging or not.

9.1.2 Minimum resolvable temperature difference (MRTD)

The MRTD characterizes the image quality of IR-cameras. It represents the ability of the combined system IR-camera and human observer to resolve small temperature differences of small structures (in relation to the whole image field). The results of MRTD measurements strongly depend on the observer and are therefore subjective.

9.1.3 Minimum detectable temperature difference (MDTD)

The MDTD characterizes the image quality of IR-cameras. It is the combined ability of an IR imaging system and a human observer to detect a target at a particular temperature and of unknown location against a vast uniform background having another temperature. The results of MDTD measurements strongly depend on the observer and are therefore subjective.

9.1.4 Field of view (FOV)

The field of view (also field of vision) is the angular extent of the observable world that is seen at any given moment, and it is described using an angle of cone or pyramid. The size of the FOV directly affects the image resolution. Under the condition of same detection distance, the bigger the FOV is, the bigger the detection area. Under the condition of same detection distance and same number of pixels, the bigger the FOV is, the lower the spatial resolution.

9.1.5 Instantaneous field of view (IFOV)

The instantaneous field of view (IFOV) is the angle seen by a single element of the detector array. It depends on the lens and the size of the pixel pitch.

9.1.6 Minimum working distance

For a calibrated instrument, the minimum working distance represents the smallest possible distance between the lens and the object, enabling both imaging and correct measurement. Imperfections in the optical system, such as (but not limited to) vignetting, may lead to a minimum imaging distance longer than the minimum working distance.

For a non-calibrated instrument, the minimum working distance represents the smallest possible distance between the lens and the object, enabling the potential of a clear image.

9.1.7 Maximum temperature measurement range

The temperature measurement range is the difference between the lowest and the highest measurable temperatures. The range should be specified for black-body temperatures (emissivity = 1). The total temperature range may consist of several partial measurement ranges that can be separately adjusted by the device. The use of optical components like spectral filters can alter/change the measurable temperature range.

9.1.8 Temperature measurement uniformity

The temperature measurement uniformity describes the uniformity of the displayed temperature distribution in case of a homogeneous thermal irradiation signal.

9.1.9 Operating temperature range

The operating temperature range is the intended ambient temperature range for operating the camera.

9.2 Integrated functions

9.2.1 Digital input/output interface

The digital input/output interface permits the input of a signal into the IR system or the output of a signal from the IR system. Generally, the input signals are used to control the IR system and the output signals are used to alarm or call attention.

9.2.2 Data transfer interface

The data transfer interface permits the real-time transfer of digital image data to a PC or other storage device.

9.2.3 Video output interface

The video output interface permits the transfer of the image signals into other suitable monitors.

10 Accessories

10.1 Infrared mirror

IR-mirrors are metal mirrors reflecting infrared radiation. They are usually used to view objects or object parts otherwise inaccessible.

10.2 Attenuation filter

In order to satisfy dynamic range of the detector, attenuation filter is used to attenuate the overall radiance reaching the detector. An attenuation filter expands the temperature measurement range to higher temperatures.

10.3 Spectral filters

Spectral filters limit the spectral sensitivity range of IR-cameras. They are used to adapt the camera to material specific emission or absorption properties and/or adjust the temperature measurement range.

10.4 Tripod

Mechanisms designed to prevent camera movement during the acquisition, such as a tripod, shall be used, especially when image enhancement algorithms are used.

10.5 Reference blocks

Reference blocks are designed to calibrate the IR system and evaluate the testing results.

Bibliography

- [1] ISO 6781, *Thermal insulation — Qualitative detection of thermal irregularities in building envelopes — Infrared method*
- [2] ISO 10880, *Non-destructive testing — Infrared thermographic testing — General principles*
- [3] ISO 18434-1, *Condition monitoring and diagnostics of machines — Thermography — Part 1: General procedures*
- [4] ISO 80000-5, *Quantities and units — Part 5: Thermodynamics*
- [5] ISO 80000-7, *Quantities and units — Part 7: Light*
- [6] IEC 60068-2-1, *Environmental testing — Part 2-1: Tests — Test A: Cold*
- [7] IEC 60068-2-2, *Environmental testing — Part 2-2: Tests — Test B: Dry heat*
- [8] IEC 60068-2-6, *Environmental testing — Part 2-6: Tests — Test Fc: Vibration (sinusoidal)*
- [9] IEC 60068-2-7, *Environmental testing — Part 2-7: Tests — Test Ea and guidance: Shock*
- [10] IEC 60068-2-78, *Environmental testing — Part 2-78: Tests — Test Cab: Damp heat, steady state*
- [11] ASTM C 1060, *Standard practice for thermographic inspection of insulation installations in envelope cavities of frame buildings*
- [12] ASTM C 1153, *Standard practice for location of wet insulation in roofing systems using infrared imaging*
- [13] ASTM E 1213, *Standard practice for minimum resolvable temperature difference for thermal imaging systems*
- [14] ASTM E 1311, *Standard practice for minimum detectable temperature difference for thermal imaging systems*
- [15] ASTM E 1316, *Standard terminology for nondestructive examinations*
- [16] ASTM E 1543, *Standard test method for noise equivalent temperature difference of thermal imaging systems*
- [17] ASTM E 1897, *Standard practice for measuring and compensating for transmittance of an attenuating medium using infrared imaging radiometers*
- [18] ASTM E 1933, *Standard practice for measuring and compensating for emissivity using infrared imaging radiometers*
- [19] ASTM E 1934, *Standard guide for examining electrical and mechanical equipment with infrared thermography*
- [20] NDIS 3005, *Glossary of standard terms for nondestructive testing by infrared thermography*
- [21] NF A09-400, *Non destructive testing — Infrared thermography — Vocabulary concerning the designation of the equipment*
- [22] NF A09-420, *Non destructive testing — Infrared thermography — Characterization of equipment*
- [23] NF A09-421, *Non destructive testing — Infrared thermography — Methods for characterization of equipment*
- [24] GB/T 19870, *Industrial inspecting thermal imager*

- [25] DIN 54190-1, *Non-destructive testing — Thermographic testing — Part 1: General principles*
- [26] DIN 54190-2, *Non-destructive testing — Thermographic testing — Part 2: Equipment*

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Copyright in BSI publications

All the content in BSI publications, including British Standards, is the property of and copyrighted by BSI or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use.

Save for the provisions below, you may not transfer, share or disseminate any portion of the standard to any other person. You may not adapt, distribute, commercially exploit, or publicly display the standard or any portion thereof in any manner whatsoever without BSI's prior written consent.

Storing and using standards

Standards purchased in soft copy format:

- A British Standard purchased in soft copy format is licensed to a sole named user for personal or internal company use only.
- The standard may be stored on more than 1 device provided that it is accessible by the sole named user only and that only 1 copy is accessed at any one time.
- A single paper copy may be printed for personal or internal company use only.

Standards purchased in hard copy format:

- A British Standard purchased in hard copy format is for personal or internal company use only.
- It may not be further reproduced – in any format – to create an additional copy. This includes scanning of the document.

If you need more than 1 copy of the document, or if you wish to share the document on an internal network, you can save money by choosing a subscription product (see 'Subscriptions').

Reproducing extracts

For permission to reproduce content from BSI publications contact the BSI Copyright & Licensing team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email subscriptions@bsigroup.com.

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Useful Contacts

Customer Services

Tel: +44 345 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 345 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK