

BS ISO 20634:2015



BSI Standards Publication

# Infant formula and adult nutritionals — Determination of vitamin B<sub>12</sub> by reversed phase high performance liquid chromatography (RP-HPLC)

**bsi.**

...making excellence a habit.™

**National foreword**

This British Standard is the UK implementation of ISO 20634:2015.

The UK participation in its preparation was entrusted to Technical Committee AW/-/2, Food Technical Committee Chairmen.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2015.  
Published by BSI Standards Limited 2015

ISBN 978 0 580 90425 7

ICS 67.050

**Compliance with a British Standard cannot confer immunity from legal obligations.**

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 30 November 2015.

**Amendments/corrigenda issued since publication**

Date	Text affected
------	---------------

---

---

---

**Infant formula and adult  
nutritionals — Determination of  
vitamin B<sub>12</sub> by reversed phase high  
performance liquid chromatography  
(RP-HPLC)**

*Formules infantiles et produits nutritionnels pour adultes —  
Détermination de la teneur en vitamine B<sub>12</sub> par chromatographie  
liquide haute performance en phase inverse (CLHP-PI)*





## **COPYRIGHT PROTECTED DOCUMENT**

© ISO 2015, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Ch. de Blandonnet 8 • CP 401  
CH-1214 Vernier, Geneva, Switzerland  
Tel. +41 22 749 01 11  
Fax +41 22 749 09 47  
copyright@iso.org  
www.iso.org

# Contents

Page

<b>Foreword</b> .....	<b>iv</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Terms and definitions</b> .....	<b>1</b>
<b>3 Principle</b> .....	<b>1</b>
<b>4 Reagents and materials</b> .....	<b>1</b>
<b>5 Apparatus</b> .....	<b>4</b>
<b>6 Procedure</b> .....	<b>5</b>
6.1 General.....	5
6.2 Sample preparation.....	5
6.2.1 General.....	5
6.2.2 Extraction.....	6
6.2.3 Sample concentration.....	6
6.3 HPLC analysis.....	7
6.3.1 System setup and configuration.....	7
6.3.2 Instrument operation conditions.....	7
<b>7 Calculations</b> .....	<b>8</b>
7.1 General.....	8
7.2 Calculation of standard solution concentrations.....	9
7.3 Preparation of standard curves.....	9
7.4 Calculation of vitamin B <sub>12</sub> concentrations in sample solutions.....	9
<b>Annex A (informative) Examples of chromatograms</b> .....	<b>10</b>
<b>Annex B (informative) Precision data</b> .....	<b>11</b>
<b>Annex C (informative) Example of SPE cartridge qualification procedure</b> .....	<b>13</b>
<b>Bibliography</b> .....	<b>14</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 34, *Food products* in collaboration with AOAC INTERNATIONAL. It is being published by ISO and separately by AOAC INTERNATIONAL. The method described in the International Standard is equivalent to the AOAC Official Method 2011.10: *Vitamin B<sub>12</sub> in infant and pediatric formulas and adult nutritionals*.

# Infant formula and adult nutritionals — Determination of vitamin B<sub>12</sub> by reversed phase high performance liquid chromatography (RP-HPLC)

**WARNING** — The use of this International Standard can involve hazardous materials, operations and equipment. This International Standard does not purport to address all the safety problems associated with its use. It is the responsibility of the user of this International Standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.

## 1 Scope

This International Standard specifies a method for the quantitative determination of vitamin B<sub>12</sub> in infant and adult formula (powders, ready-to-feed liquids and liquid concentrates) by reversed phase high performance liquid chromatography.

## 2 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

### 2.1

#### **vitamin B<sub>12</sub>**

cyanocobalamin and other cobalt-containing corrinoids with vitamin B<sub>12</sub> biological activity, such as aquocobalamin, hydroxycobalamin, methylcobalamin and adenosylcobalamin, converted to cyanocobalamin

### 2.2

#### **adult nutritional**

nutritionally complete, specially formulated food, consumed in liquid form, which may constitute the sole source of nourishment, made from any combination of milk, soy, rice, whey, hydrolysed protein, starch and amino acids, with and without intact protein

### 2.3

#### **infant formula**

breast-milk substitute specially manufactured to satisfy, by itself, the nutritional requirements of infants during the first months of life up to the introduction of appropriate complementary feeding

[SOURCE: Codex Standard 72-1981]

## 3 Principle

Cyanocobalamin and other cobalt-containing corrinoids are extracted from the sample using sodium acetate buffer (pH = 4,5) and the latter converted to cyanocobalamin using potassium cyanide at 105 °C. Extracts are purified and concentrated with C8 or C18 solid-phase extraction (SPE) cartridges and analysed with size-exclusion and reversed-phase chromatography. Determination of vitamin B<sub>12</sub> is made by liquid chromatography with visible detection at 550 nm.

## 4 Reagents and materials

During the analysis, unless otherwise stated, use only reagents of recognized analytical grade and distilled or demineralized water or water of equivalent purity.

**4.1 Glacial acetic acid.**

**4.2 Acetonitrile**, HPLC grade.

**4.3 Drierite**, desiccant, anhydrous calcium sulfate, 8 mesh.

**4.4 Ethanol**, denatured.

**4.5 Formic acid**, 88 %.

**4.6 Potassium cyanide**, 97 %.

**4.7 Riboflavin**, 98 % to 102 % purity.

**4.8 Sodium acetate anhydrous or sodium acetate trihydrate**, ACS.

**4.9 Taka-Diastase**, Accurate Chemical Co.<sup>1)</sup> or equivalent.

**4.10 Triethylamine**, HPLC grade.

**4.11 Vitamin B<sub>12</sub> (cyanocobalamin) primary reference standard**, e.g. USP Reference 1152009 (approximately 10 µg/mg), Official lot<sup>1)</sup>. Store in a desiccator protected from white light.

#### **4.12 Preparation of solutions and standard solutions**

##### **4.12.1 General**

All solutions may be scaled up or down for convenience provided good laboratory practices are observed. Solutions can be stored refrigerated or at ambient temperature in tight, inert containers unless otherwise specified.

##### **4.12.2 Preparation of solutions**

**4.12.2.1 HPLC mobile phase A.** Dilute 4,0 ml of triethylamine with 1 000 ml of water. Adjust the pH to 5 to 7 with approximately 1,25 ml concentrated formic acid (4.5). Expiration: 1 week.

**4.12.2.2 HPLC mobile phase B.** Mix 4,0 ml of triethylamine and 250 ml of acetonitrile with 750 ml of water. Adjust the pH to 5 to 7 with approximately 1,25 ml concentrated formic acid. Expiration: 1 week in tightly stoppered container.

**4.12.2.3 HPLC mobile phase C.** Mix 4,0 ml of triethylamine and 750 ml of acetonitrile with 250 ml of water. Adjust the pH to 5 to 7 with approximately 1,25 ml concentrated formic acid. Expiration: 1 week in tightly stoppered container.

**4.12.2.4 HPLC mobile phase D.** Dilute 50 ml of acetonitrile to 2 000 ml with water. Expiration: 1 week in tightly stoppered container.

**4.12.2.5 Mixture of acetonitrile and water**, volume fraction 10 %. Dilute 150 ml of acetonitrile to 1 500 ml with water. Expiration: 1 month in tightly stoppered container.

---

1) This is an example of a suitable product available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of the product named. Equivalent products may be used if they can be shown to lead to the same results.



**4.12.2.6 Mixture of acetonitrile and water**, SPE elution solvent, volume fraction 30 %. Dilute 30 ml of acetonitrile to 100 ml with water. Expiration: 1 month in tightly stoppered container.

**4.12.2.7 Mixture of acetonitrile and water**, column cleaning and storage solution, volume fraction 50 %. Dilute 500 ml of acetonitrile to 1 000 ml with water in a volumetric flask. Expiration: 6 months.

**4.12.2.8 Mixture of ethanol and water**, volume fraction 25 %. Dilute 50 ml of ethanol to 200 ml with water. Expiration: 1 year in tightly stoppered container.

**4.12.2.9 Potassium cyanide solution**, mass concentration  $\rho = 4$  g/l. Dissolve 0,02 g of potassium cyanide in and dilute to 5 ml with sodium acetate buffer ([4.12.2.11](#)) substance concentration  $c = 0,25$  mol/l). Prepare fresh immediately before use.

**4.12.2.10 Potassium cyanide solution**,  $\rho = 10$  g/l. Dissolve 0,25 g of potassium cyanide in water and dilute to 25 ml. Prepare fresh immediately before use.

**4.12.2.11 Sodium acetate buffer**,  $c = 0,25$  mol/l. Dissolve 41,0 g of sodium acetate anhydrous or 68,0 g of sodium acetate trihydrate in approximately 1 800 ml of water. Adjust the pH to 4,5 with concentrated acetic acid (approximately 40 ml). Dilute to 2 000 ml with water. Expiration: 3 months.

**4.12.2.12 Resolution test solution**. Weigh approximately 0,005 g of riboflavin onto a weigh paper. Transfer to a 100 ml volumetric flask and bring to volume with 10 % acetonitrile solution. Stir to dissolve. Mix equal amounts of solution with the highest concentration of vitamin B<sub>12</sub> working standard solution. Expiration: 1 week.

**4.12.2.13 Taka-Diastase solution**,  $\rho = 60$  g/l. Dissolve 0,6 g of Taka-Diastase in 10 ml of water. Prepare fresh daily before use.

### 4.12.3 Preparation of standard solutions

**4.12.3.1 General**. Prepare all standard solutions under UV shielded fluorescent lights and store at 2 °C to 8 °C in tightly stoppered volumetric flasks.

**4.12.3.2 Vitamin B<sub>12</sub> stock standard solution**,  $\rho = 10\ 000$  µg/l. Accurately weigh the appropriate amount of vitamin B<sub>12</sub> standard ([4.11](#)) to give a stock standard concentration of 10 000 µg/l. Dissolve in and dilute to 100 ml with 25 % ethanol ([4.12.2.8](#)). Expiration: 6 months.

Calculate the amount of vitamin B<sub>12</sub> standard to be weighed,  $m_w$ , in milligrams using Formula (1):

$$m_w = 10\ 000 \times 0,1 \times \frac{1}{P} \quad (1)$$

where

10 000 is the desired stock standard solution concentration, in µg/l;

0,1 is the dilution volume, in l;

$P$  is the purity of the vitamin B<sub>12</sub> standard ([4.11](#)) in µg of cyanocobalamin per mg of standard.

**4.12.3.3 Vitamin B<sub>12</sub> intermediate standard solution**,  $\rho = 1\ 000$  µg/l. Dilute 10 ml of stock standard solution ([4.12.3.2](#)) to 100 ml with water. Expiration: 1 week.

**4.12.3.4 Vitamin B<sub>12</sub> calibration standard solutions**,  $\rho = 2,5 \mu\text{g/l}$  to  $25 \mu\text{g/l}$ . Into separate volumetric flasks, dilute 0,5 ml, 1 ml, 2 ml, 3 ml, 4 ml and 5 ml of intermediate standard solution ([4.12.3.3](#)) to 200 ml with 10 % acetonitrile ([4.12.2.5](#)). Expiration: 1 month.

## 5 Apparatus

Usual laboratory glassware and equipment and, in particular, the following.

**5.1 HPLC system**, consisting of a gradient pump, column switching valve and isocratic pump, UV-VIS detector equipped with a tungsten lamp capable of monitoring at 550 nm and autosampler capable of injecting 900  $\mu\text{l}$  to 2 000  $\mu\text{l}$  of sample.

**5.2 HPLC column**, analytical size exclusion column:

- 4  $\mu\text{m}$  particle size, 250 mm  $\times$  9,4 mm (e.g. Zorbax GF-250<sup>2)</sup> P/N 884973-901);
- 5  $\mu\text{m}$ , 300 mm  $\times$  8 mm (Shodex Protein® KW-802.5<sup>2)</sup>, P/N F6989000), or equivalent.

**5.3 HPLC column**, analytical C18 column:

- 3  $\mu\text{m}$  particle size, 100 mm  $\times$  4,6 mm (e.g. Thermo Scientific Aquasil™<sup>2)</sup> P/N 77503-104630) with C18 drop-in guard cartridges 3  $\mu\text{m}$ , 10 mm  $\times$  4,6 mm (e.g. Thermo Scientific Aquasil™<sup>2)</sup> P/N 77503-014001);
- Epic Phenyl Hexyl, 3  $\mu\text{m}$ , 120 Å, 100 mm  $\times$  4,6 mm, (ES Industries 125191-EPHX)<sup>2)</sup> with appropriate guard cartridge, or equivalent reversed-phase column compatible with 100 % aqueous mobile phase).

**5.4 Oven**, capable of maintaining temperatures of  $95 \text{ }^\circ\text{C} \pm 5 \text{ }^\circ\text{C}$  and  $105 \text{ }^\circ\text{C} \pm 5 \text{ }^\circ\text{C}$ .

**5.5 pH-meter**, with calibration buffer.

**5.6 Analytical balance**, accuracy to the nearest 0,000 01 g.

**5.7 Beakers**, glass, assorted sizes.

**5.8 Bottle top dispenser**, capable of dispensing 30 ml or equivalent.

**5.9 Cylinders**, graduated, glass, assorted sizes.

**5.10 Desiccator**.

**5.11 Conical flasks**, 125 ml capacity or equivalent glassware.

**5.12 Filter paper**, Whatman 2V<sup>2)</sup> or equivalent.

**5.13 Funnels**, plastic, suitable to use with filter paper.

**5.14 Gloves**, disposable.

**5.15 Pipettor**, variable volume, 100  $\mu\text{l}$  to 1 000  $\mu\text{l}$ .

---

2) This is an example of a suitable product available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of the product named. Equivalent products may be used if they can be shown to lead to the same results.

**5.16 Laboratory light shields**, yellow or clear shields with a cut off of at least 385 nm.

**5.17 Solid phase extraction (SPE) cartridges**, C8, 900 mg (e.g. Alltech/Grace Davidson P/N 20966<sup>2</sup>), C18, 900 mg (e.g. Alltech/Grace Davidson P/N 20942<sup>2</sup>), or equivalent. An example of a SPE cartridge qualification procedure is given in [Annex C](#).

**5.18 Syringes**, disposable, assorted sizes.

**5.19 Syringe filters**, 0,45 µm nylon.

**5.20 Vacuum manifold**, 24 ports with stopcocks or equivalent.

**5.21 Volumetric pipets**, assorted sizes.

**5.22 Volumetric flasks**, assorted sizes.

## 6 Procedure

### 6.1 General

Prepare all samples under UV shielded fluorescent lights. Prepared product samples can be analysed for up to 14 days after preparation if stored at 2 °C to 8 °C in tightly stoppered volumetric flasks. All product samples should be as uniform and representative as possible. This should be accomplished by thoroughly mixing or stirring products before sampling.

### 6.2 Sample preparation

#### 6.2.1 General

For products containing starch, add 1 ml of Taka-Diastase solution ([4.12.2.13](#)). Allow Taka-Diastase to react with the samples for at least 30 min before continuing with the extraction.

##### 6.2.1.1 Liquid samples

For ready-to-feed liquids, mix samples well to ensure homogeneity and accurately weigh approximately 20,0 g of adult nutritionals or 25,0 g of infant formula into a 100 ml volumetric flask. Continue with extraction.

##### 6.2.1.2 Powder samples

If the powder sample homogeneity is unknown, assume that it is non-homogenous and proceed as for dry blended/non-homogenous powder samples ([6.2.1.3](#)).

##### 6.2.1.3 Dry blended powder samples

For dry blended/non-homogenous powder samples, accurately weigh approximately 25,0 g. Add 200,0 g water at 40 °C before mixing until a homogeneous suspension is obtained. A homogenizer can be used when necessary. Accurately weigh approximately 20,0 g of adult nutritionals or 25,0 g of infant formula into a 100 ml volumetric flask.

##### 6.2.1.4 Wet blended powder samples

For wet blended homogenous powder samples, accurately weigh approximately 3,0 g of powder into a 100 ml volumetric flask. Add 25 ml of water and mix until all of the powder dissolves.

### 6.2.1.5 Elemental formulas

For products containing free amino acids and no intact protein, add 0,5 g of calcium caseinate or non-fat dry milk to 3,0 g of a wet blended homogeneous powder diluted with 25 ml water or 20 g to 25 g of a liquid or reconstituted dry blended nonhomogeneous powder. Mix well to dissolve the protein. Immediately add 30 ml of sodium acetate buffer (4.12.2.11) and 1 ml of 1 % potassium cyanide. Dilute to volume with water, filter, and clean up and concentrate up to 60 ml of filtrate on a preconditioned 900 mg C8 or C18 cartridge. Do not heat the sample in the 105 °C oven.

### 6.2.2 Extraction

Add 30 ml of sodium acetate buffer (4.12.2.11) to each sample extract and swirl to mix. In a fume hood, add 1 ml of freshly prepared 1 % potassium cyanide (4.12.2.10) to each sample and swirl to mix. Heat samples in a 105 °C oven for at least 60 min, but for no more than 120 min. The oven temperature will drop when the door is opened. Start timing when the oven temperature returns to 105 °C.

Remove samples from the oven and immediately cool in an ice bath. Dilute samples to volume with water. Mix well. Filter samples through a filter paper (5.12) into 125 ml conical flasks or equivalent glassware. If necessary, filter papers can be changed if they become clogged. If prepared samples are opaque and contain very small insoluble particles, centrifuge samples and transfer the liquid layer to funnels lined with filter paper. Do not heat any samples to which calcium caseinate has been added, see 6.2.1.5.

### 6.2.3 Sample concentration

To clean up and concentrate the sample, insert a 900 mg SPE cartridge (5.17) onto the stopcock of the vacuum manifold and attach a 30 ml disposable syringe barrel to the top of each cartridge. Condition each cartridge with at least 20 ml of acetonitrile (elute by gravity) and rinse each cartridge with at least 10 ml of water. Using volumetric pipets, transfer sample filtrates to cartridges using the guidelines in Table 1. If the vitamin B<sub>12</sub> concentration is unknown, use guidelines for RTF products containing 1 µg/l to 10 µg/l. If necessary, apply enough vacuum so that the samples drip steadily through the cartridges. Sample filtrates should pass through the cartridges at a rate of no more than 120 drops/min. Discard eluent.

**Table 1 — Guidelines for loading sample filtrates onto SPE cartridges**

Vitamin B <sub>12</sub> in RTF products µg/l	Volume of filtrate loaded onto SPE cartridge ml	Final dilution volume ml
< 1	80	5
1 – 10	70 – 80	10
11 – 20	50 – 60	10
21 – 50	20 – 40	10

NOTE Do not load more than 60 ml of adult nutritionals onto an Alltech C8 or C18 cartridge.

After all of the sample filtrate has passed through the cartridge, rinse each cartridge with 5 ml water and discard eluent. Air dry each cartridge by pulling a vacuum until no more eluent is observed. Close each stopcock.

Using the guidelines in Table 1, place a 5 ml or 10 ml volumetric flask under each cartridge. Add 4,4 ml of the 30 % mixture of acetonitrile and water (4.12.2.6) to all 900 mg SPE cartridges. Open each stopcock and elute vitamin B<sub>12</sub> into the volumetric flasks with vacuum. Eluent should pass through the cartridges at a rate of no more than 120 drops/min.

In preparing the final dilution, for samples collected in 10 ml volumetric flasks, dilute to volume with water.

For samples collected in 5 ml volumetric flasks, in a hood add 0,1 ml of freshly prepared 0,4 % potassium cyanide solution (4.12.2.9) to each volumetric flask. Place prepared samples in a 95 °C oven for at least


1,5 h, but for no more than 4 h. Remove samples from the oven and cool to room temperature. Dilute to volume with water.

Filter an aliquot of each standard solution and prepared sample solution through a syringe filter (5.19) into an autosampler vial.

### 6.3 HPLC analysis

#### 6.3.1 System setup and configuration

The system setup and configuration are given in Figure 1.

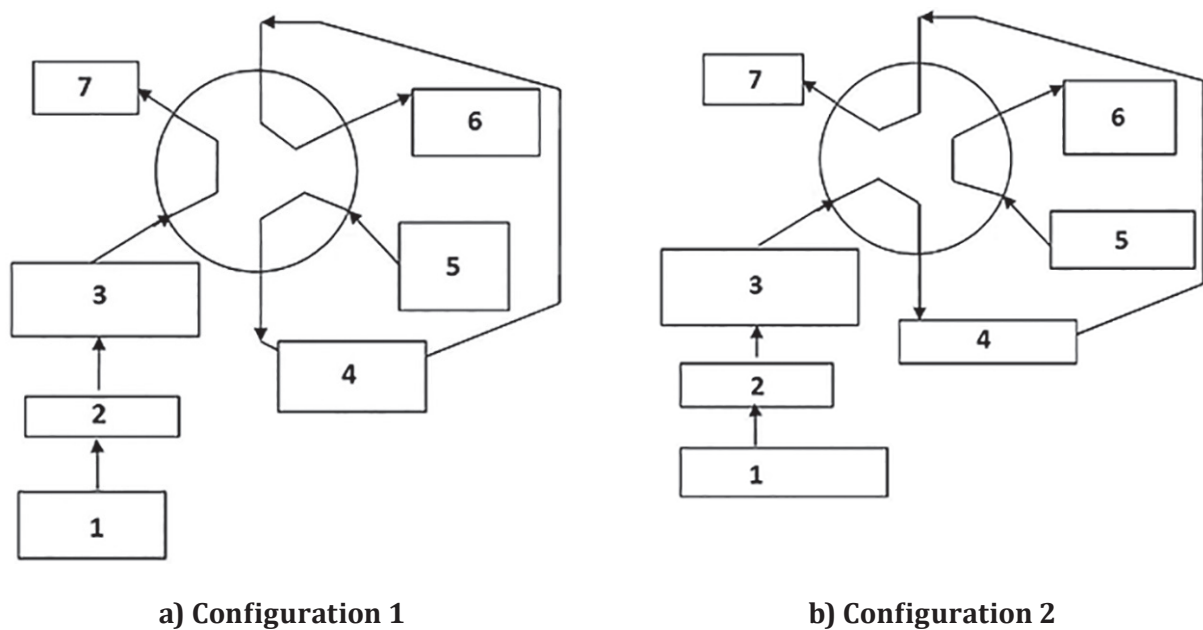

**Key**

- |                         |                   |
|-------------------------|-------------------|
| 1 isocratic pump        | 5 gradient pump   |
| 2 autosampler           | 6 UV/VIS detector |
| 3 size exclusion column | 7 waste           |
| 4 C18 analytical column |                   |

**Figure 1 — System setup and configuration of the HPLC system**

#### 6.3.2 Instrument operation conditions

- Run time: 30 min to 35 min
- Injection volume: 0,9 ml to 2,0 ml
- System configuration, see Table 2

**Table 2 — System configuration**

Time min	Valve configuration (see Figure 1)
0 - 10,5	1
10,5 - 14,5	2
14,5 - 30,0 to 35,0	1

- Isocratic pump
  - Mobile phase D ([4.12.2.4](#)).
  - Adjust the flow rate so that vitamin B<sub>12</sub> elutes from the size exclusion column between 10,5 min and 14,5 min. Typical flow rates are 1,1 ml/min to 1,2 ml/min.

To determine an appropriate flow rate, connect the size exclusion column directly to the UV/VIS detector and inject the high standard. Adjust the flow rate as necessary so that vitamin B<sub>12</sub> elutes between 10,5 min and 14,5 min.

- Gradient pump
  - Mobile phase A ([4.12.2.1](#)), B ([4.12.2.2](#)) and C ([4.12.2.3](#)).
  - Gradients to elute vitamin B<sub>12</sub> in 24 min to 30 min are given in [Table 3](#).

**Table 3 — Gradient for column (see [5.3](#))**

Time min	% mobile phase A	% mobile phase B	% mobile phase C
0	90	10	0
14,5	90	10	0
14,6	40–60 <sup>a</sup>	60–40 <sup>a</sup>	0
27,0–30,0	40–60 <sup>a</sup>	60–40 <sup>a</sup>	0
27,1–30,1	0	10	90
29,9–33,0	0	10	90

<sup>a</sup> Appropriate gradient conditions shall be established with each column to adequately resolve vitamin B<sub>12</sub> and riboflavin and to elute vitamin B<sub>12</sub> between approximately 24 min and 30 min. To establish appropriate gradient conditions with a new column, set the gradient composition at 14,6 min and 27,0 min to 30,0 min to the midpoint of the allowable range from this table. Inject the resolution test solution ([4.12.2.12](#)) and calculate the resolution (R) between the vitamin B<sub>12</sub> and riboflavin peaks. Adjust the mobile phase composition at 14,6 min and 27,0 min to 30,0 min until R > 1,5. After vitamin B<sub>12</sub> elutes from the C18 or phenyl column, rinse the column with 90 % mobile phase C for at least 2,8 min.

- Flow rate: 1,0 ml/min.
- Detector settings: detection wavelength of 550 nm and bandwidth of 10 nm.

After the system has equilibrated, inject calibration standards and a set of samples. After the last sample has injected, analyse at least one calibration standard to confirm system stability.

Example chromatograms are shown in [Annex A](#).

## 7 Calculations

### 7.1 General

The vitamin B<sub>12</sub> concentrations in samples are calculated by comparison of peak areas of samples of known weights with the peak areas of standards of known concentration.

Visually inspect each standard and sample chromatogram and verify that vitamin B<sub>12</sub> is resolved from all other peaks in the chromatograms.

Peak areas are measured with a data system. Before calculating the vitamin B<sub>12</sub> concentrations of samples, compare the vitamin B<sub>12</sub> peak areas of standards with the vitamin B<sub>12</sub> peak areas of samples and verify that the sample vitamin B<sub>12</sub> peak areas are within the range of the standard vitamin B<sub>12</sub> peak areas.

## 7.2 Calculation of standard solution concentrations

Calculate the mass concentration,  $\rho_{ws}$ , in micrograms per litre, of vitamin B<sub>12</sub> calibration standard solution (4.12.3.4) using Formula (2):

$$\rho_{ws} = S_w \times P \times \frac{A}{200} \quad (2)$$

where

- $S_w$  is the amount of vitamin B<sub>12</sub> standard weighed, in mg;
- $P$  is the purity of the vitamin B<sub>12</sub> standard (see 4.11), in µg of cyanocobalamin (vitamin B<sub>12</sub>) per mg of standard;
- $A$  is the aliquot of vitamin B<sub>12</sub> intermediate standard solution (4.12.3.3) used, in ml (here: 0,5 ml, 1,0 ml, 2,0 ml, 3,0 ml, 4,0 ml or 5,0 ml);
- 200 is the dilution volume in ml.

## 7.3 Preparation of standard curves

At each standard concentration, average the peak areas of standards injected before a set of samples with the peak areas of standards injected after the set of samples. Prepare a standard curve by performing linear least squares (regression) on concentration versus the peak areas of the working standards.

## 7.4 Calculation of vitamin B<sub>12</sub> concentrations in sample solutions

The vitamin B<sub>12</sub> concentration in each injected sample preparation is extrapolated from the vitamin B<sub>12</sub> standard curve prepared in 7.3.

Calculate the mass fraction,  $w_p$ , of vitamin B<sub>12</sub> in each product, in µg/100 g using Formula (3):

$$w_p = \rho_i \times \frac{V_1}{m_s} \times \frac{V_2}{V_f} \times \frac{m_{pr}}{m_{rp}} \times \frac{1}{10} \quad (3)$$

where

- $\rho_i$  is the vitamin B<sub>12</sub> mass concentration of the injected sample preparation extrapolated from the standard curve, in µg/l;
- $V_1$  is the volume of the first dilution, in ml (here:  $V_1 = 100$  ml);
- $m_s$  is the sample mass, in g;
- $V_2$  is the volume of the second (final) dilution, in ml;
- $V_f$  is the volume of filtrate loaded onto the cartridge, in ml;
- $m_{pr}$  is the total mass of powder reconstitution, in g (if applicable);
- $m_{rp}$  is the mass of reconstituted powder sample, in g (if applicable).

NOTE  $m_{pr}$  and  $m_{rp}$  are 1 for liquid and direct weight powder samples.

## Annex A (informative)

### Examples of chromatograms

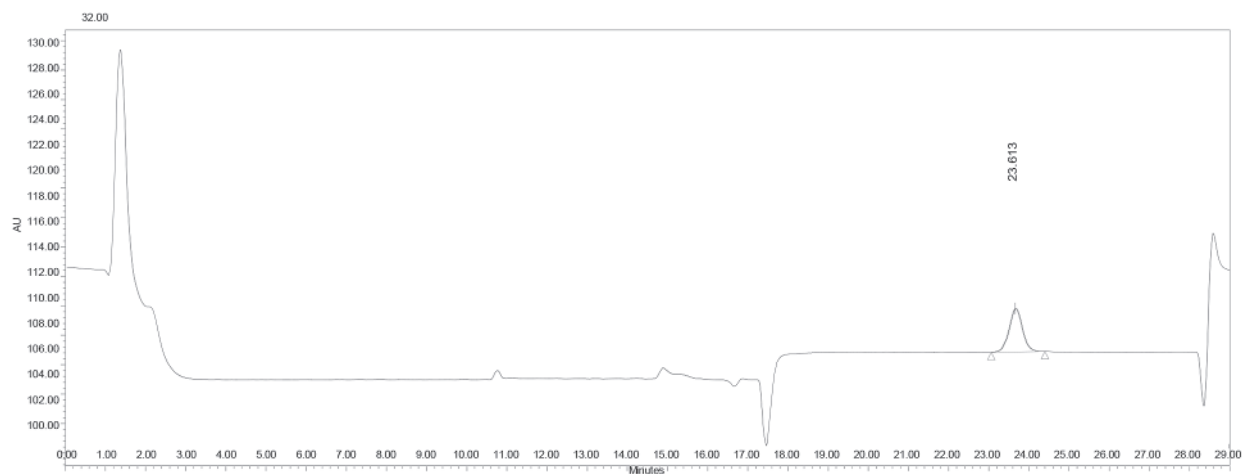


Figure A.1 — Typical standard chromatogram

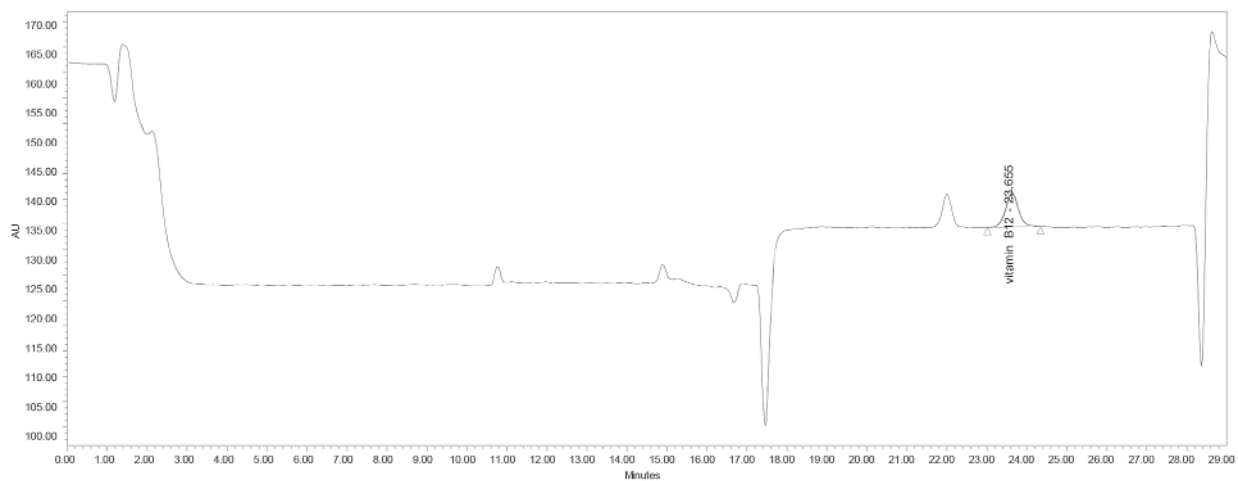


Figure A.2 — Typical sample chromatogram



## **Annex B** **(informative)**

### **Precision data**

The data given in [Table B.1](#) were obtained in an interlaboratory study and published in 2015,<sup>[1]</sup> in accordance with ISO 5725-2<sup>[2]</sup> and the AOAC-IUPAC Harmonized Protocol for collaborative study procedures, to assess precision characteristics of a method of analysis.<sup>[3]</sup> The study was performed based on requirements given in Reference.<sup>[4]</sup>

More information on the validation of the method can be found at <http://standards.iso.org/iso/20634>

Table B.1 — Precision data for vitamin B<sub>12</sub>

Sample	NIST SRM 1849a	1 <sup>a</sup>	2 <sup>b</sup>	3 <sup>c</sup>	4 <sup>d</sup>	5 <sup>e</sup>	6 <sup>f</sup>	7 <sup>g</sup>	8 <sup>h</sup>	9 <sup>i</sup>	10 <sup>j</sup>	11 <sup>k</sup>
Year of interlaboratory test	2014	2014	2014	2014	2014	2014	2014	2014	2014	2014	2014	2014
Number of laboratories	11	9	10	11	10	10	10	10	11	10	9	10
Number of non-compliant laboratories	0	0	0	0	0	0	0	0	0	0	0	0
Number of laboratories retained after eliminating outliers	10	9	10	11	9	10	10	9	10	9	8	10
Number of outliers (laboratories)	1	0	0	0	1	0	0	1	1	1	1	0
Number of accepted results	20	18	20	22	18	20	20	14	20	18	16	20
Mean value, $\bar{x}$ , µg/100 g	43,7 <sup>l</sup>	0,272	0,300	0,373	0,543	0,250	0,636	1,48	0,428	0,227	0,967	1,08
Repeatability standard deviation $s_r$ , µg/100 g	3,01 <sup>l</sup>	0,0257	0,0270	0,0200	0,0169	0,0244	0,0348	0,122	0,0208	0,0111	0,0289	0,0730
Coefficient of variation of repeatability, $C_{V,r}$ , %	6,90	9,46	8,99	5,35	3,11	9,77	5,47	8,23	4,85	4,90	2,98	6,74
Repeatability limit $r$ [ $r = 2,8 \times s_r$ ], µg/100 g	8,43 <sup>l</sup>	0,0720	0,0756	0,0560	0,0473	0,0683	0,0974	0,342	0,0582	0,0311	0,0809	0,204
Reproducibility standard deviation $s_R$ , µg/100 g	3,86 <sup>l</sup>	0,0427	0,0416	0,0694	0,0603	0,0487	0,0587	0,171	0,0305	0,0202	0,0342	0,190
Coefficient of variation of reproducibility, $C_{V,R}$ , %	8,84	15,7	13,8	18,6	11,1	19,5	9,23	11,5	7,13	8,90	3,54	17,5
Reproducibility limit $R$ [ $R = 2,8 \times s_R$ ], µg/100 g	10,8 <sup>l</sup>	0,120	0,116	0,194	0,169	0,136	0,164	0,479	0,0854	0,0566	0,0958	0,532
HorRat value, according to Reference[5]	0,34	0,40	0,36	0,50	0,32	0,50	0,27	0,38	0,20	0,22	0,11	0,55

<sup>a</sup> infant formula RTF milk based, <sup>b</sup> adult nutritional powder milk based, <sup>c</sup> infant formula powder partial hydrolysed milk based, <sup>d</sup> infant elemental powder, <sup>e</sup> infant formula powder partial hydrolysed soy based, <sup>f</sup> adult nutritional powder low fat, <sup>g</sup> adult nutritional RTF high fat (single determinations for 4 laboratories because of mislabelled product cans), <sup>h</sup> infant formula powder soy based, <sup>i</sup> infant formula powder milk based, <sup>j</sup> child formula powder, <sup>k</sup> adult nutritional RTF high protein, <sup>l</sup> results in µg/kg powder.  
RTF = ready-to-feed.

## Annex C (informative)

### Example of SPE cartridge qualification procedure

To establish SPE cartridge equivalency or to verify the suitability of new lots of cartridges, the following qualification procedure can be followed.

Prepare a solution containing 160 µg/l vitamin B<sub>12</sub> in water.

Prepare three samples from one representative product that contains the highest amount of protein of any product that will be analysed with this method using the extraction procedure described in [6.2.1](#) and [6.2.2](#).

Combine all extracted sample filtrates. Add 1 ml of the 160 µg/l vitamin B<sub>12</sub> in water solution to 80 ml or 100 ml of sample filtrate (spiked sample), and add 1 ml of water to 80 ml or 100 ml of sample filtrate (unspiked sample).

Continue preparing the spiked and unspiked sample using the sample concentration and final dilution procedures described in the sample preparation procedure ([6.2.3](#)).

Analyse the two samples chromatographically. Calculate the vitamin B<sub>12</sub> concentration of the spiked and unspiked samples and calculate the spike recovery.

In order for the cartridges to be considered acceptable, spike recoveries should be ≥ 90 %.

## Bibliography

- [1] 2011.10, Determination of Vitamin B12 in Infant, Adult, and Pediatric Formulas by HPLC-UV and Column Switching: Collaborative Study
- [2] ISO 5725-2:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*
- [3] AOAC INTERNATIONAL. AOAC Official Methods Program, Associate Referee's Manual on development, Study, Review, and Approval Process. Part IV AOAC Guidelines for Collaborative Studies, 1995, pp. 23–51.
- [4] AOAC SMPR 2011.005, Standard Method Performance Requirements for Vitamin B<sub>12</sub> in infant formula and Adult/Pediatric Nutritional formula
- [5] THOMPSON M. Recent Trends in Inter-Laboratory Precision at ppb and sub-ppb Concentrations in Relation to Fitness for Purpose Criteria in Proficiency Testing. Analyst (Lond.). 2000, **125** pp. 385–386







# British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

## About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

## Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at [bsigroup.com/standards](http://bsigroup.com/standards) or contacting our Customer Services team or Knowledge Centre.

## Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at [bsigroup.com/shop](http://bsigroup.com/shop), where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

## Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to [bsigroup.com/subscriptions](http://bsigroup.com/subscriptions).

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

**PLUS** is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit [bsigroup.com/shop](http://bsigroup.com/shop).

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email [bsmusales@bsigroup.com](mailto:bsmusales@bsigroup.com).

## BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

## Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

## Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

## Useful Contacts:

### Customer Services

**Tel:** +44 845 086 9001

**Email (orders):** [orders@bsigroup.com](mailto:orders@bsigroup.com)

**Email (enquiries):** [cservices@bsigroup.com](mailto:cservices@bsigroup.com)

### Subscriptions

**Tel:** +44 845 086 9001

**Email:** [subscriptions@bsigroup.com](mailto:subscriptions@bsigroup.com)

### Knowledge Centre

**Tel:** +44 20 8996 7004

**Email:** [knowledgecentre@bsigroup.com](mailto:knowledgecentre@bsigroup.com)

### Copyright & Licensing

**Tel:** +44 20 8996 7070

**Email:** [copyright@bsigroup.com](mailto:copyright@bsigroup.com)



...making excellence a habit.™