

BS ISO 20638:2015



BSI Standards Publication

Infant formula — Determination of nucleotides by liquid chromatography

bsi.

...making excellence a habit.™

National foreword

This British Standard is the UK implementation of ISO 20638:2015.

The UK participation in its preparation was entrusted to Technical Committee AW/-/2, Food Technical Committee Chairmen.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2015.
Published by BSI Standards Limited 2015

ISBN 978 0 580 90421 9

ICS 67.050

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 30 November 2015.

Amendments/corrigenda issued since publication

Date	Text affected
------	---------------

**Infant formula — Determination of
nucleotides by liquid chromatography**

*Formules infantiles — Détermination de la teneur en nucléotides par
chromatographie liquide*





COPYRIGHT PROTECTED DOCUMENT

© ISO 2015, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

	Page
Foreword	iv
1 Scope	1
2 Terms and definitions	1
3 Principle	1
4 Reagents and materials	1
5 Apparatus	4
6 Sample preparation	4
7 Procedure	5
7.1 Extraction	5
7.2 Chromatography	5
8 Calculations	6
9 Results	8
Annex A (informative) Examples of chromatograms	9
Annex B (informative) Precision data	10
Bibliography	14

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2. www.iso.org/directives

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received. www.iso.org/patents

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 34, *Food products* in collaboration with AOAC INTERNATIONAL. It is being published by ISO and separately by AOAC INTERNATIONAL. The method described in this International Standard is equivalent to the AOAC Official Method 2011.20: *Nucleotides in infant formula*.

Infant formula — Determination of nucleotides by liquid chromatography

WARNING — The use of this International Standard can involve hazardous materials, operations and equipment. This International Standard does not purport to address all the safety problems associated with its use. It is the responsibility of the user of this International Standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.

1 Scope

This International Standard specifies a method for the quantitative determination of 5'-mononucleotides in infant formula in solid (i.e. powders) or liquid (i.e. ready-to-feed liquids and liquid concentrates) forms using liquid chromatography.

2 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

2.1

infant formula

breast-milk substitute specially manufactured to satisfy, by itself, the nutritional requirements of infants during the first months of life up to the introduction of appropriate complementary feeding

[SOURCE: Codex Standard 72-1981]

3 Principle

The sample is dissolved in high-salt solution to inhibit protein and fat interactions. The 5'-mononucleotides — uridine 5'-monophosphate (UMP), inosine 5'-monophosphate (IMP), adenosine 5'-monophosphate (AMP), guanosine 5'-monophosphate (GMP), and cytidine 5'-monophosphate (CMP) — are separated from the sample matrix by strong-anion exchange solid-phase extraction (SPE), followed by chromatographic analysis using a C18 stationary phase with gradient elution, UV detection, and quantitation by an internal standard technique using thymidine 5'-monophosphate (TMP).[1]

4 Reagents and materials

During the analysis, unless otherwise stated, use only reagents of recognized analytical grade and distilled or demineralized water or water of equivalent purity.

4.1 Standards, $\geq 99\%$ pure (Sigma¹) or equivalent). Nucleotide sodium salts or sodium salt hydrates may be substituted if free acid forms are not readily available.

4.1.1 TMP, thymidine 5'-monophosphate, CAS No. 365-07-1.

4.1.2 AMP, adenosine 5'-monophosphate, CAS No. 61-19-8.

4.1.3 CMP, cytidine 5'-monophosphate, CAS No. 63-37-6.

1) This is an example of a suitable product available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of the product named. Equivalent products may be used if they can be shown to lead to the same results.

4.1.4 **GMP**, guanosine 5'-monophosphate, CAS No. 85-32-5.

4.1.5 **IMP**, inosine 5'-monophosphate, CAS No. 131-99-7.

4.1.6 **UMP**, uridine 5'-monophosphate, CAS No. 58-97-9.

4.2 **Potassium bromide** (KBr).

4.3 **Potassium dihydrogen phosphate** (KH_2PO_4).

4.4 **Orthophosphoric acid** (H_3PO_4).

4.5 **Potassium hydroxide** (KOH).

4.6 **Ethylenediaminetetraacetic acid, disodium salt dihydrate** (EDTA).

4.7 **Sodium chloride** (NaCl).

4.8 **Methanol** (CH_3OH).

4.9 Reagent preparation

4.9.1 **Standardizing buffer** (KH_2PO_4 , $c = 0,25$ mol/l, pH = 3,5). Dissolve 34,0 g KH_2PO_4 (4.3) in 900 ml water and adjust pH to 3,5 with orthophosphoric acid (4.4). Dilute to 1 l.

4.9.2 **Extraction solution** (NaCl, $c = 1$ mol/l, EDTA $c = 4$ mmol/l). Dissolve 58,5 g NaCl (4.7) and 1,5 g EDTA (4.6). Dilute in 1 l water.

4.9.3 **Wash solution** (KBr, $c = 0,3$ mol/l). Dissolve 3,6 g KBr (4.2) in 100 ml water.

4.9.4 **Eluent solution** (KH_2PO_4 , $c = 0,5$ mol/l, pH = 3,0). Dissolve 6,8 g KH_2PO_4 (4.3) in 90 ml water and adjust pH to 3,0 with orthophosphoric acid (4.4). Dilute to 100 ml.

4.9.5 **Mobile phase A** (KH_2PO_4 , $c = 10$ mmol/l, pH = 5,6). Dissolve 1,4 g KH_2PO_4 (4.3) in 900 ml water and adjust pH to $5,6 \pm 0,1$ with KOH solution (10 % m/v). Dilute to 1 l with water. Make daily as microbial growth often occurs at room temperature in phosphate buffers that contain little or no organic solvent.

4.9.6 **Mobile phase B**, 100 % methanol (4.8).

4.10 Standard preparation

4.10.1 **Stock standard solutions**, ρ approximately 1 mg/ml. Accurately weigh approximately 50 mg each nucleotide 5'-monophosphate into separate 50 ml volumetric flasks. Add 40 ml water, mix until dissolved, and make to volume with water.

4.10.2 **Purity standard solutions**. Pipette 1,0 ml each stock standard (4.10.1) into separate 50 ml volumetric flasks, make to volume with standardizing buffer (4.9.1), and measure absorbance at the appropriate λ_{max} to determine the concentration of each nucleotide stock standard. See Table 1 and References [1] and [2].

Table 1 — UV absorbance maxima and extinction coefficients for nucleotide 5'-monophosphates

Nucleotide 5'-monophosphate	λ_{\max} nm	$E_{1\text{cm}}^{1\%}$
Adenosine 5'-monophosphate	257	428,6
Cytidine 5'-monophosphate	280	390,9
Guanosine 5'-monophosphate	254	392,0
Inosine 5'-monophosphate	249	356,5
Uridine 5'-monophosphate	262	312,7
Thymidine 5'-monophosphate	267	288,5

4.10.3 Internal standard solution, ρ approximately 80 $\mu\text{g}/\text{ml}$. Dilute 4 ml TMP stock standard (4.10.1) into 50 ml water.

4.10.4 Working standard solution, ρ approximately 40 $\mu\text{g}/\text{ml}$. Pipette 2 ml each stock standard (4.10.1) (AMP, CMP, GMP, IMP, and UMP) into a single 50 ml volumetric flask and make to volume with water.

4.10.5 Calibration standard solutions. See Table 2 for nominal nucleotide concentrations of the calibration standard solutions.

4.10.5.1 Calibration standard 1. Pipette 0,25 ml working standard (4.10.4) and 1 ml internal standard (4.10.3) into a 25 ml volumetric flask and make to volume with water.

4.10.5.2 Calibration standard 2. Pipette 0,5 ml working standard (4.10.4) and 1 ml internal standard (4.10.3) into a 25 ml volumetric flask and make to volume with water.

4.10.5.3 Calibration standard 3. Pipette 2 ml working standard (4.10.4) and 1 ml internal standard (4.10.3) into a 25 ml volumetric flask and make to volume with water.

4.10.5.4 Calibration standard 4. Pipette 5 ml working standard (4.10.4) and 1 ml internal standard (4.10.3) into a 25 ml volumetric flask and make to volume with water.

Table 2 — Nominal concentration of calibration standards

Calibration solution	Concentration of each nucleotide: AMP, CMP, GMP, IMP, UMP $\mu\text{g}/\text{ml}$	Concentration of TMP $\mu\text{g}/\text{ml}$
1	0,4	3,2
2	0,8	3,2
3	3,2	3,2
4	8,0	3,2

5 Apparatus

Usual laboratory glassware and equipment and, in particular, the following.

- 5.1 **HPLC system**, equipped with pump, sample injector unit with a 50 µl injection loop, degasser unit, column oven, and photodiode array detector.
- 5.2 **C18 column**, Gemini²⁾ C18, 5 µm, 4,6 mm × 250 mm (Phenomenex²⁾).
- 5.3 **Spectrophotometer**, capable of digital readout to 3 decimal places.
- 5.4 **pH-meter**.
- 5.5 **Centrifuge**.
- 5.6 **Centrifuge tubes**, Amicon Ultra MWCO 3k, 4 ml (Millipore)²⁾.
- 5.7 **Polypropylene centrifuge tubes**, capacity 50 ml.
- 5.8 **Disposable syringes**, capacity 3 ml.
- 5.9 **Syringe filters**, 0,2 µm with cellulose acetate membranes.
- 5.10 **SPE vacuum manifold**.
- 5.11 **Polypropylene strong-anion exchange SPE cartridges**, 6 ml × 1 000 mg, Chromabond SB²⁾.
- 5.12 **Filter membranes**, 0,45 µm nylon.

6 Sample preparation

- a) Shake or mix sample container prior to opening.
- b) Accurately weigh approximately 1 g powder or 10 ml ready-to-feed/liquid milk infant formula into a 50 ml centrifuge tube.
- c) Add 30 ml extraction solution ([4.9.2](#)).
- d) Add 1,0 ml TMP internal standard ([4.10.3](#)).
- e) Cap the tube and vortex mix until powder dissolved.
- f) Allow sample to stand for 10 min to ensure complete hydration.
- g) Dilute to a final volume of approximately 50 ml with water.
- h) Cap the tube and vortex mix.
- i) For starch based products, transfer 2 × 4 ml of prepared sample to two separate ultra centrifuge tubes and centrifuge at 3 500g for 60 min, then pool filtrate from both tubes.

2) This is an example of a suitable product available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of the product named. Equivalent products may be used if they can be shown to lead to the same results.

7 Procedure

7.1 Extraction

Throughout the extraction procedure, do not let the cartridge run dry but drain to the top of the cartridge bed only.

When draining the cartridge, the flow rate should be < 2 ml/min.

- a) For each sample, place a single SPE cartridge on a vacuum manifold.
- b) Condition the columns by adding with 4 ml methanol and draining to top of the cartridge bed; followed by adding 2 lots of water (5 ml each) and draining to top of cartridge bed.
- c) Load the cartridge with 4 ml of sample solution and drain to the top of the cartridge bed.
- d) Wash the cartridge to remove interferences with 4 ml of wash solution (4.9.3) and drain to the top of the cartridge bed.
- e) Place a sample collection tube in SPE manifold.
- f) Elute the nucleotides with 4 ml of eluent solution (4.9.4) into a sample collection tube and completely drain the cartridge.
- g) Filter an aliquot of approximately 2 ml of the eluent through a 0,2 µm syringe filter into an autosampler vial.

7.2 Chromatography

- a) Form gradients by low pressure mixing of the two mobile phases, A and B, with separation of nucleotides achieved using the procedure given in Table 3.

Table 3 — Gradient procedure for chromatographic separation

Time min	Flow rate ml/min	Mobile Phase A %	Mobile Phase B %
0	0,6	100	0
25	0,6	80	20
26	0,6	100	0
40	0,6	100	0

- b) Acquire spectral data between 210 nm and 300 nm by the photodiode array detector with chromatograms monitored at the specified following wavelengths for quantitation.
 - 1) IMP: wavelength at 250 nm.
 - 2) AMP, GMP, and TMP: wavelength at 260 nm.
 - 3) CMP and UMP: wavelength at 270 nm.
- c) Set column oven to 40 °C.

Example chromatograms can be found in Annex A.

8 Calculations

8.1 Calculate the percent purity of each nucleotide (as free acid) in purity standard solution ([4.10.2](#)), using Formula (1):

$$\text{Purity, \%} = \frac{\text{Abs}_{\lambda_{\text{max}}}}{E_{1\text{cm}}^{1\%}} \times \frac{50}{m\text{SS}} \times \frac{50}{1} \times 1\ 000 \quad (1)$$

where

$\text{Abs}_{\lambda_{\text{max}}}$ is the UV absorbance at maximum wavelength;

$E_{1\text{cm}}^{1\%}$ is the extinction coefficient for nucleotide;

$m\text{SS}$ is the mass of nucleotide in stock standard (mg);

50 is the total volume of stock standard (ml);

50 is the total volume of purity standard (ml);

1 is the volume of stock standard added to purity standard (ml);

1 000 is the mass conversion from mg to g.

8.2 Calculate the concentration of nucleotide in stock standard solution (SS) ([4.10.1](#)), using Formula (2):

$$\text{SS } (\mu\text{g/ml}) = \frac{m\text{SS}}{50} \times \frac{\text{PS}\%}{100} \times 10^3 \quad (2)$$

where

$m\text{SS}$ is the mass of nucleotide in stock standard (mg);

50 is the total volume of SS (ml);

10^3 is the concentration conversion (mg/ml to $\mu\text{g/ml}$);

PS% is the percent purity;

100 is the mass conversion (% to decimal).

8.3 Calculate the concentration of TMP in internal standard (IS) ([4.10.3](#)), using Formula (3):

$$\text{IS } (\mu\text{g/ml}) = \text{SS} \times \frac{4}{50} \quad (3)$$

where

SS is the concentration of TMP in stock standard ($\mu\text{g/ml}$);

4 is the volume of TMP stock standard in internal standard (ml);

50 is the total volume of internal standard (ml).

8.4 Calculate the concentration of nucleotides in working standard (WS) ([4.10.4](#)), using Formula (4):

$$WS (\mu\text{g/ml}) = SS \times \frac{2}{50} \quad (4)$$

where

- SS is the concentration of nucleotide in stock standard ($\mu\text{g/ml}$);
- 2 is the volume of nucleotide stock standard in working standard (ml);
- 50 is the total volume of working standard (ml).

8.5 Calculate the concentration of TMP in calibration standards (CS) (4.10.5), using Formula (5):

$$CS (\mu\text{g/ml}) = IS \times \frac{1}{25} \quad (5)$$

where

- IS is the concentration of nucleotide in internal standard ($\mu\text{g/ml}$);
- 1 is the volume of IS in calibration standard (ml);
- 25 is the total volume of calibration standard (ml).

8.6 Calculate the concentration of nucleotides in calibration standards (CS) (4.10.5), using Formula (6):

$$CS (\mu\text{g/ml}) = WS \times \frac{V_{\text{ws}}}{25} \quad (6)$$

where

- WS is the concentration of nucleotide in working standard ($\mu\text{g/ml}$);
- V_{ws} is the volume of working standard in calibration standard (ml);
- 25 is the total volume of calibration standard (ml).

8.7 Determine the linear regression curve for the ratio of peak areas (nucleotide/TMP; y-axis) vs. the ratio of concentrations (nucleotide/TMP; x-axis) for calibration standards and calculate the slope with the y-intercept forced through 0.

8.8 Interpolate the nucleotide contents in unknown samples from this calibration curve.

a) For powders:

$$\text{Nucleotide, mg/100 g} = \frac{A_{\text{NT}}}{A_{\text{IS}}} \times \frac{1}{L} \times \frac{(C_{\text{IS}} \times V_{\text{IS}})}{m_{\text{s}}} \times \frac{100}{1\,000} \quad (7)$$

b) For ready-to-feed liquids:

$$\text{Nucleotide, mg/100 ml} = \frac{A_{\text{NT}}}{A_{\text{IS}}} \times \frac{1}{L} \times \frac{(C_{\text{IS}} \times V_{\text{IS}})}{V_{\text{s}}} \times \frac{100}{1\,000} \quad (8)$$

where

- A_{NT} is the nucleotide peak area in sample;


- A_{IS} is the TMP peak area in sample;
- L is the linear regression slope of calibration curve;
- C_{IS} is the concentration of internal standard added to sample ($\mu\text{g/ml}$);
- V_{IS} is the volume of internal standard added to sample (ml);
- m_S is the mass of sample (g);
- 1 000 is the mass conversion of result (μg to mg);
- V_S is the volume of sample (ml);
- 100 is the mass or volume conversion of result (g to 100 g or ml to 100 ml).

9 Results

Report the results in mg/100 g or mg/100 ml to one decimal place.

Annex A (informative)

Examples of chromatograms

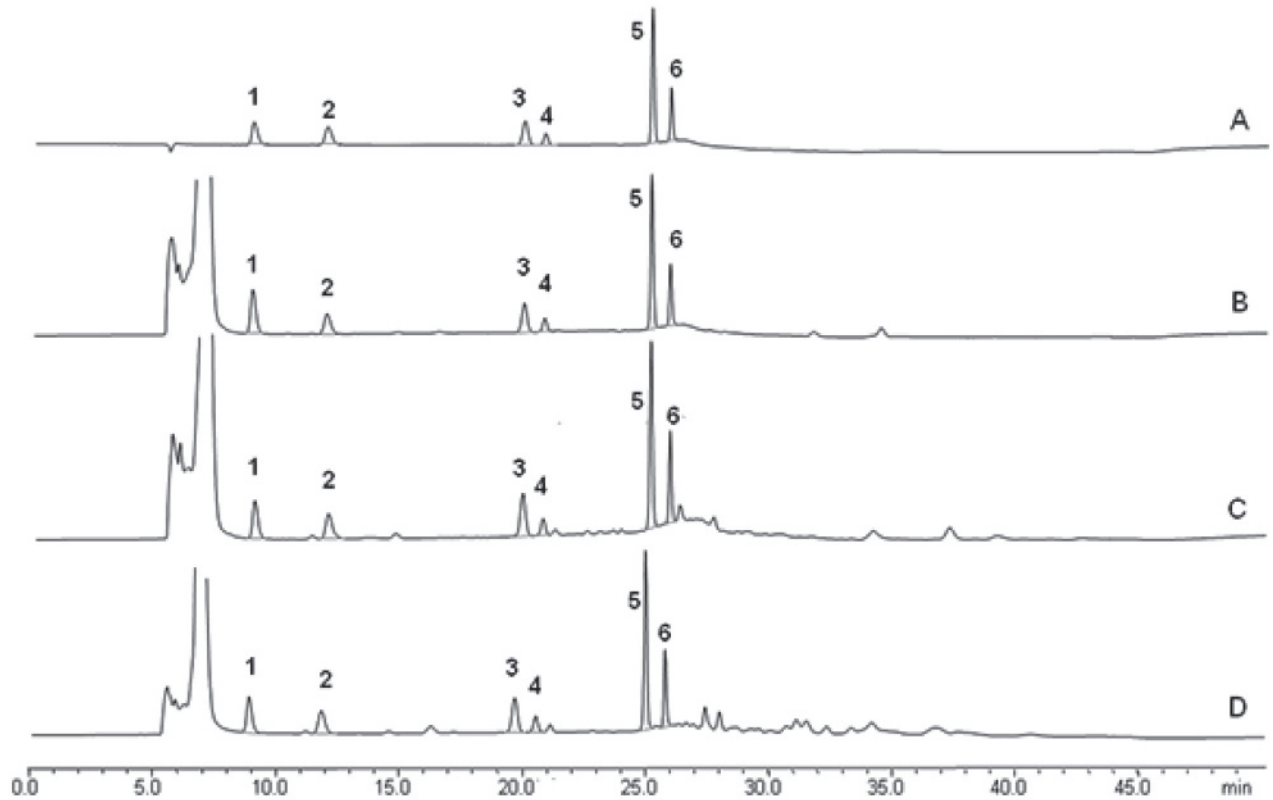

Key

A	mixture of nucleotide standards	1	cytidine 5'-monophosphate (CMP)
B	bovine milk-based infant formula	2	uridine 5'-monophosphate (UMP)
C	soy-based infant formula	3	guanosine 5'-monophosphate (GMP)
D	hydrolysed milk protein-based infant formula	4	inosine 5'-monophosphate (IMP)
		5	thymidine 5'-monophosphate (TMP)
		6	adenosine 5'-monophosphate (AMP)

Figure A.1 — Examples of chromatograms

Annex B (informative)

Precision data

The data given in [Table B.1](#) to [Table B.7](#) were obtained in an interlaboratory study and published in 2015,^[3,4] in accordance with ISO 5725-2^[5] and AOAC-IUPAC Harmonized Protocol for collaborative study procedures, to assess precision characteristics of a method of analysis.^[6] The study was evaluated based on requirements given in Reference ^[7].

More information on the validation of the method can be found at <http://standards.iso.org/iso/20638>

Table B.1 — Precision data for NIST 1849a certified reference material practice sample

Parameter	CMP	UMP	GMP	IMP	AMP
Total number of laboratories, n	12	12	12	11 ^a	12
Total number of replicates, $2n$	24	24	24	22	24
Overall mean of all data (grand mean), \bar{x} , mg/100 g	28,14	11,76	15,07	n/a	10,87
Repeatability standard deviation, s_r , mg/100 g	0,46	0,30	0,38	n/a	0,22
Reproducibility standard deviation, s_R , mg/100 g	1,36	0,59	0,68	n/a	0,47
Repeatability limit in SMPR	≤ 6 %	≤ 6 %	≤ 6 %	n/a	≤ 6 %
Coefficient of variation of repeatability, $C_{V,r}$, %	1,6	2,5	2,5	n/a	2,1
Reproducibility limit in SMPR	≤ 11 %	≤ 11 %	≤ 11 %	n/a	≤ 11 %
Coefficient of variation of reproducibility, $C_{V,R}$, %	4,8	5,0	4,5	n/a	4,4
HorRat value	0,7	0,6	0,6	n/a	0,6
^a Less than 2/9 laboratories removed from statistical analysis.					
n/a Not available.					

Table B.2 — Precision data for lactose-free infant formula test sample

Parameter	CMP	UMP	GMP	IMP	AMP
Total number of laboratories, n	12	12	24	12	12
Total number of replicates, $2n$	24	24	1,45	24	24
Overall mean of all data (grand mean), \bar{x} , mg/100 g	11,42	3,84	0,03	1,65	3,34
Repeatability standard deviation, s_r , mg/100 g	0,12	0,09	0,04	0,05	0,05
Reproducibility standard deviation, s_R , mg/100 g	0,89	0,30	24	0,10	0,09
Repeatability limit in SMPR	≤ 6 %	≤ 6 %	≤ 6 %	≤ 6 %	≤ 6 %
Coefficient of variation of repeatability, $C_{V,r}$, %	1,1 %	2,4 %	1,8 %	2,8 %	1,4 %
Reproducibility limit in SMPR	≤ 11 %	≤ 11 %	≤ 11 %	≤ 11 %	≤ 11 %
Coefficient of variation of reproducibility, $C_{V,R}$, %	7,8 %	7,9 %	2,8 %	6,1 %	2,7 %
HorRat value	1,0	0,9	0,3	0,6	0,3

Table B.3 — Precision data for starch-based infant formula test sample

Parameter	CMP	UMP	GMP	IMP	AMP
Total number of laboratories, n	11 ^a	11 ^a	11 ^a	11 ^a	11 ^a
Total number of replicates, $2n$	22	22	22	22	22
Overall mean of all data (grand mean), \bar{x} , mg/100 g	10,99	3,88	1,67	1,66	3,54
Repeatability standard deviation, s_r , mg/100 g	0,30	0,21	0,03	0,02	0,08
Reproducibility standard deviation, s_R , mg/100 g	0,81	0,31	0,07	0,17	0,11
Repeatability limit in SMPR	≤ 6 %	≤ 6 %	≤ 6 %	≤ 6 %	≤ 6 %
Coefficient of variation of repeatability, $C_{V,r}$, %	2,7 %	5,4 %	1,6 %	1,4 %	2,1 %
Reproducibility limit in SMPR	≤ 11 %	≤ 11 %	≤ 11 %	≤ 11 %	≤ 11 %
Coefficient of variation of reproducibility, $C_{V,R}$, %	7,4 %	8,4 %	4,2 %	10,3 %	3,0 %
HorRat value	0,9	0,9	0,4	1,0	0,3
^a Less than 2/9 laboratories removed from statistical analysis.					

Table B.4 — Precision data for hydrolysate-based infant formula test sample

Parameter	CMP	UMP	GMP	IMP	AMP
Total number of laboratories, n	12	12	12	11 ^a	12
Total number of replicates, $2n$	24	24	24	22	24
Overall mean of all data (grand mean), \bar{x} , mg/100 g	9,72	4,15	1,38	2,46	4,73
Repeatability standard deviation, s_r , mg/100 g	0,26	0,13	0,05	0,04	0,19
Reproducibility standard deviation, s_R , mg/100 g	0,69	0,36	0,11	0,13	0,30
Repeatability limit in SMPR	≤ 6 %	≤ 6 %	≤ 6 %	≤ 6 %	≤ 6 %
Coefficient of variation of repeatability, $C_{V,r}$, %	2,7 %	3,1 %	3,9 %	1,8 %	3,9 %
Reproducibility limit in SMPR	≤ 11 %	≤ 11 %	≤ 11 %	≤ 11 %	≤ 11 %
Coefficient of variation of reproducibility, $C_{V,R}$, %	7,1 %	8,7 %	7,7 %	5,5 %	6,2 %
HorRat value	0,9	1,0	0,7	0,6	0,7
^a Less than 2/9 laboratories removed from statistical analysis.					

Table B.5 — Precision data for soy-based infant formula test sample

Parameter	CMP ^a	UMP ^a	GMP ^a	IMP ^a	AMP ^a
Total number of laboratories, <i>n</i>	12	12	12	12	12
Total number of replicates, <i>2n</i>	24	24	24	24	24
Overall mean of all data (grand mean), \bar{x} , mg/100 g	0,50	0,19	0,22	0,16	0,54
Repeatability standard deviation, <i>s_r</i> , mg/100 g	0,19	0,05	0,05	0,07	0,11
Reproducibility standard deviation, <i>s_R</i> , mg/100 g	0,34	0,14	0,18	0,25	0,30
Repeatability limit in SMPR	≤ 8 %	≤ 10 %	≤ 10 %	≤ 10 %	≤ 8 %
Coefficient of variation of repeatability, <i>C_{V,r}</i> , %	38,5 %	25,0 %	22,9	43,7 %	20,4 %
Reproducibility limit in SMPR	≤ 16 %	≤ 20 %	≤ 20 %	≤ 20 %	≤ 16 %
Coefficient of variation of reproducibility, <i>C_{V,R}</i> , %	67,1 %	72,0 %	82,7 %	156,2 %	55,7 %
HorRat value	5,3	5,0	5,8	10,5	4,5
NOTE Soy based infant formula was not fortified with nucleotides and contained endogenous levels only.					
^a Several laboratories reported 0 for these analytes which contributed significantly to poor precision.					

Table B.6 — Precision data for whey-based infant formula test sample 1

Parameter	CMP	UMP	GMP	IMP	AMP
	Value	Value	Value	Value	Value
Total number of laboratories, <i>n</i>	12	12	12	10 ^a	12
Total number of replicates, <i>2n</i>	24	24	24	18	24
Overall mean of all data (grand mean), \bar{x} , mg/100 g	5,47	3,52	1,05	n/a	3,51
Repeatability standard deviation, <i>s_r</i> , mg/100 g	0,15	0,05	0,02	n/a	0,06
Reproducibility standard deviation, <i>s_R</i> , mg/100 g	0,48	0,31	0,04	n/a	0,18
Repeatability limit in SMPR	≤ 6 %	≤ 6 %	≤ 6 %	n/a	≤ 6 %
Coefficient of variation of repeatability, <i>C_{V,r}</i> , %	2,7 %	1,5 %	2,2 %	n/a	1,7 %
Reproducibility limit in SMPR	≤ 11 %	≤ 11 %	≤ 11 %	n/a	≤ 11 %
Coefficient of variation of reproducibility, <i>C_{V,R}</i> , %	8,7 %	8,8 %	4,1 %	n/a	5,0 %
HorRat value	1,0	0,9	0,4	n/a	0,5
^a Less than 2/9 laboratories removed from statistical analysis.					
n/a Not available.					

Table B.7 — Precision data for whey-based infant formula test sample 2

Parameter	CMP	UMP	GMP	IMP	AMP
	Value	Value	Value	Value	Value
Total number of laboratories, n	11 ^a	12	11 ^a	10 ^a	11 ^a
Total number of replicates, $2n$	22	24	22	22	22
Overall mean of all data (grand mean), \bar{x} , mg/100 g	5,43	3,54	1,05	n/a	3,51
Repeatability standard deviation, s_r , mg/100 g	0,09	0,11	0,04	n/a	0,05
Reproducibility standard deviation, s_R , mg/100 g	0,43	0,32	0,05	n/a	0,15
Repeatability limit in SMPR	≤ 6 %	≤ 6 %	≤ 6 %	n/a	≤ 6 %
Coefficient of variation of repeatability, $C_{V,r}$, %	1,6 %	3,2	3,4 %	n/a	1,3 %
Reproducibility limit in SMPR	≤ 11 %	≤ 11 %	≤ 11 %	n/a	≤ 11 %
Coefficient of variation of reproducibility, $C_{V,R}$, %	7,9 %	9,0 %	5,2 %	n/a	4,3 %
HorRat value	0,9	1,0	0,5	n/a	0,5
^a Less than 2/9 laboratories removed from statistical analysis. n/a Not available.					

Bibliography

- [1] GILL B.D., INDYK H.E., KUMAR M.C., SIEVWRIGHT N.K., MANLEY-HARRIS M.. A liquid chromatographic method for routine analysis of 5'-mononucleotides in pediatric formulas. *J. AOAC Int.* 2010, **93** pp. 966–973
- [2] GILL B.D., INDYK H.E., MANLEY-HARRIS M.. Analysis of nucleosides and nucleotides in infant formula by liquid chromatography–tandem mass spectrometry. *Anal. Bioanal. Chem.* 2013, **405** pp. 5311–5319
- [3] OMA 2011.20, *Analysis of Nucleotide 5'-Monophosphates in Infant Formulas by HPLC–UV: Collaborative Study*
- [4] GILL B.D., INDYK H.E.. Analysis of Nucleotide 5'-Monophosphates in Infant Formulas by HPLC–UV: Collaborative Study, Final Action 2011.20. *J. AOAC Int.* 2015, **98** pp. 971–979
- [5] ISO 5725-2:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*
- [6] AOAC INTERNATIONAL. AOAC Official Methods Program, Associate Referee's Manual on development, Study, Review, and Approval Process. Part IV AOAC Guidelines for Collaborative Studies, 1995, pp. 23–51.
- [7] AOAC SMPR 2011.008, Standard method performance requirements for nucleotides in infant formula and adult/pediatric nutritional formula

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email bsmusales@bsigroup.com.

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

Useful Contacts:

Customer Services

Tel: +44 845 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 845 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com



...making excellence a habit.™