

Determination of particle size distribution — Single particle light interaction methods —

Part 3: Light extinction liquid-borne particle counter

ICS 19.120

National foreword

This British Standard is the UK implementation of ISO 21501-3:2007. Together with BS ISO 21501-2:2007 and BS ISO 21501-4:2007, it supersedes BS ISO 13323-1:2000 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee LBI/37, Sieves, screens and particle sizing.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 August 2007

© BSI 2007

ISBN 978 0 580 55677 7

Amendments issued since publication

Amd. No.	Date	Comments

INTERNATIONAL
STANDARD

ISO
21501-3

First edition
2007-05-15

**Determination of particle size
distribution — Single particle light
interaction methods —**

**Part 3:
Light extinction liquid-borne particle
counter**

*Détermination de la distribution granulométrique — Méthodes
d'interaction lumineuse de particules uniques —*

*Partie 3: Compteur de particules en suspension dans un liquide par
extinction de la lumière*



Reference number
ISO 21501-3:2007(E)

Contents

Page

Foreword.....	iv
Introduction	v
1 Scope	1
2 Terms and definitions.....	2
3 Requirements	2
3.1 Size calibration.....	2
3.2 Verification of size setting	2
3.3 Counting efficiency.....	2
3.4 Size resolution	2
3.5 Maximum particle number concentration	3
3.6 Sampling flow rate.....	3
3.7 Sampling time	3
3.8 Sampling volume	3
3.9 Calibration interval	3
3.10 Test report	3
4 Test method.....	4
4.1 Size calibration.....	4
4.2 Verification of size setting	6
4.3 Counting efficiency.....	6
4.4 Size resolution	6
4.5 Maximum particle number concentration	7
4.6 Sampling flow rate.....	8
4.7 Sampling time	8
4.8 Sampling volume	8
4.9 Calibration	8
Annex A (informative) Uncertainty of particle size calibration	9
Annex B (informative) Size resolution.....	11
Bibliography	12

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 21501-3 was prepared by Technical Committee ISO/TC 24, *Sieves, sieving and other sizing methods*, Subcommittee SC 4, *Sizing by methods other than sieving*.

This first edition of ISO 21501-3, together with ISO 21501-2 and ISO 21501-4, cancels and replaces ISO 13323-1:2000, which has been technically revised.

ISO 21501 consists of the following parts, under the general title *Determination of particle size distribution — Single particle light interaction methods*:

- *Part 2: Light scattering liquid-borne particle counter*
- *Part 3: Light extinction liquid-borne particle counter*
- *Part 4: Light scattering airborne particle counter for clean spaces*

The following part is under preparation:

- *Part 1: Light scattering aerosol spectrometer*

Introduction

Monitoring particle contamination levels is required in various fields, e.g. in the electronic industry, in the pharmaceutical industry, in the manufacturing of precision machines and in medical operations. Particle counters are useful instruments for monitoring particle contamination in liquid. The purpose of this part of ISO 21501 is to provide a calibration procedure and verification method for particle counters, so as to minimize the inaccuracy in the measurement result by a counter, as well as the differences in the results measured by different instruments.

Determination of particle size distribution — Single particle light interaction methods —

Part 3: Light extinction liquid-borne particle counter

1 Scope

This part of ISO 21501 describes a calibration and verification method for a light extinction liquid-borne particle counter (LELPC), which is used to measure the size and particle number concentration of particles suspended in liquid. The light extinction method described in this part of ISO 21501 is based on single particle measurements. The typical size range of particles measured by this method is between 1 µm and 100 µm in particle size.

Instruments that conform to this part of ISO 21501 are used for the evaluation of the cleanliness of pharmaceutical products (e.g. injections, water for injections, infusions), as well as the measurement of number and size distribution of particles in various liquids.

The following are within the scope of this part of ISO 21501:

- size calibration;
- verification of size setting;
- counting efficiency;
- size resolution;
- maximum particle number concentration;
- sampling flow rate;
- sampling time;
- sampling volume;
- calibration interval;
- test report.

2 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

2.1 calibration particles
mono-disperse spherical particle with a known mean particle size, e.g. polystyrene latex (PSL) particle, that is traceable to an international standard of length, and where the standard uncertainty of the mean particle size is equal to or less than $\pm 2,5$ %

NOTE The refractive index of calibration particles is close to 1,59 at a wavelength of 589 nm (sodium D line).

2.2 counting efficiency
ratio of the measured result of a light extinction liquid-borne particle counter (LELPC) to that of a reference instrument using the same sample

2.3 particle counter
instrument that counts the number of particles and measures their size using the light scattering method or the light extinction method

**2.4 pulse height analyser
PHA**
instrument that analyses the distribution of pulse heights

2.5 size resolution
measure of the ability of an instrument to distinguish between particles of different sizes

3 Requirements

3.1 Size calibration
The recommended procedure for the size calibration is described in 4.1.

3.2 Verification of size setting
The reported particle size range setting error of LELPC shall be equal to or less than ± 10 % when the test is carried out by the method described in 4.2.

3.3 Counting efficiency
The counting efficiency shall be (100 ± 20) % when the test is carried out by the method described in 4.3.

3.4 Size resolution
The size resolution shall be equal to or less than 10 % when the test is carried out by the method described in 4.4.

3.5 Maximum particle number concentration

The maximum measurable particle number concentration shall be specified by the manufacturer. The coincidence loss at the maximum particle number concentration of an LELPC shall be equal to or less than 10 %.

NOTE When the particle number concentration is higher than the maximum particle number concentration, the number of uncounted particles increases because of an enhanced probability of multiple particles existing in the sensing volume (coincidence error) and/or saturation of the electronic system.

3.6 Sampling flow rate

The manufacturer shall specify the standard uncertainty of the sampling flow rate. It shall be checked by the user prior to the measurement so that the sampling flow rate is within the range specified by the manufacturer.

The standard uncertainty of sampling flow rate shall be within the manufacturer's specification.

If the LELPC does not have a flow rate control system this subclause does not apply, however the manufacturer shall specify the allowable flow rate range of the LELPC.

3.7 Sampling time

The standard uncertainty in the duration of sampling time shall be equal to or less than ± 1 % of the preset value.

This subclause does not apply when the LELPC is not equipped with a sampling system.

This subclause does not apply when the LELPC is equipped with a volumetric sampling system.

3.8 Sampling volume

The standard uncertainty of sampling volume shall be equal to or less than ± 5 % of the preset value.

This subclause does not apply when the LELPC is not equipped with a volumetric sampling system.

3.9 Calibration interval

It is recommended that the calibration interval of an LELPC be one year or less.

3.10 Test report


The following minimum information shall be recorded:

- a) date of calibration;
- b) calibration particle sizes;
- c) verification of size setting;
- d) flow rate;
- e) size resolution (with the particle size used);
- f) counting efficiency;
- g) voltage limit or channel of an internal pulse height analyser (PHA).

4 Test method

4.1 Size calibration

When calibrating an LELPC with calibration particles of known size, the median voltage (or internal PHA channel), corresponds to the particle size (see Figure 1). The median voltage (or internal PHA channel) should be determined by using a particle counter with variable voltage limit (or internal PHA channel) settings. The median voltage (or internal PHA channel) is the voltage (or internal PHA channel) that equally divides the total number of pulses counted. When a particle counter with variable voltage limit settings is not available, a PHA can be used in place of the counter.

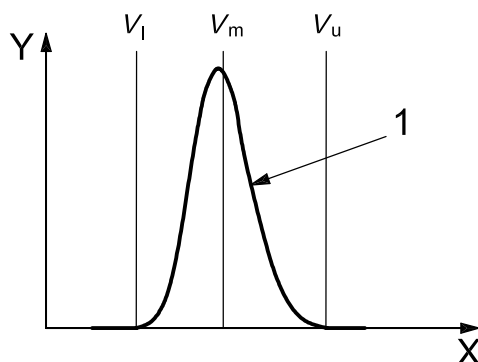

Key

X pulse height voltage (or channel)

Y density

1 pulse height distribution with PSL particles


V_l lower voltage limit

V_m median voltage

V_u upper voltage limit

Figure 1 — Pulse height distribution of PSL particle signals

When noise signals appear as if there are many small particles in the sample, the median voltage (or internal PHA channel) shall be determined by discarding the pulses due to “false particles” [see Figure 2 a)]. The discarding should only be done when the density at the peak due to real particles is more than twice the density at the valley that separates it from the pulses due to “false particles” [see Figure 2 b)]. In this case, V_u is the voltage greater than the median voltage, V_m , where the density is the same as V_l . The median is calculated using only the population between the voltage limits V_l and V_u .

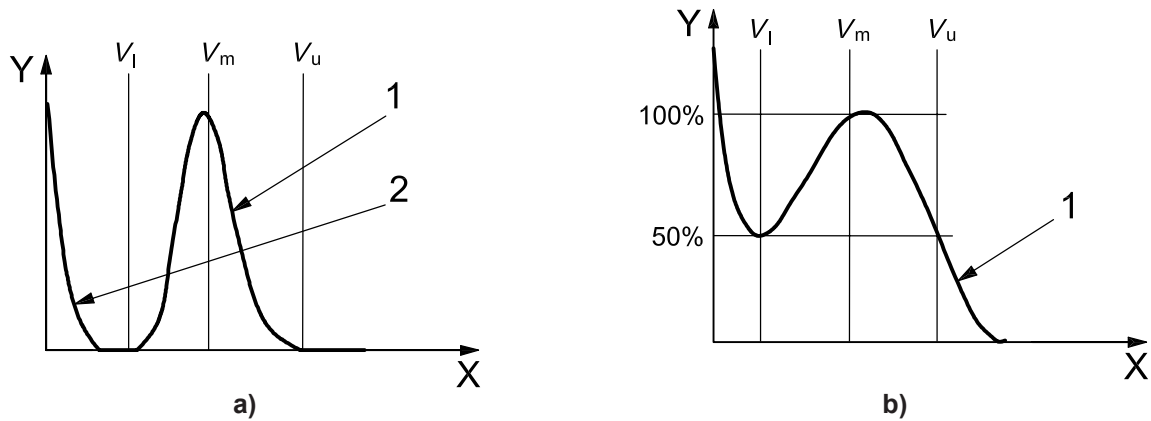**Key**

X pulse height voltage (or channel)


Y density

1 pulse height distribution with PSL particles

2 noise (false particles, small particles and/or optical, electrical noise)

 V_l lower voltage limit V_m median voltage V_u upper voltage limit**Figure 2 — Pulse height distribution of PSL particle signals with noise**

The voltages of channels corresponding to particle size should be determined in accordance with the calibration curve provided by the manufacturer (see Figure 3).

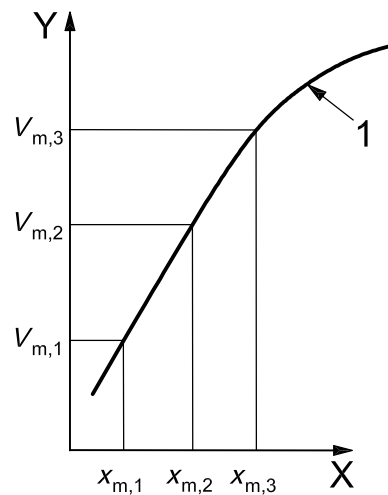**Key**

X particle size

Y median value of calibration particles

1 calibration curve

 $V_{m,1}$ median voltage corresponding to particle size $x_{m,1}$ $V_{m,2}$ median voltage corresponding to particle size $x_{m,2}$ $V_{m,3}$ median voltage corresponding to particle size $x_{m,3}$ **Figure 3 — Calibration curve**

NOTE When the median voltage is determined by using an external PHA, the uncertainty in the voltage of PHA and the voltage uncertainty of the LELPC are included in setting the voltage limits of the LELPC (see Annex A).

4.2 Verification of size setting

To test the verification of size setting of the LELPC, use the suspension of the certified reference material.

Set the LELPC to count in the cumulative mode, collect counts, C_C , at a setting greater than or equal to half particle size of the certified reference, and a particle size of 50 % counts of C_C . The size setting error is calculated as in Equation (1) below.

$$\varepsilon(\%) = \frac{x_s - x}{x} \times 100 \% \quad (1)$$

where

ε is the size setting error, in %;

x is the particle size of the certified reference material of liquid-borne particle number concentration, in μm ;

x_s is the particle size corresponding to 50 % counts of C_C , in μm .

NOTE The certified reference material of liquid-borne particle number concentration is suspended mono-disperse particles, such as PSL particles in pure water, and the particle number concentration was certified with this uncertainty.

4.3 Counting efficiency

To test the counting efficiency of the LELPC, use the suspension of the certified reference material.

Set the LELPC to count in the cumulative mode, collect counts at a setting greater than or equal to half particle size of the certified reference material.

Calculate the counting efficiency by means of Equation (2) below.

$$C_a = \frac{C_L}{C_R} \times 100 \% \quad (2)$$

where

C_a is the counting efficiency, in %;

C_L is the observed particle number concentration by the LELPC, in particles per cubic centimetre;

C_R is the particle number concentration of the certified reference material, in particles per cubic centimetre.

4.4 Size resolution

A certified reference material should be used for this test. The standard deviation of the calibration particles should be a known quantity, σ_P . Determine the median voltage (or channel), V_m , using calibration particles, as shown in Figure 4.

The lower voltage limit, V_l , and upper voltage limit, V_u , are defined as those corresponding to a density of 61 %. Using the calibration curve, determine the particle sizes corresponding to V_l and V_u . Calculate the absolute value of the differences in particle size between PSL particle size and particle size corresponding to V_l and V_u . The greater of these is the observed standard deviation, σ . Calculate the percentage of size resolution, R , of the LELPC by Equation (3) below (see also Annex B).

$$R(\%) = \frac{\sqrt{\sigma^2 - \sigma_P^2}}{x_P} \times 100 \% \quad (3)$$


where

R is the size resolution, in %;

σ is the observed standard deviation of LELPC, in μm ;

σ_P is the supplier's reported standard deviation of calibration particles, in μm ;

x_P is the particle size of the certified reference material, in μm .

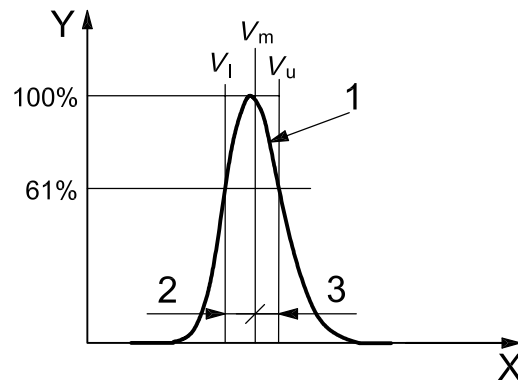

Key

X pulse height voltage (or channel)

Y density

1 pulse height distribution with PSL particles

2 lower side resolution

3 upper side resolution

V_l lower voltage limit

V_m median voltage

V_u upper voltage limit

Figure 4 — Size resolution

4.5 Maximum particle number concentration

The coincidence loss is determined by the flow rate, the time required for particles to pass through the sensing zone and the electrical signal processing time. These values are determined by the design of the LELPC. Coincidence loss is calculated as in Equation (4) below.

$$L(\%) = [1 - \exp(-q \cdot t \cdot C_{\max})] \times 100 \% \quad (4)$$

where

L is the coincidence loss, in %;

q is the flow rate, in cm^3/s ;

t is the time of passing through the sensing region plus electrical processing time, in s;

C_{\max} is the maximum particle number concentration, in particles per cubic centimetre.

NOTE If the particle number concentration becomes excessive, the coincidence error increases. This means several small particles are measured as one large particle.

4.6 Sampling flow rate

Obtain a flow rate by the sampling volume (see 4.8) and the sampling time (see 4.7), or use a calibrated flow meter. If the LELPC does not have a sampling function, this subclause does not apply.

4.7 Sampling time

Sampling time is the time during which the LELPC measures a sample (from the beginning of counting to the end of counting).

The sampling time tolerance is one minus the ratio of the measured sampling time, t , to the instrument's specified sampling time, t_0 . This is shown as $1 - \frac{t}{t_0}$.

Examine whether the sampling time tolerance satisfies the requirement given in 3.7. Calibrated instruments should be used for sampling time measurement.

If the LELPC does not have a sampling time function, this subclause does not apply.

4.8 Sampling volume

Measure the sampling volume by weighing the pure water with the balance and converting to volume, or measure the volume by means of a calibrated graduated cylinder.

If the LELPC does not have a sampling function, this subclause does not apply.

4.9 Calibration

Calibration at the calibration interval (see 3.9) should include at least size calibration, size resolution, counting efficiency and sampling volume uncertainty. If the LELPC does not have a sampling function, the standard uncertainty of sampling flow rate does not apply.

Annex A (informative)

Uncertainty of particle size calibration

A.1 Size calibration using external and internal PHA

Figure A.1 shows the particle size calibration using an external PHA and a voltmeter. In this case, there are four sources of uncertainty:

- PSL particles,
- PHA,
- voltmeter, and
- offset voltage at the size setting circuit.

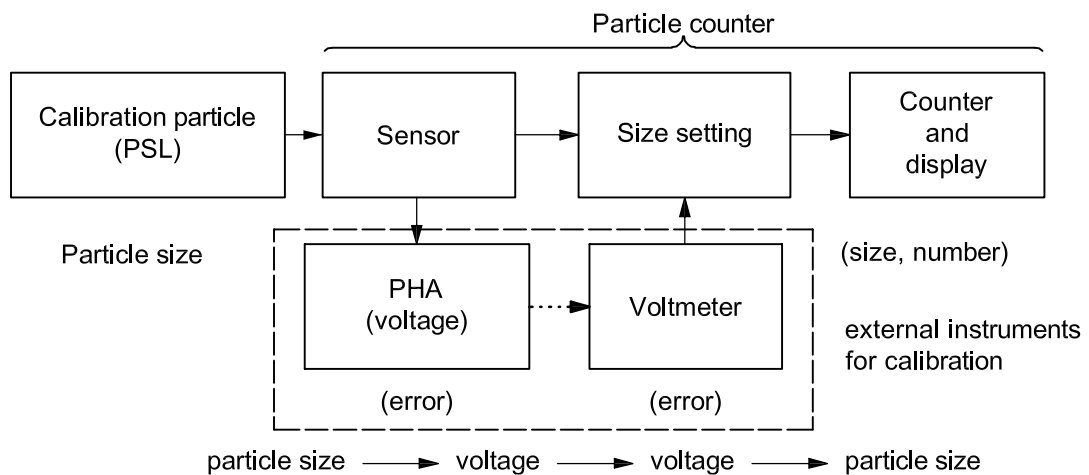


Figure A.1 — Particle size calibration using external instruments (PHA and voltmeter)

However, in Figure A.2, the uncertainty of particle size calibration depends only on the PSL particle size uncertainty.

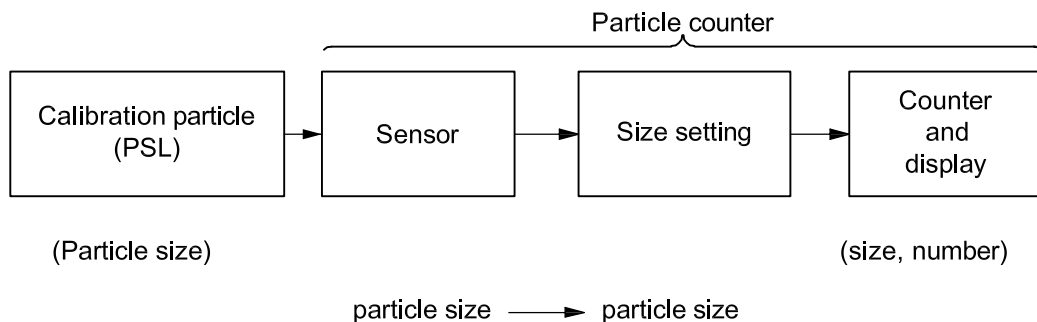


Figure A.2 — Particle size calibration using an internal PHA

A.2 Uncertainty of size calibration

Tables A.1 and A.2 show examples of uncertainty of size calibration. Table A.1 shows an example of combined standard uncertainty for size calibration using an external PHA and voltmeter. Table A.2 shows an example of combined standard uncertainty for size calibration using an internal PHA. The combined standard uncertainty for size calibration using an internal PHA is smaller than when using an external PHA.

Table A.1 — Relative standard uncertainty of size calibration using an external PHA (for example)

Items	Standard uncertainty %
PSL particles	2,5
PHA	2,5
Voltmeter	0,1
Offset voltage	0,5
Calibration curve	1,5
Combined standard uncertainty	3,9
Expanded uncertainty (k=2)	7,8

NOTE The standard uncertainty of the calibration curve is the uncertainty in the relationship between particle size and voltage limit or internal PHA channel.

Table A.2 — Relative standard uncertainty of size calibration using an internal PHA (for example)

Items	Standard uncertainty %
PSL particles	2,5
Calibration curve	1,5
Combined standard uncertainty	2,9
Expanded uncertainty (k=2)	5,8

NOTE The standard uncertainty of the calibration curve is the uncertainty in the relationship between particle size and voltage limit or internal PHA channel.

Annex B (informative)

Size resolution

Size resolution is defined as one standard deviation of the measured size distribution of monodisperse calibration particles, expressed as a percentage of the mean size of the monodisperse calibration particles.

If the distribution of calibration particles is assumed to be the Gaussian distribution,

$$f(x) = \frac{1}{\sqrt{2\pi}\sigma} \exp\left\{-\frac{1}{2}\left(\frac{x-\mu}{\sigma}\right)^2\right\} \quad (\text{B.1})$$

where

$f(x)$ is the Gaussian function;

x is the particle size;

μ is the mean value;

σ is the standard deviation.

When $(x - \mu) = \pm\sigma$, the ratio of density to the maximum density is $\exp\left(-\frac{1}{2}\right) \approx 0,61$. This is the basis for the use of 61 % in the determination of size resolution.

Bibliography

- [1] ISO 9276-1, *Representation of results of particle size analysis — Part 1: Graphical representation*
- [2] ASTM F658-00a (2006), *Standard Practice for Calibration of a Liquid-Borne Particle Counter Using an Optical System Based Upon Light Extinction*
- [3] JIS B 9925:1997, *Light scattering automatic particle counter for liquid*
- [4] Japanese Pharmacopoeia, 15th ed., *General Tests, Processes and Apparatus, Insoluble Particulate Matter Test for Injections*
- [5] United States Pharmacopoeia, *Physical Test and Determination, <788> Particulate matter in injections*
- [6] *Guide to the expression of uncertainty in measurement (GUM)*, BIPM, IEC, IFCC, ISO, IUPAC, IUPAP, OIML, 1993, corrected and reprinted in 1995

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover.
Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001.
Fax: +44 (0)20 8996 7001. Email: orders@bsi-global.com. Standards are also available from the BSI website at <http://www.bsi-global.com>.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre.
Tel: +44 (0)20 8996 7111. Fax: +44 (0)20 8996 7048. Email: info@bsi-global.com.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration.
Tel: +44 (0)20 8996 7002. Fax: +44 (0)20 8996 7001.
Email: membership@bsi-global.com.

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsi-global.com/bsonline>.

Further information about BSI is available on the BSI website at <http://www.bsi-global.com>.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright & Licensing Manager.
Tel: +44 (0)20 8996 7070. Fax: +44 (0)20 8996 7553.
Email: copyright@bsi-global.com.