

**Fine ceramics
(advanced ceramics,
advanced technical
ceramics) —
Test method for
antibacterial activity
of semiconducting
photocatalytic
materials**

ICS 81.060.30

National foreword

This British Standard is the UK implementation of ISO 27447:2009.

The UK participation in its preparation was entrusted to Technical Committee RPI/13, Advanced technical ceramics.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 30 June 2009.

© BSI 2009

ISBN 978 0 580 53006 7

Amendments/corrigenda issued since publication

Date	Comments

**Fine ceramics (advanced ceramics,
advanced technical ceramics) — Test
method for antibacterial activity of
semiconducting photocatalytic materials**

*Céramiques techniques — Méthode d'essai de l'activité antibactérienne
des matériaux photocatalytiques semiconducteurs*



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



COPYRIGHT PROTECTED DOCUMENT

© ISO 2009

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction.....	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Symbols.....	2
5 Principle.....	3
6 Materials	4
6.1 Bacteria used and preparation for tests	4
6.2 Chemicals and implements	5
7 Apparatus	6
7.1 Adhesive film	6
7.2 Adhesive glass.....	6
7.3 Moisture preservation glass.....	6
7.4 Glass tube or glass rod.....	7
7.5 Black light fluorescent lamp.....	7
7.6 Ultraviolet light radiation meter	7
7.7 Punched metal sheet.....	7
8 Test piece	8
8.1 Film adhesion method	8
8.2 Glass adhesion method	8
9 Procedure	9
9.1 Film adhesion method	10
9.2 Glass adhesion method	11
9.3 UV irradiation condition.....	12
9.4 Measurement of number of living bacteria	12
10 Calculation	13
10.1 Film adhesion method	13
10.2 Glass adhesion method	14
11 Test report.....	16
Annex A (informative) Examples of test results	17
Annex B (informative) Reference data for adhesive films and adhesive glasses	19
Annex C (informative) Reference data for damage of ultraviolet irradiation to bacteria.....	21
Bibliography.....	23

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 27447 was prepared by Technical Committee ISO/TC 206, *Fine ceramics*.

Introduction

As a result of continuing efforts to provide test methods for photocatalytic materials, this International Standard was developed for antibacterial activity. However, for test pieces with permeable or rough surfaces, etc., the antibacterial activity cannot be measured, so other test methods are required.

Under the irradiation of photons, photocatalysts show diverse functions, such as the decomposition of air and water contaminants, as well as deodorization, self-cleaning, antifogging and antibacterial actions. These functions of photocatalysts are generally based on the action of active oxygen species such as hydroxyl (OH) radicals formed on the surface of the photocatalyst (References [10] and [11] in the Bibliography). The energy- and labour-saving nature of photocatalysis has attracted keen interest when the photocatalyst is activated by sunlight (or artificial lighting).

Practical applications of photocatalysts, for both indoor and outdoor use, have rapidly expanded in recent years. Many kinds of photocatalytic materials have been proposed or are already commercialized, based on ceramics, glass, concrete, plastics, paper, etc. Such materials are produced by either the coating or mixing of a photocatalyst; in most cases, titanium dioxide (TiO₂).

However, the effect of photocatalysis is not easily inspected visually, and no appropriate and official evaluation methods have been available to date. Some confusion has thus arisen as photocatalytic materials have been introduced. Furthermore, the above-mentioned diverse functions of photocatalysts cannot be evaluated with a single method; thus, it is required to provide different evaluation methods for air purification, water decontamination and self-cleaning.

This International Standard applies to testing the antibacterial activity of photocatalytic ceramics and other materials produced by either the coating or mixing of a photocatalyst. Standards for testing the antifungal activity that use photocatalytic materials will be developed separately.

Fine ceramics (advanced ceramics, advanced technical ceramics) — Test method for antibacterial activity of semiconducting photocatalytic materials

WARNING — Handling and manipulation of microorganisms that are potentially hazardous requires a high degree of technical competence. Only personnel trained in microbiological techniques should carry out tests.

1 Scope

This International Standard specifies a test method for the determination of the antibacterial activity of materials that contain a photocatalyst or have photocatalytic films on the surface, by measuring the enumeration of bacteria under irradiation of ultraviolet light.

This International Standard is intended for use with different kinds of semiconducting photocatalytic materials used in construction materials, in flat sheet, board, plate shape or textiles that are the basic forms of materials for various applications. It does not include powder, granular or porous photocatalytic materials.

This test method is usually applicable to photocatalytic materials produced for an antibacterial effect. Other types of performance of photocatalytic materials, i.e. decomposition of water contaminants, self-cleaning, antifogging and air purification, are not determined by this method.

The values expressed in this International Standard are in accordance with the International System of Units (SI).

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 31-0, *Quantities and units — Part 0: General principles*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

photocatalyst

substance that carries out many functions based on oxidization and reduction reactions under ultraviolet (UV) irradiation, including decomposition and removal of air and water contaminants, deodorization, and antibacterial, self-cleaning and antifogging actions

3.2

photocatalytic materials

materials in which, or on which, the photocatalyst is added by coating, impregnation, mixing, etc.

NOTE Photocatalytic materials are to be used for building and road construction materials to obtain the functions mentioned in 3.1.

3.3 antibacterial

condition inhibiting the growth of bacteria on the surface of flat surface materials or cloths

3.4 photocatalyst antibacterial activity value for film adhesion method

difference between the total number of viable bacteria of photocatalytic treated flat surface materials and non-treated materials after UV irradiation

NOTE This value includes the decrease of the number of bacteria without UV irradiation.

3.5 photocatalyst antibacterial activity value for glass adhesion method

difference between the total number of viable bacteria of photocatalytic treated cloths and standard cloths after UV irradiation

NOTE This value includes the decrease of the number of bacteria without UV irradiation.

3.6 photocatalyst antibacterial activity value with UV irradiation for film adhesion method

difference between the total number of viable bacteria of photocatalytic treated flat surface materials after UV irradiation and photocatalytic treated flat surface materials in a dark place

3.7 photocatalyst antibacterial activity value with UV irradiation for glass adhesion method

difference between the total number of viable bacteria of photocatalytic treated cloths after UV irradiation and photocatalytic treated cloths in a dark place

3.8 film adhesion method

test method to evaluate the antibacterial performance of photocatalytic flat surface materials

3.9 glass adhesion method

test method to evaluate the antibacterial performance of photocatalytic cloths

3.10 fluorescent UV lamp

lamp that provides UV-A irradiation within a wavelength range of 300 nm to 400 nm

NOTE A suitable lamp is the so-called black light blue (BLB) fluorescent lamp, with a maximum at 351 nm, as described in ISO 4892-3.

4 Symbols

A average number of viable bacteria of non-treated specimens, just after inoculation

B_D average number of viable bacteria of non-treated specimens, after being kept in a dark place

B_L average number of viable bacteria of non-treated specimens, after UV irradiation of intensity L

C_D average number of viable bacteria of photocatalytic treated specimens, after being kept in a dark place

C_L average number of viable bacteria of photocatalytic treated specimens, after UV irradiation of intensity L

F_{BD} growth value, after being kept in a dark place

F_{BL} growth value, after UV irradiation of intensity L

L	UV irradiation intensity
L_{\max}	maximum logarithmic value of viable bacteria
L_{mean}	average logarithmic value of viable bacteria for 3 specimens
L_{\min}	minimum logarithmic value of viable bacteria
M	number of viable bacteria with glass adhesion method
M_{BA}	average logarithmic value of the number of viable bacteria for 3 non-treated specimens, just after inoculation
M_{BD}	average logarithmic value of the number of viable bacteria for 3 non-treated specimens, after being kept in a dark place
M_{BL}	average logarithmic value of the number of viable bacteria for 3 non-treated specimens, after UV irradiation of intensity L
M_{D}	average logarithmic value of the number of viable bacteria for 3 photocatalytic treated specimens, after being kept in a dark place
M_{L}	average logarithmic value of the number of viable bacteria for 3 photocatalytic treated specimens, after UV irradiation of intensity L
N	number of viable bacteria with film adhesion method
P	bacteria concentration
R	dilution factor
R_L	photocatalyst antibacterial activity value, after irradiation at a constant intensity (L) on a photocatalytic material
ΔR	photocatalyst antibacterial activity value with UV irradiation
S_L	photocatalyst antibacterial activity value, after UV irradiation of intensity L
ΔS	photocatalyst antibacterial activity value with UV irradiation
V	volume of soybean casein digest broth with lecithin and polysorbate 80 medium for washout
Z	average number of colonies in 2 Petri dishes

5 Principle

This International Standard is for the development, comparison, quality assurance, characterization, reliability, and design data generation of photocatalytic materials. The method is used to obtain the antibacterial activity of photocatalytic materials by the contact of a specimen with bacteria, under UV light irradiation. The film adhesion method is available for flat sheet, board or plate-shaped materials. To avoid warpage in the cloths or textiles, the glass adhesion method is available for cloths or textiles.

The specimen is laid in a Petri dish and the bacterial suspension is dripped onto the specimen. Then the adhesive film or glass is placed on the suspension and the moisture conservation glass is placed on top of the Petri dish. The Petri dish containing the specimen is exposed to light. After exposure, the test bacteria are washed out of the specimen and the adhesive film or glass. This washout suspension is measured by the viable bacterial count method.

6 Materials

6.1 Bacteria used and preparation for tests

6.1.1 Film adhesion method

- a) *Staphylococcus aureus*
- b) *Escherichia coli*

6.1.2 Glass adhesion method

- a) *Staphylococcus aureus*
- b) *Klebsiella pneumoniae*

6.1.3 Bacteria preparation

The bacteria strains to be used in the test are equivalent to those described in Table 1 and are stored by entities that are registered under the World Federation for Culture Collections or the Japan Society for Culture Collections.

Aseptic manipulations using microorganisms can be performed in an adequate safety cabinet. Inoculate each strain into a slant culture medium (nutrient agar medium), incubate for 16 h to 24 h at $37\text{ °C} \pm 1\text{ °C}$, and then store in a refrigerator at 5 °C to 10 °C . Repeat subcultures within 1 month by replicating this process. The maximum number of subcultures from the original strain transferred by culture collection is 10. The slant culture must not be used for further storage after 1 month.

NOTE 1 In the case of bacteria stored in a deep freezer, the maximum number of subcultures from the original strain transferred by culture collection is 10.

NOTE 2 If necessary, additional tests with other bacteria can be allowed.

Table 1 — Bacteria strains to be used in test

Bacteria species	Strain number	Organization for the collection
<i>Staphylococcus aureus</i>	ATCC 6538P	American Type Culture Collection
	DSM 346	German Collection of Microorganisms and Cell Cultures (DSMZ)
	NBRC 12732	NITE Biological Resource Center
<i>Escherichia coli</i>	ATCC 8739	American Type Culture Collection
	DSM 1576	German Collection of Microorganisms and Cell Cultures (DSMZ)
	NBRC 3972	NITE Biological Resource Center
<i>Klebsiella pneumoniae</i>	ATCC 4352	American Type Culture Collection
	DSM 789	German Collection of Microorganisms and Cell Cultures (DSMZ)
	NBRC 13277	NITE Biological Resource Center

6.2 Chemicals and implements

6.2.1 1/500 nutrient broth

For 1 000 ml of purified water, take 3,0 g of meat extract, 10,0 g of peptone and 5,0 g of sodium chloride, put them in a flask and dissolve them thoroughly. When the contents are thoroughly diluted, use a solution of sodium hydroxide or hydrochloric acid to bring the pH to $(7,1 \pm 0,1)$ at 25 °C. Dilute this medium 500 times using purified water, and set the pH to $(7,0 \pm 0,2)$ using hydrochloric acid solution or sodium hydroxide solution. Sterilize in an autoclave at $121 \text{ °C} \pm 2 \text{ °C}$ for at least 15 min. After preparation, if 1/500 nutrient broth is not used immediately, store it at 5 °C to 10 °C. Do not use 1/500 nutrient broth made more than 1 month ago.

6.2.2 Nutrient broth

For 1 000 ml of purified water, take 3,0 g of meat extract, 10,0 g of peptone and 5,0 g of sodium chloride, put them in a flask and dissolve them thoroughly. When the contents are thoroughly diluted, use a solution of sodium hydroxide or hydrochloric acid to bring the pH to $(7,1 \pm 0,1)$ at 25 °C. If necessary, dispense the contents in a test tube, add a cotton plug and sterilize in an autoclave (see 6.2.1). After preparation, if nutrient broth is not used immediately, store it at 5 °C to 10 °C. Do not use nutrient broth made more than 1 month ago.

6.2.3 Nutrient agar

For 1 000 ml of purified water, take 3,0 g of meat extract, 5,0 g of peptone and 15,0 g of agar powder, put them in a flask and mix. Heat the flask in boiling water to dissolve the contents thoroughly. Use a 0,1 mol/l solution of sodium hydroxide to bring the pH to $(6,8 \pm 0,2)$ at 25 °C. Add a cotton plug and sterilize in an autoclave (see 6.2.1). After preparation, if nutrient agar is not used immediately, store it at 5 °C to 10 °C. Do not use nutrient agar made more than 1 month ago. Keep the medium temperature between 45 °C and 48 °C when mixing with a bacterial suspension.

6.2.4 Soybean-casein digest broth with lecithin and polysorbate 80 (SCDLP)

For 1 000 ml of purified water, take 17,0 g of casein peptone, 3,0 g of soybean peptone, 5,0 g of sodium chloride, 2,5 g of phosphoric acid monopotassium dehydrogenate, 2,5 g of glucose and 1,0 g of lecithin, put them in a flask and dissolve them. Add 7,0 g of non-ionic surfactant and dissolve it. Use a solution of sodium hydroxide or hydrochloric acid to bring the pH to $(7,0 \pm 0,2)$ at 25 °C. If necessary, dispense it in a test tube, add a cotton plug and sterilize in an autoclave (see 6.2.1). After preparation, if SCDLP is not used immediately, store it at 5 °C to 10 °C. Do not use SCDLP medium made more than 1 month ago.

6.2.5 Physiological saline solution

For 1 000 ml of purified water, take 8,5 g of sodium chloride, put it in a flask and dissolve it thoroughly. If necessary, dispense it in a test tube and sterilize in an autoclave (see 6.2.1). After preparation, if physiological saline solution is not used immediately, store it at 5 °C to 10 °C. Do not use physiological saline solution made more than 1 month ago.

6.2.6 Physiological saline solution for washout


For 1 000 ml of purified water, take 8,5 g of sodium chloride, put it in a flask and dissolve it thoroughly. Add 2,0 g of non-ionic surfactant and dilute. If necessary, dispense 20 ml of the solution in a test tube or Erlenmeyer flask and sterilize in an autoclave (see 6.2.1). After preparation, if physiological saline solution for washout is not used immediately, store it at 5 °C to 10 °C. Do not use physiological saline solution made more than 1 month ago for washout.

6.2.7 Non-ionic surfactant

Polyoxyethylene sorbitan monooleate (polysorbate 80).

7 Apparatus

The test equipment enables a photocatalytic material to be examined for its antibacterial activity by providing UV irradiation to activate the photocatalyst. It consists of a light source and a chamber with a test piece. An example of a test system is shown in Figure 1.

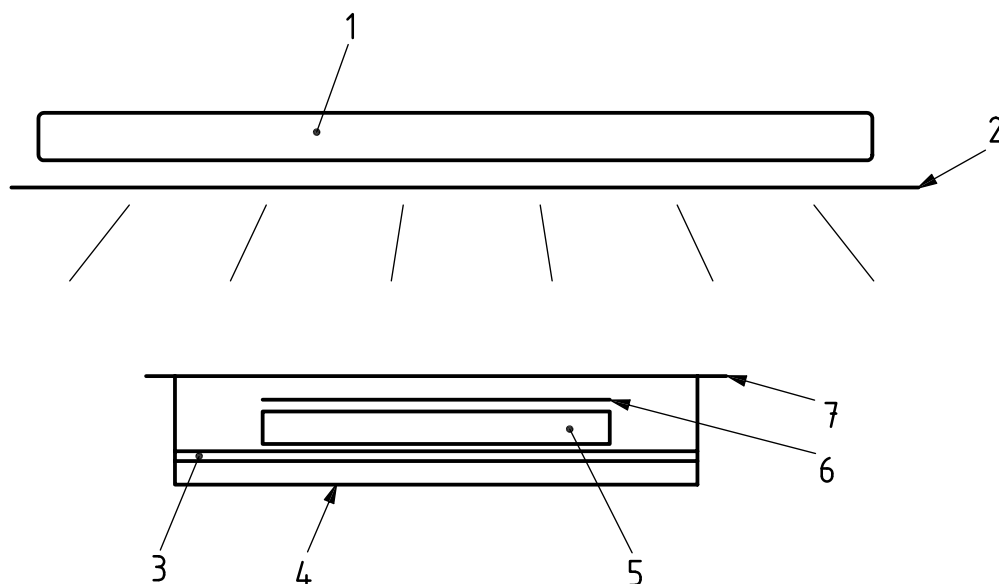

Key

- 1 light source
- 2 punched metal
- 3 glass stick
- 4 paper filter
- 5 test piece
- 6 adhesive film or glass
- 7 moisture preservation glass

Figure 1 — Schematic diagram of the test equipment

7.1 Adhesive film

The adhesive film is inert and non-water absorbent with good sealing properties, with a transparency rate over 85 % for the 340 nm to 380 nm range. The sheets are cut with dimensions of (40 ± 2) mm.

NOTE Reference data for adhesive films is given in Annex B.

7.2 Adhesive glass

The adhesive glass consists of glass panes with a thickness less than or equal to 1,1 mm, with a transparency rate over 85 % for the 340 nm to 380 nm range. The panes are cut with dimensions of (40 ± 2) mm.

NOTE Reference data for adhesive glasses is given in Annex B.

7.3 Moisture preservation glass

The moisture preservation glass consists of glass panes with a thickness less than or equal to 1,1 mm, with a transparency rate over 85 % for the 340 nm to 380 nm range. The panes are cut to fully cover Petri dishes.

7.4 Glass tube or glass rod

The glass tube or glass rod is prepared by cutting a tube or rod to a 10 cm to 15 cm length and bending it into a U-shape or V-shape.

7.5 Black light fluorescent lamp


The fluorescent lamp shall be a BLB (black light blue) lamp that has a peak wavelength of 351 nm with blue glass for absorbing visible light.

7.6 Ultraviolet light radiation meter

The irradiation intensity shall be measurable at the test sample position. The UV radiation meter shall be calibrated for the light source to be used or corrected to ascertain sensitivity within the wavelength range to be absorbed by the photocatalytic test piece.

7.7 Punched metal sheet


When the prescribed intensity cannot be obtained by tuning the light source height, attenuate the intensity by using a punched metal sheet (see Figures 2 and 3) directly below the lamp.

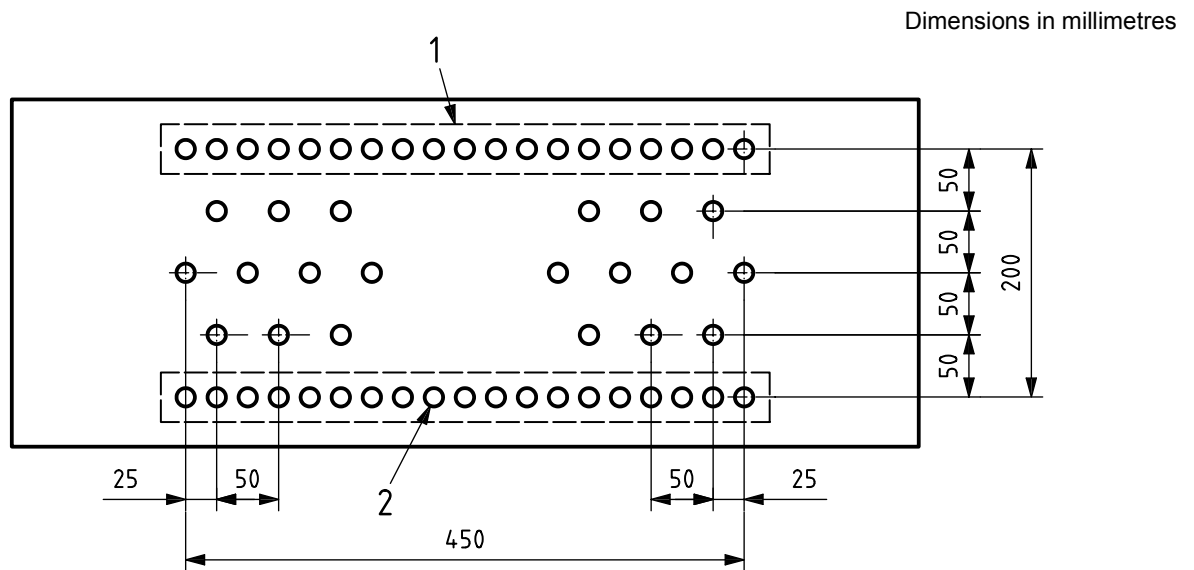

Key

- 1 lamp position
- 2 bore (diameter approximately 5 to 15)

Figure 2 — Punched metal sheet for 0,01 mW/cm² light intensity

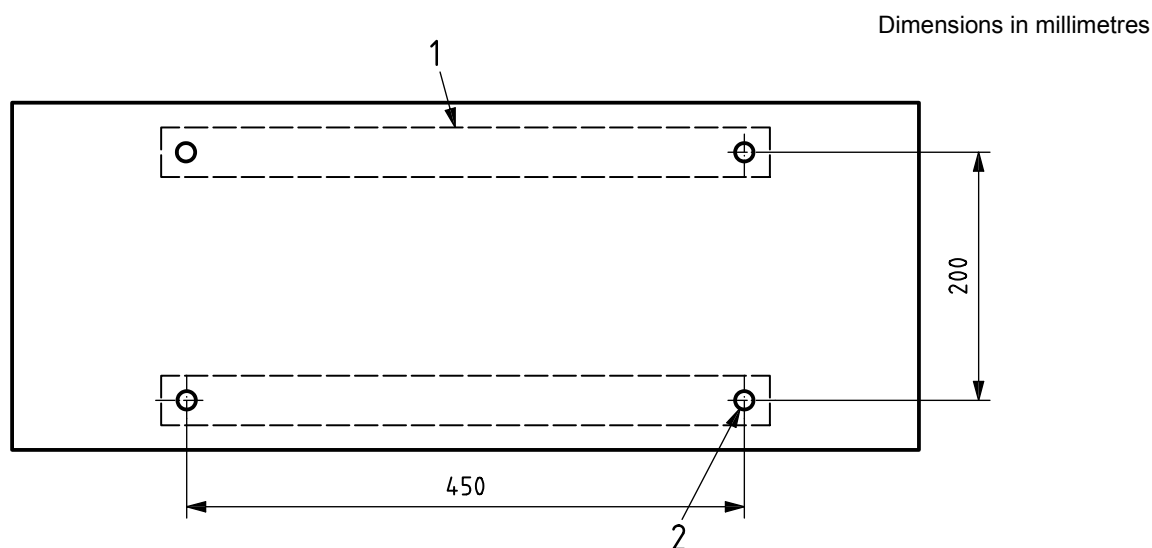

Key

- 1 lamp position
- 2 bore (diameter approximately 5 to 15)

Figure 3 — Punched metal sheet for 0,001 mW/cm² light intensity

8 Test piece

8.1 Film adhesion method

Cut a flat portion of the material in a (50 ± 2) mm \times (50 ± 2) mm square. The materials should be up to 10 mm in thickness. Use it as the standardized shaped specimen. Prepare 9 pieces of non-treated specimens and 6 pieces of photocatalytic treated specimens. When non-treated specimens cannot be provided, use glass panes instead. Take great care to avoid microbial contamination and cross-contamination among specimens.

NOTE When it is difficult or impossible to cut (50 ± 2) mm long (up to 10 mm thickness) squares, it is acceptable to use a different specimen size as long as the specimen surface can be covered with a 400 mm² to 1 600 mm² film. When the specimen surface is stained with organic contaminant, it is acceptable to first eliminate the contaminant by exposure to a 1,0 mW/cm² light source within the limit of 24 h. If necessary, specimens can be disinfected prior to testing (e.g. by wiping with ethanol or 70 % ethanol in water).

8.2 Glass adhesion method

Cut the material into (50 ± 2) mm \times (50 ± 2) mm squares and use them as specimens. Prepare 9 pieces of standard cloth and 6 pieces of photocatalytic treated specimens. Take great care to avoid microbial contamination and cross-contamination among specimens.

Put each of the specimens in a glass Petri dish. Put the dishes in a wire-mesh basket, cover the upper part with aluminum foil and sterilize them in an autoclave. After autoclaving, take off the aluminum foil, move the cover of the dishes to a clean bench and dry the specimens for about 60 min.

9 Procedure

The flowcharts of test methods are shown in Figures 4 and 5.

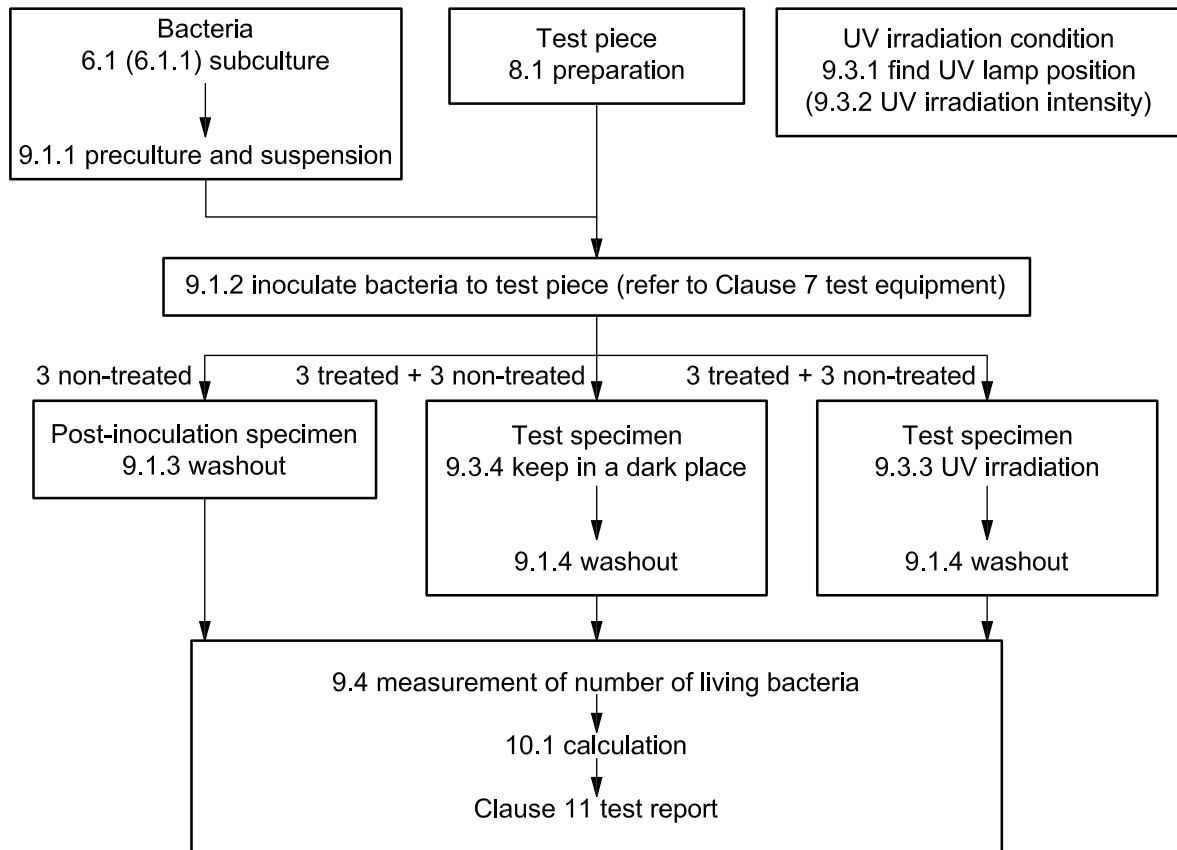


Figure 4 — Flowchart of film adhesion method

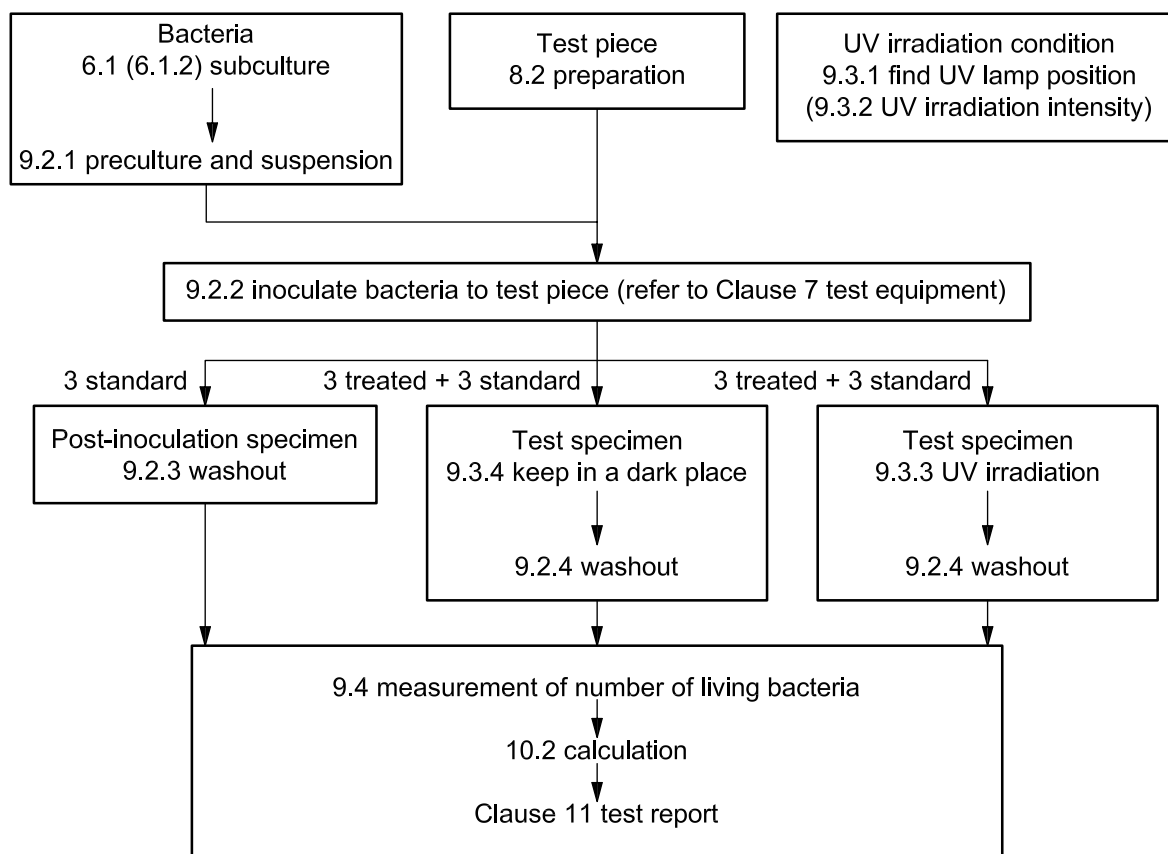


Figure 5 — Flowchart of glass adhesion method

9.1 Film adhesion method

9.1.1 Transfer the stored bacteria to the nutrient agar slant using a platinum loop and incubate at $(37 \pm 1)^\circ\text{C}$ for 16 h to 24 h. Transfer the bacteria to a new nutrient agar slant and incubate at $(37 \pm 1)^\circ\text{C}$ for 16 h to 20 h. Uniformly disperse a small quantity of test bacteria in 1/500 NB with a platinum loop, and measure the bacteria count using the optical microscope observation method or any other adequate method. Suitably dilute this bacteria suspension with 1/500 NB to obtain a count of $6,7 \times 10^5$ cells/ml to $2,6 \times 10^6$ cells/ml and use the result as the bacterial suspension for the test. If the test bacteria suspension is not to be used immediately, store it at 0°C and use it within 4 h.

9.1.2 Lay a sterilized moisture control paper filter in the bottom of a sterilized Petri dish, add an adequate quantity of sterilized water, intercalate a glass tube or glass rod in order to avoid contact between the test piece and the paper filter, and place the test piece on it with the photocatalytic treated surface up. Collect exactly 0,15 ml of test bacterial suspension with a sterilized pipette and drip it onto each test piece. Put a film on top of the dripped suspension and lightly push to get the suspension to spread to the whole film surface, while taking care that no suspension leaks out of the film edge. Then place a moisture conservation glass on the top of the Petri dish. Except for 3 non-treated specimens for a viable cell count performed just after the test bacterial suspension is inoculated, proceed with the irradiation test described in 9.3.

NOTE 1 4 ml to 6 ml sterilized water added per Petri dish is adequate.

NOTE 2 The regulated suspension quantity can create leakage of suspension from the film edge or might not be enough to spread the suspension uniformly. In such a case, it is acceptable to reduce down to half the quantity of suspension or increase to twice the quantity of suspension. However, even when the bacterial suspension quantity for inoculation has been changed, the count per specimen must be the same as with the standard size specimen, with $1,0 \times 10^5$ cells to $4,0 \times 10^5$ cells.

The quantity of test bacterial suspension for inoculation in the case of non-standard size specimens shall be proportional to the film area used.

9.1.3 For the 3 non-treated bacterial suspension inoculated specimens for the test (post-inoculation specimen of test bacteria), put the adherence film and non-treated test piece in a Stomacher bag using sterilized tweezers, taking care to avoid bacterial suspension leakage from the film and non-treated test piece. Add 10 ml of SCDLP, rub the specimens and the film well from outside the Stomacher bag by hand and washout the test bacteria. Quickly use this washout solution to perform a measurement of the number of viable cells.

Alternative equivalents of the Stomacher bag may be used if they can be shown to lead to the same results.

9.1.4 For the specimens of 9.3.3 and 9.3.4, perform the washout in the same manner as in 9.1.3.

9.2 Glass adhesion method

9.2.1 The test bacterial suspension cultivation is processed in the following way.

- a) Inoculate stock strain to the nutrient agar medium with a platinum loop. Incubate for 24 h to 48 h at $(37 \pm 1) ^\circ\text{C}$ (incubation A). Stock the medium at $5 ^\circ\text{C}$ to $10 ^\circ\text{C}$ and use within 1 week.
- b) Put 20 ml of nutrient culture in a 100 ml Erlenmeyer flask. Collect a colony with a platinum loop from incubation A, inoculate and incubate with agitation (110 min^{-1} with about 3 cm of amplitude) during 18 h to 24 h at $(37 \pm 1) ^\circ\text{C}$ (incubation B).
- c) Put 20 ml of nutrient culture in a 100 ml Erlenmeyer flask. Add 0,4 ml of bacterial suspension of incubation B with a 1×10^8 cells/ml to 2×10^8 cells/ml bacteria concentration and incubate with agitation (110 rpm with about 3 cm of amplitude) during (3 ± 1) h at $(37 \pm 1) ^\circ\text{C}$ to reach 10^7 cells/ml (incubation C).
- d) Estimate the bacteria concentration of the incubation C using the optical density absorbance method or the optical microscope observation method. Dilute the nutrient broth by 20 times at room temperature using purified water, cool it and use it to tune the bacteria concentration of incubation C at $(1 \pm 0,3) \times 10^5$ cells/ml. Use the resulting suspension as test material. If the test bacteria suspension is not to be used immediately, store it at $0 ^\circ\text{C}$ and use it within 4 h.

9.2.2 Lay a sterilized moisture control paper filter in the bottom of a sterilized Petri dish, add an adequate quantity of sterilized water, intercalate a glass tube or glass rod in order to avoid contact between the test piece and the paper filter, place the sterilized glass on it and place the test piece on the sterilized glass with the photocatalyst treated surface up. Collect exactly 0,2 ml of test bacterial suspension with a sterilized pipette and drip it on each test piece. Put a glass on top of the dripped suspension and lightly push to get the suspension to spread to the whole glass surface, while taking care that no suspension leaks out of the glass edge. Then place a moisture conservation glass on the top. Except for 3 standard cloth pieces for viable cell count performed just after the test bacterial suspension is inoculated, proceed with the irradiation test described in 9.3.

NOTE 1 4 ml to 6 ml sterilized water added per Petri dish is adequate.

NOTE 2 The regulated suspension quantity can create leakage of suspension from the edge or might not be enough to soak the suspension uniformly. In such a case, it is acceptable to reduce down to half the quantity of suspension or to increase to twice the quantity of suspension. However, even when the bacterial suspension quantity for inoculation has been changed, the count per specimen must be the same as with the standard size specimen, with $1,4 \times 10^4$ cells to $2,6 \times 10^4$ cells.

NOTE 3 In order to well permeate the sample with the test bacterial suspension, it is acceptable to use a test bacterial suspension containing 0,05 % of non-ionic surfactant. When using non-ionic surfactant in the test bacterial suspension, record the information in the output report.

9.2.3 For the 3 standard cloth pieces (post-inoculation specimen of test bacteria), put the adherence sterilized glass, non-treated cloths and glass pane in a Stomacher bag using sterilized tweezers, taking care to avoid bacterial suspension leakage. Add 20 ml of physiological saline solution for washout, rub the

Stomacher bag well by hand and also the non-treated cloths and the glasses, and washout the test bacteria. Quickly use this washout solution to perform measurement of the number of viable cells.

Alternative equivalents of the Stomacher bag may be used if they can be shown to lead to the same results.

9.2.4 For the specimens of 9.3.3 and 9.3.4, perform the washout in the same manner as in 9.2.3.

9.3 UV irradiation condition

9.3.1 Set the photoelectric sensor of a UV radiometer on the base of the irradiation apparatus. Place the film and glass plate used for testing on top of the sensor. Find the positions where UV intensity referred to 9.3.2 is complied with by reading the indicator value.

9.3.2 Test the UV intensity condition, depending on the circumstances where the materials are used. When the prescribed UV intensity cannot be obtained by tuning the height of the light source, attenuate the intensity by using a punched metal sheet.

Table 2 — UV irradiation intensity to be referred to in test

UV intensity	Example
0,25 mW/cm ²	Beside the window in the daytime, beside the assistant lamp for photocatalytic reaction (e.g. BLB)
0,10 mW/cm ²	In the room (inside, about 1,5 m from the window) in the daytime, by the window in the early morning or before sunset
0,01 mW/cm ²	In the room (inside, about 3 m from the window) in the daytime
0,001 mW/cm ²	In the room without a window (only indoor light), in the room at night (only indoor light)

NOTE The maximum UV intensity is 0,25 mW/cm² to avoid damage by UV irradiation only. The minimum UV intensity of the photoelectric sensor at present is 0,001 mW/cm². Reference data for damage of UV irradiation to bacteria is given in Annex C.

9.3.3 Expose to light the Petri dishes containing the specimens (3 non-treated specimens and 3 photocatalytic treated specimens) with bacterial suspension for 8 h.

NOTE This exposure time could be reduced to 4 h to take into account the real conditions where the photocatalytic material is effectively used.

9.3.4 Keep the Petri dishes containing the specimens (3 non-treated specimens and 3 photocatalytic treated specimens) with bacterial suspension in a dark place, for the same time as in 9.3.3.

9.4 Measurement of number of living bacteria

1 ml of washout solution is taken with a sterilized pipette and added to (9 ± 0,1) ml of physiological saline solution in a test tube and thoroughly agitated. 1 ml of the solution is extracted with a new sterilized pipette and added to another test tube containing (9 ± 0,1) ml of physiological saline solution and thoroughly agitated again. This process is repeated to obtain a series of dilutions, in compliance with the 10-times dilution method. 1 ml of the solution from the tubes of each series is extracted with new sterilized pipettes and placed in two Petri dishes each. 15 ml to 20 ml of nutrient agar kept at 45 °C to 48 °C is added to each Petri dish; allow them to stand for 15 min at room temperature. When the agar medium solidifies, the Petri dishes are placed upside down and incubated for 40 h to 48 h at (37 ± 1) °C. Colony numbers are counted in the series of Petri dishes with 30 colonies to 300 colonies. The bacteria concentration of the washout liquid is obtained by Equation (1) and expressed to two significant digits.

$$P = Z \times R \quad (1)$$

where

- P is the bacteria concentration (cells/ml);
- Z is the average number of colonies in 2 Petri dishes;
- R is the dilution factor.

When the number of viable bacteria is less than 30 in the Petri dishes with 1 ml of washout solution, the cell number is used to calculate the average number. When the number of viable bacteria is less than 1 in the Petri dishes with 1 ml of wash-out solution, the average number is taken as 1.

10 Calculation

The test results are calculated as follows. The calculated values are usually rounded to the second decimal place in accordance with ISO 31-0.

NOTE Examples of text results are given in Annex A.

10.1 Film adhesion method

10.1.1 Test requirement fulfilment validation

Use the bacteria concentration obtained in 9.4 and apply Equation (2) to calculate the number of viable bacteria.

$$N = P \times V \quad (2)$$

where

- N is the number of cells of viable bacteria;
- P is the bacteria concentration obtained in 9.4 (cells/ml);
- V is the volume of SCDLP medium for washout (ml).

A test is considered valid if it fulfils all of the following 4 items. If one or more of these items are not fulfilled, the test is considered as not valid and shall be performed again.

- 1) The logarithmic value of the number of viable bacteria of non-treated specimens after inoculation is derived from Equation (3)

$$(L_{\max} - L_{\min}) / (L_{\text{mean}}) \leq 0,2 \quad (3)$$

where

- L_{\max} is the maximum logarithmic value of viable bacteria;
 - L_{\min} is the minimum logarithmic value of viable bacteria;
 - L_{mean} is the average logarithmic value of viable bacteria for 3 specimens.
- 2) The logarithmic value of viable bacteria of non-treated specimens after inoculation shall be within the $1,0 \times 10^5$ to $4,0 \times 10^5$ cells range.

- 3) The viable bacteria of non-treated specimens after light exposure shall be more than $1,0 \times 10^3$ cells for all 3 specimens. However, when a glass pane is used as the non-treated specimen, the number of viable bacteria after light exposure shall be more than $1,0 \times 10^4$ cells.
- 4) After being kept in a dark place, the viable bacteria of non-treated specimens shall be more than $1,0 \times 10^3$ cells for all 3 specimens. However, when a glass pane is used as the non-treated specimen, the number of viable bacteria after light exposure shall be more than $1,0 \times 10^4$ cells.

10.1.2 Photocatalyst antibacterial activity value calculation

Use Equations (4) and (5) to calculate the photocatalyst antibacterial activity value after the test is completed.

Delete the second decimal and express the value with one decimal.

$$R_L = [\log(B_L/A) - \log(C_L/A)] = \log[B_L/C_L] \quad (4)$$

where

R_L is the photocatalyst antibacterial activity value, after UV irradiation of intensity L ;

L is the UV irradiation intensity (mW/cm^2);

A is the average number of viable bacteria of non-treated specimens, just after inoculation;

B_L is the average number of viable bacteria of non-treated specimens, after UV irradiation of intensity L ;

C_L is the average number of viable bacteria of photocatalytic treated specimens, after UV irradiation of intensity L .

$$\Delta R = \log[B_L/C_L] - [\log(B_D/A) - \log(C_D/A)] = \log[B_L/C_L] - \log[B_D/C_D] \quad (5)$$

where

ΔR is the photocatalyst antibacterial activity value with UV irradiation;

B_D is the average number of viable bacteria of non-treated specimens, after being kept in a dark place;

C_D is the average number of viable bacteria of photocatalytic treated specimens, after being kept in a dark place.

10.2 Glass adhesion method

10.2.1 Test requirement fulfilment validation

Use the bacteria concentration obtained in 9.4 and apply Equation (6) to calculate the number of viable bacteria.

$$M = P \times 20 \quad (6)$$

where

M is the number of cells of viable bacteria;

P is the bacteria concentration obtained in 9.4 (cells/ml);

20 is the quantity of physiological saline solution for washout (ml).

Test requirement validation uses the propagation value. The propagation value is obtained by Equations (7) and (8). The last 2 digits are rounded off. If the propagation value is over 0, the test is validated. If it is under 0, the test is not validated and shall be performed again.

$$F_{BL} = M_{BL} - M_{BA} \quad (7)$$

where

F_{BL} is the growth value, after UV irradiation of intensity L ;

L is the UV irradiation intensity (mW/cm²);

M_{BL} is the average logarithmic value of the number of viable bacteria for 3 non-treated specimens, after UV irradiation of intensity L ;

M_{BA} is the average logarithmic value of the number of viable bacteria for 3 non-treated specimens, just after inoculation.

$$F_{BD} = M_{BD} - M_{BA} \quad (8)$$

where

F_{BD} is the growth value, after being kept in a dark place;

M_{BD} is the average logarithmic value of the number of viable bacteria for 3 non-treated specimens, after being kept in a dark place.

10.2.2 Photocatalyst antibacterial activity value calculation

For the completed test, the photocatalyst antibacterial activity value is obtained with up to 2 digits using Equations (9) and (10).

$$S_L = M_{BL} - M_L \quad (9)$$

where

S_L is the photocatalyst antibacterial activity value, after UV irradiation of intensity L ;

M_L is the average logarithmic value of the number of viable bacteria for 3 photocatalytic treated specimens, after UV irradiation of intensity L .

$$\Delta S = (M_{BL} - M_L) - (M_{BD} - M_D) \quad (10)$$

where

ΔS is the photocatalyst antibacterial activity value with UV irradiation;

M_D is the average logarithmic value of the number of viable bacteria for 3 photocatalytic treated specimens, after being kept in a dark place.

11 Test report

The test report shall include the following information:

- a) description of the type, size, shape and thickness of the photocatalyst and non-treated specimens;
- b) description of conditions of pre-exposure when applied;
- c) type of test bacteria and bacteria strain number;
- d) manufacturer of fluorescent UV lamp and product number;
- e) manufacturer of ultraviolet light radiometer and product number;
- f) light exposure conditions including UV irradiation intensity and light exposure duration;
- g) in the film adhesion method, type and size of adhesive film and moisture preservation glass; quantity of inoculated test bacterial suspension; number of viable bacteria in the test suspension; values of A , B_L , C_L , R_L , B_D , C_D , ΔR in 10.1.2;
- h) in the glass adhesion method, type and size of adhesive glass and moisture preservation glass; type of test bacteria; bacteria strain number; inoculated bacteria concentration; values of S_L , ΔS in 10.2.2;
- i) in the glass adhesion method, the information when using non-ionic surfactant in the test bacterial suspension.

Annex A (informative)

Examples of test results

Examples of test results with the film adhesion method are shown in Tables A.1 and A.2.

Table A.1 — Test result example for *Staphylococcus aureus*

Laboratory	0,01 mW/cm ² , 8 h	
	$R_{0,01}$	ΔR
A	3,4	2,9
B	2,5	2,0
C	2,3	2,3
D	3,4	3,0
Average	2,90	2,55
σ_{n-1}	0,58	0,48

Table A.2 — Test result example for *Escherichia coli*

Laboratory	0,01 mW/cm ² , 8 h	
	$R_{0,01}$	ΔR
E	5,1	4,1
F	4,5	3,8
G	2,6	2,2
H	4,9	4,4
Average	4,28	3,63
σ_{n-1}	1,14	0,98

Examples of test results with the glass adhesion method are shown in Tables A.3 and A.4.

Table A.3 — Test result example for *Staphylococcus aureus*

Laboratory	0,01 mW/cm ² , 8 h	
	$S_{0,01}$	ΔS
I	0,9	0,2
J	0,7	-1,0
K	0,3	-0,4
Average	0,63	-0,40
σ_{n-1}	0,31	0,60


Table A.4 — Test result example for *Klebsiella pneumoniae*

Laboratory	0,01 mW/cm ² , 8 h	
	$S_{0,01}$	ΔS
L	2,2	1,0
M	3,1	1,3
N	2,2	1,3
Average	2,50	1,20
σ_{n-1}	0,52	0,17

Annex B (informative)

Reference data for adhesive films and adhesive glasses

The transmittance data for a suitable adhesive film made of polypropylene (VF-15¹) by KOKUYO Co., Ltd., Japan) is shown in Figure B.1.

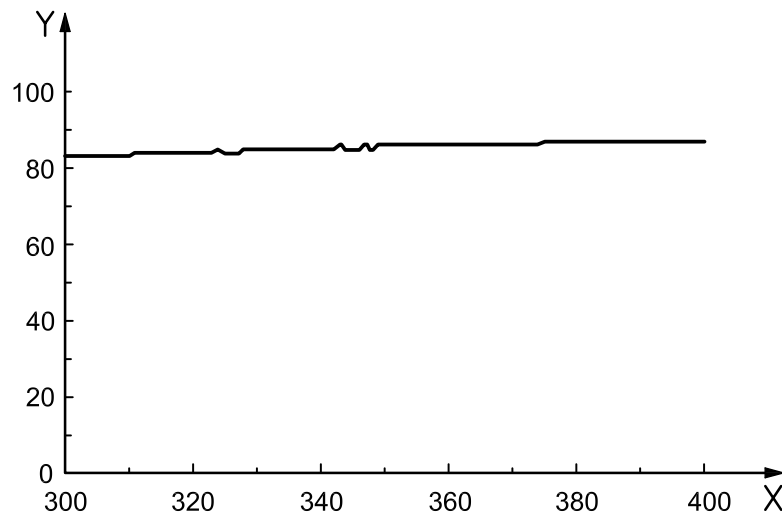


Key

X wavelength (nm)
Y transmittance (%)

Figure B.1 — Transmittance data for a suitable adhesive film

1) VF-15, TEMPAX and Pyrex7740 are examples of suitable products available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of these products.

The transmittance data for a suitable adhesive glass made by bolosilicate (TEMPAX¹) by SCHOTT AG or Pyrex7740¹) by CORNING) is shown in Figure B.2.

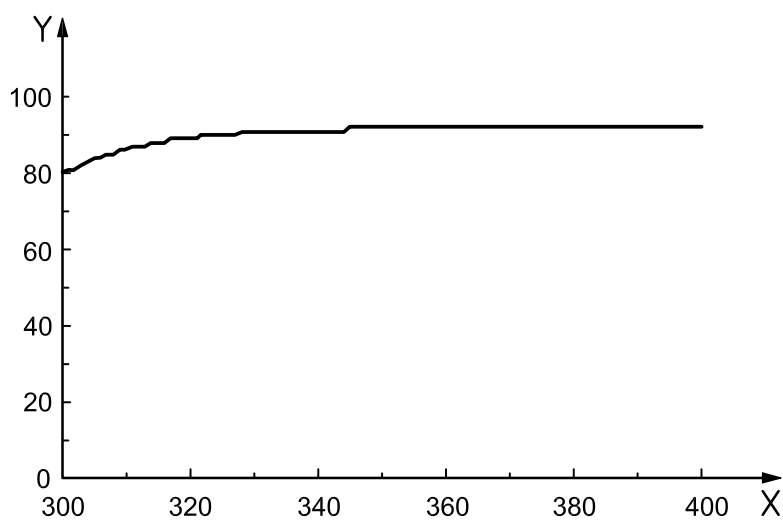

Key

X wavelength (nm)


Y transmittance (%)

Figure B.2 — Transmittance data for a suitable adhesive glass

Annex C (informative)

Reference data for damage of ultraviolet irradiation to bacteria


The damage of ultraviolet irradiation to bacteria is evaluated with glass plates (without TiO₂). The results are shown in Figure C.1 for *Escherichia coli* and in Figure C.2 for *Staphylococcus aureus*.

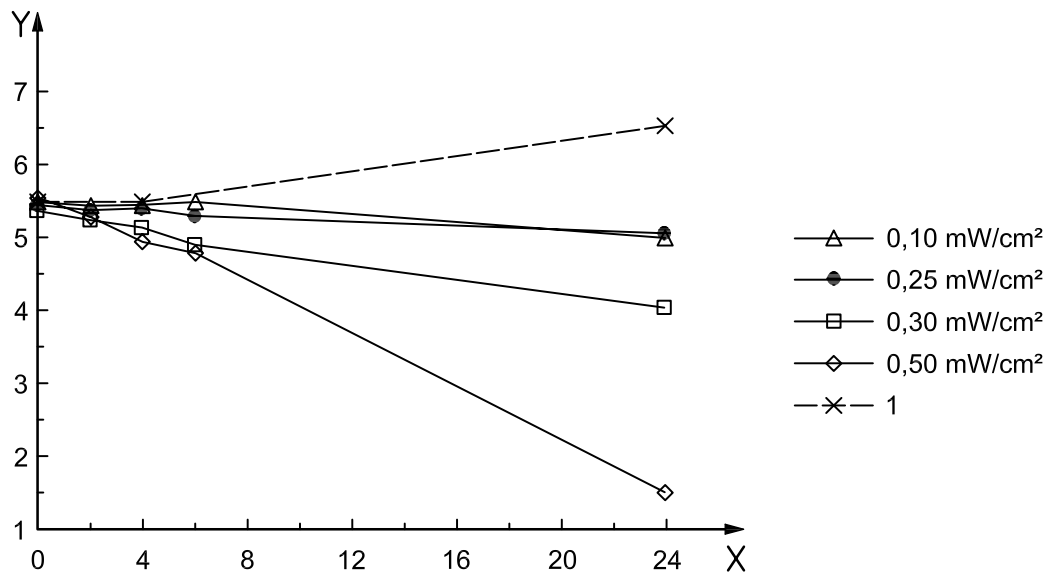

Key

- X irradiation time (h)
- Y survival bacteria (LOG)
- 1 in the dark

Figure C.1 — UV effects for *Escherichia coli*

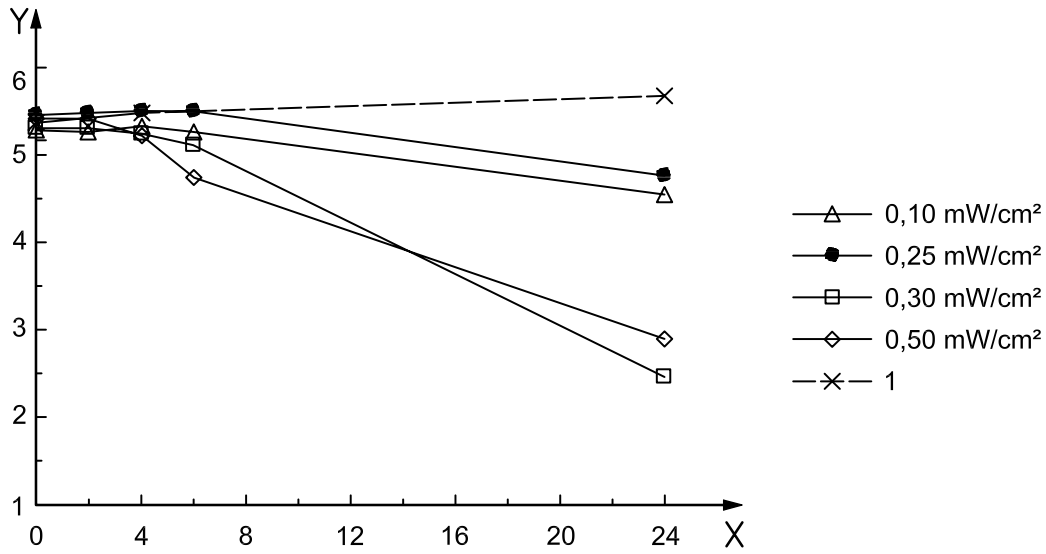

Key

- X irradiation time (h)
- Y survival bacteria (LOG)
- 1 in the dark

Figure C.2 — UV effects for *Staphylococcus aureus*

Bibliography

- [1] ISO 105-F, *Textiles — Tests for colour fastness — Part F: Standard adjacent fabrics*
- [2] ISO 554, *Standard atmospheres for conditioning and/or testing — Specifications*
- [3] ISO 835, *Laboratory glassware — Graduated pipettes*
- [4] ISO 4892-3, *Plastics — Methods of exposure to laboratory light sources — Part 3: Fluorescent UV lamps*
- [5] ISO 6353-2, *Reagents for chemical analysis — Part 2: Specifications — First series*
- [6] ISO 6353-3, *Reagents for chemical analysis — Part 3: Specifications — Second series*
- [7] ISO 10523, *Water quality — Determination of pH*
- [8] ISO 20743, *Textiles — Determination of antibacterial activity of antibacterial finished products*
- [9] ISO 22196, *Plastics — Measurement of antibacterial activity on plastics surfaces*
- [10] SUNADA, K., WATANABE, T. and HASHIMOTO, K., Studies on phototokilling of bacteria on TiO₂ thin film, *J. Photochem. Photobiol. A: Chem.*, **156**, p. 227 (2003)
- [11] SUNADA, K., WATANABE, T. and HASHIMOTO, K., Bactericidal activity of copper-deposited TiO₂ thin film under weak UV light illumination, *Environ. Sci. Technol.*, **37**, p. 4785 (2003)

ICS 81.060.30

Price based on 23 pages

BSI - British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001. Fax: +44 (0)20 8996 7001 Email: orders@bsigroup.com You may also buy directly using a debit/credit card from the BSI Shop on the Website <http://www.bsigroup.com/shop>

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact Information Centre. Tel: +44 (0)20 8996 7111 Fax: +44 (0)20 8996 7048 Email: info@bsigroup.com

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: +44 (0)20 8996 7002 Fax: +44 (0)20 8996 7001 Email: membership@bsigroup.com

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsigroup.com/BSOL>

Further information about BSI is available on the BSI website at <http://www.bsigroup.com>

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright and Licensing Manager. Tel: +44 (0)20 8996 7070 Email: copyright@bsigroup.com