

# Methods for analysis of animal feeding stuffs —

## Part 17: Determination of furazolidone content — Method using high-performance liquid chromatography

ICS 65.120

## National foreword

This British Standard reproduces verbatim ISO 14797:1999 and implements it as the UK national standard.

The UK participation in its preparation was entrusted to Technical Committee AW/10, Animal feeding stuffs, which has the responsibility to:

- aid enquirers to understand the text;
- present to the responsible international/European committee any enquiries on the interpretation, or proposals for change, and keep the UK interests informed;
- monitor related international and European developments and promulgate them in the UK.

A list of organizations represented on this committee can be obtained on request to its secretary.

### Cross-references

The British Standards which implement international or European publications referred to in this document may be found in the BSI Standards Catalogue under the section entitled "International Standards Correspondence Index", or by using the "Find" facility of the BSI Standards Electronic Catalogue.

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

**Compliance with a British Standard does not of itself confer immunity from legal obligations.**

### Summary of pages

This document comprises a front cover, an inside front cover, the ISO title page, page ii, pages 1 to 13 and a back cover.

This British Standard, having been prepared under the direction of the Consumer Products and Services Sector Committee, was published under the authority of the Standards Committee and comes into effect on 15 June 1999

© BSI 06-1999

ISBN 0 580 32339 0

### Amendments issued since publication

Amd. No.	Date	Comments

**INTERNATIONAL  
STANDARD**

**ISO  
14797**

First edition  
1999-03-15

---

**Animal feeding stuffs — Determination  
of furazolidone content — Method using  
high-performance liquid chromatography**

*Aliments des animaux — Dosage de la furazolidone — Méthode par  
chromatographie liquide à haute performance*



Reference number  
ISO 14797:1999(E)

## **Foreword**

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 14797 was prepared by Technical Committee ISO/TC 34, *Agricultural food products*, Subcommittee SC 10, *Animal feeding stuffs*.

Annexes A to C of this International Standard are for information only.

**Descriptors:** agricultural products, food, animal feeding products, chemical analysis, determination of content, furazolidonum, high performance liquid chromatography.

# Animal feeding stuffs — Determination of furazolidone content — Method using high-performance liquid chromatography

## 1 Scope

This International Standard specifies a high-performance liquid chromatographic (HPLC) method for the determination of the furazolidone content of premixtures and animal feeding stuffs.

The method is applicable to animal feeding stuffs with a furazolidone content of 25 mg/kg to 5 000 mg/kg and to premixtures with a mass fraction of furazolidone of up to 20 % [formerly written as 20 % (*m/m*)].

**NOTE 1** For animal feeding stuffs, the furazolidone content is expressed in milligrams per kilogram; for premixtures, as a mass fraction in percent [% (*m/m*)].

**NOTE 2** Furazolidone is a chemotherapeuticum belonging to the group of nitrofuranes. Nitrofuranes are bacteriostatic or bactericidal against Gram-positive and Gram-negative microorganisms and against some moulds and protozoa.

## 2 Normative reference

The following standard contains provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the edition indicated was valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent edition of the standard indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 6498:1998, *Animal feeding stuffs — Preparation of test sample*.

## 3 Principle

Furazolidone is extracted from the sample with a mixture of acetonitrile and methanol. Animal feeds are pre-wetted with water. The extract of animal feeds is purified through a short aluminum oxide column and subsequently diluted with water. The extract of premixtures is directly diluted with a mixture of water, acetonitrile and methanol. The final extract is analysed by reverse-phase HPLC with UV detection at a wavelength of 365 nm (see references [1] to [3]).

## 4 Reagents

Use only reagents of recognized analytical grade.

**4.1 Water**, demineralized or deionized, with resistivity of at least 10 M $\Omega$ -cm, or water of at least equivalent purity.

**4.2 Extraction solvent**: mixture of acetonitrile and methanol (1:1 by volume).

Combine equal volumes of acetonitrile and methanol. Mix well and allow to adjust to room temperature before use.

**4.3 Dilution solvent**: mixture of extraction solvent (4.2) and water (4.1) (35:65 by volume).

Mix 350 ml of extraction solvent (4.2) with 650 ml of water (4.1).

**4.4 Acetic acid** ( $\text{CH}_3\text{CO}_2\text{H}$ ), volume fraction of 10 % [10 % (V/V)].

Dilute 10 ml of glacial acetic acid to 100 ml with water (4.1).

**4.5 Sodium acetate buffer solution**,  $c(\text{CH}_3\text{CO}_2\text{Na}) = 0,01 \text{ mol/l}$ ,  $\text{pH} = 6,0$ .

Weigh 0,82 g of sodium acetate into a 1 000 ml one-mark volumetric flask. Dissolve in 700 ml of water. Adjust the pH to 6,0 with acetic acid (4.4). Dilute to the mark with water and mix.

**4.6 Mobile phase for HPLC.**

Combine 800 ml of sodium acetate buffer solution (4.5) and 200 ml of acetonitrile and mix. Filter the eluent through a  $0,22 \mu\text{m}$  filter using a solvent filtration system (5.2), and degas for 10 min in an ultrasonic bath (5.3) before use.

**4.7 Furazolidone standard material:** *N*-(5-nitro-2-furfurylidene)-3-amino-2-oxazolidone; CAS number 67-45-8 according to Chemical Abstracts Registry.

**WARNING — Because of the sensitivity of furazolidone to light, conduct all operations in the absence of daylight or artificial white light. Avoid inhalation of and exposure to the toxic furazolidone standard material and solutions thereof. Work in a fumehood when handling the solvents and solutions. Wear safety glasses and protective clothing.**

**4.8 Furazolidone stock solution** (approximately  $250 \mu\text{g/ml}$ ).

Weigh  $25 \text{ mg} \pm 1 \text{ mg}$  of furazolidone (4.7) to the nearest  $0,1 \text{ mg}$  into a 100 ml one-mark volumetric flask. Dissolve in extraction solvent (4.2), dilute to the mark and mix. Calculate the concentration taking into account the purity of the standard material. Prepare fresh every month. Store in the dark at  $0 \text{ }^\circ\text{C}$  to  $8 \text{ }^\circ\text{C}$ .

**4.9 Furazolidone working solutions** (approximately  $5 \mu\text{g/ml}$  and  $12,5 \mu\text{g/ml}$ ).

Pipette 2,0 ml and 5,0 ml respectively of the furazolidone stock solution (4.8) into separate 100 ml one-mark volumetric flasks. Add 65 ml of water, dilute to the mark with extraction solvent (4.2) and mix. Prepare fresh for each series of samples.

**4.10 Neutral aluminum oxide**, activity 1.

NOTE 0 % to 1 % of water is necessary for total de-activation.

## 5 Apparatus

Usual laboratory apparatus and, in particular, the following.

**5.1 pH-meter.**

**5.2 Solvent filtration system**, all-glass apparatus suitable for  $0,22 \mu\text{m}$  filters.

**5.3 Ultrasonic bath.**

**5.4 Rotary shaker**, horizontal rotation, rotation frequency  $250 \text{ min}^{-1}$  to  $300 \text{ min}^{-1}$ .

**5.5 Glass microfibre filter**, of diameter 15 cm.

**5.6 Glass wool.**

**5.7 Glass column for chromatography**, of length 30 cm, internal diameter 10 mm, restricted at the end and fitted with a wad of glass wool (5.6).

**5.8 Filtration system**, equipped with poly(vinylidene difluoride) (PVDF) filters or polytetrafluorethylene (PTFE) filters of pore size  $0,45 \mu\text{m}$ .

**5.9 HPLC system**, comprising the following.

**5.9.1 Pump**, pulse free, capable of maintaining a volume flow rate of 0,1 ml/min to 2,0 ml/min.

**5.9.2 Injection system** with loop suitable for 20 µl to 50 µl injections.

**5.9.3 UV detector**, suitable for measurements at a wavelength of 365 nm.

If available, a diode array detector may be used for confirmation purposes.

**5.9.4 Recorder**.

**5.9.5 Guard column**: silica bonded C<sub>18</sub> packing with particle size 37 µm to 100 µm, of length 20 mm, internal diameter 3,9 mm, or a guard column of equivalent quality.

**5.9.6 Analytical column**: silica bonded C<sub>18</sub> packing with particle size 5 µm, of length 200 mm, internal diameter 3,0 mm, or an analytical column of equivalent quality.

For furazolidone a capacity factor ( $K'$ ) of at least 1,0 shall be obtained.

NOTE The capacity factor is defined as:

$$K' = \frac{t_R}{t_0} - 1$$

where

$K'$  is the capacity factor;

$t_R$  is the retention time, in minutes, of furazolidone;

$t_0$  is the retention time, in minutes, of the unretained furazolidone peak.

**5.10 Disposable syringe**, of capacity 5 ml.

## 6 Sampling

Sampling is not part of the method specified in this International Standard. A recommended sampling method is given in ISO 6497 [4].

It is important that the laboratory receive a sample which is truly representative and has not been damaged or changed during transport or storage.

## 7 Preparation of test sample

Prepare the test sample in accordance with ISO 6498.

Grind the laboratory sample (usually 500 g) so that it passes completely through a sieve with 1 mm apertures. Mix thoroughly.

## 8 Procedure

### 8.1 General

In conjunction with the analysis of the test sample (or a series of test samples), analyse a blank sample, a spiked blank sample and, if available, a reference sample.

**NOTE** Blank samples are homogenates of comparable feeds with a furazolidone content of less than 10 mg/kg. Spiked blank samples are blank feed samples to which furazolidone is added. Blank samples and reference samples can be kept for a year, if stored at a temperature of 0 °C to 8 °C.

The analysis should be repeated when the recovery is lower than 94 % or higher than 106 %.

## **8.2 Preparation of a spiked sample**

The furazolidone content of the spiked sample should be approximately equal to the expected furazolidone content of the sample. For a spiked sample with a furazolidone content of 250 mg/kg, use the following procedure.

Pipette 5,0 ml of the furazolidone stock solution (4.8) into a 250 ml conical flask. Under a flow of nitrogen, evaporate to a volume of approximately 0,5 ml and add 5 g of blank feed. Mix thoroughly and allow to stand for at least 10 min before proceeding with the extraction (8.3).

## **8.3 Extraction**

### **8.3.1 Feeding stuffs with a furazolidone content of 25 mg/kg to 2 500 mg/kg**

Weigh 5,0 g of the prepared test sample to the nearest 0,05 g in a 250 ml conical flask. Add 15,0 ml of water, mix and allow to stand for 5 min. Add 35,0 ml of extraction solvent (4.2), stopper and shake vigorously for 30 min on the rotary shaker (5.4). Filter the solution through a glass microfibre filter (5.5) and use the filtrate for column chromatography according to 8.4.

### **8.3.2 Feeding stuffs with a furazolidone content of 2 500 mg/kg to 5 000 mg/kg**

Weigh 5,0 g of the prepared test sample to the nearest 0,1 g in a 250 ml conical flask. Add 30,0 ml of water, mix and allow to stand for 5 min. Add 70,0 ml of extraction solvent (4.2), stopper and shake vigorously for 30 min on the rotary shaker (5.4). Filter the solution through a glass microfibre filter (5.5) and use the filtrate for column chromatography according to 8.4.

### **8.3.3 Premixtures with a mass fraction of furazolidone of 0,5 % to 7 % [0,5 % (m/m) to 7 % (m/m)]**

Weigh 1,0 g of the prepared test sample to the nearest 0,01 g in a 250 ml conical flask. Add 100,0 ml of extraction solvent (4.2), stopper and shake vigorously for 30 min on the rotary shaker (5.4). Filter the solution through a glass microfibre filter (5.5).

Dilute the filtrate with dilution solvent (4.3) to obtain a final solution with a furazolidone content between 5 µg/ml and 10 µg/ml. The dilution factor is  $f$ .

Mix well and filter the solution using the filtration system (5.8). Use the filtrate for HPLC analysis according to 8.5.

**NOTE** The required dilution factor ( $f$ ) can be estimated by using the equation:

$$f_e = \frac{m \cdot w_{\text{exp}}}{V \cdot \rho_r}$$

where

$f_e$  is the estimated required dilution factor of the sample extract;

$m$  is the mass, in grams, of the test portion;

$w_{\text{exp}}$  is the expected furazolidone content, in milligrams per kilogram, of the sample;

$\rho_r$  is the required furazolidone content, in micrograms per millilitre, of the final solution;

$V$  is the total volume, in millilitres, of extraction solvent added to the test portion (see also note in 8.5.2).

### **8.3.4 Premixtures with a mass fraction of furazolidone of 7 % to 10 % [7 % (m/m) to 10 % (m/m)]**

Weigh 1,0 g of the prepared test sample to the nearest 0,01 g in a 500 ml conical flask. Add 200,0 ml of extraction solvent (4.2), stopper and shake vigorously for 30 min on the rotary shaker (5.4). Filter the solution through a glass microfibre filter (5.5).



Dilute the filtrate with dilution solvent (4.3) to obtain a final solution with a furazolidone content between 5 µg/ml and 10 µg/ml. The dilution factor is *f*.

Mix well and filter the solution using the filtration system (5.8). Use the filtrate for HPLC analysis according to 8.5.

NOTE See the note in 8.3.3 for the calculation of the dilution factor.

### 8.3.5 Premixtures with a mass fraction of furazolidone of 10 % to 20 % [10 % (*m/m*) to 20 % (*m/m*)]

Weigh 0,5 g of the prepared test sample to the nearest 5 mg in a 500 ml conical flask. Add 200,0 ml of extraction solvent (4.2), stopper and shake vigorously for 30 min on the rotary shaker (5.4). Filter the solution through a glass microfibre filter (5.5).

Dilute the filtrate with dilution solvent (4.3) to obtain a final solution with a furazolidone content between 5 µg/ml and 10 µg/ml. The dilution factor is *f*.

Mix well and filter the solution using the filtration system (5.8). Use the filtrate for HPLC analysis according to 8.5.

NOTE See the note in 8.3.3 for the calculation of the dilution factor.

## 8.4 Column chromatography

For each sample extract, dry-pack a glass column (5.7), fitted at the bottom with a plug of glass wool (5.6), with 4 g of aluminium oxide (4.10). Apply 20 ml of extract, prepared according to 8.3.1 or 8.3.2, to the column and discard the first 4 ml of eluate. Collect the following 8 ml of eluate in a small graduated cylinder.

Pipette 5,0 ml of eluate in a 5 ml one-mark volumetric flask and dilute to the mark with water. Mix well.

If necessary, dilute the solution with dilution solvent (4.3) to obtain a final solution with a furazolidone content between 5 µg/ml and 10 µg/ml. The dilution factor is *f*.

Filter the diluted solutions using the filtration system (5.8) and use the filtrate for HPLC analysis according to 8.5.

## 8.5 HPLC analysis

### 8.5.1 HPLC conditions

Use the following conditions:

- mobile phase (4.6) volume flow rate: 0,6 ml/min;
- injection volume: 20 µl;
- wavelength: 365 nm;
- recorder: 10 mV;
- chart speed: 0,5 cm/min.

### 8.5.2 Procedure

**8.5.2.1** Inject the furazolidone working solutions (4.9) until a stable baseline and reproducible peak heights or peak areas are obtained. For peak heights or peak areas, the difference between the highest and the lowest result should be less than 5 % of the mean result of three consecutive injections.

The furazolidone peak shall be symmetrical ( $f_{as} < 2$ ).

NOTE  $f_{as}$  is the width on the tail side of the perpendicular line of the peak, divided by the width on the front side of the perpendicular line of the peak, both measured at 10 % of the height of the peak.

There shall be a proportional relation (within 5 %) between the concentration and peak heights of the two furazolidone working solutions. If a deviation of more than 5 % is found, new furazolidone working solutions shall be prepared.

Inject the extracts of the blank sample and the spiked blank sample. If the peak of furazolidone is not symmetrical or not fully separated from the feed matrix peaks, it is necessary to use another HPLC column or to adjust the chromatographic conditions by an increase or decrease of the aqueous content of the mobile phase (4.6).

Consecutively inject furazolidone working solutions (4.9), five sample extracts and furazolidone working solutions (4.9). Repeat this sequence, if necessary, for the other sample extracts in the series.

The observed peak heights or peak areas for the furazolidone working solutions should be within a margin of 5 % of the results of the furazolidone working solutions injected before.

An example of a chromatogram is presented in annex A. From the chromatogram for furazolidone, values of  $K'$  of 2,1 can be calculated (see also note in 5.9.6).

**8.5.2.2** If the furazolidone content of a premixture is obviously lower than the expected content (taking into account the tolerance), it is recommended to repeat the analysis with an additional 50 ml of extraction solvent (4.2) applied in 8.3.3, 8.3.4 or 8.3.5.

If the new result is more than 15 % (*m/m*) higher than the original value, the analysis should be repeated with another additional 50 ml of extraction solvent (4.2). This addition should be repeated until the difference in results of consecutive determinations is less than 15 % (*m/m*).

## **9 Confirmation**

### **9.1 General**

If the identity of the substance causing the peak in the chromatogram is in doubt, based on the peak shape or on the result obtained, the identity of the determined analyte may be confirmed by either applying co-chromatography or a diode array detector. In the first case, proceed in accordance with 9.2; in the latter case, proceed in accordance with 9.3.

### **9.2 Co-chromatography**

Prepare a spiked sample extract by adding an appropriate amount of furazolidone working solution (4.9) to the sample extract. The amount of furazolidone added shall be approximately equal to the estimated amount of furazolidone in the sample extract.

Inject the sample extract, furazolidone working solution (4.9) and spiked sample extract. Only the peak in the chromatogram presumed to be the analyte peak should intensify, should increase in height proportionally to the spiking level, and should increase in peak width at half height by no more than  $\pm 10$  % of the original width.

Proceed in accordance with clause 10.

### **9.3 Diode array detector**

#### **9.3.1 Conditions**

The conditions are as specified in 8.5.1 but use a diode array detector instead of a UV detector with the following parameters:

Parameter	Setting
sample wavelength	365 nm
sample bandwidth	4 nm (i.e. wavelength of 365 nm $\pm$ 2 nm)
reference wavelength	450 nm
reference bandwidth	100 nm
spectrum range	225 nm to 400 nm
spectrum	baseline, apex, upslope and downslope inflection points

### 9.3.2 Procedure

Allow the system to stabilize. Inject the 5  $\mu\text{g/ml}$  furazolidone working solution (4.9), suspected sample extracts and again the 5  $\mu\text{g/ml}$  furazolidone working solution (4.9). Record the spectra at the baseline, upslope and downslope inflection points and peak apex. Store all data.

### 9.3.3 Evaluation

Plot in one figure the normalized difference spectra (sample - baseline) of the sample peak, recorded at the apex and at the upslope and downslope inflection points. Plot in one figure the normalized spectra of the sample peak and of the furazolidone working solution peak, recorded at the apex.

### 9.3.4 Confirmation criteria

The identity of the analyte is confirmed if the following criteria are satisfied.

- The retention time of the sample peak shall be equal ( $\pm 5\%$ ) to the retention time of the standard peak. If in doubt, standard addition (standard material added to the sample) shall be performed.
- Assess the purity of the sample peak on the basis of the conformity of the difference spectra, recorded at apex and at upslope and downslope inflection points. At each wavelength the relative absorption shall be equal (to within 15 %) for all spectra.
- Above a wavelength of 220 nm, the difference spectra of the sample and standard peaks recorded at the peak apex shall not be visually different for those parts of the spectra with a relative absorption of at least 10 %. This criterion is met when the same maxima are present within a margin determined by the resolution of the detection system (typically 2 nm to 4 nm). At no observed point shall the deviation between the two spectra exceed 15 % of the absorbance of the standard analyte at that particular wavelength.

## 10 Calculation of results

### 10.1 General

Calculate the furazolidone content of the sample extract by comparing the peak height or peak area of the sample extract chromatogram with the mean of the peak heights or peak areas of the furazolidone working solution injected before and after the sample extract. Use the results obtained with the furazolidone working solution with the best matching furazolidone content.

### 10.2 Feeding stuffs with a furazolidone content of 25 mg/kg to 5 000 mg/kg

Calculate the furazolidone content of feeding stuff samples ( $w_f$ ) by the equation:

$$w_f = \frac{h}{h_s} \times \rho_s \times \frac{V}{m} \times f$$

where

- $w_f$  is the furazolidone content, in milligrams per kilogram, of the test sample;
- $h$  is the peak height, in length units, obtained for the sample extract;
- $h_s$  is the peak height, in length units, obtained for the furazolidone working solution;
- $\rho_s$  is the furazolidone content, in micrograms per millilitre, of the furazolidone working solution;
- $V$  is the total volume, in millilitres, of extraction solvent added to the test portion;
- $m$  is the mass, in grams, of the test portion;
- $f$  is the dilution factor of the sample extract (see 8.4).

NOTE Alternatively, the peak area may be used in the calculation instead of the peak height.

Round the result to the nearest 1 mg/kg.

### **10.3 Premixtures with a mass fraction of furazolidone of up to 20 % [20 % (m/m)]**

Calculate the mass fraction of furazolidone in premixtures ( $w_{fp}$ ) by the equation:

$$w_{fp} = \frac{h}{h_s} \times \rho_s \times \frac{V}{m} \times f \times 10^{-4} \times f_u$$

where

- $w_{fp}$  is the mass fraction of furazolidone in the test sample, in percent [% (m/m)];
- $h$  is the peak height, in length units, obtained for the sample extract;
- $h_s$  is the peak height, in length units, obtained for the furazolidone working solution;
- $\rho_s$  is the furazolidone content, in micrograms per millilitre, of the furazolidone working solution;
- $V$  is the total volume, in millilitres, of extraction solvent added to the test portion;
- $m$  is the mass, in grams, of the test portion;
- $f$  is the dilution factor of the sample extract (see 8.3.3, 8.3.4 or 8.3.5);
- $f_u$  is the units correction factor, in kg·mg<sup>-1</sup>·% ( $f_u = 1 \text{ kg} \cdot \text{mg}^{-1} \cdot \%$ ).

NOTE Alternatively, the peak area may be used in the calculation instead of the peak height.

Round the result to the nearest 0,01 % (m/m).

## **11 Precision**

### **11.1 Interlaboratory test**

Details of an interlaboratory test on the precision of the method are given in annex B. The values derived from this interlaboratory test may not be applicable to concentration ranges and matrices other than those given.

## 11.2 Repeatability

The absolute difference between two independent single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, will in not more than 5 % of cases exceed:

- 8 % of the mean of the two test results for furazolidone contents between 80 mg/kg and 300 mg/kg;
- 10 % of the mean of the two test results for mass fractions of furazolidone of between 4 % and 6 % [4 % (*m/m*) and 6 % (*m/m*)].

## 11.3 Reproducibility

The absolute difference between two single test results, obtained using the same method on identical test material in different laboratories by different operators using different equipment, will in not more than 5 % of cases exceed:

- 17 % of the mean of the two test results for furazolidone contents between 80 mg/kg and 300 mg/kg;
- 20 % of the mean of the two test results for mass fractions of furazolidone of between 4 % and 6 % [4 % (*m/m*) and 6 % (*m/m*)].


## 12 Test report

The test report shall specify:

- all information necessary for the complete identification of the sample;
- the sampling method used, if known;
- the test method used, with reference to this International Standard;
- all operating details not specified in this International Standard, or regarded as optional, together with details of any incidents which may have influenced the test result(s);
- the test result(s) obtained; or
- if the repeatability has been checked, the final quoted result obtained.

**Annex A**  
(informative)

**Example of a chromatogram**

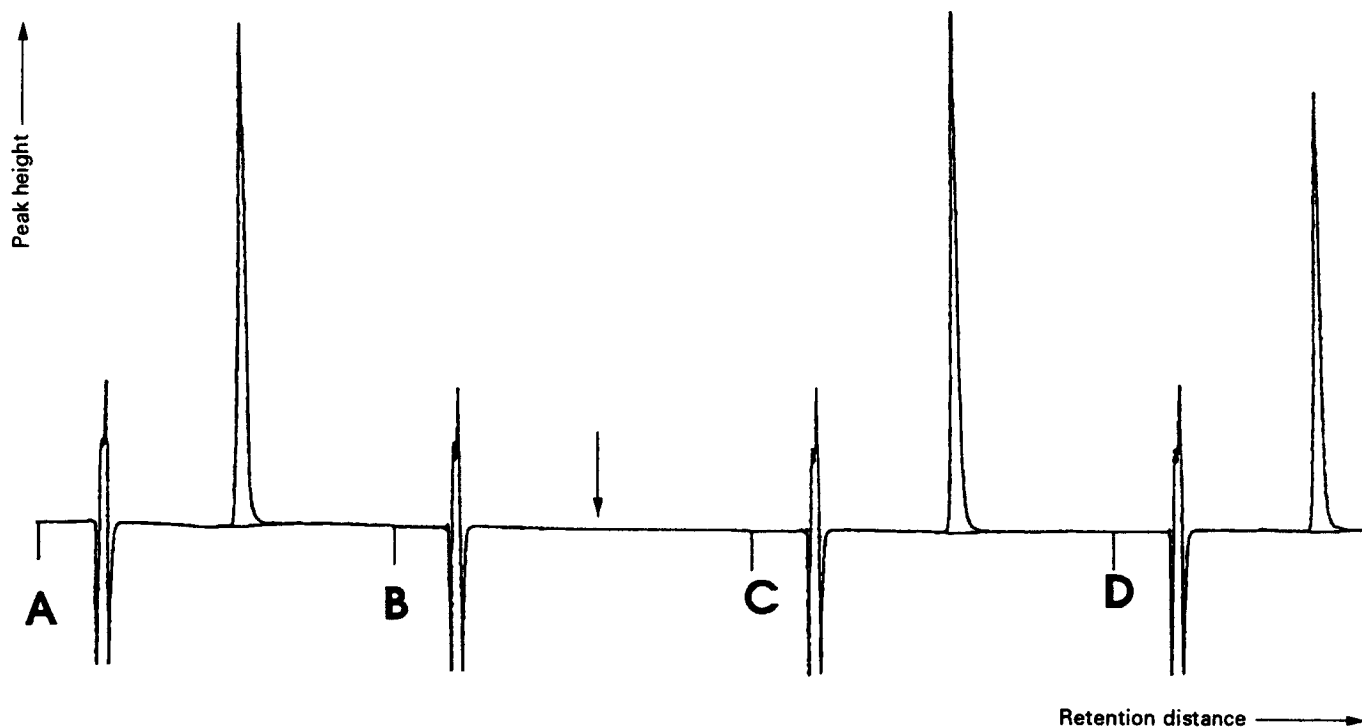

**Key**

- A Standard, 12,1  $\mu\text{g/ml}$
- B Blank sample
- C Spiked blank feed, 242 mg/kg
- D Sample (real)

**Figure A.1**

## Annex B (informative)

### Results of an interlaboratory trial

The precision of the method was established by an interlaboratory test carried out in accordance with ISO 5725 [5].<sup>1)</sup> In this test, 30 laboratories from 7 European countries participated; 14 samples (including 3 blanks) were investigated. The samples were selected on the basis of information about the use of the materials in several countries. The results are given in tables B.1 and B.2.

**Table B.1 — Statistical results of the interlaboratory test on feeding stuffs**

Parameter	Sample <sup>1)</sup>						
	Pi6	Pi7	Ra9	Ch11	Ch12	Ca13	Fi14
Number of laboratories retained after eliminating outliers	27	29	28	29	28	29	28
Mean furazolidone content, mg/kg	199	274	89	92	189	190	2853
Repeatability standard deviation, $s_r$ , mg/kg	2,8	3,9	2,4	2,8	3,6	5,9	57,6
Coefficient of variation of repeatability, %	1,4	1,4	2,7	3,0	1,9	3,1	2,0
Repeatability limit, $r$ ( $r = 2,8 s_r$ ), mg/kg	7,9	8,5	6,8	7,9	10,2	16,7	163,0
Reproducibility standard deviation, $s_R$ , mg/kg	9,9	12,1	6,9	7,4	10,6	13,6	173,4
Coefficient of variation of reproducibility, %	5,0	4,4	7,7	8,0	5,6	7,1	6,1
Reproducibility limit, $R$ ( $R = 2,8 s_R$ ), mg/kg	28,0	34,2	19,5	22,4	28,9	47,3	490,7
1) Pi6: pig feed with a sulfadimidine sodium content of 400 mg/kg; Pi7: pig feed; Ra9: rabbit feed with a robenidine content of 66 mg/kg and a flavophospholipol content of 4 mg/kg; Ch11: broiler feed with an average fat content, an avoparcine content of 15 mg/kg and a salinomycine sodium content of 60 mg/kg; Ch12: broiler feed with a high fat content, an avoparcine content of 15 mg/kg and a salinomycine sodium content of 60 mg/kg; Ca13: milk replacer for veal calves with a chlortetracycline content of 200 mg/kg; Fi14: fish feed.							

<sup>1)</sup> ISO 5725:1986 (now withdrawn) was used to obtain the precision data.

Table B.2 — Statistical results of the interlaboratory test with premixtures

Parameter	Sample <sup>1)</sup>			
	P1	P2	P3	P4
Number of laboratories retained after eliminating outliers	29	29	29	29
Mean furazolidone content, % (m/m)	3,89	6,21	3,72	19,9
Repeatability standard deviation, $s_r$ , % (m/m)	0,14	0,20	0,22	0,38
Coefficient of variation of repeatability, %	3,6	3,2	5,9	1,9
Repeatability limit, $r$ ( $r = 2,8 s_r$ ), % (m/m)	0,40	0,57	0,62	1,08
Reproducibility standard deviation, $s_R$ , % (m/m)	0,26	0,45	0,30	0,82
Coefficient of variation of reproducibility, %	6,58	7,23	8,05	4,13
Reproducibility limit, $R$ ( $R = 2,8 s_R$ ), % (m/m)	0,74	1,27	1,75	2,32
1) P1 and P2: premixtures with corn meal as carrier; P3: premixture with corn meal as carrier and sulfadimidine sodium content of 8 % (m/m); P4: premixture with calcium carbonate as carrier.				



## Annex C (informative)

### Bibliography

- [1] Keukens, H.J., Aerts, M.M.L. and Strating, K. (1994) (in press).
- [2] SOP A0520, State Institute for Quality Control of Agricultural Products (RIKILT-DLO), Agricultural Research Department, The Netherlands.
- [3] Lowie, Jr., D.M., Teague, Jr., R.T., Quick, F.E. and Foster, C.L. *J. AOAC*, **66**, 1983, pp. 602-605.
- [4] ISO 6497:—<sup>2)</sup>, *Animal feeding stuffs — Sampling*.
- [5] ISO 5725:1986, *Precision of test methods — Determination of repeatability and reproducibility for a standard test method by inter-laboratory tests*.
- [6] ISO 5725-1:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions*.
- [7] ISO 5725-2:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*.

---

<sup>2)</sup> To be published.

---

## **BSI — British Standards Institution**

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

### **Revisions**

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

### **Buying standards**

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

### **Information on standards**

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre. Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: 020 8996 7002. Fax: 020 8996 7001.

### **Copyright**

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager. Tel: 020 8996 7070.