

Analysis of iron ores —

Part 7: Methods for the determination of sulphur content —

Section 7.1 Gravimetric method

[ISO title: Iron ores — Determination of sulfur content — Barium sulfate gravimetric method]

UDC 622.341.1:[620.113:622.7.016.34]:622.7.092:543.845:543.21:620.1

Committees responsible for this British Standard

The preparation of this British Standard was entrusted by the Iron and Steel Standards Committee (ISM/-) to Technical Committee ISM/58, upon which the following bodies were represented:

British Steel Industry
Institution of Mining and Metallurgy

The following body was also represented in the drafting of the standard, through subcommittees and panels:

British Ceramic Research Ltd.

This British Standard, having been prepared under the direction of the Iron and Steel Standards Committee, was published under the authority of the Board of BSI and comes into effect on 31 January 1989

© BSI 10-1999

The following BSI references relate to the work on this standard:
Committee reference ISM/58
Draft for comment 81/78396 DC

ISBN 0 580 16911 1

Amendments issued since publication

| Amd. No. | Date of issue | Comments |
|----------|---------------|----------|
| | | |
| | | |
| | | |
| | | |

Contents

| | Page |
|---|--------------------|
| Committees responsible | Inside front cover |
| National foreword | ii |
| 1 Scope and field of application | 1 |
| 2 References | 1 |
| 3 Principle | 1 |
| 4 Reagents | 1 |
| 5 Apparatus | 1 |
| 6 Sampling and samples | 2 |
| 7 Procedure | 2 |
| 8 Expression of results | 4 |
| 9 Test report | 5 |
| Annex A Flowsheet of the procedure for the acceptance of analytical values for test samples | 6 |
| Annex B Derivation of repeatability and permissible tolerance equations | 7 |
| Annex C Precision data obtained by international analytical trial | 8 |
| Figure — Least-squares fit of precision against X for sulfur | 8 |
| Table — Mass of test portion and volume of acid mixture (4.10) required for decomposition | 2 |
| Publications referred to | Inside back cover |

National foreword

This Section of BS 7020 has been prepared under the direction of the Iron and Steel Standards Committee. It is identical with ISO 4689-1986 “*Iron ores — Determination of sulfur content — Barium sulfate gravimetric method*” published by the International Organization for Standardization (ISO).

Terminology and conventions. The text of the International Standard has been approved as suitable for publication as a British Standard without deviation. Some terminology and certain conventions are not identical with those used in British Standards; attention is drawn especially to the following.

The comma has been used as a decimal marker. In British Standards it is current practice to use a full point on the baseline as the decimal marker.

In British Standards it is current practice to use the spelling “sulphur” etc., instead of “sulfur”, etc.

Wherever the words “International Standard” appear, referring to this standard, they should be read as “Section of BS 7020”.

Cross-references

| International Standard | Corresponding British Standard |
|------------------------|--|
| | BS 5660 <i>Methods of sampling iron ores</i> |
| ISO 3081:1986 | Part 1:1987 <i>Manual method of increment sampling</i> (Identical) |
| ISO 3082:1987 | Part 2:1987 <i>Mechanical method of increment sampling and sample preparation</i> (Identical) |
| ISO 3083:1986 | BS 5661:1987 <i>Method for preparation of samples of iron ores by manual means</i> (Identical) |
| ISO 7764:1985 | BS 7020 <i>Analysis of iron ores</i> Part 1:1988 <i>Method for the preparation of pre-dried test samples for chemical analysis</i> (Identical) |

The reference to ISO 5725 is for information only.

Additional information. In clause 2 the footnote to ISO 3082 no longer applies as this standard has now been published.

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

Summary of pages

This document comprises a front cover, an inside front cover, pages i and ii, pages 1 to 8, an inside back cover and a back cover.

This standard has been updated (see copyright date) and may have had amendments incorporated. This will be indicated in the amendment table on the inside front cover.

1 Scope and field of application

This International Standard specifies a barium sulfate gravimetric method for the determination of the sulfur content of iron ores.

This method is applicable to a concentration range of 0,01 to 1,0 % (*m/m*) of sulfur in natural iron ores, and iron ore concentrates and agglomerates including sinter products.

2 References

ISO 3081, *Iron ores — Increment sampling — Manual method*.

ISO 3082, *Iron ores — Increment sampling and sample preparation — Mechanical method¹⁾*.

ISO 3083, *Iron ores — Preparation of samples — Manual method*.

ISO 7764, *Iron ores — Preparation of predried test samples for chemical analysis*.

3 Principle

Decomposition of a test portion by treatment with potassium chlorate and hydrochloric and nitric acids followed by evaporation to dryness.

Dissolution of the salts in hydrochloric acid and filtration of the insoluble residue. Removal of the major portion of the iron in the filtrate by extraction with methyl isobutyl ketone.

Ignition of the insoluble residue and removal of silicon dioxide by evaporation with hydrofluoric and nitric acids. Fusion of the residue with sodium carbonate followed by leaching and filtration. Acidification of the filtrate and combination with the main solution.

Reduction of any remaining iron to the bivalent state, adjustment of the acidity and addition of barium chloride solution. Filtration of barium sulfate and gravimetric determination.

4 Reagents

During the analysis, use only reagents of recognized analytical grade, and only distilled water or water of equivalent purity.

4.1 Potassium chlorate (KClO_3), powder.

4.2 Sodium carbonate (Na_2CO_3), anhydrous.

4.3 Zinc

Use zinc with the lowest available sulfur content and with a particle size of 1 to 3 mm.

4.4 Hydrochloric acid, ρ 1,16 to 1,19 g/ml.

4.5 Hydrochloric acid, ρ 1,16 to 1,19 g/ml, diluted 2 + 1.

4.6 Hydrochloric acid, ρ 1,16 to 1,19 g/ml, diluted 1 + 1.

4.7 Hydrochloric acid, ρ 1,16 to 1,19 g/ml, diluted 2 + 100.

4.8 Nitric acid, ρ 1,4 g/ml.

4.9 Hydrofluoric acid, 40 % (*m/m*), ρ 1,13 g/ml, or 48 % (*m/m*), ρ 1,185 g/ml.

4.10 Acid mixture: hydrochloric acid (4.4) + nitric acid (4.8), 4 + 1.

NOTE Do not store this mixture; prepare immediately before use.

4.11 Barium chloride ($\text{BaCl}_2 \cdot 2\text{H}_2\text{O}$), 100 g/l solution.

Dissolve 100 g of crystalline barium chloride dihydrate ($\text{BaCl}_2 \cdot 2\text{H}_2\text{O}$) in 1 litre of water, cover and heat to boiling point. Keep warm on a water bath for a minimum of 2 h and allow to cool to room temperature overnight. Store the solution in a plastics bottle and before each use, filter the required volume through a close-texture filter paper.

4.12 Hydrochloric acid wash solution, containing barium chloride.

Filter 10 ml of barium chloride solution (4.11) through a close-texture filter paper, and dilute to 1 000 ml with hydrochloric acid solution (4.7).

4.13 Sodium nitrate (NaNO_3), saturated solution.

4.14 Sodium carbonate (Na_2CO_3), 20 g/l solution. Store in a plastics bottle.

4.15 Ammonium thiocyanate (NH_4SCN), 100 g/l solution.

4.16 Silver nitrate, 20 g/l solution.

4.17 Methyl orange, 0,1 g/100 ml solution.

Dissolve 0,10 g of methyl orange in 100 ml of water.

4.18 Methyl isobutyl ketone [$\text{CH}_3\text{COCH}_2\text{CH}(\text{CH}_3)_2$] (4-Methylpentan-2-one).

Pre-treat as follows before use: transfer 200 ml of methyl isobutyl ketone and 100 ml of hydrochloric acid solution (4.6) to a 500 ml separating funnel, and shake thoroughly for about 1 min. Allow the layers to separate and discard the lower aqueous layer.

5 Apparatus

Ordinary laboratory apparatus.

¹⁾ At present at the stage of draft.

6 Sampling and samples

6.1 Laboratory sample

For analysis, use a laboratory sample of minus 100 μm particle size which has been taken in accordance with ISO 3081 or ISO 3082 and prepared in accordance with ISO 3082 or ISO 3083. In the case of ores with significant contents of combined water or oxidizable compounds, use a particle size of minus 160 μm .

NOTE A guideline on significant contents of combined water and oxidizable compounds is incorporated in ISO 7764.

6.2 Preparation of predried test samples

Thoroughly mix the laboratory sample and, taking multiple increments, extract a test sample in such a manner that it is representative of the whole contents of the container. Dry the test sample at $105 \pm 2^\circ\text{C}$ as specified in ISO 7764. (This is the predried test sample.)

7 Procedure

7.1 Number of determinations

Carry out the analysis at least in duplicate in accordance with Annex A, independently, on one predried test sample.

NOTE The expression "independently" means that the second and any subsequent result is not affected by the previous result(s). For this particular analytical method, this condition implies that the repetition of the procedure shall be carried out either by the same operator at a different time or by a different operator, including, in either case, appropriate recalibration.

7.2 Blank test and check test

In each run, one blank test and one analysis of a certified reference material of the same type of ore shall be carried out in parallel with the analysis of the ore sample(s) under the same conditions. A predried test sample of the certified reference material shall be prepared as specified in 6.2.

NOTE The certified reference material should be of the same type as the sample to be analysed and the properties of the two materials should be sufficiently similar to ensure that in either case no significant changes in the analytical procedure become necessary.

When the analysis is carried out on several samples at the same time, the blank value may be represented by one test, provided that the procedure is the same and the reagents used are from the same reagent bottles.

When the analysis is carried out on several samples of the same type of ore at the same time, the analytical value of one certified reference material may be used.

7.3 Test portion

Taking several increments, weigh, to the nearest 0,000 2 g, the amount of the predried test sample (6.2) specified in the table.

NOTE The test portion should be taken and weighed quickly in order to avoid reabsorption of moisture.

Table — Mass of test portion and volume of acid mixture (4.10) required for decomposition

| Sulfur content, w_S % (m/m) | Mass of test portion g | Volume of acid mixture ml |
|----------------------------------|---------------------------|------------------------------|
| $0,01 < w_S \leq 0,1$ | 5,0 | 70 |
| $0,1 < w_S \leq 0,5$ | 2,0 | 40 |
| $0,5 < w_S \leq 1,0$ | 1,0 | 25 |

7.4 Determination

7.4.1 Decomposition of the test portion

Place the test portion (7.3) in a 500 ml beaker, add 1 g of potassium chlorate (4.1) and 3 to 4 ml of water, and mix thoroughly.

Add, in accordance with the table, the required volume of acid mixture (4.10) and heat gently to decompose the test portion. Evaporate the solution to dryness on a hot-plate heated to about 150°C , cool and add 10 ml of hydrochloric acid (4.4).

Again evaporate to dryness, continuing the heating at about 110°C for 30 min. Cool, add 30 ml of hydrochloric acid (4.6) and warm to dissolve soluble salts.

NOTE Samples that are not decomposed in 1 to 2 h by this procedure should be digested by keeping the solution warm for an extended period.

Add 25 ml of water and boil for about 5 min. Filter the solution through a close-texture paper, collecting the filtrate in a 500 ml beaker. Wash the paper and residue with the warm hydrochloric acid (4.7) until iron(III) ion can no longer be detected in the washings by testing a small portion with the ammonium thiocyanate solution (4.15). Reserve the filtrate and washings. Transfer the filter paper containing the residue to a platinum crucible.

7.4.2 Extraction of the bulk of the iron

Evaporate the filtrate and washings (7.4.1) to about 10 ml. Cool and transfer the solution to a 200 ml separating funnel, using a total of 50 ml of hydrochloric acid (4.5), taken in several portions, to rinse the beaker. Add 50 ml of the methyl isobutyl ketone (4.18) and shake thoroughly for about 1 min. Allow the layers to separate, then drain the lower aqueous layer into a second 200 ml separating funnel. Wash the organic layer by adding 10 ml of hydrochloric acid (4.5) and shaking for about 30 s. Allow the layers to separate, then combine the aqueous layer with the first. Repeat the washing of the organic phase with another 10 ml of hydrochloric acid (4.5), combine the aqueous solutions and reject the organic phase.

Add 50 ml of methyl isobutyl ketone (4.18) to the funnel containing the aqueous solution and shake thoroughly for about 1 min. Allow the layers to separate, then run the lower aqueous solution into a 500 ml beaker. Wash the organic phase by extracting twice with 10 ml of hydrochloric acid (4.5), transferring the washings to the beaker. Evaporate the combined aqueous solutions almost to dryness.

Add 10 ml of acid mixture (4.10) to the salts and evaporate to dryness to decompose the organic matter. Add 10 ml of hydrochloric acid (4.4) and evaporate to dryness on a hot-plate heated to about 150 °C. Add a further 10 ml of hydrochloric acid (4.4) and evaporate to dryness, continuing the heating at 110 °C for about 30 min. Cool, add 5 ml of hydrochloric acid (4.4) and 30 ml of water to dissolve the salts, and reserve as the main solution.

7.4.3 Treatment of the residue

Moisten the filter paper containing the residue obtained in 7.4.1 with 1 or 2 drops of sodium nitrate solution (4.13), carefully heat the crucible to char the paper, then ignite at a temperature of 800 to 850 °C. Allow the crucible to cool and moisten the ignited residue with a few drops of nitric acid (4.8). Add about 5 ml of hydrofluoric acid (4.9), and heat gently to dryness to remove silicon dioxide and nitric acid.

NOTE With high silicon contents, the treatment to remove silicon dioxide may be repeated with another 5 ml of hydrofluoric acid (4.9).

Allow the crucible to cool, add 3 g of sodium carbonate (4.2) and fuse the residue at about 1 000 °C for 15 min. Place the cold crucible in a 300 ml beaker, add about 100 ml of warm water and heat to dissolve the melt. Remove the crucible and rinse with water.

Filter the solution through a close-texture filter paper, collecting the filtrate in a 300 ml beaker. Wash the filter paper several times with sodium carbonate solution (4.14), and discard the residue. Add 0,5 ml of methyl orange indicator solution (4.17) to the filtrate and washings and neutralize the solution by adding hydrochloric acid (4.6) in small portions, while stirring. Add 5 ml of hydrochloric acid (4.6) in excess and combine this solution with the main solution from 7.4.2.

7.4.4 Precipitation of barium sulfate

Cover the beaker containing the combined solution with a watch glass, and heat to evaporate the solution to 25 ml. Allow to cool, add 3 ml of hydrochloric acid (4.6) and 50 ml of water, and heat to dissolve soluble salts. Heat on a water bath at 60 to 70 °C and add 1,0 g of zinc (4.3) to reduce the remaining iron(III) to iron(II). Immediately after complete dissolution of the zinc, filter the solution through a close-texture filter paper, collecting the filtrate in a 300 ml tall-form beaker. Wash the paper and residue with hydrochloric acid (4.7) until the volume of the filtrate is approximately 120 ml, then discard the residue.

Heat the solution to 60 to 70 °C, then, while stirring, slowly add 5 ml of barium chloride solution (4.11) from a burette. Continue to stir for a further 5 min, then cover the beaker with a watch glass and heat the solution on a water bath at 60 to 70 °C for about 2 h. Allow the solution to cool to room temperature overnight.

Filter the barium sulfate precipitate through a close-texture filter paper.

NOTE If necessary, a small amount of filter pulp may be used to prevent the fine precipitate from passing through the filter.

Wash the beaker once with hydrochloric acid wash solution containing barium chloride (4.12) and with the aid of a rubber-tipped glass rod, remove the precipitate still adhering to the walls of the beaker, transferring it to the filter paper using hydrochloric acid wash solution containing barium chloride (4.12). Wash out the beaker several times with the same solution and wash the precipitate on the filter paper with warm water until chloride ion is no longer detected in the washings by testing with silver nitrate solution (4.16).

7.4.5 Weighing

Place the paper and precipitate from 7.4.4 in a tared platinum crucible. Dry and char the paper at a low temperature then carefully ignite, first at about 500 °C for 20 min and then at about 800 °C for the same period. Cool the crucible in a desiccator to room temperature and weigh as barium sulfate. Repeat the ignition at 800 °C until constant mass, to the nearest 0,000 1 g, is obtained.

8 Expression of results

8.1 Calculation of sulfur content

The sulfur content, w_S , is calculated as a percentage by mass, to five decimal places, using the equation

$$w_S (\%) = \frac{[(m_1 - m_2) - (m_3 - m_4)] \times 0,137\,4 \times 100}{m_5} \dots (1)$$

$$= \frac{[(m_1 - m_2) - (m_3 - m_4)] \times 13,74}{m_5}$$

where

m_1 is the mass, in grams, of the platinum crucible containing barium sulfate from the test portion;

m_2 is the tare, in grams, of the platinum crucible used for the determination;

m_3 is the mass, in grams, of the platinum crucible for the blank test;

m_4 is the tare, in grams, of the platinum crucible for the blank test;

m_5 is the mass, in grams, of the test portion (7.3);

0,137 4 is the mass ratio of sulfur in barium sulfate.

8.2 General treatment of results

8.2.1 Repeatability and permissible tolerance

The precision of this analytical method is expressed by the following regression equations:²⁾

$$r = 0,026 X + 0,004 \dots (2)$$

$$P = 0,027 X + 0,006 \dots (3)$$

$$\sigma_r = 0,009 X + 0,002 \dots (4)$$

$$\sigma_L = 0,007 X + 0,002 \dots (5)$$

where

X is the sulfur content, expressed as a percentage by mass, of the predried test sample, calculated as follows:

- within-laboratory equations (2, 4); the arithmetic mean of the duplicate values,
- between-laboratories equations (3, 5); the arithmetic mean of the final results (8.2.3) of the two laboratories;

r is the permissible tolerance within a laboratory (repeatability);

P is the permissible tolerance between laboratories;

σ_r is the within-laboratory standard deviation;

σ_L is the between-laboratories standard deviation.

8.2.2 Acceptance of analytical values

The result obtained for the certified reference material shall be such that the difference between this result and the certified value of the certified reference material is statistically insignificant. For a certified reference material that has been analysed by at least 10 laboratories using method(s) that are comparable both in accuracy and precision with this method, the following condition may be used to test the significance of the difference:

$$|A_c - A| < 2 \sqrt{\frac{s_{Lc}^2 + \frac{s_{Wc}^2}{n}}{N_c} + \sigma_L^2 + \frac{\sigma_r^2}{n}} \dots (6)$$

where

A_c is the certified value;

A is the result or the mean of results obtained for the certified reference material;

s_{Lc} is the between-laboratories standard deviation of the certifying laboratories;

s_{Wc} is the within-laboratory standard deviation of the certifying laboratories;

n_{Wc} is the average number of replicate determinations in the certifying laboratories;

N_c is the number of certifying laboratories;

n is the number of replicate determinations on the reference sample (in most cases, $n = 1$);

σ_L and σ_r are as defined in 8.2.1.

If condition (6) is satisfied, i.e. if the left-hand side of the condition is less than or equal to the right-hand side, then the difference $|A_c - A|$ is statistically insignificant; otherwise, it is statistically significant.

When the difference is significant, the analysis shall be repeated, simultaneously with an analysis of the test sample. If the difference is again significant, the procedure shall be repeated using a different certified reference material of the same type of ore.

²⁾ Additional information is given in Annex B and Annex C.

When the range of the two values for the test sample is outside the limit for r calculated according to equation (2) in 8.2.1, one or more additional tests shall be carried out in accordance with the flowsheet presented in Annex A, simultaneously with an analysis of a certified reference material of the same type of ore.

Acceptability of the results for the test sample shall in each case be subject to the acceptability of the results for the certified reference material.

NOTE The following procedure should be used when the information on the reference material certificate is incomplete:

- a) if there are sufficient data to enable the between-laboratories standard deviation to be estimated, delete the expression $s_{w_c}^2/n_{w_c}$ and regard s_{L_c} as the standard deviation of the laboratory means;
- b) if the certification has been made by only one laboratory or if the interlaboratory results are missing, use the following condition:

$$|A_c - A| < 2 \sqrt{2\sigma_L^2 + \frac{\sigma_r^2}{n}} \quad \dots (7)$$

8.2.3 Calculation of final result

The final result is the arithmetic mean of the acceptable analytical values for the test sample or as otherwise determined by the operations specified in Annex A, calculated to five decimal places and rounded off to the third decimal place as follows:

- a) when the figure in the fourth decimal place is less than 5, it is discarded and the figure in the third decimal place is kept unchanged;

b) when the figure in the fourth decimal place is 5 and there is a figure other than 0 in the fifth decimal place, or

when the figure in the fourth decimal place is greater than 5, the figure in the third decimal place is increased by one;

c) when the figure in the fourth decimal place is 5 and there is the Figure 0 in the fifth decimal place, the 5 is discarded and the figure in the third decimal place is kept unchanged if it is 0, 2, 4, 6 or 8, and is increased by one if it is 1, 3, 5, 7 or 9;


9 Test report

The test report shall include the following information:

- a) reference to this International Standard;
- b) details necessary for the identification of the sample;
- c) result of the analysis;
- d) reference number of the result;
- e) any characteristics noticed during the determination and any operations not specified in this International Standard, or in the International Standards to which reference is made, which may have influenced the result, either for the test sample or the certified reference material(s).

Annex A Flowsheet of the procedure for the acceptance of analytical values for test samples

(An integral part of this International Standard.)

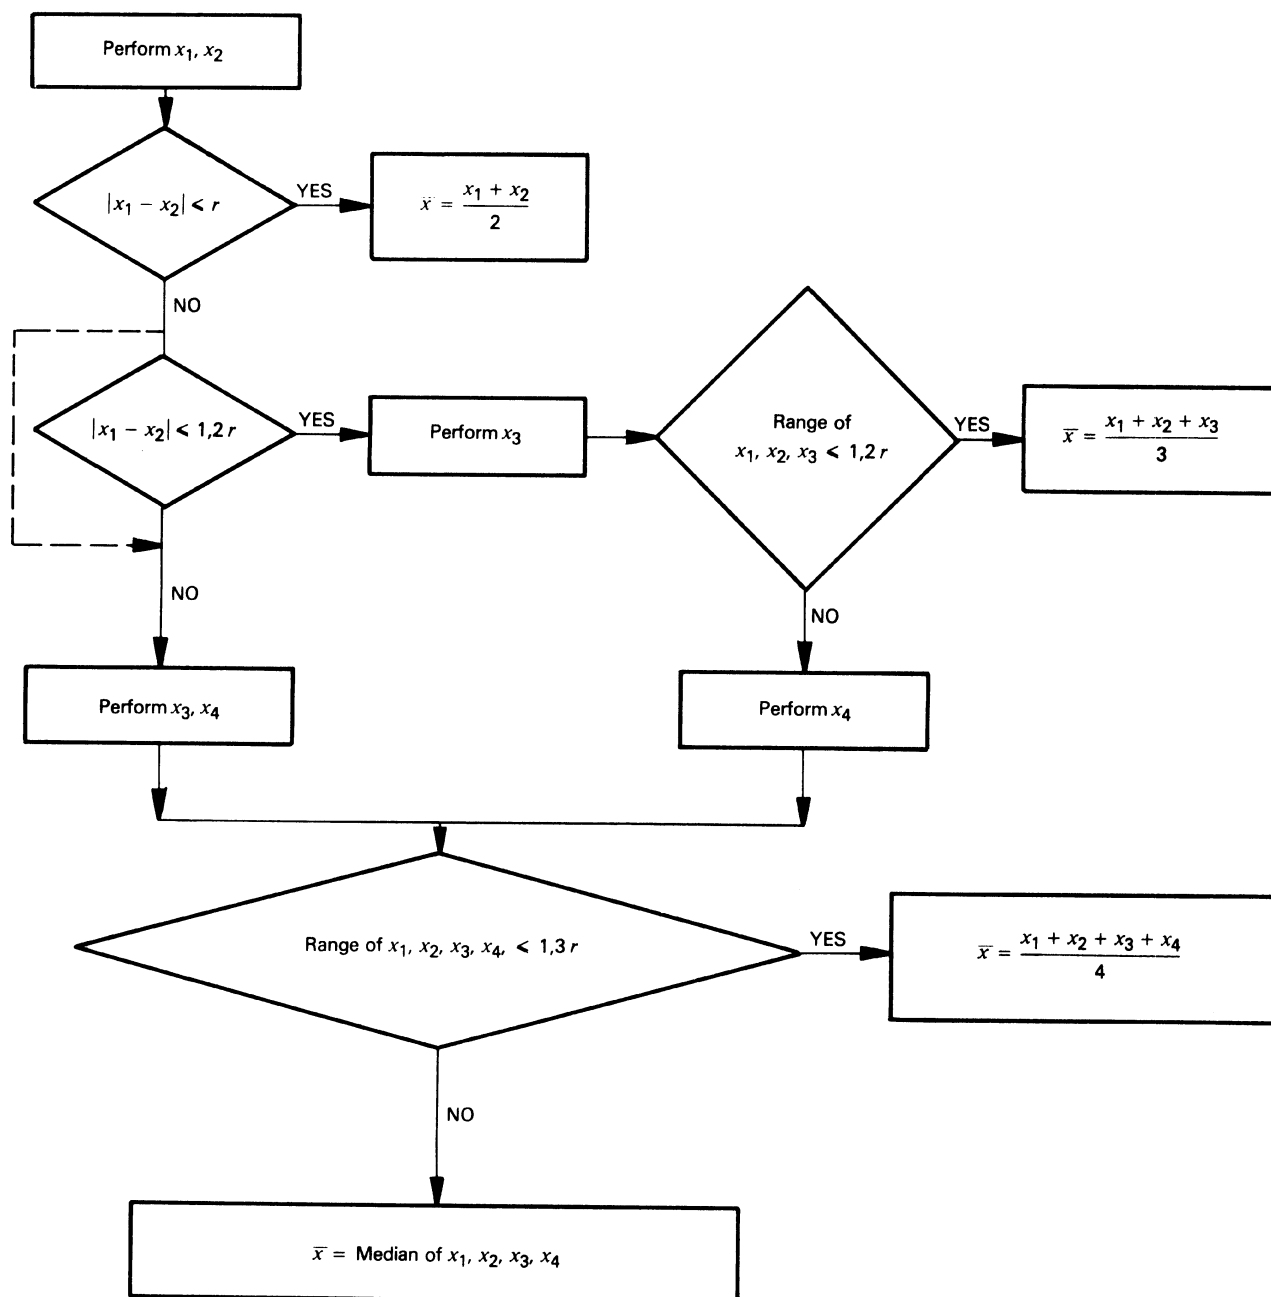

r: as defined in 8.2.1.

Annex B Derivation of repeatability and permissible tolerance equations

(This annex is for information only, and is not an integral part of this International Standard.)

The regression equations in 8.2.1 have been derived from the results of international analytical trials carried out in 1974/1975 on five iron ore samples involving 23 laboratories in six countries.

Graphical treatment of the precision data is given in Annex C.

The test samples used were:

| Sample | Sulfur content [% (m/m)] |
|------------------------------|--------------------------|
| Nimba | 0,006 |
| Kiruna D | 0,019 |
| Rompin | 0,078 |
| Texada | 0,255 |
| Roasting residue (Purpurerz) | 0,534 |


NOTE 1 A report of the international trial and a statistical analysis of the results (Document ISO/TC 102/SC 2 N 440 E, April 1976) is available either from the Secretariat of ISO/TC 102/SC 2 or from the Secretariat of ISO/TC 102.

NOTE 2 The statistical analysis has been performed in accordance with the principles embodied in ISO 5725.

Annex C Precision data obtained by international analytical trial

(This annex is for information only, and is not an integral part of this International Standard.)

NOTE This figure is a graphical presentation of the equations in 8.2.1.

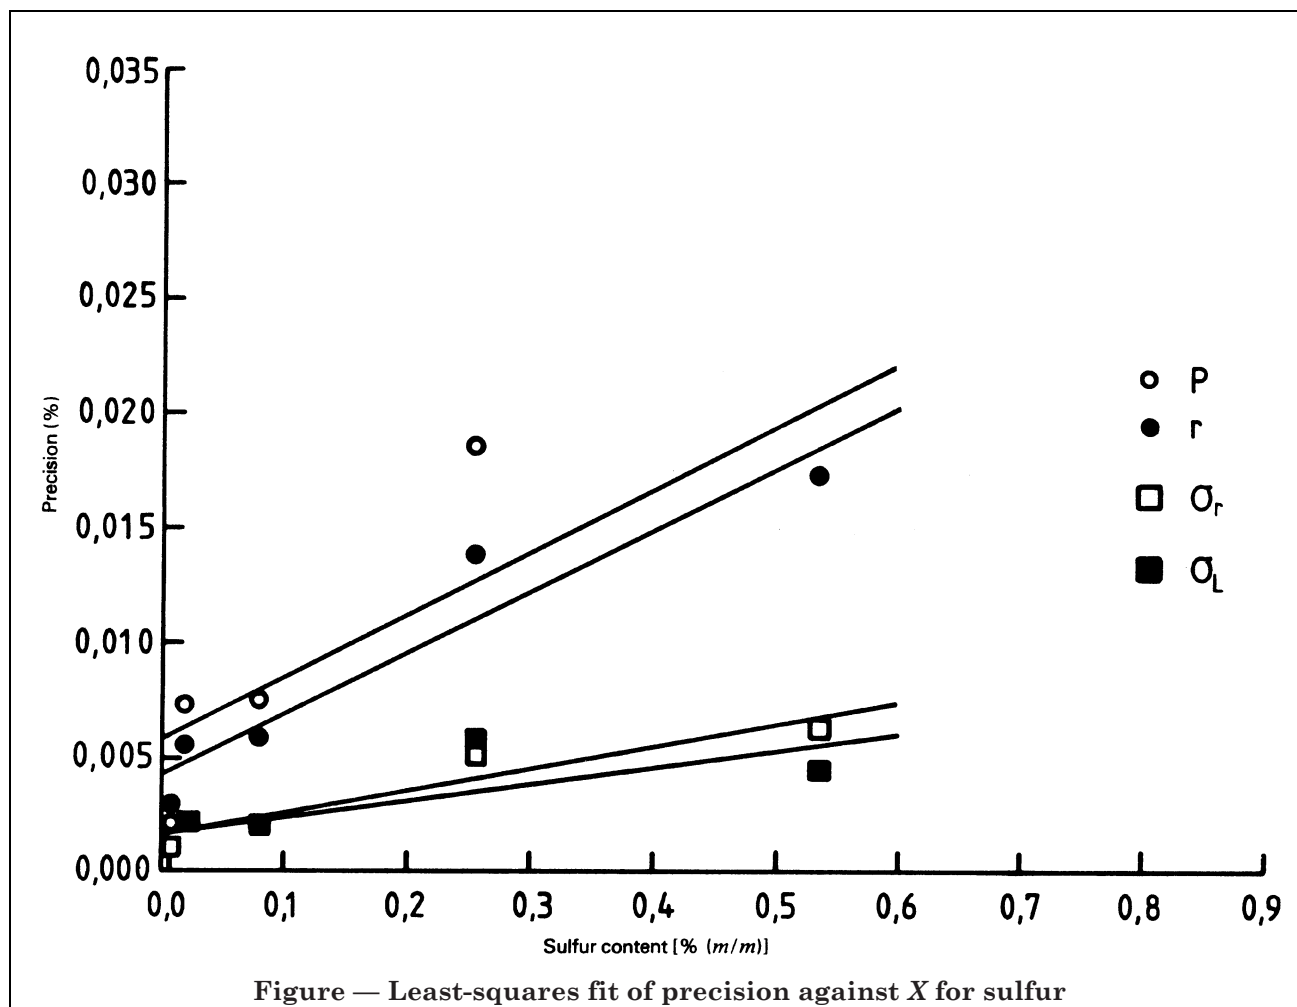

Publications referred to

See national foreword.

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover.
Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre.
Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration.
Tel: 020 8996 7002. Fax: 020 8996 7001.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager.
Tel: 020 8996 7070.