



BSI Standards Publication

# Industrial process control devices — Radiation thermometers

Part 2: Determination of the technical data for radiation thermometers

### **National foreword**

This Published Document is the UK implementation of IEC/TS 62492-2:2013.

The UK participation in its preparation was entrusted by Technical Committee GEL/65, Measurement and control, to Subcommittee GEL/65/2, Elements of systems.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2013.  
Published by BSI Standards Limited 2013

ISBN 978 0 580 80684 1  
ICS 17.200.20; 25.040.40

**Compliance with a British Standard cannot confer immunity from legal obligations.**

This Published Document was published under the authority of the Standards Policy and Strategy Committee on 31 August 2013.

### **Amendments/corrigenda issued since publication**

<b>Date</b>	<b>Text affected</b>
-------------	----------------------

---



# TECHNICAL SPECIFICATION



---

## Industrial process control devices – Radiation thermometers – Part 2: Determination of the technical data for radiation thermometers

INTERNATIONAL  
ELECTROTECHNICAL  
COMMISSION

PRICE CODE

U

---

ICS 17.200.20; 25.040.40

ISBN 978-2-83220-737-6

**Warning! Make sure that you obtained this publication from an authorized distributor.**

## CONTENTS

FOREWORD.....	4
1 Scope.....	6
2 Normative references .....	6
3 Terms, definitions and abbreviations .....	6
3.1 Terms and definitions .....	6
3.2 Abbreviations .....	9
4 Measurement conditions.....	9
5 Determination of technical data .....	9
5.1 Measuring temperature range.....	9
5.1.1 General .....	9
5.1.2 Test method .....	10
5.2 Measurement uncertainty .....	10
5.2.1 General .....	10
5.2.2 Test method .....	10
5.3 Noise equivalent temperature difference (NETD).....	11
5.3.1 General .....	11
5.3.2 Test method .....	11
5.4 Measuring distance .....	12
5.5 Field-of-view (target size).....	12
5.5.1 General .....	12
5.5.2 Test method .....	13
5.6 Distance ratio .....	14
5.7 Size-of-source effect (SSE) .....	14
5.7.1 General .....	14
5.7.2 Test method .....	14
5.8 Emissivity setting .....	15
5.9 Spectral range.....	15
5.10 Influence of the internal instrument or ambient temperature (temperature parameter) .....	15
5.10.1 General .....	15
5.10.2 Test method .....	16
5.11 Influence of air humidity (humidity parameter) .....	17
5.12 Long-term stability.....	17
5.12.1 General .....	17
5.12.2 Test method .....	17
5.13 Short-term stability .....	18
5.13.1 General .....	18
5.13.2 Test method .....	18
5.14 Repeatability .....	18
5.14.1 General .....	18
5.14.2 Test method .....	19
5.15 Interchangeability.....	19
5.15.1 General .....	19
5.15.2 Test method .....	19
5.16 Response time .....	20
5.16.1 General .....	20
5.16.2 Test method .....	21

5.17	Exposure time .....	22
5.17.1	General .....	22
5.17.2	Test method .....	23
5.18	Warm-up time.....	24
5.18.1	General .....	24
5.18.2	Test method .....	24
5.19	Operating temperature and air humidity range .....	25
5.19.1	General .....	25
5.19.2	Test method .....	25
5.20	Storage and transport temperature and air humidity range .....	26
5.20.1	General .....	26
5.20.2	Test method .....	26
6	Safety requirement .....	27
Annex A (informative) Change in indicated temperature of a radiation thermometer corresponding to a change in the radiation exchange.....		28
Bibliography.....		29
Figure 1 – Relative signal to a signal at a defined aperture size (source size) of 100 mm in diameter for two infrared radiation thermometers A and B versus the source diameter .....		12
Figure 2 – Demonstration of the response time to a rising temperature step .....		20
Figure 3 – Possible arrangement for determining the response time with two reference sources.....		22
Figure 4 – Demonstration of the exposure time .....		22
Figure 5 – Example of warm-up time .....		25
Table A.1 – The change in indicated temperature corresponding to a 1 % change in the radiation exchange with a radiation thermometer at 23 °C (Example).....		28

## INTERNATIONAL ELECTROTECHNICAL COMMISSION

**INDUSTRIAL PROCESS CONTROL DEVICES –  
RADIATION THERMOMETERS –****Part 2: Determination of the technical data  
for radiation thermometers**

## FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

The main task of IEC technical committees is to prepare International Standards. In exceptional circumstances, a technical committee may propose the publication of a technical specification when

- the required support cannot be obtained for the publication of an International Standard, despite repeated efforts, or
- the subject is still under technical development or where, for any other reason, there is the future but no immediate possibility of an agreement on an International Standard.

Technical specifications are subject to review within three years of publication to decide whether they can be transformed into International Standards.

IEC 62492-2, which is a technical specification, has been prepared by subcommittee 65B: Measurement and control devices, of IEC technical committee 65: Industrial-process measurement, control and automation.

The text of this technical specification is based on the following documents:

Enquiry draft	Report on voting
65B/844/DTS	65B/859/RVC

Full information on the voting for the approval of this technical specification can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

A list of all parts in the IEC 62492 series, published under the general title *Industrial process control devices – Radiation thermometers*, can be found on the IEC website.

The committee has decided that the contents of this publication will remain unchanged until the stability date indicated on the IEC web site under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- transformed into an International Standard,
- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

A bilingual version of this publication may be issued at a later date.

**IMPORTANT – The 'colour inside' logo on the cover page of this publication indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this document using a colour printer.**

# INDUSTRIAL PROCESS CONTROL DEVICES – RADIATION THERMOMETERS –

## Part 2: Determination of the technical data for radiation thermometers

### 1 Scope

This part of IEC 62492, which is a Technical Specification, applies to radiation thermometry and addresses all technical data specified in IEC/TS 62492-1. It defines standard test methods which can be used by the end user of radiation thermometers to determine or confirm the fundamental metrological data of radiation thermometers with one wavelength range and one measurement field.

The purpose of this specification is to facilitate comparability and testability. Therefore, unambiguous test methods are stipulated for determining technical data, under standardised measuring conditions that can be performed by a sufficiently skilled end user to serve as standard performance criteria for instrument evaluation or selection.

It is not compulsory for manufacturers and sellers of radiation thermometers to include all technical data given in this document in the data sheets for a specific type of radiation thermometer. Only the relevant data should be stated and should comply with this specification and IEC/TS 62492-1.

NOTE Infrared ear thermometers are excluded from this Technical Specification.

### 2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC/TS 62492-1:2008, *Industrial process control devices – Radiation thermometers – Part 1: Technical data for radiation thermometers*

### 3 Terms, definitions and abbreviations

#### 3.1 Terms and definitions

For the purposes of this document the following terms and definitions apply.

NOTE The terms and definitions listed below comply with IEC/TS 62492-1.

##### 3.1.1

##### **measuring temperature range**

temperature range for which the radiation thermometer is designed

##### 3.1.2

##### **measurement uncertainty**

parameter, associated with the result of a measurement, that characterises the dispersion of the values that could reasonably be attributed to the measurand



**3.1.3****noise equivalent temperature difference**

parameter which indicates the contribution of the measurement uncertainty in °C, which is due to instrument noise

**3.1.4****measuring distance**

distance or distance range between the radiation thermometer and the target (measured object) for which the radiation thermometer is designed

**3.1.5****field-of-view**

a usually circular, flat surface of a measured object from which the radiation thermometer receives radiation

**3.1.6****distance ratio**

the ratio of the measuring distance to the diameter of the field-of-view, when the target is in focus

**3.1.7****size-of-source effect**

the difference in the radiance or temperature reading of the radiation thermometer when changing the size of the radiating area of the observed source

**3.1.8****emissivity setting**

ratio between the radiation emitted from this surface and the radiation from a blackbody at the same temperature

Note 1 to entry: In most measuring situations a radiation thermometer is used on a surface with an emissivity significantly lower than 1. For this purpose most thermometers have the possibility of adjusting the emissivity setting. The temperature reading is then automatically corrected.

**3.1.9****spectral range**

parameter which gives the lower and upper limits of the wavelength range over which the radiation thermometer collects radiation from a source

**3.1.10****influence of the internal instrument temperature****influence of the ambient temperature****temperature parameter**

parameter which gives the additional uncertainty of the measured temperature value depending on the deviation of the temperature of the radiation thermometer from the value for which the technical data is valid after warm-up time and under stable ambient conditions

**3.1.11****influence of air humidity****humidity parameter**

parameter which gives the additional uncertainty of the measured temperature value depending on the relative air humidity at a defined ambient temperature

**3.1.12****long-term stability**

the reproducibility of measurements repeated over a long time period

Note 1 to entry: The time period is typically three months or one year.

### **3.1.13**

#### **short-term stability**

the reproducibility of measurements repeated over a short time period

Note 1 to entry: The time period is several hours.

### **3.1.14**

#### **repeatability**

twice the standard deviation of measurements repeated under the same conditions within a very short time span

Note 1 to entry: The time span is several minutes.

### **3.1.15**

#### **interchangeability**

the maximum deviation between the readings of two instruments of the same type operating under identical conditions divided by two

### **3.1.16**

#### **response time**

time interval between the instant of an abrupt change in the value of the input parameter and the instant from which the measured value of the radiation thermometer remains within specified limits of its final value

Note 1 to entry: The input parameter is an object temperature or an object radiation, and the output value is an output parameter.

### **3.1.17**

#### **exposure time**

time interval between an abrupt rise and an abrupt fall in the value of the input parameter, such that the output value of the radiation thermometer reaches a given measurement value

Note 1 to entry: The input parameter is an object temperature or an object radiation.

### **3.1.18**

#### **warm-up time**

time period needed for the radiation thermometer, after switching on, before it operates according to its specifications

### **3.1.19**

#### **operating temperature**

the permissible temperature range within which the radiation thermometer may be operated

Note 1 to entry: For this temperature the specifications are valid.

### **3.1.20**

#### **operating air humidity range**

the permissible humidity range within which the radiation thermometer may be operated

Note 1 to entry: For this humidity range the specifications are valid.

### **3.1.21**

#### **storage and transport temperature**

the permissible ambient temperature range within which the radiation thermometer may be stored and transported without suffering permanent change

### **3.1.22**

#### **storage and transport air humidity range**

the permissible humidity range within which the radiation thermometer may be stored and transported without suffering permanent change

### **3.1.23**

#### **safety**

freedom from unacceptable risk

### **3.1.24**

#### **risk**

combination of the probability of the occurrence of harm and the severity of that harm

### **3.1.25**

#### **harm**

physical injury or damage to the health of people, or damage to property or the environment

### **3.1.26**

#### **tolerable risk**

risk which is accepted in a given context based on the current values of society

## **3.2 Abbreviations**

FWHM Full width at half maximum

NETD Noise equivalent temperature difference

SSE Size-of-source effect

## **4 Measurement conditions**

The following test conditions apply for all measurements, if not stated otherwise:

- a) laboratory ambient temperature range from 18 °C to 28 °C;
- b) any special ambient conditions (e.g. humidity range, maximum ambient temperature change per time) and measurement conditions (e.g. measuring distance, radiating area diameter, response time) given by the manufacturer for the specific radiation thermometer to be adhered to;
- c) the radiation thermometer to be connected to a power supply in accordance to the manufacturer's instructions;
- d) the warm-up time specified by the manufacturer to be adhered to;
- e) internal standardization check (initial self-test) to be carried out, if available;
- f) emissivity setting set to 1 (one), if available;
- g) the reference temperature source shall have a radiating area diameter as large as possible and in any case greater than the radiation thermometer field-of-view (target area) diameter;
- h) all tests have to be performed with the reference temperature source set to a temperature that is significantly different from ambient temperature and the internal temperature of the radiation thermometer.

NOTE The reference temperature source is a radiation source of known radiation temperature in the spectral range of the radiation thermometer. Usually it is a blackbody source realised by a cavity radiator of known temperature. It will be called "reference source" throughout this document.

## **5 Determination of technical data**

### **5.1 Measuring temperature range**

#### **5.1.1 General**

The purpose of this test is to determine the measuring temperature range. For this temperature range, the measurement uncertainty remains within the specified limits.

Measurement temperature range (5.1), as well as Measurement uncertainty (5.2) and Noise equivalent temperature difference (5.3), are the most important parameters that specify a radiation thermometer. These three parameters are correlated with each other and in general noise equivalent temperature difference is larger at the lower limit of the measuring temperature range where uncertainty is larger. This relation is demonstrated in Table A.1 and the equation of Annex A.

NOTE Sometimes it is useful to determine additionally a wider *indicating temperature range* over which the thermometer will display a temperature but its specifications are not guaranteed.

### 5.1.2 Test method

**5.1.2.1** The determination of the *measuring temperature range* is performed in accordance with 5.2.2 at the top and the bottom temperature of the specified measuring temperature range.

Determination of the *indicating temperature range*:

**5.1.2.2** Sight the radiation thermometer at the centre of the radiating area of the reference source.

**5.1.2.3** The temperature of the reference source is sequentially adjusted and stabilised at temperatures around the minimum temperature and the maximum temperature of the *indicating temperature range* given by the manufacturer, to determine the minimum and maximum temperatures for which the radiation thermometer is still indicating.

**5.1.2.4** These two temperatures give the *indicating temperature range*.

## 5.2 Measurement uncertainty

### 5.2.1 General

A detailed description of the different methods to determine the measurement uncertainty and its confidence level is beyond the scope of this technical specification. In this technical specification terms, concept and definition of uncertainty is based on ISO/IEC Guide 98-3 and ISO/IEC Guide 99.

The described method is a basic test of the measurement uncertainty across the measuring temperature range.

### 5.2.2 Test method

**5.2.2.1** Sight the radiation thermometer at the centre of the radiating area of the reference source.

**5.2.2.2** The temperature of the reference source is sequentially stabilised at, at least, three temperatures distributed at the top, the bottom and an intermediate temperature of the measuring temperature range (see Note 1 of 5.2.2.5).

**5.2.2.3** The temperature of the reference source and the temperature indicated by the radiation thermometer are recorded. The difference between these two values is calculated and recorded.

**5.2.2.4** The test sequence is performed three times for the same three calibration points. An average temperature difference is calculated and recorded for each calibration temperature point.

**5.2.2.5** The value of the measurement uncertainty of the radiation thermometer at each calibration temperature is taken to be the average difference determined in 5.2.2.4 plus the

temperature uncertainty of the reference source in respect to the current International Temperature Scale.

NOTE 1 The number of temperature points depends on the requirements of the specific thermometer and its application.

NOTE 2 For radiation thermometers with more than one measuring temperature range each range is calibrated as if it were a separate instrument.

Due to the small number of observations care shall be taken not to infer too much significance from this basic test (i.e. no confidence level can be given).

In order to use this method to test for compliance of measuring temperature range and measurement uncertainty with the data provided by the manufacturer, the temperature uncertainty of the reference source shall be significantly smaller than the uncertainty of the radiation thermometer.

### **5.3 Noise equivalent temperature difference (NETD)**

#### **5.3.1 General**

The purpose of this method is to determine the NETD. The measured temperature and the response time of the radiation thermometer are to be stated with the NETD. For some instruments the NETD depends on the instrument or ambient temperature. For these instruments the instrument or ambient temperature also has to be stated. For low cost instruments the NETD may be limited by their resolution.

The NETD is generally largest at the lowest temperature of the measuring temperature range. When using electronic measuring equipment, its bandwidth shall be noted or set accordingly. In particular, the bandwidth of the radiation thermometer shall not be limited by the bandwidth of the external measuring equipment. In contrast to the other metrological data, the confidence level in this case is 68,3 % (standard uncertainty,  $k = 1$ ).

#### **5.3.2 Test method**

**5.3.2.1** Sight the radiation thermometer at the centre of the radiating area of the reference source.

**5.3.2.2** The temperature of the reference source is stabilised at a temperature within the measuring temperature range of the radiation thermometer. The greatest expected noise amplitudes may not exceed the limits of the measuring temperature range.

**5.3.2.3** The total measurement time is at least 100 times the set response time of the radiation thermometer with at least 100 measured values taken.

**5.3.2.4** The NETD of the radiation thermometer is calculated as the standard deviation of the measured values, and stated together with the reference source temperature and the set response time.

Noise caused by the temperature stability of the reference source and additional measurement equipment shall be significantly lower than the noise of the radiation thermometer.

According to 5.3.1 the NETD is expected to vary across the measuring temperature range. Therefore, for completeness, the NETD should be determined at a minimum of two temperatures, one of which is the lowest measuring temperature.

## 5.4 Measuring distance

For this distance or distance range the specifications are valid, if not stated otherwise. No specific test method is needed.

NOTE The calibration of a radiation thermometer, with respect to a reference source of the same area, gives different results at different distances due to the SSE of the instrument.

## 5.5 Field-of-view (target size)

### 5.5.1 General

Its magnitude is determined by the optical components in the radiation thermometer. As the field-of-view is not sharply defined, it is necessary to state the diameter of the field-of-view at which the radiation signal has dropped to a certain fraction of its total integrated value (hemispherical value or the value for an infinitely extended source). The fraction value should be at least 90 %; typical values are 90 %, 95 % and 99 %.

For some radiation thermometers, especially for high temperature instruments, it is impracticable to relate the field-of-view to a hemispherical value. In this case it is allowed to relate the given field-of-view to a larger source (e.g. twice as large in area as the field-of-view).

As the field-of-view value depends on the measuring distance, it is necessary to state the measuring distance in addition to the fraction.

The transfer function between the *measured radiation* (input parameter) and *temperature* (output parameter) is non-linear. As an example the change in indicated temperature corresponding to a 1 % change in the radiation exchange with a radiation thermometer is given in Annex A. The field-of-view is therefore either defined for the *fraction of measured radiation* or, for instruments which only read directly in temperature, it is necessary to specify a *change in the measured temperature* in °C at a given temperature for the field-of-view in comparison to the total integrated value (hemispherical value or the value for an infinitely extended source). As a minimum, these values should be given for the top, middle and bottom of the temperature range.

The complete field-of-view information would be a graph (see Figure 1), which shows the signal or temperature versus source size (size-of-source effect).

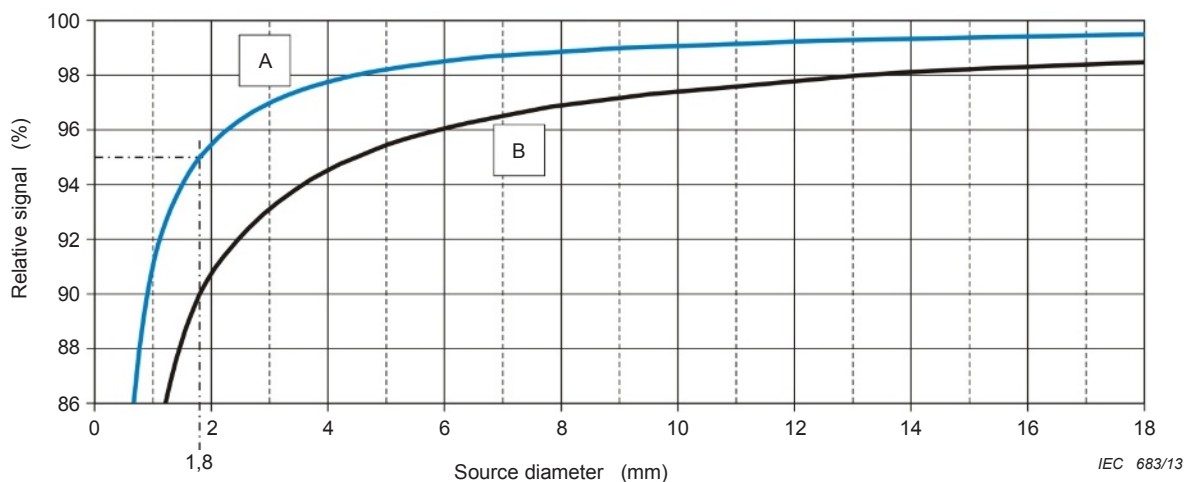


Figure 1 – Relative signal to a signal at a defined aperture size (source size) of 100 mm in diameter for two infrared radiation thermometers A and B versus the source diameter

Explanation of Figure 1: The field-of-view diameter (target diameter) is stated as 1,8 mm for each of the two radiation thermometers A and B. For radiation thermometer A, this corresponds to 95 % of the maximum measuring signal, while for radiation thermometer B it corresponds to 90 % of the maximum measuring signal. The figure indicates the change in the measuring signal with the change in source diameter. In order to achieve 98 % of the maximum measuring signal, a source diameter of 4,5 mm is required for radiation thermometer A while a source diameter of 13 mm is required for radiation thermometer B. The maximum measuring signal in this example is determined at a source (aperture) diameter of 100 mm and is taken to be 100 % of the hemispherical value.

The following test method determines the diameter of the field-of-view at which the signal has dropped to a 99 % fraction of the hemispherical value or is related to a 99 % fraction of the signal at a defined aperture size of the source. The method can be adapted accordingly to determine the field of view of radiation thermometers which relates to 95 % or 90 % of the hemispherical value or the signal at a defined aperture size of the source.

## 5.5.2 Test method

**5.5.2.1** Sight the radiation thermometer at the centre of the radiating area of the reference source at the specified measuring distance. Position an iris diaphragm in front of and concentric with the opening of the reference source. The minimum opening of the reference source shall be large enough so as not to obstruct the optical path (i.e. the nominal field-of-view as specified by the manufacturer) of the radiation thermometer when the thermometer is sighted through the plane of the iris and the iris is set at a diameter of at least twice the field-of-view of the instrument.

**5.5.2.2** The temperature of the reference source is stabilised at a temperature near the top of the measuring temperature range of the radiation thermometer.

**5.5.2.3** The iris is adjusted to a diameter slightly smaller (typically 10 % less) than the expected field-of-view.

**5.5.2.4** The position of the radiation thermometer is adjusted vertically and horizontally and focused if applicable to produce maximum output while also maintaining the line of sight perpendicular to the iris.

**5.5.2.5** The iris is opened to the point where the temperature indicated by the radiation thermometer stops increasing, but its diameter is still smaller than the reference source opening. In this case, the field-of-view is defined in terms of the 99 % fraction of the hemispherical value. If the temperature indicated by the radiation thermometer does not stabilize after exceeding the largest possible iris diameter, the field-of-view is defined in terms of the maximum iris diameter for which the temperature source does not obstruct the optical path of the radiation thermometer.

**5.5.2.6** The iris diameter is decreased until the radiation measured by the radiation thermometer decreases by 1 % of the original signal or the temperature indicated by the radiation thermometer decreases by the amount appearing in Annex A.

**5.5.2.7** The value for the field-of-view at the measuring distance chosen is taken to be the diameter of the iris opening for which the radiant power received by the radiation thermometer or the temperature indicated by the radiation thermometer has been reduced according to 5.5.2.6.

The reference source shall have a stable and homogenous radiance temperature within its radiating area (i.e. *the temperature and emissivity of the source shall not change when changing the size of the radiating area* or such changes have to be corrected).

The iris shall be kept cool enough so that its thermal emission does not contribute significantly to the output signal. In most cases the error is insignificant if the iris is



maintained near room temperature and the temperature of the reference source is at or above 200 °C.

## 5.6 Distance ratio

As the distance ratio is defined as the ratio of the measuring distance to the diameter of the field-of-view no specific test method is needed.

## 5.7 Size-of-source effect (SSE)

### 5.7.1 General

To describe the SSE the difference in the radiance or temperature reading of the radiation thermometer when changing the size of the radiating area of the observed source shall be stated. The complete information would be a graph, which shows the signal or temperature reading versus source diameter (see Figure 1).

To simplify the SSE statement and make it more comparable, the following measurement conditions shall be used as far as possible: the SSE is to be stated at a given measuring distance, measured temperature and ambient temperature, when observing a target with the area of the nominal field-of-view and twice the area of the nominal field-of-view or more than twice the area of the nominal field-of-view. In the latter case, the area should be specified.

The SSE is either defined as the relative change in the observed radiance or, for instruments which only read in temperature, as the absolute change in the measured temperature at a given temperature, when changing the observed target area. Since the latter definition depends on the source temperature it is necessary to state the SSE at the top, middle and bottom temperatures of the measuring temperature range.

The following test method determines the SSE when increasing the area of the target from the nominal field-of-view to twice the field-of-view. With the size-of-source effect it is necessary to state the measuring distance, the measured temperature and the surrounding temperature of the source.

### 5.7.2 Test method

**5.7.2.1** Sight the radiation thermometer at the centre of the radiating area of the reference source at the specified measuring distance. Position an iris diaphragm in front of and concentric with the opening of the reference source. The minimum opening of the reference source shall be large enough so as not to obstruct the optical path of the radiation thermometer, i.e. the nominal field-of-view as specified by the manufacturer, when the thermometer is sighted through the plane of the iris and the iris is set at a diameter of at least twice the field-of-view of the instrument.

**5.7.2.2** The temperature of the reference source is stabilised at a temperature near the top of the measuring temperature range of the radiation thermometer.

**5.7.2.3** The iris is adjusted to a diameter slightly smaller (typically 10 % less) than the expected field-of-view.

**5.7.2.4** The position of the radiation thermometer is adjusted vertically and horizontally and focused if applicable to produce maximum output while also maintaining the line of sight perpendicular to the iris.

**5.7.2.5** The iris is opened to the diameter specified as the nominal field-of-view by the manufacturer and the radiation signal or the temperature indicated by the radiation thermometer is recorded.



**5.7.2.6** The iris area is increased to an area twice the nominal field-of-view of the radiation thermometer. The radiation signal or the temperature indicated by the radiation thermometer is recorded.

**5.7.2.7** The relative change in radiance reading or the absolute change in temperature reading when changing the size of the iris is recorded as the SSE of the radiation thermometer.

**5.7.2.8** For radiation thermometers which indicate temperature the test method is repeated for a temperature of the reference source stabilized near the middle and bottom of the temperature range.

The reference source shall have a stable and homogenous radiance temperature within its radiating area (i.e. *the temperature and emissivity of the source shall not change when changing the size of the radiating area* or such changes have to be corrected).

The iris shall be kept cool enough so that its thermal emission does not contribute significantly to the output signal. In most cases the error is insignificant if the iris is maintained near room temperature and the temperature of the reference source is at or above 200 °C.

## **5.8 Emissivity setting**

The range and the resolution of the emissivity setting shall be given by the manufacturer. For information on the internal emissivity correction procedure the manufacturer has to be contacted. A test method for the emissivity setting is beyond the scope of this technical specification.

## **5.9 Spectral range**

A test method for the determination of the spectral range is beyond the scope of this technical specification.

The spectral range is given in  $\mu\text{m}$  or nm. The lower and upper wavelength limits at which the spectral responsivity has reached 50 % of the peak responsivity are given as the spectral range. Alternatively, a mean wavelength and full wavelength width at which the responsivity has reached 50 % of the peak sensitivity (full width at half maximum (FWHM)) are given.

For some radiation thermometers, especially for narrow band or spectral radiation thermometers, it is more useful to give lower and upper wavelength limits at which the spectral responsivity has reached significantly less than 50 % of the peak responsivity (e.g. 10 %). In this case the criteria for the wavelength limits have to be stated.

## **5.10 Influence of the internal instrument or ambient temperature (temperature parameter)**

### **5.10.1 General**

The technical data of a radiation thermometer, e.g. the measurement uncertainty, shall be valid over the complete operating instrument or ambient temperature range and air humidity range, if not stated otherwise. If the measurement uncertainty is not valid in the complete operating instrument or ambient temperature range, the manufacturer shall state a temperature parameter which gives the additional measurement uncertainty when the instrument or ambient temperature deviates from a given reference temperature after warm-up time and under stable ambient conditions. It is given as the absolute or relative increase in the uncertainty of the measured value when the instrument or ambient temperature deviates from the reference temperature.

### 5.10.2 Test method

**5.10.2.1** The radiation thermometer is operated in an adjustable temperature enclosure (e.g. climate chamber) at the instrument reference temperature given by the manufacturer. For instruments with no internal temperature indication the ambient temperature (i.e. the temperature of the climate chamber) shall be used as the instrument reference temperature.

**5.10.2.2** Sight the radiation thermometer at the centre of the radiating area of the reference source.

No window should be used between the radiation thermometer and the reference source. If a window is used, the influence of the window on the temperature indicated by the radiation thermometer shall be corrected for.

**5.10.2.3** The temperature of the reference source is stabilised near the bottom of the measuring temperature range of the radiation thermometer. If another source temperature is used, this should be stated.

**5.10.2.4** The temperature of the reference source and the temperature indicated by the radiation thermometer are recorded. The difference between these two values is calculated and recorded.

**5.10.2.5** The radiation thermometer is stabilised at the minimum internal temperature specified by the manufacturer.

**5.10.2.6** The temperature of the reference source and the temperature indicated by the radiation thermometer are recorded. The difference between these two values is calculated and recorded.

**5.10.2.7** The radiation thermometer is stabilised at the maximum internal temperature specified by the manufacturer.

**5.10.2.8** The temperature of the reference source and the temperature indicated by the radiation thermometer are recorded. The difference between these two values is calculated and recorded.

**5.10.2.9** The value of the measurement uncertainty of the radiation thermometer at each internal temperature is taken to be the difference determined in 5.10.2.4, 5.10.2.6 and 5.10.2.8 plus the temperature uncertainty of the reference source in respect to the current International Temperature Scale. From these uncertainties the temperature parameter of the radiation thermometer, as the absolute or relative increase in uncertainty as the ambient temperature deviates from the reference temperature, is derived.

Due to the small number of observations special care shall be taken not to infer too much significance from this test (i.e. no confidence level can be given).

Moisture condensation on the radiation thermometer (i.e. on the optics) shall be avoided throughout the test.

In order to use this method to test for compliance of the temperature parameter with the data provided by the manufacturer the temperature uncertainty of the reference source shall be significantly smaller than the uncertainty of the radiation thermometer.

The minimum time necessary for the thermal stabilisation of the radiation thermometer has to elapse after each change of temperature of the climate chamber. This stabilisation time might be longer than the climate chamber stabilisation time.

### 5.11 Influence of air humidity (humidity parameter)

The technical data of a radiation thermometer, e.g. the measurement uncertainty, shall be valid over the specified measuring distance and operating temperature range and air humidity range, if not stated otherwise. If within the specified measurement distance range the measurement uncertainty is not valid in the complete operating air humidity range, the manufacturer shall state a humidity parameter which gives the additional measurement uncertainty when the air humidity deviates from a given reference humidity.

A deviation of the air humidity from the reference air humidity leads to an additional uncertainty in temperature measurement. The humidity parameter gives the additional uncertainty of the measured temperature value depending on the relative air humidity at a defined ambient temperature. It is given as the absolute or relative increase in uncertainty in the measured value per percentage change in the air humidity relative to the reference humidity.

For the determination of the humidity parameter well defined atmospheric conditions regarding the chemistry and temperature of the atmosphere have to be realised. A test method for the humidity parameter is beyond the scope of this technical specification.

### 5.12 Long-term stability

#### 5.12.1 General

The long-term stability should be stated in °C over a time span of 90 days or over one year.

The long-term stability depends on the stability of the mechanical, electrical and optical components of the radiation thermometer, the measured temperature and the confidence level.

#### 5.12.2 Test method

**5.12.2.1** Sight the radiation thermometer at the centre of the radiating area of the reference source.

**5.12.2.2** The temperature of the reference source is stabilised at a temperature within the measuring temperature range of the radiation thermometer.

**5.12.2.3** The total measurement time is at least 10 times the set response time of the radiation thermometer with at least 10 measured values of the temperature indicated by the radiation thermometer taken. The arithmetic mean of the measurement values is calculated.

**5.12.2.4** The test sequence from 5.12.2.1 to 5.12.2.3 is performed at least once a month at the same temperature of the reference source over a time span of three months or one year. The radiation thermometer shall be turned off between the test sequences.

It is allowed for a manufacturer to perform an accelerated test in accordance with an established procedure based on the manufacturer's technical knowledge and experience.

**5.12.2.5** The long-term stability is taken to be the difference between the maximum and minimum mean values of temperature reading obtained over the test interval.

The long-term stability of the reference source shall be significantly better than the long-term stability of the radiation thermometer.

The test shall be performed with the reference source set to a temperature such that the radiation thermometer does not indicate its internal temperature or ambient temperature.

The radiation thermometer shall be kept under ambient conditions in accordance with the manufacturer's specifications during the complete test interval.

Due to the small number of observations special care shall be taken not to infer too much significance from this basic test (i.e. no confidence level can be given).

### **5.13 Short-term stability**

#### **5.13.1 General**

The short-term stability should be stated in a rate °C/h or as a maximum temperature deviation within a short time span (several hours) after warm-up time.

The short-term stability depends on the measured temperature, the confidence level, the response time and the internal instrument or ambient temperature. These parameters are to be stated.

#### **5.13.2 Test method**

**5.13.2.1** Sight the radiation thermometer at the centre of the radiating area of the reference source.

**5.13.2.2** The temperature of the reference source is stabilised at a temperature within the measuring temperature range of the radiation thermometer.

**5.13.2.3** The total measurement time is at least 3 h with at least 10 measurement sequences evenly distributed over the measurement time. For each measurement sequence the measurement time is at least 10 times the set response time of the radiation thermometer with at least 10 measured values of the temperature indicated by the radiation thermometer taken. The radiation thermometer shall not be turned off during the total measurement time. The lens system of the radiation thermometer may be covered in time periods between taking measurement sequences to avoid heating of the radiation thermometer.

**5.13.2.4** The arithmetic mean of the measured values of the thermometer output for each measurement sequence is calculated.

**5.13.2.5** The short-term stability is taken to be the difference between the maximum and minimum mean values of temperature reading obtained over the measurement time. It may also be stated as the difference between the maximum and minimum mean values of temperature reading divided by the measurement time. The short-term stability should be calculated from half the difference between the maximum and minimum mean values if it is given as a plus or minus (+/-) statement.

The short-term stability of the reference source shall be significantly better than the short-term stability of the radiation thermometer.

The test shall be performed with the reference source set to a temperature such that the radiation thermometer does not indicate its internal temperature or ambient temperature.

The radiation thermometer shall be kept under ambient conditions in accordance with the manufacturer's specifications during the complete test interval.

### **5.14 Repeatability**

#### **5.14.1 General**

The repeatability is closely related to the NETD of a radiation thermometer and is determined over a time span of several minutes. The confidence level of the repeatability is twice as large as the confidence level of the NETD.

The measured temperature and the response time of the radiation thermometer are to be stated with the repeatability. For some instruments the repeatability depends on the instrument or ambient temperature. For these instruments the instrument or ambient temperature also has to be stated. For low cost instruments the repeatability may be limited by their resolution.

When using electronic measuring equipment, its bandwidth shall be noted or set accordingly. In particular, the bandwidth of the radiation thermometer shall not be limited by the bandwidth of the external measuring equipment.

#### **5.14.2 Test method**

**5.14.2.1** Sight the radiation thermometer at the centre of the radiating area of the reference source.

**5.14.2.2** The temperature of the reference source is stabilised at a temperature within the measuring temperature range of the radiation thermometer. The greatest expected noise amplitudes may not exceed the limits of the measuring temperature range.

**5.14.2.3** The total measurement time shall be at least 3 min, and of a duration of at least 100 times the set response time of the radiation thermometer, with at least 100 measured values of the temperature indicated by the radiation thermometer taken (see 5.14.2.4).

**5.14.2.4** The standard deviation is calculated from the measured values. The repeatability is twice the value of the standard deviation of the measured values of the temperature indicated by the radiation thermometer.

If the thermometer is affected by the heat of the reference source a shorter total measurement time shall be chosen.

Noise caused by the temperature stability of the reference source and additional measurement equipment shall be significantly lower than the noise of the radiation thermometer.

#### **5.15 Interchangeability**

##### **5.15.1 General**

No two instruments will differ by more than twice this figure.

The interchangeability value will not necessarily be the same as the uncertainty value. It is a critical parameter for the production control, when an instrument has to be replaced by another of the same type.

##### **5.15.2 Test method**

**5.15.2.1** For the determination of the interchangeability at least three instruments of the same type are needed.

**5.15.2.2** Sight the first radiation thermometer at the centre of the radiating area of the reference source.

**5.15.2.3** The temperature of the reference source is stabilised at a temperature within the measuring temperature range of the radiation thermometer.

**5.15.2.4** The total measurement time is at least 100 times the set response time of the radiation thermometer with at least 100 measured values of the temperature indicated by the radiation thermometer taken.

**5.15.2.5** The arithmetic mean of the measured temperature values indicated by the radiation thermometer is calculated.

**5.15.2.6** The test sequence from 5.15.2.2 to 5.15.2.5 is repeated for at least two more radiation thermometers of the same type, while the temperature of the reference source stays at the same temperature as in the first test.

**5.15.2.7** The interchangeability is the difference between the maximum and the minimum calculated arithmetic mean values from the radiation thermometers divided by 2.

Identical and stable ambient conditions shall be realized during the test of all radiation thermometers.

The stability of the temperature of the reference source throughout the test has to be significantly better than the interchangeability of the radiation thermometers.


Due to the small number of radiation thermometers special care shall be taken not to infer too much significance from this test (i.e. no confidence level can be given).

## 5.16 Response time

### 5.16.1 General

The lower/upper temperature value for specifying the response time has to be a temperature value within, respectively, the lower/upper quartile of the measuring temperature range (see Figure 2).

For a radiation thermometer the rise and fall times (response times for rising and falling temperature steps) might be different. If this is the case, it shall be stated.

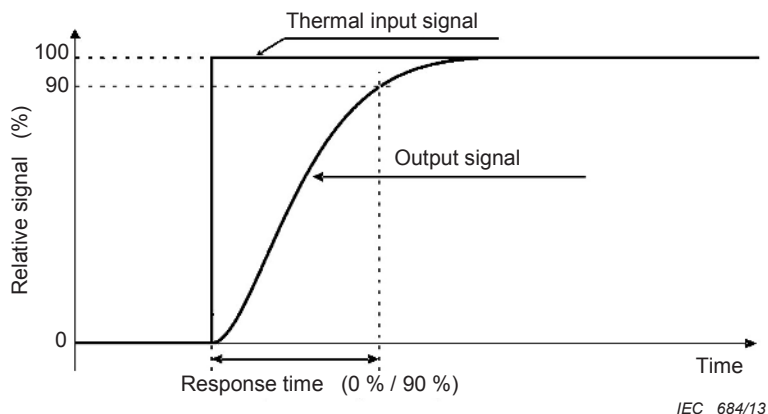

**Figure 2 – Demonstration of the response time to a rising temperature step**

The response time depends on the type of signal processing within the radiation thermometer. The magnitude of the temperature step (lower value and upper value) as well as the percentage or temperature limits are to be given when stating the response time.

The following test method outlines the procedure to determine the time required for the output signal of a radiation thermometer to reach 90 % of the full scale response to a corresponding step change of input radiant power starting at ambient temperature radiation to a temperature radiation close to the top of the measuring temperature range of the radiation thermometer. The response time may be specified as a different percentage level of the full scale response, e.g. 99 % (see IEC/TS 62492-1:2008, 4.1.1.16.3). In this case the test method has to be adjusted accordingly.

### 5.16.2 Test method

**5.16.2.1** Sight the radiation thermometer at the centre of the radiating area of the reference source.

**5.16.2.2** The reference source is stabilised at a temperature close to the top of the measuring temperature range of the radiation thermometer.

**5.16.2.3** The sight path between the radiation thermometer and the reference source is interrupted by a shutter mechanism and the output of the radiation thermometer is allowed to stabilize at the radiation temperature of the shutter (ambient temperature).

**5.16.2.4** The data acquisition system is triggered and the shutter is opened such that the signal over time from the radiation thermometer in response to the full-scale step change in input radiant power can be measured and recorded (e.g. using a storage oscilloscope).


**5.16.2.5** As a digitally processed radiation thermometer may have a variation in the measured value of response time the measurement has to be repeated a sufficient number of times (at least five times) until the maximum value of response time is uniquely determined. Care has to be taken that the response time test method is only performed when the radiation thermometer is in the temperature measurement mode of operation, as radiation thermometers may periodically perform e.g. a calibration routine.

**5.16.2.6** The response time (0 %/90 %) is the longest measured time period for the thermometer to reach 90 % of the final (maximum) measured value (see Figure 2).

The time period needed for the shutter mechanism to open shall be much shorter than the response time (not more than 10 % of the response time) and the shutter shall have a stable radiation temperature near ambient temperature (i.e. no heating up by the reference source).

Instead of a reference source with a shutter mechanism a radiation source with rapidly adjustable radiation intensity and appropriate wavelength may be used. This can be for example a light emitting diode (LED) which is operated with a pulse generator. The radiation source is switched to continuous output and the signal output of the radiation thermometer is monitored with a rapid signal recording device e. g. a storage oscilloscope. If applying a LED, its operating current shall be adjusted until the required temperature indication at the radiation thermometer is achieved at the beginning of the test method. The pulse width is then reduced until the temperature display indicates a specific proportion of the minimum/maximum signal, e.g. 0 %/90 % of the original display. The set pulse width is now the response time.

For the determination of response times starting at temperatures different from ambient temperature an analogous method based on a more sophisticated setup with two reference sources (see Figure 3) shall be applied.

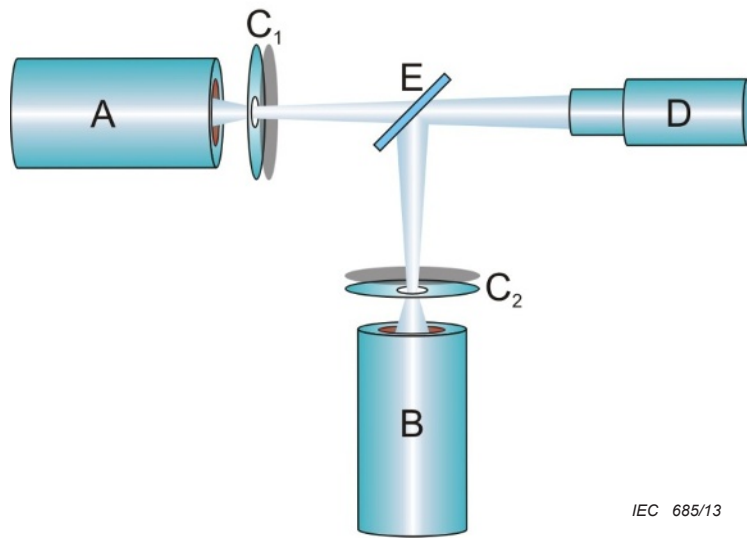

IEC 685/13

**Key**


- A Reference source 1
- C<sub>1</sub>, C<sub>2</sub> Shutter mechanisms
- B Reference source 2
- D Radiation thermometer
- E Beam splitter

**Figure 3 – Possible arrangement for determining the response time with two reference sources**

**5.17 Exposure time**

**5.17.1 General**

The exposure time is a relevant specification for radiation thermometers which have a significant delay time as part of their response time and observe objects passing through their field of view within a time span shorter than the response time (see Figure 4). In this case the exposure time is a relevant specification which shall be given by the manufacturer of the radiation thermometer.

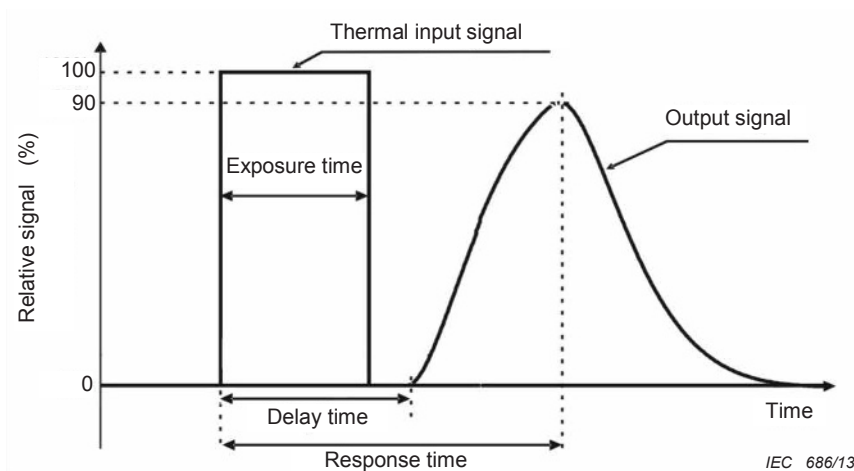

IEC 686/13

**Figure 4 – Demonstration of the exposure time**



The exposure time depends on the signal processing conditions within the radiation thermometer, the magnitude of the temperature step (starting value and plateau value) as well as the reached percentage of the temperature step of the output signal.

The following test method outlines the procedure to determine the time interval, a step change in the input radiation power, starting and ending at ambient temperature and, in between, reaching a temperature close to the top of the measuring temperature range of the thermometer, has to be present, such that the output signal of a radiation thermometer reaches 90 % of the full scale response to continuous radiation. The exposure time may be specified as a different percentage level of the full scale response to continuous radiation, e.g. 99 % (see IEC/TS 62492-1:2008, 4.1.1.17.3). In this case the test method has to be adjusted accordingly.

### **5.17.2 Test method**

**5.17.2.1** Sight the radiation thermometer at the centre of the radiating area of the reference source.

**5.17.2.2** The reference source is stabilised at a temperature close to the top of the measuring temperature range of the radiation thermometer.

**5.17.2.3** The sight path between the radiation thermometer and the reference source is interrupted by a shutter mechanism which can be opened and closed very quickly and whose open time can be adjusted with sufficient precision. The output of the radiation thermometer is allowed to stabilize at the radiation temperature of the closed shutter (ambient temperature).

**5.17.2.4** The shutter is opened and the final (maximum) output signal of the radiation thermometer for continuous radiation is measured (i.e. 100 % value).

**5.17.2.5** The data acquisition system is triggered and the shutter is opened and closed such that the signal over time from the radiation thermometer in response to the step change interval in input radiant power can be measured and recorded (e.g. a storage oscilloscope). Starting with a long pulse time of illumination (significantly longer than the expected exposure time) the pulse width (i.e. the time period of open shutter) is reduced step by step until the maximum signal is only 90 % of the output signal measured for continuous radiation in 5.17.2.4.

As a digitally processed radiation thermometer may have a variation in the measured value of exposure time the measurement has to be repeated a sufficient number of times (at least five times) until the maximum value of exposure time is uniquely determined. Care has to be taken that the exposure time test method is only performed when the radiation thermometer is in the temperature measurement mode of operation, as radiation thermometers may periodically perform e.g. a calibration routine.

**5.17.2.6** The exposure time (0 % / 90 %) is the longest measured time period the shutter has to stay open to reach 90 % of the maximum measured value (i.e. the value of continuous radiation) (see Figure 4).

The time period needed by the shutter mechanism to open and close shall be much shorter than the exposure time (not more than 10 % of the exposure time) and the shutter shall have a stable radiation temperature near ambient temperature (i.e. no heating up by the reference source).

Instead of a reference source with a shutter mechanism a radiation source with rapidly adjustable radiation intensity and appropriate wavelength may be used. This can be for example a light emitting diode (LED) which is operated with a pulse generator. The radiation source is switched to continuous output and the signal output of the radiation thermometer is monitored with a rapid signal recording device e.g. a storage oscilloscope. If applying a LED, the operating current shall be adjusted until the required temperature indication at the

radiation thermometer is achieved at the beginning of the test method. The pulse width is then reduced until the temperature display is only a specific proportion of the minimum/maximum signal, e.g. 0 %/90 % of the original display. The set pulse width is now the exposure time.

For the determination of exposure times starting at temperatures different from ambient temperature an analogous method based on a more sophisticated setup with two reference sources (see Figure 3) should be applied.

## **5.18 Warm-up time**

### **5.18.1 General**

This test method outlines the procedure to be used to evaluate the time interval, after switching the power of a radiation thermometer on, that is required for the output signal or temperature reading of the radiation thermometer to stabilize within the manufacturer's repeatability specification (5.14) (see Figure 5).

### **5.18.2 Test method**

**5.18.2.1** The radiation thermometer is turned off and allowed to stand and stabilize under ambient conditions within the operating temperature range and air humidity range as specified by the manufacturer. The time period shall be sufficiently long for the instrument to reach equilibrium with the environment.


**5.18.2.2** The reference source is stabilised at a temperature within the measuring temperature range of the radiation thermometer.

**5.18.2.3** The radiation thermometer is sighted on the reference source and switched on. The output signal is periodically recorded as the radiation thermometer warms to its operating temperature. The time span between two measurements has to be significantly shorter than the expected warm-up time. The minimum total test time shall be ten times the warm-up time specified by the manufacturer (see Figure 5).

**5.18.2.4** The value for the warm-up time is taken to be the elapsed time required for the output signal to equal its value recorded near the end of the test minus one-half of the manufacturer's repeatability band.

The repeatability of the reference source shall be significantly better than the repeatability of the radiation thermometer.

For some radiation thermometers, the warm-up time may depend on the temperature of the reference source. For such radiation thermometers the test method should be carried out at, at least, a reference source temperature close the top and a temperature close to the bottom of the measuring temperature range of the radiation thermometer.

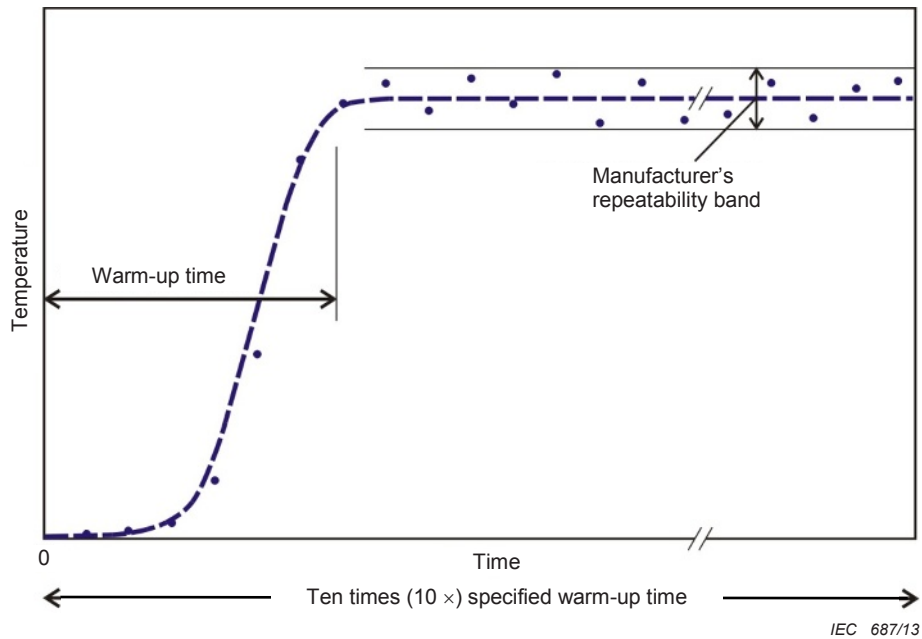

**Figure 5 – Example of warm-up time**

## 5.19 Operating temperature and air humidity range

### 5.19.1 General

For instruments with no internal temperature indication the ambient temperature shall be stated instead of the instrument temperature.

For the determination of the air humidity range well defined atmospheric conditions regarding the humidity and temperature of the atmosphere have to be realised. A test method for the air humidity range is beyond the scope of this technical specification.

Within the operating temperature range given by the manufacturer the radiation thermometer shall stay with all specifications fully functional over the full measuring temperature range. A critical test for the operating temperature range is the following test of the measurement uncertainty over the full measuring and operating temperature range.

### 5.19.2 Test method

**5.19.2.1** The radiation thermometer is operated in an adjustable temperature enclosure (e.g. climate chamber) which allows stable operation of the radiation thermometer within the complete operating temperature range given by the manufacturer. For instruments with no internal temperature indication the ambient temperature (i.e. the temperature of the climate chamber) shall be used as the instrument temperature.

**5.19.2.2** Sight the radiation thermometer at the centre of the radiating area of the reference source.

No window should be used between the radiation thermometer and the reference source. If a window is used, the influence of the window on the temperature indicated by the radiation thermometer has to be corrected for.

**5.19.2.3** The temperature of the reference source is stabilised near the bottom of the measuring temperature range of the radiation thermometer.

**5.19.2.4** The internal temperature of the radiation thermometer is stabilised at the minimum temperature of its operating temperature range.

**5.19.2.5** The temperature of the reference source and the temperature indicated by the radiation thermometer are recorded. The difference between these two values is calculated and recorded.

**5.19.2.6** The internal temperature of the radiation thermometer is stabilised at the maximum temperature of its operating temperature range.

**5.19.2.7** The temperature of the reference source and the temperature indicated by the radiation thermometer are recorded. The difference between these two values is calculated and recorded.

**5.19.2.8** The temperature of the reference source is stabilised near the top of the measuring temperature range of the radiation thermometer.

**5.19.2.9** The measuring sequence 5.19.2.4 to 5.19.2.7 is repeated.

**5.19.2.10** The value of the measurement uncertainty of the radiation thermometer at each internal temperature within the operating temperature range is taken to be the differences determined in 5.19.2.5 and 5.19.2.7 plus the temperature uncertainty of the reference source with respect to the current International Temperature Scale. These uncertainties have to stay within the manufacturer's specification. The temperature parameter determined in 5.10 needs to be considered when deciding whether or not the uncertainties determined are within the manufacturer's specifications.

Due to the small number of observations special care shall be taken not to infer too much significance from this test (i.e. no confidence level can be given).

Moisture condensation on the radiation thermometer (i.e. on the optics) shall be avoided throughout the test.

In order to use this method to test for compliance of the temperature parameter with the data provided by the manufacturer the temperature uncertainty of the reference source should be significantly smaller than the uncertainty of the radiation thermometer.

The minimum time required for the thermal stabilisation of the radiation thermometer has to elapse after each change of temperature of the climate chamber. This stabilisation time might be longer than the climate chamber stabilisation time.

## **5.20 Storage and transport temperature and air humidity range**

### **5.20.1 General**

The specified relative air humidity range is valid over the complete specified storage temperature range, if not stated otherwise.

Condensation is a major cause of damage to instruments in 'storage', often resulting when a cold instrument is brought into a warm and humid environment.

### **5.20.2 Test method**

The radiation thermometer shall stay with all specifications fully functional when it is stored switched off within the storage and transport temperature and air humidity range given by the manufacturer. A critical test is the test of the measurement uncertainty before and after the radiation thermometer has been stored in a climate chamber for at least for 24 h under temperature and humidity conditions which are at the top and the bottom of the storage

temperature and humidity range specified by the manufacturer. The measurement uncertainty is tested according to 5.2.2 over the full measuring temperature range.

## **6 Safety requirement**

Definition of terms and concept of safety are in accordance with IEC/ISO Guide 51.

The instrument`s tolerable risk should be achieved in accordance with IEC Guide 116.

Any harm that can occur from the instrument and the procedures specified in this technical specification should be clearly stated by the manufacturer.

**Annex A**  
 (informative)

**Change in indicated temperature of a radiation thermometer  
 corresponding to a change in the radiation exchange**

**Table A.1 – The change in indicated temperature corresponding to a 1 % change  
 in the radiation exchange with a radiation thermometer at 23 °C (Example)**

Wave length / $\mu\text{m}$	0,65	0,85	1,0	1,6	2,2	3,43	3,9	5,2	8,00	11,5
Measured temperature / $^{\circ}\text{C}$	Temperature change / $^{\circ}\text{C}$									
-100										
-50										1,2
0									0,3	0,3
50						0,2	0,2	0,2	0,2	0,2
100					0,2	0,3	0,3	0,4	0,6	0,6
150					0,3	0,4	0,5	0,6	0,8	1,0
200					0,3	0,5	0,6	0,8	1,1	1,3
250			0,3	0,4	0,4	0,7	0,7	1,0	1,4	1,7
300			0,4	0,5	0,5	0,8	0,9	1,2	1,7	2,1
350			0,4	0,6	0,6	0,9	1,1	1,4	2,0	2,4
400			0,5	0,7	0,7	1,1	1,2	1,6	2,3	2,8
450			0,4	0,6	0,8	1,2	1,4	1,8	2,6	3,2
500			0,4	0,7	0,9	1,4	1,6	2,1	2,9	3,6
550			0,5	0,8	1,0	1,6	1,8	2,4	3,3	4,0
600		0,5	0,5	0,9	1,2	1,8	2,0	2,6	3,6	4,4
650		0,5	0,6	1,0	1,3	2,0	2,3	2,9	4,0	4,8
700		0,6	0,7	1,1	1,5	2,2	2,5	3,2	4,4	5,3
750	0,5	0,6	0,7	1,2	1,6	2,5	2,8	3,5	4,8	5,7
800	0,5	0,7	0,8	1,3	1,8	2,7	3,0	3,8	5,2	6,1
850	0,6	0,7	0,9	1,4	1,9	2,9	3,3	4,2	5,6	6,6
900	0,6	0,8	1,0	1,5	2,1	3,2	3,6	4,5	6,0	7,0
950	0,7	0,9	1,0	1,7	2,3	3,5	3,9	4,8	6,4	7,5
1 000	0,7	1,0	1,1	1,8	2,5	3,7	4,2	5,2	6,8	7,9
1 100	0,9	1,1	1,3	2,1	2,9	4,3	4,8	5,9	7,6	8,8
1 200	1,0	1,3	1,5	2,4	3,3	4,9	5,4	6,6	8,5	9,7
1 300	1,1	1,5	1,7	2,8	3,7	5,5	6,1	7,4	9,3	10,7
1 400	1,3	1,7	2,0	3,1	4,2	6,1	6,8	8,2	10,2	11,6
1 500	1,4	1,9	2,2	3,5	4,7	6,8	7,5	9,0	11,1	12,5
1 600	1,6	2,1	2,4	3,9	5,2	7,5	8,2	9,8	12,0	13,5
1 700	1,8	2,3	2,7	4,3	5,8	8,2	8,9	10,6	12,9	14,4
1 800	1,9	2,5	3,0	4,7	6,3	8,9	9,7	11,5	13,8	15,4
1 900	2,1	2,8	3,3	5,2	6,9	9,6	10,5	12,3	14,7	16,3
2 000	2,3	3,1	3,6	5,7	7,5	10,4	11,3	13,2	15,7	17,3

The change in indicated temperature corresponding to a change in the radiant power received by the radiation thermometer is calculated as:

$$\Delta T = | T( (1 + B) (L_{(\lambda, T_S)} - L_{(\lambda, T_{Ref})}) + L_{(\lambda, T_{Ref})} ) - T_S |$$

where

$T_{(\lambda, L)}$  is the temperature according to the inverse function of Planck's law;

$L_{(\lambda, T)}$  is the spectral radiance according to Planck's law;

$\lambda$  is the wavelength;

$T_S$  is the temperature of the source;

$T_{Ref}$  is the temperature of the radiation thermometer (23 °C);

B is 0,01 (corresponding to 1 % change in the radiation exchange).

\_\_\_\_\_ For "Measured Temperature" lower than marked by the **Bold Line**, the temperature of the radiation thermometer (23 °C) has to be taken in account.

## Bibliography

ISO/IEC Guide 51:1999, *Safety aspects – Guidelines for their inclusion in standards*

ISO/IEC Guide 98-3:2008, *Uncertainty of measurement – Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*

ISO/IEC Guide 99:2007, *International vocabulary of metrology – Basic and general concepts and associated terms (VIM)*

IEC Guide 116:2010, *Guidelines for safety related risk assessment and risk reduction for low voltage equipment*

---







# British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

## About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

## Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at [bsigroup.com/standards](http://bsigroup.com/standards) or contacting our Customer Services team or Knowledge Centre.

## Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at [bsigroup.com/shop](http://bsigroup.com/shop), where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

## Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to [bsigroup.com/subscriptions](http://bsigroup.com/subscriptions).

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

**PLUS** is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit [bsigroup.com/shop](http://bsigroup.com/shop).

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email [bsmusales@bsigroup.com](mailto:bsmusales@bsigroup.com).

## BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

## Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

## Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

## Useful Contacts:

### Customer Services

**Tel:** +44 845 086 9001

**Email (orders):** [orders@bsigroup.com](mailto:orders@bsigroup.com)

**Email (enquiries):** [cservices@bsigroup.com](mailto:cservices@bsigroup.com)

### Subscriptions

**Tel:** +44 845 086 9001

**Email:** [subscriptions@bsigroup.com](mailto:subscriptions@bsigroup.com)

### Knowledge Centre

**Tel:** +44 20 8996 7004

**Email:** [knowledgecentre@bsigroup.com](mailto:knowledgecentre@bsigroup.com)

### Copyright & Licensing

**Tel:** +44 20 8996 7070

**Email:** [copyright@bsigroup.com](mailto:copyright@bsigroup.com)



...making excellence a habit.™