



BSI Standards Publication

Dentistry — Screw loosening test using cyclic torsional loading for implant body/ implant abutment connection of endosseous dental implants

National foreword

This Published Document is the UK implementation of ISO/TS 18130:2016.

The UK participation in its preparation was entrusted to Technical Committee CH/106/8, Dental implants.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2016. Published by BSI Standards Limited 2016

ISBN 978 0 580 82458 6

ICS 11.060.15

Compliance with a British Standard cannot confer immunity from legal obligations.

This Published Document was published under the authority of the Standards Policy and Strategy Committee on 31 May 2016.

Amendments issued since publication

Date	Text affected
------	---------------

**Dentistry — Screw loosening test
using cyclic torsional loading for
implant body/implant abutment
connection of endosseous dental
implants**

Medecine bucco-dentaire — Essai de dévissage d'une vis utilisant une charge de torsion cyclique pour le corps d'implant/pilier implantaire des implants dentaires endo-osseux



COPYRIGHT PROTECTED DOCUMENT

© ISO 2016, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 General principle	2
5 Test methods	2
5.1 Test condition.....	2
5.2 Torque meter.....	2
5.3 Preparation of test specimens.....	2
5.4 Initial screw removal torque.....	3
5.4.1 Procedure.....	3
5.5 Screw removal torque after cyclic torque test.....	3
5.5.1 Cyclic torque tester.....	3
5.5.2 Torque transducer.....	4
5.5.3 Procedure.....	4
5.6 Evaluation.....	5
6 Test report	5
Bibliography	6

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

The committee responsible for this document is ISO/TC 106, *Dentistry*, Subcommittee SC 8, *Dental implants*.

Introduction

Most endosseous dental implants currently marketed employ a dental implant body that is inserted within the jaw bone and to which other components may be joined when constructing a prosthetic superstructure. The connection between these components and the implant body should be sufficiently rigid to resist vertical masticatory loads, which have a significant torsional component. Endosseous dental implants may, therefore, incorporate features to restrict rotation at the connection. If this is insufficiently strong, then undesirable incidents, including screw loosening, distortion and fracture of the linked components will occur. A cyclic torsional screw loosening test for the connection between implant body and implant abutment would facilitate comparative evaluation.

Dentistry — Screw loosening test using cyclic torsional loading for implant body/implant abutment connection of endosseous dental implants

1 Scope

This Technical Report provides guidelines for a method to determine the extent of screw loosening of the metallic implant body/implant abutment joint of endosseous dental implants, such as two-part implants or multi-part implants under cyclic torsional loading. This test is most appropriate for evaluating new types of joints fixed using screw(s) and metallic connecting parts. This Technical Report provides a protocol for torsional cyclic torque on an implant body/implant abutment joint, but its intended use is for prefabricated implant bodies, implant abutments and, if appropriate, implant connecting parts that are made of metallic materials.

It is not applicable to ensure the *in vivo* performance of endosseous dental implants and is not derived from observations of clinical failures.

NOTE This Technical Report is not intended for use with temporary abutments.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1942, *Dentistry – Vocabulary*

ISO 16443, *Dentistry – Vocabulary for dental implants systems and related procedure*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1942 and ISO 16443 and the following apply.

3.1 cyclic torque

repeated torsional force alternatively clockwise and counter clockwise

3.2 screw loosening

decrease in screw removal torque relative to the removal torque when the abutment screw was first installed

3.3 screw tightening torque

torque value for screw required to tighten the implant abutment, and the implant connecting part if appropriate, to the implant body as per specified by the manufacturer

3.4 screw removal torque

torque value for screw required to deconstruct the connection between the implant body and the implant abutment, and the implant connecting part if appropriate

3.5 temporary abutment

implant abutment for temporary usage

4 General principle

The endurance properties of implant body/implant abutment interface should be tested by applying a cyclic alternating torsional load to the implant body and implant abutment clamped in the testing device.

Testing should be performed on finished devices or specimens that have an implant abutment joint equivalent to the finished device (i.e. components that have undergone the same manufacturing process as the device that is to be marketed). If the manufacturer intends the implant components to be sterilized by the clinician prior to surgery, sterilization should be carried out before testing as specified in the manufacturer's instructions for use. However, if there is evidence that the specified sterilization method has no significant effect on the properties of all the materials of the specimens being tested, sterilization is not necessary prior to testing. If so, this should be documented in the test report.

If a dental implant system to be tested consists of several types of implant abutments with the same connecting interface, a straight implant abutment having a metallic connecting interface should be selected for testing.

NOTE Angulated implant abutments cannot be tested because the central axis of connected test specimens is not straight.

5 Test methods

5.1 Test condition

Carry out the test at (25 ± 10) °C.

5.2 Torque meter

Use a torque meter with an accuracy of 0,3 N·cm or less.


NOTE An example of a torque meter is HDP-5¹⁾ manufactured by HIOS INC, Japan.

5.3 Preparation of test specimens

The implant abutment, and implant connecting part if appropriate, should be fixed on the implant body using the specified/recommended screw at screw tightening torques stated by the manufacturer's instructions for use. The screw tightening torque should be applied using a torque meter. The ends of the test specimens may be modified into shapes larger than the maximum diameter of implant body and/or implant abutment to more easily clamp with the holders. An example of a test specimen is illustrated in [Figure 1](#).

NOTE At least six specimens for each test according to [5.4](#) and [5.5](#) are required to compare the mean of the screw removal torques after cyclic torque test with the mean of the initial screw removal torques.

1) HDP-5 is an example of a suitable product available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of this product.

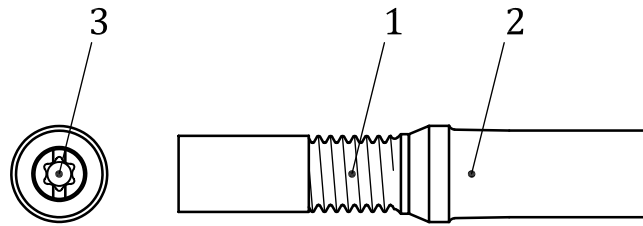

Key

- 1 implant body
- 2 implant abutment
- 3 abutment screw

Figure 1 — Schematic of a test specimen

5.4 Initial screw removal torque

5.4.1 Procedure

The initial screw removal torque of six specimens should be measured according to the following procedure.

- a) The implant abutment, and implant connecting part, if appropriate, should be fixed on the implant body using the specified screw at screw tightening torques stated in the manufacturer's instructions for use. These implant components should be new ones that have never previously been assembled.
- b) After 5 min, measure the screw removal torque by torque meter.
- c) Calculate the mean and standard deviation of initial screw removal torque from the obtained values for the at least six specimens.

5.5 Screw removal torque after cyclic torque test


5.5.1 Cyclic torque tester

The test device should have the following parts:

- specimen holders (the implant body and implant abutment should each be held at a maximum of 5 mm from the joint line between them);
- torque transducer;
- torsional cyclic driving device that can apply cyclic torque greater than 10 % of screw tightening torque;
- torsional cyclic displacement transducer.

An example of a torsional testing device is illustrated in [Figure 2](#).

The central long axes of the shafts of the torque transducer and torsional driving device should coincide.

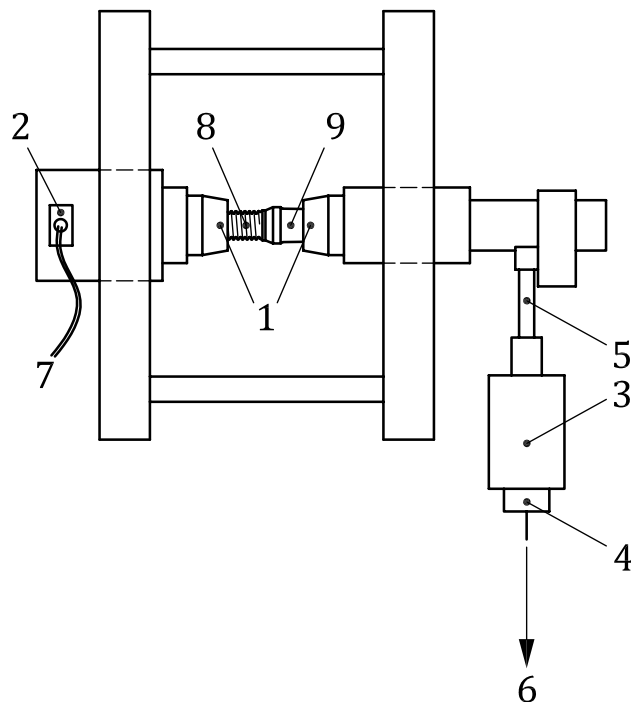

Key

- 1 specimen holder
- 2 torque transducer
- 3 torsional cyclic driving device
- 4 torsional cyclic displacement transducer
- 5 lever arm
- 6 output of torsional displacement to recorder
- 7 output of torsional torque to recorder
- 8 implant body
- 9 implant abutment

Figure 2 — Example of testing device for cyclic torque test

5.5.2 Torque transducer

The accuracy of the torque transducer equipped in the cyclic torque tester (see 5.5.1) should be less than $\pm 1\%$ of the maximum torque to be tested.

5.5.3 Procedure

- a) The implant abutment, and implant connecting part, if appropriate, should be fixed on the implant body using the specified screw at screw tightening torques as stated in the manufacturer's instructions for use. These implant components should be new ones that have never previously been assembled.
- b) After 5 min, clamp the retaining portions of the implant body and implant abutment of a test specimen into the specimen holders of the testing device. The implant body and implant abutment should each be held at a maximum of 5 mm from the joint line between them.
- c) Apply cyclic torque (clockwise and counter clockwise) up to 10 % of the screw tightening torque stated in the manufacture's instruction to the implant abutment with the velocity of 10 degree per minute. Repeat this cyclic torque up to 100 000 cycles.

- d) When the specimen survives without deformation and/or fracture after 100 000 cycles, measure the screw removal torque by torque meter. When the specimen does not survive, record the number of cycles which it survives.
- e) After the test, observe the wear and deformation of the implant body/connecting joint by a microscope.
- f) At least six specimens should be tested.
- g) Calculate the mean and standard deviation of the measured screw removal torque after cyclic torque test of at least six specimens

NOTE 1 Implant body and implant abutment joint part are sealed by screw tightening and the part may not be affected by corrosion during 100 000 times cyclic torque test (e.g. 1 d or 2 d).

NOTE 2 An example of the testing machine is AG-XR²⁾ manufactured by Shimadzu Corporation, Japan.

5.6 Evaluation

Calculate the ratio of the mean initial screw removal torque to the screw tightening torque. Calculate the ratio of the mean screw removal torque after cyclic torque test to the mean initial screw removal torque.

6 Test report

The test report should include at least the following information:

- a) a reference to this Technical Report, i.e. ISO/TR 18130;
- b) the identification of the employed test specimens, including the type of connection (internal anti-rotation: taper-fit, notch-fit, hexagonal, etc.; external anti-rotation: hexagonal, etc.), manufacturer(s), part numbers and lot numbers of the tested parts, material(s) of the tested parts, diameter and length of the implant body and implant abutment;
- c) if applicable, the documented evidence that the specified sterilization method has no significant effect on the properties of all materials;
- d) the test method including the test condition, testing device, screw tightening torque applied to the screws, cyclic torque, number of cycles, distance from the interface at which the components were held and a drawing of the employed test specimens;
- e) the results obtained, namely
 - 1) the initial screw removal torque and the ratio to the screw tightening torque,
 - 2) the screw removal torque if the specimen survived 100 000 cycles and the ratio to the initial screw removal torque,
 - 3) if the specimen does not survive, the number of cycles which the testing specimen survives,
 - 4) the microscopic observation on deformed and/or fractured parts of test specimens.

2) AG-XR is an example of a suitable product available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of this product.

Bibliography

- [1] ISO 898-7, *Mechanical properties of fasteners — Part 7: Torsional test and minimum torques for bolts and screws with nominal diameters 1 mm to 10 mm*
- [2] ISO/TS 13498, *Dentistry — Torsion test of implant body/connecting part joints of endosseous dental implant systems*
- [3] ASTM F543-07, *Standard specification and test methods for metallic medical bone screws*
- [4] ANDERSSON B., ODMAN P., CARLSSON L., BRÅNEMARK P.I. A new Brånemark single tooth abutment: handling and early clinical experiences. *Int. J. Oral Maxillofac. Implants.* 1992, **7** (1) pp. 105–111
- [5] BALFOUR A., & O'BRIEN G.R. Comparative study of antirotational single tooth abutment. *J. Prosthet. Dent.* 1995, **73** (1) pp. 36–43
- [6] CARDOSO M., TORRES M.F., LOURENÇO E.J., DE MORAES TELLES D., RODRIGUES R.C., RIBEIRO R.F. Torque removal evaluation of prosthetic screws after tightening and loosening cycles: an in vitro study. *Clin. Oral Implants Res.* 2012, **23** pp. 475–480
- [7] GUZAITIS K.L., KNOERNSCHILD K.L., VIANA M.A. Effect of repeated screw joint closing and opening cycles on implant prosthetic screw reverse torque and implant and screw thread morphology. *J. Prosthet. Dent.* 2011, **106** (3) pp. 159–169
- [8] KHRAISAT A., HASHIMOTO A., NOMURA S., MIYAKAWA O. Effect of lateral cyclic loading on abutment screw loosening of an external hexagon implant system. *J. Prosthet. Dent.* 2004, **91** (4) pp. 326–334
- [9] KIM S.K., KOAK J.Y., HEO S.J., TAYLOR T.D., RYOO S., LEE S.Y. Screw loosening with interchangeable abutments in internally connected implants after cyclic loading. *Int. J. Oral Maxillofac. Implants.* 2012, **27** (1) pp. 42–47
- [10] YAO K.T., KAO H.C., CHENG C.K., FANG H.W., YIP S.W., HSU M.L. The effect of clockwise and counterclockwise twisting moments on abutment screw loosening. *Clin. Oral Implants Res.* 2012, **23** (10) pp. 1181–1186
- [11] PIERMATTI J., YOUSEF H., LUKE A., MAHEVICH R., WEINER S. An in vitro analysis of implant screw torque loss with external hex and internal connection implant systems. *Implant Dent.* 2006, **15** (4) pp. 427–435
- [12] WATANABE F. Torsion test at the interface between implant and abutment. Conference Program of 13th Biennial Meeting of International College of Prosthodontists. Cape Town, South Africa. 10–13 Sep. 2009, pp. 172–173
- [13] JORGE J.R., BARAO V.A., DELBEN J.A., ASSUNCAO W.G. The role of implant/abutment on torque maintenance of retention screws and vertical misfit of implant-supported crowns before and after cycling. *Int. J. Oral Maxillofac. Implants.* 2013, **28** (2) pp. 415–422
- [14] RANGERT B., JEMT T., JÖRNEUS L. Forces and moments on Brånemark implants. *Int. J. Oral Maxillofac. Implants.* 1989, **4** (3) pp. 241–247
- [15] YOKOYAMA D., SHINYA A., LASSILA L.V., GOMI H., NAKASONE Y., VALLITTU P.K., SHINYA A. Framework design of an anterior fiber-reinforced hybrid composite fixed partial denture: a 3D finite element study. *Int. J. Prosthodont.* 2009, **22** (4) pp. 405–412
- [16] JEMT T., & PETERSSON P. A 3-year follow-up study on single implant treatment. *J. Dent.* 1993, **21** (4) pp. 203–208

- [17] GOODACRE C.J., KAN J.Y., RUNGCHARASSAENG K. Clinical complications of osseointegrated implants. *J. Prosthet. Dent.* 1999, **81** (5) pp. 537–552
- [18] THEOHARIDOU A., PETRIDIS H.P., TZANNAS K., GAREFIS P. Abutment screw loosening in single-implant restoration: a systematic review. *Int. J. Oral Maxillofac. Implants.* 2008, **23** (4) pp. 681–690
- [19] KATSUTA Y., & WATANABE F. Abutment screw loosening of endosseous dental implant body/abutment joint by cyclic loading test at the initial stage. *Dent. Mater. J.* 2015, **34** (6) pp. 896–902

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Copyright in BSI publications

All the content in BSI publications, including British Standards, is the property of and copyrighted by BSI or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use.

Save for the provisions below, you may not transfer, share or disseminate any portion of the standard to any other person. You may not adapt, distribute, commercially exploit, or publicly display the standard or any portion thereof in any manner whatsoever without BSI's prior written consent.

Storing and using standards

Standards purchased in soft copy format:

- A British Standard purchased in soft copy format is licensed to a sole named user for personal or internal company use only.
- The standard may be stored on more than 1 device provided that it is accessible by the sole named user only and that only 1 copy is accessed at any one time.
- A single paper copy may be printed for personal or internal company use only.

Standards purchased in hard copy format:

- A British Standard purchased in hard copy format is for personal or internal company use only.
- It may not be further reproduced – in any format – to create an additional copy. This includes scanning of the document.

If you need more than 1 copy of the document, or if you wish to share the document on an internal network, you can save money by choosing a subscription product (see 'Subscriptions').

Reproducing extracts

For permission to reproduce content from BSI publications contact the BSI Copyright & Licensing team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email subscriptions@bsigroup.com.

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Useful Contacts

Customer Services

Tel: +44 345 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 345 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK