

---

---

**Dentistry — Polymer-based restorative  
materials**

*Art dentaire — Produits de restauration à base de polymères*



Reference number  
ISO 4049:2009(E)

© ISO 2009

**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2009

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

Foreword .....	iv
Introduction.....	v
<b>1 Scope .....</b>	<b>1</b>
<b>2 Normative references .....</b>	<b>1</b>
<b>3 Terms and definitions .....</b>	<b>1</b>
<b>4 Classification .....</b>	<b>2</b>
<b>5 Requirements.....</b>	<b>2</b>
<b>5.1 Biocompatibility.....</b>	<b>2</b>
<b>5.2 Physical and chemical properties .....</b>	<b>2</b>
<b>5.3 Shade, restorative materials .....</b>	<b>4</b>
<b>5.4 Colour stability after irradiation and water sorption .....</b>	<b>4</b>
<b>5.5 Radio-opacity.....</b>	<b>4</b>
<b>6 Sampling .....</b>	<b>5</b>
<b>7 Test methods .....</b>	<b>5</b>
<b>7.1 General reagent — Water .....</b>	<b>5</b>
<b>7.2 Test conditions .....</b>	<b>6</b>
<b>7.3 Inspection.....</b>	<b>6</b>
<b>7.4 Preparation of test specimens .....</b>	<b>6</b>
<b>7.5 Measurement of film thickness of luting materials.....</b>	<b>6</b>
<b>7.6 Working time, Class 1 and Class 3 restorative materials, excluding luting materials .....</b>	<b>9</b>
<b>7.7 Working time, Class 1 and Class 3 luting materials .....</b>	<b>11</b>
<b>7.8 Setting time, Class 1 and Class 3 materials .....</b>	<b>11</b>
<b>7.9 Sensitivity to ambient light, Class 2 materials .....</b>	<b>13</b>
<b>7.10 Depth of cure, Class 2 materials.....</b>	<b>14</b>
<b>7.11 Flexural strength .....</b>	<b>15</b>
<b>7.12 Water sorption and solubility.....</b>	<b>18</b>
<b>7.13 Shade and colour stability after irradiation and water sorption.....</b>	<b>21</b>
<b>7.14 Radio-opacity.....</b>	<b>22</b>
<b>8 Packaging, marking and instructions and information to be supplied by the manufacturer.....</b>	<b>25</b>
<b>8.1 Packaging.....</b>	<b>25</b>
<b>8.2 Marking.....</b>	<b>25</b>
<b>8.3 Manufacturer's instructions and information for the user.....</b>	<b>27</b>
<b>Bibliography.....</b>	<b>28</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 4049 was prepared by Technical Committee ISO/TC 106, *Dentistry*, Subcommittee SC 1, *Filling and restorative materials*.

This fourth edition cancels and replaces the third edition (ISO 4049:2000) which has been reviewed and essentially reconfirmed. Several minor changes have been made to clarify content. Changes have been made to the test method for radio-opacity (see 7.14) in order to simplify this test.

## Introduction

Specific qualitative and quantitative requirements for freedom from biological hazard are not included in this International Standard, but it is recommended that when assessing possible biological or toxicological hazards, reference should be made to ISO 10993-1 and ISO 7405.



# Dentistry — Polymer-based restorative materials

## 1 Scope

This International Standard specifies requirements for dental polymer-based restorative materials supplied in a form suitable for mechanical mixing, hand-mixing, or intra-oral and extra-oral external energy activation, and intended for use primarily for the direct or indirect restoration of cavities in the teeth and for luting.

The polymer-based luting materials covered by this International Standard are intended for use in the cementation or fixation of restorations and appliances such as inlays, onlays, veneers, crowns and bridges. This International Standard does not cover those polymer-based luting materials that have an adhesive component within the structure of the material.

This International Standard does not cover materials intended to prevent caries (see ISO 6874) or those used for veneering metal sub-frames (see ISO 10477).

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1942, *Dentistry — Vocabulary*

ISO 3665, *Photography — Intra-oral dental radiographic film — Specification*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 7491, *Dental materials — Determination of colour stability*

ISO 8601, *Data elements and interchange formats — Information interchange — Representation of dates and times*

## 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1942 and the following apply.

### 3.1

#### **opaque luting material**

intensely pigmented polymer-based luting material intended to mask underlying materials and tooth structure

### 3.2

#### **opaque**

shade of an intensely pigmented polymer-based restorative material

## 4 Classification

For the purposes of this International Standard, dental polymer-based restorative materials are classified as the following types.

- a) **Type 1:** polymer-based restorative materials claimed by the manufacturer as suitable for restorations involving occlusal surfaces;
- b) **Type 2:** all other polymer-based restorative materials, and luting materials.

The three classes of dental polymer-based restorative materials are as follows.

- **Class 1:** materials whose setting is effected by mixing an initiator and activator (“self-curing” materials).
- **Class 2:** materials whose setting is effected by the application of energy from an external source, such as blue light or heat [“external-energy-activated” materials, see also 8.3 e)]. They are subdivided as follows:
  - 1) **Group 1:** materials whose use requires the energy to be applied intra-orally;
  - 2) **Group 2:** materials whose use requires the energy to be applied extra-orally. When fabricated, these materials will be luted into place.

Certain materials may be claimed by manufacturers to be both Group 1 and Group 2. In this event, the material should fulfil the requirements for both groups.

NOTE Class 2 luting materials will fall into Group 1 only.

- **Class 3:** materials that are cured by the application of external energy and also have a self-curing mechanism present (“dual cure” materials).

## 5 Requirements

### 5.1 Biocompatibility

See the Introduction for guidance on biocompatibility. Further information is available in ISO 7405 and ISO 10993-1.

### 5.2 Physical and chemical properties

#### 5.2.1 General

If a restorative material is supplied by the manufacturer in various shades, each shade, including opaque shades, shall be capable of satisfying all the requirements for sensitivity to ambient light (5.2.7), depth of cure (5.2.8), shade (5.3) and colour stability (5.4) appropriate to the material type and class. If the material is supplied such that it can be “tinted” or “blended” to the user’s prescription, the material shall comply with the requirements both when used alone and when used with the maximum recommended proportion of tint or blender [see 8.3 d)].

Similarly, if the manufacturer supplies a luting material in various shades, each shade, including opaque luting materials, shall be capable of satisfying all the requirements for depth of cure (5.2.8). Colour stability (5.4) of luting materials shall not be tested unless the manufacturer claims such a property.

In respect of the other requirements of 5.2 and those of 5.5, only one representative shade of restorative material shall be tested. This representative shade shall be either that classified by the manufacturer as



“universal” or, in the event that no shade is so classified, that shade corresponding to “A3” in the Vita® 1) classification of shade. However, if the manufacturer claims a higher value for radio-opacity [see 5.5 and 8.3 o)] for any other shade, this claim shall be tested.

The requirements are summarised in Tables 1, 2 and 3.

#### **5.2.2 Film thickness, luting materials**

The film thickness of luting materials when determined in accordance with 7.5 shall be no more than 10 µm above any value claimed by the manufacturer and in any event shall be no greater than 50 µm.

#### **5.2.3 Working time, Class 1 and Class 3 restorative materials, excluding luting materials**

The working time for Class 1 and Class 3 restorative materials, excluding luting materials, determined in accordance with 7.6, shall be not less than 90 s.

#### **5.2.4 Working time, Class 1 and Class 3 luting materials**

When tested in accordance with 7.7, the material shall be capable of forming a thin layer; during its formation there shall be no detectable change in its homogeneity.

#### **5.2.5 Setting time, Class 1 materials**

The setting time for Class 1 restorative materials, excluding luting materials, determined in accordance with 7.8, shall be not more than 5 min. The setting time for Class 1 luting materials, determined in accordance with 7.8, shall be not more than 10 min.

#### **5.2.6 Setting time, Class 3 materials**

The setting time for Class 3 materials, determined in accordance with 7.8, shall be not more than 10 min.

#### **5.2.7 Sensitivity to ambient light, Class 2 materials**

When tested in accordance with 7.9, the material shall remain physically homogeneous.

#### **5.2.8 Depth of cure, Class 2 materials**

When determined in accordance with 7.10, the depth of cure of Class 2 restorative materials, excluding luting materials, shall be not less than 1 mm if they are labelled by the manufacturer as opaque, or not less than 1,5 mm for other restorative materials.

The depth of cure of luting materials when determined in accordance with 7.10 shall be not less than 0,5 mm if they are labelled by the manufacturer as opaque materials, or not less than 1,5 mm for other materials.

In any event, the values for all materials, with the exception of opaque luting materials, shall be no more than 0,5 mm below the value stated by the manufacturer.

#### **5.2.9 Flexural strength**

The flexural strength of polymer-based restorative materials determined in accordance with 7.11 shall be equal to or greater than the limits specified in Table 1.

---

1) Vita® is a trade name of Vita Zahnfabrik, H Rauter GmbH & Co K G, Postfach 1338, D-79704 Bad Sackingen, Germany. This information is given for the convenience of the users of this International Standard and does not constitute an endorsement of this system by ISO.

**Table 1 — Flexural strength**

Restorative Materials		Flexural strength MPa minimum
Type 1	Class 1	80
	Class 2, Group 1	80
	Class 2, Group 2	100
	Class 3	80
Type 2 (including luting materials)	Class 1	50
	Class 2, Group 1	50
	Class 3	50

**5.2.10 Water sorption and solubility**

When determined in accordance with 7.12:

- a) the water sorption of all materials shall be  $\leq 40 \mu\text{g}/\text{mm}^3$ .
- b) the solubility of all materials shall be  $\leq 7,5 \mu\text{g}/\text{mm}^3$ .

**5.3 Shade, restorative materials**

When the material is assessed in accordance with 7.13 and ISO 7491, the shade of the set material shall match closely that of the manufacturer’s shade guide. If a shade guide is not supplied by the manufacturer, then the manufacturer shall nominate a commercially available shade guide that shall be used in assessing compliance with this requirement [see 8.3 l)]. In addition, the set material shall be evenly pigmented when viewed without magnification.

**5.4 Colour stability after irradiation and water sorption**

When the material is tested in accordance with 7.13 and ISO 7491, no more than a slight change in colour shall be observed. In respect of luting materials, colour stability shall be tested only in the event of a manufacturer’s claim for colour stability. In the event of such a claim, no more than a slight change in colour shall be observed after the material has been tested in accordance with 7.13 and ISO 7491.

**5.5 Radio-opacity**

**5.5.1** If the manufacturer claims that the material is radio-opaque [see 8.2.3 h)], the radio-opacity, determined in accordance with 7.14, shall be equal to or greater than that of the same thickness of aluminium and no less than 0,5 mm below any value claimed by the manufacturer.

**5.5.2** This test shall be performed on a “universal” shade (see 5.2.1), but if the manufacturer claims a value for one or more other shades that is at least twice the “universal” shade value, this other shade or shades shall be tested as described in 5.5.1 [see 8.3 o)].

**NOTE** Aluminium has a radio-opacity equivalent to that of dentine, thus 1 mm of material having a radio-opacity equivalent to 1 mm of aluminium has a radio-opacity equivalent to that of dentine.

**Table 2 — Physical and chemical property requirements for restorative materials, excluding luting materials** (see Table 1 for minimum flexural strength)

Material Class	Requirement (subclause)				
	Working time (5.2.3)	Setting time (5.2.5, 5.2.6)	Depth of Cure <sup>a</sup> (5.2.8)	Water sorption (5.2.10)	Solubility (5.2.10)
	s minimum	min maximum	mm minimum	$\mu\text{g}/\text{mm}^3$ maximum	$\mu\text{g}/\text{mm}^3$ maximum
Class 1	90	5 (5.2.5)	—	40	7,5
Class 2	—	—	1,0 (opaque shade) 1,5 (others)	40	7,5
Class 3	90	10 (5.2.6)	—	40	7,5

<sup>a</sup> The values for all materials shall be no more than 0,5 mm below the value stated by the manufacturer.

**Table 3 — Physical and chemical property requirements for luting materials**

Material Class	Requirement (subclause)					
	Film thickness <sup>a</sup> (5.2.2)	Working time (5.2.4)	Setting time (5.2.5, 5.2.6)	Depth of cure <sup>b</sup> (5.2.8)	Water sorption (5.2.10)	Solubility (5.2.10)
	$\mu\text{m}$ maximum	s minimum	min maximum	mm minimum	$\mu\text{g}/\text{mm}^3$ maximum	$\mu\text{g}/\text{mm}^3$ maximum
Class 1	50	60	10 (5.2.5)	—	40	7,5
Class 2	50	—	—	0,5 (opaquer) 1,5 (others)	40	7,5
Class 3	50	60	10 (5.2.6)	—	40	7,5

<sup>a</sup> The determined value shall be no more than 10  $\mu\text{m}$  above any value claimed by the manufacturer.

<sup>b</sup> In any event, the values for all materials, with the exception of opaque luting materials, shall be no more than 0,5 mm below the value stated by the manufacturer.

## 6 Sampling

The test sample shall consist of packages prepared for retail sale from the same batch containing enough material to carry out the specified tests, plus an allowance for repeat tests, if necessary.

NOTE 50 g should be sufficient.

## 7 Test methods

### 7.1 General reagent — Water

For the tests, use water prepared in accordance with ISO 3696 Grade 2.

## 7.2 Test conditions

Unless specified otherwise by the manufacturer, prepare and test all specimens at  $(23 \pm 1) ^\circ\text{C}$ . Control the relative humidity to ensure that it remains greater than 30 % and less than 70 % at all times. If the material was refrigerated for storage, allow it to attain  $(23 \pm 1) ^\circ\text{C}$ .

For Class 3 materials, the tests for working time (see 7.6) and setting time (see 7.8) shall be performed in the absence of activating radiation.

NOTE Ambient light, both natural and artificial, is capable of activating these materials. For good control, the test should be performed in a dark room with any artificial light filtered by a yellow filter. <sup>2)</sup>

## 7.3 Inspection

Inspect visually to check that requirements specified in Clause 8 have been met.

## 7.4 Preparation of test specimens

For the preparation of Class 2 and Class 3 materials, reference shall be made to the manufacturer's instructions [see 8.3 e)] that state the external energy source or sources recommended for the materials to be tested. Care shall be taken to ensure that the source is in a satisfactory operating condition. [ISO 10650 (both parts) gives guidance on this.]

Mix or otherwise prepare the material in accordance with the manufacturer's instructions and the test conditions specified in 7.2.

Where fully cured specimens are required for testing (7.11 to 7.14), it is important to ensure that the specimens are homogeneous after removal from the mould. There shall be no clefts, voids, discontinuities or air inclusions present when viewed without magnification.

Some polymer-based materials, particularly certain luting materials, have a chemical affinity for base metals. This property creates difficulty when removing specimens from metal moulds. Reference shall be made to the information supplied by the manufacturer [see 8.3 m)] regarding this property and, if it is claimed, moulds for the preparation of specimens of such materials may be made from non-metallic material such as high-density polyethylene.

## 7.5 Measurement of film thickness of luting materials

### 7.5.1 Apparatus

**7.5.1.1 Two glass plates**, optically flat, square or circular, each having a contact surface area of  $(200 \pm 25) \text{ mm}^2$ . Each plate shall be of a uniform thickness not less than 5 mm.

**7.5.1.2 Loading device**, of the type illustrated in Figure 1, or an equivalent means, whereby a force of  $(150 \pm 2) \text{ N}$  may be applied vertically to the specimen via the upper glass plate. In Figure 1, the anvil that is attached to the bottom of the rod shall be horizontal and parallel to the base. The load shall be applied smoothly and in such a manner that no rotation occurs.


NOTE A holder can be used to assist in the positioning of the plates. Such a device consists of a baseplate with three vertical pins to align circular plates or four pins to align square plates. (See Figure 2.)

**7.5.1.3 External energy source** (for Class 2 and Class 3 materials), as recommended by the manufacturer for use with the test material.

---

2) Polyester filter 101, Lee Filters, Andover, Hants, UK is an example of a suitable product available commercially. This information is given for the convenience of the users of this International Standard and does not constitute an endorsement of this product by ISO.

**7.5.1.4 Micrometer** or equivalent measuring instrument, accurate to 0,001 mm.

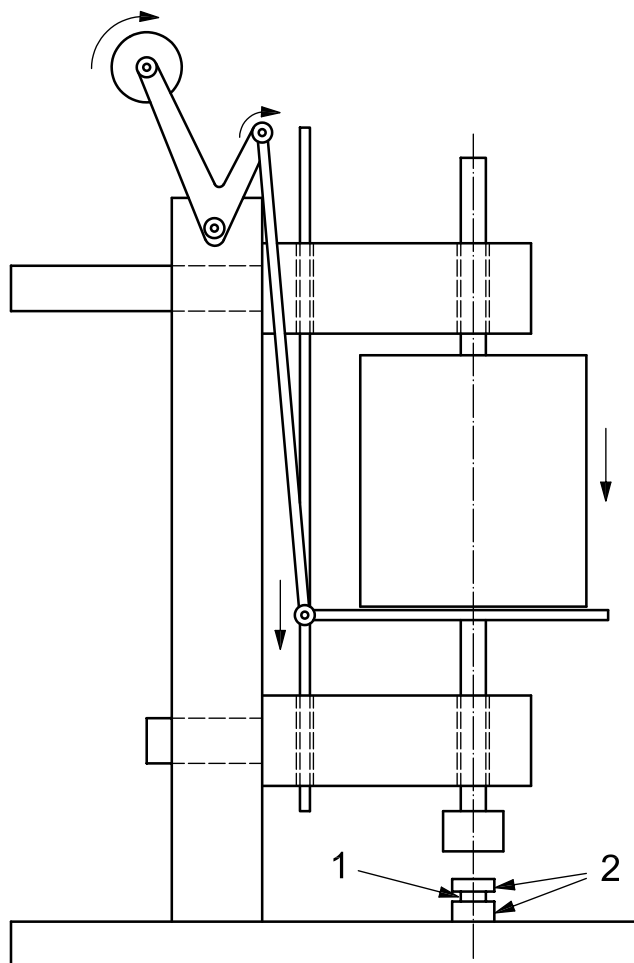

**Key**

- 1 specimen
- 2 glass plates (7.5.1.1)

**Figure 1 — Loading device for use in the film thickness test**

**7.5.2 Test procedure**

**7.5.2.1 Preliminary steps**


Measure, to an accuracy of 0,001 mm, the combined thickness of the two optically flat glass plates (7.5.1.1) stacked in contact with the micrometer (7.5.1.4) (reading A). Remove the upper plate and place between 0,02 ml and 0,10 ml of the test material treated in accordance with the manufacturer's instructions in the centre of the lower plate and centre it below the loading device (7.5.1.2) on its lower platen. Centre the second glass plate on the test specimen in the same orientation as in the original measurement. The holder (Figure 2) is helpful.

**7.5.2.2 Class 1 materials**

At  $(60 \pm 2)$  s after mixing Class 1 materials, carefully apply a force of  $(150 \pm 2)$  N vertically and centrally to the specimen via the top plate for  $(180 \pm 10)$  s. Ensure that the cement has completely filled the space between the glass plates. At least 10 min after the commencement of mixing, remove the plates from the loading device and measure the combined thickness of the two glass plates and the specimen film, again taking the reading in the centre of the plates (reading B).

Record the difference between reading A and reading B, to the nearest micrometre, as the film thickness of the luting material.

Carry out five determinations.

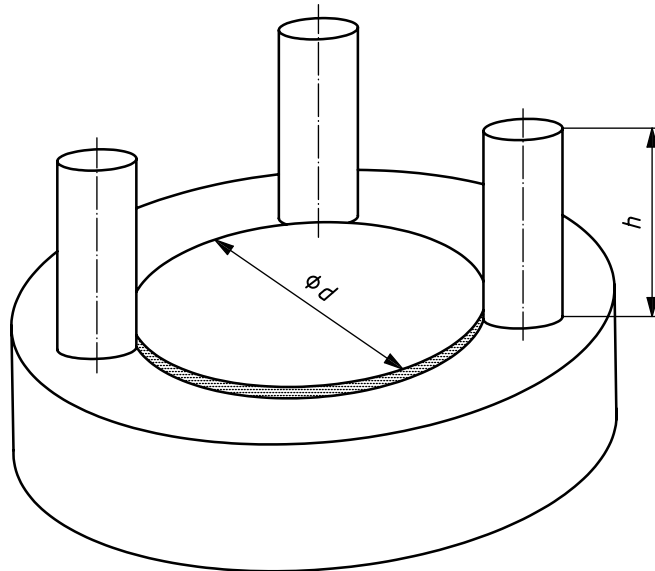

NOTE 1 The diameter,  $d$ , slightly exceeds the diameter of the glass plates.

NOTE 2 The height,  $h$ , of the pins is  $1,5 \times$  the height of one of the glass plates.

**Figure 2 — Holder to assist stabilisation of the glass plates (7.5)**

### 7.5.2.3 Class 2 and Class 3 materials

Immediately after dispensing Class 2 materials or after mixing Class 3 materials, carefully apply a force of  $(150 \pm 2)$  N vertically and centrally to the specimen via the top plate for  $(180 \pm 10)$  s. Ensure that the cement has completely filled the space between the glass plates. After  $(180 \pm 10)$  s, release the loading system and irradiate the specimen through the centre of the upper glass plate for twice the recommended exposure time.

NOTE This irradiation is not intended to cure the material totally, but to stabilize the specimen for measurement.

After the irradiation of Class 2 and Class 3 materials, remove the plates from the loading device and measure the combined thickness of the two glass plates and the specimen film, again taking the reading in the centre of the plates (reading B).

Record the difference between reading A and reading B, to the nearest micrometre, as the film thickness of the luting material.

Carry out five determinations.

### 7.5.3 Treatment of results

Record the film thickness and report as follows.

- a) If at least four of the values are  $\leq 50 \mu\text{m}$ , the material is deemed to have complied with the second requirement of 5.2.2.
- b) If three or more values are  $> 50 \mu\text{m}$ , the material is deemed to have failed.


- c) If only three of the values are  $\leq 50 \mu\text{m}$ , repeat the whole test. If one or more of the values is  $> 50 \mu\text{m}$  on the second occasion, the material is deemed to have failed the whole test.
- d) If the manufacturer claims a specific value for film thickness, at least four of the five values shall be no more than  $10 \mu\text{m}$  greater than the claimed value in order to comply with the first requirement of 5.2.2.

## 7.6 Working time, Class 1 and Class 3 restorative materials, excluding luting materials

### 7.6.1 Apparatus

#### 7.6.1.1 Thermocouple apparatus, as shown in Figure 3.

Dimensions in millimetres

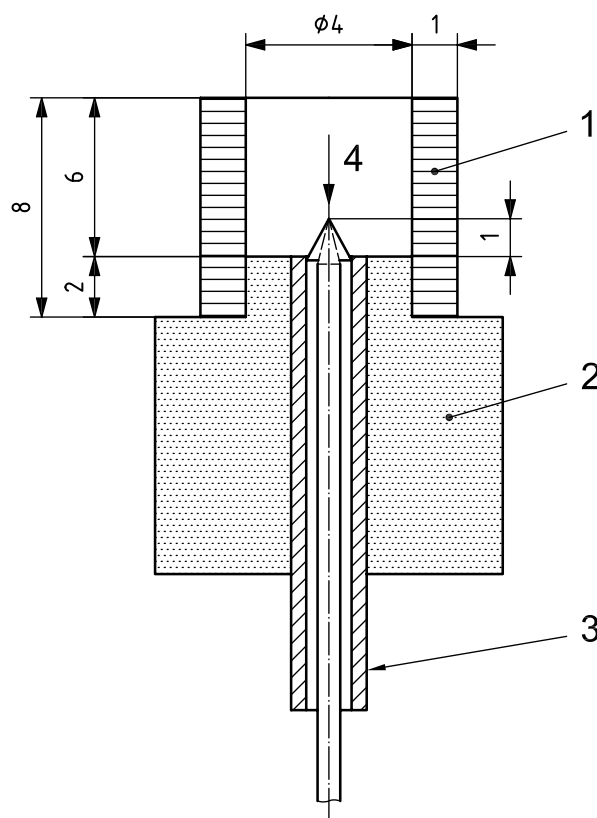

#### Key

- 1 polyethylene tubing
- 2 polyamide block
- 3 stainless steel tube
- 4 thermocouple-cone of solder

**Figure 3 — Apparatus for determination of working and setting times (7.6, 7.8)**

The apparatus consists of a piece of high density polyethylene (or similar material) tubing (Key 1), located on a block of polyamide or similar material, (Key 2), having a hole into which is inserted a stainless steel tube (Key 3) containing a stabilized thermocouple (Key 4).

The tubing shall be 8 mm long, be 4 mm in internal diameter and have a wall thickness of 1 mm. The locating part of the polyamide block shall be 4 mm in diameter and 2 mm high. When assembled, the two components shall form a specimen well 6 mm high  $\times$  4 mm in diameter. In order to facilitate removal of the specimen after testing, the thermocouple shall have a conical tip which protrudes 1 mm into the base of the specimen well. The tolerances on the above-mentioned dimensions are  $\pm 0,1 \text{ mm}$ .


The thermocouple shall consist of wires  $(0,20 \pm 0,05)$  mm in diameter, made of a material (e.g. copper/constantan) capable of registering temperature changes in a specimen of setting material to an accuracy of  $0,1$  °C. The thermocouple is connected to an instrument (e.g. voltmeter or chart recorder) capable of recording the temperature to that accuracy.

**7.6.2 Procedure**

Prepare the test material in accordance with the manufacturer’s instructions (see 8.3) and start timing from the moment mixing is begun. Maintain the mould at  $(23 \pm 1)$  °C and, 30 s after the start of mixing, place the mixed material in the mould and record the temperature,  $T_0$ , of the material. Maintain the apparatus (7.6.1.1) at  $(23 \pm 1)$  °C and continuously record the temperature of the material until the maximum temperature is passed.

A typical recording trace is shown in Figure 4. As soon as the material is inserted into the mould, the temperature will rise slightly to  $T_1$  and then fall until it becomes steady at  $T_0$  and then starts to increase. The point at which the temperature begins to increase denotes the start of the setting reaction and, therefore, the end of the working time. Determine this point by drawing a horizontal base line at  $(T_0 \pm 0,1)$  °C and recording the working time,  $t_w$ , at the point of intersection with the trace. The results are extremely temperature-dependent and slight variations within the permitted temperature range will cause variations of several seconds. Record  $t_w$  from the start of mixing until the temperature starts to increase.

Carry out five determinations.

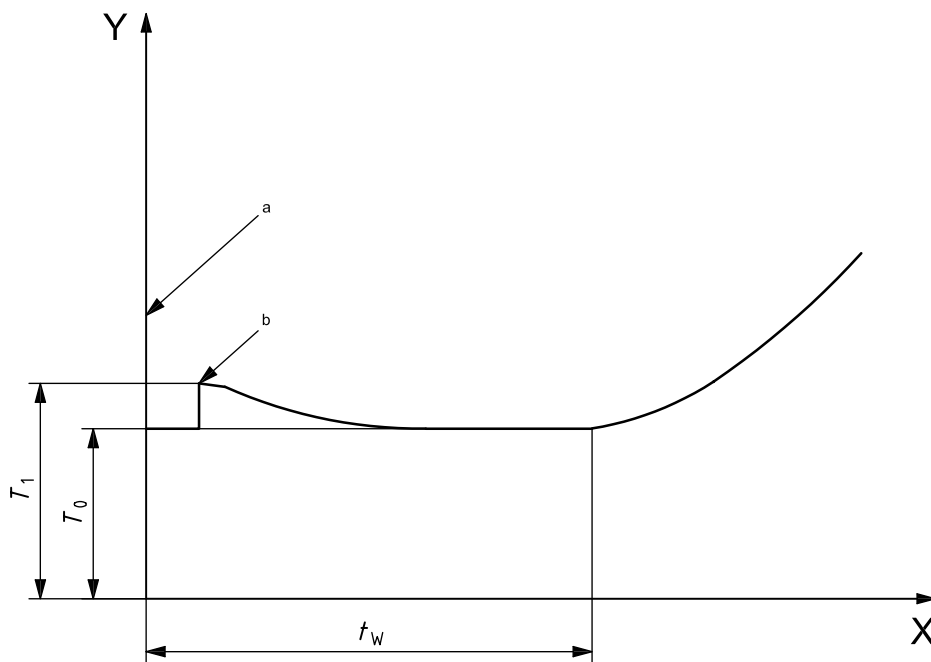

**Key**

- X time
- Y temperature
- a Start of mixing.
- b Insertion.

NOTE The schematic diagram shows the temperature at the time of insertion,  $T_0$ , the slight temperature increase immediately after insertion,  $T_1$ , and the initial time of temperature increase which denotes the start of the setting reaction and, therefore, the end of the working time,  $t_w$ .

**Figure 4 — Determination of working time**



### 7.6.3 Treatment of results

Record the working times and report as follows.

- a) If at least four of the times obtained are  $\geq 90$  s, the material is deemed to have complied with the requirement of 5.2.3.
- b) If three or more of the times are  $< 90$  s, the material is deemed to have failed.
- c) If only three of the times are  $\geq 90$  s, repeat the whole test. If one or more times are  $< 90$  s on the second occasion, the material is deemed to have failed the whole test.

## 7.7 Working time, Class 1 and Class 3 luting materials

### 7.7.1 Apparatus

7.7.1.1 Two glass microscope slides.

7.7.1.2 Timer, accurate to 1 s.

### 7.7.2 Procedure

At 60 s after the completion of mixing, place a spheroidal mass of approximately 30 mg of material on a glass microscope slide (7.7.1.1) and immediately press the second microscope slide against the material using a shearing action to produce a thin layer.

Visually inspect the material to see whether it is physically homogeneous.

NOTE During this test, if the material has begun to set, clefs and voids will appear in the specimen when the thin layer is being produced. Alternatively, with rapid setting materials, there will be an increase in viscosity that will prevent the layer being produced.

Repeat the entire procedure twice, using a new sample for each test. Record the results of all three tests.

### 7.7.3 Treatment of results

If, on visual inspection, the material of all three samples remains physically homogeneous and has formed a thin layer, the material is deemed to have complied with the requirement of 5.2.4.

## 7.8 Setting time, Class 1 and Class 3 materials

### 7.8.1 Apparatus for the determination of setting time of Class 1 and Class 3 restorative materials

7.8.1.1 Thermocouple apparatus, as specified in 7.6.1.1.

### 7.8.2 Apparatus for the determination of setting time of Class 1 and Class 3 luting materials

7.8.2.1 Thermocouple apparatus, as specified in 7.6.1.1 except that the tubing shall be 6 mm long and thus form a specimen well 4 mm in height. All other dimensions specified in 7.6.1.1 shall apply.

### 7.8.3 Procedure

Use the procedure specified in 7.6.2, but maintain the apparatus (7.8.1) at  $(37 \pm 1)$  °C.


Measure the time from the start of mixing until a plateau at maximum temperature is reached. (See Figure 5.) Extend the plateau backwards to meet an extension of the straight line of temperature increase. Record this time,  $t_s$ , as the setting time.

Perform the test five times.

**7.8.4 Treatment of results**

Record the setting times, referring to Table 2 or Table 3 for the particular material under test, and report as follows.

- a) If at least four of the times obtained are not more than the value specified in Table 2 or Table 3 for the particular material, the material is deemed to have complied with the requirement of 5.2.5 or 5.2.6.
- b) If three or more of the times are longer than the value specified in Table 2 or Table 3 for the particular material, the material is deemed to have failed to comply with the requirement of 5.2.5 or 5.2.6.
- c) If only three of the times are not more than the value specified in Table 2 or Table 3 for the particular material, repeat the whole test. If one or more times are longer than the value specified in Table 2 or Table 3 for the particular material, the material is deemed to have failed to comply with the requirement of 5.2.5 or 5.2.6.

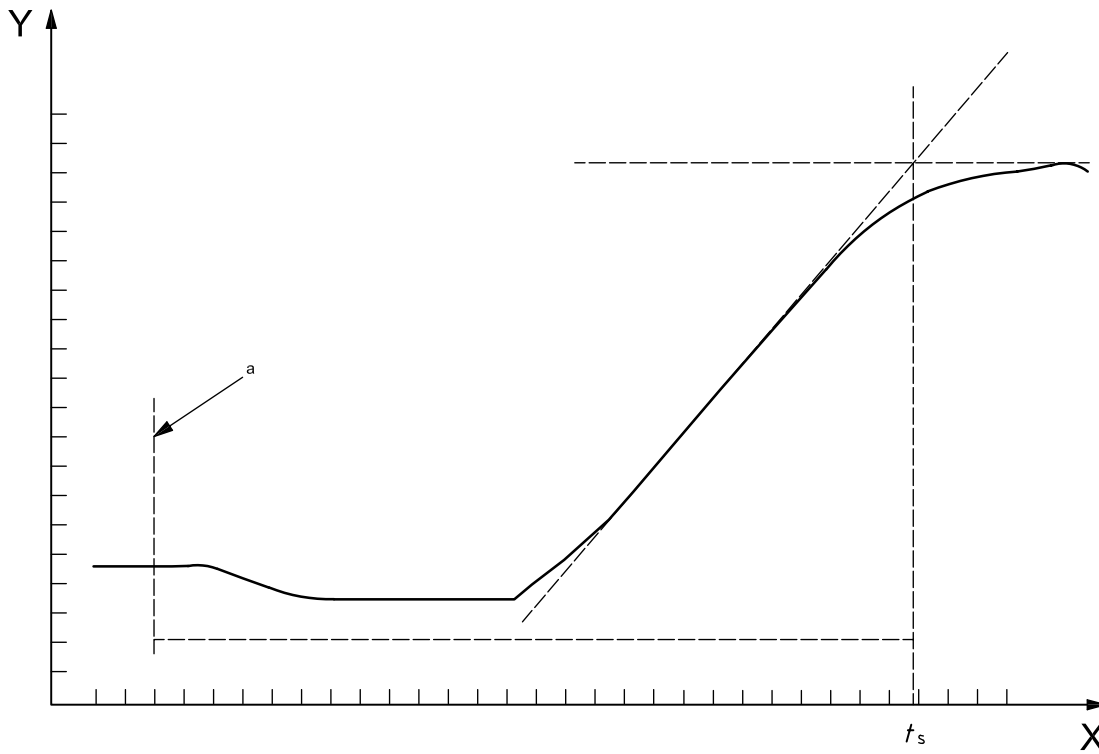

**Key**

- X time
- Y temperature
- a Start of mixing.

NOTE The setting time,  $t_s$ , is determined by extending the plateau backwards to meet an extension of the straight line of temperature increase. This provides a distinct datum point.

**Figure 5 — Method for determining setting time**

## 7.9 Sensitivity to ambient light, Class 2 materials

### 7.9.1 Apparatus

**7.9.1.1 Xenon lamp**, or radiation source of equivalent performance (a suitable apparatus is described in ISO 7491) with colour conversion and ultraviolet filters inserted.

The colour conversion filter <sup>3)</sup> shall have an internal transmittance that matches to within  $\pm 10\%$  of that shown in Figure 6.


The ultraviolet filter shall be made of borosilicate glass with a transmittance  $< 1\%$  below 300 nm and  $> 90\%$  above 370 nm.

The purpose of the filter is to convert the spectrum of the xenon radiation, or equivalent, to that approximating to a dental operating light. The filters and the output of the light should be checked periodically to ensure that the colour temperature at the luxmeter cell is 3 600 K to 6 500 K.

**7.9.1.2 Two glass microscope slides/plates.**

**7.9.1.3 Illuminance-measuring device**, e.g. luxmeter, capable of measuring illuminance of  $(8\,000 \pm 1\,000)$  lx.

**7.9.1.4 Adjustable table.**

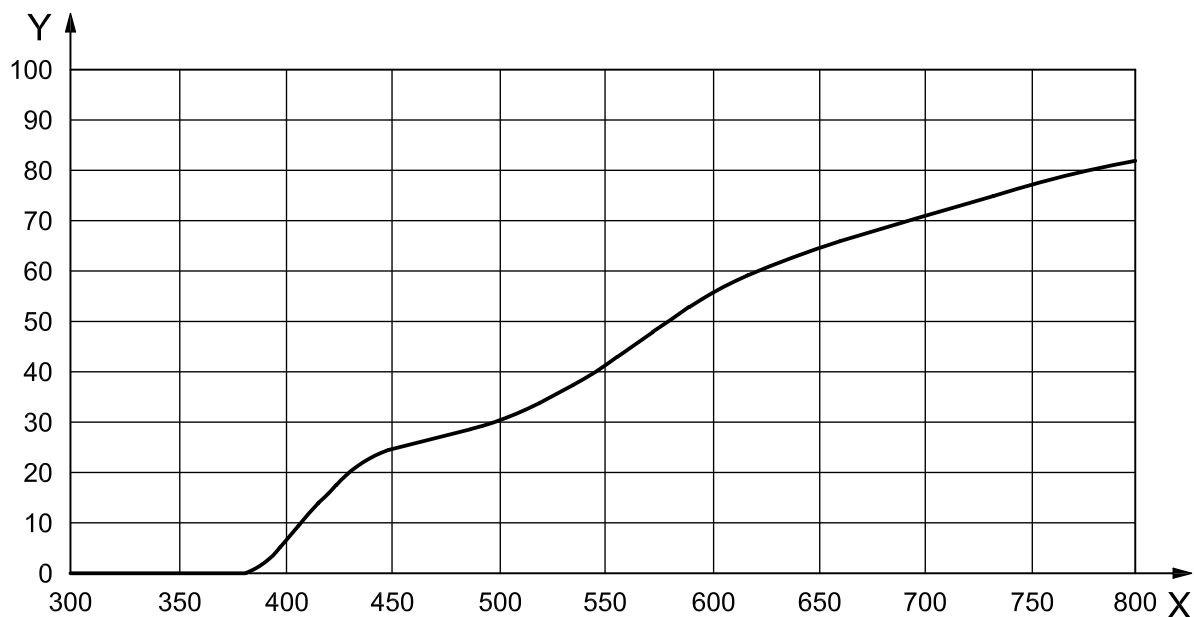

#### Key

X wavelength, in nanometres

Y internal transmission,  $T_i$

**Figure 6 — Internal transmittance for colour conversion filter**

3) The KR 12 filter supplied by Schott AG, Advanced Materials, Hüttenstr. 1, 31073 Grünenplan, Germany, website: [www.schott.com/advanced\\_materials](http://www.schott.com/advanced_materials) is an example of a suitable product available commercially. This information is given for the convenience of the users of this International Standard and does not constitute an endorsement of this product by ISO.

**7.9.1.5 Matt black cover**, for the luxmeter cell.

NOTE This is intended to prevent reflection from the cell interfering with the observation of the specimen.

**7.9.1.6 Timer**, accurate to 1 s.

## 7.9.2 Procedure

In a dark room, position the illuminance-measuring device cell (7.9.1.3) under the xenon lamp (7.9.1.1) with colour conversion and ultraviolet filters inserted at such a height as to provide an illuminance of  $(8\ 000 \pm 1\ 000)$  lx. [The adjustable table (7.9.1.4) is required to do this efficiently.] Cover the cell with the matt black cover (7.9.1.5). Place a spheroidal mass of approximately 30 mg of material on a glass microscope slide (7.9.1.2), position the slide on top of the cell and expose it to the light for  $(60 \pm 5)$  s. Remove the slide with the sample from the irradiated area and immediately press the second microscope slide against the material using a shearing action to produce a thin layer.

Visually inspect the material to see whether it is physically homogeneous.

NOTE During this test, if the material has begun to set, discontinuities and voids will appear in the specimen when the thin layer is being produced. It might aid the inspection to compare the test specimen with one that has been produced in the absence of light.

Repeat the entire procedure twice, using a new sample of material for each test. Record the results of all three tests.

## 7.9.3 Treatment of results

If, on visual inspection, the material of all three samples remains physically homogeneous, the material is deemed to have complied with the requirement of 5.2.7.

## 7.10 Depth of cure, Class 2 materials

### 7.10.1 Apparatus

**7.10.1.1 Stainless steel mould**, for the preparation of a cylindrical specimen, 6 mm long and 4 mm in diameter unless the manufacturer claims a depth of cure in excess of 3 mm; in this event, the mould shall be at least 2 mm longer than twice the claimed depth of cure.

NOTE A mould release agent which does not interfere with the setting reaction, for example a 3 % solution of polyvinyl ether wax in hexane, can be used to facilitate removal of the specimen.

**7.10.1.2 Two glass slides/plates**, each of sufficient area to cover one side of the mould.

NOTE Standard glass microscope slides can be used.

**7.10.1.3 White filter paper**.

**7.10.1.4 Film**, transparent to the activating radiation,  $(50 \pm 30)$   $\mu\text{m}$  thick, e.g. polyester.

**7.10.1.5 External energy source**, as recommended by the manufacturer for use with the test material [see 8.3 e)].

**7.10.1.6 Micrometer**, accurate to 0,01 mm.

**7.10.1.7 Plastics spatula**.

### 7.10.2 Procedure

Place the mould (7.10.1.1) on a strip of the transparent film (7.10.1.4) on a glass microscope slide (7.10.1.2). Fill the mould with the test material, prepared in accordance with the manufacturer's instructions, taking care to exclude air bubbles. Slightly overfill the mould and put a second strip of the transparent film on top, followed by the second microscope slide. Press the mould and strips of film between the glass slides (7.10.1.2) to displace excess material. Place the mould on the filter paper (7.10.1.3), remove the microscope slide covering the upper strip of film and gently place the exit window of the external energy source (7.10.1.5) against the strip of film. Irradiate the material for the time recommended by the manufacturer to achieve a depth of cure of at least 0,5 mm for more opaque luting materials, 1,0 mm for opaque shade restorative materials or 1,5 mm for all other materials.

Immediately after completion of irradiation, remove the specimen from the mould and remove the uncured material with the plastics spatula (7.10.1.7). Measure the height of the cylinder of cured material using the micrometer (7.10.1.6) to an accuracy of  $\pm 0,1$  mm and divide the value by two.

Record this value as the depth of cure.

Repeat the test twice.

Class 2 Group 2 materials shall be tested after exposure to irradiation from the primary source and not after processing in a curing oven. The test is intended to demonstrate the conversion of monomer to polymer at the modelling stage that enables the material to be transferred from the die to the curing oven.

### 7.10.3 Treatment of results

If all three values for opaque luting materials are  $> 0,5$  mm, for other opaque shade restorative materials are  $> 1,0$  mm, and for all other materials are  $> 1,5$  mm, the material has complied with the first two requirements of 5.2.8.

In order to comply with the third requirement of 5.2.8, all three values shall be no more than 0,5 mm below the value stated by the manufacturer.

## 7.11 Flexural strength

### 7.11.1 Apparatus

**7.11.1.1 Mould**, e.g. stainless steel, for the preparation of a test specimen  $(25 \pm 2)$  mm  $\times$   $(2,0 \pm 0,1)$  mm  $\times$   $(2,0 \pm 0,1)$  mm. A mould release agent (see 7.10.1.1, Note) may be used. A suitable mould is illustrated in Figure 7. See also 7.4 para 4 for the preparation of metal affinity materials.

**7.11.1.2 Two metal plates**, each of sufficient area to cover the mould. For Class 2 and Class 3 materials, a **glass microscope slide** for use during polymerization.

**7.11.1.3 Small screw clamp** capable of exerting pressure on the metal plates during specimen preparation.


**NOTE** The results from this test are extremely sensitive to errors in specimen preparation, such as discontinuities or air inclusions which may be more common when preparing highly viscous materials that are particularly difficult to insert into the mould. If difficulty is experienced in preparing satisfactory specimens for this type of material, it is advised that the clamp should be replaced by a press, capable of applying a load of 1 000 kg to the metal plates during specimen preparation.

**7.11.1.4 Film**, transparent to the activating radiation,  $(50 \pm 30)$   $\mu$ m thick, e.g. polyester.

**7.11.1.5 White filter paper.**

**7.11.1.6 Water bath** capable of being maintained at  $(37 \pm 1)$  °C.

Dimensions in millimetres

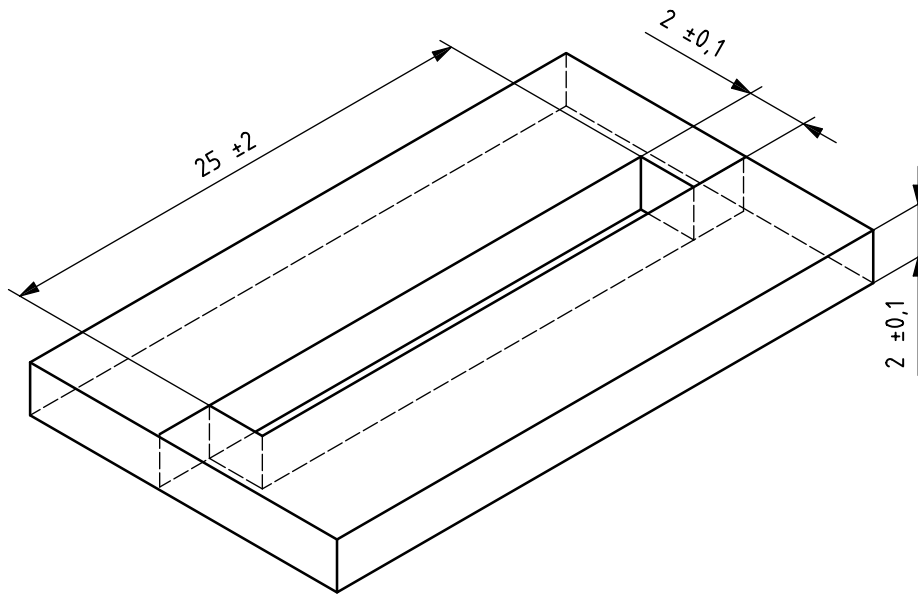

**Figure 7 — Mould for flexural strength test specimens**

**7.11.1.7 External energy source(s)**, (for Class 2 and Class 3 materials) as recommended by the manufacturer for use with the test material [see 8.3 e)].

**7.11.1.8 Micrometer**, accurate to at least 0,005 mm.

**7.11.1.9 Flexural strength test apparatus**, appropriately calibrated, to provide a constant cross-head speed of  $(0,75 \pm 0,25)$  mm/min or a rate of loading of  $(50 \pm 16)$  N/min.

The apparatus consists essentially of two rods (2 mm in diameter), mounted parallel with  $(20 \pm 0,1)$  mm between centres, and a third rod (2 mm in diameter) centred between, and parallel to, the other two, so that the three rods in combination can be used to give a three-point loading to the specimen.

## 7.11.2 Preparation of test specimens

### 7.11.2.1 Class 1 materials

Cover one of the metal plates (7.11.1.2) with the filter paper (7.11.1.5) followed by the film (7.11.1.4) and position the mould (7.11.1.1) upon it. Prepare the material in accordance with the manufacturer's instructions and immediately place it as evenly as possible without bubbles or voids in the mould with a slight excess. Place a second piece of film on the material in the mould and cover this with the second metal plate.

Apply pressure to displace the excess material by means of the clamp (7.11.1.3) for 1 min. After the manufacturer's recommended curing time, place the assembly in the water bath (7.11.1.6), maintained at  $(37 \pm 1)$  °C. After 60 min from the start of mixing, separate the mould and remove the specimen carefully. Inspect the specimen visually for any bubbles, voids or other defects. If there are any irregularities, the specimen shall be discarded and a new one made. Remove any flash by gently abrading it with 320 grit abrasive paper. Store the specimen in water (7.1) at  $(37 \pm 1)$  °C until the start of testing (see 7.11.3).

Prepare five specimens.

### 7.11.2.2 Class 2 and Class 3 materials

Prepare the material in accordance with the manufacturer's instructions and fill the mould with the material, as described in 7.11.2.1. For Class 2 Group 1 and Class 3 materials, replace one of the metal plates with a glass slide (7.11.1.2) and place the exit window of the external energy source (7.11.1.7) at the centre of the specimen and against the glass plate. Irradiate that section of the specimen for the recommended exposure time. Move the exit window to the section next to the centre overlapping the previous section by half the diameter of the exit window and irradiate for the appropriate time. Then irradiate the section on the other side of the centre in the same way. Continue this procedure until the entire length of the specimen has been irradiated for the recommended exposure time. Repeat the irradiation procedure on the other side of the specimen. Place the assembly in the water bath maintained at  $(37 \pm 1) ^\circ\text{C}$  for 15 min. Then remove the specimen from the mould and carefully remove any flash by gently abrading it with 320 grit abrasive paper. Store in water (7.1) at  $(37 \pm 1) ^\circ\text{C}$  until the start of testing (see 7.11.3).

For Class 2 Group 2 materials, follow the manufacturer's instructions regarding the use of the external energy source. [See 8.3 e)]. If the instructions require a preliminary exposure to blue light prior to the placement of the specimen in the external energy apparatus, perform this exposure in accordance with the procedure specified in the paragraph above (Group 1 materials). Remove the specimen from the mould and carefully remove any flash by gently abrading it with 320 grit abrasive paper. Place it directly in the external energy apparatus. After curing, remove the specimen from the apparatus and store in water (7.1) at  $(37 \pm 1) ^\circ\text{C}$  until the start of testing (see 7.11.3).

If no preconditioning is required prior to the insertion of the material in the apparatus, the material and the mould shall be placed in the apparatus for curing. After curing, remove the specimen from the mould and carefully remove any flash by gently abrading it with 320 grit abrasive paper. Store in water (7.1) at  $(37 \pm 1) ^\circ\text{C}$  until the start of testing (see 7.11.3).

Prepare five specimens.

### 7.11.3 Procedure

Measure the dimensions of the specimen at its centre to an accuracy of 0,01 mm. Transfer the specimen to the flexural strength testing apparatus (7.11.1.9).

At 24 h after the start of mixing (Class 1 materials) or irradiation (Class 2 and Class 3 materials), apply a load to the specimen at a cross-head speed of  $(0,75 \pm 0,25)$  mm/min or at a rate of loading  $(50 \pm 16)$  N/min until either the specimen reaches the yield point or, if there is no yield point, fractures.

Record the maximum load exerted on the specimen either at the yield point or at the point of fracture.

Repeat the test on the four other specimens.

### 7.11.4 Treatment of results

Calculate the flexural strength,  $\sigma$ , in megapascals, from Equation (1):

$$\sigma = \frac{3Fl}{2bh^2} \quad (1)$$

where

$F$  is the maximum load, in newtons, exerted on the specimen;

$l$  is the distance, in millimetres, between the supports, accurate to 0,01 mm;

$b$  is the width, in millimetres, at the centre of the specimen measured immediately prior to testing;

$h$  is the height, in millimetres, at the centre of the specimen measured immediately prior to testing.

Report as follows.

- a) If at least four of the results are equal to or greater than the limit specified in Table 1, the material is deemed to have complied with the requirement of 5.2.9.
- b) If three or more of the results are below the limit specified in Table 1, the material is deemed to have failed absolutely.
- c) If only three of the results are equal to or greater than the limit specified in Table 1, repeat the whole test. All five specimens of the second series shall be equal to or greater than the limit specified in Table 1 for the material to comply with the requirement of 5.2.9.

## 7.12 Water sorption and solubility

### 7.12.1 Apparatus

**7.12.1.1 Mould**, of internal dimensions  $(15,0 \pm 0,1)$  mm in diameter and  $(1,0 \pm 0,1)$  mm deep, for the preparation of specimen discs.

A split ring or “washer” mould is suitable. See also 7.4 para 4 for the preparation of metal affinity materials.

NOTE A mould release agent that does not interfere with the setting reaction, for example a 3 % solution of polyvinyl ether wax in hexane, can be used to facilitate removal of the specimen.

**7.12.1.2 Film**, transparent to the activating radiation, e.g. polyester,  $(50 \pm 30)$   $\mu\text{m}$  thick.

**7.12.1.3 Two metal plates**, of sufficient area to cover the mould.

For Class 2 and Class 3 materials, a **glass microscope slide** for use during polymerization.

**7.12.1.4 Two desiccators**, containing silica gel freshly dried for 5 h at 130 °C. Replace the silica gel with freshly dried gel after each weighing sequence.

**7.12.1.5 External energy source(s)**, (for Class 2 and 3 materials), as recommended by the manufacturer for use with the test material [see 8.3 e)].

**7.12.1.6 Oven**, capable of being maintained at  $(37 \pm 2)$  °C.

**7.12.1.7 Analytical balance**, accurate to 0,05 mg in the measuring range required in the test.

**7.12.1.8 Micrometer**, accurate to at least 0,005 mm.

**7.12.1.9 Clamps**.

**7.12.1.10 Plastics tweezers**.

To avoid contamination, the specimens shall be handled at all times using the tweezers.

**7.12.1.11 Hand dust blower or source of oil-free compressed air**, with micro-jet nozzle.

### 7.12.2 Preparation of test specimens

#### 7.12.2.1 Class 1 materials

Place a piece of film (7.12.1.2) on one of the metal plates (7.12.1.3) and place the mould (7.12.1.1) upon it. Slightly overfill the mould with the material prepared in accordance with the manufacturer's instructions. Place a second piece of film on the material in the mould and cover this with the second metal plate, thus displacing excess material.



Clamp the mould together and transfer the assembly immediately to the oven (7.12.1.6) maintained at  $(37 \pm 2) ^\circ\text{C}$ . After 60 min, timed from the start of mixing, remove the specimen from the mould, taking care to avoid surface contamination. Finish the periphery of the specimen to remove flash and irregularities. Hold the periphery of the specimen against 1 000 grit abrasive paper on a non-rotating grinding table and rotate the specimen so that the periphery is abraded. Visually inspect the specimen periphery to ensure it is smooth. Blow debris away with the compressed air jet or dust blower (7.12.1.11). The diameter of the finished specimen shall be  $\geq 14,8$  mm.

Prepare five specimen discs in this way.

### 7.12.2.2 Class 2 and Class 3 materials

Prepare the material in accordance with the manufacturer's instructions and fill the mould with the material as described in 7.12.2.1 and, having displaced excess material, remove the metal plate, leaving the film in place, and replace it with the glass plate. For Class 2 Group 1 and Class 3 materials, place the exit window of the external energy source (7.12.1.5) against the glass plate (see 7.12.1.3). Irradiate that section of the specimen for the recommended exposure time. Move the exit window and irradiate a section of the specimen overlapping the previous section of the specimen. Continue this procedure until the whole specimen has been irradiated for the recommended exposure time. Turn the mould over, remove the other metal plate and replace it with a glass slide. Irradiate the second side of the specimen in the same way as the first side.

A template is required to perform this overlapping irradiation efficiently, and the exact number of exposures is dependent on the diameter of the exit window. Figure 8 shows an example of such a template.


Immediately after irradiation, transfer the mould to the oven (7.12.1.6) maintained at  $(37 \pm 2) ^\circ\text{C}$ . At 15 min after the commencement of irradiation, remove the specimen from the mould and finish the periphery as described in 7.12.2.1.

Prepare five specimen discs in this way.

For Class 2 Group 2 materials, follow the manufacturer's instructions regarding the use of the external energy source(s), [see 8.3 e)]. If the instructions require a preliminary exposure to blue light prior to the placement of the specimen in the external energy apparatus, perform this in accordance with the procedure specified in the paragraph above, remove the specimen from the mould and place it directly in the external energy apparatus. After curing, remove the specimen from the apparatus and finish the periphery as described in 7.12.2.1.

If no preconditioning is required prior to the insertion of the material in the apparatus, the material shall be left in the mould for curing. After curing, remove the specimen from the mould and finish the periphery as described in 7.12.2.1.

Prepare five specimens.



**Figure 8 — Schematic diagram of overlapping irradiation zones for the preparation of the water sorption specimens (external energy source tip diameter is 7 mm)**

**7.12.3 Procedure**

**7.12.3.1** Transfer the specimens to one of the two desiccators (7.12.1.4) maintained at  $(37 \pm 2)^\circ\text{C}$ . After 22 h, remove the specimens, store them in the second desiccator maintained at  $(23 \pm 1)^\circ\text{C}$  for 2 h and then weigh them to an accuracy of 0,1 mg. Repeat this cycle until a constant mass,  $m_1$ , is obtained, i.e. until the mass loss of each specimen is not more than 0,1 mg in any 24 h period.

NOTE Approximately 2 weeks to 3 weeks might be necessary to achieve constant mass.

**7.12.3.2** After final drying, take two measurements of the diameter, at right angles to each other, to an accuracy of 0,01 mm and calculate the mean diameter. Measure the thickness of the specimen to an accuracy of 0,01 mm at the centre of the specimen and at four equally spaced points on the circumference. Calculate the area, in square millimetres, from the mean diameter and then, using the mean thickness, calculate the volume,  $V$ , in cubic millimetres.

**7.12.3.3** Immerse the specimens in water (7.1) at  $(37 \pm 1)^\circ\text{C}$  for 7 d in such a way that they are vertical and have a minimum of 3 mm separation between them. A rack is needed to do this efficiently. The volume of water for immersion of the specimens shall be at least 10 ml per specimen. After 7 d, remove the specimens, wash with water (7.1), blot away surface water until free from visible moisture, wave in the air for 15 s, and weigh 1 min after removal from the water. Record this mass as  $m_2$ .

**7.12.3.4** After this weighing, recondition the specimens to constant mass in the desiccators using the cycle described in 7.12.3.1. Record the constant mass as  $m_3$ .

**7.12.4 Treatment of results**

**7.12.4.1 Water sorption**

Calculate the values for water sorption,  $W_{\text{sp}}$ , in micrograms per cubic millimetre, for each of the five specimens using Equation (2):

$$W_{\text{sp}} = \frac{m_2 - m_3}{V} \tag{2}$$

where

$m_2$  is the mass of the specimen, in micrograms, after immersion in water for 7 d (see 7.12.3.3);

$m_3$  is the mass of the reconditioned specimen, in micrograms (see 7.12.3.4);

$V$  is the volume of the specimen, in cubic millimetres (see 7.12.3.2).

**7.12.4.2 Treatment of water sorption test results**

Report the water sorption results as follows.

- a) If at least four of the values obtained are  $\leq 40 \mu\text{g}/\text{mm}^3$ , the material is deemed to have complied with the first requirement of 5.2.10.
- b) If two or fewer of the values obtained are  $\leq 40 \mu\text{g}/\text{mm}^3$ , the material is deemed to have failed.
- c) If three of the values are  $\leq 40 \mu\text{g}/\text{mm}^3$ , repeat the whole test. If all the values are  $\leq 40 \mu\text{g}/\text{mm}^3$  on the second occasion, the material is deemed to have passed the whole test.

### 7.12.4.3 Solubility

Calculate the values for solubility,  $W_{\text{sl}}$ , in micrograms per cubic millimetre, for each of the five specimens using Equation (3):

$$W_{\text{sl}} = \frac{m_1 - m_3}{V} \quad (3)$$

where

$m_1$  is the conditioned mass, in micrograms, prior to immersion in water (see 7.12.3.1);

$m_3$  and  $V$  are as given in 7.12.4.1.

### 7.12.4.4 Treatment of solubility test results

Report the solubility results as follows.

- If at least four of the values obtained are  $\leq 7,5 \mu\text{g}/\text{mm}^3$ , the material is deemed to have complied with the second requirement of 5.2.10.
- If two or fewer of the values obtained are  $\leq 7,5 \mu\text{g}/\text{mm}^3$ , the material is deemed to have failed.
- If three of the values are  $\leq 7,5 \mu\text{g}/\text{mm}^3$ , repeat the whole test. If, on the second occasion, at least four of the values are  $\leq 7,5 \mu\text{g}/\text{mm}^3$ , the material is deemed to have passed the whole test.

**NOTE** The test for solubility is technically demanding, and it is for this reason that the requirement following a second series of tests is lower than for other tests in this International Standard. The estimation of solubility is considered to be a manifestation of material quality.

## 7.13 Shade and colour stability after irradiation and water sorption

### 7.13.1 General

The test is intended to demonstrate the colour stability of a material after xenon irradiation and after water sorption by comparing an irradiated specimen and a non-irradiated, water-immersed specimen with a dry reference specimen. Carry out the test in accordance with ISO 7491.

### 7.13.2 Apparatus

**7.13.2.1 Oven**, capable of being maintained at  $(37 \pm 2) ^\circ\text{C}$ .

**7.13.2.2 Radiation source, water bath and other apparatus**, as described in ISO 7491.

### 7.13.3 Preparation of test specimens

Prepare three disc specimens as described in 7.12.2.1 for Class 1 materials or 7.12.2.2 for Class 2 and Class 3 materials but omitting the precise finishing of the periphery.

### 7.13.4 Procedure

- Specimen 1: after removal from the mould, store one specimen in the dark and dry in the oven (7.13.2.1) at  $(37 \pm 2) ^\circ\text{C}$  for 7 d; this is the reference specimen.
- Specimen 2: after removal from the mould, store one specimen in the dark in the oven (7.13.2.1) in water (7.1) at  $(37 \pm 2) ^\circ\text{C}$  for 7 d; this specimen will demonstrate any deterioration in colour due to water sorption alone.

- Specimen 3: after removal from the mould, store one specimen in the dark and dry in the oven (7.13.2.1) at  $(37 \pm 2)$  °C for  $(24 \pm 2)$  h. After this time, remove the specimen from the oven and blank off half of it with aluminium or tin foil. Place this specimen in the radiation chamber (7.13.2.2), immerse it in water at  $(37 \pm 5)$  °C and expose it to radiation for 24 h. Ensure that the water level is  $(10 \pm 3)$  mm above the specimen. After exposure, remove the metal foil and transfer the specimen back to the oven at  $(37 \pm 2)$  °C and store it in the dark and dry for 5 d.

#### 7.13.5 Colour comparison for shade

After 7 d, remove wet specimen 2 from the oven, blot it dry with absorbent paper and compare its colour with the manufacturer's nominated shade guide [see 8.3 l)]. Carry out the colour comparison in accordance with 5.3 and ISO 7491.

#### 7.13.6 Colour comparison for colour stability

After 7 d, remove specimens 1 and 3 from the oven. Compare the colour of wet specimen 2 (see 7.13.5) with the reference specimen 1.

Compare the colour of both halves of specimen 3 with each other and with the reference specimen 1.

Carry out all the colour comparisons in accordance with 5.4 and ISO 7491.

### 7.14 Radio-opacity

NOTE This test can be conducted with analogue or digital X-ray apparatus at the discretion of the test laboratory.

#### 7.14.1 Analogue apparatus

**7.14.1.1 Single-phase dental X-ray unit**, with a total filtration of 1,5 mm aluminium and capable of operation at  $(65 \pm 5)$  kV, with suitable accessories.

**7.14.1.2 Dental X-ray film**, of speed group D (as specified in ISO 3665), developing solution and fixer.

**7.14.1.3 Aluminium step wedge**, purity at least 98 % (mass fraction) with less than 0,1 % (mass fraction) copper and less than 1,0 % (mass fraction) iron present, 50 mm long  $\times$  20 mm wide, having a thickness range from 0,5 mm to 5,0 mm in equally spaced steps of  $(0,50 \pm 0,01)$  mm. The wedge shall be free-standing.

NOTE The overall dimensions (50  $\times$  20) mm can be adjusted in relation to the film size for the convenience of the user.

**7.14.1.4 Sheet of lead**, not less than 2 mm thick.

**7.14.1.5 Photographic densitometer**, capable of measuring in the range 0,5 to 2,5 of optical density.

**7.14.1.6 Micrometer**, accurate to 0,005 mm.

#### 7.14.2 Digital apparatus

**7.14.2.1 Digital X-ray unit.**

NOTE Testing has shown that these units should be used without "Automatic Gain Control" for the purposes of this test.

**7.14.2.2 X-ray sensor of occlusal film size**, calibrated for use with the digital X-ray unit (7.14.2.1) with appropriate software.

**7.14.2.3 Software capable of greyscale analysis**, with an accuracy of  $\pm 1$  grey value, e.g. Adobe Photoshop<sup>4)</sup>.

### 7.14.3 Preparation of test specimens

Prepare one disc specimen as described in 7.12.2.1 for Class 1 materials or 7.12.2.2 for Class 2 and Class 3 materials, omitting the precise finishing of the periphery. This method shall produce specimens with a thickness in the range  $(1,0 \pm 0,1)$  mm.

### 7.14.4 Test procedure for analogue equipment

Position the X-ray film (7.14.1.2) on the sheet of lead (7.14.1.4). Place the specimen and the aluminium step wedge (7.14.1.3) upright in the centre of the film.

Irradiate the specimen, aluminium step wedge and film with X-rays at  $(65 \pm 5)$  kV at a target film distance of 300 mm to 400 mm for such a time that, after processing, the region of film beside the specimen and aluminium has an optical density of between 1,5 and 2.

NOTE Exposures of between 0,3 s and 0,4 s at 10 mA are typical.

Measure the thickness of the specimen,  $\delta_s$ , to an accuracy of 0,01 mm using the micrometer (7.14.1.6).

If the thickness of the specimen is in the range  $(1,0 \pm 0,1)$  mm, then, after developing and fixing the film, measure the optical density of the image of the specimen and that of each step of the aluminium using the densitometer (7.14.1.5).

### 7.14.5 Test procedure for digital equipment

Measure the thickness of the specimen,  $\delta_s$ , to an accuracy of 0,01 mm using the micrometer (7.14.1.6).

Position the X-ray sensor (7.14.2.2) on the sheet of lead (7.14.1.4). Place the specimen and the step wedge (7.14.1.3) near the centre of the sensor. Irradiate the assembly with X-rays at a cathode target-film distance of 300 mm to 400 mm without the automatic gain control. Repeat the procedure to find the appropriate exposure time to make a clear image.

NOTE Exposures that are about five times to ten times as long as that for conventional X-ray film should be expected.

Export the digital image file to the greyscale analysis software (7.14.2.3). The number of grey shades is assessed using the measuring tool in the software. The number of grey shades in the digital image is given by the number of binary digits (bits) used to define a pixel.

Using the greyscale analysis software, define a rectangular area to measure in the specimen image and measure the average grey value in that area.

Repeat this procedure with each of the steps of the step wedge.

In the greyscale, the darkest grey shade is usually defined by the value zero while the lightest has a value of 255. This score is the reverse order to the density of X-ray film.

---

4) Adobe Photoshop is an example of a suitable product available commercially. This information is given for the convenience of users of this International Standard and does not constitute an endorsement by ISO of this product.

7.14.6 Treatment of results


Plot the individual optical densities/grey values of each aluminium step against the thickness of each step (see Figure 9 for analogue, Figure 10 for digital equipment). Take the optical density/grey value for the specimen of thickness  $\delta_s$  and determine from the plot the corresponding value of aluminium,  $\delta_a$ .

The radio-opacity (aluminium equivalent) value of a specimen of 1,0 mm thickness is then given by  $\delta_a/\delta_s$ .

If this value is  $\geq 1$  mm, the material is deemed to have complied with the first requirement of 5.5.

If the manufacturer has claimed a specific value for radio-opacity [see 8.2.3 h) and 8.3 o)], then the aluminium equivalent determined above shall be no more than 0,5 mm below the value claimed by the manufacturer.

The plot of optical density against aluminium thickness of the step wedge shall be made for each radiographic exposure, since minor variations may occur due to radiographic processing.

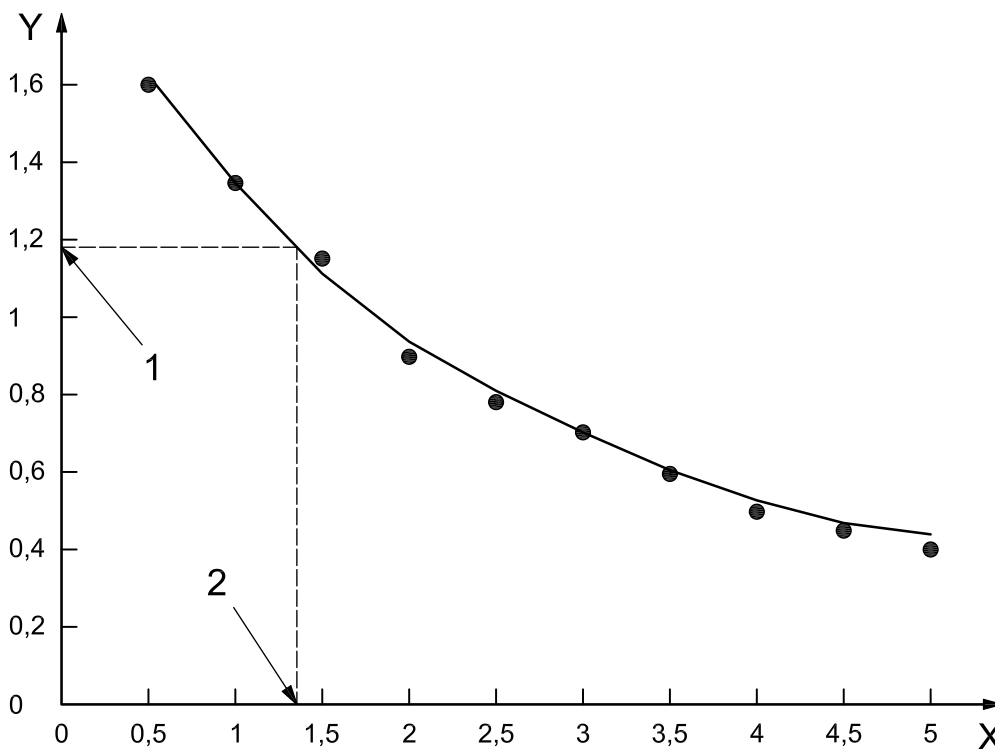


Key

- X aluminium steps, in millimetres
- Y optical density
- 1 specimen reading
- 2 aluminium equivalent

**Figure 9 — Determination of radio-opacity**

Plot of optical density against aluminium step thickness and superimposition of a specimen reading determined by analogue equipment

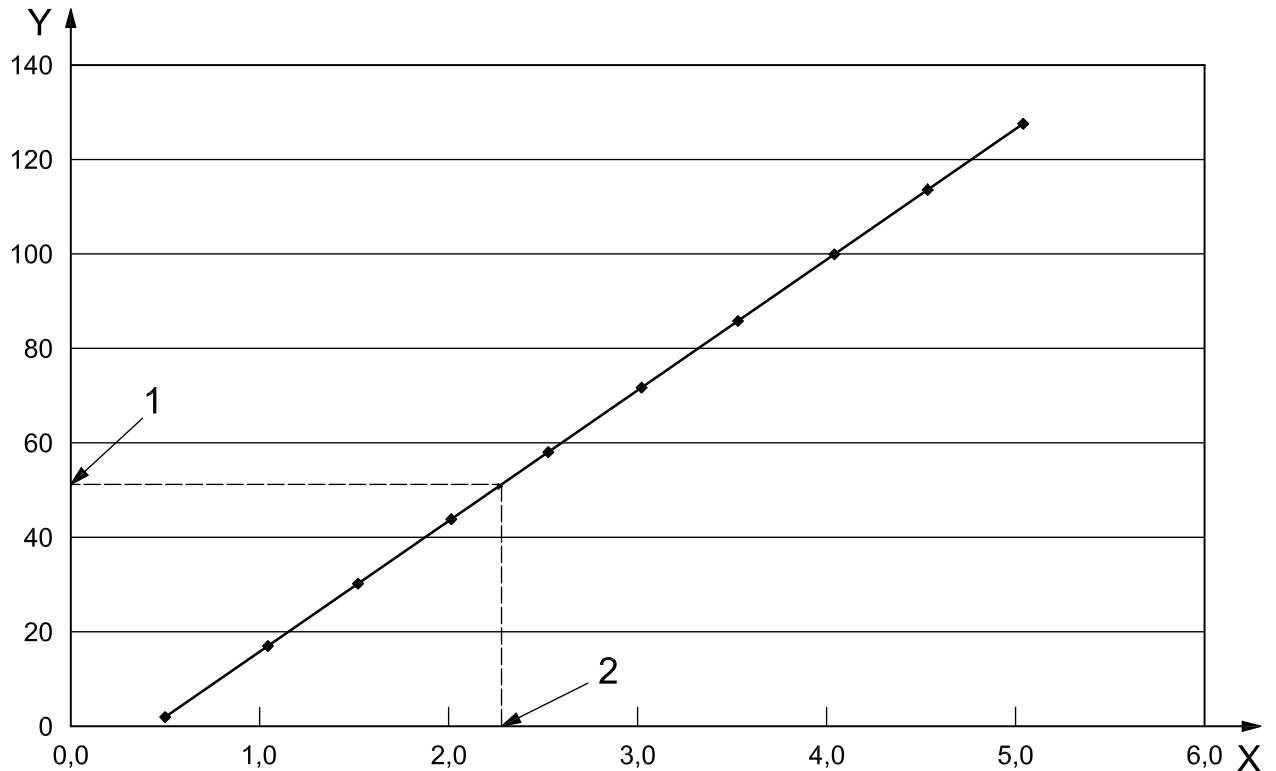**Key**

- X aluminium steps, in millimetres
- Y grey value
- 1 specimen reading
- 2 aluminium equivalent

**Figure 10 — Determination of radio-opacity**

Plot of optical density against aluminium step thickness and superimposition of a specimen reading determined by digital equipment

## 8 Packaging, marking and instructions and information to be supplied by the manufacturer

NOTE Additional information can be included at the discretion of the manufacturer or as required by legislation.

### 8.1 Packaging

The materials shall be supplied in containers or capsules that afford adequate protection and have no adverse effect on the quality of the contents. For the purposes of this International Standard, the container or capsule shall be considered to be the immediate wrapping of the material.

An outer pack may also be used to present the containers or capsules as a single unit that provides protection for them.

### 8.2 Marking

#### 8.2.1 Capsule or single dose container

NOTE The single dose container is a small syringe containing no more than 0,5 ml of material.

## ISO 4049:2009(E)

- a) Each capsule or single dose container shall be marked in order to identify the product.
- b) If the product is supplied in pre-coloured shades, each capsule or single dose container shall be marked or colour coded so that the shade of its contents can be identified.
- c) Each capsule or single dose container shall show the batch identification, consisting of a serial number or a combination of letters and numbers, that refers to the manufacturer's records for that particular batch of material.

### 8.2.2 Multi-dose container

EXAMPLE A dispensing syringe containing 2 g of material.

The following information shall be clearly visible on each container:

- a) the trade name of the material;
- b) the shade or description that can be related to the manufacturer's nominated shade guide, if the material is supplied in a range of pre-coloured shades;
- c) batch identification, consisting of a serial number or a combination of letters and numbers, that refers to the manufacturer's records for that particular batch of material;
- d) the net mass, in grams, or net volume, in millilitres.

### 8.2.3 Outer pack

The outer pack shall have the following information clearly visible:

- a) the manufacturer's name and address and/or agent responsible for the country of sale;
- b) the trade name of the material;
- c) recommended conditions of storage;
- d) the net mass, in grams, or net volume, in millilitres;
- e) the expiry date, expressed in accordance with ISO 8601, for the material if stored under the manufacturer's recommended conditions [see 8.3 i)];
- f) presence of hazardous substances indicated by text or symbol;
- g) the legend "polymer-based dental restorative material" or "resin-based dental restorative material" if the product is a restorative material or "polymer-based dental luting material" or "resin-based dental luting material" if the product is a luting material.

Furthermore, the following information shall be clearly visible either on the outer pack or in the manufacturer's instructions (see 8.3) or both:

- h) the word "radio-opaque" if the material complies with the requirements of 5.5; if the manufacturer wishes to claim a specific value for radio-opacity, this shall be stated in the manufacturer's instructions [see 8.3 o)] and shall be determined by the method specified in 7.14;
- i) in the case of restorative materials, a statement indicating whether or not the material is suitable for the restoration of occlusal surfaces;
- j) a statement indicating whether the material is chemically activated, activated by external energy or dual cure, either intra-orally and/or extra-orally;
- k) in the case of a luting material, a statement indicating whether the manufacturer claims colour stability.



### 8.3 Manufacturer's instructions and information for the user

The following information, together with a description of the product, shall accompany each individual pack of material:

- a) the principal organic component of the polymer base;
- b) the range of dimensions of inorganic filler particles and the percentage by volume of total inorganic filler;
- c) the indications for clinical use;
- d) instructions for the preparation and proportioning of components and mixing, including any necessary precautions regarding the manipulation of the material, including, if appropriate, the maximum proportion of tints and blenders that may be used without detriment to the physical properties (the ambient conditions under which this should be carried out may be included);
- e) recommended external energy source(s) and exposure/processing times for all versions of Class 2 and Class 3 materials, and, in the case of Class 2 materials, the depth to which the material is cured after the recommended exposure (determined in accordance with 7.10);
- f) working and setting times for Class 1 and Class 3 materials, and an indication of the time when a matrix may be removed, if this differs from the setting time;
- g) information on the use of a base or liner, if recommended, or other recommended protective measures if the material is likely to cause pulpal irritation, and information on whether any base or liner is known to be incompatible with the material (e.g. eugenol-containing materials);
- h) recommended instructions for finishing;
- i) recommended storage conditions (e.g. need for refrigeration) and the shelf life under those conditions of storage beyond which the material should not be used, making reference to the expiry date [see 8.2.3 e)];
- j) any pharmacologically active ingredients, when present and referred to in the material claim for use;
- k) special indications or warnings, when necessary, in respect of such properties as toxicity, hazard, flammability or tissue irritancy, for both patient and operator;
- l) in order to identify pre-coloured shades for restorative materials, a shade guide or a nominated commercially available shade guide for use with the material (the shade guide shall indicate the colour of the fully water-saturated material and, in the case of luting materials, this requirement shall only apply when colour stability is claimed);

NOTE A manufacturer can include such information when colour stability is not claimed without contravening this standard.

- m) in the case of luting materials, whether the material has a chemical affinity for metal;
- n) information about the use and compatibility of the material with adhesives or bonding agents;
- o) whether or not radio-opacity is claimed.

If a specific value for radio-opacity is stated, this shall be determined in accordance with 7.14. If certain shades amongst others that are radio-opaque are not radio-opaque, this shall be stated. If the radio-opacity value of another shade or shades is more than twice the "universal" shade value, this shall be stated and the manufacturer shall give an indication, either quantitatively or qualitatively, of the differences. An explanation of the radio-opacity value shall be included, e.g. aluminium has a radio-opacity equivalent to that of dentine. Thus 1 mm of material having a radio-opacity equivalent to 1 mm of aluminium has a radio-opacity equivalent to that of dentine.

## Bibliography

- [1] ISO 6874, *Dentistry — Polymer-based pit and fissure sealants*
- [2] ISO 7405, *Dentistry — Evaluation of biocompatibility of medical devices used in dentistry*
- [3] ISO 10477, *Dentistry — Polymer-based crown and bridge materials*
- [4] ISO 10993-1, *Biological evaluation of medical devices — Part 1: Evaluation and testing within a risk management process*
- [5] ISO 10650-1, *Dentistry — Powered polymerization activators — Part 1: Quartz tungsten halogen lamps*
- [6] ISO 10650-2, *Dentistry — Powered polymerization activators — Part 2: Light-emitting diode (LED) lamps*

.....



---

---

**ICS 11.060.10**

Price based on 28 pages