
**Rubber, vulcanized — Determination of
temperature rise and resistance to fatigue
in flexometer testing —**

Part 2:
Rotary flexometer

*Caoutchouc vulcanisé — Détermination de l'élévation de température et
de la résistance à la fatigue dans les essais aux flexomètres —*

Partie 2: Flexomètre à rotation



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



COPYRIGHT PROTECTED DOCUMENT

© ISO 2008

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

| | |
|--|----|
| Foreword..... | iv |
| 1 Scope | 1 |
| 2 Normative references | 1 |
| 3 Terms and definitions..... | 1 |
| 4 Principle..... | 2 |
| 5 Test pieces | 2 |
| 6 Apparatus | 2 |
| 6.1 Rotary flexometer (see Figures 1 and 2)..... | 2 |
| 6.2 Measuring gauge | 4 |
| 6.3 Temperature-measurement device | 4 |
| 6.4 Timer | 4 |
| 7 Procedure | 4 |
| 7.1 Preparation | 4 |
| 7.2 Test operation | 4 |
| 7.2.1 General..... | 4 |
| 7.2.2 Measurement of temperature rise | 4 |
| 7.2.3 Determination of resistance to fatigue breakdown | 4 |
| 8 Test conditions | 5 |
| 8.1 General..... | 5 |
| 8.2 Measurement of temperature rise | 5 |
| 8.3 Determination of resistance to fatigue breakdown | 5 |
| 9 Evaluation of test data..... | 6 |
| 9.1 Temperature rise..... | 6 |
| 9.2 Resistance to fatigue breakdown..... | 6 |
| 9.2.1 Fatigue life | 6 |
| 9.2.2 Fatigue-life curves | 6 |
| 10 Test report | 8 |
| Bibliography | 9 |

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 4666-2 was prepared by Technical Committee ISO/TC 45, *Rubber and rubber products*, Subcommittee SC 2, *Testing and analysis*.

This second edition cancels and replaces the first edition (ISO 4666-2:1982), of which it constitutes a minor revision. The main change is the replacement of ISO 4648 by ISO 23529 in Clause 2 and in 6.2.

ISO 4666 consists of the following parts, under the general title *Rubber, vulcanized — Determination of temperature rise and resistance to fatigue in flexometer testing*:

- *Part 1: Basic principles*
- *Part 2: Rotary flexometer*
- *Part 3: Compression flexometer*
- *Part 4: Constant-stress flexometer*

Rubber, vulcanized — Determination of temperature rise and resistance to fatigue in flexometer testing —

Part 2: Rotary flexometer

WARNING — Persons using this part of ISO 4666 should be familiar with normal laboratory practice. This part of ISO 4666 does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

CAUTION — Certain procedures specified in this part of ISO 4666 may involve the use or generation of substances, or the generation of waste, that could constitute a local environmental hazard. Reference should be made to appropriate documentation on safe handling and disposal after use.

1 Scope

This part of ISO 4666 specifies a rotary flexometer test for the determination of the temperature rise and resistance to fatigue of vulcanized rubbers under rotary shear loading. It allows the use of all four types of test conditions described in ISO 4666-1.

It gives directions for carrying out measurements which make possible predictions regarding the durability of rubbers in finished articles (tyres, bearings, supports, V-belts, cable pulley insert rings and similar products subject to dynamic flexing in service). However, owing to the wide variations in service conditions, no simple correlation between the accelerated tests described in this part of ISO 4666 and service performance can be assumed.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 4666-1, *Rubber, vulcanized — Determination of temperature rise and resistance to fatigue in flexometer testing — Part 1: Basic principles*

ISO 23529, *Rubber — General procedures for preparing and conditioning test pieces for physical test methods*

3 Terms and definitions

For definitions of the terms and concepts used in connection with this test and in evaluating the test results, see ISO 4666-1.

4 Principle

A cylindrical test piece is compressed axially to a predetermined stress or strain (pre-stress or pre-strain) between two chuck plates. One of the chuck plates is mounted on a freely rotating shaft while the other plate is mounted on a shaft which is driven by a motor. The shafts are displaced laterally relative to each other by a predetermined amount or by means of a predetermined force. The eccentricity of the two rotating plates produces a flexing of the rotating test piece, while it is under compression, resulting in a rise in temperature and ultimately fatigue breakdown. The rise in temperature is determined at the centre of the test piece by means of a needle probe. The fatigue life is also determined.

5 Test pieces

For general guidance as to number, preparation and conditioning of test pieces, see ISO 4666-1.

The test pieces shall be cylinders of height equal to their diameter. The dimensions shall be either $20 \text{ mm} \pm 0,2 \text{ mm}$ or $38 \text{ mm} \pm 0,4 \text{ mm}$. The smaller test piece is preferred because it is usually more uniform in degree of vulcanization throughout the whole mass.

If test pieces are prepared by vulcanization in moulds, it is recommended that the mould cavities have a diameter and depth of $20,2 \text{ mm} \pm 0,05 \text{ mm}$ or $38,2 \text{ mm} \pm 0,05 \text{ mm}$ in order to allow for thermal shrinkage after vulcanization. If test pieces are prepared from finished parts by cutting, it is recommended that the circular die used for this purpose has an inside diameter of $20 \text{ mm} \pm 0,03 \text{ mm}$ or $38 \text{ mm} \pm 0,03 \text{ mm}$.

6 Apparatus

6.1 Rotary flexometer (see Figures 1 and 2)

The schematic illustration in Figure 1 shows the important parts of the flexometer. The cylindrical test piece acts as a friction clutch between two chuck plates mounted on parallel shafts such that they can be rotated. The shaft carrying the right-hand chuck plate (see Figure 1) shall be mounted on a movable bearing so that almost frictionless movement in the axial direction is possible. This is in order that the test piece can be subjected to axial compression by displacing the movable chuck plate by a predetermined amount (testing under constant pre-strain) or through the action of a predetermined force (testing under constant pre-stress), for example by means of a compression spring.


The movable bearing shall also be capable of being displaced transversely with respect to the axis of the test piece. This displacement can be obtained by movement of the bearing carrier or by means of a cross support arrangement. In this manner, a transverse deformation is imposed upon the test piece.

The deflection can be by a predetermined amount (testing under constant cyclic strain) or under the action of a predetermined force (testing under constant cyclic stress).

The left-hand chuck plate shall be driven by a motor at a rotational frequency of $14,6 \text{ Hz} \pm 0,1 \text{ Hz}$ or $25,0 \text{ Hz} \pm 0,2 \text{ Hz}$. The test piece transmits the rotation from the driven chuck plate to the displaceable chuck plate.

The rotation and simultaneous deflection subject the test piece to a sinusoidal form of shear deformation. Suitable devices such as dial gauges and electronic transducers shall be incorporated in order to determine all the deformations and loadings of the test piece. The devices for measuring the deformations shall have a precision of at least $0,01 \text{ mm}$. The precision of the force-measuring devices shall be at least $0,1 \text{ N}$. The use of chart recorders for recording the transverse force or the transverse displacement is recommended. The measuring devices shall be mounted so that their pressure acts against the loading as shown in Figure 1.


The chuck plates shall be made of steel. Caps made of plastics or other heat-insulating materials having a conductivity of not more than $0,28 \text{ W/(m}\cdot\text{K)}$ can be placed over these for heat-generation tests if considered necessary. The caps shall have a thickness of $10,0 \text{ mm} \pm 0,2 \text{ mm}$ and shall lie in close contact with the metal plates over their entire surface. As an alternative to caps, discs of heat-insulating material can be placed immediately behind the chuck plates.

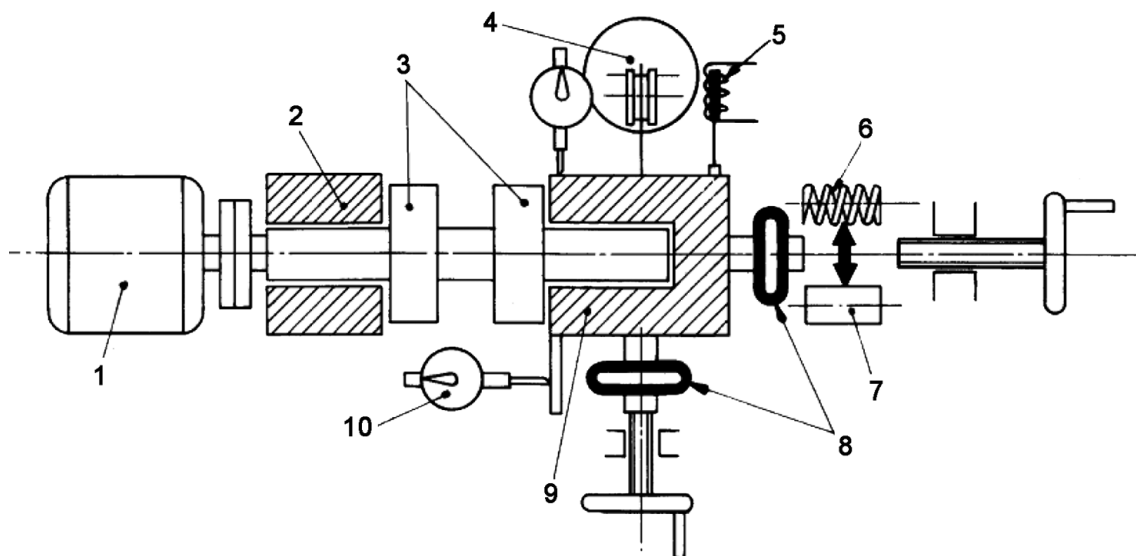

Key

- | | | |
|---------------------------------|---------------------------|---------------------|
| 1 motor | 5 displacement transducer | 8 force transducers |
| 2 fixed bearing | 6 compression spring | 9 movable bearing |
| 3 chuck plates | 7 intermediate piece | 10 dial gauge |
| 4 weight for transverse loading | | |

Figure 1 — Rotary flexometer before application of force

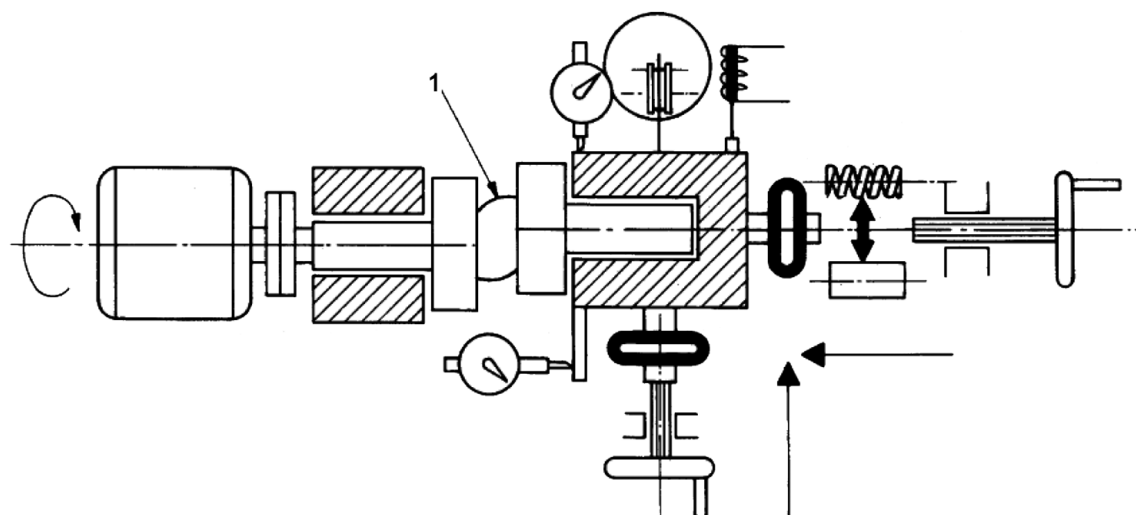

Key

- | |
|--------------|
| 1 test piece |
|--------------|

Figure 2 — Rotary flexometer after application of force

To facilitate location of the cylindrical test piece between the chuck plates or caps, and in order to avoid sideways displacement during the test, the chuck plates and caps shall be provided with a centrally located recess to receive the test piece. The recess shall have the following dimensions:

- for small cylinders: diameter 20,2 mm ± 0,03 mm, depth 0,7 mm ± 0,03 mm;
- for large cylinders: diameter 38,4 mm ± 0,05 mm, depth 1,0 mm ± 0,05 mm.

6.2 Measuring gauge

The gauge for measuring the height and diameter of the test pieces shall conform to the requirements of ISO 23529. A dial gauge having a circular foot probe of diameter 10 mm and exerting a pressure of $22 \text{ kPa} \pm 5 \text{ kPa}$ is suitable.

6.3 Temperature-measurement device

A temperature-measurement device with a temperature-sensing probe consisting of a needle of diameter not more than 1 mm shall be used. The maximum allowable error shall be $\pm 0,5 \text{ }^\circ\text{C}$.

6.4 Timer

The error of time measurement shall not be greater than 5,0 s.

7 Procedure

7.1 Preparation

When the small-size test piece is used for the heat-generation test, it is recommended that the insulating caps be fitted on the chuck plates. When using the larger size of test piece or when determining the fatigue resistance, the caps need not be fitted.

Measure the height of the test piece to within 0,05 mm in the unloaded condition before placing in the flexometer.

Before beginning the actual test, carry out a preliminary run of 15 min under test conditions, using a rubber of similar hardness to that of the test piece. In this way, the chuck plates (and caps when fitted) are warmed up and the apparatus is brought to normal conditions.

7.2 Test operation

7.2.1 General

With the device stationary, bring the two chucks into axial alignment and set up the test piece between them. Then compress the test piece axially by about 10 %; that is to about 90 % of the original height. Switch on the motor and check that the test piece is properly located. If the test piece is not running centrally, remove and re-install it. Thereafter, i.e. at the beginning of the running of the test, compress the test piece to the desired deformation or apply the desired force by means of the compression spring or a weight. Directly thereafter, displace the right-hand (displaceable) bearing using the transverse spindle or by means of a transverse force perpendicular to the axis. The full deflection shall be reached within 10 s. The test duration begins after the required transverse deformation has been imposed.

7.2.2 Measurement of temperature rise

At the end of the specified test duration, switch off the motor, remove the transverse deformation and the axial deformation, and immediately measure the temperature at the centre of the test piece with the needle probe. The time between switching off the motor and the temperature measurement shall be $10 \text{ s} \pm 2 \text{ s}$. The temperature measurement in the test piece can be carried out with the test piece in the apparatus or after its removal.

7.2.3 Determination of resistance to fatigue breakdown

Measure the period of time from the beginning of cyclic deformation to the start of breakdown in the interior of the test piece.

If breakdown does not occur after 30 min, stop the test, unless a longer-running test is specified. In this case, report the fatigue deformability or fatigue stress instead of the limiting fatigue deformability or limiting fatigue stress (see 9.2.2).

The onset of breakdown is indicated by changes in the transverse force or transverse displacement. The criterion for determining the onset of breakdown shall be the same for all comparative tests.

After termination of the test, section the test piece by cutting in an axial plane and examine it visually to ensure that the level of damage (indicated by the presence of fine pores, cracks or degradation of the rubber in the centre of the test piece) is comparable. In the case of rubbers in which the beginning of breakdown is difficult to detect, subject several test pieces to the test to ensure correct assessment.

8 Test conditions

8.1 General

Tests shall be conducted at standard laboratory temperature, i.e. at $23\text{ °C} \pm 2\text{ °C}$ or $27\text{ °C} \pm 2\text{ °C}$.

The forces produced by the dial gauges or strain gauges shall be taken into account.

8.2 Measurement of temperature rise

After a running time of $20\text{ min} \pm 0,5\text{ min}$, after which temperature equilibrium is generally reached, measure the temperature rise. Recommended loadings are the forces or deformations given under "normal" in Table 1. If the resulting temperature rise is too small to allow a meaningful comparison, the "increased" values can be used.

Table 1 — Loading conditions for measurement of temperature rise

| Test conditions | Test piece dimensions mm | Normal | | Increased | |
|---|-----------------------------|-----------------|------------------|---------------|--------------|
| | | Axial | Transverse | Axial | Transverse |
| Constant pre-stress and cyclic stress amplitude | 20 × 20 | 300 ± 2 N | 30 N ± 0,2 N | 500 N ± 2 N | 40 N ± 0,2 N |
| | 38 × 38 | 1 000 N ± 5 N | 100 N ± 0,5 N | 1 400 N ± 5 N | 200 N ± 1 N |
| Constant pre-strain and cyclic strain amplitude | 20 × 20 | 6 mm ± 0,02 mm | 2,8 mm ± 0,02 mm | — | — |
| | 38 × 38 | 10 mm ± 0,04 mm | 3,0 mm ± 0,04 mm | — | — |

8.3 Determination of resistance to fatigue breakdown

If the fatigue life has only to be determined for one loading, or for preliminary investigations to determine the appropriate loading ranges for plotting the fatigue-life curve, the test conditions normally recommended are those given under "normal" in Table 2. If the resulting duration of the test is too short, the "reduced" values can be used.

Table 2 — Loading conditions for determination of resistance to fatigue breakdown

| Test conditions | Test piece dimensions mm | Normal | | Reduced | |
|---|-----------------------------|-----------------|------------------|-----------------|------------------|
| | | Axial | Transverse | Axial | Transverse |
| Constant pre-stress and cyclic stress amplitude | 20 × 20 | 500 N ± 2 N | 80 N ± 0,2 N | 500 N ± 2 N | 50 N ± 0,2 N |
| | 38 × 38 | 1 700 N ± 5 N | 270 N ± 2 N | 1 700 N ± 5 N | 150 N ± 1 N |
| Constant pre-strain and cyclic strain amplitude | 20 × 20 | 6 mm ± 0,02 mm | 6,5 mm ± 0,02 mm | 6 mm ± 0,02 mm | 3,5 mm ± 0,02 mm |
| | 38 × 38 | 10 mm ± 0,04 mm | 10 mm ± 0,04 mm | 10 mm ± 0,04 mm | 5 mm ± 0,04 mm |

9 Evaluation of test data

9.1 Temperature rise

Measure the rise in temperature above ambient temperature of the centre of the test piece.

9.2 Resistance to fatigue breakdown

9.2.1 Fatigue life

The fatigue life is the number of loading cycles to failure, N , which can be calculated by the product of the time, in seconds, to failure and the test frequency, in hertz, or can be measured directly.

9.2.2 Fatigue-life curves

The resistance to fatigue breakdown is best presented graphically. The values for the fatigue life N (number of cycles to breakdown) and the loading amplitudes are plotted on a graph with a logarithmically scaled abscissa (number of cycles) and a linearly scaled ordinate (loading). Figure 3 shows an example of an evaluation of the testing of cylindrical test pieces 20 mm in height and 20 mm in diameter under conditions of predetermined cyclic deformation. The axial deformation (pre-stress) used was 6 mm.

The cyclic strain amplitude or cyclic stress amplitude at which the fatigue-life curve becomes essentially parallel to the $\log N$ axis is taken as the limiting fatigue deformability, γ_{∞} , or limiting fatigue stress amplitude, τ_{∞} .

If required, a plot of fatigue life against cyclic strain amplitude or cyclic stress amplitude can be used to calculate the fatigue deformability or fatigue stress for a given fatigue life. In this case, it is not necessary to undertake tests at cyclic strain amplitudes or cyclic stress amplitudes where the fatigue life approaches infinity.

The values selected in accordance with 8.3 for the cyclic loading amplitudes are used together with the nominal dimensions of the test piece to calculate the cyclic strain amplitude, γ , and cyclic stress amplitude, τ , in megapascals, using the formulae

$$\gamma = \frac{s}{h} = \frac{s}{h_0 - h_r}$$

where

s is the transverse deformation, in millimetres;

h_0 is the height of the test piece, in millimetres (20 or 38);

h_r is the static compression, in millimetres;

and


$$\tau = \frac{Q}{A}$$

where

Q is the transverse force, in newtons;

A is the cross-sectional area, in square millimetres, of the test piece.

This simplified evaluation method is applicable, since the permitted tolerances for the dimensions of the test piece are fixed very closely. The method makes possible the direct plotting of the fatigue-life curve from values of Q , in newtons, and s , in millimetres.

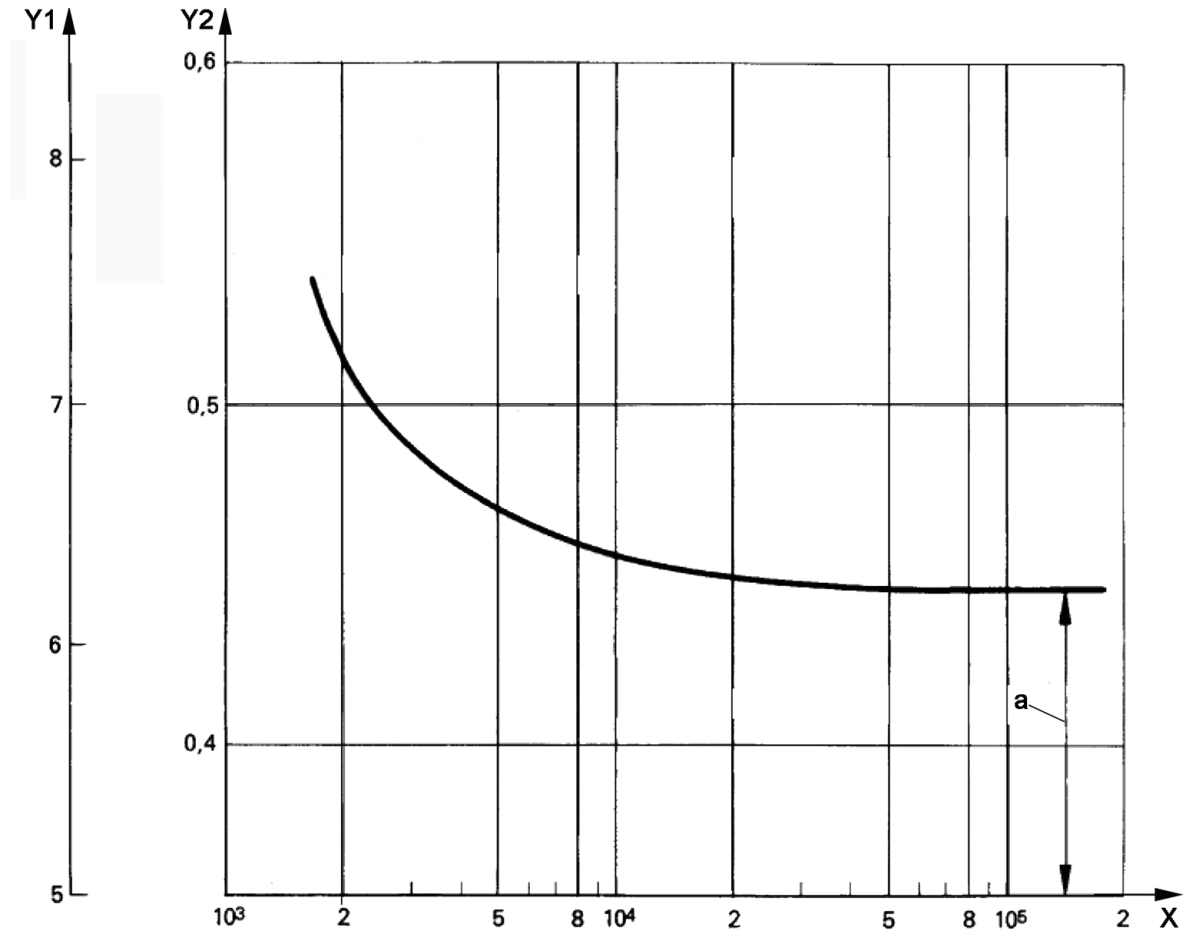**Key**

- X number of loading cycles, N
- Y_1 transverse cyclic deformation (mm)
- Y_2 cyclic strain amplitude, γ
- ^a Limiting fatigue deformability, γ_∞ .

Figure 3 — Example of fatigue-life curve with predetermined cyclic deformation

10 Test report

The test report shall include the following particulars:

- a) sample details:
 - 1) a full description of the sample and its origin,
 - 2) compound details and cure details, where appropriate,
 - 3) the method of preparation of the test piece from the sample, for example whether moulded or cut or taken from finished products;
- b) test method:
 - 1) a full reference to the test method used, i.e. the number of this International Standard (ISO 4666-2),
 - 2) the test procedure used,
 - 3) the original height of the test piece and, in the case of deviation from the standard dimensions, the diameter,
 - 4) the type of chuck or cap;
- c) test details:
 - 1) the number of test pieces used,
 - 2) the standard laboratory temperature,
 - 3) the time and temperature of conditioning prior to test,
 - 4) the pre-strain (or static axial compression, in millimetres),
 - 5) the pre-stress, in megapascals (or static axial force, in newtons),
 - 6) the cyclic strain amplitude (or cyclic transverse deformation, in millimetres),
 - 7) the cyclic stress amplitude, in megapascals (or cyclic force, in newtons),
 - 8) the rotational frequency, in hertz;
- d) test results:
 - 1) for the measurement of temperature rise: the test duration, the individual values (in degrees Celsius) and the mean value (in degrees Celsius),
 - 2) for determinations of fatigue life: the individual values of the measured number of cycles to breakdown, N , and the arithmetical averages calculated therefrom,
 - 3) the confidence limits of the mean values, if an adequate number of test pieces have been tested,
 - 4) if a fatigue-life curve has been plotted: the fatigue deformability or limiting fatigue deformability and the fatigue stress or limiting fatigue stress, as appropriate;
- e) any departures from the procedures specified in this part of ISO 4666;
- f) the date of the test.

Bibliography

- [1] KAINRADL, P., WOLF, F. and ECKER, H. Fatigue tests on vulcanizates in the rotary flexometer, *Gummi, Asbest, Kunststoffe*, **24** (1971), pp. 578 and 686
- [2] KAINRADL, P., WOLF, F. and ECKER, H. Variations in testing procedures on the rotary flexometer, *Rubber Chemistry and Technology*, **49** (1976), pp. 258-277

