

---

---

**Laboratory glassware — Graduated  
measuring cylinders**

*Verrerie de laboratoire — Éprouvettes graduées cylindriques*



Reference number  
ISO 4788:2005(E)

© ISO 2005

**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

© ISO 2005

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 4788 was prepared by Technical Committee ISO/TC 48, *Laboratory glassware and related apparatus*, Subcommittee SC 6, *Laboratory and volumetric ware*.

This second edition cancels and replaces the first edition (ISO 4788:1980), which has been technically revised to incorporate the following changes:

- a) three types of graduated measuring cylinders have been specified;
- b) two classes of accuracy have been introduced;
- c) cylinders of squat form have been added;
- d) marking of cylinders has been changed;
- e) capacity at lowest graduation line for 5 ml and 10 ml cylinders has been increased.

## Introduction

The first edition of this International Standard (ISO 4788:1980) was originally written when the use of measuring cylinders was largely limited to the approximate dispensing of reagents in wet chemical analytical procedures; only one grade of accuracy was specified.

More recently, with the increasing demand for accreditation and changing uses to which measuring cylinders are put, a significant demand has emerged worldwide for a more accurate class to complement the originally specified range.

Also, with more work being carried out in laminar-flow cabinets, glove boxes and fume extraction hoods, in which working heights are restricted, a need for short (squat) measuring cylinders has emerged.

This International Standard addresses these two needs, and has been prepared to meet the requirements of ISO 384. This International Standard includes

- a) spouted measuring cylinders of traditional (tall) form, accuracy classes A and B,
- b) stoppered measuring cylinders of traditional (tall) form, accuracy classes A and B, and
- c) spouted measuring cylinders of squat form, accuracy class B.

Class A has been considered for the third type (squat cylinders) but discounted because ISO 384 requirements would only be met by cylinders having manufacturing specifications which would be virtually impossible to satisfy.

# Laboratory glassware — Graduated measuring cylinders

## 1 Scope

This International Standard specifies dimensions, material and constructional and metrological requirements of graduated measuring cylinders of tall form (Type 1a and Type 1b) and of squat form (Type 2). All types are suitable for general laboratory use.

The specifications in this International Standard are in conformity with the principles of design and construction of volumetric glassware given in ISO 384.

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 384:1978, *Laboratory glassware — Principles of design and construction of volumetric glassware*

ISO 719, *Glass — Hydrolytic resistance of glass grains at 98 °C — Method of test and classification*

ISO 4787, *Laboratory glassware — Volumetric glassware — Methods for use and testing of capacity*

## 3 Basis of adjustment

### 3.1 Unit of volume

The unit of volume shall be the millilitre (ml), which is equivalent to the cubic centimetre (cm<sup>3</sup>).

### 3.2 Reference temperature

The standard reference temperature, i.e. the temperature at which the cylinder is intended to contain its nominal capacity, shall be 20 °C.


When the cylinder is required for use in a country which has adopted a standard reference temperature of 27 °C; however, this value shall be substituted for 20 °C.

## 4 Types and classes of accuracy

### 4.1 Types

The following three types of graduated measuring cylinders are specified (see Figure 1):

- a) tall form with spouted neck — Type 1a;
- b) tall form with stoppered neck — Type 1b;
- c) squat form with spouted neck — Type 2.

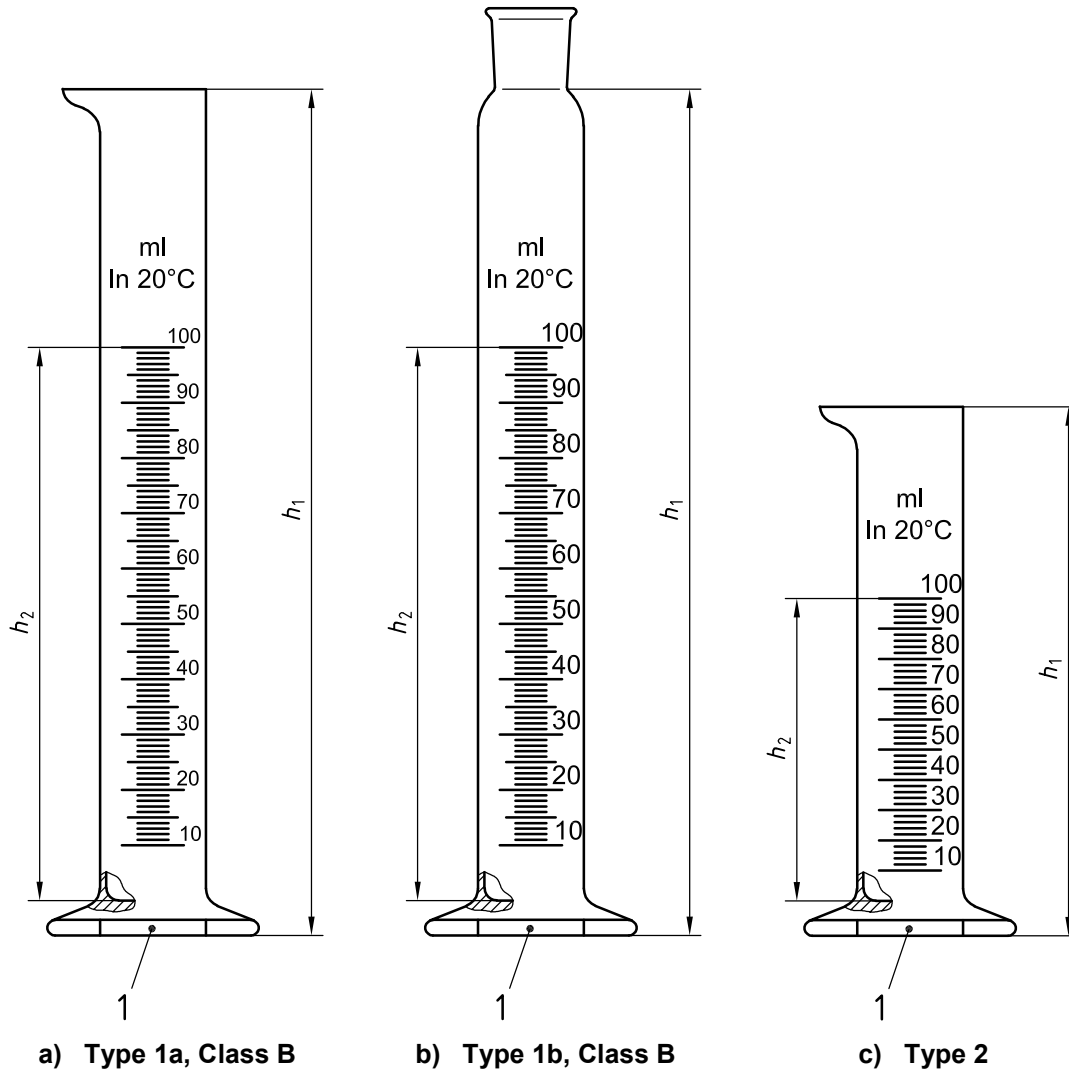

#### Key

- $h_1$  overall height
- $h_2$  internal height to highest graduation line
- 1 hexagonal or circular base

**Figure 1 — General forms of graduated measuring cylinders**

### 4.2 Classes of accuracy

Two classes of accuracy are specified:

- a) Class A for the higher grade (Type 1a and Type 1b only);
- b) Class B for the lower grade.

## 5 Series of capacities and dimensions

The three types of cylinder shall have a series of nominal capacities as shown in Table 1 and Table 2. If cylinders of capacities other than those listed below are required, it is recommended that they conform, as far as possible, to the essential requirements of this International Standard.

**Table 1 — Dimensions, subdivisions and limits of error for Type 1 (a and b) cylinders**

Nominal capacity ml	Overall height $h_1$ mm max.	Distance from top of scale to top of cylinder mm min.	Internal height to highest graduation line $h_2$ mm min.	Sub-divisions ml	Capacity at lowest graduation line ml max.	Max. permissible error $\pm$ ml	
						Class A	Class B
5	115	20	55	0,1	1,0	0,05	0,1
10	140	20	65	0,2	1,4	0,1	0,2
25	170	25	85	0,5	2,5	0,25	0,5
50	200	30	110	1	5	0,5	1
100	260	35	145	1	10	0,5	1
250	335	40	200	2	26	1	2
500	390	45	250	5	50	2,5	5
1000	470	50	310	10	100	5	10
2000	570	50	380	20	200	10	20

**Table 2 — Dimensions, subdivisions and limits of error for Type 2 cylinders**

Nominal capacity ml	Overall height $h_1$ mm max.	Distance from top of scale to top of cylinder mm min.	Internal height to highest graduation line $h_2$ mm min.	Sub-divisions ml	Capacity at lowest graduation line ml max.	Max. permissible error <sup>a</sup> $\pm$ ml
5	80	25	30	0,5	1	0,2
10	100	30	40	1	2	0,3
25	125	30	65	1	5	0,5
50	150	30	90	1 or 2	10	1
100	170	35	90	2	12	1
250	220	35	125	5	30	2
500	255	50	160	10	60	5
1000	295	50	190	20	100	10
2000	345	50	240	50	200	20

<sup>a</sup> These maximum permissible errors correspond to accuracy Class B in accordance with ISO 384.

## 6 Definition of capacity

The capacity of a graduated measuring cylinder is defined as the volume of water at 20 °C, expressed in millilitres, contained by the cylinder when filled to the highest graduation line. Where, exceptionally, the reference temperature is 27 °C, this value shall be substituted for 20 °C.

Setting the meniscus shall be performed according to ISO 4787.

The meniscus is set so that the plane of the top edge of the graduation line is horizontally tangential to the lowest point of the meniscus, the line of sight being in the same plane.

## 7 Maximum permissible error

Maximum permissible errors in capacity shall not exceed the values specified in Table 1 for Type 1 cylinders, and in Table 2 for Type 2 cylinders.

These errors represent the maximum permissible error at any point on the scale, and also the maximum permissible difference between the errors at any two points.

## 8 Material

The cylinders shall be manufactured from glass of hydrolytic class not lower than HGB3 in accordance with ISO 719. The glass shall be as free as possible from visible defects, and steps shall be taken in manufacture to ensure that it is reasonably free from internal stress.

## 9 Construction and form

### 9.1 Wall thickness

The cylinders shall be sufficiently robust in construction to withstand usual laboratory usage, and the wall thickness shall show no gross departure from uniformity.

### 9.2 Stability

The cylinders shall stand vertically without rocking or spinning when placed on a level surface. They shall not topple when placed empty (without stopper, if provided) on a surface inclined at an angle of 15° to the horizontal.

### 9.3 Base

The base may be integral, of glass, or it may be detachable, of a suitable plastics or other material, and may be either hexagonal or of other form provided the cylinder satisfies the requirements of 9.2.

### 9.4 Rim and spout

**9.4.1** The rim of the cylinder shall be fire-polished and shall lie in a plane at right angles to the axis of the cylinder.

**9.4.2** The spout of a Type 1a spouted cylinder shall be so formed as to enable the contents of the cylinder to be poured out in a narrow stream without spilling or running down the outside of the cylinder.

### 9.5 Neck and stopper

On a Type 1b stoppered cylinder, the neck shall be ground to a suitable socket size, preferably selected from ISO 383.

A well-fitting stopper of glass or suitable inert plastics material shall be supplied. If individually ground stoppers are supplied, each stopper, and the cylinder it fits, shall be marked with an identification number.

### 9.6 Dimensions

Type 1 (a and b) cylinders shall comply with the dimensional requirements given in Table 1. In the case of a stoppered cylinder, the "overall height" shall be considered to be the height to the base of the ground neck (see Figure 1, Type 1b).

Type 2 cylinders shall comply with the dimensional requirements given in Table 2.



## 10 Graduation and figuring

### 10.1 Graduation

The graduation of all cylinders within this specification shall be in accordance with ISO 384:1978, Clause 9, Graduation pattern II in the case of Class A cylinders and Graduation pattern III in the cases of Class B and Type 2 measuring cylinders.

### 10.2 Figuring

Figuring shall be in accordance with ISO 384:1978, 10.4.

## 11 Accuracy testing

Testing of capacity and accuracy shall be performed in accordance with ISO 4787.

## 12 Marking

12.1 The following shall be permanently marked on each cylinder:

- a) number indicating the nominal capacity;
- b) the symbol “ml” or “cm<sup>3</sup>” to indicate the unit of volume;  
The 1 000 ml and 2 000 ml cylinders may, if desired, be inscribed in terms of the litre in place of the millilitre.
- c) the inscription “20 °C” to indicate the standard reference temperature (but see 3.2 for a reference temperature of 27 °C);
- d) the abbreviation “In” to indicate that the cylinder has been adjusted to contain its indicated capacity;
- e) for Type 1a and Type 1b cylinders, the letter “A” or “B” to indicate the class of accuracy and the tolerance in accordance with Table 1;
- f) the maker's or vendor's name or mark;
- g) in the case of a cylinder with an interchangeable stopper (Type 1b), the size number of the joint shall be marked;
- h) the type of glass material, in accordance with Clause 8.

The permanence of marking may be assessed by the test methods specified in ISO 4794.

12.2 An individual identification number shall be permanently marked on each Class A cylinder intended for official verification or certification, or on the stopper and cylinder in all cases where stoppers are individually ground to fit only one cylinder.

## 13 Visibility of graduation lines, figures and marking

13.1 All figures and marking shall be of such size and form as to be clearly legible under usual conditions of use.

13.2 The graduation lines, the figures and the marking shall be clearly visible and permanent, under usual conditions of use.

## Bibliography

- [1] ISO 383, *Laboratory glassware — Interchangeable conical ground joints*
- [2] ISO 4794, *Laboratory glassware — Methods for assessing the chemical resistance of enamels used for colour coding and colour marking*



.....

---

---

**ICS 17.060**

Price based on 6 pages