

# INTERNATIONAL STANDARD

# ISO 5302

First edition  
2003-07-15

---

---

## Vacuum technology — Turbomolecular pumps — Measurement of performance characteristics

*Technique du vide — Pompes turbomoléculaires — Mesurage des  
caractéristiques fonctionnelles*



Reference number  
ISO 5302:2003(E)

© ISO 2003

**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

© ISO 2003

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

Foreword.....	iv
<b>1</b> <b>Scope</b> .....	<b>1</b>
<b>2</b> <b>Normative references</b> .....	<b>1</b>
<b>3</b> <b>Terms and definitions</b> .....	<b>1</b>
<b>4</b> <b>Symbols and abbreviated terms</b> .....	<b>3</b>
<b>5</b> <b>Apparatus for volume flow rate (pumping speed) measurement</b> .....	<b>3</b>
<b>5.1</b> <b>Test dome for the throughput method: Inlet pressures &gt; 10<sup>-4</sup> Pa (10<sup>-6</sup> mbar)</b> .....	<b>3</b>
<b>5.2</b> <b>Test dome for the standard conductance method: Inlet pressures &lt; 10<sup>-4</sup> Pa (10<sup>-6</sup> mbar)</b> .....	<b>4</b>
<b>5.3</b> <b>Pressure gauges</b> .....	<b>4</b>
<b>6</b> <b>Test methods and procedures</b> .....	<b>5</b>
<b>6.1</b> <b>Principle</b> .....	<b>5</b>
<b>6.2</b> <b>Measurement of partial pressures</b> .....	<b>5</b>
<b>6.3</b> <b>Size of backing pump</b> .....	<b>5</b>
<b>6.4</b> <b>Volume flow rate (pumping speed)</b> .....	<b>6</b>
<b>6.5</b> <b>Methods of measurement of volume flow rate (pumping speed)</b> .....	<b>6</b>
<b>6.6</b> <b>Test procedures</b> .....	<b>7</b>
<b>6.7</b> <b>Maximum throughput</b> .....	<b>10</b>
<b>6.8</b> <b>Critical backing pressure</b> .....	<b>10</b>
<b>6.9</b> <b>Minimum operational pressure</b> .....	<b>10</b>
<b>6.10</b> <b>Compression ratio</b> .....	<b>11</b>
<b>6.11</b> <b>Vibration</b> .....	<b>12</b>
<b>7</b> <b>Test report: Additional parameters</b> .....	<b>13</b>
<b>Annex A</b> (informative) <b>Derivation of Equations (1) and (2)</b> .....	<b>14</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 5302 was prepared by Technical Committee ISO/TC 112, *Vacuum technology*, Subcommittee SC 3, *Vacuum pumps — Performance*.

# Vacuum technology — Turbomolecular pumps — Measurement of performance characteristics

## 1 Scope

This International Standard specifies methods for the measurement of performance characteristics of turbomolecular pumps. It is applicable to all sizes and all types of turbomolecular pumps

- a) with mechanical or magnetic bearings, and
- b) with or without an additional drag stage.

**NOTE** Since turbomolecular pumps are backed by primary pumps, their performance cannot be completely defined without having the following in addition to the curve of the volume flow rate against suction pressure:

- the throughput curve,
- the compression ratio curve, and
- the curve for the variation in inlet pressure,

over the whole of the range concerned and for various gases.

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3529-2, *Vacuum technology — Vocabulary — Part 2: Vacuum pumps and related terms*

## 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 3529-2 and the following apply.

### 3.1 critical backing pressure

$p_c$   
maximum backing pressure  $p_2$  while the pump still has a compression rate  $p_2/p_1 \geq 2$  and the purge gas flow is on

**NOTE**  $p_1$  is the (high) vacuum pressure on inlet.

**3.2**  
**maximum throughput**

$Q_{\max}$   
highest gas load, in pascal litres per second (Pa·l/s) [millibar litres per second (mbar·l/s)], that can be pumped continuously without damage or destruction of the pump

NOTE The limiting parameter depends on the design of the pump. In most cases it will be given as a maximum temperature at a defined location. The value of  $Q_{\max}$  depends on the gas pumped, the backing pump used, and the conditions of cooling, etc.

**3.3**  
**volume flow rate**

$q_V$   
volume of gas which, under ideal conditions, flows from the test dome through the pump inlet per unit time

NOTE 1 For practical reasons, however, the volume flow rate of a given pump and for a given gas is conventionally taken as equal to the quotient of the throughput of this gas and of the equilibrium pressure at a given point. The units adopted for the volume flow rate are cubic metres per hour (m<sup>3</sup>/h) or litres per second (l/s).

NOTE 2 The term "pumping speed" and symbol "S" are sometimes used instead of "volume flow rate".

**3.4**  
**ultimate pressure**  
value towards which the pressure in the test dome approaches asymptotically

NOTE 1 It is the lowest pressure obtainable with the pump.

NOTE 2 It is recommended not to give ultimate pressure values in the manufacturer's specification. Therefore, no procedure to measure the ultimate pressure is given in this International Standard. However, if the manufacturer lists the ultimate pressure, the operating conditions under which the measurement is made should be stated.

**3.5**  
**minimum operational pressure**

$p_0$   
pressure obtained in the dome 48 h after the bake-out procedure

**3.6**  
**compression ratio**  
 $K_{\text{eff}}$   
ratio of the backing pressure  $p_2$  to the inlet pressure  $p_1$  of the turbomolecular pump

$$K_{\text{eff}} = p_2/p_1$$

NOTE To obtain the compression rate at zero flow rate,  $K_0$ , for a given gas, the partial pressure of this gas in the outlet duct should be at least 90 % of  $p_2$ .

**3.7**  
**maximum working pressure**

$p_{1\max}$   
highest pressure on the inlet side that the turbomolecular pump and the driving device can withstand without being damaged

## 4 Symbols and abbreviated terms


Symbol	Designation	Unit
$C$	conductance	$\text{m}^3/\text{s}$ ( $=10^3$ l/s)
$d$	orifice diameter	m
$D$	nominal diameter of test dome	m
$K_{\text{eff}}$	compression ratio of vacuum pump	—
$K_{\text{eff,a}}, K_{\text{eff,b}}$	special values of compression ratio	—
$K_0$	compression ratio at zero throughput	—
$L$	thickness of orifice wall	m
$M$	molecular mass of gas	kg/mol
$p_0$	minimum operational pressure on inlet	Pa (or mbar)
$p_1$	(high) vacuum pressure on inlet	Pa (or mbar)
$p_{1\text{max}}$	maximum working pressure on inlet	Pa (or mbar)
$p_2$	vacuum pressure in backing line	Pa (or mbar)
$p_a, p_b$	special values of pressure	Pa (or mbar)
$p_c$	critical backing pressure	Pa (or mbar)
$Q$	throughput of vacuum pump	Pa·l/s (or mbar·l/s)
$Q_0$	leakage gas load	Pa·l/s (or mbar·l/s)
$Q_T$	test gas load	Pa·l/s (or mbar·l/s)
$Q_{\text{max}}$	maximum throughput	Pa·l/s (or mbar·l/s)
$Q_1, Q_2$	special values of throughput	Pa·l/s (or mbar·l/s)
$R$	ideal gas constant	N·m/mol·K
$q_V$	volume flow rate	l/s
$q_{V0}$	volume flow rate at $K_{\text{eff}} = 1$	l/s
$q_{VB}$	volume flow rate of backing pump	l/s
$q_{Vx}$	maximum expected volume flow rate (see 6.3)	l/s
$T$	absolute temperature	K

## 5 Apparatus for volume flow rate (pumping speed) measurement

### 5.1 Test dome for the throughput method: Inlet pressures $> 10^{-4}$ Pa ( $10^{-6}$ mbar)

For these measurements, use a test dome as shown in Figure 1 with the same nominal diameter  $D$  as that of the pump inlet. The face of the dome opposite the inlet flange may be flat, conical or slightly curved with the same average height above the flange as the flat face. The test dome shall be fitted with a device for bake-out ensuring uniform heating of the dome to achieve the minimum operational pressure.

For pumps with an inlet flange diameter less than the nominal diameter DN 100, the diameter of the dome shall correspond to DN 100. The transition to the pump inlet flange shall be made through a  $45^\circ$  taper fitting as short as possible according to Figure 1.

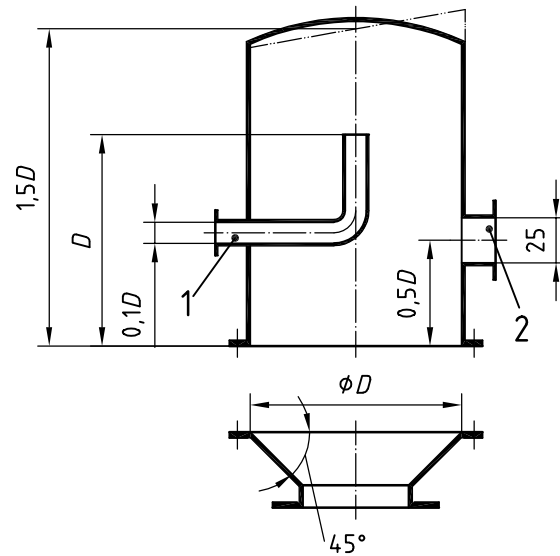**Key**

- 1 gas inlet
- 2 vacuum gauge connection

**Figure 1 — Test dome****5.2 Test dome for the standard conductance method: Inlet pressures  $< 10^{-4}$  Pa ( $10^{-6}$  mbar)**

The test dome shall be cylindrical and of the shape shown in Figure 2. The dome shall be fitted with a device for bake-out that ensures uniform heating of the dome to achieve the minimum operational pressure.

The diameter of the thin wall orifice plate shall be chosen according to the expected flow rate and shall be such that the ratio of the pressures measured at  $p_a$  and  $p_b$  lies between 3 and 50. Care shall be taken to ensure that at the inlet pressure  $p_1$  the mean free path of the gas particles is not smaller than the orifice diameter  $d$ .

For pumps with an inlet flange diameter less than the nominal diameter DN 100, the diameter of the dome shall correspond to DN 100. Then the transition to the pump inlet flange shall be made through a 45° taper fitting according to Figure 1.

For pumps with an inlet flange diameter greater than DN 100, the nominal diameter  $D$  of the dome shall be equal to the actual diameter of the inlet flange.

**5.3 Pressure gauges**

Total pressure measurements shall be made using pressure gauges calibrated to within 5 % accuracy for pressures greater than  $10^{-4}$  Pa ( $10^{-6}$  mbar), or within 10 % for pressures less than this value.

It is recommended that after completion of the tests, the calibration of the vacuum gauge(s) is checked, for example by comparison with a reference gauge *in situ*.

With the test dome (5.2), the pressure gauge agreement may be ensured by fitting at B a gas admission pipe leading to the pump orifice in the lower part of the dome (see Figure 2). The adjustable valve for gas admission in this pipe line shall be opened so as to obtain approximately the desired pressure. After stabilization, the pressure gauges at the points shown shall give the same readings ( $p_a$  and  $p_b$ ). If not, the required correction can be deduced.



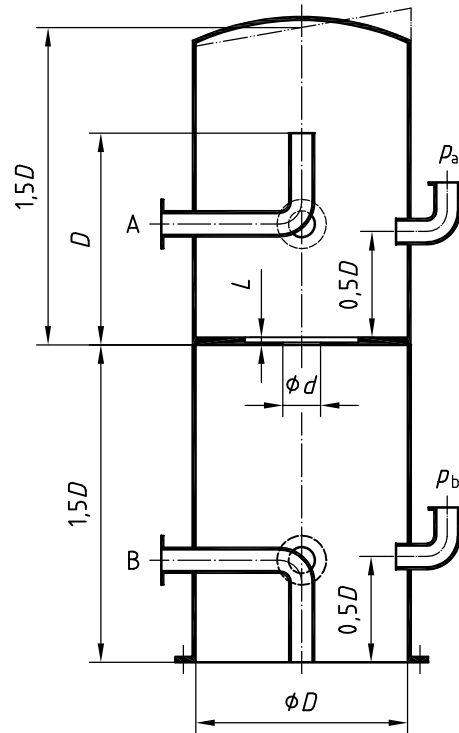


Figure 2 — Test dome

## 6 Test methods and procedures

### 6.1 Principle

Measurements are made with 99,9 % (by mass) pure test gas: nitrogen, hydrogen, helium and argon.

### 6.2 Measurement of partial pressures

For measurements of backing pressure, a pressure gauge with a trap may be used. For measurements of inlet pressure, a partial pressure gas analyser supplemented by a total pressure gauge may be used.

Partial pressure gas analysers used at the pump inlet shall have sufficient resolving power in the mass range from 1 to 100.

### 6.3 Size of backing pump

The effective volume flow rate,  $q_V$ , of a turbomolecular pump depends on the volume flow rate  $q_{V0}$  at zero pressure difference ( $p_1 = p_2$ ), the compression ratio  $K_0$  at zero rate of throughput ( $Q = 0$ ) and the volume flow rate  $q_{VB}$  of the backing pump according to the relationship

$$q_V = q_{V0} \left( \frac{K_0 - q_V/q_{VB}}{K_0 - 1} \right) \quad (1)$$

which may be solved to give

$$q_V = \frac{q_{V0}}{1 - 1/K_0 + q_{V0}/(K_0 \cdot q_{VB})} \quad (2)$$

See Annex A for the derivation of these equations.

For small values of  $K_0$  (e.g. for hydrogen,  $K_0 \approx 1\,000$ ), the volume flow rate of the turbomolecular pump is influenced by the size of the backing pump. This influence may be regarded as small if a backing pump is used with a volume flow rate  $q_{VB}$  deduced from

$$\frac{q_{VX}}{q_{VB}} < 0,05 K_0 \quad \text{or} \quad q_{VB} > 20 \left( \frac{q_{VX}}{K_0} \right) \quad (3)$$

for the whole pressure range, where  $q_{VX}$  is the expected maximum volume flow rate of the turbomolecular pump.

From Equation (3), the choice of a suitable backing pump may be made for a gas with known value of  $K_0$  from the specification of the turbomolecular pump.

#### 6.4 Volume flow rate (pumping speed)

Under ideal conditions, the volume flow rate is the volume of gas which flows from the test dome through the pump inlet per unit time. For practical reasons, however, the volume flow rate of a given pump and for a given gas is conventionally taken as equal to the quotient of the throughput of this gas and of the equilibrium pressure at a given location.

The units adopted for the volume flow rate  $q_V$  are cubic metres per hour ( $\text{m}^3/\text{h}$ ) or litres per second ( $\text{l/s}$ ).

#### 6.5 Methods of measurement of volume flow rate (pumping speed)

##### 6.5.1 Method for inlet pressures $> 10^{-4}$ Pa ( $10^{-6}$ mbar): Throughput method

The method adopted for the measurement of the volume flow rate  $q_V$  is the steady pressure method for which the gas throughput,  $Q$ , is measured outside the dome. If the pressure  $p_1$  in the test dome, which is measured by a vacuum gauge in the determined area (Figure 1), is held constant, the volume flow rate  $q_V$  is obtained by the relationship

$$q_V = \frac{Q}{p_1 - p_0} \quad (4)$$

where  $p_0$  is the minimum operational pressure in the test dome (see 6.9).

This pressure limit may be shifted to lower pressures, if the accuracy of the flow meter is appropriate.

##### 6.5.2 Method for inlet pressures $< 10^{-4}$ Pa ( $10^{-6}$ mbar): Standard conductance method

The method adopted for the measurement of the volume flow rate  $q_V$  is the steady pressure method known as "standard conductance" method, in which a thin orifice plate divides the test dome (Figure 2) into two volumes. If pressure is measured in each volume by pressure gauges having the same sensitivity, the volume flow rate is then given by

$$q_V = C \left( \frac{p_a - p_{0a}}{p_b - p_{0b}} - 1 \right) \quad (5)$$

where  $C$  is the calculated conductance, taking account of the orifice size and the gas properties. Pressures  $p_{0a}$  and  $p_{0b}$  are measured inside the dome before admission of the gas. The conductance of the orifice with diameter  $d$  and thickness  $L$  may be calculated using the following formula:

$$C = \sqrt{\frac{\pi RT}{32M}} \left( \frac{1}{1 + L/d} \right) d^2 \quad (6)$$

The term  $1/(1 + L/d)$  is a correction factor that can be defined as the average throughput probability.

The formula shall be applied with consistent units. Special values such as

$$R = 8,314 \text{ N} \cdot \text{m}/(\text{mol} \cdot \text{K})$$

$$M_{\text{air}} = 28,8 \times 10^{-3} \text{ kg/mol}$$

$$T = 293 \text{ K} = 20 \text{ }^\circ\text{C}$$

will give

$$C_{\text{air}} = 91 d^2 / (1 + L/d) \text{ m}^3/\text{s}$$

or

$$C_{\text{air}} = 91000 d^2 / (1 + L/d) \text{ l/s}$$

where  $L$  and  $d$  are measured in metres.

## 6.6 Test procedures

### 6.6.1 Procedure for the throughput method: Inlet pressures $> 10^{-4}$ Pa ( $10^{-6}$ mbar)

The arrangement of the measuring equipment with the test dome from Figure 1 is given in Figure 3. First, with valve 5 closed, the minimum operational pressure shall prevail in the test dome (see 3.4). Then gas is admitted to the test dome through the adjustable valve 5. Measurements are made with increasing pressures from a threshold value allowing the correct use of the throughput meter 6.

When the required pressure is obtained, wait for at least 5 min. Then measure the pressure, temperature, barometric pressure and either the admitted volume flow rate (when using a flow meter) or the displaced gas volume and time (when using a calibrated burette). If the flow rate remains steady to within  $\pm 1\%$  for the subsequent 5 min, the measurement at this point may be regarded as valid. If the flow rate is unsteady due to a transient condition, wait until it stabilizes.

If the throughput measurement lasts for more than 60 s, the pressure  $p_1$  in the dome shall be noted at least every minute. If during measurement the pressure varies by more than  $\pm 1\%$ , the measurement shall be repeated until the readings are stable. Then the throughput is the average of the measured values.

Measurement at three points per pressure decade shall be made up to a value  $p_1$  where the ratio  $p_2/p_1$  becomes 2, or

$$p_2 = 2 p_1 \tag{7}$$

### 6.6.2 Procedure for the standard conductance method: Inlet pressures $< 10^{-4}$ Pa ( $10^{-6}$ mbar)

The arrangement of the measuring equipment is given in Figure 4. First, with all valves closed, the minimum operational pressure shall prevail in the test dome (see 6.9). Then the gas is admitted to the test dome through the adjustable valve 5. Take measurements with increasing pressures, beginning from a threshold value of twice that of the minimum operational pressure. When the required pressure  $p_1$  is obtained and remains stable for the following 5 min to within  $\pm 5\%$ , this point may be regarded as valid.


If pressure is unsteady due to a transient condition, wait until it stabilizes. Measure the pressures  $p_a$  and  $p_b \equiv p_1$  together with the backing pressure  $p_2$ , and the temperature. If during this measurement one of the pressures varies by more than  $\pm 5\%$ , the measurement shall be repeated until stability is obtained. Then the throughput is calculated from the average of the measured values.

Take measurements at three points per pressure decade made up to  $p_b = 1 \times 10^{-3}$  Pa ( $1 \times 10^{-5}$  mbar), or to a pressure at which the mean free path of the gas molecules in the upper part of the test dome becomes less than  $2d$ , where  $d$  is the diameter of the orifice.

If the measurement of the volume flow rate is to be continued to higher pressures, the procedure given in 6.6.1 shall be applied.

**6.6.3 Evaluation of measurement**


Plot the volume flow rate  $q_V$  of the turbomolecular pump against the inlet pressure ( $p_1 = p_b$ ) in a semi-logarithmic graph (Figure 5). Then plot the volume flow rate  $q_{VB}$  measured at the outlet of the turbomolecular pump against  $p_2$  on the same graph so as to show the type of the backing pump. The range of abscissa shall cover the whole range of pressures  $p_1$  and  $p_2$ . The minimum operational pressures of the turbomolecular pump and of the backing pump shall be indicated.

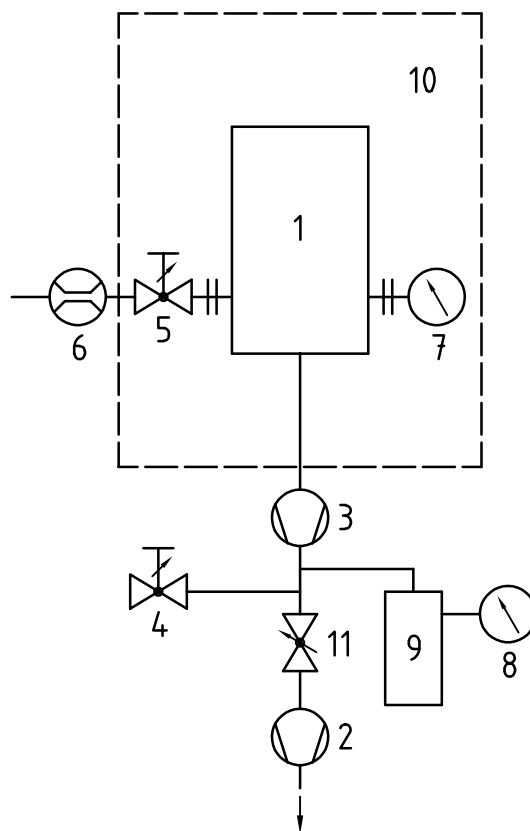

**Key**

- |                       |                                  |
|-----------------------|----------------------------------|
| 1 test dome           | 7 vacuum gauge (measures $p_1$ ) |
| 2 backing pump        | 8 vacuum gauge (measures $p_2$ ) |
| 3 turbomolecular pump | 9 cold trap                      |
| 4 gas inlet valve     | 10 heating jacket                |
| 5 gas inlet valve     | 11 conductance valve             |
| 6 throughput meter    |                                  |


**Figure 3 — Arrangement for measurement of volume flow rate (pumping speed) for throughput method**

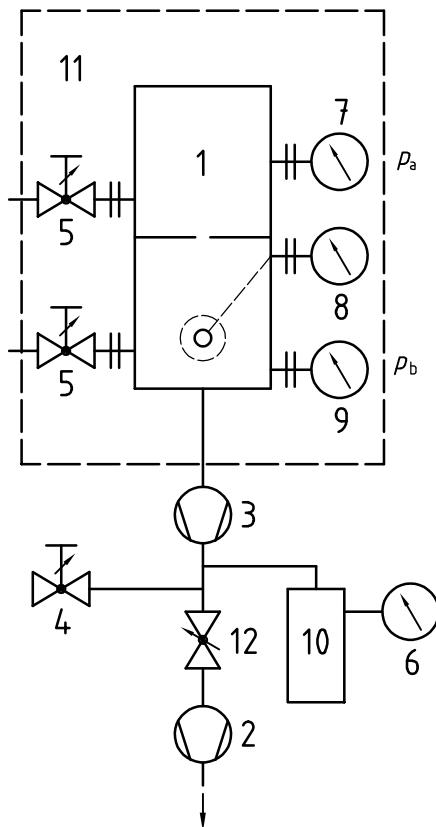

**Key**

- |                                  |                                  |
|----------------------------------|----------------------------------|
| 1 test dome                      | 7 vacuum gauge (measures $p_a$ ) |
| 2 backing pump                   | 8 vacuum gauge (measures $p_b$ ) |
| 3 turbomolecular pump            | 9 residual gas analyser          |
| 4 gas inlet valve                | 10 cold trap                     |
| 5 gas inlet valves               | 11 heating jacket                |
| 6 vacuum gauge (measures $p_2$ ) | 12 conductance valve             |

**Figure 4 — Arrangement for measurement of volume flow rate (pumping speed) for standard conductance method**

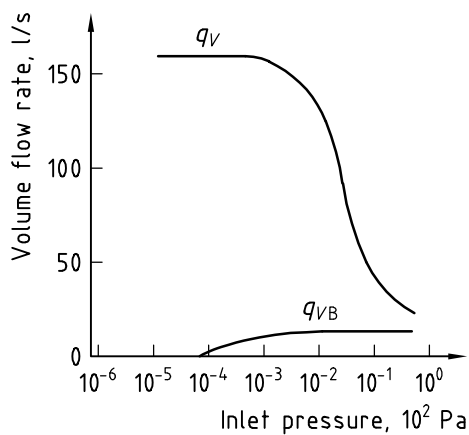

**Figure 5 — Example of volume flow rate (pumping speed) curve**

## 6.7 Maximum throughput

### 6.7.1 Measurement method

For at least two sizes of backing pump, measure the throughput  $Q$  as a function of the backing pressure  $p_2$  while the pump is operated under conditions as specified by the manufacturer. The test dome shown in Figure 1 shall be used. Suitable sensors should be provided to monitor the limiting parameter(s) (see Note in 3.2). When the maximum throughput  $Q_{\max}$  is reached, all monitored values shall become stable and shall not exceed the prescribed limit for a minimum time of 4 h. One of the backing pumps should preferably be smaller than the other, with a throughput as proposed by the manufacturer, and the other pump much larger (about 5 to 10 times).

This procedure is intended to verify the data given by the pump manufacturer and so it is non-destructive. However, it shall not be used to find the limit.

### 6.7.2 Test procedure

Connect the pump to the test dome (5.1), which is able of establishing a constant gas flow and of measuring the inlet pressure  $p_1$ . The backing line is equipped with a vacuum gauge to measure the backing pressure  $p_2$ . Increase the gas load on the high vacuum side stepwise. The readings of the sensors be stable before they are recorded. If one sensor reading passes the prescribed limit, close the gas inlet valve and the test shall be regarded as failed. With the maximum throughput  $Q_{\max}$ , the test shall run for a minimum time of 4 h with all readings well within the limits.

## 6.8 Critical backing pressure

### 6.8.1 Measurement method

By admitting test gas into the backing line, increase the backing pressure  $p_2$  and set it to a value where a compression ratio of  $K_{\text{eff}} = p_2/p_1 = 2$  is measured. Then this backing pressure  $p_2$  is the critical backing pressure  $p_c$ .

Use the apparatus shown in Figure 3, which is capable of establishing a constant gas flow and of measuring the inlet pressure  $p_1$ . The backing line is equipped with a second gas inlet (valve 4 in Figure 3) and a vacuum gauge to measure the backing pressure  $p_2$ . The backing pump used shall be able to handle twice the test gas load at the expected pressure  $p_2 = p_c$ .

### 6.8.2 Test procedure

Prior to the admission of gas, a steady-state pressure  $p_0 < 10^{-2}$  Pa ( $10^{-4}$  mbar) shall be established in the test dome from which a leakage gas load of  $Q_0 < p_0 \times q_{V0}$  can be deduced.

Then with a constant test gas load  $Q_T$ , increase the pressure  $p_2$  in the backing line by admitting the test gas into it. Record the pressures  $p_1$  and  $p_2$ ; they shall be stable to within 10 % over a time interval of > 15 min.

Depending on the type of pump, it is possible to make this measurement at two different values for  $p_2$ . If for  $p_{2a}$  the measured  $K_{\text{eff},a}$  is  $1,5 < K_{\text{eff},a} < 2$ , and with  $p_{2b}$  the measured  $K_{\text{eff},b}$  is  $2 < K_{\text{eff},b} < 4$ , the pressure  $p_c$  may be interpolated from these two values  $p_{2a}$  and  $p_{2b}$ .

## 6.9 Minimum operational pressure

### 6.9.1 Operating conditions

The operating conditions of the turbomolecular pump are those given by the manufacturer (rotational speed, quantity and quality of lubrication fluid, etc.). The ambient temperature shall be between 15 °C and 25 °C during the whole test procedure. After the specified bake-out procedure (see 6.9.2 or 6.9.3), the apparatus shall be at a stable temperature to within  $\pm 3$  °C.

Use the apparatus from Figure 3 for this test.

### 6.9.2 Test procedure for pumps with an minimum operational pressure $> 10^{-4}$ Pa ( $10^{-6}$ mbar)

One hour after starting the pump, heat the test dome (see Figure 1) to a maximum temperature of 120 °C for 3 h. If the turbomolecular pump is fitted with a bake-out device, it shall be baked following the manufacturer's instructions. The temperature of the upper part of the turbomolecular pump shall be monitored to remain within the limits of the pump specification. The bake-out of the turbomolecular pump and the test dome shall be terminated simultaneously. The bake-out procedure shall be described in the test report. Ionization gauges shall be degassed according to the manufacturer's recommendations during and at the end of the bake-out, at the latest 2 h before the measurement. The outlet pressure of the turbomolecular pump shall be recorded at the same time.

The pressure  $p_1$  in the test dome measured 48 h after the end of bake-out is the minimum operational pressure of the turbomolecular pump. At this time, the slope of the function of pressure against time shall not be positive.

### 6.9.3 Test procedure for pumps with an minimum operational pressure $< 10^{-4}$ Pa ( $10^{-6}$ mbar)

When fitting the test dome (see Figure 1), the conditions usually required for UHV-technology shall be met.

One hour after starting the pump, heat the test dome to a maximum temperature of 300 °C. If the turbomolecular pump is fitted with a bake-out device, it shall be baked following the manufacturer's instructions. The temperature of the upper part of the turbomolecular pump shall be monitored to remain within the limits of the pump specification. The bake-out of the turbomolecular pump and the test dome shall be terminated simultaneously when a pressure of 100 times the expected minimum operational pressure is reached, but at the latest after 48 h of baking. The bake-out procedure shall be described in the test report. Ionization gauges shall be degassed according to the manufacturer's recommendations during and at the end of the bake out, at the latest 2 h before the measurement. The outlet pressure of the turbomolecular pump shall be recorded at the same time.

The pressure  $p_1$  in the test dome measured 48 h after the end of bake-out is the minimum operational pressure of the turbomolecular pump. At this time, the slope of the function of pressure against time shall not be positive.

## 6.10 Compression ratio

### 6.10.1 Measurement method

The compression ratio is determined by admitting gas into the outlet duct of the turbomolecular pump with no gas injection into the test dome.

### 6.10.2 Test apparatus

The test gases used shall have a purity of 99,9 % by mass. Pressure records shall be made using devices calibrated for the test gas. Use the apparatus shown in Figure 3. It is recommended to use a set of different pressure gauges to measure the whole range of pressure  $p_1$ . An adjustable valve (4 in Figure 3) for gas admission shall be fitted at the inlet of the backing pump to vary the backing pressure  $p_2$ .

A pressure gauge 8 shall be mounted as near as possible to the outlet of the turbomolecular pump, in a straight uniform section of the backing line, the diameter of which is equal to that of the turbomolecular pump outlet. The connected pipe of the pressure gauge shall be perpendicular to the outlet line axis and flush with its inside wall. It shall be clearly displaced from the gas admission pipe.

To reduce the amount of any other gas at the turbomolecular pump outlet, the use of another turbo-pump or a diffusion pump as a backing pump is strongly recommended. This lowers the outlet pressure  $p_2$  to  $< 10^{-2}$  Pa ( $10^{-4}$  mbar). No cold trap is necessary.

### 6.10.3 Test procedure

For each test gas, first wait until the minimum operational pressure  $p_{01}$  prevails in the test dome. The corresponding backing pressure  $p_{02}$  shall be less than 0,1 Pa ( $10^{-3}$  mbar) to make the measurement valuable.

Then open valve 4 progressively so that the pressure  $p_2$  increases step by step. The values of the backing pressure  $p_2$  and inlet pressure  $p_1$  (always total and partial) shall be recorded simultaneously. When these are stable to within  $\pm 5\%$  over 5 min, the compression ratio  $K_{\text{eff}}$  is given by

$$K_{\text{eff}} = \frac{p_2 - p_{02}}{p_1 - p_{01}} \quad (8)$$

Measurements shall be recorded at three points per decade of the backing pressure.

### 6.10.4 Evaluation of measurements

Plot the inlet pressure  $p_1$  against  $p_2$  both on logarithmic scales. The minimum operational pressure  $p_0$  shall be indicated. Then plot the compression ratio  $K_{\text{eff}}$  against  $p_2$  also on a logarithmic scale. The test gas shall be clearly indicated on each diagram.

## 6.11 Vibration

### 6.11.1 General

The vibration of the turbomolecular pump shall be measured in a direction radial to the motor axis, in the frequency range from 10 Hz to three times the normal rotational speed of the pump, running under normal conditions with no gas load. Both the vibration acceleration and vibration velocity shall be recorded.

### 6.11.2 Test apparatus

The turbomolecular pump shall be freely mounted, in a vertical and/or horizontal position following the manufacturer's operating instructions, on a sheet of rubber at least 4 mm thick on a solid vibration-free base. The base may be a concrete block of at least five times the mass of the pump but no less than 100 kg.

**WARNING — Provisions shall be made for the safety of personnel in the area.**

The inlet flange of the pump shall be blanked off with a standard flange and seal. The vibration measurement head(s) shall be mounted on the pump in a plane at a right angle to the rotor axis. This plane shall not be more than a tenth of the largest dimension of the pump, away from the centre of mass of the pump.

In preparing the pump with the test equipment the mass of the pump with its blanking flange shall not increase by more than 3%. No additional masses shall be connected to the pump during the tests.

The pump shall be connected to the backing pump by a flexible hose at least 750 mm long and bent by more than  $90^\circ$ .

### 6.11.3 Test procedure

Before taking a measurement, the pump shall be run under normal operating conditions without gas load for at least 30 min. While measurements are taken, the backing pump shall be switched off.



## 7 Test report: Additional parameters

To complete the test report, the following items shall be listed:

- a) the type and serial number of the turbomolecular pump;
- b) the DN size of the test dome(s) with the values of the orifice diameter and thickness;
- c) the value of the standard conductance and the formula used for the calculation;
- d) the maximum temperature and duration of bake-out;
- e) the type and performance of the gas flow rate measuring apparatus;
- f) the type of joints used;
- g) the maximum and minimum temperatures of the cooling water at the inlet and outlet;
- h) the flow rate of the cooling water;
- i) the type, quantity and vapour pressure at 20 °C of the lubricating fluid used;
- j) the type and flow rate of the backing pumps used;
- k) the power input of the driving motor;
- l) the speed of rotation of the turbomolecular pump;
- m) the ambient temperature.

## Annex A (informative)

### Derivation of Equations (1) and (2)

A linear relationship is assumed between the compression ratios  $K_{\text{eff}}$ ,  $K_0$  and the volume flow rate  $q_V$  (pumping speed) with its theoretical maximum  $q_{V0}$

$$q_V = q_{V0} \left( \frac{K_0 - K_{\text{eff}}}{K_0 - 1} \right)$$

Here the volume flow rate  $q_V$  becomes its maximum  $q_{V0}$  if the effective compression ratio  $K_{\text{eff}}$  approaches unity. On the other hand, for the maximum  $K_{\text{eff}} = K_0$ , the volume flow rate will be zero by definition.

The effective compression ratio  $K_{\text{eff}} = p_2/p_1$  may be written as the ratio of the volume flow rates of the backing pump and the turbomolecular pump

$$K_{\text{eff}} = q_V / q_{VB}$$

Now the equation reads

$$q_V = q_{V0} \left( \frac{K_0 - (q_V / q_{VB})}{K_0 - 1} \right)$$

This can be solved as

$$q_V = q_{V0} \left( \frac{K_0}{K_0 + (q_{V0} / q_{VB}) - 1} \right)$$

or, reducing by  $K_0$

$$q_V = \frac{q_{V0}}{1 + q_{V0} / (K_0 \cdot q_{VB}) - 1 / K_0}$$



---

---

**ICS 23.160**

Price based on 14 pages