

# INTERNATIONAL STANDARD

# ISO 6101-4

Second edition  
1997-06-01

---

---

## Rubber — Determination of metal content by atomic absorption spectrometry —

### Part 4: Determination of manganese content

*Caoutchouc — Détermination de la teneur en métal par spectrométrie  
d'absorption atomique —*

*Partie 4: Dosage du manganèse*

This material is reproduced from ISO documents under International Organization for Standardization (ISO) Copyright License number IHS/ICC/1996. Not for resale. No part of these ISO documents may be reproduced in any form, electronic retrieval system or otherwise, except as allowed in the copyright law of the country of use, or with the prior written consent of ISO (Case postale 56, 1211 Geneva 20, Switzerland, Fax +41 22 734 10 79), IHS or the ISO Licensor's members.



Reference number  
ISO 6101-4:1997(E)

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 6101-4 was prepared by Technical Committee ISO/TC 45, *Rubber and rubber products*.

This second edition cancels and replaces the first edition (ISO 6101-4:1988), which has been technically revised.

ISO 6101 consists of the following parts, under the general title *Rubber — Determination of metal content by atomic absorption spectrometry*:

- *Part 1: Determination of zinc content*
- *Part 2: Determination of lead content*
- *Part 3: Determination of copper content*
- *Part 4: Determination of manganese content*
- *Part 5: Determination of iron content*

Annex A forms an integral part of this part of ISO 6101.

© ISO 1997

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization  
Case postale 56 • CH-1211 Genève 20 • Switzerland  
Internet central@iso.ch  
X.400 c=ch; a=400net; p=iso; o=isocs; s=central

Printed in Switzerland

# Rubber — Determination of metal content by atomic absorption spectrometry —

## Part 4: Determination of manganese content

**WARNING** — Persons using this part of ISO 6101 should be familiar with normal laboratory practice. This part of ISO 6101 does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

### 1 Scope

This part of ISO 6101 specifies an atomic absorption spectrometric method for the determination of the manganese content of rubbers.

The method is applicable to raw rubber and rubber products having manganese contents above 0,5 ppm. Manganese contents below this limit may be determined, provided that suitable adjustments are made to the mass of the test portion and/or to the concentrations of the solutions used. The use of the standard additions method may lower the bottom limit of detection.

### 2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this part of ISO 6101. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this part of ISO 6101 are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 123:1985, *Rubber latex — Sampling.*

ISO 247:1990, *Rubber — Determination of ash.*

ISO 648:1977, *Laboratory glassware — One-mark pipettes.*

ISO 1042:1983, *Laboratory glassware — One-mark volumetric flasks.*

ISO 1772:1975, *Laboratory crucibles in porcelain and silica.*

ISO 1795:1992, *Rubber, raw, natural and synthetic — Sampling and further preparative procedures.*

ISO 4793:1980, *Laboratory sintered (fritted) filters — Porosity grading, classification and designation.*

### 3 Principle

A test portion is ashed at  $550\text{ °C} \pm 25\text{ °C}$  in accordance with ISO 247:1990, method A. The ash is dissolved in hydrochloric acid. The solution is aspirated into an atomic absorption spectrometer and the absorption is measured at a wavelength of 279,5 nm, using a manganese hollow-cathode lamp as the manganese emission source. Any silicates are volatilized by sulfuric and hydrofluoric acid.

NOTE — ISO 6955:1982, *Analytical spectroscopic methods — Flame emission, atomic absorption, and atomic fluorescence — Vocabulary*, defines the spectrometric terms used in this part of ISO 6101.

### 4 Reagents

During the analysis, unless otherwise stated, use only reagents of recognized analytical grade and only distilled water or water of equivalent purity.

**4.1 Hydrochloric acid**,  $\rho_{20} = 1,18\text{ Mg/m}^3$ .

**4.2 Hydrochloric acid**, diluted 1+2.

Dilute 1 volume of concentrated hydrochloric acid (4.1) with 2 volumes of water.

**4.3 Sulfuric acid**,  $\rho_{20} = 1,84\text{ Mg/m}^3$ .

**4.4 Sulfuric acid**, diluted 1+3.

Add carefully 1 volume of concentrated sulfuric acid (4.3) to 3 volumes of water.

**4.5 Hydrofluoric acid**,  $\rho_{20} = 1,13\text{ Mg/m}^3$ , 38 % (m/m) to 40 % (m/m).

**4.6 Standard manganese stock solution**, containing 1 g of Mn per cubic decimetre.

Either use a commercially available standard manganese solution, or prepare as follows:

Using electrolytic manganese of purity  $\geq 99,9\%$ , free the surface of any manganese oxides by placing a few grams of the metal in a beaker containing  $60\text{ cm}^3$  to  $80\text{ cm}^3$  of 1+3 sulfuric acid (4.4) with about  $100\text{ cm}^3$  of water. Stir and, after a few minutes, decant the acid solution and pour water into the beaker. Repeat the decantation and washing with water several times. Then place the manganese metal in acetone and stir. Decant the acetone, dry the metal in a hot-air oven (5.13), maintained at  $100\text{ °C} \pm 5\text{ °C}$ , for about 2 min and allow it to cool in a desiccator.

In a  $600\text{ cm}^3$  tall-form beaker, weigh, to the nearest 0,1 mg, 1 g of this purified manganese metal, and dissolve it with  $40\text{ cm}^3$  of 1+3 sulfuric acid solution (4.4) and about  $80\text{ cm}^3$  of water. Boil the solution for several minutes. Allow to cool and transfer quantitatively to a  $1\ 000\text{ cm}^3$  one-mark volumetric flask (see 5.5). Dilute to the mark and mix thoroughly.

$1\text{ cm}^3$  of this standard stock solution contains  $1\ 000\ \mu\text{g}$  of Mn.

**4.7 Standard manganese solution**, containing 10 mg of Mn per cubic decimetre.

Carefully pipette  $10\text{ cm}^3$  of the standard manganese stock solution (4.6) into a  $1\ 000\text{ cm}^3$  one-mark volumetric flask (see 5.5), dilute to the mark with 1+2 hydrochloric acid (4.2) and mix thoroughly.

Prepare this solution on the day of use.

$1\text{ cm}^3$  of this standard solution contains  $10\ \mu\text{g}$  of Mn.

## 5 Apparatus

Ordinary laboratory apparatus, plus the following:

**5.1 Atomic absorption spectrometer**, fitted with a burner fed with acetylene and air, compressed to at least 60 kPa and 300 kPa, respectively, and also fitted with a manganese hollow-cathode lamp as the manganese emission source. The instrument shall be operated in accordance with the manufacturer's instructions for optimum performance.

Alternatively, an **electrothermal atomization device (graphite furnace)** may be used. It shall be operated by a competent person in accordance with the manufacturer's instructions for optimum performance.

**5.2 Balance**, accurate to 0,1 mg.

**5.3 Muffle furnace**, capable of being maintained at a temperature of  $550\text{ °C} \pm 25\text{ °C}$ .

**5.4 Glass filter crucible**, filter pore size 16  $\mu\text{m}$  to 40  $\mu\text{m}$  (porosity grade P 40 — see ISO 4793).

**5.5 One-mark volumetric flasks**, glass-stoppered, of capacities 50  $\text{cm}^3$ , 100  $\text{cm}^3$ , 200  $\text{cm}^3$ , 500  $\text{cm}^3$  and 1 000  $\text{cm}^3$ , complying with the requirements of ISO 1042, class A.

**5.6 Volumetric pipettes**, of capacities 5  $\text{cm}^3$ , 10  $\text{cm}^3$ , 20  $\text{cm}^3$  and 50  $\text{cm}^3$ , complying with the requirements of ISO 648, class A.

**5.7 Electric hotplate or heated sand bath.**

**5.8 Steam bath.**

**5.9 Platinum or borosilicate-glass rod**, for use as a stirrer.

**5.10 Crucible**, of platinum, and of capacity 50  $\text{cm}^3$  to 150  $\text{cm}^3$  depending on the test portion size.

**5.11 Crucible**, of silica or borosilicate glass, of capacity 50  $\text{cm}^3$  to 150  $\text{cm}^3$  depending on the test portion size, complying with the requirements of ISO 1772.

**5.12 Ashless filter paper.**

**5.13 Hot-air oven**, capable of being maintained at a temperature of  $100\text{ °C} \pm 5\text{ °C}$ .

## 6 Sampling

Carry out sampling as follows:

raw rubber: in accordance with ISO 1795;

latex: in accordance with ISO 123;

products: to be representative of the whole batch.

## 7 Procedure

### 7.1 Test portion

Weigh, to the nearest 0,1 mg, approximately 10 g of milled or finely cut rubber into an appropriate crucible (5.10 or 5.11). The size of the test portion shall be judged by prior knowledge of the approximate amount of manganese present.

### 7.2 Preparation of test solution

#### 7.2.1 Destruction of organic matter

Ash the test portion in accordance with method A of ISO 247:1990, in the muffle furnace (5.3), maintained at  $550\text{ }^{\circ}\text{C} \pm 25\text{ }^{\circ}\text{C}$ . If the ash is black, caused by small amounts of carbon black, stir carefully with the platinum or borosilicate-glass rod (5.9) and continue heating.

#### 7.2.2 Dissolution of inorganic residue

After ashing, allow the crucible and its contents to cool to ambient temperature. Add 20 cm<sup>3</sup> of concentrated hydrochloric acid (4.1). Heat the mixture on the steam bath (5.8) for at least 10 min. Do not let the reaction mixture boil. Allow to cool to ambient temperature and transfer the solution quantitatively, with the aid of water, to a 50 cm<sup>3</sup> one-mark volumetric flask (see 5.5). If the ash is not totally dissolved, proceed as follows:

Transfer the solution and the undissolved ash quantitatively, with the aid of water, to a platinum crucible (5.10). Add a few drops of concentrated sulfuric acid (4.3) and 5 cm<sup>3</sup> of hydrofluoric acid (4.5). Heat on the electric hotplate or sand bath (5.7) in a fume cupboard and evaporate to dryness, while stirring with a platinum rod (5.9). Repeat this digestion with the same quantities of sulfuric and hydrofluoric acids two more times.

Allow to cool to ambient temperature, add 20 cm<sup>3</sup> of concentrated hydrochloric acid (4.1), heat for 10 min and transfer quantitatively, with the aid of water, to a 50 cm<sup>3</sup> one-mark volumetric flask (see 5.5).

Dilute to the mark with water and mix thoroughly. Insoluble matter may settle and, if so, shall be filtered off using a filter crucible (5.4) just before making spectrometric measurements in accordance with 7.3.

Test solutions should contain approximately 12 % hydrochloric acid. If evaporation, etc., has reduced or increased this concentration, adjust accordingly with concentrated hydrochloric acid (4.1) or water.

### 7.3 Preparation of the calibration graph

#### 7.3.1 Preparation of calibration solutions

7.3.1.1 Into a series of five 100 cm<sup>3</sup> one-mark volumetric flasks (see 5.5) introduce, using pipettes (see 5.6), the volumes of standard manganese solution (4.7) indicated in table 1. Dilute to the mark with 1 + 2 hydrochloric acid (4.2) and mix thoroughly.

Table 1 — Standard calibration solutions

Volume of standard manganese solution cm <sup>3</sup>	Mass of manganese contained in 1 cm <sup>3</sup> µg
25	2,5
10	1
5	0,5
2	0,2
0	0

**7.3.1.2** Prepare the set of calibration solutions immediately prior to the determination.

### **7.3.2 Spectrometric measurements**

Switch on the spectrometer (5.1) sufficiently in advance to ensure stabilization. With the manganese hollow-cathode tube suitably positioned, adjust the wavelength to 279,5 nm and the sensitivity and slit aperture according to the characteristics of the instrument.

Adjust the pressures and flow rates of the air and of the acetylene in accordance with the manufacturer's instructions so as to obtain a clear blue, non-luminous, oxidizing flame, suited to the characteristics of the particular spectrometer being used.

Aspirate the set of calibration solutions in succession into the flame and measure the absorbance of each solution twice, averaging the readings. Take care that the aspiration rate is constant throughout this process. Ensure also that at least one calibration solution is at or below the analyte level found in the rubber being tested.

Aspirate water through the burner after each measurement.

### **7.3.3 Plotting the calibration graph**

Plot a graph having, for example, the masses, in micrograms, of manganese contained in 1 cm<sup>3</sup> of the calibration solutions as abscissae and the corresponding values of absorbance, corrected for the absorbance of the calibration blank, as ordinates. Represent the points on the graph by the best straight line as judged visually or as calculated by the least-squares fit method.

## **7.4 Determination**

### **7.4.1 Spectrometric measurements**

Carry out duplicate spectrometric measurements at a wavelength of 279,5 nm on the test solution prepared in 7.2.2, following the procedure specified in 7.3.2.

### **7.4.2 Dilution**

If the instrument response for the test solution is greater than that found for the calibration solution having the highest manganese content, dilute, as appropriate, with 1+2 hydrochloric acid (4.2) in accordance with the following procedure.

Pipette carefully a suitable volume ( $V$  cm<sup>3</sup>) of the test solution into a 100 cm<sup>3</sup> one-mark volumetric flask (see 5.5) so that the manganese concentration lies within the range covered by the calibration solutions. Dilute to the mark with 1+2 hydrochloric acid (4.2). Repeat the spectrometric measurements.

NOTE — To increase the reliability of the test method, the standard-additions method may be used (see annex A).

### **7.5 Blank determination**

Carry out a blank test in parallel with the determination, using 1+2 hydrochloric acid solution (4.2), but omitting the test portion.

If the preparation of the test solution involved the use of sulfuric acid and hydrofluoric acid, prepare the blank test solution by repeating that procedure, but omitting the test portion.

### **7.6 Number of determinations**

Carry out the procedure in duplicate, using separate test portions cut from the same homogenized sample.

## 8 Expression of results

8.1 Read the manganese content of the test solution directly from the calibration graph plotted in 7.3.3.

The manganese content of the test portion, expressed as a percentage by mass, is given by the formula

$$\frac{\rho(\text{Mn})_t - \rho(\text{Mn})_b}{200m} \times f$$

where

$\rho(\text{Mn})_t$  is the manganese content, in micrograms per cubic centimetre, of the test solution, read from the calibration graph;

$\rho(\text{Mn})_b$  is the manganese content, in micrograms per cubic centimetre, of the blank test solution, read from the calibration graph;

$m$  is the mass, in grams, of the test portion;

$f$  is the test solution dilution factor, if required (see 7.4.2), given by

$$f = \frac{100}{V}$$

$V$  being the volume, in cubic centimetres, of the test solution taken in 7.4.2.

8.2 Alternatively, the manganese content, expressed as a percentage by mass, is given by the formula

$$\frac{\rho(\text{Mn})_t - \rho(\text{Mn})_b}{200m} \times f$$

where

$\rho(\text{Mn})_t$  is the manganese content, in micrograms per cubic centimetre, of the test solution, given by

$$\rho(\text{Mn})_t = \frac{A_t \times \rho(\text{Mn})_n}{A_n}$$

$\rho(\text{Mn})_b$  is the manganese content, in micrograms per cubic centimetre, of the test solution, given by

$$\rho(\text{Mn})_b = \frac{A_b \times \rho(\text{Mn})_n}{A_n}$$

$A_t$  being the absorbance of the test solution,

$A_b$  being the absorbance of the blank test solution,

$A_n$  being the absorbance of the standard calibration solution having the manganese content closest to that of the test solution,

$\rho(\text{Mn})_n$  being the manganese content, in micrograms per cubic centimetre, of the standard calibration solution having the absorbance closest to that of the test solution;

$m$  is the mass, in grams, of the test portion;

$f$  is the test solution dilution factor, if required (see 7.4.2), given by

$$f = \frac{100}{V}$$

$V$  being the volume, in cubic centimetres, of the test solution taken in 7.4.2.



**8.3** The test result is the average of two determinations, rounded to two decimal places when the manganese concentration is expressed as a percentage and to the nearest whole number when the concentration is expressed in milligrams per kilogram.

**8.4** Report the manganese content as a percentage if greater than or equal to 0,1 %, or in milligrams per kilogram if less than 0,1 %.

## 9 Test report

The test report shall include the following information:

- a) a reference to this part of ISO 6101;
- b) all details necessary for the complete identification of the product tested;
- c) the method of sampling;
- d) the type of instrument used (flame or graphite furnace spectrometer);
- e) the results obtained and the units in which they have been expressed;
- f) any unusual features noted during the determination;
- g) any operation not included in this part of ISO 6101, or in the International Standards to which reference is made, as well as any incident which might have affected the results.

## Annex A (normative)

### Method of standard additions

The method of standard additions provides the analyst with a powerful tool for increasing the accuracy of an atomic absorption analysis.

It is used with samples containing unknown concentrations of matrix materials, with samples which are difficult to duplicate with blanks and/or when it is necessary to lower the limits of detection.

The method of standard additions can be found in any standard text book on atomic absorption and is usually described in the user's manual supplied with the atomic absorption spectrometer.

The following example illustrates the method:

From a test solution prepared as described in 7.2, take four aliquots of the same size. To three of these aliquots, add a different, but known, volume of standard manganese solution. Make up the volumes to the same total for all four aliquots. Use concentrations which fall on the linear portion of the calibration graph.

Measure the absorbance of each of the four solutions so obtained.

Plot absorbance on the  $y$ -axis and the concentration, in micrograms of manganese per cubic centimetre of solution, on the  $x$ -axis.

Extrapolate the straight line to intersect the  $x$ -axis (zero absorbance). At the point of intersection with the  $x$ -axis, read the concentration of manganese in the test solution.

An example is given in figure A.1.

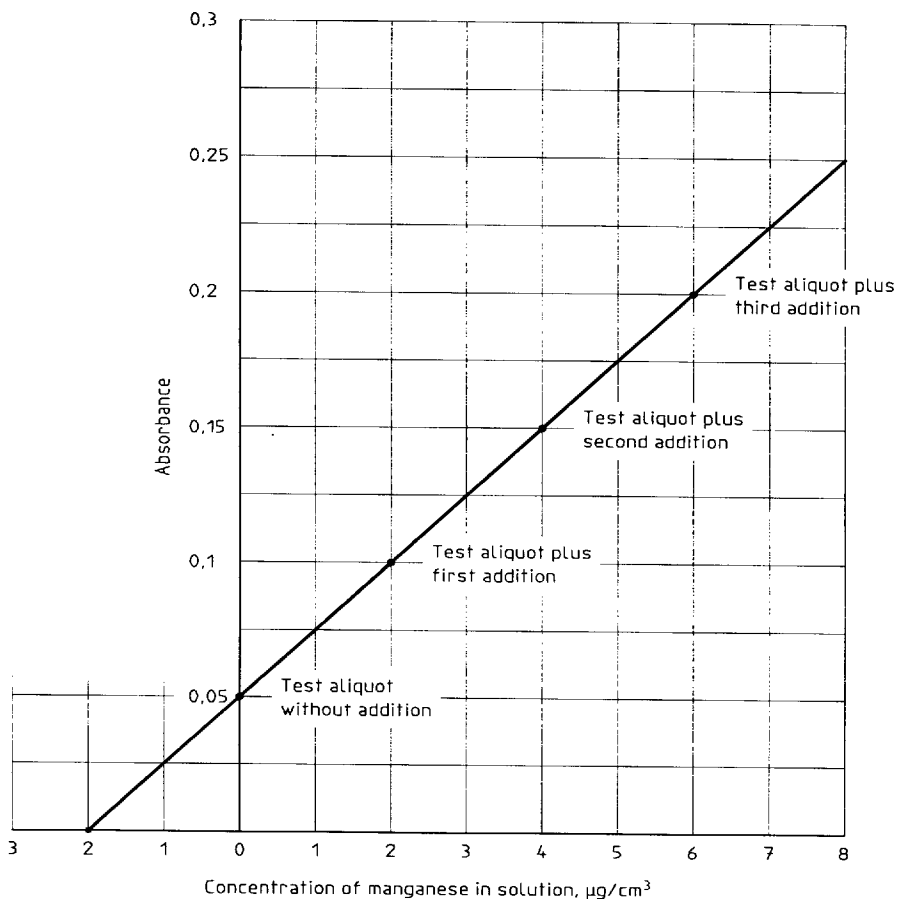


Figure A.1 — Example of graph obtained using the method of standard additions

---

---

**ICS 83.060**

**Descriptors:** rubber, chemical analysis, determination of content, manganese, atomic absorption spectrometric method.

Price based on 9 pages

---

---