
**Anodizing of aluminium and its alloys —
Measurement of reflectance
characteristics of aluminium surfaces
using integrating-sphere instruments**

*Anodisation de l'aluminium et de ses alliages — Mesurage des
caractéristiques de réflectivité des surfaces d'aluminium à l'aide
d'instruments à sphère d'intégration*



Reference number
ISO 6719:2010(E)

© ISO 2010

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



COPYRIGHT PROTECTED DOCUMENT

© ISO 2010

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Principle.....	1
4 Apparatus	1
4.1 General	1
4.2 Geometrical specifications of the apparatus.....	2
4.3 Specular-included and specular-excluded determinations	2
4.4 Irradiation beam.....	2
4.5 Housing	3
5 Calibration and operation of the reflectometer	7
5.1 General	7
5.2 Reference standards	8
6 Measurement	8
7 Expression of results	8
7.1 Calculation of reflectance values	8
8 Test report.....	9

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 6719 was prepared by Technical Committee ISO/TC 79, *Light metals and their alloys*, Subcommittee SC 2, *Organic and anodic oxidation coatings on aluminium*.

This second edition cancels and replaces the first edition (ISO 6719:1986), which has been technically revised.

Anodizing of aluminium and its alloys — Measurement of reflectance characteristics of aluminium surfaces using integrating-sphere instruments

1 Scope

This International Standard specifies a method of measuring the total and diffuse luminous reflectance characteristics of aluminium surfaces, using integrating-sphere instruments.

The method described is also applicable to the measurement of specular reflectance (principal gloss value), specularity and diffuseness.

The method is unsuitable for use with lighting reflectors.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 7724-2, *Paints and varnishes — Colorimetry — Part 2: Colour measurement*

ISO 11664-2:2007, *Colorimetry — Part 2: CIE standard illuminants*

3 Principle

Measurement, using an integrating-sphere reflectometer, of the total and diffuse reflected light at different angles of incidence, close to the normal surface of a test specimen.

4 Apparatus

4.1 General

The reflectometer, suitable for measuring the reflectance of metallic surfaces, consists of a suitable light source, an integrating sphere and a photometer comprising a photo-electric cell with a signal multiplier and recording, indicating, or computing equipment. Figures 1 to 5 show the optical systems and geometry of typical instruments.

The incident light beam is allowed to fall onto the specimen and is reflected into the sphere, the interior of which is white, where it is automatically integrated. The average light flux, as measured by the photometer, is a measure of the quantity of the reflected light.

The spectral product of the light source, spectral filters, and spectral response of the light detector shall closely simulate the spectral product of the CIE source C (or D65) and the spectral luminous efficiency $V(\lambda)$ for photopic vision, in accordance with ISO 11664-2.

4.2 Geometrical specifications of the apparatus

4.2.1 Integrating sphere

The interior of the sphere, white-coated and fitted with a device to permit measurement of reflectance, either including or excluding specular reflectance, serves to collect the reflected light flux.

Any diameter of sphere is satisfactory, provided that the total port area does not exceed 5 % of the total internal surface.

The internal surface shall be diffusing and of a highly reflective white for the whole of the visible spectrum. The entrance and specimen ports of the instrument shall be centred on the same great circle with an arc of more than 170° between their centres. The specimen port shall subtend $8^\circ \pm 1^\circ$ of arc in relation to the centre of the entrance port. The irradiating beam shall pass through the centreline of the entrance and specimen ports. A photometer shall be positioned on the sphere at $90^\circ \pm 0,5^\circ$ from the entrance port.

4.3 Specular-included and specular-excluded determinations

4.3.1 Pivotal sphere

In the pivotal-sphere type of instrument (Figures 1 to 4), the sphere can turn about a vertical axis passing through the specimen port, rotating $9^\circ \pm 1^\circ$ to provide for the measurements of specular-included or total reflectance (Q) and specular-excluded or diffuse reflectance (Q_d).

4.3.2 Fixed sphere (Type 1)

In the fixed-sphere Type 1 instrument, the specimen is held so that the incident beam falls on it at an angle of $9^\circ \pm 1^\circ$ to the normal. A port, of the same dimensions as the entrance port, is provided in order to accept the specular reflection. Interchangeable caps are provided for this port, a black one to absorb the specular reflection for diffuse reflectance (Q_d) measurements and one coated with the same material as the inside of the sphere for total reflectance (Q) measurements.

4.3.3 Fixed sphere (Type 2)

In the fixed-sphere Type 2 instrument (see Figure 5), the sphere is fixed and only the specimen can be inclined. A wedge, as shown in Figure 5, designed to exclude ambient light, and white-coated like the sphere interior, allows adjustment of the angle of the specimen surface. For measurement of diffuse reflectance (Q_d), the specimen surface is adjusted to be perpendicular to the incident beam. For measurement of total reflectance (Q), the specimen surface is inclined at $9^\circ \pm 1^\circ$ from the normal incident beam by insertion of the wedge.

4.4 Irradiation beam


The light beam shall be substantially unidirectional with a maximum angle of any ray being less than 3° from the axis of the beam. It shall not be vignetted at either port.

The incident light beam shall have a circular cross-section concentric with the specimen port and shall have an annulus of $1,3^\circ \pm 0,1^\circ$ subtended at the entrance port. On reflection from a first surface mirror, the specular-excluded beam shall be concentric with the centre of the port when the sphere is in the specular-excluded position. The mirror-reflected beam shall have a concentric circle with the port and shall have an annulus of $0,6^\circ \pm 0,2^\circ$ subtended at the level of the exit port. The size of the exit port shall be not more than $0,1^\circ$ greater than that of the annulus.

NOTE The dimensions of this beam can be most easily measured at a point beyond the sphere at a distance corresponding to the diameter of the integrating sphere, with no obstruction at either port. However, this will not ensure alignment when specularly reflected.

4.5 Housing


A housing shall be provided to prevent ambient light from entering the entrance port.

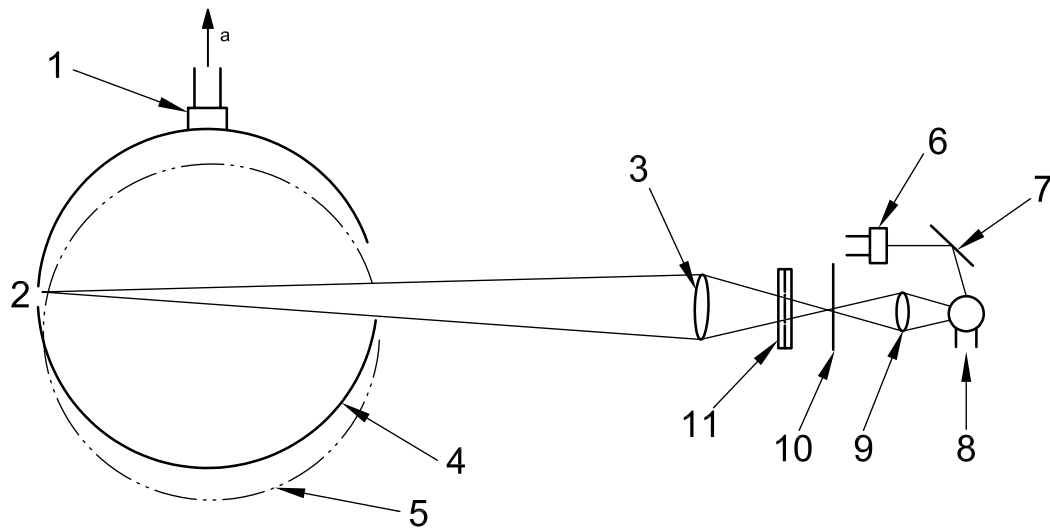

Key

- | | | | |
|---|---|----|-----------------|
| 1 | photoelectric cell | 7 | mirror |
| 2 | test piece | 8 | light source |
| 3 | lens | 9 | lens |
| 4 | 0° incidence for diffuse reflectance | 10 | aperture |
| 5 | 9° ± 1° incidence for total reflectance | 11 | spectral filter |
| 6 | photoelectric cell for comparison | | |
| a | To the amplifiers and recorders. | | |


Figure 1 — Schematic optical plan of one type of pivotable-sphere reflectometer

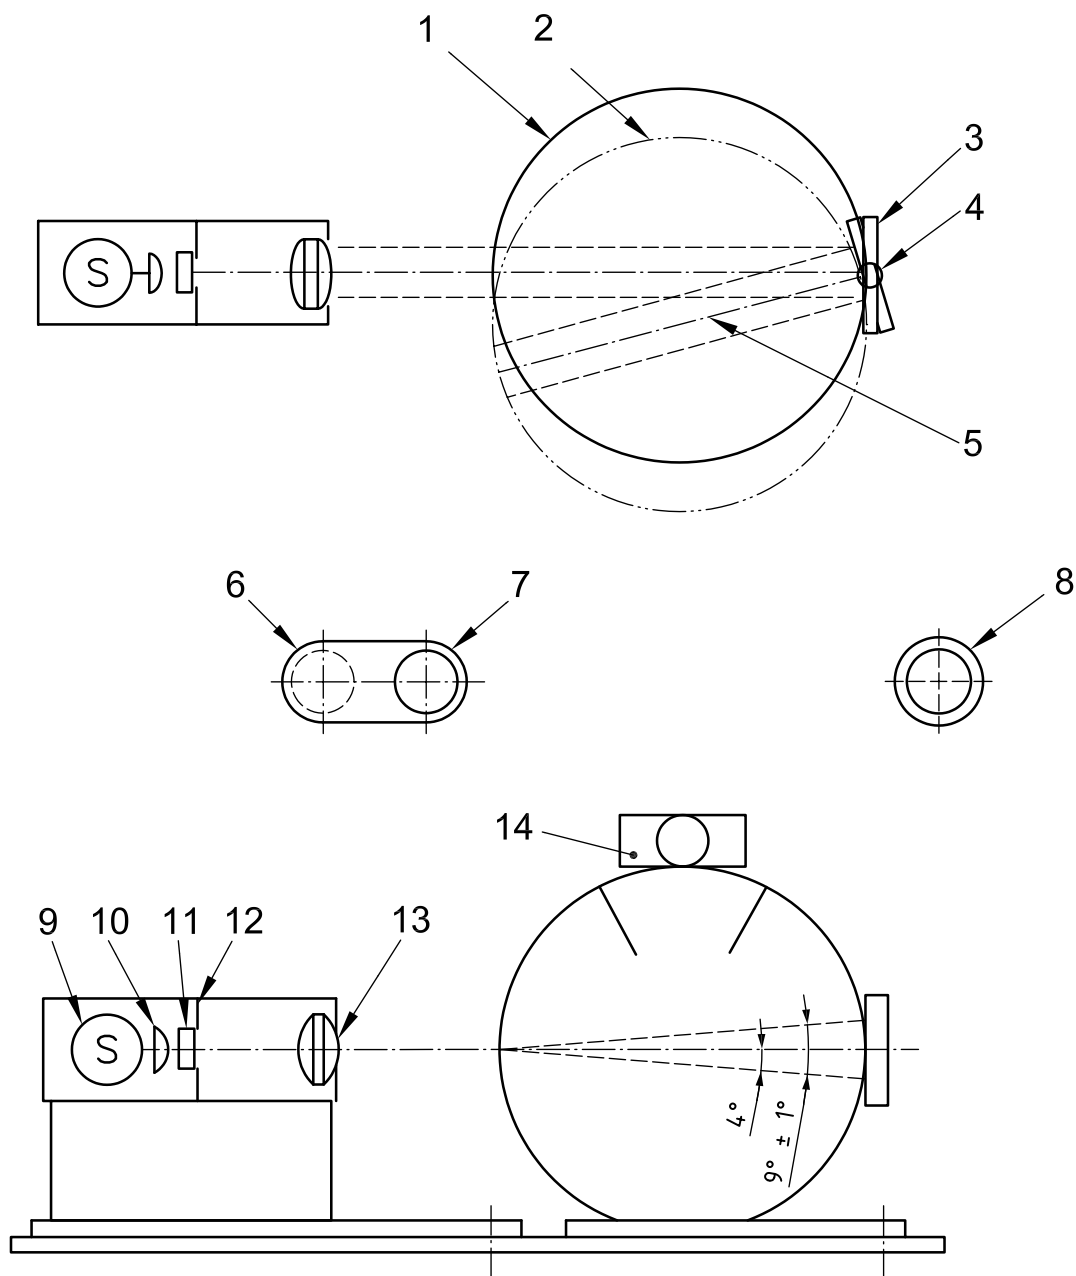

Key

- | | | | |
|---|---|----|-------------------------|
| 1 | sphere in axial position | 8 | light beam at exit port |
| 2 | sphere in pivoted position | 9 | source |
| 3 | test piece | 10 | convex lens |
| 4 | specular pivot | 11 | specular filter |
| 5 | specular beam — sphere in pivoted position | 12 | aperture |
| 6 | incoming light beam from the axial position | 13 | lens |
| 7 | incoming light beam at entrance port (axis positions) | 14 | receiver |


Figure 2 — Schematic optical plan of another type of pivotable-sphere reflectometer

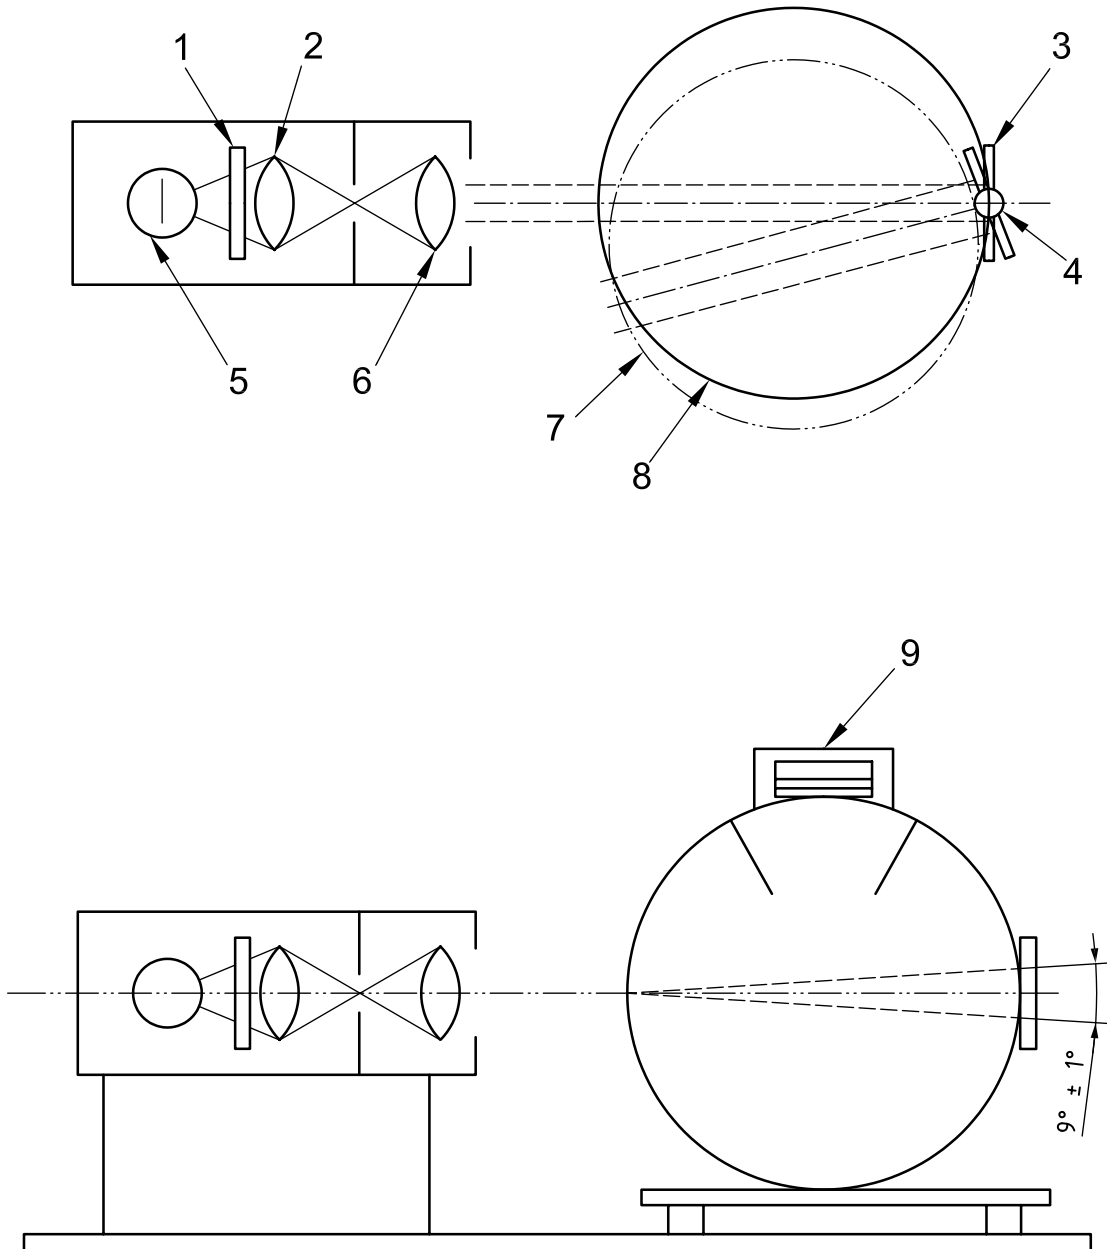

Key

- | | |
|-------------------|-----------------------|
| 1 spectral filter | 6 lens |
| 2 lens | 7 in pivoted position |
| 3 test piece | 8 in axial position |
| 4 sphere pivot | 9 recorder |
| 5 light source | |


Figure 3 — Geometry of typical pivotable-sphere reflectometers

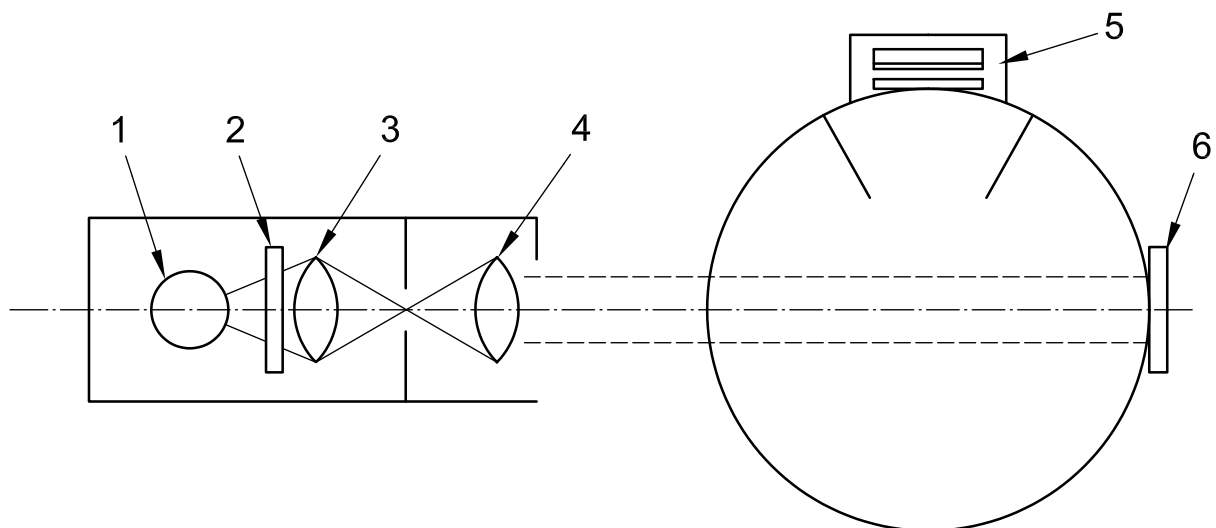

Key

- | | |
|-------------------|--------------|
| 1 light source | 4 lens |
| 2 spectral filter | 5 receiver |
| 3 lens | 6 test piece |

Figure 4 — Geometry of typical pivotable-sphere reflectometers (specular-excluded)

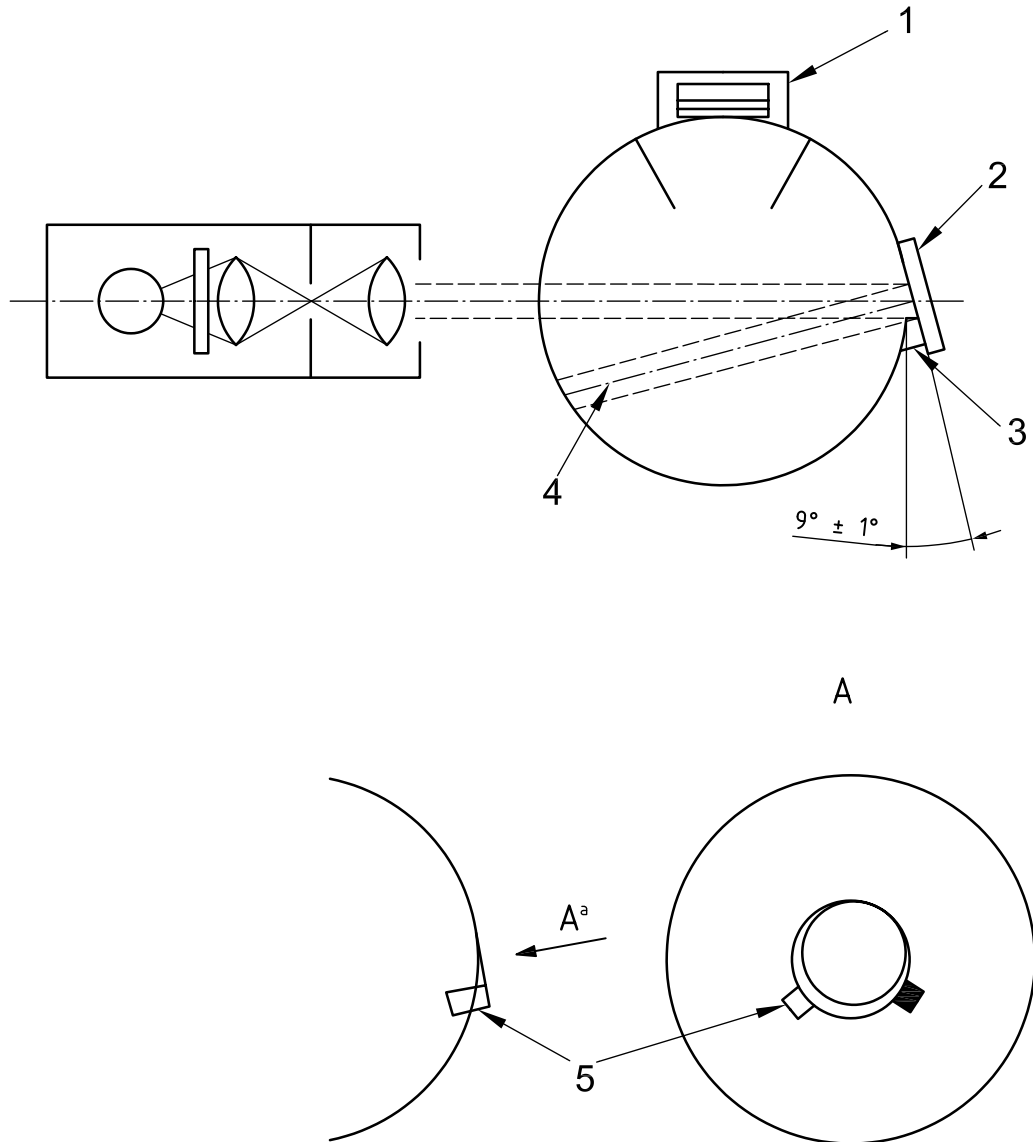

Key

- | | |
|------------------------|-----------------|
| 1 receiver | 4 specular beam |
| 2 test piece | 5 wedge |
| 3 wedge (white-coated) | |
| a Exit port. | |

Figure 5 — Geometry of a typical fixed-sphere (Type 2), specimen-inclining reflectometer (specular-excluded)

5 Calibration and operation of the reflectometer

5.1 General

The reflectometer shall be operated and calibrated in accordance with the manufacturer's instructions.

5.2 Reference standards

5.2.1 A white primary standard shall be employed, consisting of a pressed barium sulfate powder tablet prepared in accordance with ISO 7724-2.

5.2.2 The zero of the instrument shall be calibrated using a black-surface or light-trap standard by recording the values of total and diffuse reflectance. A black-velvet textile surface should read 0,2 % to 0,5 % of the total reflectance.

5.2.3 A first surface mirror, calibrated for both total and diffuse reflectance against the primary standard, shall be used as a working standard. The total reflectance shall be greater than 90 % and the diffuse reflectance 0,2 % to 1,5 %.

6 Measurement

Take three measurements of both total and diffuse reflectance on the surface for each orientation of the test piece. Orientate the test piece at angles of 0°, 45° and 90° to the direction of rolling, extruding or machining of the test piece and the plane of measurement (optical plane) of the reflectometer. Calculate the average values.

If directionality is to be measured, record separately the measurements made at the angles of 0° and 90° to the direction of rolling, extruding or machining of the test piece; 0° is defined as with (w) this direction and 90° is defined as against (a) this direction.

7 Expression of results

7.1 Calculation of reflectance values

7.1.1 Specular-reflectance values

Calculate the specular-reflectance ratio, R_d , using Equation (1):

$$R_d = \frac{Q - Q_d}{Q} = \frac{Q_r}{Q} \quad (1)$$

where

Q_r is the average specular reflectance (or principal gloss value);

Q is the average total reflectance;

Q_d is the average diffuse reflectance.

7.1.2 Diffuseness value

Calculate the diffuse-reflectance ratio, D , using Equation (2):

$$D = \frac{Q_d}{Q} \quad (2)$$

7.1.3 Directionality

Calculate $R_{d(w)}$ and $R_{d(a)}$ as in 7.1.1 and express the directionality, Z , as a percentage, using Equation (3):

$$Z = \frac{R_{d(w)} - R_{d(a)}}{R_{d(w)}} \times 100 \quad (3)$$

For surfaces primarily of a diffuse nature, substitute $D_{(w)}$ and $D_{(a)}$ values (see 7.1.2) for the $R_{d(w)}$ and $R_{d(a)}$ values used in the equation.

8 Test report

The test report shall include at least the following information:

- a) a reference to this International Standard;
- b) type and identification of the product tested;
- c) method(s) of preparing the test pieces;
- d) instrument used, including the manufacturer's name and model;
- e) average specular reflectance (or principal gloss) value, average total reflectance value, and average diffuse reflectance value (see Clause 7);
- f) specular-reflectance or diffuseness value (see 7.1.1 and 7.1.2);
- g) directionality (see 7.1.3);
- h) date of the test.

ICS 25.220.20

Price based on 9 pages