

INTERNATIONAL
STANDARD

ISO
6721-7

First edition
1996-06-01

**Plastics — Determination of dynamic
mechanical properties —**

Part 7:

Torsional vibration — Non-resonance method

*Plastiques — Détermination des propriétés mécaniques dynamiques —
Partie 7: Vibration en torsion — Méthode hors résonance*



Reference number
ISO 6721-7:1996(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 6721-7 was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 2, *Mechanical properties*.

Together with the other parts of ISO 6721, it cancels and replaces ISO 537:1989 and ISO 6721:1983, which have been technically revised.

ISO 6721 consists of the following parts, under the general title *Plastics — Determination of dynamic mechanical properties*:

- *Part 1: General principles*
- *Part 2: Torsion-pendulum method*
- *Part 3: Flexural vibration — Resonance-curve method*
- *Part 4: Tensile vibration — Non-resonance method*
- *Part 5: Flexural vibration — Non-resonance method*
- *Part 6: Shear vibration — Non-resonance method*
- *Part 7: Torsional vibration — Non-resonance method*
- *Part 8: Longitudinal and shear vibration — Wave-propagation method*
- *Part 9: Tensile vibration — Sonic-pulse propagation method*
- *Part 10: Complex shear viscosity using a parallel-plate oscillatory rheometer*

© ISO 1996

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization
Case postale 56 • CH-1211 Genève 20 • Switzerland

Printed in Switzerland

Plastics — Determination of dynamic mechanical properties —

Part 7: Torsional vibration — Non-resonance method

1 Scope

This part of ISO 6721 describes a torsional, non-resonance method for determining the components of the shear complex modulus G^* of solid polymers in the form of bars or rods at frequencies typically in the range 0,001 Hz to 100 Hz. The method is suitable for measuring dynamic storage moduli ranging from about 10 MPa, which is typical of values obtained for stiff rubbers, to values of about 10 GPa which are representative of fibre-reinforced plastics. Although materials with moduli less than 10 MPa may be studied, more accurate measurements of their dynamic properties can be made using simple shear (see ISO 6721-6) or torsional deformations of thin layers between parallel plates.

This method is particularly suited to the measurement of loss factors greater than 0,1 and may therefore be conveniently used to study the variation of dynamic properties with temperature and frequency through most of the glass-rubber relaxation region (see ISO 6721-1:1994, subclause 9.4). The availability of data determined over wide ranges of both frequency and temperature enable master plots to be derived, using frequency-temperature shift procedures, which display dynamic properties over an extended frequency range at different temperatures.

Although loss factors below 0,1 may be more accurately determined using the torsion pendulum (see ISO 6721-2), the method described in this part of

ISO 6721 enables a much wider and continuous frequency range to be covered.

2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this part of ISO 6721. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this part of ISO 6721 are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 6721-1:1994, *Plastics — Determination of dynamic mechanical properties — Part 1: General principles*.

ISO 6721-2:1994, *Plastics — Determination of dynamic mechanical properties — Part 2: Torsion-pendulum method*.

ISO 6721-6:1996, *Plastics — Determination of dynamic mechanical properties — Part 6: Shear vibration — Non-resonance method*.

3 Definitions

See ISO 6721-1:1994, clause 4.

4 Principle

The specimen is subjected to a sinusoidal torque or angular displacement at a frequency significantly below the fundamental torsion resonance frequency (see 10.2.1). The amplitudes of the torque and displacement cycles applied to the specimen and the phase angle between these cycles are measured. The storage and loss components of the shear complex modulus and the loss factor are calculated using equations given in clause 10 of this part of ISO 6721.

5 Test device

5.1 Loading assembly

The requirements on the apparatus are that it shall permit measurements of the amplitudes of, and phase angle between, the torque and angular displacement cycles for a specimen subjected to a sinusoidal torque or displacement. Various designs of apparatus are possible, as illustrated schematically in figures 1a) and 1b). In figure 1a), a sinusoidal angular displacement is generated by the drive unit D and applied to one end of the specimen S through the moving clamp C₁. The amplitude and frequency of the angular displacement are variable and monitored by the rotary displacement transducer R. The specimen is held at the opposite end by a fixed clamp C₂ and thus undergoes sinusoidal torsional deformations. The sinusoidal torque applied in deforming the specimen is monitored by a torque transducer T connected to C₂. The members between the clamp C₁ and D and between C₂ and T should be much stiffer than the specimen and should have a low thermal conductance if the specimen is to be enclosed in a temperature-controlled cabinet (see note 1). Where tests are carried out at elevated temperatures, a facility shall be included in the loading assembly to avoid buckling of the specimen resulting from thermal expansion.

NOTE 1 Whilst each member of the loading assembly may have a much higher stiffness than the specimen, the presence of clamped or bolted connections can significantly increase the apparatus compliance. It may then be necessary to apply a compliance correction as described in 10.2.3.

Various other loading assemblies may be employed as alternatives to that detailed above. For example, the torque on the specimen may be calculated from the current supplied to the drive unit, thus eliminating the need for a separate torque transducer. With this method [figure 1b)], it should be recognized that part of the torque generated by the drive current is used to accelerate the drive shaft and also to deform any drive shaft suspension (S_u) in parallel with the specimen. That part of the generated torque used to deform the specimen shall be determined with the aid of a separate calibration with the specimen absent. Alternatively, the suspension member may be replaced by an air bearing, thereby making the torsional rigidity of the suspension zero.

5.1.1 Clamps

The clamps shall be capable of gripping the test specimen with a force which is sufficient to prevent the specimen from slipping during the torsional deformation and maintaining the force at low temperatures.

The separation between the two clamps should preferably be variable so that specimens of different length can be accommodated and length corrections may be determined (see 10.2.4). A facility to permit small variations in the clamp separation would also allow for thermal expansion of the specimens and is necessary to avoid errors in the apparent moduli due to buckling of the specimens at high temperatures.

Any misalignment of the clamps with respect to the force transducer will produce a lateral component of the torque applied to the transducer during loading of the specimen. The alignment of the loading assembly and test specimen shall be such that any lateral component recorded by the transducer is less than 1 % of the applied torque.

5.1.2 Transducers

The term transducer in this part of ISO 6721 refers to any device capable of measuring the applied torque or displacement, or the ratio of these quantities, as a function of time. The calibrations of the transducers shall be traceable to national standards for the measurement of torque and length. The calibrations shall be accurate to $\pm 2\%$ of the minimum torque and displacement cycle amplitudes applied to the specimen for the purpose of determining dynamic properties.

5.2 Electronic data-processing equipment

Data-processing equipment shall be capable of recording the torque and displacement cycle amplitudes to an accuracy of $\pm 1\%$ the phase angle between the torque and displacement cycles to an accuracy of $\pm 0,1^\circ$ and the frequency to an accuracy of $\pm 10\%$.

5.3 Temperature measurement and control

See ISO 6721-1:1994, subclauses 5.3 and 5.5.

5.4 Devices for measuring test specimen dimensions

See ISO 6721-1:1994, subclause 5.6.

6 Test specimens

See ISO 6721-1:1994, clause 6.

6.1 Shape and dimensions

Test specimens in the form of rectangular bars or cylindrical rods are recommended. The width and thick-

ness of the bars and the diameter of the rods shall not vary along the specimen length by more than 2 % of a mean value. Dimensions of the specimens are not critical, although length corrections for clamping effects can be minimized by increasing the length of the specimen and, for rectangular specimens, these corrections become negligible for certain values of b/d (see 10.1 and 10.2.4). For test conditions under which the storage moduli are high (≥ 1 GPa), sufficiently long, thin specimens should preferably be employed so that angular displacements are generated that may be measured with high accuracy. Alternatively, when the storage moduli are low (< 100 MPa), relatively short, thick specimens may be required to achieve sufficient accuracy in the measurement of torque.

NOTE 2 A variation in dynamic properties may be observed between specimens of different thickness prepared by injection moulding owing to slight differences which may be present in the structure of the polymer in each specimen.

6.2 Preparation

See ISO 6721-1:1994, subclause 6.2.

7 Number of specimens

See ISO 6721-1:1994, clause 7.

8 Conditioning

See ISO 6721-1:1994, clause 8.

9 Procedure

9.1 Test atmosphere

See ISO 6721-1:1994, subclause 9.1.

9.2 Measuring the cross-section of the specimen

See ISO 6721-1:1994, subclause 9.2.

9.3 Clamping the specimen

Mount the specimen between the clamps using a clamping force that is sufficient to prevent slip under all test conditions. If measurements are observed to depend upon clamp pressure, then a constant pressure should preferably be used for all measurements, especially when applying a length correction (see 10.2.4 and note 3).

NOTE 3 If measurements are observed to depend upon clamp pressure, then the clamped area of the specimen is

probably too small. A larger clamp face or a wider specimen should eliminate this problem.

9.4 Varying the temperature

See ISO 6721-1:1994, subclause 9.4.

9.5 Performing the test

A dynamic torque shall be applied by the drive motor which yields torque and displacement amplitudes for the specimen that can be measured to the accuracy specified in 5.1.2.

NOTE 4 If the maximum shear strain within the specimen exceeds the limit for linear behaviour, then the derived dynamic properties will depend on the magnitude of the applied displacement. The limiting strain varies with the composition of the polymer and the temperature and is typically in the region of 0,2 % for glassy plastics.

The amplitudes of, the phase difference between and the frequency of the torque and displacement signals and the temperature of the test shall be recorded. Where measurements are to be made over ranges of frequency and temperature, it is recommended that the lowest temperature be selected first and measurements be made with increasing frequency, keeping the temperature constant. The frequency range is then repeated at the next higher temperature (see ISO 6721-1:1994, subclause 9.4).

For those test conditions under which the polymer exhibits medium or high loss (for example in the glass-rubber transition region), the energy dissipated by the polymer may raise its temperature sufficiently to give a significant change in dynamic properties. Any temperature rise will increase rapidly with increasing strain amplitude and frequency. If the data processing electronics is capable of analysing the transducer outputs within the first few cycles, then the influence of any temperature rise will be minimized. Subsequent measurements will then change with time as the specimen temperature continues to rise, and such observations will indicate the need to exercise some caution in the presentation and interpretation of results.

10 Expression of results

10.1 Symbols

L_a	length of specimen between the two clamps, in metres
l	length correction term for clamping, in metres
b	width of rectangular specimen, in metres
d	thickness of rectangular specimen, in metres

r	radius of cylindrical specimen, in metres
f	measurement frequency, in hertz
θ_A	measured amplitude of the dynamic angular displacement, in radians
T_A	measured amplitude of the dynamic torque applied to the specimen, in newton metres
δ_{Ga}, δ_G	measured phase difference and corrected phase difference, respectively, between the torque and angular-displacement cycles, in degrees
Γ_a, Γ	measured absolute value and corrected absolute value, respectively, of the torsional complex stiffness of the specimen, in newton metres per radian (N·m·rad ⁻¹)
G'_a, G'	apparent shear storage modulus and corrected shear storage modulus, respectively, in pascals
G''	shear loss modulus, in pascals
$\tan \delta_{Ga}, \tan \delta_G$	apparent shear loss factor and corrected shear loss factor, respectively
κ	shape factor giving the ratio of torsional complex stiffness to shear complex modulus per unit length of specimen, in metres to the power four per radian (m ⁴ ·rad ⁻¹)
I_p	polar second moment of area of the cross-section per unit specimen length, in metres to the power four (m ⁴)
Γ_T	torsional stiffness of the torque transducer, in newton metres per radian (N·m·rad ⁻¹)
I_T	moment of inertia of that part of the loading assembly between the torque transducer and the test specimen, in kilogram square metres (kg·m ²)
Γ_∞	measured torsional stiffness, in newton metres per radian (N·m·rad ⁻¹), of a steel test specimen whose cross-sectional dimensions and length are such that it is at least 100 times stiffer than the stiffest polymer specimen to be tested

NOTE 5 The magnitude of Γ_∞ will give an estimate of the torsional stiffness of the loading assembly, which is equivalent to a spring connected in series with the specimen, and will enable a correction for apparatus compliance to be deduced (see 10.2.3).

10.2 Calculation of the shear storage modulus G'

An approximate value for the storage modulus G'_a is determined from the equation

$$G'_a = \frac{T_A}{\theta_A} \times \frac{L_a}{\kappa} \cos \delta_{Ga} = \Gamma_a \times \frac{L_a}{\kappa} \cos \delta_{Ga} \quad \dots (1)$$

where the shape constant κ is calculated from the following equations:

Rectangular bar

$$\kappa = \frac{bd^3}{3} (1 - 0,63 d/b) \quad \text{for } 0 < \frac{d}{b} < 0,6$$

$$\kappa = \frac{bd^3}{3} \times \frac{0,843}{(1 + d^2/b^2)} \quad \text{for } 0,6 \leq \frac{d}{b} \leq 1$$

Cylindrical rod

$$\kappa = \frac{\pi r^4}{2}$$

10.2.1 Avoidance of specimen resonance

Equation (1) becomes invalid as the drive frequency approaches the fundamental torsional resonance frequency f_s of the specimen given approximately by

$$f_s = \frac{1}{2L_a} \left[\frac{\kappa G'_a}{\rho I_p} \right]^{1/2} \quad \dots (2)$$

where ρ is the polymer density in kilograms per cubic metre and I_p is given by the following equations:

Rectangular bar

$$I_p = \frac{bd}{12} (b^2 + d^2)$$

Cylindrical rod

$$I_p = \frac{\pi r^4}{2}$$

Errors in the use of equation (1) become significant at applied frequencies such that

$$f \geq 0,08 f_s \quad \dots (3)$$

Calculations of dynamic properties shall therefore be confined to frequencies below that given by the equality in equation (3).

10.2.2 Correction for transducer resonance

At sufficiently high frequencies, the applied deformation will excite the torque transducer into resonance. The resonance frequency f_T is given by

$$f_T = \frac{1}{2\pi} \left[\frac{\Gamma_T}{I_T} \right]^{1/2} \quad \dots (4)$$

The transducer output will have a significant error for all applied frequencies such that

$$f > 0,1 f_T \quad \dots (5)$$

The resonance frequency f_T of the torque transducer and supported inertia member can be determined directly by recording the natural frequency of the transducer output after applying a torque impulse to the attached clamp without specimen.

The torsional stiffness of the specimen corrected for transducer resonance is given to a good approximation by the equation

$$\Gamma = \Gamma_a \left[1 - \frac{4\pi^2 I_T f^2}{\Gamma_T} \right] = \Gamma_a \left[1 - \frac{f^2}{f_T^2} \right] \quad \dots (6)$$

It is recommended that equations (4) and (5) be used to select a torque transducer whose resonance frequency is above the frequency range for which a correction to the torque measurement is necessary.

10.2.3 Correction for apparatus compliance

If Γ_a is greater than $0,02 \Gamma_\infty$ then the torsional compliance of the test assembly is not negligible and the measured angular displacement differs significantly from that of the specimen. The following correction shall then be applied:

$$\Gamma \cos \delta_G = \frac{\Gamma_a (\cos \delta_{Ga} - \Gamma_a / \Gamma_\infty)}{1 - 2(\Gamma_a / \Gamma_\infty) \cos \delta_{Ga}} \quad \dots (7)$$

where δ_G is given by equation (9). The value of $\Gamma \cos \delta_G$ obtained from equation (7) shall be used in place of $\Gamma_a \cos \delta_{Ga}$ in equation (1) to give a more accurate estimate for G'_a .

NOTE 6 The compliance correction is unnecessary if the displacement transducer is located so as to measure the relative angular displacement of the two clamps.

10.2.4 Application of a length correction

Using the measured clamp separation L_a for the specimen length in equation (1) takes no account of some deformation of the specimen within the clamps or, in the case of rectangular bars, of restraints provided by the clamps on the out-of-plane warping of specimen cross-sections. These two effects may be allowed for by applying a small correction to L_a such that the effective length is $L_a + l$. Assuming that l is independent of L_a , equation (1) yields

$$G' = \Gamma \times \frac{(L_a + l)}{\kappa} \cos \delta_G = G'_a \times \frac{(L_a + l)}{L_a} \quad \dots (8)$$

Here G'_a is the apparent storage modulus corrected for apparatus compliance if necessary. A value for l may be determined from measurements of G'_a for a series of clamp separations L_a . From equation (8), a plot of L_a/G'_a against L_a enables l to be determined from the intercept at $L_a/G'_a = 0$ and G' from the gradient.

NOTE 7 The value of l will vary with the cross-sectional shape and dimensions of the specimen and with temperature if this causes significant changes in dynamic modulus. For rectangular specimens, the value of l may be either positive or negative depending on whether the effect of deformation within the clamps or of warping restraint is dominant. At a certain b/d ratio, which depends on the clamp design and other instrumental factors, these effects cancel to give a zero length correction.

10.3 Calculation of the shear loss factor

$\tan \delta_G$

An approximate value for the shear loss factor is given by $\tan \delta_{Ga}$. If Γ_a is greater than $0,02 \Gamma_\infty$ then the compliance of the loading assembly will influence the accuracy of the phase angle measurement. The loss factor shall then be obtained using

$$\tan \delta_G = \frac{\tan \delta_{Ga}}{1 - [(\Gamma_a / \Gamma_\infty) \cos \delta_{Ga}]} \quad \dots (9)$$

NOTE 8 If the origin of the source of compliance in the loading assembly arises through clamped or bolted connections, there may be a contribution from friction to the measured phase angle δ_{Ga} . The magnitude of the resulting error increases with the ratio Γ_a / Γ_∞ . This source of error can be avoided by locating the displacement transducer so that the relative displacement of the upper and lower clamps is measured.

10.4 Calculation of the shear loss modulus

The loss modulus G'' shall be calculated from

$$G'' = G' \tan \delta_G \quad \dots (10)$$

10.5 Presentation of data as a function of temperature

See ISO 6721-1:1994, subclause 9.4.

11 Precision


The precision of this test method is not known because interlaboratory data are not available.

When interlaboratory data are obtained, a precision statement will be added at the following revision.

12 Test report

The test report shall include the following information:

- a) a reference to this part of ISO 6721;
- b) to m) see ISO 6721-1:1994, clause 12, items b) to m);
- n) the maximum dynamic strain amplitude, given approximately by θ_{Ad}/L_a for rectangular bar specimens and by θ_{Ar}/L_a for cylindrical rods.

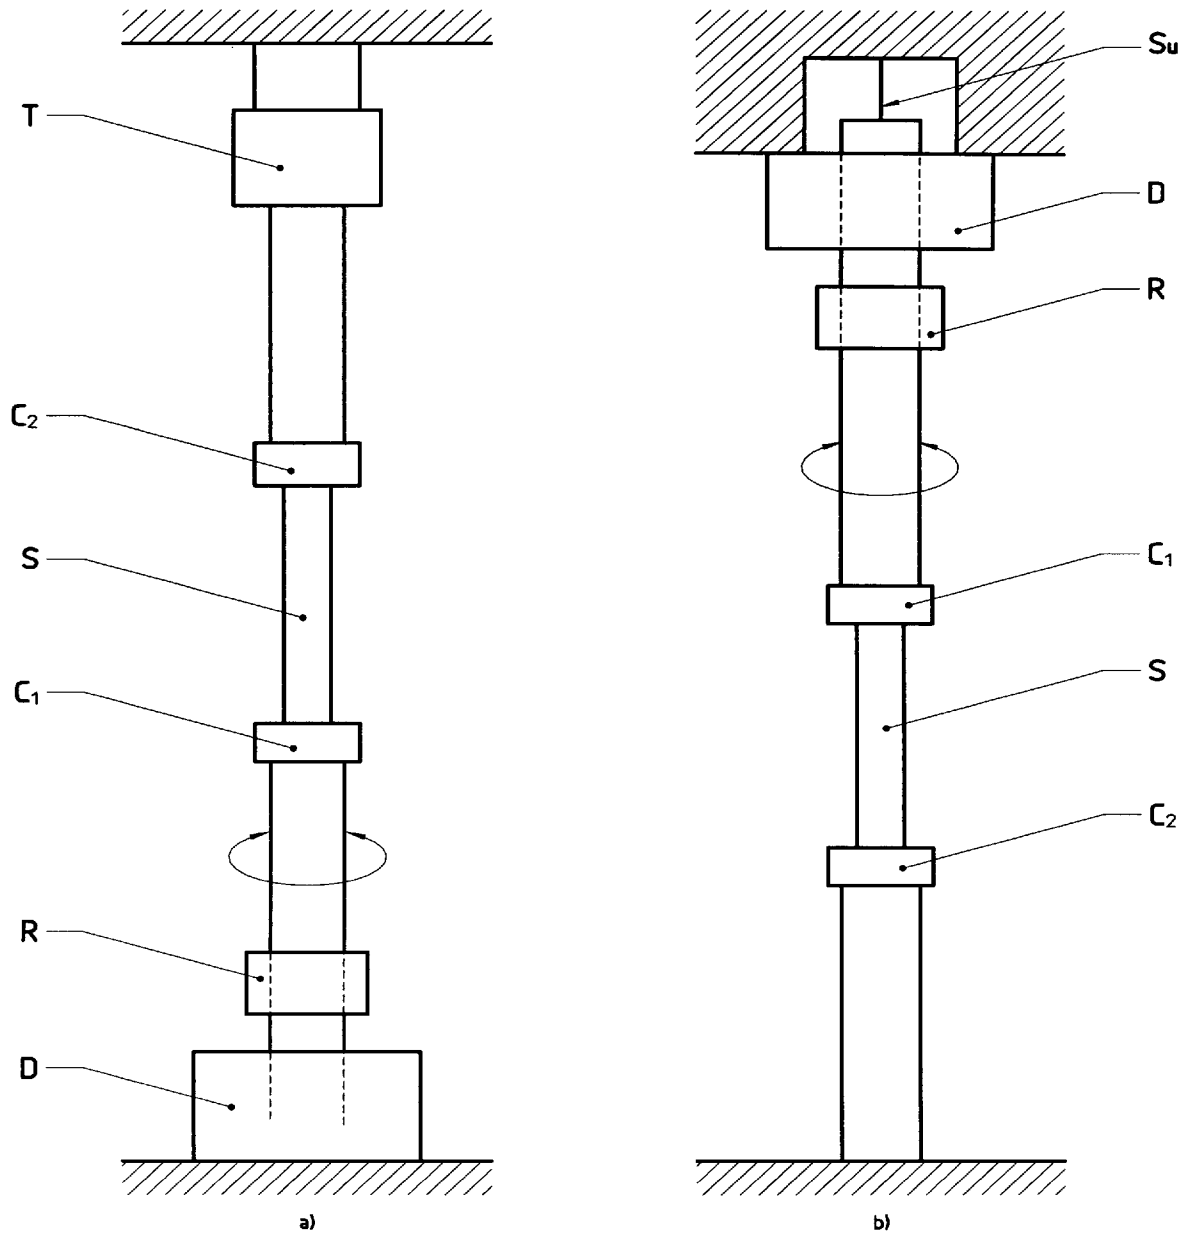

Key

- | | | | | | |
|---------------------------------|-------------------|---|--------------------------------|----|--------------------|
| T | Torque transducer | S | Test specimen | D | Angular drive unit |
| C ₁ , C ₂ | Clamps | R | Rotary displacement transducer | Su | Suspension |

NOTE — In figure 1a) the angular drive unit D and the torque transducer T are separate components, whereas in figure 1b) a single component D carries out both functions.

Figure 1 — Schematic diagrams of suitable loading assemblies for determining dynamic shear moduli by a forced torsional non-resonance method

ICS 83.080

Descriptors: plastics, rigid plastics, tests, mechanical tests, determination, mechanical properties, dynamic properties, shear modulus, test equipment.

Price based on 7 pages
