

INTERNATIONAL STANDARD

ISO 7786

Third edition
2001-04-01

Dental rotary instruments — Laboratory abrasive instruments

Instruments rotatifs dentaires — Instruments abrasifs de laboratoire



Reference number
ISO 7786:2001(E)

© ISO 2001

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

© ISO 2001

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.ch
Web www.iso.ch

Printed in Switzerland

Contents

Page

Foreword.....	iv
Introduction.....	v
1 Scope	1
2 Normative references	1
3 Symbols	1
4 Requirements	1
4.1 Materials	1
4.2 Shapes	2
4.3 Dimensions.....	2
4.4 Specifications for dental laboratory abrasive instruments.....	2
4.5 Run-out	7
5 Test procedures	7
5.1 Shapes	7
5.2 Dimensions.....	7
5.3 Run-out	7
6 Sampling and acceptance level (AQL)	7
7 Manufacturer's instructions.....	8
8 Marking on abrasive instruments	8
9 Labelling	8
10 Packaging	8
Bibliography	9

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this International Standard may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

International Standard ISO 7786 was prepared by Technical Committee ISO/TC 106, *Dentistry*, Subcommittee SC 4, *Dental instruments*.

This third edition cancels and replaces the second edition (ISO 7786:1990), which has been technically revised as follows:

- addition of new shape: Spherical;
- truncated conical: Nominal size 031;
- addition of requirement for manufacturer's instructions;
- addition of requirement for marking;
- addition of requirement for labelling.

Introduction

This International Standard is one of a series of standards relating to dental rotary instruments.

This International Standard contains the specifications for laboratory abrasive instruments. The various dimensional and other requirements specified for laboratory abrasive instruments are those considered important to ensure the interchangeability and safe usage of these grinding instruments in the dental laboratory.

The nominal diameters of the working part listed in Tables 1 to 10 comply with the diameters specified in ISO 2157.

Attention is drawn to the ISO 6360 series, which specifies a 15-digit numbering system for the identification of dental rotary instruments of all types.

Dental rotary instruments — Laboratory abrasive instruments

1 Scope

This International Standard specifies dimensional and other relevant requirements for the six most commonly available shapes of ceramic bonded abrasive instruments used for grinding in the dental laboratory, including a quality control and specifications for labelling of these instruments.

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 1797-1, *Dental rotary instruments — Shanks — Part 1: Shanks made of metals.*

ISO 2859-1, *Sampling procedures for inspection by attributes — Part 1: Sampling schemes indexed by acceptance quality limit (AQL) for lot-by-lot inspection.*

ISO 6360-2, *Dental rotary instruments — Number coding system — Part 2: Shape and specific characteristics.*

ISO 8325:1985, *Dental rotary instruments — Test methods.*

3 Symbols

For the purposes of this International Standard, the following symbols apply.

d diameter of working part, head diameter;

l_1 length of working part, head length;

l_2 overall length;

α angle of the working part.

4 Requirements

4.1 Materials

4.1.1 Working part

The working part shall be made of abrasive materials. The selection of the type and the treatment of the abrasive material shall be left to the discretion of the manufacturer.

4.1.2 Shank

The material of the shank shall comply with ISO 1797-1.

4.2 Shapes

The shapes of the working part shall be as specified in Figures 1 to 10. Variations of the shapes within the limited dimensions and the descriptions used in the subclause titles are permitted.

Testing shall be carried out in accordance with 5.1.

4.3 Dimensions

Dimensions in tables and figures are given in millimetres and angles are given in degrees.

4.3.1 Working part and overall length

The dimensions of the working part and the overall length shall be as specified in Figures 1 to 10 as appropriate and Tables 1 to 10 as appropriate.

Testing shall be carried out in accordance with 5.2.

4.3.2 Shank

The shank shall be Type 2 in accordance with ISO 1797-1.

4.4 Specifications for dental laboratory abrasive instruments

4.4.1 Spherical (round)

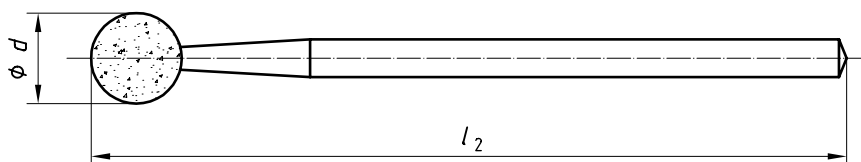


Figure 1 — Spherical (round)

Table 1 — Dimensions — Spherical (round)

Designation of nominal diameter (Nominal size)	d + 0,5 0	l_2 ± 3
031	3,1	45
040	4	46
050	5	47
060	6	48

4.4.2 Inverted truncated, conical

4.4.2.1 Inverted truncated, conical, short, $l_1 < d$

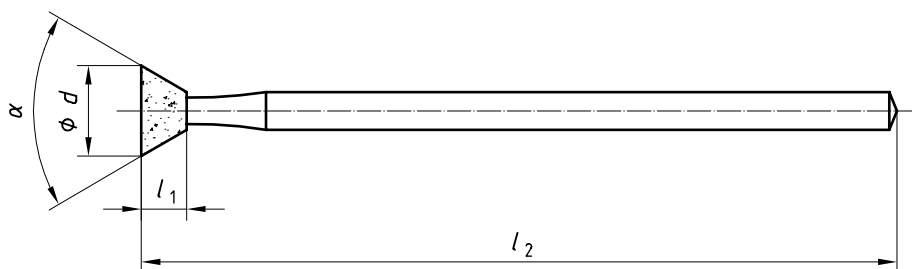


Figure 2 — Inverted truncated, conical, short

Table 2 — Dimensions — Inverted truncated, conical, short

Designation of nominal diameter (Nominal size)	d + 0,5 0	l_1 + 1 - 0,5	l_2 ± 3	α
040	4	2	42	50° to 90°
050	5	2,5	42	
060	6	3	42	
070	7	3,5	42	

4.4.2.2 Inverted truncated, conical, standard, $l_1 = d$

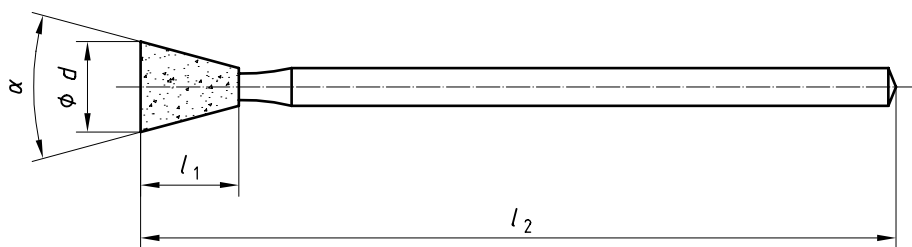


Figure 3 — Inverted truncated, conical, standard

Table 3 — Dimensions — Inverted truncated, conical, standard

Designation of nominal diameter (Nominal size)	d + 0,5 0	l_1 + 0,5 0	l_2 ± 3	α
065	6,5	6,5	48	20° to 30°

4.4.3 Inverted conical (hyperboloidal-inverted)

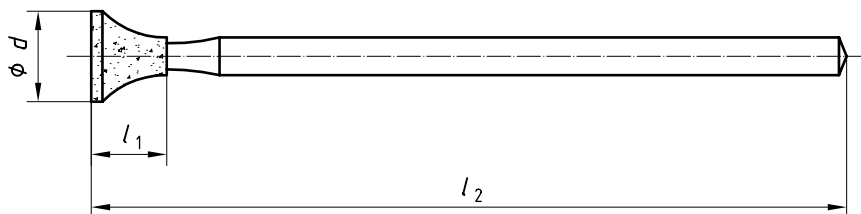


Figure 4 — Inverted conical (hyperboloidal-inverted)

Table 4 — Dimensions — Inverted conical (hyperboloidal-inverted)

Designation of nominal diameter (Nominal size)	d + 0,5 0	l_1 + 0,5 0	l_2 ± 3
070	7	5	46

4.4.4 Cylindrical

4.4.4.1 Cylindrical, short, $l_1 < d$

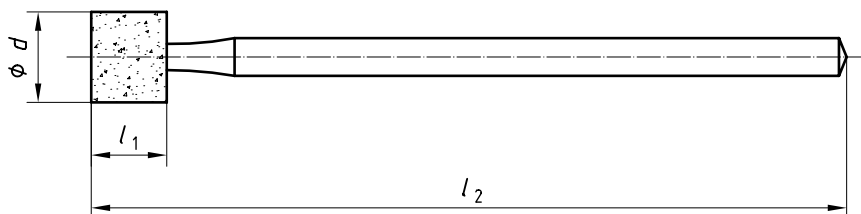


Figure 5 — Cylindrical, short

Table 5 — Dimensions — Cylindrical, short

Designation of nominal diameter (Nominal size)	d + 0,5 0	l_1 + 1 - 0,5	l_2 ± 3
060	6	3	44
060	6	5	44
100	10	2	44
100	10	3	44
100	10	4	44

4.4.4.2 Cylindrical, regular, $l_1 > d$

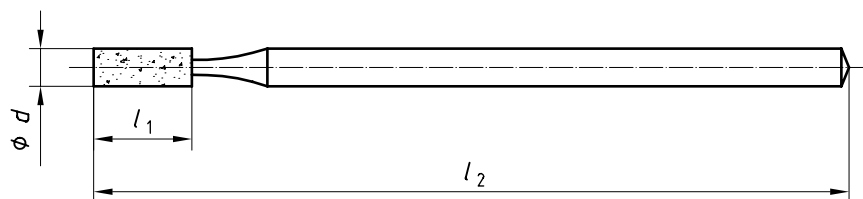


Figure 6 — Cylindrical, regular

Table 6 — Dimensions — Cylindrical, regular

Designation of nominal diameter (Nominal size)	d + 0,5 0	l_1 + 1 - 0,5	l_2 ± 3
021	2,1	6	44
031	3,1	6	44
040	4	6	44
050	5	6	44

4.4.4.3 Cylindrical, long, $l_1 \geq 2d$

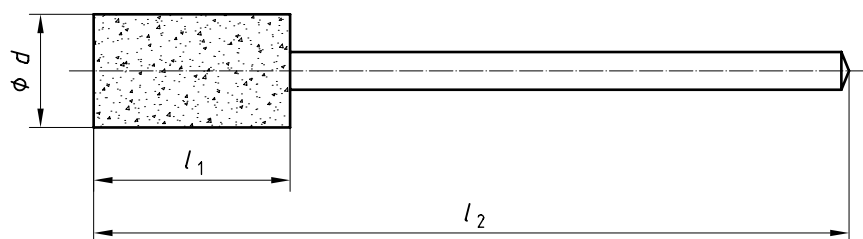


Figure 7 — Cylindrical, long

Table 7 — Dimensions — Cylindrical, long

Designation of nominal diameter (Nominal size)	d + 0,5 0	l_1 + 1 - 0,5	l_2 ± 3
050	5	12	48
065	6,5	13	50

4.4.5 Knife-edge (conico, inverted hyperboloidal)

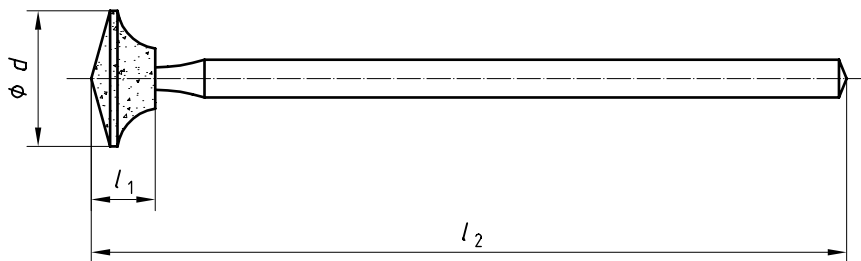


Figure 8 — Knife-edge (conico, inverted hyperboloidal)

Table 8 — Dimensions — Knife-edge (conico, inverted hyperboloidal)

Designation of nominal diameter (Nominal size)	d + 0,5 0	l_1 + 0,5 0	l_2 ± 3
090	9	4	46

4.4.6 Truncated conical

4.4.6.1 Truncated conical, regular, $l_1 > d$

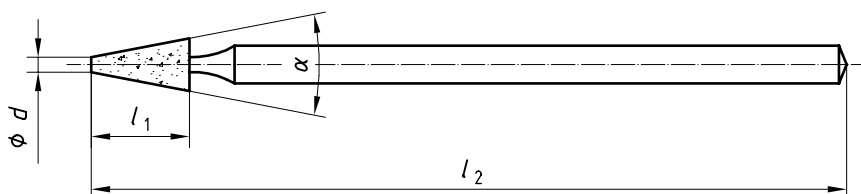


Figure 9 — Truncated conical, regular

Table 9 — Dimensions — Truncated conical, regular

Designation of nominal diameter (Nominal size)	d + 0,5 0	l_1 + 1 - 0,5	l_2 ± 3	α
021	2,1	6	44	8° to 14°
031	3,1	6	44	
040	4	6	44	
050	5	6	44	

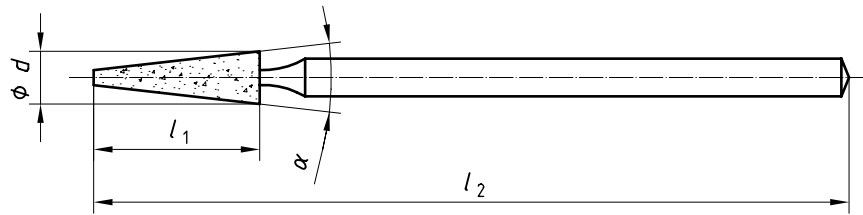
4.4.6.2 Truncated conical, long, $l_1 > 2d$ 

Figure 10 — Truncated conical, long

Table 10 — Dimensions — Truncated conical, long

Designation of nominal diameter (Nominal size)	d + 0,5 0	l_1 + 1 - 0,5	l_2 ± 3	α
031	3,1	7	46	6° to 10°
035	3,5	10,5	53	

4.5 Run-out

The run-out shall not exceed 0,3 mm.

Testing shall be carried out in accordance with 5.3.

5 Test procedures

5.1 Shapes

Determine the shapes by using a shadowgraph or measuring the relevant dimensions in accordance with ISO 8325.

5.2 Dimensions

Measure the dimensions in accordance with ISO 8325.

5.3 Run-out

Determine the run-out in accordance with ISO 8325.

Measurement shall be made at the largest diameter or, for the cylindrical form, at the middle of the working part.

6 Sampling and acceptance quality level (AQL)

The acceptance quality level (AQL) determined in accordance with ISO 2859-1 shall be 6,5.

7 Manufacturer's instructions

The manufacturer shall provide information on maximum rotational speed.

8 Marking on abrasive instruments

Marking on abrasive instrument may contain information on the abrasive material.

9 Labelling

Labelling on the package of abrasive instruments shall contain at least the following information:

- a) name and/or trade mark of manufacturer or distributor;
- b) material of the working part, identification of abrasive material;
- c) type of shank, in accordance with ISO 1797-1;
- d) shape number, in accordance with ISO 6360-2;
- e) specific characteristics;
- f) nominal diameter, nominal size;
- g) lot number.

The information should preferably be given in accordance with the appropriate part of ISO 6360.

10 Packaging

Abrasive instruments are packaged at the discretion of the manufacturer.

.....

Bibliography

- [1] ISO 2157, *Dental rotary instruments — Nominal diameters and designation code number.*
- [2] ISO 6360-1, *Dental rotary instruments — Number coding system — Part 1: General characteristics.*

.....

ICS 11.060.20

Price based on 9 pages

© ISO 2001 – All rights reserved