
**Cereals — Determination of bulk density,
called mass per hectolitre —**

Part 2:

**Method of traceability for measuring
instruments through reference
to the international standard instrument**

*Céréales — Détermination de la masse volumique, dite masse
à l'hectolitre —*

*Partie 2: Méthode de raccordement des instruments de mesure
à l'étalon international*



Reference number
ISO 7971-2:2009(E)

© ISO 2009

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



COPYRIGHT PROTECTED DOCUMENT

© ISO 2009

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword.....	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions.....	1
4 Requirements	2
4.1 Certified international or national standard instrument	2
4.2 National standard instrument.....	2
4.3 Secondary or internal standard instrument.....	2
4.4 Routine measuring instrument.....	2
5 Principle	3
6 Apparatus	3
7 Procedure	4
7.1 Traceability of national standard instruments through reference to the certified international or national standard instrument.....	4
7.2 Traceability of the secondary standard instruments through reference to the national standard instrument	6
7.3 Verification of instruments in operation.....	7
8 Monitoring of instrument performance	9
9 Test reports	9
9.1 Analysis certificate	9
9.2 Conformity certificate.....	10
10 Identification of traced measuring instruments	10
Annex A (normative) Method for calculation of performance parameters of standard instruments and of measurement instruments.....	11
Annex B (informative) Some owners of certified standard measurement instruments.....	18
Bibliography	19

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 7971 (all parts) was prepared by the European Committee for Standardization (CEN) Technical Committee CEN/TC 338, *Cereal and cereal products*, in collaboration with Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 4, *Cereals and pulses*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This edition is the second to bear the number ISO 7971-2, but the technical content is new. ISO 7971-3:2009 cancels and replaces the first edition (ISO 7971-2:1995).

ISO 7971 consists of the following parts, under the general title *Cereals — Determination of bulk density, called mass per hectolitre*:

- *Part 1: Reference method*
- *Part 2: Method of traceability for measuring instruments through reference to the international standard instrument*
- *Part 3: Routine method*

Cereals — Determination of bulk density, called mass per hectolitre —

Part 2: Method of traceability for measuring instruments through reference to the international standard instrument

1 Scope

This part of ISO 7971 specifies a test method for ensuring the traceability of mass per hectolitre measuring instruments through reference to standard measurement instruments. The mass per hectolitre or bulk density is of commercial importance for grain cereals. Several types of instruments with varying performances exist for measuring it.

This part of ISO 7971 also specifies the performances required of national standards instruments, secondary standards instruments, and measuring instruments used in laboratories or in collection or storage silos.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 712, *Cereals and cereal products — Determination of moisture content — Reference method*

ISO 7971-1, *Cereals — Determination of bulk density, called “mass per hectolitre” — Part 1: Reference method*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

bulk density **“mass per hectolitre”**

(cereals) ratio of the mass of a cereal to the volume it occupies after being poured into a container under well-defined conditions

NOTE Bulk density is expressed in kilograms per hectolitre of grains as received.

[ISO 7971-1:2009]

3.2

traceability

(cereals) establishment of a relationship between the usual measuring instrument and the international standard instrument via a chain

3.3 analysis certificate
document supplied by the international standard instrument holder body or national standard instrument holder body containing the individual values of measurements, the mass per hectolitre average value and its uncertainty for the test sample being analysed

3.4 conformity certificate
document, issued by the body in charge of verifying the performances of the instrument, specifying the conformity decision for the requested use

3.5 control chart
chart on which some statistical measure of a series of samples is plotted in a particular order to steer the process with respect to that measure and to control and reduce variation

[ISO 3534-2:2006^[1], 2.3.1]

NOTE The analysis values are plotted on the ordinate against the date (day or hour) of carrying out the measurement on the abscissa.

4 Requirements

4.1 Certified international or national standard instrument

A standard measurement instrument for mass per hectolitre has a 20 l hopper and is certified by a national or international authority. An informative list of such instruments is given in Annex B.

4.2 National standard instrument

Each country defines, on the basis of the specifications given in 6.2, the instrument designated as a national standard instrument within the respective country.

This national standard instrument should be an instrument designated by its name (model, manufacturer, serial number). Any other instrument of the same model as that adopted as the national standard instrument shall not be referred to as a "national standard instrument".

Each country defines the public or private organization responsible for the safe keeping, use, and maintenance of this national standard instrument. This same organization ensures its traceability through reference to a certified international or national standard instrument (4.1), according to the provisions specified in 7.1, every 10 years.

Each country shall ensure that no natural or legal person is refused access to the results of this national standard instrument so that any manufacturer, holder, repairer, controller or user can ensure the traceability of his own instruments through reference to the national standard instrument.

4.3 Secondary or internal standard instrument

For the purposes of inspection of instruments in operation, a body may possess an appliance specific to this activity. This instrument shall have the required qualities, established using the national standard instrument. It shall then constitute the reference which ensures the traceability of the instruments in operation.

Verify and adjust these secondary standard instruments every 2 years in accordance with 7.2.

4.4 Routine measuring instrument

This term designates any mass per hectolitre measuring instrument used in commercial transactions.

The traceability of instruments in operation and of new instruments (prior to commissioning) shall be ensured through reference to a secondary standard instrument (4.3) according to the provisions specified in 7.3.

The frequency of this traceability operation is 1 year.

5 Principle

This part of ISO 7971 specifies a procedure for ensuring the traceability of mass per hectolitre measuring instruments through reference to standard instruments.

The traceability principle is illustrated by Figure 1.

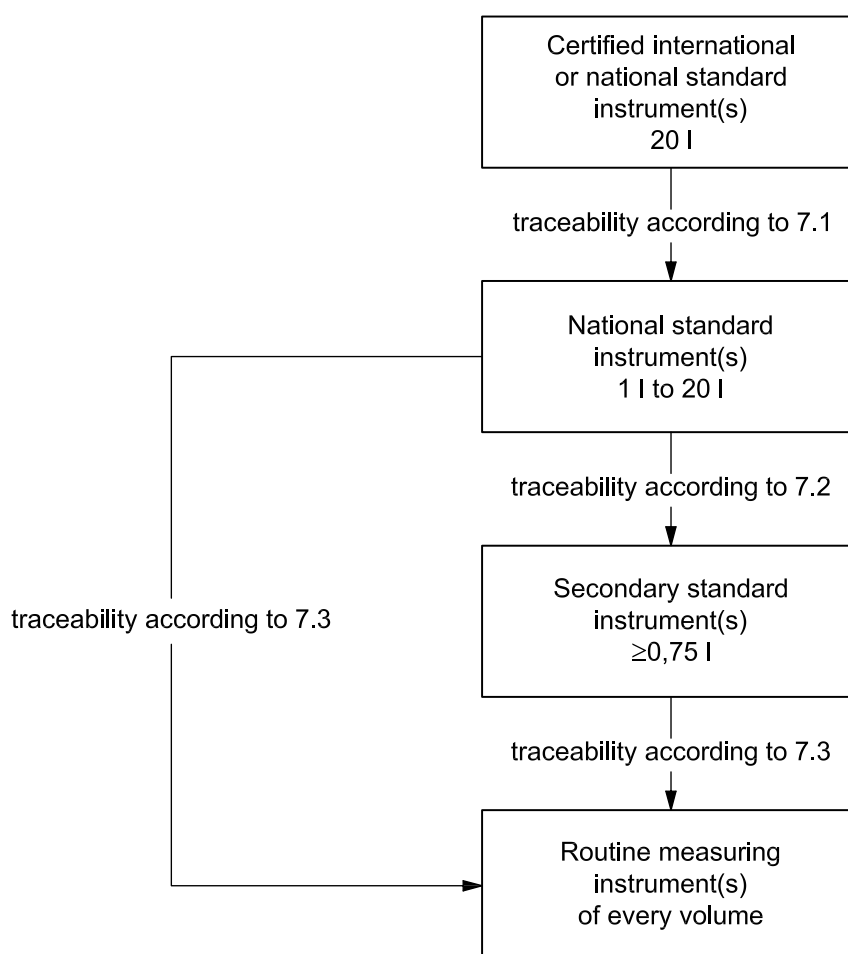


Figure 1 — Principle of traceability of instruments through reference to standard instruments

6 Apparatus

6.1 International standard instrument for mass per hectolitre as specified in ISO 7971-1.

6.2 National standard instrument for mass per hectolitre. Manual or automatic, mechanical, electric or electronic mass per hectolitre measuring instrument, of which the capacity of the measuring container is at least 1 l, accepting a bias correction or a bias and slope correction.

This instrument is used according to the requirements given in 4.2 and traceability is ensured through reference to the international standard instrument according to the procedure specified in 7.1.

The correction made to the instrument ensures a slope and an intercept which are not significantly different from 1 and 0 at the 5 % threshold [see Equations (A.8), (A.9), and (A.10), A.7.3 and A.8.2].

If the national standard instrument is a 20 l apparatus, for any correction refer to ISO 7971-1.

6.3 Secondary standard instrument for the mass per hectolitre. Manual or automatic, mechanical, electric or electronic mass per hectolitre measuring instrument, of which the capacity of the measuring container is at least 750 ml, accepting a bias and/or slope correction.

This instrument is used according to the requirements given in 4.3 and traceability is ensured through reference to the national standard instrument according to the procedure specified in 7.2.

The correction made to the instrument ensures a slope and an intercept which are not significantly different from 1 and 0 at the 5 % threshold [see Equations (A.8), (A.9), and (A.10), A.7.3 and A.8.2].

6.4 Mass per hectolitre measuring instrument. Manual or automatic, mechanical, electric or electronic, adjustable or fixed mass per hectolitre measuring instrument, associated if necessary with an equivalence or correction table and used according to the requirements given in 4.4.

The verification of these instruments specified in 7.3 concerns both new instruments and instruments in operation.

The amplitude between the highest and the lowest value, $\Delta\rho_i$, measured on each control sample (see 7.3.4), shall not exceed 0,3 kg/hl.

For each control sample, the difference between the value given by the national standard instrument or the secondary standard instrument and the mean of the measurements carried out on the instrument, $\Delta\rho_{i,2-m}$, (see 7.3.4), shall not exceed 0,3 kg/hl for mass per hectolitre under 70 kg/hl and 0,4 kg/hl for mass per hectolitre greater than or equal to 70 kg/hl.

6.5 Divider. Manual or mechanical cone-shaped divider that can representatively reduce a 25 l volume of grains to a volume suited to the instruments to undergo traceability.

7 Procedure

7.1 Traceability of national standard instruments through reference to the certified international or national standard instrument

7.1.1 General description

The traceability of national standard instruments is conducted using a series of test samples referenced with their mass per hectolitre and accompanied by their analysis certificate (3.3). The use of wheat and barley test samples is recommended because of the regular shape of the grain and the good availability of these species of grains. Other seeds with regular shape of grain, e.g. triticale or rye, can be used if performance requirements are fulfilled. The use of grains with inhomogeneous shape, e.g. oats, is not advisable.

7.1.2 Preparation of the test samples

Select three test samples of common wheat and/or durum wheat and three test samples of barley having the following characteristics:

- a) for wheat (common or durum), one test sample with a mass per hectolitre in each of the following ranges: 72 kg/hl to 76 kg/hl, 75 kg/hl to 79 kg/hl, and 78 kg/hl to 82 kg/hl;
- b) for barley, one test sample with a mass per hectolitre in each of the following ranges: 60 kg/hl to 64 kg/hl, 65 kg/hl to 69 kg/hl, and 70 kg/hl to 74 kg/hl;

- c) a minimum difference between two successive test samples of at least 2 kg/hl;
- d) an approximate mass of 30 kg, packed in correctly identified, rigid, airtight containers;
- e) a moisture content (mass fraction) between 9 % and 14 % (as determined by ISO 712);
- f) freedom from abnormal odours and from live insects, not containing any heterogeneous impurities of a size over 10 mm and guaranteeing a residual impurity content below 2 % mass fraction.

Dispatch the six test samples prepared in this manner to an owner of a certified standard measurement instrument (see list in Annex B) for determination of their mass per hectolitre and of the uncertainty associated with this quantity.

When these test samples come back, if they have to be stored prior to use, place them in ambient conditions which do not affect their properties: temperature below 22 °C and relative humidity below 60 %. Do not store these test samples at negative temperatures.

EXAMPLES

A set of test samples with masses per hectolitre of 73 kg/hl, 76 kg/hl, and 80 kg/hl for wheat and 60 kg/hl, 66 kg/hl, and 71 kg/hl for barley is suitable.

A set of test samples with masses per hectolitre of 73 kg/hl, 74 kg/hl, and 80 kg/hl for wheat and 60 kg/hl, 65 kg/hl, and 66 kg/hl for barley is not suitable because there is less than 2 kg/hl between two of the three test samples of each type.

A set of test samples with masses per hectolitre of 70 kg/hl, 73 kg/hl, and 76 kg/hl for wheat and 66 kg/hl, 68 kg/hl, and 70 kg/hl for barley is not suitable because the total range is not covered.

7.1.3 Use of the referenced test samples

If the mass per hectolitre referenced test samples have been stored in a refrigerating chamber, it is necessary to wait until their temperature has reached equilibrium with that of the premises where the tests are being carried out before opening the containers.

If the volume of the referenced test samples is such that they cannot be fully used in the national standard instrument, constitute test portions of appropriate mass, which are representative of the initial test sample, using a divider.

Select three of these test portions and conduct a mass per hectolitre measurement on each of them using the national standard instrument or, if the test samples can be used in their entirety, measure each of them three times. Three individual values marked ρ_{i1} to ρ_{i3} , where i represents the serial number of the referenced sample, are thus obtained.

When equipment using a cutting edge is employed, the test sample shall not be analysed more than 50 times. After that the test sample has to be replaced.

7.1.4 Interpretation of the results

From the unit results obtained on the control test samples, calculate the performance parameters according to the relevant equations in Annex A.

Check that the specifications defined for the national standard instrument in 6.2 are fulfilled. If so, draw up the national standard instrument conformity certificate.

If not, adjust the national standard instrument according to 7.1.5. In the event of it being impossible to obtain the specifications requested in 6.2, the national standard instrument shall be repaired or declassified then replaced by another instrument in order to re-obtain the required performances.

The national standard instrument holder shall keep all of the data (raw and calculated) relative to this traceability operation throughout the instrument's lifetime.

7.1.5 Adjustment of the national standard instrument

If the slope a and the intercept b calculated in 7.1.4 are outside the limits specified in 6.2, introduce into the instrument, according to the manufacturer's recommendations, the necessary correction factors required to theoretically bring the slope to 1 and the intercept to 0.

Then resume the operations specified in 7.1.3 and 7.1.4 in order to verify the validity of this correction.

7.2 Traceability of the secondary standard instruments through reference to the national standard instrument

7.2.1 General description

The traceability of the secondary standards is conducted using a series of test samples referenced with the mass per hectolitre obtained with the national standard instrument (6.2). The use of wheat and barley test samples is recommended because of the regular shape of the grain and the availability of these species of grains. Other seeds with regular shape of grain, e.g. triticale or rye, can be used if performance requirements are fulfilled. The use of grains with inhomogeneous shape, e.g. oats, is not advisable.

7.2.2 Preparation of the test samples

Select three test samples of common wheat and/or durum wheat and three test samples of barley having the following characteristics:

- a) for wheat (common or durum), one test sample with a mass per hectolitre in each of the following ranges: 72 kg/hl to 76 kg/hl, 75 kg/hl to 79 kg/hl, and 78 kg/hl to 82 kg/hl;
- b) for barley, one test sample with a mass per hectolitre in each of the following ranges: 60 kg/hl to 64 kg/hl, 65 kg/hl to 69 kg/hl, and 70 kg/hl to 74 kg/hl;
- c) a minimum difference between two successive test samples of at least 2 kg/hl;
- d) sufficient quantity for measurement on the national standard instrument (1,5 l to 25 l), packed in correctly identified, rigid, airtight containers;
- e) a moisture content (mass fraction) between 9 % and 14 % (as determined by ISO 712);
- f) freedom from abnormal odours and from live insects, not containing any heterogeneous impurities of a size over 10 mm and guaranteeing a residual impurity content below 2 % mass fraction.

Dispatch the six thus prepared test samples to the national standard instrument holder body for determination of their mass per hectolitre and of the uncertainty associated with this quantity.

When these test samples come back, if they have to be stored prior to use, place them in ambient conditions which do not affect their properties: temperature below 22 °C and relative humidity below 60 %. Do not store these test samples at negative temperatures.

NOTE See 7.1.2 for examples of suitable sets of test samples.

7.2.3 Use of the referenced test samples

If the mass per hectolitre referenced test samples have been stored in a refrigerating chamber, it is necessary to wait until their temperature has reached equilibrium with that of the premises where the tests are being carried out before opening the containers.

If the volume of the referenced test samples is such that they cannot be fully used in the secondary standard instrument, constitute test portions of appropriate mass, which are representative of the initial test sample, using a divider.

Select three of these test portions and conduct a mass per hectolitre measurement on each of them using the secondary standard instrument or, if the test samples can be entirely used, measure each of them three times. Three individual values marked ρ_{i1} to ρ_{i3} , where i represents the serial number of the referenced sample, are thus obtained.

When equipment using a cutting edge is employed, the test sample shall not be analysed more than 50 times. After that the test sample shall be replaced.

7.2.4 Interpretation of the results

From the unit results obtained on the control test samples, calculate the performance parameters according to the relevant equations in Annex A.

Check that the specifications defined for the secondary standard instrument (6.3) are fulfilled. If so, draw up the secondary standard conformity certificate.

If not, adjust the secondary standard instrument according to 7.2.5. In the event of it being impossible to obtain the specifications requested in 6.3, the secondary standard shall be repaired or declassified then replaced by another instrument in order to re-obtain the required performances.

The secondary standard instrument holder shall keep all of the data (raw and calculated) relative to this traceability operation throughout the instrument's lifetime.

7.2.5 Adjustment of the secondary standard instrument

If the slope a and the intercept b calculated in 7.2.4 are outside the limits specified in 6.3, introduce into the instrument, according to the manufacturer's recommendations, the necessary correction factors required to theoretically bring the slope to 1 and the intercept to 0.

Then resume the operations specified in 7.2.3 and 7.2.4 in order to verify the validity of this correction.

7.3 Verification of instruments in operation

7.3.1 General description

The traceability of instruments in operation is carried out using a series of four control test samples of which the mass per hectolitre has been previously measured using a secondary standard (6.3) or, failing this, using a national standard instrument (6.2). The use of wheat and barley test samples is recommended because of the regular shape of the grain and the availability of these species of grains. Other seeds with regular shape of grain, e.g. triticale or rye, can be used if performance requirements are fulfilled. The use of grains with inhomogeneous shape, e.g. oats, is not advisable.

7.3.2 Preparation of the control test samples

Select two test samples of common wheat and/or durum wheat and two test samples of barley having the following characteristics:

- a) for wheat (common and durum), one test sample with a mass per hectolitre in each of the following ranges: 72 kg/hl to 78 kg/hl and 77 kg/hl to 83 kg/hl;
- b) for barley, one test sample with a respective mass per hectolitre in each of the following ranges: 61 kg/hl to 67 kg/hl and 67 kg/hl to 73 kg/hl;
- c) a minimum difference between two successive test samples of at least 5 kg/hl;

- d) sufficient quantity for measurement on the secondary standard, packed in correctly identified, rigid, airtight containers;
- e) a moisture content (mass fraction) between 9 % and 14 % (as determined by ISO 712);
- f) freedom from abnormal odours and from live insects, not containing any heterogeneous impurities of a size over 10 mm and guaranteeing a residual impurity content below 2 % mass fraction.

Measure or have measured the mass per hectolitre of these four test samples on a secondary standard instrument traced according to the provisions specified in 7.2. The period of validity of the analysis certificate specifying these values shall not exceed 1 year.

Store these test samples under ambient conditions which do not affect their properties: temperature below 22 °C and relative humidity below 60 %. Do not store these test samples at negative temperatures.

Each test sample may be used a maximum of 50 times. After this number of uses, each test sample shall be re-referenced using the secondary standard instrument (or the national standard instrument). When equipment using a cutting edge is employed, the test sample shall not be analysed more than 50 times. After that the test sample shall be replaced.

7.3.3 Use of the referenced test samples

If the referenced test samples are stored in cold conditions, it is necessary to wait until their temperature has reached equilibrium with that of the premises where the tests are being carried out before opening the containers.

If the volume of the referenced test samples is such that they cannot be fully used in the instrument to be controlled, divide each test sample with the appropriate means in order to obtain test portions which are representative of each overall test sample having a size suited to the instrument to be controlled and select one of these test portions. Otherwise, use each test sample in its entirety.

For each test sample or test portion, carry out two measurements using the instrument to be checked. If provided for by the instrument's method of use, calculate the final result of the measurement using an equation or an equivalence table. One thus has, for each of the four referenced test samples, two individual values designated ρ_{i1} to ρ_{i2} , where i represents the serial number of each control test sample.

7.3.4 Interpretation of the results

For each control test sample, calculate the quantities listed.

The amplitude (magnitude of the difference) between the highest and the lowest measurement, $\Delta\rho_i$, is given by

$$\Delta\rho_i = |\rho_{i1} - \rho_{i2}|$$

The mean of the two measurements, $\bar{\rho}_i$, is given by

$$\bar{\rho}_i = \frac{\rho_{i1} + \rho_{i2}}{2}$$

The difference between the referenced value obtained on the secondary (or national) standard instrument, $\rho_{i,m}$, and the measuring instrument, $\bar{\rho}_i$, to undergo traceability, $\Delta\rho_{i,2-m}$, is given by

$$\Delta\rho_{i,2-m} = |\rho_{i,m} - \bar{\rho}_i|$$

If the specifications given in 6.4 are obtained, produce the conformity certificate (9.2) and mark the instrument as specified in Clause 10. Otherwise, adjust by following 7.3.5.

7.3.5 Adjustment of the instrument

If the instrument is an adjustable model, adjust its bias according to the manufacturer's recommendations. Resume the operations specified in 7.3.3 and 7.3.4 in order to verify the validity of this adjustment.

If specifications given in 6.4 are not obtained and the instrument cannot be adjusted, this one is unfit for this purpose and shall not be used.

8 Monitoring of instrument performance

To protect oneself against a possible drift between two traceability operations of national standard instruments and secondary standard instruments, a self-control system should be set up by using a control chart (3.5). The control chart measures whether the performances remain within the defined limits at a given point.

Control and surveillance limits are plotted on the graph. These fixed limits are usually estimated at $3s_{ILR}$, where s_{ILR} is an intralaboratory reproducibility standard deviation, corresponding to a risk, α , of 0,2 %, for the control limits and $2s_{ILR}$, corresponding to a risk, α , of 5 %, for the surveillance limits. They are located on either side of a *central line* corresponding to the so-called reference value. The intralaboratory reproducibility standard deviation is calculated on 30 measurements (six measurements per day for 5 days) on the same test sample.

Each time those standard instruments are used, a test sample referenced with its mass per hectolitre is analysed. The value obtained is plotted on the control chart and decision rules are applied in order to decide whether the system is to be corrected.

The following are generally selected:

- a) any value between the surveillance limits and the control limits indicates correct performance;
- b) any distribution which makes one suspect a non-random distribution indicates that close surveillance of the instrument is required and correction necessary if a systematic bias persists;
- c) three consecutive points all located above or below the surveillance limit indicates close surveillance of the instrument is required in order to launch, if necessary, a new traceability operation;
- d) one point outside the control limit indicates the need for the immediate performance of a new traceability operation in order to carry out the adequate setting.

9 Test reports

9.1 Analysis certificate

The test report establishing the mass per hectolitre of a referenced test sample shall include at least the following information:

- a) all information required for the complete identification of the test sample;
- b) the method used together with reference to this part of ISO 7971;
- c) the final result obtained;
- d) the uncertainty associated with this result;
- e) all operating details not specified in this part of ISO 7971, or regarded as optional, together with details of any incidents which may have influenced the test result(s).

9.2 Conformity certificate

The certificate establishing the traceability of a standard or the conformity of an instrument in operation shall include at least the following information:

- a) all information required for the complete identification of the instrument (manufacturer, model, serial number, etc.);
- b) the date of the tests and the identification of the operator who carried them out;
- c) the method and details used together with reference to this part of ISO 7971;
- d) the mean result of the measurements of each test sample, the corresponding reference value and the associated uncertainty;
- e) all operating details not specified in this part of ISO 7971, or regarded as optional, together with details of any incidents which may have influenced the test result(s).

10 Identification of traced measuring instruments

Measuring instruments used on a routine basis (6.4) for commercial transactions shall, once they have successfully undergone the traceability operations specified in 7.3, receive an identification mark specifying:

- a) INSTRUMENT TRACED THROUGH REFERENCE TO A CERTIFIED STANDARD MEASUREMENT INSTRUMENT FOR MASS PER HECTOLITRE;
- b) a reference to this part of ISO 7971;
- c) the date of the next traceability operation;
- d) the name of the body (public or private) which carried out the traceability operation.

Annex A (normative)

Method for calculation of performance parameters of standard instruments and of measurement instruments

A.1 Principle

The traceability of a measurement instrument to a standard instrument of superior level is made by a statistical validation of results obtained on this instrument with reference to the results obtained on the standard instrument.

This work consists of validation of an alternate method (the standard instrument to be traced) versus a reference method (the standard instrument of superior level). This annex gives the statistical tools to evaluate different criteria necessary to validate an alternative method. It specifies a check of freedom from bias by comparison of means and a specificity control by testing the slope and the intercept of the straight regression line between the two methods.

The evaluation of capacity of instruments to be traced is done by the same procedure in the case of traceability of a national standard instrument through a certified standard measurement instrument as in the case of traceability of a secondary standard through the national instrument.

A.2 Control of the freedom from bias by comparison of means

To make such calculations easier, the use of a spreadsheet with statistical treatment tools is strongly recommended. For example, it is possible to use the *t*-test on paired two samples of means available in the data analysis tool of Microsoft® Excel^{®1)}. Such an example is given in A.8.

For each referenced test sample, calculate the mean, $\bar{\rho}_i$, of the n measurements carried out on the instrument to undergo traceability according to Equation (A.1)

$$\bar{\rho}_i = \frac{\sum_{j=1}^n \rho_{ij}}{n} \quad (\text{A.1})$$

where n is the number of measurements for each test sample (normally, $n = 3$).

For each referenced test sample, calculate the difference, $\Delta\rho_{i,m-\text{ref}}$ between $\rho_{i,m}$ and the reference value, $\rho_{i,\text{ref}}$, then calculate the mean, $\Delta\rho$, of these m differences as well as their standard deviation, $s_{\Delta\rho}$.

$$\Delta\rho_{i,m-\text{ref}} = \rho_{i,m} - \rho_{i,\text{ref}} \quad (\text{A.2})$$

1) Microsoft® Excel[®] is an example of appropriate software available commercially. This information is given for the convenience of users of this part of ISO 7971 and does not constitute an endorsement by ISO of the product named. Other equivalent products can be used, provided that they give the same results.

$$\bar{\Delta\rho} = \frac{\sum_{i=1}^m \Delta\rho_{i,m-\text{ref}}}{m} \quad (\text{A.3})$$

$$s_{\Delta\rho} = \sqrt{\frac{\sum_{i=1}^m (\bar{\Delta\rho} - \Delta\rho_{i,m-\text{ref}})^2}{m-1}} \quad (\text{A.4})$$

where m is the number of referenced test samples used for the traceability (normally, $m = 6$).

Calculate the ratio t_{obs} according to Equation (A.5)

$$t_{\text{obs}} = \frac{|\bar{\Delta\rho}|}{s_{\Delta\rho}} \sqrt{m} \quad (\text{A.5})$$

Compare the t_{obs} value with a critical value, t_{val} , corresponding to that of a 5 % risk Student variable with five degrees of freedom.

If t_{obs} is lower than t_{val} , the means equality presumption is accepted.

A.3 Calculation of coordinates of the straight regression line and signification tests

To make such calculations easier, the use of a spreadsheet with statistical treatment tools is strongly recommended. For example, it is possible to use the regression tool available in the data analysis tool of Microsoft® Excel®⁽¹⁾. Such an example is given in A.8.

Calculate the coordinates of the straight regression line of slope, a , and intercept, b , between the means, $\rho_{i,m}$, found by the standard instrument to be traced on each referenced test sample with the values given by the standard instrument of superior level, $\rho_{i,\text{ref}}$, according to Equations (A.6) and (A.7):

$$a = \frac{m \sum_{i=1}^m \rho_{i,\text{ref}} \rho_{i,m} - \left(\sum_{i=1}^m \rho_{i,\text{ref}} \right) \left(\sum_{i=1}^m \rho_{i,m} \right)}{m \sum_{i=1}^m \rho_{i,m}^2 - \left(\sum_{i=1}^m \rho_{i,m} \right)^2} \quad (\text{A.6})$$

$$b = \bar{\rho}_{i,\text{ref}} - a \bar{\rho}_{i,m} \quad (\text{A.7})$$

where

m is the number of referenced test samples used for the traceability (normally, $m = 6$);

$\bar{\rho}_{i,m}$ are the means of masses per hectolitre based on the instrument to be traced for the m control test samples;

$\bar{\rho}_{i,\text{ref}}$ are the means of masses per hectolitre provided by the standard instrument of superior level for the same m control test samples.

A.4 Test for slope

Calculate the ratio t_{obs} according to Equation (A.8):

$$t_{\text{obs}} = \frac{|(1-a)| \sqrt{\sum_{i=1}^m (\rho_{i,m} - \bar{\rho}_{i,m})^2}}{s_a} \quad (\text{A.8})$$

where the slope standard deviation, s_a , is given by

$$s_a = \sqrt{\frac{\sum_{i=1}^m (\rho_{i,\text{ref}} - \bar{\rho}_{i,\text{ref}})^2 - a^2 \sum_{i=1}^m (\rho_{i,m} - \bar{\rho}_{i,m})^2}{m-2}} \quad (\text{A.9})$$

Compare the t_{obs} value with a critical value, t_{val} , corresponding to that of a 5 % risk Student variable with $m - 2$ degrees of freedom.

If t_{obs} is lower than t_{val} , the slope is not significantly different from 1.

A.5 Test for intercept

Calculate the ratio t'_{obs} according to Equation (A.10):

$$t'_{\text{obs}} = \frac{\sum_{i=1}^m (\rho_{i,m} - \rho_{i,\text{ref}})}{m} \sqrt{\frac{\sum_{i=1}^m (\rho_{i,m} - \rho_{i,\text{ref}})^2 - \frac{\left[\sum_{i=1}^m (\rho_{i,m} - \rho_{i,\text{ref}}) \right]^2}{m}}{m \times (m-1)}} \quad (\text{A.10})$$

Compare the t'_{obs} value with a critical value, t_{val} , corresponding to that of a 5 % risk Student variable with $m - 2$ degrees of freedom.

If t'_{obs} is lower than t_{val} , the intercept is not significantly different from 0.

A.6 Interpretation and conclusion

If tests for freedom from bias by comparison of means and/or the tests for slope and intercept are not satisfactory, the instrument to be traced shall be adjusted by correcting bias and slope according to the values specified in 7.1.5 or 7.2.5.

It is necessary to resume the measurements and calculations after this adjustment to verify the conformity of new results.

If the instrument is not adjustable, it cannot claim the status of a standard (national or secondary) and shall be replaced by a more powerful instrument that meets the required specifications.

A.7 Example of calculations

A.7.1 General

Each of six test samples is measured three times by the standard instrument then by the instrument to be traced. Results are given in Tables A.1 and A.2.

Table A.1 — Reference values, standard instrument

Reference values on standard instrument kg/hl	Test sample 1	Test sample 2	Test sample 3	Test sample 4	Test sample 5	Test sample 6	Average of all test samples
	$\rho_{1,ref}$	$\rho_{2,ref}$	$\rho_{3,ref}$	$\rho_{4,ref}$	$\rho_{5,ref}$	$\rho_{6,ref}$	
	65,70	68,23	70,23	74,53	77,23	80,53	72,74

Table A.2 — Instrument values

Instrument measurements		Test sample 1	Test sample 2	Test sample 3	Test sample 4	Test sample 5	Test sample 6	Average of all test samples
		$\rho_{1j,m}$	$\rho_{2j,m}$	$\rho_{3j,m}$	$\rho_{4j,m}$	$\rho_{5j,m}$	$\rho_{6j,m}$	
Measure 1 kg/hl	$\rho_{i1,m}$	65,9	68,0	70,0	74,4	77,1	80,5	
Measure 2 kg/hl	$\rho_{i2,m}$	65,8	68,0	70,1	74,4	77,1	80,6	
Measure 3 kg/hl	$\rho_{i3,m}$	66,0	68,1	70,0	74,5	77,1	80,7	
Averages kg/hl	$\rho_{i,m}$	65,90	68,03	70,03	74,43	77,10	80,60	72,68

A.7.2 Comparison of means

See Table A.3.

Table A.3 — Comparison of means

Comparison of averages	Test sample 1	Test sample 2	Test sample 3	Test sample 4	Test sample 5	Test sample 6	Average $\overline{\Delta\rho}$
Difference kg/hl $\Delta\rho_{i,m-ref}$	0,20	-0,20	-0,20	-0,10	-0,13	0,07	-0,06

	Sum						
$\overline{(\Delta\rho)^2}$	0,068	0,020	0,020	0,002	0,005	0,017	0,130

Standard deviation $s_{\Delta\rho}$	0,161
---	-------

Ratio	t_{obs}	0,913
Student 5 %	t_{val}	2,571

Conclusion

$t_{obs} < t_{val}$

The two means are not significantly different.
The two instruments give similar average results.

A.7.3 Calculations and tests for slope and intercept

See Table A.4.

Table A.4 — Calculations and tests for slope and intercept

Averages of measurements		Test sample 1	Test sample 2	Test sample 3	Test sample 4	Test sample 5	Test sample 6	Sum	Average
Standard	$\rho_{i,ref}$	65,70	68,23	70,23	74,53	77,23	80,53	436,45	72,74
Instrument	$\rho_{i,m}$	65,90	68,03	70,03	74,43	77,10	80,60	436,09	72,68
	$(\rho_{i,ref} - \bar{\rho}_{i,ref})^2$	49,59	20,36	6,31	3,20	20,15	60,66	160,25	
	$(\rho_{i,m} - \bar{\rho}_{i,m})^2$	45,99	21,64	7,03	3,06	19,52	62,70	159,94	
	$\rho_{i,m}^2$	4 342,81	4 628,08	4 904,20	5 539,82	5 944,41	6 496,36	31 855,69	
	$\rho_{i,ref} \rho_{i,m}$	4 329,63	4 641,69	4 918,21	5 547,27	5 954,43	6 490,72	31 881,94	
	$\rho_{i,m} - \rho_{i,ref}$	0,20	-0,20	-0,20	-0,10	-0,13	0,07	-0,36	
	$(\rho_{i,m} - \rho_{i,ref})^2$	0,040	0,040	0,040	0,010	0,017	0,005	0,152	
Slope	a	1,001	<p>Conclusion Slope is not significantly different from 1. The instrument is not skewed.</p> <p>Conclusion Intercept is not significantly different from 0. The instrument is not biased.</p>						
Intercept	b	0,019							
Slope standard deviation	s_a	0,180							
Test for slope	t_{obs}	0,040							
Student 5 %	t_{val}	2,776							
Test for intercept	t'_{obs}	0,911							
Student 5 %	t'_{val}	2,776							

A.8 Example of calculations using data analysis tool in Microsoft® Excel® 1)

A.8.1 Comparison of means

Use the *t*-test of paired two samples for means [on the “Tools” menu, select “Data analysis” (after downloading the “Analysis ToolPak”), select “t-Test: Paired Two Samples for Means”].

With the values given in Clause A.7, Table A.5 is obtained:

Table A.5 — *t*-Test: paired two sample for means

	Variable 1	Variable 2
Mean	72,73	72,69
Variance	32,33	31,81
Observations	6	6
Pearson correlation	0,999 7	
Hypothesized mean difference	0	
Degrees of freedom	5	
<i>T</i> stat	0,600 2	
$P(T \leq t)$ one-tail	0,245 2	
<i>t</i> Critical one-tail	2,015 0	
$P(T \leq t)$ two-tail	0,574 5	
<i>T</i> Critical two-tail	2,570 6	

A.8.2 Calculation and tests for slope and intercept

Use the linear regression program (on the “Tools” menu, “Data analysis” function, select “Regression”).

With the values given in Clause A.7, Table A.6 is obtained:

Table A.6 — Summary output

Regression statistics	
Multiples <i>R</i>	0,999 610 39
<i>R</i> -Square	0,999 220 93
Adjusted <i>R</i> -Square	0,999 026 16
Standard Error	0,176 667 93
Observations	6

An analysis of variance is given in Table A.7.

Table A.7 — Analysis of variance (ANOVA)

	Degrees of freedom	Sum of squares	Mean square	<i>F</i>	Significance of <i>F</i>
Regression	1	160,125 237	160,125 237	5 130,318 46	2,276 66E – 07
Residual	4	0,124 846 24	0,031 211 56		
Total	5	160,250 083			

	Coefficients	Standard error	<i>t</i> Stat	<i>P</i> -value	Lower 95 % limit value	Upper 95 % limit value
Intercept	–0,198 727 74	1,020 898 27	–0,194 659 69	0,855 146 4	–3,033 201 63	2,635 746 147
X variable 1	1,003 398 68	0,014 008 81	71,626 241 4	2,276 7E–07	0,964 503 89	1,042 293 459

The slope value appears in the cell which lies at the intersection of the “Coefficients” column and “X variable 1” row; the intercept value appears in the cell which lies at the intersection of the “Coefficients” column and “Intercept” row; the slope standard deviation value appears in the cell which lies at the intersection of the “Standard error” column and “X variable 1” row.

Calculate the t_{obs} statistic

$$t_{\text{obs}} = \frac{|1 - a|}{s_a}$$

where

a is the slope, whose complement of 1 is given as an absolute value (modulus);

s_a is the slope standard deviation.

Compare the t_{obs} value with a critical value corresponding to that of a 5 % risk Student variable with $m - 2$ degrees of freedom (usually, $m - 2 = 4$).

The last two columns list the limit values for a zero equivalent intercept and for a one equivalent slope. On the “Intercept” row, these two limits shall include 0; on the “X variable 1” row, these two limits shall include 1.

Annex B
(informative)

Some owners of certified standard measurement instruments

Chambre Arbitrale et de Conciliation pour Grains et Graines d'Anvers asbl

Lange Nieuwstraat, 17
2000 ANTWERPEN
Belgium

Telephone: +32 3 233 43 93

Fax: +32 3 233 34 60

e-mail: catherine@imexgra.org

Farm-Tec Ltd

Unit 3D, Larpool Lane Industrial Estate
WHITBY
YO22 4LX
United Kingdom

Telephone: +44 1947 825160

Fax: +44 1947 821372

e-mail: AndrewFarmTec@aol.com

Główny Urząd Miar (Central Office of Measures)

Zakład Mechaniki i Akustyki (Department of Mechanics and Acoustics)
Laboratorium Masy (Mass Laboratory)
ul. Elektoralna 2
00-139 WARSZAWA
Poland

Telephone: +48 22 5819216

e-mail: mass.force@gum.gov.pl

Institutul National de Metrologie (National Institute of Metrology)

Sos. Vitan-Bârzesti Steet, No. 11
Sector 4
042 122 BUCURESTI
Romania

e-mail: george.popa@inm.ro

Bibliography

- [1] ISO 3534-2:2006, *Statistics — Vocabulary and symbols — Part 2: Applied statistics*
- [2] ISO 10012, *Measurement management systems — Requirements for measurement processes and measuring equipment*
- [3] EN 15587, *Cereals and cereal products — Determination of Besatz in wheat (Triticum aestivum L.) , durum wheat (Triticum durum Desf.), rye (Secale cereale L.) and feed barley (Hordeum vulgare L.)*
- [4] OIML R15, *Instruments for measuring the hectolitre mass of cereals*. Available (2009-04-24) at: <http://www.oiml.org/publications/R/R015-e74.pdf>
- [5] Council Directive 71/347/EEC, 12 October 1971. Approximation of the laws of the Member States relating to the measuring of the standard mass per storage volume of grain. *Official J. L* (239), Annex I. Available (2009-04-24) at: <http://eur-lex.europa.eu/LexUriServ/LexUriServ.do?uri=CELEX:31971L0347:EN:HTML>

ICS 67.060

Price based on 19 pages