

---

---

**Nuclear energy — Uranium dioxide  
powder and sintered pellets —  
Determination of oxygen/uranium atomic  
ratio by the amperometric method**

*Énergie nucléaire — Poudre et pastilles frittées de dioxyde d'uranium —  
Détermination du rapport atomique oxygène/uranium par la méthode  
ampérométrique*



Reference number  
ISO 9005:2007(E)

© ISO 2007

**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

© ISO 2007

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

**Contents**

Page

|   |           |
|---|-----------|
| <b>Foreword</b> .....                         | <b>iv</b> |
| <b>1 Scope</b> .....                          | <b>1</b>  |
| <b>2 Principle</b> .....                      | <b>1</b>  |
| <b>3 Reactions</b> .....                      | <b>1</b>  |
| <b>4 Reagents</b> .....                       | <b>1</b>  |
| <b>5 Apparatus</b> .....                      | <b>2</b>  |
| <b>6 Preparation of the test sample</b> ..... | <b>7</b>  |
| <b>7 Procedure</b> .....                      | <b>7</b>  |
| <b>8 Expression of results</b> .....          | <b>8</b>  |
| <b>9 Test report</b> .....                    | <b>10</b> |
| <b>Bibliography</b> .....                     | <b>11</b> |

.....

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 9005 was prepared by Technical Committee ISO/TC 85, *Nuclear energy*, Subcommittee SC 5, *Nuclear fuel technology*.

This second edition cancels and replaces the first edition (ISO 9005:1994), which has been technically revised.

# Nuclear energy — Uranium dioxide powder and sintered pellets — Determination of oxygen/uranium atomic ratio by the amperometric method

## 1 Scope

This International Standard specifies an analytical method for the determination of the oxygen/uranium atomic ratio in uranium dioxide powder and sintered pellets.

The method is applicable to reactor grade samples of hyper-stoichiometric uranium dioxide powder and pellets. The presence of reducing agents or residual organic additives invalidates the procedure.


## 2 Principle

**2.1** The test sample is dissolved in orthophosphoric acid, which does not oxidize the uranium(IV) from  $\text{UO}_2$  molecules. Thus, the uranium(VI) that is present in the dissolved solution is from  $\text{UO}_3$  and/or  $\text{U}_3\text{O}_8$  molecules only, and is proportional to the excess oxygen in these molecules. The uranium(VI) content of the solution is determined by titration with a previously standardized solution of ammonium iron(II) sulfate hexahydrate in orthophosphoric acid. The end-point of the titration is determined amperometrically using a pair of polarized platinum electrodes. The oxygen/uranium ratio is calculated from the uranium(VI) content.

**2.2** A portion, weighing about 1 g, of the test sample is dissolved in orthophosphoric acid. The dissolution is performed in an atmosphere of nitrogen or carbon dioxide when sintered material is being analysed. When highly sintered material is being analysed, the dissolution is performed at a higher temperature in purified phosphoric acid from which the water has been partly removed.

The cooled solution is titrated with an orthophosphoric acid solution of ammonium iron(II) sulfate, which has previously been standardized against potassium dichromate. The end-point of the titration is detected by the sudden increase of current between a pair of polarized platinum electrodes on the addition of an excess of ammonium iron(II) sulfate solution.

## 3 Reactions



## 4 Reagents

Use only reagents of recognised analytical grade and demineralised water.

**4.1 Orthophosphoric acid**,  $\rho(\text{H}_3\text{PO}_4) = 1,75 \text{ g/ml}$ .

**4.2 Concentrated nitric acid**,  $c(\text{HNO}_3) = 14 \text{ mol/l}$ ;  $\rho(\text{HNO}_3) = 1,4 \text{ g/ml}$ .

**4.3 Orthophosphoric acid**, purified.

Add 1 500 ml of orthophosphoric acid (4.1) to 40 ml of nitric acid (4.2) to a cylinder quartz vessel and raise the temperature gradually to 275 °C. Maintain this temperature for 45 min while a gentle stream of nitrogen or carbon dioxide is passed through the solution. After cooling to room temperature, store the liquid in a glass bottle.

**4.4 Ammonium iron(II) sulfate**, approximately  $c[(\text{NH}_4)_2\text{Fe}(\text{SO}_4)_2] = 0,05 \text{ mol/l}$  or  $\rho[(\text{NH}_4)_2\text{Fe}(\text{SO}_4)_2] = 14,5 \text{ g/l}$ .

Heat 1 000 ml of orthophosphoric acid (4.1) to a temperature of 60 °C to 70 °C in a glass vessel. Add 20 g of ammonium iron(II) sulfate hexahydrate  $[(\text{NH}_4)_2\text{Fe}(\text{SO}_4)_2 \cdot 6\text{H}_2\text{O}]$  and stir until dissolved. Cool and store the solution in a nitrogen or carbon dioxide atmosphere.

Standardize this solution against potassium dichromate in the conventional way with each run of samples. Calculate the molarity of the iron(II) solution.

**4.5 Naturally occurring  $\text{U}_3\text{O}_8$  standard solution**,  $c(\text{U}_3\text{O}_8) = 0,01 \text{ mol/l}$  or  $\rho(\text{U}_3\text{O}_8) = 0,084 21 \text{ g/l}$ .

Dissolve 0,842 1 g of pure  $\text{U}_3\text{O}_8$  in purified orthophosphoric acid (4.3), warming if necessary. Cool and dilute to 100 ml with purified orthophosphoric acid (4.3).

NOTE The concentration of  $\text{UO}_2^{2+}$  in this solution is 0,02 mol/l. Upon dissolution, one mole of  $\text{U}_3\text{O}_8$  forms one mole of  $\text{U}^{4+}$  ions (non-reactive) and two moles of  $\text{UO}_2^{2+}$  ions, which is equivalent to dissolving one mole of  $\text{UO}_2$  (non-reactive) and two moles of  $\text{UO}_3$ . Thus, this solution contains 0,02 moles of  $\text{UO}_2^{2+}$  per litre.

To ensure stoichiometric  $\text{U}_3\text{O}_8$ , ignition just prior to use is recommended.

**4.6 Nitrogen or carbon dioxide**, containing less oxygen than a volume fraction of  $20 \times 10^{-6}$ .

## 5 Apparatus

Use laboratory apparatus and

**5.1 Inert dissolution apparatus**, type A; see Figure 1.

**5.2 Inert dissolution apparatus**, type B; see Figure 2.

**5.3 Electrode assembly**; see Figure 3.

When not in use, the electrodes shall be stored in a completed titration solution; see 7.4.2.


The electrodes should be cleaned when needed as follows. Immerse the platinum electrodes in boiling concentrated nitric acid (4.2) containing 10 g/l to 20 g/l of potassium dichromate for about 5 min. Rinse with demineralized water, then immerse in 1 mol/l iron(II) sulfate solution for 30 s to 60 s and then rinse with demineralized water.

**5.4 Bi-amperometric endpoint-detection circuit**; see Figure 4.

**5.5 Piston burette**, 5 ml or 1 ml capacity, capable of reading to 0,001 ml, fitted with a capillary end to dip into the titration solution.

**5.6 Thermostatically controlled heating block or isomantle**.


Dimensions in millimetres

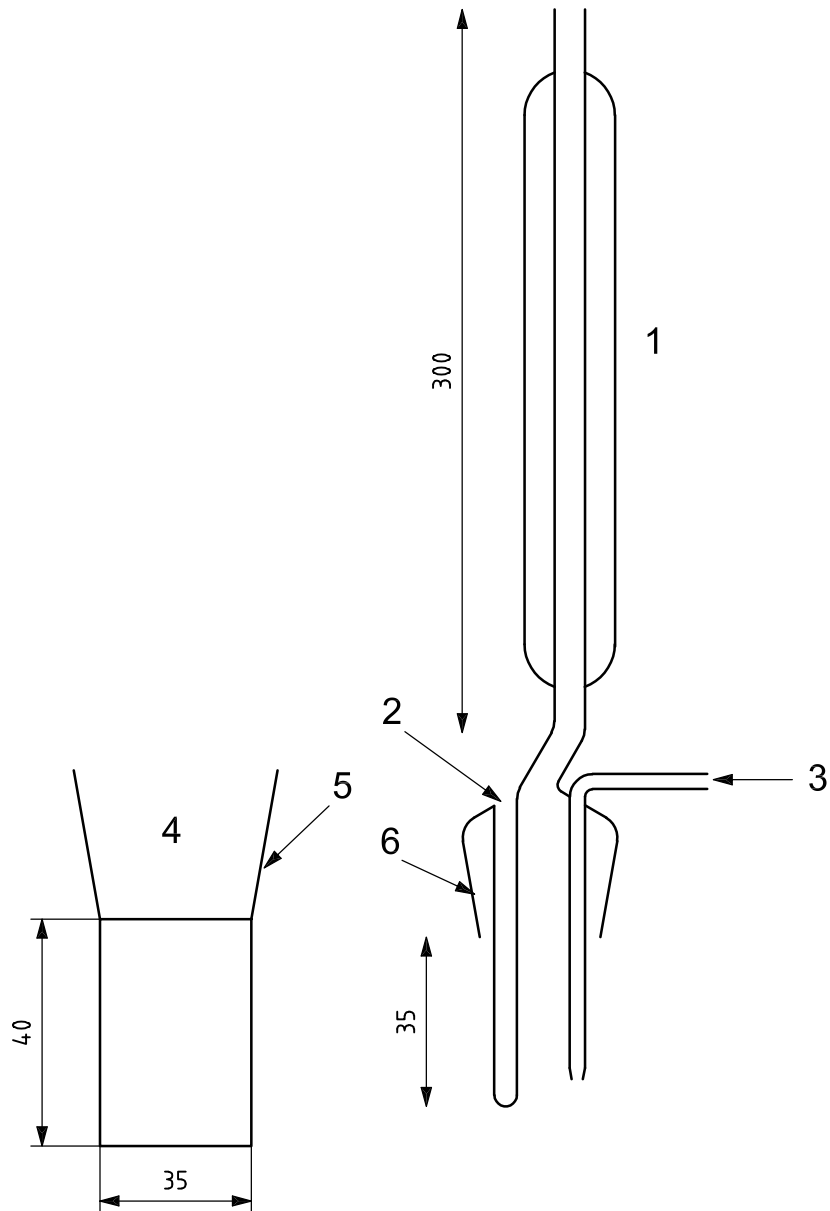

**Key**

- 1 condenser
- 2 thermometer well
- 3 nitrogen purge
- 4 flask
- 5 ISO 383-34/35 tapered, ground socket
- 6 ISO 383-34/35 tapered, ground cone


**Figure 1 — Dissolution apparatus —Type A**

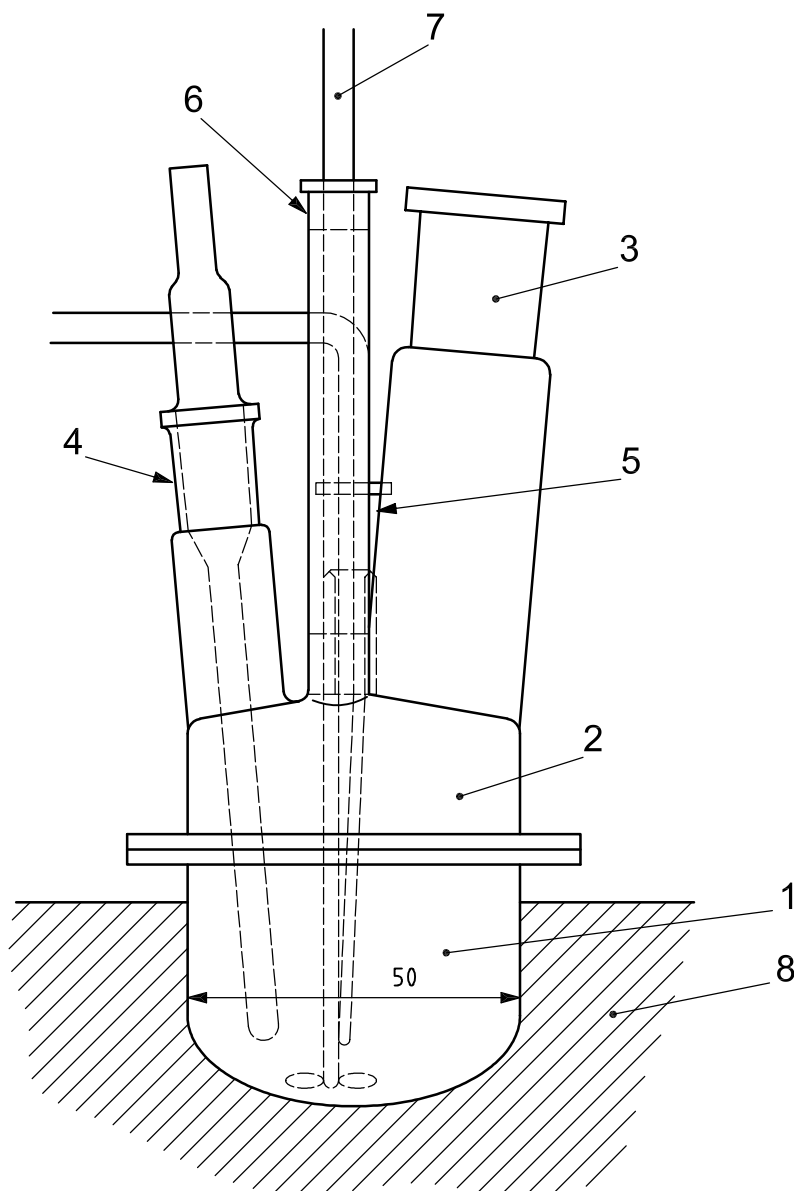**Key**

- 1 quartz dissolution vessel with ground rim
- 2 pyrex or equivalent cover with ground rim, equipped with four (items 3 to 6) joints
- 3 ISO 383-24/29 tapered ground joint for adding the test portion
- 4 ISO 383-14/23 tapered ground joint for inserting the thermometer
- 5 ISO 383-7/16 tapered ground joint for inserting the nitrogen-purge tube
- 6 central tube for inserting the stirrer, equipped with two polytetrafluoroethylene (PTFE) bearings
- 7 quartz stirrer, with the total length of the stirring blades equal to 25 mm, rotating at a constant angular velocity of 900 r/min
- 8 electric heating mantle powered by a temperature regulator in combination with the thermocouple in the joint number 4

**Figure 2 — Dissolution apparatus —Type B**




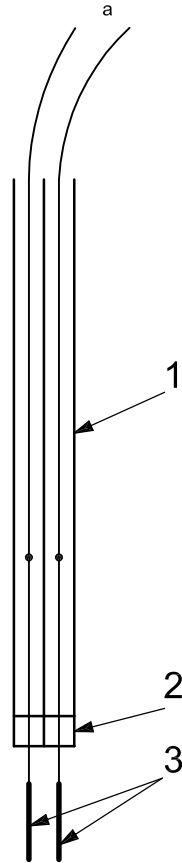


**Key**

- 1 glass tubes, ID 3 mm, taped together
  - 2 glass seal
  - 3 platinum electrodes (10 × 10)
- a To the bi-amperometric endpoint-detection circuit.

**Figure 3 — Electrode assembly**

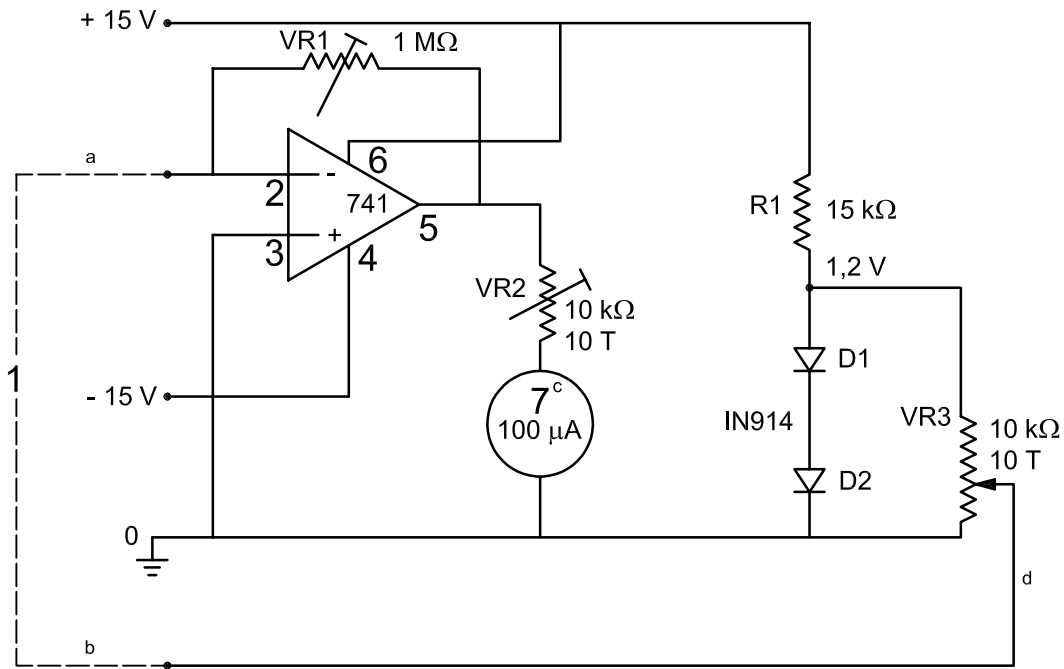

a) Circuit

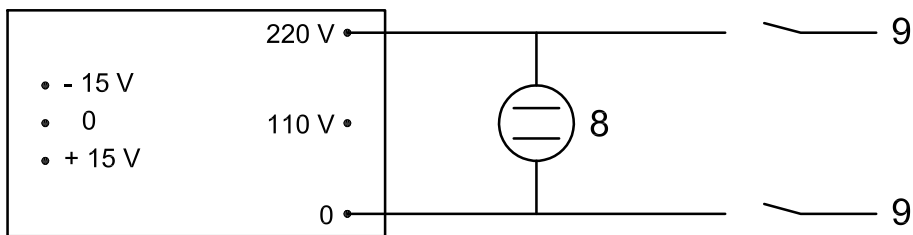

b) Underside (pin view)

**Key**

- 1 electrode assembly
- 2-6 pin numbers
- 7 multimeter, 100 μA
- 8 neon
- 9 mains switch
- a Red.
- b Black.
- c To adjust multimeter for full scale, remove 741, or equivalent, feed 1 V in at pin 6 and adjust VR2 for full-scale deflection.
- d Adjust for 300 mV.

Power supply: Ancom DPS or equivalent.

**Figure 4 — Bi-ampereometric endpoint-detection circuit**

## 6 Preparation of the test sample

### 6.1 Uranium dioxide powder

The laboratory sample is analysed without further preparation.

### 6.2 Uranium dioxide sintered pellets

Crush the laboratory sample in a percussion mortar and pass it through 250  $\mu\text{m}$  and 150  $\mu\text{m}$  aperture sieves until about 2 g of sample has passed through the 250  $\mu\text{m}$  sieve and has been retained in the 150  $\mu\text{m}$  sieve. Retain this 150  $\mu\text{m}$  to 250  $\mu\text{m}$  portion for use as the test sample.

The test sample should not be in a finely ground form; otherwise significant oxidation can occur.

Whole pellets or large pieces may be used but dissolution times are prolonged.

The crushing of sintered pellets implies an important risk of re-oxidation. The crushing should be carried out in an inert atmosphere to minimize measurement uncertainty.

## 7 Procedure

### 7.1 Uranium dioxide powder

**7.1.1** Weigh, to the nearest 0,001 g, approximately 1 g of the test sample and record this value as *m*. Transfer the test portion to a 50 ml squat-form beaker and add 30 ml  $\pm$  0,5 ml of orthophosphoric acid (4.1). Cover the beaker with a watch-glass.

**7.1.2** Prepare the blank test solution using normal dissolution, by adding 30 ml  $\pm$  0,5 ml of orthophosphoric acid (4.1) to a 50 ml squat-form beaker. Cover the beaker with a watch-glass.

**7.1.3** Heat the test portion and blank-test solution to a temperature of 160 °C to 180 °C until dissolution is complete. Cool to room temperature.

**7.1.4** To correct for humidity, the sample may be dried before the weighing or the uranium content determined independently.

**7.1.5** If greater accuracy is required, the dissolution should be performed in an inert dissolution apparatus, type A (5.1).

### 7.2 Sintered pellets of uranium dioxide

**7.2.1** Weigh, to the nearest 0,001 g, approximately 1 g of the test sample and record this value as *m*. Transfer the test portion to the flask of an inert dissolution apparatus, type A (5.1), and add 30 ml  $\pm$  0,5 ml of orthophosphoric acid (4.1).

**7.2.2** Prepare the blank-test solution, using inert dissolution by adding 30 ml  $\pm$  0,5 ml of orthophosphoric acid (4.1) to the flask of an inert solution apparatus, type A (5.1).

**7.2.3** Assemble the inert-dissolution apparatus. Pass a stream of nitrogen or carbon dioxide (4.6) through the solution and heat the test portion and blank to a temperature of 160 °C to 180 °C until dissolution is complete. Cool at room temperature.

NOTE 1 Some batches of orthophosphoric acid can contain reducing impurities. The procedure in 7.3 is more accurate.

NOTE 2 It can be necessary to heat certain highly sintered samples at a higher temperature to achieve dissolution. The procedure can continue as described in 7.3.

### 7.3 Highly sintered pellets of uranium dioxide

**7.3.1** Weigh, to the nearest 0,001 g, approximately 1 g of the test sample and record this value as  $m$ . Transfer the test portion to the quartz vessel of an inert dissolution apparatus, type B (5.2) and add 50 ml  $\pm$  1 ml of purified orthophosphoric acid (4.3).

**7.3.2** Prepare the blank-test solution, using inert dissolution of highly sintered pellets, as follows. Add 50 ml  $\pm$  1 ml of purified orthophosphoric acid (4.3) to the quartz vessel of an inert-dissolution apparatus, type B (5.2). Add 0,5 ml of standard  $U_3O_8$  solution (4.5) measured to the nearest 0,001 ml.

**7.3.3** Assemble the inert dissolution apparatus. Start stirring the test portion and blank with the quartz stirrer and pass a stream of nitrogen or carbon dioxide through the solution.

Heat to a maximum temperature of 275 °C and maintain the temperature for 1 h. Cool to about 70 °C and add 5 ml of demineralized water to the test portion and blank solution.

### 7.4 Determination

**7.4.1** Stir the test and blank solutions at high speed to create a vortex of about 5 mm depth. Insert the electrode assembly (5.3) into the solution and switch on the bi-amperometric endpoint-detection circuit (5.4).

**7.4.2** Titrate with ammonium iron(II) sulfate solution (4.4) from the piston burette (5.5) until a small permanent current reading is obtained. Record the volume of the titrant used for the test solution as  $V_1$  and for the blank solution as  $V_2$ .

NOTE 1 To minimize measurement uncertainty, it is possible pass a stream of nitrogen or carbon dioxide through the solution during the titration.

NOTE 2 It is preferable to use a more concentrated titrant when analysing samples with an oxygen/uranium ratio of more than 2,1.

NOTE 3 The aim should be to obtain the same small permanent current at the end-point for both test solution and blank solution.

## 8 Expression of results

### 8.1 Method of calculation

#### 8.1.1 Uranium dioxide powder and uranium dioxide sintered pellets

Calculate the corrected mass,  $m_1$ , expressed in milligrams, of uranium(VI) reduced in the titration of the test solution using Equation (1):

$$m_1 = \frac{\rho_{AIS} \times A_U}{2} (V_1 - V_2) \quad (1)$$

where

$\rho_{AIS}$  is the concentration of the ammonium iron(II) sulfate solution (4.4), expressed in grams per litre;

$V_1$  is the volume of titrant used for the test solution, expressed in millilitres;

$V_2$  is the volume of titrant used for the blank solution, expressed in millilitres;

$A_U$  is the relative atomic mass of the uranium in the test sample.

The mass of uranium(VI) in the test portion is equal to  $m_1$ .

NOTE In material where the uranium-235 level is less than 10 %, a value of  $A_U$  of 238 is sufficiently accurate.

### 8.1.2 Uranium dioxide, highly sintered pellets

Calculate the corrected mass,  $m_1$ , expressed in milligrams, of uranium(VI) reduced in the titration of the test solution using Equation (2):

$$m_1 = \frac{\rho_{\text{AIS}} \times A_{\text{U}}}{2} \left[ V_1 - \left( V_2 - \frac{0,02}{\rho_{\text{AIS}}} \right) \right] \quad (2)$$

NOTE 1 The value of  $0,02/\rho_{\text{AIS}}$  gives the volume, expressed in millilitres, of ammonium iron(II) sulfate hexahydrate solution (4.4) of concentration,  $\rho_{\text{AIS}}$ , equivalent to 0,5 ml of 0,01 mol/l standard  $\text{U}_3\text{O}_8$  solution (4.5).

NOTE 2 The value of  $[V_2 - (0,02/\rho_{\text{AIS}})]$  can be positive or negative depending upon whether the purified orthophosphoric acid (4.3) has any residual oxidizing or reducing properties.

### 8.1.3 Calculation of oxygen/uranium atomic ratio

8.1.3.1 Calculate the expected mass,  $m_2$ , expressed in milligrams, of total uranium in the test solution from the mass of the test sample taken, using Equation (3):

$$m_2 = \frac{m \times A_{\text{U}}}{A_{\text{U}} + (2+x)16} \quad (3)$$

where

$m$  is the mass of the test portion, expressed in milligrams; see 7.1.1, 7.2.1 and 7.3.1;

$x$  is the estimated/preliminary calculated hyper-stoichiometric part of the oxygen/uranium ratio.

8.1.3.2 Calculate the oxygen/uranium atomic ratio,  $R_{\text{O/U}}$ , using Equation (4):

$$R_{\text{O/U}} = 2,000 \ 0 + \frac{m_1}{m_2} \quad (4)$$

## 8.2 Precision

### 8.2.1 Uranium dioxide powder

The precision (one standard deviation) based on 50 between-run determinations of a synthetic sample with a mean  $R_{\text{O/U}}$  of 2,069 is 0,003.

### 8.2.2 Pellets

The precision (one standard deviation) based on 50 between-run determinations of a synthetic sample with a mean  $R_{\text{O/U}}$  of 2,004 4 is 0,000 5.

## 9 Test report

The test report shall include the following information:

- a) reference to this International Standard;
- b) identification of the sample;
- c) reference to method used within this International Standard;
- d) any results and method of expression used;
- e) any unusual features noted during the test;
- f) any operations not included in this International Standard or regarded as optional.

## Bibliography

- [1] RAO, G.G. and SAGI, S.R. A new Reductimetric Reagent: Iron(II) in a strong Phosphoric Acid Medium, *Talanta*, **9**, 1962, pp. 715
- [2] ENGELSMANN, J.J., KNAAPE, J. and VISSER, J. Volumetric Determination of the U/O Ratio in Uranium Oxides, *Talanta*, **15**, 1968, pp. 171
- [3] TOLK, A. and LINGERAK, W.A. Determination of Oxygen to Uranium Ratio in Hyperstoichiometric Uranium Dioxide, RCN-127, Reactor Centrum Nederland, Pelten, 1970
- [4] BNFL Report 113 (S), Determination of Oxygen to Uranium ratio in Uranium Dioxide by the Amperometric Titration of Uranium(VI) with Iron(II) in Phosphoric Acid
- [5] ISO 383:1976, *Laboratory glassware — Interchangeable conical ground joints*

© ISO 2007. All rights reserved.

---

---

**ICS 27.120.30**

Price based on 11 pages