

INTERNATIONAL STANDARD

ISO 9439

Second edition
1999-03-01

Water quality — Evaluation of ultimate aerobic biodegradability of organic compounds in aqueous medium — Carbon dioxide evolution test

*Qualité de l'eau — Évaluation de la biodégradabilité aérobie ultime en
milieu aqueux des composés organiques — Essai de dégagement de
dioxyde de carbone*



Reference number
ISO 9439:1999(E)

Contents

1 Scope	1
2 Definitions	1
3 Principle	3
4 Test environment	3
5 Reagents	3
6 Apparatus	4
7 Procedure	5
8 Calculation	7
9 Validity of results	8
10 Test report	9
Annex A (informative) Principle of a test system for measuring carbon dioxide (example)	10
Annex B (informative) Examples of the determination of released carbon dioxide	11
Annex C (informative) Example of a biodegradation curve	13
Annex D (informative) Combined determination of carbon dioxide and DOC	14
Bibliography	17

© ISO 1999

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization
Case postale 56 • CH-1211 Genève 20 • Switzerland
Internet iso@iso.ch

Printed in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 9439 has been prepared by Technical Committee ISO/TC 147, *Water quality*, Subcommittee SC 5, *Biological methods*.

This second edition cancels and replaces the first edition (ISO 9439:1990), which has been technically revised.

Annexes A to D of this International Standard are for information only.

Introduction

The conditions described in this International Standard do not always correspond to the optimal conditions for allowing the maximum degree of biodegradation to occur. With this test system, the microbially derived carbon dioxide (CO₂) is measured in the traps through which gas exhausted from the test vessels is passed. Some of the CO₂ remains in the medium in the vessels as dissolved inorganic carbon (DIC), the concentration of which may increase as biodegradation proceeds. As the organic carbon approaches complete removal, the concentration of DIC gradually falls and tends to reach zero by the end of incubation. It is thus necessary to acidify the medium at the end of the test to measure the biogenically formed CO₂ completely. The measurement of CO₂ in the external traps may differ from the true production of CO₂ and the kinetic rate may also be lower than a rate based on DOC removal measurement. The consequence may be that the biodegradation curves based on the trapped CO₂ may not fully represent the true microbial kinetic rate. For alternative biodegradation methods, see ISO 15462 and in particular ISO 14593, which is based on CO₂ production as well but does not have this defect.

Water quality — Evaluation of ultimate aerobic biodegradability of organic compounds in aqueous medium — Carbon dioxide evolution test

WARNING — Activated sludge and sewage may contain potentially pathogenic organisms. Appropriate precautions should be taken when handling them. Toxic test compounds and those whose properties are unknown should be handled with care.

1 Scope

This International Standard specifies a method, by determination of carbon dioxide (CO₂), for the evaluation in an aqueous medium of the ultimate biodegradability of organic compounds at a given concentration by aerobic microorganisms.

The method applies to organic compounds which are:

- a) water-soluble under the conditions of the test, in which case removal of DOC may be determined as additional information (see annex D);
- b) poorly water-soluble under the conditions of the test, in which case special measures may be necessary to achieve good dispersion of the compound (see, for example, ISO 10634);
- c) non-volatile or which have a negligible vapour pressure under the conditions of the test;

NOTE For volatile substances use for example ISO 9408 or ISO 14593.

- d) not inhibitory to the test microorganisms at the concentration chosen for the test.

NOTE The presence of inhibitory effects can be determined as specified in 8.3, or by using any other method for determining the inhibitory effect of a compound on bacteria (see, for example, ISO 8192).

2 Terms and definitions

For the purposes of this International Standard, the following terms and definitions apply.

2.1

ultimate aerobic biodegradation

breakdown of a chemical compound or organic matter by microorganisms in the presence of oxygen to carbon dioxide, water and mineral salts of any other elements present (mineralization) and the production of new biomass

2.2

primary biodegradation

structural change (transformation) of a chemical compound by microorganisms resulting in the loss of a specific property

2.3

activated sludge

biomass produced in the aerobic treatment of wastewater by the growth of bacteria and other microorganisms in the presence of dissolved oxygen

2.4 concentration of suspended solids

<activated sludge> amount of solids obtained by filtration or centrifugation of a known volume of activated sludge and drying at about 105 °C to constant mass

2.5 dissolved organic carbon DOC

that part of the organic carbon in a water sample which cannot be removed by specified phase separation

NOTE For example, by centrifugation at $40\,000\text{ m} \cdot \text{s}^{-2}$ for 15 min or by membrane filtration using membranes with pores of diameter 0,2 µm to 0,45 µm.

2.6 total inorganic carbon TIC

all that inorganic carbon in the water deriving from carbon dioxide and carbonate

2.7 dissolved inorganic carbon DIC

that part of the inorganic carbon in water which cannot be removed by specified phase separation

NOTE For example, by centrifugation at $40\,000\text{ m} \cdot \text{s}^{-2}$ for 15 min or by membrane filtration using membranes with pores of diameter 0,2 µm to 0,45 µm.

2.8 theoretical amount of formed carbon dioxide ThCO₂

theoretical maximum amount of carbon dioxide formed after oxidizing a chemical compound completely

NOTE It is calculated from the molecular formula and expressed in this case as milligrams carbon dioxide per milligram (or gram) test compound.

2.9 lag phase

time from the start of a test until adaptation and/or selection of the degrading microorganisms are achieved and the biodegradation degree of a chemical compound or organic matter has increased to about 10 % of the maximum level of biodegradation

NOTE It is normally recorded in days.

2.10 maximum level of biodegradation

maximum biodegradation degree of a chemical compound or organic matter in a test, above which no further biodegradation takes place during the test

NOTE It is normally recorded in percent.

2.11 biodegradation phase

time from the end of the lag phase of a test until about 90 % of the maximum level of biodegradation has been reached

NOTE It is normally recorded in days.

2.12 plateau phase

time from the end of the biodegradation phase until the end of the test

NOTE It is normally recorded in days.

2.13**pre-exposure**

pre-incubation of an inoculum in the presence of the test chemical compound or organic matter, with the aim of enhancing the ability of this inoculum to biodegrade the test material by adaptation and/or selection of the microorganisms

2.14**preconditioning**

pre-incubation of an inoculum under the conditions of the subsequent test in the absence of the test chemical compound or organic matter, with the aim of improving the performance of the test by acclimatization of the microorganisms to the test conditions

3 Principle

The biodegradability of organic compounds by aerobic microorganisms is determined using a static aqueous test system. The test mixture contains an inorganic medium, the organic compound as the nominal sole source of carbon and energy at a concentration of 10 mg/l to 40 mg/l organic carbon and a mixed inoculum obtained from a wastewater treatment plant or from another source in the environment. The mixture is agitated in test vessels and aerated with CO₂-free air normally up to 28 d (for example see annex A). The CO₂ formed during the microbial degradation is trapped in external vessels, determined by an appropriate analytical method (for examples see annex B), compared with the theoretical amount (ThCO₂) and expressed as a percentage.

For sufficiently water-soluble compounds, removal of DOC may optionally be measured to obtain additional information on the ultimate biodegradability. This can be done in the method given, but a convenient procedure is described in annex D which allows the use of higher concentrations of the test compound and the inoculum, thus improving the biodegradation potential of the test. If a substance-specific analytical method is available, information on the primary degradability may also be obtained.

4 Test environment

Incubation shall take place in the dark or in diffused light, at a temperature within the range 20 °C to 25 °C which shall not vary by more than ± 2 °C during the test.

5 Reagents

Use only reagents of recognized analytical grade.

5.1 Water, distilled or deionized, containing less than 1 mg/l DOC.

5.2 Test medium.

5.2.1 Composition

a) **Solution a)**

Dissolve

anhydrous potassium dihydrogenphosphate (KH ₂ PO ₄)	8,5 g
anhydrous dipotassium hydrogenphosphate (K ₂ HPO ₄)	21,75 g
disodium hydrogenphosphate dihydrate (Na ₂ HPO ₄ ·2H ₂ O)	33,4 g
ammonium chloride (NH ₄ Cl)	0,5 g
in water (5.1), quantity necessary to make up to	1 000 ml

In order to check this buffer solution it is recommended to measure the pH, which should be about 7,4. If this is not the case, prepare a new solution.

b) **Solution b)**

Dissolve 22,5 g magnesium sulfate heptahydrate ($\text{MgSO}_4 \cdot 7\text{H}_2\text{O}$) in water (5.1), quantity necessary to make up to 1 000 ml.

c) **Solution c)**

Dissolve 36,4 g calcium chloride dihydrate ($\text{CaCl}_2 \cdot 2\text{H}_2\text{O}$) in water (5.1), quantity necessary to make up to 1 000 ml.

d) **Solution d)**

Dissolve 0,25 g iron(III) chloride hexahydrate ($\text{FeCl}_3 \cdot 6\text{H}_2\text{O}$) in water (5.1), quantity necessary to make up to 1 000 ml. To avoid precipitation, prepare this solution freshly before use or add a drop of concentrated hydrochloric acid (HCl).

5.2.2 Preparation of the test medium

For 1 000 ml of test medium add to about 800 ml of water (5.1):

- 10 ml of solution a);
- 1 ml of each of the solutions b) to d).

Make up to 1 000 ml with water (6.1).

6 Apparatus

Ensure that all glassware is thoroughly cleaned and free from both organic and toxic matter.

6.1 Test vessels. Glass vessels (e.g. Erlenmeyer vessels or bottles) allowing gas purging and shaking or stirring, including tubing impermeable to CO_2 . Located in a constant-temperature room or in a thermostatically controlled environment (e.g. water bath).

6.2 CO_2 -free air production system, capable of supplying each test vessel at a flowrate between about 50 ml/min and 100 ml/min for 3 l of medium, held constant (see example of assembly with the test vessels in annex A).

6.3 Analytical equipment for determining CO_2 .

Any suitable apparatus or technique with sufficient accuracy, e.g. CO_2 - or DIC analyzer or device for titrimetric determination after complete absorption in an alkaline solution (see examples in annex B).

6.4 Analytical equipment for measuring dissolved organic carbon (DOC) (optional).

6.5 Centrifuge or device for filtration, with membrane filters (nominal aperture diameter of 0,2 μm to 0,45 μm pore size) which adsorb or release organic carbon to a minimum degree.

6.6 pH meter.

7 Procedure

7.1 Preparation of the test solutions

7.1.1 Test compound

Prepare a stock solution of a sufficiently water-soluble test compound in water (5.1) or the test medium (5.2) and add a suitable amount of this to obtain an organic carbon concentration in the final test medium of between 10 mg/l and 40 mg/l. Depending on the properties of the test compound (e.g. toxicity) and the purpose of the test, other concentrations may be used. Add compounds of low water solubility directly into the test vessels. Determine the added amount exactly.

NOTE For more details on handling poorly water-soluble compounds, see ISO 10634.

7.1.2 Reference compound

Use as reference compound an organic compound of known biodegradability, such as aniline or sodium benzoate. Prepare a stock solution of the reference compound in the test medium (5.2) in the same way as with a water-soluble test compound (7.1.1), in order to obtain a final organic carbon concentration of 20 mg/l or a concentration equivalent to that of the test compound.

7.1.3 Solution to check inhibition

If required (when e.g. no information on the toxicity of test compound is available), prepare a solution containing, in the test medium (5.2), both the test compound (7.1.1) and the reference compound (7.1.2) preferably at concentrations of organic carbon of 20 mg/l for each.

7.2 Preparation of the inoculum

7.2.1 General

Prepare the inoculum using activated sludge (7.2.2) or the sources described in 7.2.3 and 7.2.4 or a mixture of these sources to obtain a microbial population that offers sufficient biodegradative activity. Check the activity of the inoculum by means of the reference compound (7.1.2 and clause 9). The CO₂ production of the blank should fulfil the validity criteria (see clause 9). To reduce the influence of the blank, it may be helpful to precondition the inoculum, e.g. by washing with medium (5.2.2) and aerating it, from 1 d to 7 d, before use. Use a suitable volume for inoculation (see note 2 below).

NOTE 1 Normally the inoculum should not be pre-exposed to the test compound to allow a general prediction of the degradation behaviour in the environment. In certain circumstances, depending on the purpose of the test, pre-exposed inocula may be used, provided that this is clearly stated in the test report (e. g. percent biodegradation = x %, using pre-exposed inocula) and the method of pre-exposure is detailed in the test report. Pre-exposed inocula can be obtained from laboratory biodegradation tests conducted under a variety of conditions (e.g. Zahn-Wellens test ISO 9888 and SCAS test ISO 9887) or from samples collected from locations where relevant environmental conditions exist (e.g. treatment plants dealing with similar compounds or contaminated areas).

NOTE 2 Based on experience, suitable volume means:

- sufficient to give a population which offers enough biodegradation activity;
- degrades the reference compound by the stipulated percentage (see clause 9);
- gives between 10³ to 10⁶ colony-forming units per millilitre in the final mixture;
- gives not greater than the equivalent of 30 mg/l suspended solids of activated sludge in the final mixture;
- the quantity of dissolved organic carbon provided by the inoculum should be less than 10 % of the initial concentration of organic carbon introduced by the test compound;
- generally 1 ml to 10 ml of inoculum are sufficient for 1 000 ml of test solution.

7.2.2 Inoculum from an activated sludge plant

Take a sample of activated sludge collected from the aeration tank of a full-scale or a laboratory wastewater treatment plant dealing with predominantly domestic sewage. Mix well and determine the concentration of suspended solids of the activated sludge (use e.g. ISO 11923). If necessary remove coarse particles by filtration through a sieve and concentrate the sludge by settling, so that the volume of sludge added to the test assay is minimal. Keep the sample under aerobic conditions and use preferably on the day of collection. Use a suitable volume to obtain 30 mg/l of suspended solids in the final mixture.

7.2.3 Inoculum from wastewater

Take a sample from the influent or from the effluent of a full-scale or a laboratory wastewater treatment plant dealing with predominantly domestic sewage. If necessary, remove gross particulate matter by coarse filtration and concentrate the sample, e.g. by centrifugation. Mix well, keep the sample under aerobic conditions and use preferably on the day of collection. Before use, let the sample settle for 1 h and take a suitable volume of the supernatant for inoculation.

7.2.4 Inoculum from a surface water

Take a sample of an appropriate surface water. If necessary, concentrate the sample by filtration using a coarse paper filter or centrifugation. Keep the sample under aerobic conditions and use preferably on the day of collection. Use a suitable volume as inoculum.

7.3 Test procedure

Provide a sufficient number of vessels (6.1) in order to have

- at least two test vessels (denoted F_T) for the test compound (7.1.1);
- at least two blank vessels (denoted F_B) containing test medium and inoculum;
- at least one vessel, for checking the procedure (denoted F_C) containing the reference compound (7.1.2);
- if needed, one vessel for checking a possible inhibitory effect of the test compound (denoted F_I) containing solution 7.1.3;
- if needed, one vessel for checking a possible abiotic elimination (denoted F_S) containing the test compound (7.1.1) but no inoculum, sterilized by autoclaving or by addition of a suitable inorganic toxic compound to prevent microbial activity. Use, for example, 1 ml/l of a solution containing 10 g/l of mercury(II) chloride ($HgCl_2$). Add the same amount of the toxic substance two weeks after the test was begun.

Add appropriate amounts of the test medium (5.2), and the inoculum (7.2) to the vessels as indicated in Table 1 to obtain a final test volume of e.g. 3 l. Other final test volumes are possible; adapt in such a case all relevant parameters and the calculation of test results. Connect the vessels to the CO_2 -free air production system (see annex A). Incubate at the desired test temperature (see clause 4) and aerate the vessels for 24 h to purge CO_2 from the system. Agitate throughout the test with a magnetic stirrer. If excessive foaming is observed, replace the air sparge by headspace aeration while stirring. After the pre-aeration period, connect the air exit of each vessel to the CO_2 trapping or measuring system.

Add the test sample (7.1.1) and the reference compound (7.1.2) at the desired concentrations to the respective vessels in accordance with Table 1 and start the test by bubbling CO_2 -free air through the vessels with 3 l medium at a rate of about 50 ml/min to 100 ml/min.

Measure the amount of CO_2 released from each vessel at timed intervals, depending on the rate of evolution of CO_2 , using an appropriate and sufficiently accurate method (see annex B). If a nearly constant level of CO_2 formation is attained (plateau phase) and no further biodegradation is expected, the test is considered to be completed. Usually the maximum test period should not exceed 28 d. Extend the test by one to two weeks, if degradation has obviously started but has not reached a plateau.

Table 1 — Final distribution of test and reference compounds in the test vessels

Vessel	Test medium (5.2)	Test compound (7.1.1)	Reference compound (7.1.2)	Inoculum (7.2)
F _T Test compound	+	+	—	+
F _T Test compound	+	+	—	+
F _B Blank	+	—	—	+
F _B Blank	+	—	—	+
F _C Inoculum check	+	—	+	+
F _I Inhibition control (optional)	+	+	+	+
F _S Abiotic elimination check (optional)	+	+	—	—

On the last day of the test, measure the pH, acidify all the bottles with 1 ml to 10 ml of concentrated hydrochloric acid in order to decompose the carbonates and bicarbonates and purge the CO₂. Continue aeration for up to 24 h and measure the amount of CO₂ released from each vessel.

NOTE 1 During the handling of samples for the regular measurement of CO₂ in the traps it cannot be excluded that, especially in the case of DIC determinations, small amounts of CO₂ from the air are included and added up during the test. This has normally no effect on the test results as the CO₂ values of the blank vessels, where the same occurs, are subtracted. However, in the case of the abiotic elimination control (vessel F_S) this may lead to an apparent and unjustified impression of degradation. Therefore it is recommended to determine the CO₂ evolution from vessel F_S only at the end of the test.

NOTE 2 If the DOC removal is measured to provide additional information on the biodegradability of a water-soluble test compound, or if a substance-specific analytical method is used to determine the primary biodegradability, use the information given in annex D.

8 Calculation

8.1 Amount of theoretical carbon dioxide from the test compound

The theoretical amount, in milligrams, of released carbon dioxide (ThCO₂) in the test vessels is given by equation (1):

$$\text{ThCO}_2 = \rho_C \times V_L \times \frac{44}{12} \quad (1)$$

where

ρ_C is the concentration of organic carbon of the test compound in the test vessel, in milligrams per litre, measured or calculated from the stock solution of the test compound (7.1.1);

V_L is the volume of the test solution in the test vessel, expressed in litres;

44 and 12 are the relative molar and atomic masses of CO₂ and carbon, respectively, to calculate the amount of CO₂ from the measured organic carbon.

Calculate in the same way the ThCO₂ of the reference compound and the inhibition solution (7.1.3).

8.2 Percentage biodegradation

Calculate the percentage of biodegradation D_m (%) for each of the test vessels F_T for each measurement interval using equation (2)

$$D_m = \frac{\sum m_{Tt} - \sum m_{Bt}}{\text{ThCO}_2} \times 100 \quad (2)$$

where

$\sum m_{Tt}$ is the mass, in milligrams, of CO_2 released in vessel F_T between the start of the test and time t ;

$\sum m_{Bt}$ is the average mass, in milligrams, of CO_2 released in the blank controls F_B between the start of the test and time t .

Calculate in the same way the biodegradation degree of the reference compound in the inoculum check vessel F_C , and, if included, of the mixture of test and reference compound in the inhibition control F_I , and, without subtracting the blanks, of the test compound in the abiotic elimination control F_S .

NOTE If DOC removal and primary biodegradation by substance-specific analyses were measured, it is recommended that results be calculated according to annex D.

8.3 Expression of results

Compile a table of CO_2 released ($\sum m_{Tt}$ and $\sum m_{Bt}$) and the percentages of biodegradation (D_m) for each measuring interval and each test vessel. Plot a biodegradation curve in percent as a function of time, and indicate lag phase and degradation phase. Optionally, plot a curve of the net released CO_2 versus time. If comparable results are obtained for the duplicate test vessels F_T (< 20 % difference), plot a mean curve, otherwise plot curves for each vessel (see example in annex C). Plot in the same way a biodegradation curve of the reference compound F_C and, if included of the abiotic elimination check F_S and the inhibition control F_I .

Determine the mean value of percent biodegradation in the plateau phase or use the highest value, e.g. when the curve decreases in the plateau phase and indicate this maximum level of biodegradation as "degree of biodegradation of the test compound" in the test report.

Information on the toxicity of the test compound may be useful in the interpretation of test results showing a low biodegradation. If in vessel F_I the degradation percentage is < 25 % and insufficient degradation of the test compound is observed, it can be assumed that the test compound is inhibitory. In this case, the test should be repeated using a lower test concentration or another inoculum. If in vessel F_S (abiotic elimination check, if included) a significant amount (> 10 %) of released CO_2 is observed, abiotic degradation processes may have taken place.

9 Validity of results

9.1 Validity criteria

The test is considered as valid if

- the percentage degradation in vessel F_C (inoculum check) is greater than 60 % on the 14th day;
- the concentration of CO_2 which has evolved from the blank F_B at the end of the test at a test volume of 3 l is about 40 mg/l and does not exceed 70 mg/l;
- the amount of DIC at the beginning of the test is < 5 % of the organic carbon of the test compound.

If a) and b) are not fulfilled, the test should be repeated using another or a better preconditioned inoculum. If c) is not fulfilled, verify that the air for aerating the vessels is really free from CO_2 .

9.2 Inhibition

If the vessel F_I (inhibition control) was included, the test compound is assumed to be inhibiting if the degradation percentage of the reference compound in vessel F_I is lower than 40 % at the end of the test. In this case, it is advisable to repeat the test with a lower concentration of the test compound.

9.3 pH value

If the pH value at the end of the test is outside the range 6 to 8,5 and if the percentage degradation of the test compound is less than 60 %, it is advisable to repeat the test with a lower concentration of the test compound or to use the test modification described in annex D of this method.

10 Test report


The test report shall contain at least the following information:

- a) a reference to this International Standard and the annex if a variation was used;
- b) all necessary information for the identification of the test compound;
- c) all the data (for example in tabular form) obtained and the degradation curve;
- d) the concentration of the test compound used and the ThCO_2 and, in the case of water-soluble test compounds, the DOC of this concentration;
- e) the name of the reference compound used and the degradation obtained with this compound;
- f) the source, the characteristics, the concentration or the volume of the inoculum used and information on any pre-treatment;
- g) the main characteristics of the CO_2 analysing system used;
- h) the incubation temperature of the test;
- i) if included the percentage of DOC removal or primary biodegradation;
- j) if included, the percentage of degradation obtained in vessel F_S (abiotic elimination);
- k) if included, the percentage of degradation in vessel F_I (inhibition check) and a statement on the toxicity of the test compound;
- l) the reasons, in the event of rejection of the test;
- m) any alteration of the standard procedure or any other circumstance that may have affected the results.

Annex A (informative)

Principle of a test system for measuring carbon dioxide (example)

Set up vessels in series as shown in Figure A.1 and connect them with gas-impermeable tubing. Aerate the test system with CO_2 -free air at 50 ml/min to 100 ml/min and a constant low pressure. Count air bubbles or use a suitable gas-flow controller to check the flowrate. Use synthetic CO_2 -free air or compressed air. In the latter case, remove CO_2 by passing the air through a vessel with dry soda lime or through at least two gas-washing vessels containing e.g. 500 ml of an aqueous NaOH solution ($c = 10 \text{ mol/l}$). A second vessel containing 100 ml $\text{Ba}(\text{OH})_2$ solution ($c = 0,0125 \text{ mol/l}$) is used to indicate any CO_2 in the air by turbidity. An empty vessel between the indicator and the following test vessel prevents liquid carry-over. In the test vessel, CO_2 is produced if biodegradation takes place and absorbed in the subsequent absorber vessels as described in annex B.

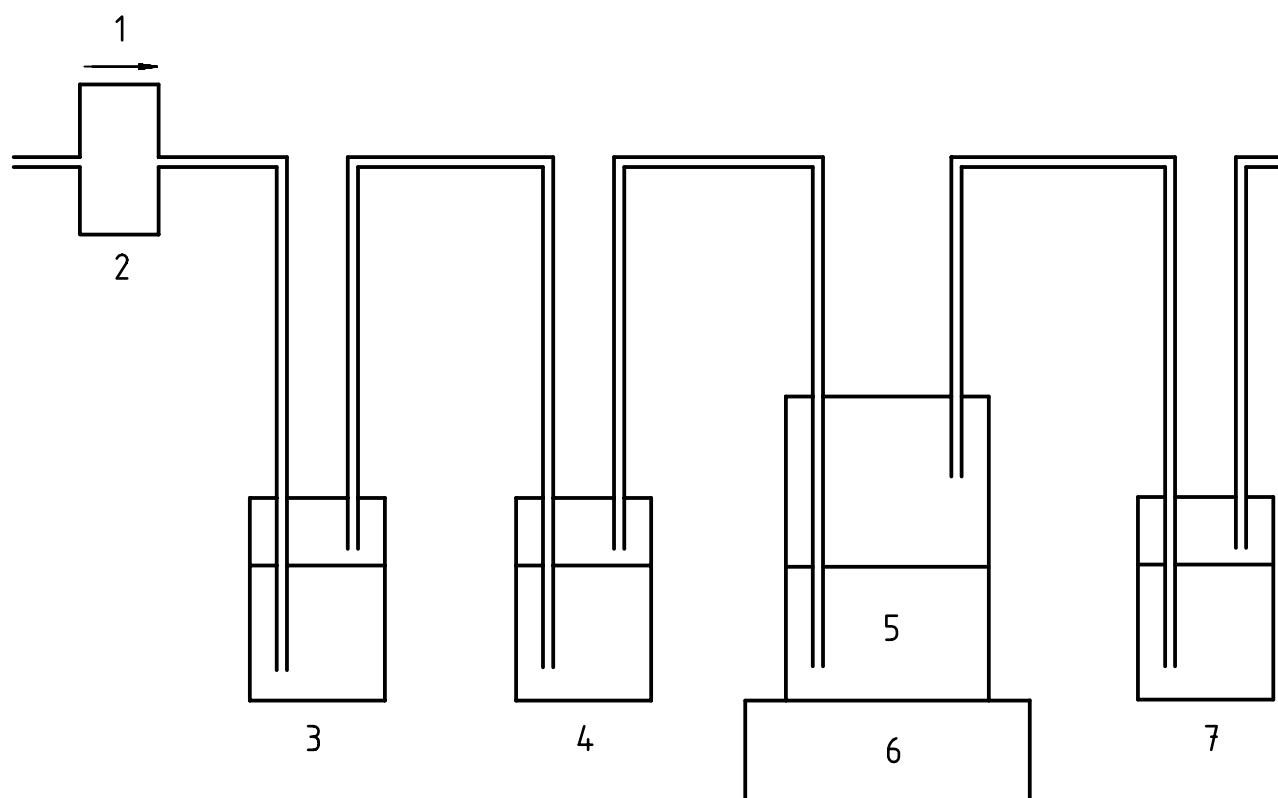

Key

- 1 Compressed air
- 2 Flow controller
- 3 Carbon dioxide trap (NaOH)
- 4 Carbon dioxide indicator [$\text{Ba}(\text{OH})_2$]
- 5 Test vessels
- 6 Stirrer
- 7 Carbon dioxide trap [$\text{Ba}(\text{OH})_2$ or (NaOH)]

Figure A.1

Annex B (informative)

Examples of the determination of released carbon dioxide

B.1 CO₂ determination by DIC measurement

The CO₂ released is absorbed in sodium hydroxide (NaOH) solution and determined as dissolved inorganic carbon (DIC) using e.g. a DOC analyser without incineration or oxidation.

Prepare a solution of NaOH ($c = 0,05$ mol/l) in deionized water. Measure the DIC of this solution and consider this blank value (ρ_B) when calculating the CO₂ production. Connect two absorber vessels in series with the test vessel, each containing at least 100 ml of the NaOH solution. Close the outlet of the last vessel with a small syphon to prevent introduction of CO₂ from the air to the NaOH solution. On the days of CO₂ determination, remove the vessel closest to the test vessel and take a sufficient sample for DIC measurement (e.g. 10 ml). Replace the vessel by the second and add a new one with freshly prepared NaOH solution. On the last day measure, after acidification of the test solution, DIC in both vessels.

Calculate the CO₂ produced using equation (B.1):

$$m_{Tt} = \frac{(\rho_T - \rho_B) \times 3,67}{10} \quad (\text{B.1})$$

where

m_{Tt} is the mass, in milligrams, of CO₂ released in vessel F_T between the start of the test and time t ;

ρ_T is the measured DIC concentration, in milligrams per litre, of the NaOH in vessel F_T solution at time t ;

ρ_B is the measured DIC concentration, in milligrams per litre, of the NaOH in the blank F_B solution at time t ;

3,67 is the ratio of the relative molecular/atomic masses CO₂/C (44/12);

10 is a correction factor, expressed in reciprocal litres, for 100 ml volume of the NaOH solution. If other volumes are used adapt this factor.

B.2 Titrimetric method using barium hydroxide

The CO₂ produced reacts with the barium hydroxide [Ba(OH)₂·8H₂O] and is precipitated as barium carbonate (BaCO₃) [equation (B.2)]. The amount of released CO₂ is determined by titrating the remaining Ba(OH)₂ with hydrochloric acid (HCl) [equation (B.3)].



Dissolve 4,0 g Ba(OH)₂·8H₂O in 1 000 ml deionized or distilled water to obtain a 0,0125 mol/l solution. It is recommended that a sufficient amount, e.g. 5 l, be prepared at one time when running a series of tests. Filter free of solid material and determine the exact normality by titration with a standard HCl solution for calculation of the test results. Store sealed as a clear solution to prevent absorption of CO₂ from the air.

Dissolve 50 ml of HCl solution ($c = 1 \text{ mol/l}$) (36,5 g/l) in 1 000 ml deionized or distilled water to obtain a 0,05 mol/l solution. Use phenolphthalein as an indicator or an automatic titrator to determine the endpoint.

At the start of the test, dispense exactly 100 ml of the Ba(OH)_2 solution into each of the three absorber vessels. Depending on the character and amount of the test compound, use modifications of the trapping volumes. Periodically, on each day of measurement, remove the vessel nearest the test vessel for titration. This should take place as needed, e.g. when the first absorber vessel is turbid due to precipitation of BaCO_3 and before any turbidity can be observed in the second vessel. Usually, at the beginning of the test, titration may be required every other day and then every fifth day when the plateau phase is reached. After removing the absorber vessel, immediately seal it with a plug to avoid CO_2 input from air. Move the remaining two vessels one position closer to the test vessel and place at the end of the series a new vessel filled with fresh Ba(OH)_2 solution. Handle all vessels containing test compound, reference compound, blank, inhibition and inoculum control in exactly the same way.

Immediately after removing the vessel, titrate either the whole amount (100 ml) or two or three portions of the Ba(OH)_2 solution with the HCl solution. Note the volumes of the HCl solution needed for neutralization.

The mass of CO_2 trapped in the absorber vessel is given by equation (B.4):

$$m_T = \left\{ \frac{2c_{\text{Ba}} \cdot V_{\text{B0}}}{c_{\text{HCl}}} - V_A \cdot \frac{V_{\text{BT}}}{V_{\text{BZ}}} \right\} \cdot c_{\text{HCl}} \times 22 \quad (\text{B.4})$$

where

m_T is the mass of CO_2 , in milligrams, trapped in the absorber of vessel F_T ;

c_{HCl} is the exact concentration, in moles per litre, of the HCl solution;

c_{Ba} is the exact concentration, in moles per litre, of the Ba(OH)_2 solution;

V_{B0} is the volume, in millilitres, of the Ba(OH)_2 solution at the beginning of the test;

V_{BT} is the volume, in millilitres, of the Ba(OH)_2 solution at time t before filtration;

V_{BZ} is the volume, in millilitres, of the aliquots of the Ba(OH)_2 solution used for titration;

V_A is the volume, in millilitres, of the HCl solution used for titration of the Ba(OH)_2 solution;

22 is the half-molarity of CO_2 .

When the following conditions apply:

- volume of the Ba(OH)_2 solution before and after absorption is exactly 100 ml and the complete solution is used for titration ($V_{\text{B0}} = V_{\text{BT}} = V_{\text{BZ}}$);
- concentration of the Ba(OH)_2 solution is exactly $c_{\text{Ba}} = 0,0125 \text{ mol/l}$;
- concentration of the HCl solution is exactly $c_{\text{HCl}} = 0,05 \text{ mol/l}$;

use equation (B.5):

$$m_T = 1,1 (50 - V_A) \quad (\text{B.5})$$

Annex C (informative)

Example of a biodegradation curve

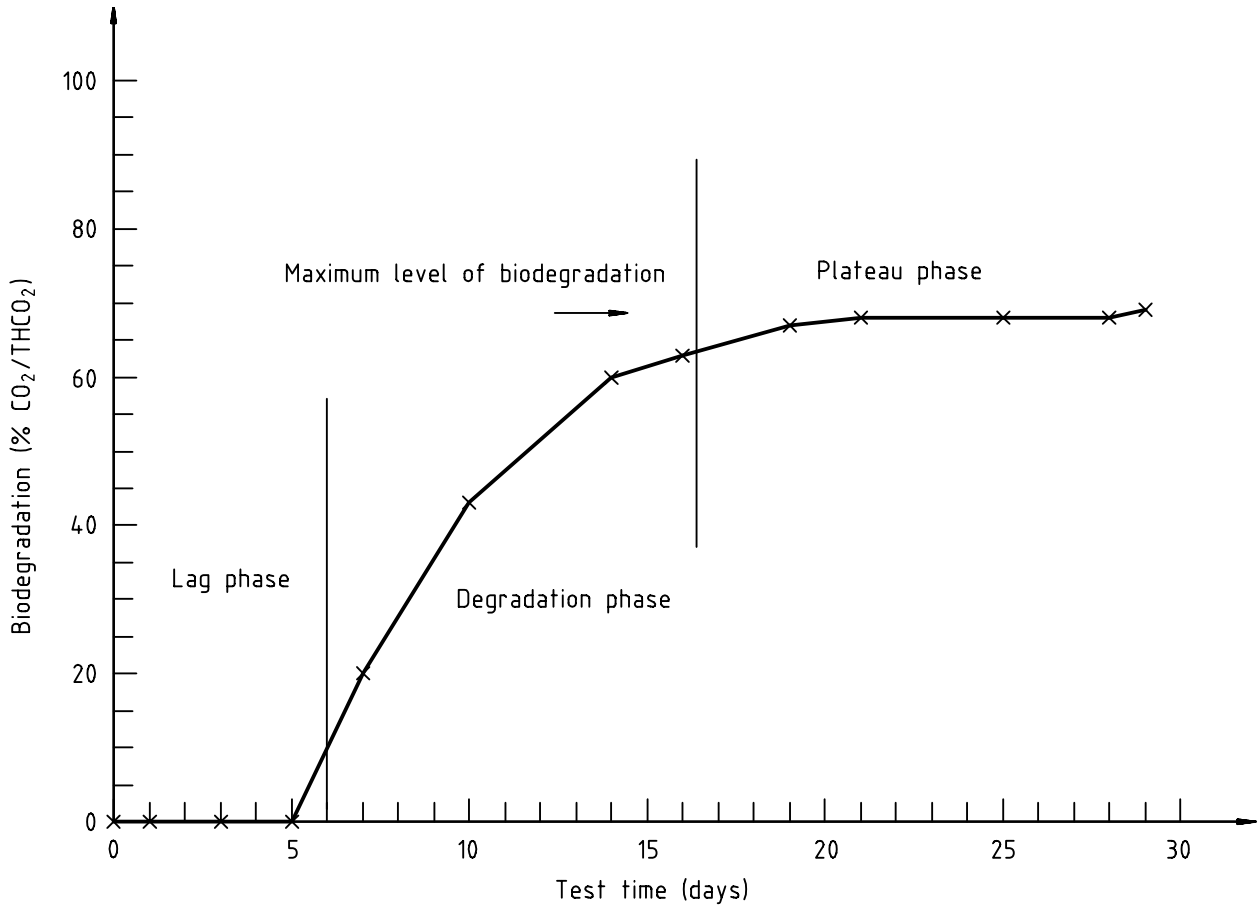


Figure C.1 — Biodegradation of aniline in the CO₂ evolution test

Annex D (informative)

Combined determination of carbon dioxide and DOC

D.1 Scope and principle

This variation of the CO₂ evolution test combines two different independent parameters in a single test system, DOC removal and CO₂ production; the latter is an unambiguous parameter for biodegradation and provides therefore more reliable information. This test variation can be used only for sufficiently water-soluble test compounds and is especially recommended if a higher degradation potential is required as it allows higher concentrations of the inoculum and the test compound. The method is also recommended to determine biodegradation and not only abiotic elimination for adsorbing compounds instead of a test based only on DOC removal such as ISO 9888.

The same principle of CO₂ measurement is used, but in addition DOC is determined at the beginning and end of the test, or in samples taken regularly during the incubation period, and the DOC removal is calculated.

If a substance-specific analytical method is available, it can be used to determine the primary biodegradation of the test compound when this is measured in addition to, or instead of, DOC.

If this variation of the CO₂ evolution test is used, it shall be quoted in the test report.

D.2 Reagents

If the higher inoculum and test compound concentrations are used, as recommended in this annex, an increase of the buffering capacity and the nutrient content of the inorganic medium is required. Use in this case the following optimized test medium:

a) Solution a)

Dissolve

anhydrous potassium dihydrogen phosphate (KH ₂ PO ₄)	13,6 g
disodium hydrogen phosphate dihydrate (Na ₂ HPO ₄ ·2H ₂ O)	26,9 g
ammonium chloride (NH ₄ Cl)	2,0 g
in water (6.1), quantity necessary to make up to	1 000 ml

b) Solution b)

Dissolve 22,5 g magnesium sulfate heptahydrate (MgSO₄·7H₂O) in water (6.1), quantity necessary to make up to 1 000 ml.

c) Solution c)

Dissolve 36,4 g calcium chloride dihydrate (CaCl₂·2H₂O) in water (6.1), quantity necessary to make up to 1 000 ml

d) Solution d)

Dissolve 0,25 g iron(III) chloride hexahydrate (FeCl₃·6H₂O) in water (5.1), quantity necessary to make up to 1 000 ml. Acidify with a drop of concentrated hydrochloric acid to avoid precipitation.

e) Solution e) (trace elements solution, optional)

Dissolve in 10 ml aqueous hydrochloric acid (HCl) solution (25 %, 7,7 mol/l) in the following sequence: 70 mg ZnCl₂, 100 mg MnCl₂·4H₂O, 6 mg H₃BO₃, 190 mg CoCl₂·6H₂O, 3 mg CuCl₂·2H₂O, 240 mg NiCl₂·6H₂O, 36 mg Na₂MoO₄·2 H₂O, 33 mg Na₂WO₄·2 H₂O, 26 mg Na₂SeO₃·5 H₂O and make up to 1 000 ml with the water (5.1).

For 1 litre of test medium, add to about 800 ml of water (5.1) 100 ml of solution a) and 1 ml of each of the solutions b) to e). Make up to 1 000 ml with the water (5.1) and measure the pH.

D.3 Inoculum

Use the same inoculum as in 7.2. The concentration of activated sludge can, however, be increased up to 150 mg/l suspended solids. Use in this case the optimized test medium.

D.4 Test procedure

Provide sufficient suitable vessels as described in 7.3 in the test environment (clause 4). Use vessels as described in 6.1 fitted with magnetic stirrer rods. If samples are to be taken during the test, locate at the side of each vessel a neck with a valve for taking samples for DOC or substance-specific analyses. In this case shaking is not recommended. Connect the incubation vessels to absorption vessels as described in annex B.

Add standard or optimized test medium and inoculum. Add normally 40 mg/l organic carbon of the test compound (7.1.1) or the reference compound (7.1.2). Use a final test volume of e.g. 1500 ml. Start the incubation with aerating and stirring the mixtures. Aerate in the case of 150 mg/l suspended solids with 150 ml/h to 300 ml/h CO₂-free air as described in annex A.

Take at regular time intervals, as described in 7.3, samples of sufficient volume (e.g. 15 ml) and determine DOC at least in duplicate (use e.g. ISO 8245). Determine the CO₂ released as described in 7.3 and annex B. If samples are taken for DOC or substance specific analyses consider on each day of sampling the change of ThCO₂ in the test vessel. Adapt in this case V_L in equation (1) (8.1) to the new volume.

If DOC removal shall not be followed during the test, take samples only at the beginning and the end (before acidification) and determine DOC. In this case no special test vessels are required.

If a suitable substance-specific analytical test method is available and primary biodegradation shall be determined, measure the concentration of the test compound in the samples taken for DOC analysis.

D.5 Calculation of biodegradation based on CO₂ evolution

Calculate the test result as given in 8.1

D.6 Calculation of DOC removal

Calculate for each test vessel F_T the percentage elimination of dissolved organic carbon D_C using equation (8):

$$D_C = \left(1 - \frac{\rho_{CTt} - \rho_{CBt}}{\rho_{CT0} - \rho_{CB0}} \right) \times 100 \quad (8)$$

where

ρ_{CT0} is the DOC concentration, in milligrams per litre, at time 0, in the test vessel F_T ;

ρ_{CB0} is the DOC concentration, in milligrams per litre, at time 0 in the blank vessel F_B ;

ρ_{CTt} is the DOC concentration, in milligrams per litre, at time t in the test vessel F_T ;

ρ_{CBt} is the DOC concentration, in milligrams per litre, at time t in the blank vessel F_B .

In the case of adsorbing substances it is important to determine ρ_0 before the inoculum is added and to ignore in this case ρ_{B0} .

Calculate in the same way the biodegradation of the reference compound F_C and, if included, of the abiotic elimination check F_S and the inhibition control F_I .

D.7 Calculation of primary degradation

When specific analyses of the test compound are performed, calculate the percentage of primary degradation D_S of the test compound using equation (9).

$$D_S = \frac{\rho_S - \rho_T}{\rho_S} \times 100 \quad (9)$$

where

ρ_T is the concentration of the test compound, in milligrams per litre, in vessel F_T at time t ;

ρ_S is the concentration of the test compound, in milligrams per litre, in vessel F_S at time t .

D.8 Expression of results

Compile and handle the data, e.g. plotting an elimination curve, as described in 8.3.

D.9 Validity criteria

See 9.1. If the higher concentration of the inoculum is used (150 mg/l dry matter, see D.3), the concentration of CO_2 in the blank at the end of the test should be at about 150 mg/l.

Bibliography

- [1] ISO 7827, *Water quality — Evaluation in an aqueous medium of the ultimate aerobic biodegradability of organic compounds — Method by analysis of dissolved organic carbon (DOC)*.
- [2] ISO 8192, *Water quality — Test for inhibition of oxygen consumption by activated sludge*.
- [3] ISO 8245, *Water quality — Guidelines for the determination of total organic carbon (TOC)*.
- [4] ISO 9408, *Water quality — Evaluation in an aqueous medium of the ultimate aerobic biodegradability of organic compounds — Method by determining the oxygen demand in a closed respirometer*.
- [5] ISO 9887, *Water quality — Evaluation of the aerobic biodegradability of organic compounds in an aqueous medium — Semi-continuous activated sludge method (SCAS)*.
- [6] ISO 9888, *Water quality — Evaluation of the aerobic biodegradability of organic compounds in an aqueous medium — Static test (Zahn-Wellens method)*.
- [7] ISO 10634, *Water quality — Guidance for the preparation and treatment of poorly water-soluble organic compounds for the subsequent evaluation of their biodegradability in an aqueous medium*.
- [8] ISO 11923, *Water quality — Determination of suspended solids by filtration through glass-fibre filters*.
- [9] ISO 14593, *Water quality — Evaluation of the ultimate aerobic biodegradability of organic compounds in aqueous medium — Method by analysis of released inorganic carbon in sealed flasks*.
- [10] ISO 15462, *Water quality — Selection of tests for biodegradability*.
- [11] Birch, R.R., and Fletcher, R.J. The application of dissolved inorganic carbon measurements to the study of aerobic biodegradability. *Chemosphere*, **23**, 1991, pp. 507-524.
- [12] *OECD Guidelines for the Testing of Chemicals*, 301 B CO₂ Evolution Test. Organisation for Economic Cooperation and Development, Paris, 1993.
- [13] Strotmann U., Schwarz H. and Pagga U. The CO₂/DOC-combination test — A new method to determine the biodegradability of chemical compounds. *Chemosphere*, **30**, 1995, pp. 525-538.
- [14] Weytjens D., van Ginneken I. and Painter H.A. The recovery of carbon dioxide in the Sturm test for ready biodegradability. *Chemosphere*, **28**, 1994, pp. 801-812.

ICS 13.060.70

Price based on 17 pages
