

INTERNATIONAL STANDARD

ISO 9898

First edition
2000-02-15

Equipment for crop protection — Test methods for air-assisted sprayers for bush and tree crops

*Matériel de protection des cultures — Méthodes d'essai des pulvérisateurs
à jet porté pour les arbustes et arbres fruitiers*



Reference number
ISO 9898:2000(E)

© ISO 2000

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

© ISO 2000

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 734 10 79
E-mail copyright@iso.ch
Web www.iso.ch

Printed in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this International Standard may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

International Standard ISO 9898 was prepared by Technical Committee ISO/TC 23, *Tractors and machinery for agriculture and forestry*, Subcommittee SC 6, *Equipment for crop protection*.

Annex A forms a normative part of this International Standard.

Equipment for crop protection — Test methods for air-assisted sprayers for bush and tree crops

1 Scope

This International Standard specifies the methods for measuring the characteristics of mounted, towed and self-propelled air-assisted sprayers, including pneumatic sprayers, used for crop protection in bushes, vineyards and tree crops.

This International Standard specifies testing methods to define sprayers' performances in control conditions (laboratory) with respect to minimising the risk of environmental contamination.

2 Normative reference

The following normative document contains provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the normative document indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 13441-1, *Air-assisted agricultural sprayers — Data sheets — Part 1: Typical layout.*

3 Test conditions

3.1 Sprayer settings

Tests shall be done with the machine in working order (grids, nozzles, deflectors, etc.).

3.2 Sprayer set-up

The deflector positions, the shapes and the orientation of the air outlet, the nozzle orientation and the other device modifying the air or the liquid distribution should be described in the report. Schematic diagrams and photographs can be used to describe the sprayer set-up.

3.3 Sprayer environment

There should be no obstacles within a distance of at least 5 m in the direction(s) of the outlet velocity.

3.4 PTO speed

The test shall be done at least for the nominal PTO (power take-off) speed (540 ± 5) r/min¹⁾.

1) (1000 ± 10) r/min in the case of sprayers operating at 1000 r/min.

3.5 Sprayer gear box

If the power transmission includes a device providing different speeds for the fan rotation, the tests should be done for all the gear box positions. The PTO speed and the different fan rotation speeds should be measured.

3.6 Fan with variable pitch blades

For the sprayer's fan equipped with variable pitch blades, the test should be done at least with the angle recommended by the manufacturer. Otherwise, the medium position or the nearest medium position of the adjustment range shall be adopted for the test.

3.7 Variable width fan outlet

For the sprayer equipped with a variable outlet, the tests should be done at least with the width recommended by the manufacturer. Otherwise, the central position or the nearest central position of the adjustment range shall be adopted for the test.

3.8 Mounted sprayer equipped with an axial fan

The height of the fan axis should be mentioned in the report.

3.9 Test liquid

Clean water free from solids in suspension. If any tracer or dye is used on the tests, it shall be reported.

3.10 Atmospheric conditions

Temperature and humidity should be reported.


4 Measurement of the sprayer power consumption

The total power consumption in working order (fan, pump, etc.) shall be measured, for example with a torquemeter. During the test the liquid flow from the nozzle shall be switched off. The measurement shall be made with the maximum pressure recommended by the manufacturer.

5 Measurement of the flow rate

5.1 Reference method

A measuring chamber connected to two measuring tubes shall be used as a general method to measure the air flow rate at the inlet or at the outlet of the single or multiple fans of the sprayer. For the basic set-up of the chamber test stand, see Figure 1. For the possible connections between the measuring chamber and the different types of air-assisted sprayers, see Figure 2.

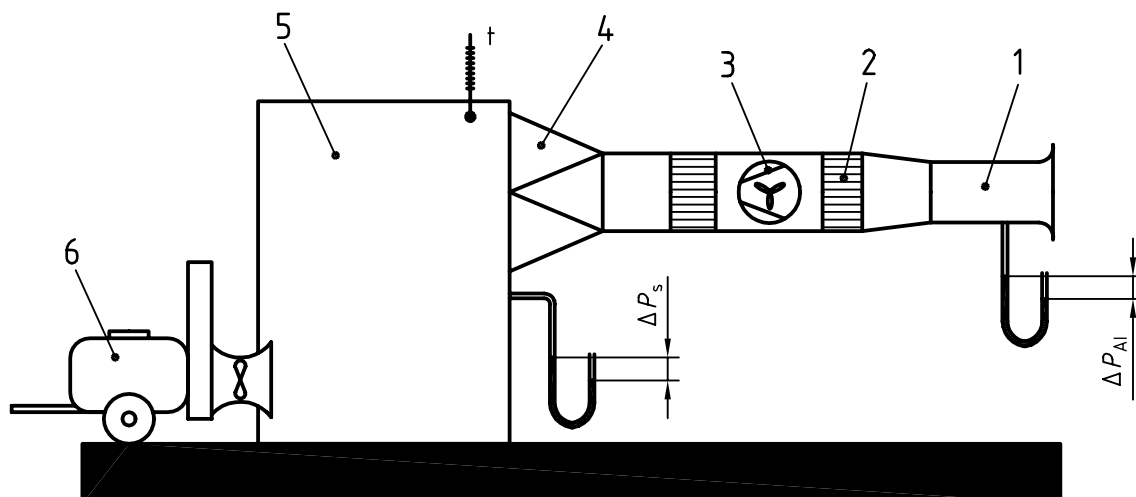**Key**

- 1-4 Measuring tube
- 1 Calibrated air intake
- 2 Flow straightener
- 3 Auxiliary fan
- 4 Connecting piece
- 5 Measuring chamber
- 6 Air-assisted sprayer

Figure 1 — Basic set-up of the chamber test stand

The chamber test stand shall have the following specifications.

Its main parts are a tight chamber and, connected to it, two measuring tubes (measuring range of tube 1 with 900 mm diameter is 20 000 m³/h to 110 000 m³/h and for tube 2 with 450 mm diameter it is 2 000 m³/h to 20 000 m³/h). The dimensions of the chamber are: width = 4,6 m, length = 6,15 m and height = 3,7 m. One wall of the chamber is made from removable stays and metal plates and allows the sprayer to be connected with the chamber. The fan of the sprayer sucks the air volume out of the chamber and the same amount of air volume is blown into the chamber with the auxiliary fan of one of the measuring tubes. To make sure that the fan operates under the same conditions as outside in the field, its speed shall be controlled and the air flow rate of the auxiliary fan shall be adjusted to the flow rate of the tested fan. This shall be verified by the static pressure difference $\Delta P_s = 0$ between measuring chamber and the ambient atmosphere. The pressure ΔP_{AI} in the calibrated air intakes of the measuring tubes represents the air flow rate. The formulae to calculate the air flow rate from the pressure ΔP_{AI} are:

for tube 1:

$$q_V = 3\,203,20 \times \sqrt{\frac{\Delta P_{AI}}{\rho}}$$

for tube 2:


$$q_V = 88,288\,3 \times \sqrt{\frac{\Delta P_{AI}}{\rho}}$$

where


q_V is the flow rate, expressed in cubic metres per hour;

ΔP_{AI} is the pressure in the calibrated air intakes of the measuring tubes, expressed in pascals;


ρ is the air density, expressed in kilograms per cubic metre.

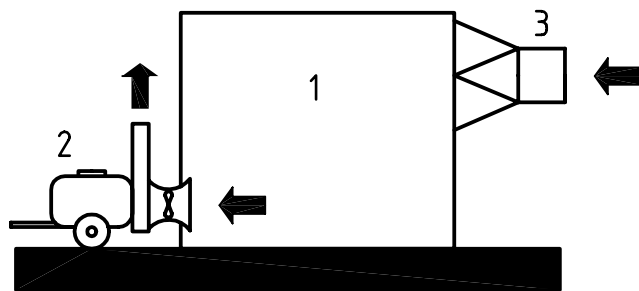

a) Set-up for a one way sucking air-assisted sprayer in the measuring chamber

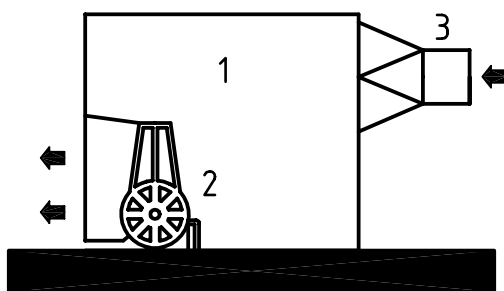

b) Set-up to measure the half side air flow rate of an air-assisted sprayer

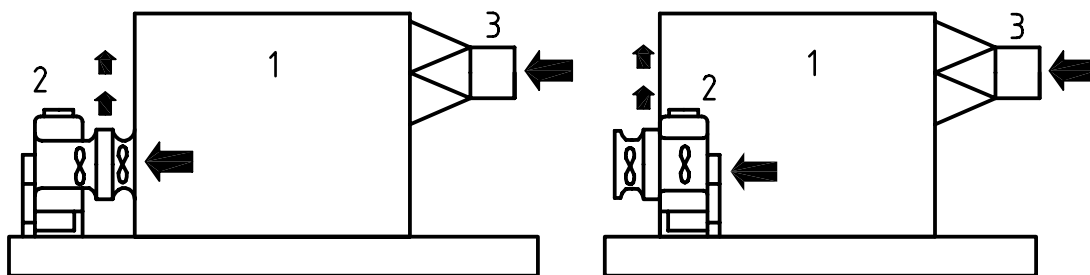

c) Set-up for a two way sucking air-assisted sprayer in the measuring chamber

Key

- 1 Measuring chamber
- 2 Sprayer
- 3 Measuring tube

Figure 2 — Possible connections between the measuring chamber and the different types of air-assisted sprayers

5.2 Other methods

5.2.1 General

The air flow rate of air-assisted sprayers also can be measured at the intake or outlet side of the fan with different instruments for measuring the air velocity. Instruments could be Prandtl tubes, hot wire, small propeller anemometers or laser anemometer. An ultrasonic anemometer could be used to measure the air flow rate at the outlet of the air-assisted sprayers, but not at the intake. In order to provide representative measurements of the air velocity in the cross section area, a minimum number of measuring points shall be taken (see 5.2.2 and 5.2.3). The flow rate shall be calculated by multiplying the air speed in the 90° cross section area by the cross section area of the wind flow. Obstacles like deflectors, nozzles or structural components of the fan, shall be accounted for when the total cross area of the fan is calculated.

For hot wire, small propeller anemometers and laser anemometers, ensure that their measurements agree with Prandtl tube measurements. The number of measuring points to be taken in the cross section area shall be the same as established for Prandtl tube measurements.

For each measurement point, a mean of air velocities for a minimum period of 10 s with a minimum of 100 data samples will be taken.

The higher dimension (length or diameter) of the head including the sensing device to be introduced into the air stream shall be less than 25 mm.

The measuring error shall be less than 5 %.

With Prandtl tubes for each measuring point, air speed shall be calculated by means of the following expression:

$$v = \sqrt{\frac{2 \times \Delta P}{\rho}}$$

where

- v is the air velocity, expressed in metres per second;
- ΔP is the differential pressure measured by means of the Prandtl tube, expressed in pascals;
- ρ is the air density, expressed in kilograms per cubic metre.

To calculate the air density, the atmospheric pressure and the air temperature shall be measured. For the calculation, use the following expression:


$$\rho = 0,348 \times p / T$$

where

- ρ is the air density, expressed in kilograms per cubic metre;
- p is the atmospheric pressure, expressed in millibar;
- T is the air temperature, expressed in kelvins.

5.2.2 Measurement of air flow rate on the suction side of a fan

The measurement should be done in a pipe connected to the suction side of the fan. In order not to influence the suction of the fan, the diameter of the pipe should be 1,5 times of the suction diameter of the fan. The length of the pipe should be at least 2 m. The measurement of the air velocity should be done with Prandtl Tubes in a cross section of the pipe, ¾ of the pipe length away from the suction opening of the fan (see Figure 3).

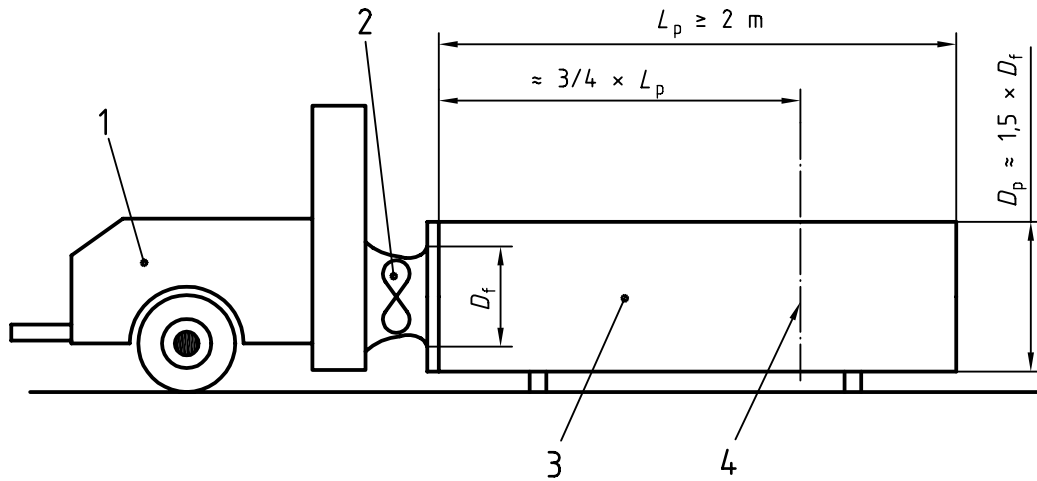

- D_f suction diameter of fan
- D_p diameter of the pipe connected to the fan
- L_p length of the pipe connected to the fan

Key

- 1 Air-assisted sprayer
- 2 Fan
- 3 Pipe
- 4 Cross-section for measurement

Figure 3 — Measurement of air flow rate on the suction side of a fan

The measuring points in the cross section should be positioned on centroidal circles of five circular rings with uniform surface areas. There should be at least three measuring points (every 120°) on each centroidal circle (see Figure 4).


Circular rings are defined by the following formulas:

$$R_i / R = \sqrt{1 - (i / n)}$$

$$Y_i / R = 1 - \sqrt{1 - \frac{2i - 1}{2n}}$$

where

- Y_i are the distances between the pipe side and the measuring points;
- R_i are the radii of the circles;
- n is the total number of circular rings;
- i is the special number of circular ring.

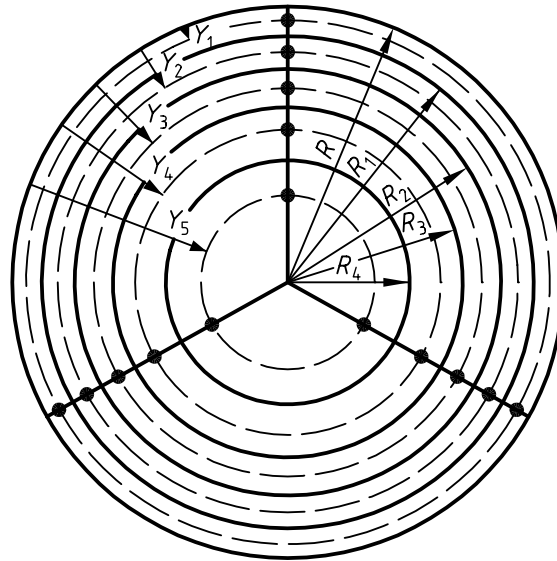

Key

- measuring points
- - - - concentric circles

Figure 4 — Cross-section for measuring, position of measuring points

For different pipe diameters, divided into 5 circular rings ($n = 5$), the distances Y_1 to Y_5 between the pipe side and the measuring points on centroidal circles are calculated and shown in Table 1.

Table 1 — Distances between the pipe side and measuring points for different pipe diameters

Dimensions in millimetres

Pipe diameter	Distances between the pipe side and measuring points				
	Y_1	Y_2	Y_3	Y_4	Y_5
100	3	8	15	23	34
200	5	16	29	45	68
300	8	25	44	68	103
400	10	33	59	90	137
500	13	41	73	113	171
600	15	49	88	136	205
700	18	57	103	158	239
800	21	65	117	181	274
900	23	74	132	204	308
1000	26	82	146	226	342
1100	28	90	161	249	376
1200	31	98	176	271	410
1300	33	106	190	294	444
1400	36	114	205	317	479
1500	38	123	220	339	513

This method can also be used for measurements on the pressure side if there are circular shaped outlets.

5.2.3 Measurement of air flow rate on the outlet side of a fan

For rectangular areas a rectangular grid of measuring points is recommended and the minimum number of measuring points shall be taken according to Table 2.

Table 2 — Definition of measuring points


Dimension of cross-section cm ²	Type or shape of air outlet (inlet)	Maximum area covered by each point cm ² /point	Minimum number of measurement points	Point area/total outlet area
< 100	<ul style="list-style-type: none"> ▪ Single outlets on radial, axial or cross flow fans (ISO 13441-1 - 502.4) ▪ Secondary outlets on axial fan (ISO 13441-1 - 502.1) 	5	20	> 0,05
100 to 500	<ul style="list-style-type: none"> ▪ Secondary outlets on axial fan (ISO 13441-1 - 502.1) ▪ Rectangular outlets on cross-flow fan (ISO 13441-1 - 502.5) 	10	10 to 50	0,1 to 0,02
500 to 2 000	<ul style="list-style-type: none"> ▪ Main (ring) outlets on axial fan (ISO 13441-1 - 502.1) ▪ Rectangular outlets on axial fan, vertical deflectors (ISO 13441-1 - 502.2) ▪ Rectangular outlet on cross-flow fans (ISO 13441-1 - 502.5) 	25	25 to 80	0,05 to 0,012 5
2 000 to 4 000	<ul style="list-style-type: none"> ▪ Main (ring) outlets on axial fan (ISO 13441-1 - 502.1) ▪ Rectangular outlets on axial fan, vertical deflectors (ISO 13441-1 - 502.2) ▪ Rectangular outlet on cross-flow fans (ISO 13441-1 - 502.5) 	50	40 to 80	0,025 to 0,012 5
> 4 000	<ul style="list-style-type: none"> ▪ Rectangular outlets on axial fan, vertical deflectors (ISO 13441-1 - 502.2) 	100	40	< 0,025
> 4 000	<ul style="list-style-type: none"> ▪ Pipes connected to the suction side (circle section) 	250	16	< 0,125

6 Measurement of the air velocity distribution at distance (static test)

Scanning velocities and air flow direction at 0,5 m distance from the air outlet. Displacement of the sprayer or the measuring sensors at a speed less than 1 cm/s.

Measuring sensors for air flow direction could be vanes with angle decoder (for air velocity, see 5.2.1). Velocity and direction also can be measured in combination by use of a five-hole Pitot tube or a laser anemometer.

In a static measurement on the vertical line with the maximum air velocity, the air velocity in the flow direction and the flow direction shall be measured in 10 cm sections with 1 cm steps within 10 s. The representative air velocity and air flow angle shall be evaluated by temporal integration and reported for each section (see example in Figure 5).

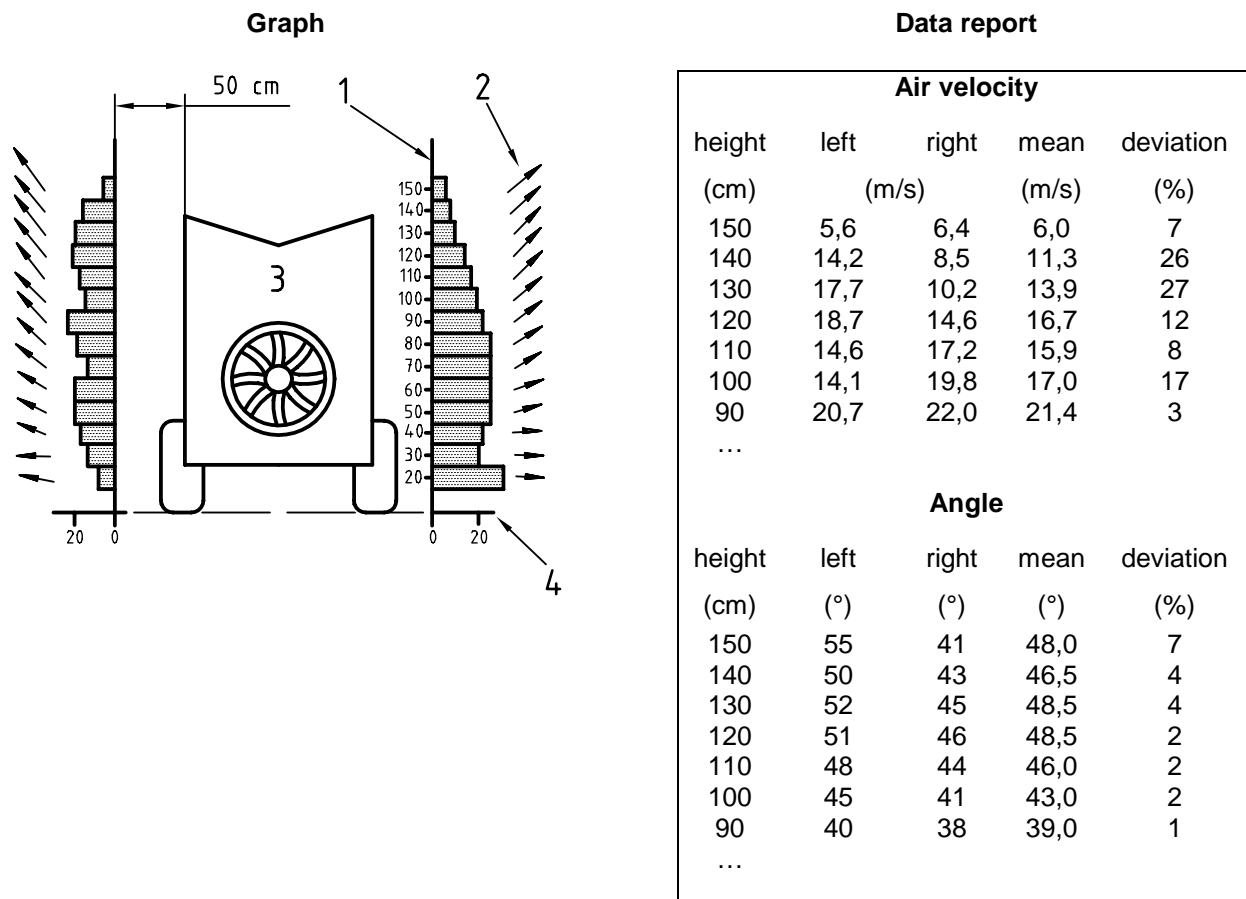


Key

- 1 Height (cm)
- 2 Angle (°)
- 3 Air-assisted sprayer
- 4 Air velocity (m/s)

Figure 5 — Example of a graph and data report about air flow direction and air velocity distribution at distance

On request of the manufacturer, the air velocity along the width of the air outlet may be scanned and reported as well (see Figure 6).

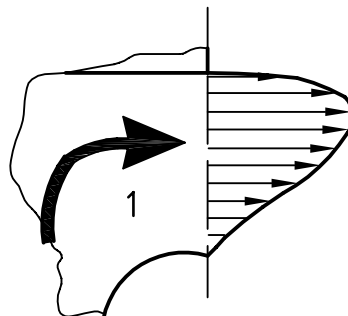

Key

- 1 Air outlet

Figure 6 — Optional measurement of the air velocity along the width of the air outlet

7 Measurement of the liquid distribution

7.1 General

The liquid distribution can be measured in static (7.2) or dynamic conditions (7.3).

For the air-assisted sprayers for the use in vineyards (and sometime orchards), the test should be done at 1,25 m from the sprayer axis and with those for the use in orchards and in hops the distance from the sprayer axis should be 2 m (see Figure 7).

For the sprayer types used to treat overlapping canopies (for example pergola vineyards), the horizontal liquid distribution can be done by putting collectors at 2,5 m above the soil.

The nozzles, the orientation of the nozzles, the hydraulic pressure should be given by the manufacturer in order to obtain an even distribution at the measured height.

7.2 Static tests (sprayer static)

7.2.1 The lamellae vertical patternator

The characteristics of the lamellae vertical patternator are given in annex A.

The water should be collected in sections of 0,25 m maximum.

The measuring height should be 4,5 m measured from the ground.

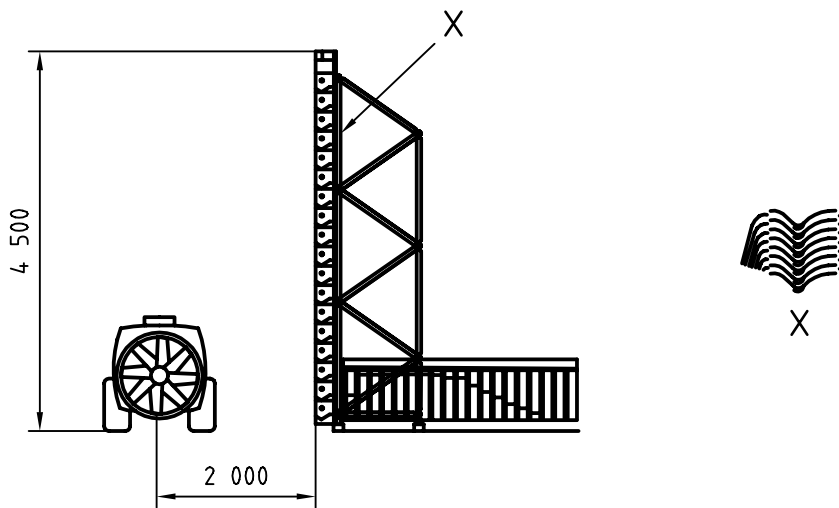


Figure 7 — Lamellae spray patternator with a conventional air-assisted sprayer

The results shall be presented in the form of tables (see Table 3) and graphs (see Figure 8).

Table 3 — Example of vertical liquid distribution (see graphs in Figure 8)


Adjustment

Tester	name	name	name	name	name	name
Date	97-02-20	97-02-20	97-02-20	97-02-20	97-02-20	97-02-20
Nozzle	type	type	type	type	type	type
Gear of fan	1	1	1	1	1	1
Pressure, bar	10,0	10,0	10,0	10,0	10,0	10,0
Rotation, 1/min	540	540	540	540	540	540
Distance, m	2,00	2,00	2,00	2,00	2,00	2,00
Adjustment of air jet	0...2,80 m	0...2,80 m	0...2,80 m	0...2,80 m	0...2,80 m	0...2,80 m
Side	left	left	left	right	right	right
Nozzle number						
10						
9						
8	off	off	off	off	off	off
7	off	off	2,80 m / on	2,80 m / on	off	off
6	off	2,45 m / on	2,45 m / on	2,45 m / on	2,45 m / on	off
5	1,95 m / on	1,95 m / on	1,95 m / on	1,95 m / on	1,95 m / on	1,95 m / on
4	1,45 m / on	1,45 m / on	1,45 m / on	1,45 m / on	1,45 m / on	1,45 m / on
3	0,95 m / on	0,95 m / on	0,95 m / on	0,95 m / on	0,95 m / on	0,95 m / on
2	0,45 m / on	0,45 m / on	0,45 m / on	0,45 m / on	0,45 m / on	0,45 m / on
1	off	off	off	off	off	off

Results

Height, m	Inflow, ml/min					
4,125...4,375						
3,875...4,125						
3,635...3,875						
3,375...3,635						
3,125...3,375						
2,875...3,125						
2,635...2,875			0	0		
2,375...2,635		0	128,8	133,3	0	
2,125...2,375	0	44,8	301,9	325,9	45,3	0
1,875...2,125	24,3	161,1	328,6	376,4	149,2	18,5
1,621...1,875	138,5	330,6	329,6	394,7	375,3	141,3
1,375...1,625	303,5	433,4	413,9	443,4	409,1	249,0
1,125...1,375	316,6	372,8	376,2	363,3	394,9	367,6
0,875...1,125	448,1	452,8	426,1	438,4	461,8	478,1
0,625...0,875	406,5	483,8	419,4	516,1	404,6	462,6
0,375...0,625	393,3	507,9	443,9	407,6	437,1	306,2
0,125...0,375	342,1	222,2	295,0	273,5	345,9	327,2

Positions of opened nozzles

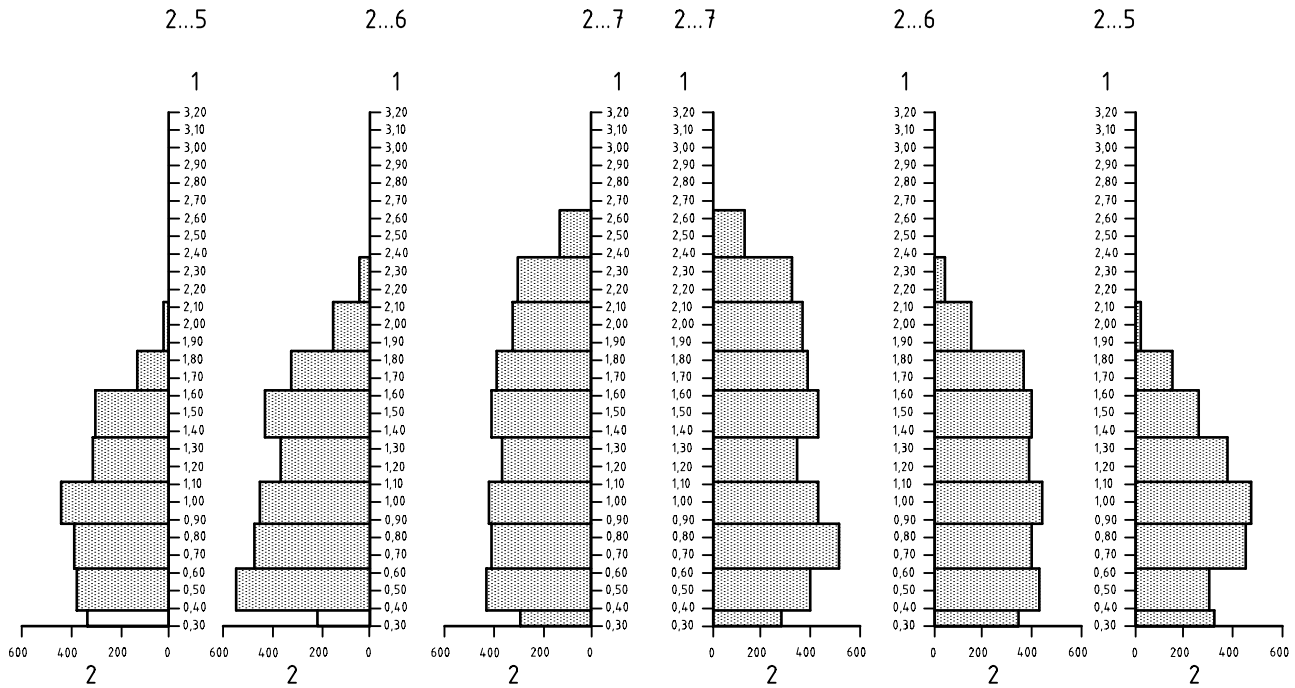

Key

- 1 Height (m)
- 2 Inflow (ml/min)

Figure 8 — Example of vertical liquid distribution

NOTE Other test benches are acceptable, if the same measuring accuracy can be achieved.

7.2.2 Artificial targets

The measuring principle relates to quantifying the spray retention on collectors (filter paper, cellulose cotton spongy sheet, etc.). As the collectors absorb the spray, their weight increases. This parameter shall be measured and recorded. The maximum time delay between spraying and recording should be mentioned in the test report.

The collectors should be fixed on a vertical pole. The size of these collectors should be less than 0,25 m × 0,25 m. The step between collectors in the vertical direction should be 0,25 m in order to limit the gaps.

The test should be done the sprayer static or the measuring device (vertical pole) moving very slowly in front of the sprayer at a constant velocity.

The measuring height should be 4,5 m measured from the ground.

The results should be presented in the form of tables (see Table 3) and graphs (see Figure 8).

7.3 Dynamic tests (sprayer moving)

7.3.1 General

This method requires a dynamic situation with the sprayer moving at its working speed (4 km/h) in front of a plane of collectors (Figure 9).

The collector shall have a high absorption capacity to the spray (filter paper, pipe cleaners, cellulose cotton spongy sheet for example).

Dimensions in centimetres

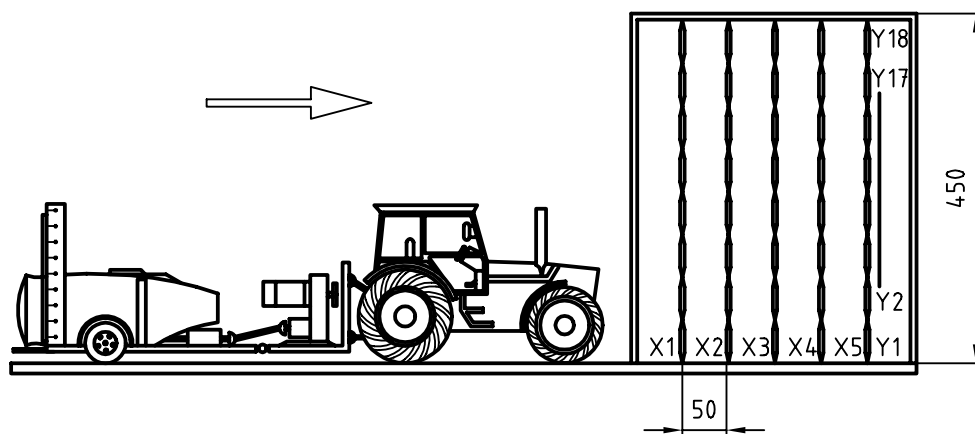


Figure 9 — Deposit in artificial targets with a vertical deflector sprayer

7.3.2 Pipe cleaners

At least five continuous vertical lines of collectors (4,5 m high) shall be built to monitor depositions at different heights.

The recommended distance between these vertical lines is between 0,1 m and 0,5 m.

The liquid to be sprayed shall contain a fluorescent tracer compound, e.g. Brilliant Sulfoflavine (BSF, maximum concentration: 1,5 g/l), for analysing the deposit. The solution shall be stirred to ensure a total mixing. Samples shall be taken before and after the application in order to verify the homogeneity of the mixture (for example, if the BSF is used as tracer, it is reached after 20 min).

After the treatment, the collectors shall be collected as soon as possible. Pipe cleaners shall be picked up using pincers. All the pipe cleaners of the same horizontal level shall be placed in a separate box or in plastic bag. The maximum distance of the horizontal levels shall be 0,25 m. The collectors shall be put immediately in a dark box to avoid photochemical degradation.

The collectors shall be washed with pure water and the concentration of tracer measured.

The results should be presented in the form of tables (see Table 3) and graphs (see Figure 8).

7.3.3 Filter papers

The collectors shall be fixed on a vertical pole. The size of these collectors shall be less than 0,25 m × 0,25 m. The step between collectors in the vertical direction should be 0,25 m in order to limit the gaps.

The measuring height should be 4,5 m measured from the ground.

The sprayed liquid shall contain a fluorescent tracer (Brilliant Sulfoflavine for example). The collectors shall be washed with pure water and the concentration of tracer measured.

The results should be presented in the form of tables (see Table 3) and graphs (see Figure 8).

8 Measurement of droplet size

This International Standard does not deal with the droplet sizes whose study is conditioned by the work conducted by the BCPC (British Crop Protection Council) and ISO/TC 23/SC 6.

9 Test report

9.1 Test conditions

The test conditions shall be noted in the report:

- sprayer set-up;
- PTO speed;
- position of the sprayer gear box and fan rotation speed;
- position of the fan variable pitch blades;
- width of the fan outlet;
- the height of the fan axis for the mounted sprayer;
- test liquid;
- atmospheric conditions:
 - temperature;
 - atmospheric pressure;
 - humidity;
 - wind direction and speed.

9.2 Instrumentation accuracy


The accuracy of all the measuring devices should be described in the report.

Annex A (normative)

Characteristics of the lamellae vertical patternator

A lamellae vertical patternator (see Figure A.1) shall be used to measure the liquid distribution in a static test. The main part of the patternator is a vertical wall, consisting of horizontal lamellae which separate the liquid droplets from the air flow. The air flow can pass freely through the wall. The separated liquid is collected in vertical sections and drained off in measuring cylinders. The vertical liquid distribution is represented by the filling height in the cylinders.

Dimensions in millimetres

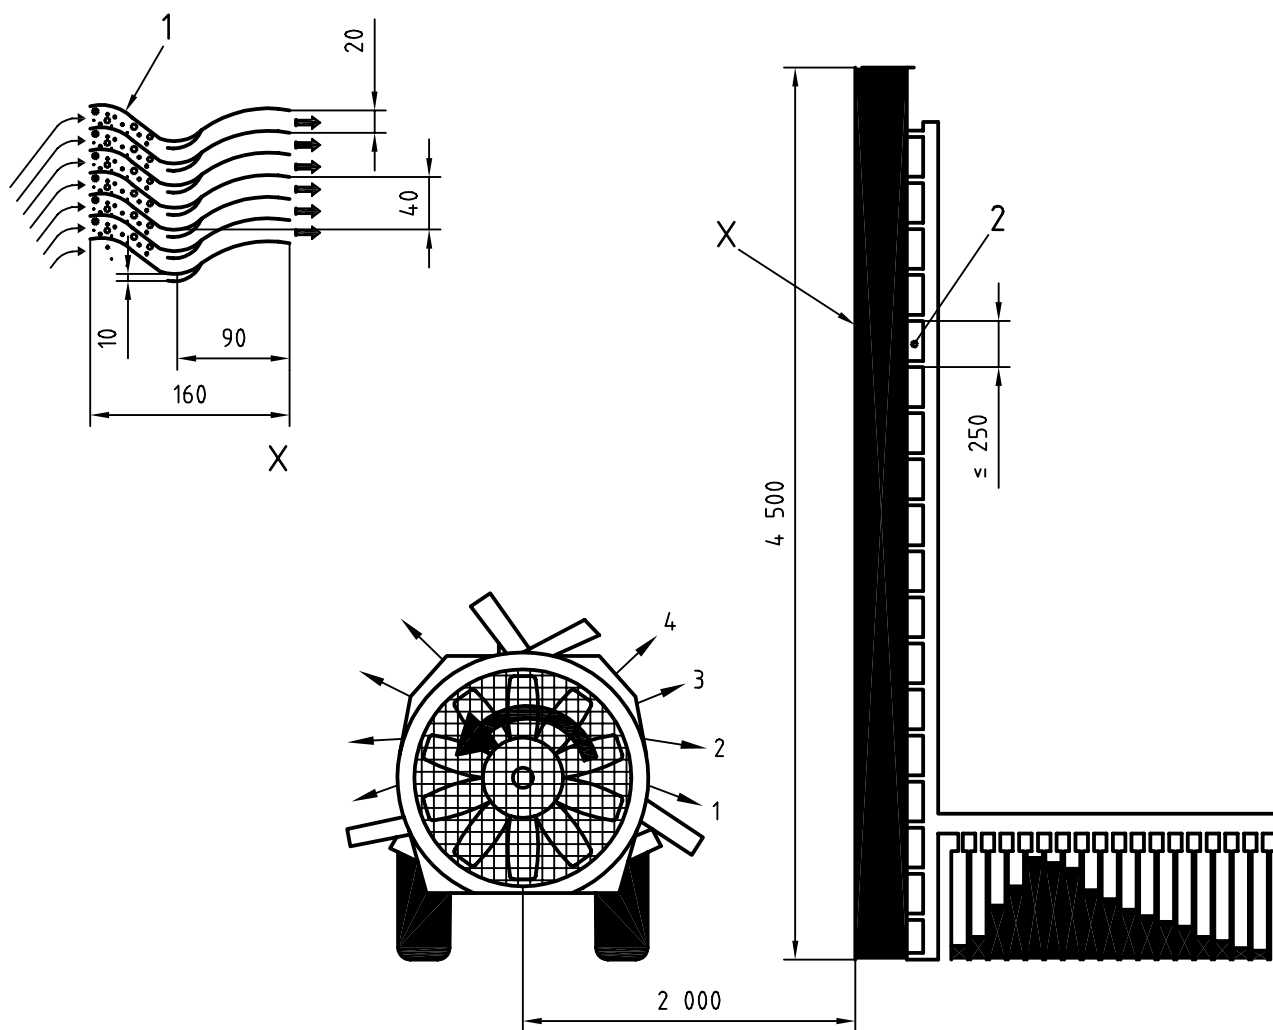

Key

- 1 Lamellae
- 2 Sampling raster

Figure A.1 — Schema of the vertical distribution test method with the vertical patternator

Vertical line of small characters or artifacts.

ICS 65.060.40

Price based on 15 pages

© ISO 2000 – All rights reserved