

---

---

**Animal and vegetable fats and  
oils — Determination of tocopherol  
and tocotrienol contents by high-  
performance liquid chromatography**

*Corps gras d'origines animale et végétale — Détermination des  
teneurs en tocophérols et en tocotriénols par chromatographie en  
phase liquide à haute performance*



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2016, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Ch. de Blandonnet 8 • CP 401  
CH-1214 Vernier, Geneva, Switzerland  
Tel. +41 22 749 01 11  
Fax +41 22 749 09 47  
copyright@iso.org  
www.iso.org

# Contents

Page

<b>Foreword</b> .....	<b>iv</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Principle</b> .....	<b>1</b>
<b>5 Reagents</b> .....	<b>1</b>
<b>6 Apparatus</b> .....	<b>2</b>
<b>7 Sampling</b> .....	<b>3</b>
<b>8 Preparation of test sample</b> .....	<b>3</b>
<b>9 Procedure</b> .....	<b>3</b>
9.1 Preparation of calibration solutions.....	4
9.1.1 Stock calibration solutions.....	4
9.1.2 Standard solution.....	4
9.2 Optimization of working parameters.....	4
9.3 Preparation of test solution.....	5
9.4 Determination.....	5
<b>10 Expression of results</b> .....	<b>6</b>
<b>11 Precision</b> .....	<b>6</b>
11.1 Interlaboratory test.....	6
11.2 Repeatability.....	6
11.3 Reproducibility.....	7
<b>12 Test report</b> .....	<b>7</b>
<b>Annex A (informative) Examples of chromatograms</b> .....	<b>8</b>
<b>Annex B (informative) Saponification</b> .....	<b>10</b>
<b>Annex C (informative) Results of interlaboratory tests</b> .....	<b>12</b>
<b>Bibliography</b> .....	<b>16</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 34, *Food products*, Subcommittee SC 11, *Animal and vegetable fats and oils*.

This third edition cancels and replaces the second edition (ISO 9936:2006), which has been technically revised. It also incorporates the Amendment ISO 9936:2006/Amd.1:2011 and the Technical Corrigendum ISO 9936:2006/Cor.1:2008. A non-applicability statement for milk and milk products has been added to the Scope.

# Animal and vegetable fats and oils — Determination of tocopherol and tocotrienol contents by high-performance liquid chromatography

## 1 Scope

This International Standard specifies a method for the determination of the contents of free  $\alpha$ -,  $\beta$ -,  $\gamma$ -, and  $\delta$ -tocopherols and tocotrienols (referred to jointly as tocols) in animal and vegetable fats and oils (referred to hereinafter as fats) by high-performance liquid chromatography (HPLC).

For products containing tocopherol or tocotrienol esters, it is necessary to carry out a preliminary saponification.

Milk and milk products (or fat coming from milk and milk products) are excluded from the Scope of this International Standard.

NOTE A suitable method involving a cold saponification procedure is described in [Annex B](#) for information only.

## 2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 661, *Animal and vegetable fats and oils — Preparation of test sample*

## 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

### 3.1

#### **tocol content**

mass fraction of the individual tocols, determined using the method specified in this International Standard

Note 1 to entry: The content is expressed in milligrams per kilogram as a whole number.

## 4 Principle

A test portion is dissolved in *n*-heptane and the individual tocols are separated by high-performance liquid chromatography (HPLC). The content of each tocol is calculated using calibration factors determined from calibration solutions.

## 5 Reagents

Use only reagents of HPLC grade or equivalent.

### 5.1 $\alpha$ -, $\beta$ -, $\gamma$ - and $\delta$ -tocopherol and tocotrienol standards.

If tocopherol standards are not available, a blend of wheat germ and soya bean oil may be used to identify  $\alpha$ -,  $\beta$ -,  $\gamma$ - and  $\delta$ -tocopherols.

If tocotrienol standards are not available, palm oil may be used to identify  $\alpha$ - and  $\gamma$ -tocotrienols. The chromatograms obtained can be used to assist peak identification in test sample chromatograms, in which case the calibration factors for the corresponding tocopherols should be used.

NOTE  $\alpha$ -,  $\beta$ -,  $\gamma$ - and  $\delta$ -tocopherol and tocotrienol standards can be obtained from Merck<sup>1</sup>);  $\alpha$ -tocopherol can be obtained from various suppliers. Tocotrienol standards are available from Sigma Aldrich<sup>2</sup>). It has been reported that the purity of some commercially available tocopherol standards may vary between 85 % and 100 %. Thus, it is important to determine the concentration of prepared calibration solutions by UV spectrometry (see [9.1.1](#)).

**5.2 Tetrahydrofuran**, filtered through an HPLC nylon filter (0,45  $\mu\text{m}$ ).

**5.3 *n*-Heptane**, filtered through an HPLC nylon filter (0,45  $\mu\text{m}$ ).

**5.4 HPLC mobile phase.**

Any suitable mixture of solvents that has been proven to reach a chromatographic resolution of peaks as good as the one presented in [Table 2](#) (relative retention time of tocopherols and tocotrienols) and in [Annex A](#) (chromatograms of a mixture of vegetable oils), should be used (see [Table C.3](#)).

A good separation of  $\gamma$ -tocopherol and  $\beta$ -tocotrienol can be achieved by using a mixture of 5 % volume fraction *t*-butyl methyl ether + 95 % volume fraction *n*-heptane and a diol-column.

The preparation of a suitable mobile phase, 3,85 % (volume fraction) tetrahydrofuran solution in *n*-heptane, is as follows. Using a 1 000 ml graduated cylinder ([6.5](#)), introduce 1 000 ml of *n*-heptane ([5.3](#)) in a 2 litre bottle. Add twice 20 ml of tetrahydrofuran ([5.2](#)) using a 20 ml volumetric pipette ([6.6](#)). Homogenize the mobile phase by means of an ultrasonic bath ([6.8](#)) for 15 min.

**5.5 Methanol.**

## 6 Apparatus

Usual laboratory apparatus and, in particular, the following.

**6.1 HPLC system**, consisting of a high-pressure pump, a sample injection device, column thermostat adjusted to 25 °C (optional), a fluorescence detector with the excitation wavelength set at 295 nm and emission wavelength at 330 nm, and a recording integrator.

An ultraviolet (UV) detector may be used if a fluorescence detector is not available but it is not recommended. However, if a UV detector is used, the wavelength should be set at 292 nm.

**6.2 HPLC analytical column**, two types are possible:

- 250 mm  $\times$  4 mm, packed with microparticulate **diol** having a mean particle size of about 5  $\mu\text{m}$ , or
- 250 mm  $\times$  4,6 mm, packed with microparticulate **silica** having a mean particle size of about 5  $\mu\text{m}$ .

---

1) Merck Tocopherol set 613424 is available from Calbiochem ([www.calbiochem.com](http://www.calbiochem.com)). It contains one 50 mg vial each of DL- $\alpha$ -tocopherol, D- $\beta$ -tocopherol, D- $\gamma$ -tocopherol, and D- $\delta$ -tocopherol with a purity of 95 % by HPLC (for each component). Merck Tocotrienol set 613432 is available from Calbiochem also. It contains one 50 mg vial each of  $\alpha$ -tocotrienol,  $\beta$ -tocotrienol,  $\gamma$ -tocotrienol, and  $\delta$ -tocotrienol with a purity of 95 % by HPLC (75 % for  $\gamma$ -tocotrienol). This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of the products named. Equivalent products may be used if they can be shown to lead to the same results.

2) Tocotrienols are available from Sigma Aldrich ([www.sigmaaldrich.com](http://www.sigmaaldrich.com)) and from Chromadex ([www.chromadex.com](http://www.chromadex.com)) with purities between 65 % and 98 %. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of the products named. Equivalent products may be used if they can be shown to lead to the same results.

NOTE 1 Suitable diol silica column packing material available commercially is 5 µm LiChrospher 100 Diol; suitable silica column packing materials available commercially are 5 µm LiChrosob SI 60 and Kromasil 100<sup>3)</sup>. When β-tocotrienol is expected in the sample, the diol silica column is preferred as γ-tocopherol and β-tocotrienol are co-eluted when using the silica column.

NOTE 2 The length and the diameter of the column can be varied according to the HPLC technique used.

NOTE 3 Both types of columns have been used for the evaluation of the precision data ([Annex C](#)).

**6.3 UV spectrometer**, capable of absolute measurement of absorbance at precisely defined wavelengths, with a 10-mm path length cell.

**6.4 Rotary evaporator.**

**6.5 Graduated cylinder**, of 1 000 ml capacity.

**6.6 Volumetric pipettes**, of 5 ml, 10 ml and 20 ml capacities.

**6.7 Volumetric flasks**, 50 ml and 25 ml capacities.

**6.8 Ultrasonic bath.**

## 7 Sampling

A representative sample should be sent to the laboratory. It is important that the sample has not been damaged or changed during transport or storage.

Sampling is not part of the method specified in this International Standard. A recommended sampling method is given in ISO 5555.

## 8 Preparation of test sample

In the case of liquid laboratory samples, prepare the test sample by homogenization as described in ISO 661, except that filtration should be avoided.

In the case of solid samples, transfer a representative portion (i.e. not less than 10 % by mass of the laboratory sample) to a glass beaker and carefully homogenize by melting, with gentle mixing, in a water bath at a temperature not exceeding 40 °C.

Preparation of the test samples should be carried out, as far as is practicable, in subdued light and in all cases out of direct sunlight.

## 9 Procedure

**IMPORTANT — In general, the oxidation of tocopherols during the analysis may lead to low results. The rate of oxidation is increased in the presence of alkalis, or under the influence of heat or light, and measures should be taken to guard against these influences.**

---

3) These types of columns are examples of suitable products available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of these products.

## 9.1 Preparation of calibration solutions

### 9.1.1 Stock calibration solutions

Prepare a stock solution of each tocol by weighing  $10 \text{ mg} \pm 1 \text{ mg}$  of the standard (5.1) into a 50 ml volumetric flask (6.7) and diluting to the mark with *n*-heptane (5.3).

Pipette 5 ml (6.6) of this solution into an amber glass round-bottomed flask and remove all *n*-heptane on a rotary evaporator (6.4) under vacuum at a temperature not greater than 40 °C. Restore atmospheric pressure with nitrogen and remove the flask from the evaporator as soon as all the solvent has been removed. Pipette into the flask 10 ml (6.6) of methanol (5.5) and swirl to dissolve the residue. Measure the maximum absorbance of this solution in a wavelength range between 270 nm and 310 nm (see appropriate wavelength in Table 1) using the UV spectrometer (6.3) with a 10-mm path length cell. The measured absorbance should be between 0,2 and 0,8. Calculate the concentration (in micrograms per millilitre) by dividing the absorbance value by the appropriate factor given in Table 1.

**Table 1 — Division factors**

Wavelength nm	Tocopherol	Division factor
292	$\alpha$ -tocopherol	0,007 6
296	$\beta$ -tocopherol	0,008 9
298	$\gamma$ -tocopherol	0,009 1
298	$\delta$ -tocopherol	0,008 7

NOTE The factors quoted are derived from the *E* values (1 %/1 cm) of the tocopherols. For example, the *E* value (1 %/1 cm) of  $\alpha$ -tocopherol is 76 at 292 nm (in methanol); therefore a 1  $\mu\text{g/ml}$  solution of  $\alpha$ -tocopherol will have an absorbance of 0,007 6 at 292 nm.

### 9.1.2 Standard solution

A suitable standard solution should be prepared, according to the sensitivity of the fluorescence detector used.

The following preparation of working solution is given as an example: mix appropriate volumes, for example 1 ml, of the stock calibration solutions (see 9.1.1) to obtain a mixed tocol standard solution, and dilute with *n*-heptane to give a solution containing between 1  $\mu\text{g}$  and 5  $\mu\text{g}$  of each standard per millilitre.

The standard solution shall be freshly prepared each working day.

Protect all solutions from light and store them at between 0 °C and 4 °C.

Stock standard solutions can be satisfactorily stored in amber glassware for up to 1 week if refrigerated. Flasks may be wrapped in aluminium foil.

NOTE If a UV detector is used, a more concentrated solution might be needed.

## 9.2 Optimization of working parameters

**9.2.1** If the column (6.2) is new or of unknown history, or if for any other reason it is necessary to condition it, wash and condition it for about 10 min with methanol, then dichloromethane, followed by *n*-heptane at a flow rate of about 1 ml/min.

Pump the HPLC mobile phase (5.4) through the column at a flow rate of 1 ml/min for at least 30 min.

**WARNING — Methanol and dichloromethane are hazardous to humans and to the environment. Handle them with care.**

**9.2.2** Inject 10 µl or 20 µl (according to detector sensitivity) of the standard solution (see [9.1.2](#)) into the column and, if necessary, adjust the tetrahydrofuran content of the mobile phase and the flow rate to achieve the following conditions:

- a) α-tocopherol retention time between 8 min and 12 min;
- b) resolution factor, RF, for the separation of β- and γ-tocopherols of not less than 1,0; i.e. almost baseline separation, where RF is calculated using Formula (1):

$$RF = \frac{d_r(I) - d_r(II)}{0,5 \cdot [b(I) + b(II)]} \quad (1)$$

where

$d_r(I)$  is the retention distance of γ-tocopherol;

$d_r(II)$  is the retention distance of β-tocopherol;

$b(I)$  is the width at the base of the γ-tocopherol peak;

$b(II)$  is the width at the base of the β-tocopherol peak.

**9.2.3** Select the optimum settings for the detection and integration system. Inject 10 µl or 20 µl of the standard solution (see [9.1.2](#)). Repeat the injection and check that reproducible chromatograms are obtained.

### 9.3 Preparation of test solution

Depending on the tocol concentration (see [9.1.2](#)), weigh, to the nearest 1 mg, 0,25 g ± 0,1 g of the test sample (see [Clause 8](#)) into a 25 ml one-mark volumetric flask. Add a quantity of *n*-heptane ([5.3](#)), swirling to dissolve the test portion, and dilute to the mark with the same solvent. Filter the solution with an HPLC nylon filter 0,45 µm if not clear.

It is important that the test solutions be protected from light prior to analysis, and analysed on the day of preparation.

NOTE It may be necessary to prepare a more concentrated solution or to dilute the solution further prior to chromatography.

### 9.4 Determination

**9.4.1** Inject 10 µl or 20 µl (according to detector sensitivity) of the standard solution (see [9.1.2](#)) into the column and record the areas of the peaks.

**9.4.2** Inject 10 µl or 20 µl (according to detector sensitivity) of the test solution (see [9.3](#)) into the column and identify the tocols present by reference to the calibration chromatograms. Record the areas of the peaks. Repeat the injection of the test solution and the measurement. Use the mean values of the two measurements as the result of one determination.

Inject a further 10 µl or 20 µl (according to detector sensitivity) of the standard solution (see [9.1.2](#)) and record the areas of the peaks.

The relative retention times shown in [Table 2](#) have been found to be typical.

**Table 2 — Example of relative retention time of tocopherols and tocotrienols**

Silica column ( $\alpha$ -tocopherol as reference substance)		Diol column ( $\alpha$ -tocopherol as reference substance)	
$\alpha$ -tocopherol = 1,00	$\alpha$ -tocotrienol = 1,19	$\alpha$ -tocopherol = 1,00	$\alpha$ -tocotrienol = 1,24
$\beta$ -tocopherol = 1,34	$\beta$ -tocotrienol = 1,63	$\beta$ -tocopherol = 1,59	$\beta$ -tocotrienol = 2,03
$\gamma$ -tocopherol = 1,63	$\gamma$ -tocotrienol = 2,00	$\gamma$ -tocopherol = 1,74	$\gamma$ -tocotrienol = 2,22
$\delta$ -tocopherol = 2,24	$\delta$ -tocotrienol = 2,79	$\delta$ -tocopherol = 2,46	$\delta$ -tocotrienol = 3,19

## 10 Expression of results

The  $\alpha$ -tocopherol content,  $w$ , of the sample, expressed in milligrams per kilogram (mg/kg), is given by Formula (2):

$$w = \frac{\rho \times \bar{A}_t \times V}{\bar{A}_s \times m} \quad (2)$$

where

$\rho$  is the concentration, in micrograms per millilitre, of  $\alpha$ -tocopherol in the standard solution (9.1.2);

$\bar{A}_s$  is the mean of the peak areas obtained for the  $\alpha$ -tocopherol standard;

$\bar{A}_t$  is the mean of the peak areas obtained for the  $\alpha$ -tocopherol in the test sample;

$m$  is the mass, in grams, of the test sample (9.3);

$V$  is the volume of test solution prepared (= 25 ml).

Calculate the remaining tocol contents of the test sample in the same way using the data obtained from the corresponding standard.

If the only standard available is  $\alpha$ -tocopherol, relate all tocopherols to this standard, but make this clear when reporting the results. If UV detection is used, again relate all tocopherols to the  $\alpha$ -tocopherol standard, but normalize the peak areas to  $\alpha$ -tocopherol using the division factors given in 9.1.1.

NOTE The fluorescence intensity of tocotrienols is the same as of the corresponding tocopherols, and the UV absorbencies are similar.

The content is expressed in milligrams per kilogram as a whole number.

## 11 Precision

### 11.1 Interlaboratory test

Details of an interlaboratory test on the precision of the method are summarized in Annex C. The values derived from this interlaboratory test may not be applicable to concentration ranges and matrices other than those given.

### 11.2 Repeatability

The absolute difference between two independent single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, will in not more than 5 % of cases be greater than the value of  $r$  given in Table 3.

### 11.3 Reproducibility

The absolute difference between two single test results, obtained using the same method on identical test material in different laboratories with different operators using different equipment, will in not more than 5 % of cases be greater than the value of  $R$  given in [Table 3](#).

**Table 3 — Repeatability limit ( $r$ ) and reproducibility limit ( $R$ )**

Tocol content mg/kg	Range of concentration mg/kg	$r$ mg/kg	$R$ mg/kg
$T_1$ = mean value of individual <b>tocopherol</b> content	0 to 2 220	0,082 5 $T_1$	0,209 4 $T_1$
$T_2$ = mean value of individual <b>tocotrienol</b> content	10 to 210	0,090 0 $T_2$	0,255 2 $T_2$
$T_3$ = mean value of <b>total content</b> (tocopherols + tocotrienols)	200 to 3 250	0,071 8 $T_3$	0,255 7 $T_3$


## 12 Test report


The test report shall specify the following:

- a) all information necessary for the complete identification of the sample;
- b) the sampling method used, if known;
- c) the test method used, together with mention of this International Standard, i.e. ISO 9936;
- d) all operating details not specified in this International Standard, or regarded as optional, together with details of any incidents which may have influenced the test result(s);
- e) the test result(s) obtained;
- f) if the repeatability has been checked, the final quoted result obtained.

## Annex A (informative)

### Examples of chromatograms

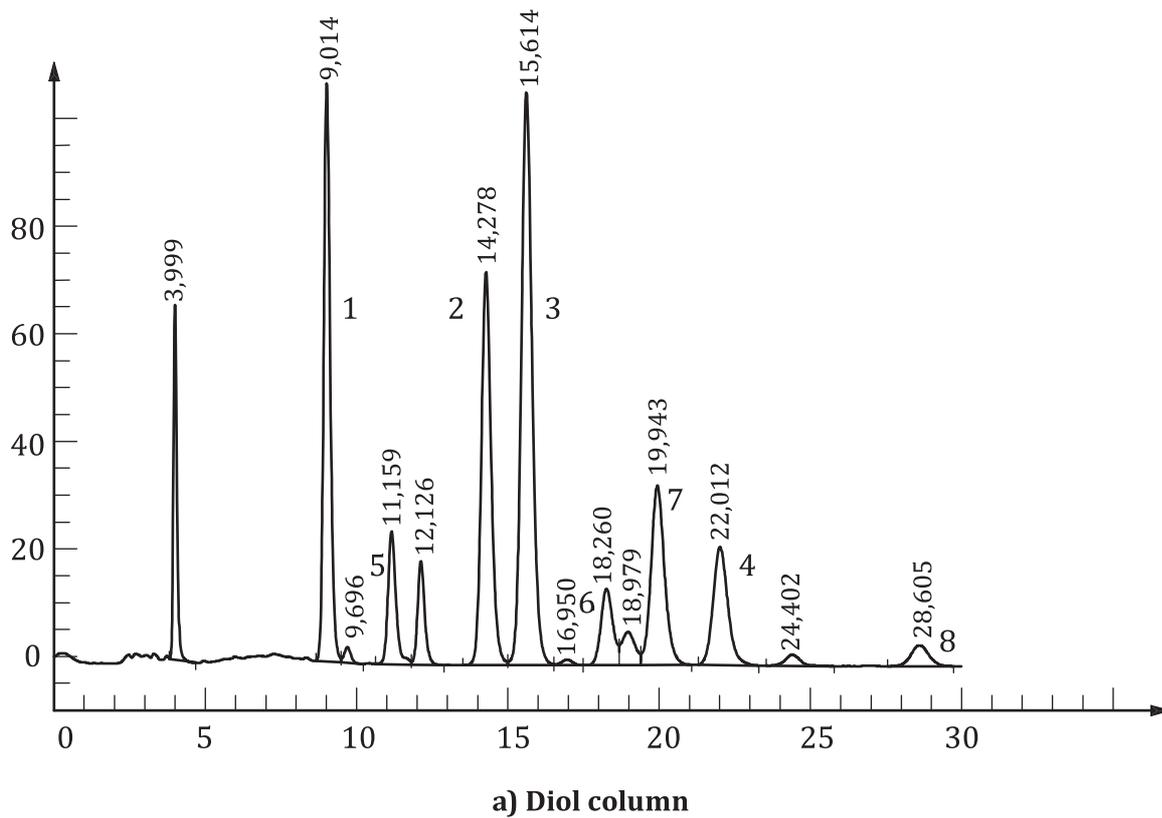

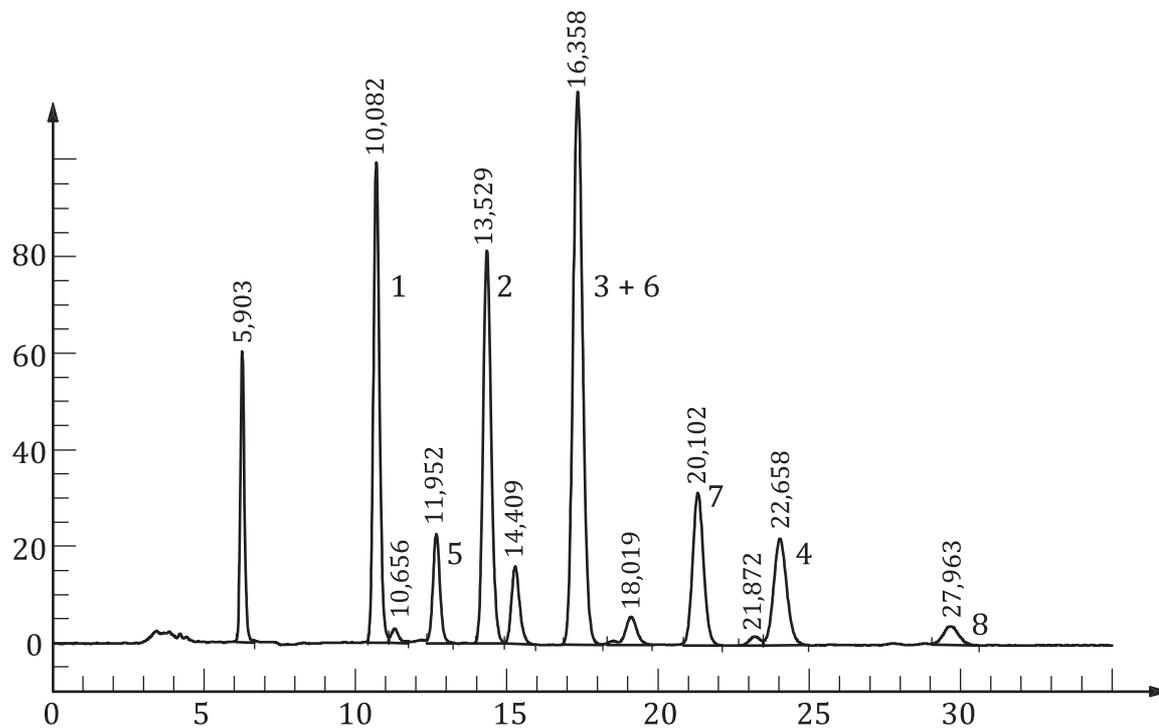

b) Silica column

**Peak identification**

- 1  $\alpha$ -tocopherol
- 2  $\beta$ -tocopherol
- 3  $\gamma$ -tocopherol
- 4  $\delta$ -tocopherol
- 5  $\alpha$ -tocotrienol
- 6  $\beta$ -tocotrienol
- 7  $\gamma$ -tocotrienol
- 8  $\delta$ -tocotrienol

**Conditions**

Mobile phase: 3,85 % (volume fraction) THF in *n*-heptane

Flow rate: 1 ml/min

Detector: fluorescence

NOTE The chromatograms shown above are presented with an x-axis related to time in minutes and y-axis related to abundance.

**Figure A.1 — Mixture of vegetable oils (soybean, grape seeds, wheat germ, palm oil) with added  $\alpha$ -tocopherol acetate**

## Annex B (informative)

### Saponification

#### B.1 General

When analysing processed products containing added tocopherol or tocotrienol esters, a cold saponification procedure should be performed prior to chromatography. It is advisable to analyse samples containing known amounts of esters at the same time.

#### B.2 Reagents

Use only reagents of recognized analytical grade.

**B.2.1 Ethanol**,  $w = 94$  g/100 g to 96 g/100 g.

**B.2.2 Ethanol**, absolute,  $w \geq 99,7$  g/100 g.

**B.2.3 Pyrogallol**.

**B.2.4 Potassium hydroxide**,  $w = 60$  g/100 g aqueous solution.

**B.2.5 Diethyl ether**, peroxide free, containing 0,1 % pyrogallol.

**B.2.6 Hydrochloric acid**,  $c(\text{HCl}) = 0,01$  mol/l.

**B.2.7 Sodium sulfate**, anhydrous.

**B.2.8 Water**, complying with the requirements of grade 3 of ISO 3696.

#### B.3 Procedure

**WARNING — Particular attention must be paid to the saponification temperature and time, otherwise low recoveries from esters may result.**

Weigh accurately about 2 g of the well-mixed sample into a 100 ml flat-bottomed flask and thoroughly disperse the molten test portion in approximately 8 ml of ethanol ([B.2.1](#)) by gentle swirling. Add 100 mg of pyrogallol ([B.2.3](#)) and swirl to dissolve.

Purge the flask with nitrogen, add 4 ml of potassium hydroxide solution ([B.2.4](#)), re-purge the flask with nitrogen, and close with a glass stopper. Place the flask in a water bath set at 26 °C and shake vigorously for 10 min or until saponification is complete. Perform all operations in the absence of direct sunlight, using amber glassware or shielding with aluminium foil.

Add 50 ml of water ([B.2.8](#)) to the flask and transfer quantitatively the contents to a 250 ml separating funnel. Wash the flask with 50 ml of diethyl ether ([B.2.5](#)) and transfer the washings to the funnel. Shake the separating funnel vigorously for 1 min, releasing the pressure occasionally. Allow the layers to separate and draw off the lower aqueous layer. Extract the aqueous layer a further four times with 30 ml aliquots of diethyl ether and combine the ether extracts.

Wash the combined diethyl ether extracts with 50 ml of water (shaking carefully to avoid emulsion formation) and then with 30 ml of dilute hydrochloric acid (B.2.6). Add about 3 g of anhydrous sodium sulfate (B.2.7) with gentle mixing to absorb water. Filter the ether extracts through a phase-separating paper and collect the filtrate in a round-bottomed amber rotary evaporator flask. Remove the ether under reduced pressure at a temperature of not more than 40 °C. If a liquid residue remains in the flask, add ethanol (B.2.2) and evaporate to dryness.

Wash the sides of the flask with *n*-heptane (5.3) and transfer the contents quantitatively to a 50 ml one-mark volumetric flask and dilute to the mark with the *n*-heptane. Make a suitable dilution of the prepared test solution (as described in 9.3) and proceed to 9.4.

## Annex C (informative)

### Results of interlaboratory tests

The precision of the method has been established by an international interlaboratory test organized in 2003 by the Institute for Lipid Research from the Federal Research Centre for Nutrition and Food (Münster, Germany) and carried out in accordance with ISO 5725-1 and ISO 5725-2. In this test, 12 laboratories from four countries (1 Hungary, 1 Canada, 4 France, 6 Germany) participated and samples of eight different types of fat were investigated (see [Table C.1](#)). A statistical summary of the results is given in [Table C.2](#).

The various types of HPLC mobile phases used by the participants in this test are listed in [Table C.3](#). While six participants used a silica gel column, six participants also used a diol column. Therefore, the statistical results, given in [Table C.2](#), are valid for both types of columns.

**Table C.1 — Description of samples**

Sample A	wheat germ oil
Sample B	50 % wheat germ oil + 50 % corn oil
Sample C	25 % wheat germ oil + 75 % corn oil
Sample D	25 % wheat germ oil + 75 % soybean oil
Sample E	10 % wheat germ oil + 90 % palm oil
Sample F	25 % wheat germ oil + 75 % palm oil
Sample G	palm oil
Sample H	virgin olive oil

**Table C.2 — Statistical results**

<b><math>\alpha</math>-Tocopherol</b>	<b>A</b>	<b>B</b>	<b>C</b>	<b>D</b>	<b>E</b>	<b>F</b>	<b>G</b>	<b>H</b>
Number of participating laboratories	12	12	12	12	12	12	12	12
Number of laboratories retained after eliminating outliers	12	12	12	12	12	12	11	11
Number of test results in all laboratories	24,0	24,0	24,0	24,0	24,0	24,0	22,0	22,0
Mean, mg/kg	2 214,5	1 284,8	813,7	662,8	311,5	625,0	106,5	193,1
Repeatability standard deviation ( $s_r$ ), mg/kg	68,3	34,9	24,3	18,4	10,4	25,4	5,0	7,8
Repeatability relative standard deviation, %	3,1	2,7	3,0	2,8	3,3	4,1	4,7	4,0
Repeatability limit ( $r$ ), mg/kg	191,3	97,7	68,1	51,5	29,1	71,1	13,9	21,7
Reproducibility standard deviation ( $s_R$ ), mg/kg	173,1	87,9	56,4	48,5	20,9	38,1	7,1	11,4
Reproducibility relative standard deviation, %	7,8	6,8	6,9	7,3	6,7	6,1	6,6	5,9
Reproducibility limit ( $R$ ), mg/kg	484,7	246,1	157,8	135,9	58,4	106,6	19,7	31,8
<b><math>\beta</math>-Tocopherol</b>	<b>A</b>	<b>B</b>	<b>C</b>	<b>D</b>	<b>E</b>	<b>F</b>	<b>G</b>	<b>H</b>
Number of participating laboratories	12	12	12	12	12	12	7	9
Number of laboratories retained after eliminating outliers	12	12	12	12	12	12	7	9
Number of test results in all laboratories	24,0	24,0	24,0	24,0	24,0	24,0	14,0	18,0
Mean, mg/kg	841,4	417,8	212,5	214,5	79,1	202,6	0,7	2,2
Repeatability standard deviation ( $s_r$ ), mg/kg	22,6	6,8	5,1	6,1	2,8	7,6	0,0	0,3

Table C.2 (continued)

Repeatability relative standard deviation, %	2,7	1,6	2,4	2,8	3,5	3,7	0,0	15,0
Repeatability limit ( $r$ ), mg/kg	63,4	19,0	14,3	17,1	7,8	21,2	0,0	0,9
Reproducibility standard deviation ( $s_R$ ), mg/kg	108,3	55,7	24,7	26,3	10,2	25,9	1,1	0,7
Reproducibility relative standard deviation, %	12,9	13,3	11,6	12,3	12,9	12,8	155,8	29,8
Reproducibility limit ( $R$ ), mg/kg	303,1	156,0	69,1	73,8	28,7	72,4	3,1	1,9
<b><math>\gamma</math>-Tocopherol</b>	<b>A</b>	<b>B</b>	<b>C</b>	<b>D</b>	<b>E</b>	<b>F</b>	<b>G</b>	<b>H</b>
Number of participating laboratories	10	12	12	12		8		12
Number of laboratories retained after eliminating outliers	6	11	7	9		8		12
Number of test results in all laboratories	12,0	22,0	14,0	18,0		16,0		24,0
Mean, mg/kg	19,5	403,8	546,6	325,4		3,6		13,8
Repeatability standard deviation ( $s_r$ ), mg/kg	1,4	7,5	11,7	10,5		0,4		1,1
Repeatability relative standard deviation, %	7,3	1,9	2,1	3,2		9,8		8,1
Repeatability limit ( $r$ ), mg/kg	4,0	21,0	32,7	29,4		1,0		3,1
Reproducibility standard deviation ( $s_R$ ), mg/kg	2,4	62,9	12,3	19,2		2,2		4,2
Reproducibility relative standard deviation, %	12,5	15,6	2,3	5,9		59,7		30,2
Reproducibility limit ( $R$ ), mg/kg	6,8	176,0	34,5	53,8		6,1		11,6
<b><math>\delta</math>-Tocopherol</b>	<b>A</b>	<b>B</b>	<b>C</b>	<b>D</b>	<b>E</b>	<b>F</b>	<b>G</b>	<b>H</b>
Number of participating laboratories		12	12	12				
Number of laboratories retained after eliminating outliers		10	12	12				
Number of test results in all laboratories		20,0	24,0	24,0				
Mean, mg/kg		13,0	20,0	71,0				
Repeatability standard deviation ( $s_r$ ), mg/kg		0,6	1,7	2,5				
Repeatability relative standard deviation, %		4,9	8,5	3,5				
Repeatability limit ( $r$ ), mg/kg		1,8	4,7	6,9				
Reproducibility standard deviation ( $s_R$ ), mg/kg		2,7	3,9	8,3				
Reproducibility relative standard deviation, %		20,8	19,3	11,6				
Reproducibility limit ( $R$ ), mg/kg		7,6	10,8	23,1				
<b><math>\alpha</math>-Tocotrienol</b>	<b>A</b>	<b>B</b>	<b>C</b>	<b>D</b>	<b>E</b>	<b>F</b>	<b>G</b>	<b>H</b>
Number of participating laboratories	9	9	8	7	9	9	9	
Number of laboratories retained after eliminating outliers	7	7	7	7	8	8	8	
Number of test results in all laboratories	14,0	14,0	14,0	14,0	16,0	16,0	16,0	
Mean, mg/kg	42,0	25,1	18,1	10,1	149,7	138,1	162,5	
Repeatability standard deviation ( $s_r$ ), mg/kg	1,1	1,2	0,8	0,9	5,3	7,4	5,0	
Repeatability relative standard deviation, %	2,5	4,9	4,7	8,8	3,6	5,4	3,1	
Repeatability limit ( $r$ ), mg/kg	3,0	3,4	2,4	2,5	14,9	20,8	14,0	
Reproducibility standard deviation ( $s_R$ ), mg/kg	24,7	12,0	6,3	6,7	12,6	26,3	11,0	
Reproducibility relative standard deviation, %	58,7	47,8	34,6	66,2	8,4	19,1	6,7	
Reproducibility limit ( $R$ ), mg/kg	69,0	33,6	17,6	18,7	35,3	73,7	30,7	
<b><math>\beta</math>-Tocotrienol</b>	<b>A</b>	<b>B</b>	<b>C</b>	<b>D</b>	<b>E</b>	<b>F</b>	<b>G</b>	<b>H</b>
Number of participating laboratories	7	7	7	7	9	9	8	
Number of laboratories retained after eliminating outliers	6	7	6	6	8	9	7	
Number of test results in all laboratories	12,0	14,0	12,0	12,0	16,0	18,0	14,0	

Table C.2 (continued)

Mean, mg/kg	113,5	63,7	34,3	28,6	23,9	37,7	15,8	
Repeatability standard deviation ( $s_r$ ), mg/kg	3,0	2,5	0,9	1,0	2,0	2,9	2,1	
Repeatability relative standard deviation, %	2,6	4,0	2,5	3,3	8,2	7,6	13,4	
Repeatability limit ( $r$ ), mg/kg	8,3	7,1	2,4	2,7	5,5	8,1	5,9	
Reproducibility standard deviation ( $s_R$ ), mg/kg	54,8	34,3	26,0	20,4	8,3	14,1	3,7	
Reproducibility relative standard deviation, %	48,3	53,8	75,9	71,4	34,6	37,3	23,7	
Reproducibility limit ( $R$ ), mg/kg	153,6	96,1	72,8	57,1	23,2	39,4	10,5	
<b><math>\gamma</math>-Tocotrienol</b>	<b>A</b>	<b>B</b>	<b>C</b>	<b>D</b>	<b>E</b>	<b>F</b>	<b>G</b>	<b>H</b>
Number of participating laboratories			8		9	9	9	
Number of laboratories retained after eliminating outliers			7		6	6	6	
Number of test results in all laboratories			14,0		12,0	12,0	12,0	
Mean, mg/kg			3,6		185,3	152,1	205,2	
Repeatability standard deviation ( $s_r$ ), mg/kg			0,7		3,4	4,9	6,3	
Repeatability relative standard deviation, %			19,4		1,9	3,2	3,1	
Repeatability limit ( $r$ ), mg/kg			2,0		9,6	13,6	17,6	
Reproducibility standard deviation ( $s_R$ ), mg/kg			1,9		8,1	6,9	8,5	
Reproducibility relative standard deviation, %			53,0		4,4	4,5	4,2	
Reproducibility limit ( $R$ ), mg/kg			5,4		22,8	19,3	23,9	
<b><math>\delta</math>-Tocotrienol</b>	<b>A</b>	<b>B</b>	<b>C</b>	<b>D</b>	<b>E</b>	<b>F</b>	<b>G</b>	<b>H</b>
Number of participating laboratories					10	9	9	
Number of laboratories retained after eliminating outliers					9	8	9	
Number of test results in all laboratories					18,0	16,0	18,0	
Mean, mg/kg					40,8	35,3	47,7	
Repeatability standard deviation ( $s_r$ ), mg/kg					2,1	1,6	1,4	
Repeatability relative standard deviation, %					5,0	4,6	2,9	
Repeatability limit ( $r$ ), mg/kg					5,8	4,6	3,9	
Reproducibility standard deviation ( $s_R$ ), mg/kg					4,4	4,1	6,6	
Reproducibility relative standard deviation, %					10,8	11,7	13,8	
Reproducibility limit ( $R$ ), mg/kg					12,4	11,6	18,4	
<b>Total content</b>	<b>A</b>	<b>B</b>	<b>C</b>	<b>D</b>	<b>E</b>	<b>F</b>	<b>G</b>	<b>H</b>
Number of participating laboratories	12	12	12	12	12	12	12	12
Number of laboratories retained after eliminating outliers	9	9	9	8	8	8	6	11
Number of test results in all laboratories	18,0	18,0	18,0	16,0	16,0	16,0	12,0	22,0
Mean, mg/kg	3 248,8	2 209,4	1 708,7	1 290,4	813,7	1 192,1	522,5	210,6
Repeatability standard deviation ( $s_r$ ), mg/kg	91,1	47,4	33,6	39,8	22,4	32,5	14,8	8,8
Repeatability relative standard deviation, %	2,8	2,1	2,0	3,1	2,7	2,7	2,8	4,2
Repeatability limit ( $r$ ), mg/kg	255,1	132,6	94,0	111,3	62,7	90,9	41,5	24,6
Reproducibility standard deviation ( $s_R$ ), mg/kg	292,3	217,5	161,2	62,3	98,2	85,2	17,1	14,9
Reproducibility relative standard deviation, %	9,0	9,8	9,4	4,8	12,0	7,1	3,3	7,1
Reproducibility limit ( $R$ ), mg/kg	818,4	609,1	451,3	174,4	274,8	238,5	47,8	41,6
NOTE	Mean concentrations, repeatability and reproducibility limits are expressed in mg/kg.							

**Table C.3 — Examples of HPLC mobile phases used during the 2003 interlaboratory test**

<b>Eluent mixtures</b>	<b>Number of participants that used this eluent</b>
3,85 % (volume fraction) tetrahydrofuran in <i>n</i> -heptane	2
tetrahydrofuran/ <i>n</i> -heptane (1:99)	1
tetrahydrofuran/ <i>n</i> -hexane (2:98)	1
<i>t</i> -butyl methyl ether/ <i>n</i> -hexane (4:96)	1
5 % <i>t</i> -butyl methyl ether in <i>n</i> -hexane	1
6 % <i>t</i> -butyl methyl ether in isohexane	1
<i>t</i> -butyl methyl ether/ <i>n</i> -heptane (5:95)	1
<i>t</i> -butyl methyl ether/isooctane (4:96)	1
2,8 % dioxan in <i>n</i> -hexane	1
dioxin/isooctane (3:97)	1
isopropanol/ <i>n</i> -heptane (0,5:99,5)	1

## Bibliography

- [1] ISO 3696, *Water for analytical laboratory use — Specification and test methods*
- [2] ISO 5555, *Animal and vegetable fats and oils — Sampling*
- [3] ISO 5725-1, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions*
- [4] ISO 5725-2, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*



