

First edition  
2009-05-01

---

---

**Methods of testing cement — Report of a  
test programme — Chemical analysis by  
x-ray fluorescence**

*Méthodes d'essai des ciments — Rapport d'un programme d'essais —  
Analyse chimique par fluorescence X*



Reference number  
ISO/TR 12389:2009(E)

© ISO 2009

**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2009

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

Foreword .....	iv
Introduction.....	v
<b>1 Scope .....</b>	<b>1</b>
<b>2 Test methods .....</b>	<b>1</b>
<b>2.1 General arrangements .....</b>	<b>1</b>
<b>2.2 Test method and constituents to be determined .....</b>	<b>2</b>
<b>3 Samples .....</b>	<b>2</b>
<b>3.1 Test samples .....</b>	<b>2</b>
<b>3.2 Calibration standards.....</b>	<b>2</b>
<b>3.3 Validation materials.....</b>	<b>2</b>
<b>3.4 Participating laboratories .....</b>	<b>3</b>
<b>4 Method for analysis of results.....</b>	<b>3</b>
<b>4.1 Statistics.....</b>	<b>3</b>
<b>4.2 Definition of Q-laboratories .....</b>	<b>4</b>
<b>5 Results and considerations.....</b>	<b>5</b>
<b>5.1 Laboratory number.....</b>	<b>5</b>
<b>5.2 Validation results for all laboratories .....</b>	<b>5</b>
<b>5.3 Test results of Q-laboratories .....</b>	<b>12</b>
<b>6 Conclusions .....</b>	<b>26</b>
<b>6.1 Result of test sample analyses .....</b>	<b>26</b>
<b>6.2 Factors affecting conformity with the validation criteria .....</b>	<b>27</b>
<b>6.3 Application to other international inter-laboratory testing .....</b>	<b>27</b>
<b>Annex A (informative) List of participating laboratories.....</b>	<b>28</b>
<b>Annex B (informative) Individual results of all laboratories .....</b>	<b>30</b>
<b>Annex C (informative) Questionnaire results .....</b>	<b>46</b>
<b>Annex D (informative) Other international inter-laboratory round-robin analyses of cement.....</b>	<b>48</b>
<b>Annex E (informative) Acknowledgements .....</b>	<b>51</b>
<b>Bibliography.....</b>	<b>52</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

In exceptional circumstances, when a technical committee has collected data of a different kind from that which is normally published as an International Standard ("state of the art", for example), it may decide by a simple majority vote of its participating members to publish a Technical Report. A Technical Report is entirely informative in nature and does not have to be reviewed until the data it provides are considered to be no longer valid or useful.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO/TR 12389 was prepared by Technical Committee ISO/TC 74, *Cement and lime*.

## Introduction

This Technical Report summarizes the results of inter-laboratory testing of the chemical analysis of cement by x-ray fluorescence undertaken by laboratories in Japan, in Asian countries and in Europe. This testing programme was planned and conducted by the Committee on Cement Chemistry, Japan Cement Association and extended to the members of ISO in Asia and members of CEN/TC 51/WG 15 (Revision of methods of testing cement) in Europe. A total of 42 laboratories participated.

The wet method is a longstanding technique used for chemical analysis of cement. However, since this manner of analysis is extremely time-consuming, more rapid methods have been investigated, leading to the development of chemical analysis of cement by x-ray fluorescence (XRF method). As a result, Japanese Industrial Standard JIS R 5204 was established in July 2002.

JIS R 5204 established a scheme to confirm the validity of calibration equations when the concentrations of a pair of validation beads made from certified reference materials satisfy the criteria for both the repeatability limits and accuracy limits specified in JIS R 5204. Use of this validation system improves the repeatability and accuracy of results obtained by the JIS R 5204 method.

Since an International Standard for this analysis method had not yet been established, the Japanese National Committee for ISO/TC 74 (J/TC 74) proposed the "Development of chemical analysis of cement by x-ray fluorescence" to ISO/TC 74 in June 2004. The English version of JIS R 5204 was included as the first working draft at that time.

In order to introduce JIS R 5204 to Asian members of ISO/TC 74 and to promote technical exchange among them, an inter-laboratory testing programme was organized. This inter-laboratory testing was carried out with the participation of 16 laboratories in Japan and 14 outside Japan, mostly Asian members of ISO/TC 74.

As this first part of the round-robin testing was taking place, work was in progress within CEN committee TC 51/WG 15 to produce a standard method for the chemical analysis of cement by x-ray fluorescence. The Japanese Industrial Standard JIS R 5204 was accepted by this committee and, working jointly with the Japanese co-opted member, was incorporated into the draft for ISO 29581-2. At the invitation of the Japanese Cement Association, members of CEN/TC 51/WG 15 were invited to join in the Japanese/Asian round robin and in 2005 twelve European laboratories participated. The results of their testing are included in this report.

Those laboratories that obtained analyses of JCA-CRM-1 and/or JCA-CRM-2 satisfying the criteria for both the repeatability limits and accuracy limits for all components were defined as "Q-laboratories". A comparison of the results for "Q-laboratories" with those obtained from other inter-laboratory testing for all constituents other than CaO indicates that the variation was equal to or smaller than that of wet analysis. The variation in results for CaO in "Q-laboratories" was slightly larger than that by wet analysis. Therefore, this inter-laboratory testing demonstrates that the accuracy of results obtained by the JIS R 5204/ISO 29581-2 method is generally the same as that for the wet method.



# Methods of testing cement — Report of a test programme — Chemical analysis by x-ray fluorescence

## 1 Scope

This Technical Report describes the results of the inter-laboratory testing of the chemical analysis of cement by x-ray fluorescence. In the first instance, the inter-laboratory testing was carried out in Japan and in Asian countries in accordance with JIS R 5204:2002. A total of 30 laboratories, 16 in Japan and 14 outside Japan, participated in the original testing programme. A further 12 European laboratories participated in tests with the same materials in 2005 in accordance with EN 196-2, a development by CEN/TC 51/WG 15/TG 1 of JIS R 5204. The latest version, developed as ISO 29581-2, is, as of the date of publication of this Technical Report, in the process of being circulated for technical enquiry.

The test samples used were Portland cement conforming to CEM I of EN 197-1 and a mixture of Portland cement and blast furnace slag. The mixture corresponded to the composition of Portland blast furnace slag cement, class B, specified in JIS R 5211 and CEM III/A of EN 197-1. Cement reference materials for x-ray fluorescence analysis (No. 601A) are used for the calibration standards, and certified reference materials JCA-CRM-1 and JCA-CRM-2 are used as the validation materials.

Constituents analysed include  $\text{SiO}_2$ ,  $\text{Al}_2\text{O}_3$ ,  $\text{Fe}_2\text{O}_3$ ,  $\text{CaO}$ ,  $\text{MgO}$ ,  $\text{SO}_3$ ,  $\text{Na}_2\text{O}$ ,  $\text{K}_2\text{O}$ ,  $\text{TiO}_2$ ,  $\text{P}_2\text{O}_5$ ,  $\text{MnO}$  and  $\text{SrO}$ . The loss on ignition is also determined.

The ISO round robin is a method-performance study conducted under close to optimum conditions with clear calibration and measurement guidelines. This is conducive to producing “best practice” values representative of the ideal situation. However, ISO 29581-2 is intended for use under everyday conditions in laboratories that operate to “good practice”. Annex D sets out the results of some international round robins carried out by a large number of laboratories demonstrating the suitability of ISO 29581-2 as a means for comparing the everyday performance of laboratories.

## 2 Test methods

### 2.1 General arrangements

The outline of the inter-laboratory testing is shown in Table 1.

**Table 1 — Outline of the inter-laboratory testing**

Test method	First part – JIS R 5204:2002 Second part – ISO 29581-1
Test samples	JCA #1 Portland cement JCA #2 Cement made by mixing Portland cement with blast furnace slag (composition corresponding to Portland blast furnace slag cement Class B specified in JIS R 5211 and CEM III/A of EN 197-1)
Calibration standards	Cement reference materials for x-ray fluorescence analysis, JCA No. 601A
Validation materials	JCA-CRM-1 Ordinary Portland cement JCA-CRM-2 Portland blast furnace slag cement
Constituents determined	SiO <sub>2</sub> , Al <sub>2</sub> O <sub>3</sub> , Fe <sub>2</sub> O <sub>3</sub> , CaO, MgO, SO <sub>3</sub> , Na <sub>2</sub> O, K <sub>2</sub> O, TiO <sub>2</sub> , P <sub>2</sub> O <sub>5</sub> , MnO, SrO, loss on ignition (LOI)

**2.2 Test method and constituents to be determined**

The first phase of this inter-laboratory testing was based on JIS R 5204. The second phase of this inter-laboratory testing was based on ISO 29581-2. There were no substantial differences between the two methods. For the remainder of this report they will be referred to as “the XRF method”.

Twelve constituents: SiO<sub>2</sub>, Al<sub>2</sub>O<sub>3</sub>, Fe<sub>2</sub>O<sub>3</sub>, CaO, MgO, SO<sub>3</sub>, Na<sub>2</sub>O, K<sub>2</sub>O, TiO<sub>2</sub>, P<sub>2</sub>O<sub>5</sub>, MnO, and SrO, determined by XRF method using glass beads, and loss on ignition were to be evaluated. Although SO<sub>3</sub> for Portland blast furnace slag cement was outside the scope of JIS R 5204, it was an option for Sample #2 in this testing.

**3 Samples**

**3.1 Test samples**

Two test samples were used: Portland cement (Sample #1) conforming to EN 197-1 CEM I, and a cement mixture of Portland cement and blast furnace slag (Sample #2). Sample #2 corresponded to the B-type Portland blast furnace slag cement specified in JIS R 5211 and CEM III/A of EN 197-1. Approximately 30 g of each sample was distributed.

**3.2 Calibration standards**

Cement reference materials for x-ray fluorescence analysis (see NOTE), provided by the Japan Cement Association, were used for the calibration standards.

Approximately 12 g of each standard of JCA No. 601A was distributed to the foreign laboratories. The only requirement was that seven or more calibration standards be used when making calibration equations in accordance with the XRF method.

NOTE JCA No. 601A is a set of 15 cement reference materials consisting of nine Portland cements and six Portland blast furnace slag cements.

**3.3 Validation materials**

Validation of calibration equations was specified in the XRF method. Certified reference materials JCA-CRM-1 and JCA-CRM-2, provided by the Japan Cement Association, were used as the validation materials.

Approximately 30 g of each CRM was distributed to the laboratories.



### 3.4 Participating laboratories

#### 3.4.1 Japan

An announcement of the inter-laboratory testing was sent out to members of the Japan Cement Association. In response to the announcement, 16 laboratories registered as participants in this testing programme. A list of participating laboratories is shown in Annex A.

#### 3.4.2 Asia

An announcement of the inter-laboratory testing was sent out to Asian members registered as P-members or O-members in ISO/TC 74 (See NOTE). Sixteen laboratories responded to the announcement and expressed their desire to participate, and 14 laboratories registered for the programme. A list of participating laboratories is shown in the Annex A.

NOTE The announcement was sent out to member bodies registered in ISO/TC74, and to Cement Associations of the members; see Reference [10].

#### 3.4.3 Europe

Invitations were issued to the members of European Standards Organization Technical Committee TC 51, *Cement and building limes*, Working Group 15, *Methods of testing cement*, Task Group 1, *Analysis by x-ray fluorescence*, to nominate participating laboratories. Twelve laboratories undertook to participate. A list of participating laboratories is shown in Annex A.

## 4 Method for analysis of results

### 4.1 Statistics

Symbols and definitions of statistical terms used in this report are shown in Table 2.

**Table 2 — Definitions of the statistical terms**

Statistical term	Abbreviation/symbol	Definition of the statistical term <sup>a</sup>
Average	Av./ $\bar{x}$	$\bar{x} = \frac{\sum_{i=1}^n x_i}{n}$
Maximum value	Max.	Maximum value in the data
Minimum value	Min.	Minimum value in the data
Range	—	Range is equal to max. minus min.
Standard deviation	S.D./ $\sigma$	$\sigma = \sqrt{\frac{\sum_{i=1}^n (x_i - \bar{x})^2}{n-1}}$
Coefficient of variation	C.V./ $C_V$	$C_V = \frac{\sigma \times 100}{\bar{x}}$ , expressed as a percentage
<sup>a</sup> $n$ is the number of laboratories; $x$ is the mean value of a pair of results from each laboratory.		

**4.2 Definition of Q-laboratories**

**4.2.1 General**

In this inter-laboratory testing, a Q-laboratory is one where the concentration of a pair of validation beads made from certified reference materials satisfies the criteria for both the repeatability limits and accuracy limits set out in the XRF method.

**4.2.2 Validation procedure**

**4.2.2.1** Determination of the concentration of a pair of validation beads made from at least one certified reference material for all analysis constituents.

**4.2.2.2** Check that the difference in the concentration, rounded off to three decimal places, of a pair of validation beads is within the repeatability limits obtained from Equation (1):

$$\log(y) = 0,48 \log(x) - 1,499 \tag{1}$$

where

*y* is the repeatability limit, as a percentage;

*x* is the mean value of the concentration of a pair of validation beads, as a percentage.

When *x* is less than 0,5 %, a limit for *y* of 0,020 % is applied to all values.

NOTE Equation (1) is specified in JIS R 5204.

**4.2.2.3** Check that the difference between the mean values, rounded off to two decimal places, of the concentration of a pair of validation beads and the “certified values” of the certified reference materials are within the accuracy limits specified according to the level of concentration in Table 3 for each analysed constituent.

Both JCA-CRM-1 and JCA-CRM-2 are used for the validation materials in this inter-laboratory testing. However, in the XRF method, the use of just one certified reference material is permitted. Therefore, for the purpose of this inter-laboratory test, the validations are considered as satisfied if the analysis of either JCA-CRM-1 or JCA-CRM-2 meets the validation criteria. Laboratories that obtained concentrations of JCA-CRM-1 and/or JCA-CRM-2 satisfying the criteria for both the repeatability limits and accuracy limits for all constituents, were defined as “Q-laboratories” in this inter-laboratory testing. In ISO 29581-2, these are referred to as “expert” laboratories.

**Table 3 — Accuracy limits for analysis validation**

Level of the certified value (% absolute)	Accuracy limits for analysis validation (% absolute)
0,00 to 0,49	0,02
0,50 to 0,99	0,03
1,00 to 6,99	0,08
7,00 to 14,99	0,12
15,00 to 29,99	0,15
30,00 to 49,99	0,20
50,00 to 79,99	0,25
80,00 to 100,00	0,30

## 5 Results and considerations

### 5.1 Laboratory number

Validation results for all laboratories and results of determination for Q-laboratories are shown in Tables B.1 to B.8. Laboratories No. 1 to No. 16 represent laboratories in Japan; Laboratories No. 101 to No. 113 represent ISO member laboratories outside Japan. Although there were 14 participating laboratories outside Japan, the report submitted by Laboratory No. 114 is mentioned only in Tables B.2, B.4, B.6 and B.8, because the laboratory carried out XRF analysis by the pellet method. Laboratories No. E1 to E12 represent laboratories participating in the European stage.

### 5.2 Validation results for all laboratories

The difference in concentration for each pair of JCA-CRM-1 is shown in Table 4, and that for JCA-CRM-2 is shown in Table 5. The difference between the mean values of concentration for each pair of JCA-CRM-1 and the certified values is shown in Table 6, and that for JCA-CRM-2 is shown in Table 7.

Data in the shaded cells of Table 4 and Table 5 denote results that did not satisfy the required criteria for repeatability. Data in the shaded cells of Table 6 and Table 7 represent results that did not satisfy the required criteria for accuracy limits. “-” in each table indicates that there is no report from the laboratory for that constituent.

The presence of data in the shaded cells indicates that some validation results did not satisfy the required criteria for repeatability or accuracy limits. Therefore, in determining the Q-laboratories according to the definition described in 4.2, 27 laboratories were judged as Q-laboratories.

**Table 4 — Difference in concentrations for each pair of validation beads**  
(All laboratories — Validation material: JCA-CRM-1)

Laboratory ref.	SiO <sub>2</sub> %	Al <sub>2</sub> O <sub>3</sub> %	Fe <sub>2</sub> O <sub>3</sub> %	CaO %	MgO %	SO <sub>3</sub> %	Na <sub>2</sub> O %	K <sub>2</sub> O %	TiO <sub>2</sub> %	P <sub>2</sub> O <sub>5</sub> %	MnO %	SrO %
1	0,039	0,028	0,009	0,180	0,006	0,010	0,015	0,007	0,000	0,001	0,000	-
2	0,034	0,004	0,001	0,072	0,005	0,032	0,001	0,003	0,007	0,001	0,001	0,000
3	0,012	0,005	0,017	0,018	0,012	0,028	0,013	0,002	0,003	0,001	0,000	-
4	0,080	0,010	0,013	0,020	0,001	0,009	0,002	0,004	0,004	0,002	0,000	0,000
5	0,032	0,012	0,003	0,004	0,003	0,009	0,001	0,003	0,002	0,001	0,000	0,000
6	0,024	0,027	0,002	0,083	0,039	0,012	0,011	0,007	0,008	0,002	0,002	0,000
7	0,014	0,013	0,003	0,046	0,005	0,006	0,002	0,002	0,005	0,000	0,001	0,000
8	0,040	0,006	0,004	0,115	0,010	0,008	0,007	0,001	0,008	0,001	0,000	0,000
9	0,011	0,017	0,004	0,041	0,003	0,006	0,001	0,001	0,002	0,001	0,000	0,000
10	0,028	0,035	0,003	0,012	0,017	0,017	0,007	0,001	0,003	0,000	0,000	-
11	0,012	0,006	0,008	0,061	0,014	0,018	0,012	0,010	0,004	0,005	0,001	-
12	0,011	0,006	0,006	0,073	0,005	0,024	0,007	0,002	0,011	0,000	0,003	0,001
13	0,018	0,004	0,003	0,042	0,009	0,005	0,002	0,000	0,004	0,000	0,001	0,000
14	0,080	0,029	0,006	0,112	0,006	0,001	0,002	0,018	0,013	0,010	0,001	0,000
15	0,090	0,008	0,004	0,038	0,003	0,015	0,002	0,001	0,006	0,000	0,001	0,001
16	0,007	0,011	0,004	0,014	0,003	0,008	0,008	0,001	0,005	0,002	0,000	0,000
101	0,005	0,005	0,007	0,006	0,012	0,130	0,006	0,004	0,003	0,003	-	-
102	0,017	0,058	0,004	0,005	0,007	0,001	-	0,000	-	-	-	-
103	0,020	0,020	0,010	0,060	0,170	0,020	0,010	0,010	-	-	-	-
104	0,016	0,020	0,009	0,193	0,011	0,035	0,010	0,016	0,002	0,004	0,001	0,000
105	0,084	0,052	0,008	0,024	0,001	0,006	0,003	0,001	0,011	0,003	0,000	0,001
106	0,118	0,014	0,002	0,090	0,002	0,014	0,017	0,003	-	-	-	-
107	0,006	0,211	0,008	0,045	0,033	0,032	0,005	0,006	-	0,011	0,001	-
108	0,010	0,010	0,010	0,020	0,010	0,010	0,030	0,000	-	0,000	-	-
109	0,032	0,009	0,014	0,116	0,003	0,015	-	0,002	-	-	-	-
110	0,122	0,099	0,059	0,041	0,261	0,136	0,082	0,161	-	0,022	-	-
111	0,040	0,030	0,010	0,010	0,020	0,000	0,010	0,000	0,010	0,010	0,000	0,000
112	0,110	0,010	0,000	0,020	0,090	0,010	0,000	0,000	-	-	-	-
113	0,030	0,030	0,010	0,150	0,090	0,030	0,010	0,000	0,000	0,010	0,000	0,000
E1	0,112	0,045	0,013	0,039	0,007	0,025	0,009	0,002	0,006	0,000	0,000	0,000
E2	0,001	0,053	0,008	0,016	0,019	0,021	0,002	0,005	0,002	0,003	0,000	-
E3	0,020	0,050	0,040	0,030	0,000	0,060	0,000	0,000	0,000	0,010	0,000	0,000
E4	0,034	0,012	0,009	0,038	0,008	0,003	0,005	0,002	0,000	0,003	0,001	0,000
E5	0,020	0,010	0,020	0,050	0,010	0,010	0,010	0,010	0,010	0,030	0,000	0,000
E6	0,036	0,039	0,003	0,093	0,003	0,042	0,004	0,004	0,001	0,010	0,001	-
E7	0,208	0,051	0,003	0,204	0,051	0,006	0,008	0,006	0,010	0,005	0,001	0,001
E8	0,085	0,036	0,002	0,014	0,004	0,007	0,011	0,001	0,004	0,000	0,001	0,000
E9	0,038	0,039	0,008	0,169	0,028	-	0,009	0,001	0,011	-	-	-
E10	0,010	0,010	0,020	0,050	0,020	0,000	0,000	0,000	-	-	-	-
E11	0,003	0,005	0,007	0,010	0,021	0,002	0,000	0,002	0,001	0,000	0,001	0,000
E12	0,240	0,014	0,022	0,700	0,001	0,017	0,020	0,011	0,007	0,007	0,001	0,000
<b>Average</b>	0,048	0,028	0,010	0,076	0,025	0,021	0,009	0,008	0,005	0,005	0,001	0,000
<b>Max.</b>	0,240	0,211	0,059	0,700	0,261	0,136	0,082	0,161	0,013	0,030	0,003	0,001
<b>Min.</b>	0,001	0,004	0,000	0,004	0,000	0,000	0,000	0,000	0,000	0,000	0,000	0,000
<b>Range</b>	0,239	0,207	0,059	0,696	0,261	0,136	0,082	0,161	0,013	0,030	0,003	0,001
<b>Certified analysis</b>	20,99	5,260	2,670	65,210	2,130	2,050	0,260	0,560	0,350	0,280	0,060	0,050
<b>Limit value</b>	0,150	0,080	0,080	0,250	0,080	0,080	0,020	0,030	0,020	0,020	0,020	0,020

NOTE Data in shaded cells represent results that did not satisfy the required criteria for repeatability specified for "expert" laboratories for the XRF method.

**Table 5 — Difference in concentrations for each pair of validation beads**  
(All laboratories — Validation material: JCA-CRM-2)

Laboratory ref.	SiO <sub>2</sub> %	Al <sub>2</sub> O <sub>3</sub> %	Fe <sub>2</sub> O <sub>3</sub> %	CaO %	MgO %	SO <sub>3</sub> <sup>a</sup> %	Na <sub>2</sub> O %	K <sub>2</sub> O %	TiO <sub>2</sub> %	P <sub>2</sub> O <sub>5</sub> %	MnO %	SrO %
1	0,001	0,001	0,003	0,002	0,002	0,00	0,005	0,006	0,001	0,000	0,000	-
2	0,051	0,010	0,001	0,020	0,018	0,03	0,003	0,002	0,014	0,002	0,000	0,000
3	0,032	0,010	0,013	0,013	0,009	-	0,009	0,001	0,000	0,000	0,001	-
4	0,008	0,016	0,006	0,047	0,010	0,02	0,003	0,003	0,000	0,001	0,003	0,000
5	0,038	0,019	0,001	0,012	0,009	0,02	0,001	0,001	0,002	0,000	0,000	0,000
6	0,113	0,044	0,018	0,105	0,025	0,03	0,012	0,007	0,007	0,002	0,000	0,000
7	0,009	0,003	0,001	0,038	0,026	0,00	0,000	0,001	0,002	0,001	0,000	0,000
8	0,005	0,016	0,003	0,040	0,003	0,00	0,000	0,000	0,007	0,001	0,001	0,000
9	0,094	0,016	0,001	0,101	0,012	-	0,002	0,002	0,004	0,000	0,001	0,000
10	0,035	0,091	0,015	0,183	0,040	-	0,011	0,002	0,003	0,000	0,001	-
11	0,020	0,030	0,002	0,100	0,047	0,00	0,016	0,000	0,014	0,001	0,001	-
12	0,006	0,052	0,020	0,022	0,004	-	0,014	0,004	0,006	0,000	0,001	0,001
13	0,010	0,008	0,003	0,058	0,008	0,01	0,002	0,000	0,005	0,000	0,000	0,000
14	0,071	0,052	0,006	0,156	0,009	0,01	0,008	0,004	0,014	0,015	0,003	0,001
15	0,052	0,006	0,005	0,021	0,001	0,01	0,006	0,002	0,003	0,001	0,000	0,000
16	0,054	0,046	0,006	0,019	0,011	0,03	0,005	0,002	0,003	0,000	0,001	0,001
101	0,005	0,039	0,011	0,060	0,013	-	0,017	0,001	0,001	0,000	-	-
102	0,022	0,011	0,004	0,029	0,008	0,00	-	0,001	-	-	-	-
103	0,020	0,070	0,010	0,000	0,140	0,03	0,010	0,000	-	-	-	-
104	0,034	0,039	0,010	0,188	0,009	0,02	0,007	0,017	0,003	0,001	0,003	0,000
105	0,043	0,019	0,002	0,010	0,020	0,00	0,004	0,004	0,010	0,005	0,006	0,000
106	0,057	0,045	0,043	0,107	0,015	-	0,002	0,001	-	-	-	-
107	0,121	0,014	0,048	0,012	0,015	-	0,009	0,005	-	0,002	0,003	-
108	0,250	0,060	0,000	0,250	0,020	0,03	0,070	0,000	-	0,010	-	-
109	0,054	0,023	0,013	0,057	0,002	0,02	-	0,010	-	-	-	-
110	0,022	0,119	0,018	0,138	0,037	0,02	0,021	0,019	-	0,008	-	-
111	0,060	0,050	0,010	0,070	0,030	0,02	0,000	0,000	0,010	0,020	0,000	0,000
112	-	-	-	-	-	-	-	-	-	-	-	-
113	0,050	0,050	0,020	0,050	0,030	-	0,010	0,010	0,010	0,000	0,000	0,000
E1	0,045	0,063	0,025	0,121	0,002	0,179	0,008	0,005	0,007	0,007	0,001	0,001
E2	0,003	0,003	0,008	0,017	0,002	0,025	0,005	0,005	0,001	0,006	0,002	-
E3	0,010	0,010	0,010	0,030	0,030	0,020	0,000	0,000	0,000	0,010	0,000	0,000
E4	0,062	0,054	0,001	0,111	0,026	0,047	0,013	0,001	0,001	0,002	0,004	0,002
E5	0,040	0,030	0,010	0,120	0,100	0,030	0,015	0,000	0,003	0,010	0,001	0,002
E6	0,002	0,019	0,008	0,041	0,033	-	0,000	0,003	0,000	0,007	0,002	-
E7	0,118	0,052	0,001	0,179	0,008	0,013	0,003	0,002	0,003	0,005	0,001	0,001
E8	0,049	0,003	0,014	0,070	0,038	0,005	0,008	0,002	0,000	0,004	0,000	0,000
E9	0,063	0,025	0,006	0,082	0,008	-	-	0,001	0,016	-	-	-
E10	0,010	0,010	0,010	0,040	0,000	0,000	0,000	0,000	-	-	-	-
E11	0,086	0,030	0,006	0,052	0,009	0,003	0,008	0,001	0,000	0,001	0,000	0,001
E12	0,260	0,193	0,023	0,430	0,005	-	0,016	0,003	0,003	0,009	0,000	-
<b>Average</b>	0,052	0,036	0,010	0,080	0,021	0,022	0,009	0,003	0,005	0,004	0,001	0,000
<b>Max.</b>	0,260	0,193	0,048	0,430	0,140	0,179	0,070	0,019	0,016	0,020	0,006	0,002
<b>Min.</b>	0,001	0,001	0,000	0,000	0,000	0,000	0,000	0,000	0,000	0,000	0,000	0,000
<b>Range</b>	0,259	0,192	0,048	0,430	0,140	0,179	0,070	0,019	0,016	0,020	0,006	0,002
<b>Certified analysis Limit value</b>	25,66	8,940	2,080	56,330	3,050	-	0,240	0,310	0,500	0,070	0,150	0,070
<b>Limit value</b>	0,150	0,120	0,080	0,250	0,080	-	0,020	0,020	0,030	0,020	0,020	0,020

NOTE Data in shaded cells represent results that did not satisfy the required criteria for repeatability specified for "expert" laboratories for the XRF method.

<sup>a</sup> SO<sub>3</sub> for JCA-CRM-2 is outside the scope of JIS R 5204.

**Table 6 — Differences between the mean value of the concentrations of a pair of validation beads and the certified value**  
(All laboratories — Validation material: JCA-CRM-1)

Laboratory ref.	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> %	
	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>
1	20,96	-0,03	5,27	0,01	2,61	-0,06	65,29	0,08	2,11	-0,02	2,08	0,03
2	20,92	-0,07	5,26	0,00	2,65	-0,02	65,33	0,12	2,13	0,00	2,02	-0,03
3	20,94	-0,05	5,25	-0,01	2,68	0,01	65,11	-0,10	2,14	0,01	2,08	0,03
4	20,97	-0,02	5,26	0,00	2,68	0,01	65,20	-0,01	2,14	0,01	2,08	0,03
5	20,93	-0,06	5,26	0,00	2,67	0,00	65,24	0,03	2,13	0,00	2,09	0,04
6	20,93	-0,06	5,24	-0,02	2,61	-0,06	65,17	-0,04	2,12	-0,01	2,07	0,02
7	21,00	0,01	5,27	0,01	2,66	-0,01	65,20	-0,01	2,17	0,04	2,06	0,01
8	20,92	-0,07	5,27	0,01	2,68	0,01	65,05	-0,16	2,16	0,03	2,06	0,01
9	20,91	-0,08	5,26	0,00	2,61	-0,06	65,21	0,00	2,12	-0,01	2,07	0,02
10	20,96	-0,03	5,24	-0,02	2,63	-0,04	65,32	0,11	2,11	-0,02	2,08	0,03
11	21,02	0,03	5,28	0,02	2,67	0,00	65,21	0,00	2,12	-0,01	2,07	0,02
12	20,98	-0,01	5,27	0,01	2,68	0,01	65,27	0,06	2,14	0,01	2,09	0,04
13	21,03	0,04	5,27	0,01	2,68	0,01	64,98	-0,23	2,14	0,01	2,05	0,00
14	21,00	0,01	5,28	0,02	2,72	0,05	65,40	0,19	2,15	0,02	2,07	0,02
15	21,04	0,05	5,26	0,00	2,67	0,00	65,21	0,00	2,11	-0,02	1,98	-0,07
16	21,01	0,02	5,29	0,03	2,67	0,00	65,18	-0,03	2,15	0,02	2,09	0,04
101	21,05	0,06	5,29	0,03	2,62	-0,05	65,34	0,13	2,12	-0,01	2,03	-0,02
102	21,17	0,18	5,21	-0,05	2,64	-0,03	66,29	1,08	2,13	0,00	2,43	0,38
103	20,98	-0,01	5,21	-0,05	2,64	-0,03	65,25	0,04	2,14	0,01	2,08	0,03
104	20,98	-0,01	5,24	-0,02	2,63	-0,04	64,96	-0,25	2,10	-0,03	2,08	0,03
105	21,02	0,03	5,27	0,01	2,64	-0,03	65,38	0,17	2,18	0,05	2,06	0,01
106	20,95	-0,04	5,26	0,00	2,67	0,00	65,13	-0,08	2,12	-0,01	2,06	0,01
107	21,06	0,07	5,42	0,16	2,69	0,02	64,47	-0,74	2,15	0,02	2,04	-0,01
108	20,90	-0,09	5,26	0,00	2,62	-0,05	65,17	-0,04	2,10	-0,03	2,06	0,01
109	20,98	-0,01	5,26	0,00	2,63	-0,04	65,50	0,29	2,11	-0,02	1,95	-0,10
110	20,91	-0,08	5,25	-0,01	2,61	-0,06	65,13	-0,08	2,17	0,04	1,99	-0,06
111	20,92	-0,07	4,98	-0,28	2,62	-0,05	64,68	-0,53	2,38	0,25	2,00	-0,05
112	21,00	0,01	5,86	0,60	2,58	-0,09	64,77	-0,44	2,06	-0,07	1,80	-0,25
113	22,98	1,99	5,24	-0,02	2,64	-0,03	65,28	0,07	2,02	-0,11	2,06	0,01
E1	20,91	-0,08	5,26	0,00	2,66	-0,01	65,16	-0,05	2,14	0,01	2,20	0,15
E2	20,80	-0,19	5,30	0,04	2,61	-0,06	65,00	-0,21	2,11	-0,02	2,07	0,02
E3	20,79	-0,20	5,17	-0,09	2,71	0,04	65,17	-0,04	2,27	0,14	1,98	-0,07
E4	20,93	-0,06	5,28	0,02	2,65	-0,02	65,01	-0,20	2,17	0,04	2,04	-0,01
E5	21,01	0,02	5,25	-0,01	2,65	-0,02	65,33	0,12	2,14	0,01	2,07	0,02
E6	20,95	-0,04	5,23	-0,03	2,68	0,01	65,16	-0,05	2,15	0,02	2,13	0,08
E7	21,00	0,01	5,27	0,01	2,69	0,02	65,34	0,13	2,15	0,02	2,07	0,02
E8	20,89	-0,10	5,27	0,01	2,58	-0,09	65,13	-0,08	2,14	0,01	2,07	0,02
E9	20,99	0,00	5,22	-0,04	2,68	0,01	65,21	0,00	2,15	0,02	-	-
E10	21,09	0,10	5,16	-0,10	2,61	-0,06	65,14	-0,07	2,11	-0,02	2,01	-0,04
E11	20,75	-0,24	5,27	0,01	2,67	0,00	65,52	0,31	2,17	0,04	1,99	-0,06
E12	20,88	-0,11	5,29	0,03	2,67	0,00	64,91	-0,30	2,15	0,02	2,05	0,00
<b>Average</b>	21,01		5,27		2,65		65,19		2,14		2,06	
<b>Max.</b>	22,98		5,86		2,72		66,29		2,38		2,43	
<b>Min.</b>	20,75		4,98		2,58		64,47		2,02		1,80	
<b>Range</b>	2,23		0,88		0,14		1,82		0,36		0,63	
<b>S.D.</b>	0,325		0,111		0,033		0,268		0,053		0,085	
<b>C.V.</b>	1,5		2,1		1,3		0,4		2,5		4,1	
<b>Certified value</b>	20,99		5,26		2,67		65,21		2,13		2,05	

Table 6 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %	
	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>
1	0,26	0,00	0,54	-0,02	0,34	-0,01	0,29	0,01	0,07	0,01	-	-
2	0,26	0,00	0,53	-0,03	0,35	0,00	0,28	0,00	0,07	0,01	0,04	-0,01
3	0,26	0,00	0,57	0,01	0,36	0,01	0,28	0,00	0,06	0,00	-	-
4	0,26	0,00	0,56	0,00	0,36	0,01	0,29	0,01	0,06	0,00	0,04	-0,01
5	0,26	0,00	0,56	0,00	0,36	0,01	0,28	0,00	0,06	0,00	0,04	-0,01
6	0,27	0,01	0,58	0,02	0,34	-0,01	0,29	0,01	0,06	0,00	0,04	-0,01
7	0,25	-0,01	0,56	0,00	0,36	0,01	0,28	0,00	0,06	0,00	0,04	-0,01
8	0,25	-0,01	0,56	0,00	0,35	0,00	0,28	0,00	0,06	0,00	0,04	-0,01
9	0,26	0,00	0,57	0,01	0,35	0,00	0,29	0,01	0,07	0,01	0,04	-0,01
10	0,24	-0,02	0,57	0,01	0,35	0,00	0,28	0,00	0,07	0,01	-	-
11	0,25	-0,01	0,53	-0,03	0,36	0,01	0,29	0,01	0,06	0,00	-	-
12	0,27	0,01	0,57	0,01	0,35	0,00	0,28	0,00	0,06	0,00	0,04	-0,01
13	0,26	0,00	0,56	0,00	0,36	0,01	0,29	0,01	0,06	0,00	0,04	-0,01
14	0,27	0,01	0,58	0,02	0,33	-0,02	0,30	0,02	0,06	0,00	0,04	-0,01
15	0,27	0,01	0,56	0,00	0,35	0,00	0,29	0,01	0,06	0,00	0,04	-0,01
16	0,26	0,00	0,58	0,02	0,35	0,00	0,28	0,00	0,06	0,00	0,04	-0,01
101	0,23	-0,03	0,57	0,01	0,35	0,00	0,29	0,01	-	-	-	-
102	-	-	0,60	0,04	-	-	-	-	-	-	-	-
103	0,28	0,02	0,58	0,02	-	-	-	-	-	-	-	-
104	0,24	-0,02	0,56	0,00	0,34	-0,01	0,27	-0,01	0,07	0,01	0,04	-0,01
105	0,25	-0,01	0,60	0,04	0,35	0,00	0,29	0,01	0,07	0,01	0,04	-0,01
106	0,27	0,01	0,57	0,01	-	-	-	-	-	-	-	-
107	0,25	-0,01	0,56	0,00	-	-	0,28	0,00	0,06	0,00	-	-
108	0,26	0,00	0,59	0,03	-	-	0,28	0,00	-	-	-	-
109	-	-	0,57	0,01	-	-	-	-	-	-	-	-
110	0,28	0,02	0,58	0,02	-	-	0,29	0,01	-	-	-	-
111	0,28	0,02	0,57	0,01	0,38	0,03	0,36	0,08	0,07	0,01	0,04	-0,01
112	0,19	-0,07	0,58	0,02	-	-	-	-	-	-	-	-
113	0,26	0,00	0,58	0,02	0,35	0,00	0,28	0,00	0,07	0,01	0,04	-0,01
E1	0,26	0,00	0,56	0,00	0,35	0,00	0,29	0,01	0,06	0,00	0,04	-0,01
E2	0,27	0,01	0,57	0,01	0,34	-0,01	0,29	0,01	0,07	0,01	-	-
E3	0,26	0,00	0,55	-0,01	0,35	0,00	0,30	0,02	0,07	0,01	0,05	0,00
E4	0,27	0,01	0,57	0,01	0,34	-0,01	0,29	0,01	0,07	0,01	0,04	-0,01
E5	0,27	0,01	0,58	0,02	0,35	0,00	0,28	0,00	0,07	0,01	0,04	-0,01
E6	0,13	-0,13	0,56	0,00	0,35	0,00	0,31	0,03	0,06	0,00	-	-
E7	0,27	0,01	0,56	0,00	0,36	0,01	0,28	0,00	0,06	0,00	0,05	0,00
E8	0,27	0,01	0,57	0,01	0,34	-0,01	0,28	0,00	0,07	0,01	0,04	-0,01
E9	0,26	0,00	0,56	0,00	0,34	-0,01	-	-	-	-	-	-
E10	0,29	0,03	0,57	0,01	-	-	-	-	-	-	-	-
E11	0,25	-0,01	0,57	0,01	0,34	-0,01	0,28	0,00	0,06	0,00	0,05	0,00
E12	0,25	-0,01	0,57	0,01	0,35	0,00	0,29	0,01	0,07	0,01	-	-
<b>Average</b>	0,26		0,57		0,35		0,29		0,06		0,04	
<b>Max.</b>	0,29		0,60		0,38		0,36		0,07		0,05	
<b>Min.</b>	0,13		0,53		0,33		0,27		0,06		0,04	
<b>Range</b>	0,16		0,07		0,05		0,09		0,01		0,01	
<b>S.D.</b>	0,027		0,015		0,010		0,015		0,005		0,003	
<b>C.V.</b>	10,2		2,6		2,7		5,3		8,4		6,9	
<b>Certified value</b>	0,26		0,56		0,35		0,28		0,06		0,05	

NOTE Data in shaded cells represent concentrations that did not satisfy the required criteria for accuracy limits for "expert" laboratories specified for the XRF method.

<sup>a</sup> "Mean value" is the mean value of the concentrations of a pair of validated beads.

<sup>b</sup> "Diff." is the difference between the mean value of the concentrations of a pair of validated beads and the certified value for the validation material.

**Table 7 — Differences between the mean value of the concentrations of a pair of validation beads and the certified value**  
(All laboratories — Validation material: JCA-CRM-2)

Laboratory ref.	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> <sup>a</sup> %	
	Mean value <sup>b</sup>	Diff. c	Mean Value <sup>b</sup>	Diff. c	Mean value <sup>b</sup>	Diff. c	Mean value <sup>b</sup>	Diff. c	Mean value <sup>b</sup>	Diff. c	Mean value <sup>b</sup>	Diff. c
1	25,65	-0,01	8,94	0,00	2,14	0,06	56,49	0,16	3,05	0,00	2,56	-
2	25,55	-0,11	8,92	-0,02	2,09	0,01	56,47	0,14	3,03	0,02	2,57	-
3	25,52	-0,14	8,94	0,00	2,10	0,02	56,53	0,20	2,97	-0,08	-	-
4	25,64	-0,02	8,93	-0,01	2,10	0,02	56,38	0,05	3,04	-0,01	2,58	-
5	25,61	-0,05	8,93	-0,01	2,08	0,00	56,43	0,10	3,03	-0,02	2,57	-
6	25,59	-0,07	9,00	0,06	2,14	0,06	56,56	0,23	3,06	0,01	2,53	-
7	25,69	0,03	8,95	0,01	2,07	-0,01	56,48	0,15	3,08	0,03	2,60	-
8	25,57	-0,09	8,90	-0,04	2,04	-0,04	56,15	-0,18	3,06	0,01	2,37	-
9	25,58	-0,08	8,93	-0,01	2,14	0,06	56,49	0,16	3,06	0,01	-	-
10	25,59	-0,07	8,90	-0,04	2,13	0,05	56,53	0,20	2,98	-0,07	-	-
11	25,69	0,03	8,88	-0,06	2,08	0,00	56,41	0,08	3,02	-0,03	2,61	-
12	25,68	0,02	8,94	0,00	2,08	0,00	56,43	0,10	3,04	-0,01	-	-
13	25,73	0,07	8,92	-0,02	2,08	0,00	56,24	-0,09	3,06	0,01	2,63	-
14	25,75	0,09	8,94	0,00	2,12	0,04	56,51	0,18	3,06	0,01	2,64	-
15	25,58	-0,08	8,96	0,02	2,09	0,01	56,32	-0,01	3,02	-0,03	2,60	-
16	25,68	0,02	8,96	0,02	2,08	0,00	56,52	0,19	3,04	-0,01	2,59	-
101	25,63	-0,03	8,92	-0,02	2,12	0,04	56,56	0,23	3,02	-0,03	-	-
102	25,60	-0,06	8,92	-0,02	2,13	0,05	56,66	0,33	3,07	0,02	1,32	-
103	25,66	0,00	8,96	0,02	2,16	0,08	56,53	0,20	2,99	-0,06	2,56	-
104	25,53	-0,13	8,87	-0,07	2,12	0,04	56,32	-0,01	3,03	-0,02	1,89	-
105	25,63	-0,03	8,92	-0,02	2,12	0,04	56,55	0,22	3,08	0,03	2,57	-
106	25,52	-0,14	8,94	0,00	2,07	-0,01	56,56	0,23	3,02	-0,03	-	-
107	25,57	-0,09	8,94	0,00	2,06	-0,02	56,48	0,13	2,88	-0,17	-	-
108	25,74	0,08	8,95	0,01	2,13	0,05	56,64	0,31	3,04	-0,01	2,56	-
109	25,72	0,06	8,98	0,04	2,15	0,07	56,51	0,18	3,08	0,03	2,44	-
110	25,65	-0,01	8,88	-0,06	2,07	-0,01	56,55	0,22	3,07	0,02	1,92	-
111	25,31	-0,35	8,62	-0,32	2,10	0,02	56,30	-0,03	3,24	0,19	1,27	-
112	-	-	-	-	-	-	-	-	-	-	-	-
113	25,72	0,06	8,94	0,00	2,13	0,05	56,82	0,49	3,12	0,07	-	-
E1	25,65	-0,01	8,92	-0,02	2,08	0,00	56,43	0,10	3,04	-0,01	2,38	-
E2	25,58	-0,10	8,92	-0,02	2,12	0,04	56,52	0,19	3,03	-0,02	2,58	-
E3	25,35	-0,31	8,72	-0,22	2,12	0,04	56,35	0,02	3,21	0,16	2,52	-
E4	25,59	-0,07	8,87	-0,07	2,12	0,04	56,10	-0,23	2,99	-0,06	-	-
E5	25,65	-0,01	8,93	-0,01	2,10	0,02	56,23	-0,10	3,03	-0,02	-	-
E6	25,57	-0,09	8,87	-0,07	2,10	0,02	56,42	0,09	3,05	0,00	-	-
E7	25,79	0,13	8,91	-0,03	2,09	0,01	56,45	0,12	3,04	-0,01	2,62	-
E8	25,61	-0,05	8,93	-0,01	2,15	0,07	56,40	0,07	3,04	-0,01	2,71	-
E9	25,68	0,02	8,89	-0,05	2,10	0,02	56,54	0,21	3,06	0,01	-	-
E10	25,50	-0,16	8,64	-0,30	2,13	0,05	57,10	0,77	2,97	-0,08	2,16	-
E11	25,50	-0,16	8,99	0,05	2,14	0,06	57,04	0,71	3,11	0,06	2,50	-
E12	25,65	-0,01	8,96	0,02	2,09	0,01	56,46	0,13	3,09	0,04	-	-
<b>Average</b>	25,61		8,91		2,11		56,49		3,05		2,40	
<b>Max.</b>	25,79		9,00		2,16		57,10		3,24		2,71	
<b>Min.</b>	25,31		8,62		2,04		56,10		2,88		1,27	
<b>Range</b>	0,48		0,38		0,12		1,00		0,36		1,44	
<b>S.D.</b>	0,097		0,079		0,028		0,191		0,059		0,376	
<b>C.V.</b>	0,4		0,9		1,4		0,3		1,9		-	
<b>Certified value</b>	25,66		8,94		2,08		56,33		3,05		-	



Table 7 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %	
	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>
1	0,27	0,03	0,31	0,00	0,50	0,00	0,07	0,00	0,16	0,01	-	-
2	0,24	0,00	0,32	0,01	0,51	0,01	0,07	0,00	0,16	0,01	0,07	0,00
3	0,22	-0,02	0,32	0,01	0,51	0,01	0,08	0,01	0,16	0,01	-	-
4	0,24	0,00	0,32	0,01	0,51	0,01	0,08	0,01	0,15	0,00	0,06	-0,01
5	0,24	0,00	0,32	0,01	0,50	0,00	0,08	0,01	0,15	0,01	0,07	0,00
6	0,24	0,00	0,32	0,01	0,51	0,01	0,07	0,00	0,16	0,01	0,07	0,00
7	0,23	-0,01	0,32	0,01	0,50	0,00	0,07	0,00	0,15	0,00	0,07	0,00
8	0,23	-0,01	0,32	0,01	0,50	0,00	0,08	0,01	0,16	0,01	0,06	-0,01
9	0,25	0,01	0,31	0,00	0,50	0,00	0,07	0,00	0,16	0,01	0,06	-0,01
10	0,23	-0,01	0,32	0,01	0,51	0,01	0,07	0,00	0,16	0,01	-	-
11	0,25	0,01	0,32	0,01	0,50	0,00	0,08	0,01	0,16	0,01	-	-
12	0,24	0,00	0,33	0,02	0,51	0,01	0,08	0,01	0,16	0,01	0,06	-0,01
13	0,24	0,00	0,32	0,01	0,51	0,01	0,08	0,01	0,15	0,00	0,07	0,00
14	0,25	0,01	0,33	0,02	0,48	-0,02	0,09	0,02	0,15	0,00	0,07	0,00
15	0,25	0,01	0,32	0,01	0,52	0,02	0,08	0,01	0,16	0,01	0,06	-0,01
16	0,24	0,00	0,31	0,00	0,50	0,00	0,08	0,01	0,15	0,00	0,07	0,00
101	0,21	-0,03	0,32	0,01	0,51	0,01	0,07	0,00	-	-	-	-
102	-	-	0,31	0,00	-	-	-	-	-	-	-	-
103	0,24	0,00	0,31	0,00	-	-	-	-	-	-	-	-
104	0,26	0,02	0,32	0,01	0,50	0,00	0,07	0,00	0,16	0,01	0,07	0,00
105	0,23	-0,01	0,34	0,03	0,51	0,01	0,08	0,01	0,16	0,01	0,06	-0,01
106	0,25	0,01	0,33	0,02	-	-	-	-	-	-	-	-
107	0,26	0,02	0,33	0,02	-	-	0,07	0,00	0,16	0,01	-	-
108	0,24	0,00	0,32	0,01	-	-	0,08	0,01	-	-	-	-
109	-	-	0,31	0,00	-	-	-	-	-	-	-	-
110	0,23	-0,01	0,32	0,01	-	-	0,08	0,01	-	-	-	-
111	0,27	0,03	0,33	0,02	0,52	0,02	0,02	-0,05	0,16	0,01	0,06	-0,01
112	-	-	-	-	-	-	-	-	-	-	-	-
113	0,24	0,00	0,32	0,01	0,50	0,00	0,08	0,01	0,16	0,01	0,06	-0,01
E1	0,25	0,01	0,32	0,01	0,50	0,00	0,08	0,01	0,16	0,01	0,07	0,00
E2	0,28	0,04	0,32	0,01	0,50	0,00	0,08	0,01	0,16	0,01	-	-
E3	0,24	0,00	0,31	0,00	0,49	-0,01	0,08	0,01	0,18	0,03	0,08	0,01
E4	0,24	0,00	0,32	0,01	0,50	0,00	0,07	0,00	0,16	0,01	0,06	-0,01
E5	0,23	-0,01	0,32	0,01	0,51	0,01	0,07	0,00	0,16	0,01	0,08	0,01
E6	0,12	-0,12	0,32	0,01	0,50	0,00	0,11	0,04	0,15	0,00	-	-
E7	0,25	0,01	0,32	0,01	0,50	0,00	0,08	0,01	0,16	0,01	0,08	0,01
E8	0,26	0,02	0,32	0,01	0,51	0,01	0,07	0,00	0,16	0,01	0,06	-0,01
E9	-	-	0,33	0,02	0,53	0,03	-	-	-	-	-	-
E10	0,26	0,02	0,34	0,03	-	-	-	-	-	-	-	-
E11	0,23	-0,01	0,33	0,02	0,50	0,01	0,08	0,01	0,16	0,01	0,08	0,01
E12	0,25	0,01	0,32	0,01	0,50	0,01	0,08	0,01	0,18	0,03	-	-
<b>Average</b>	0,24		0,32		0,50		0,08		0,16		0,07	
<b>Max.</b>	0,28		0,34		0,53		0,11		0,18		0,08	
<b>Min.</b>	0,12		0,31		0,48		0,02		0,15		0,06	
<b>Range</b>	0,16		0,03		0,05		0,09		0,03		0,02	
<b>S.D.</b>	0,025		0,007		0,009		0,013		0,007		0,008	
<b>C.V.</b>	10,3		2,4		1,8		18,0		4,5		10,7	
<b>Certified value</b>	0,24		0,31		0,50		0,07		0,15		0,07	

NOTE Data in shaded cells represent concentrations that did not satisfy the required criteria for accuracy limits for "expert" laboratories specified for the XRF method.

<sup>a</sup> SO<sub>3</sub> determination for JCA-CRM-2 is outside the scope of JIS R 5204.

<sup>b</sup> "Mean value" is the mean value of the concentrations of a pair of validated beads.

<sup>c</sup> "Diff." is the difference between the mean value of the concentrations of a pair of validated beads and the certified value for the validation material.

5.3 Test results of Q-laboratories

5.3.1 Differences in concentration for each pair of test samples

The differences in concentration for each pair of Sample JCA #1 and Sample JCA #2 is shown in Table 8 and Table 9.

**Table 8 — Differences in concentrations for each pair of test sample**  
(Q-laboratories —Test sample: Sample JCA #1)

Laboratory ref.	SiO <sub>2</sub> %	Al <sub>2</sub> O <sub>3</sub> %	Fe <sub>2</sub> O <sub>3</sub> %	CaO %	MgO %	SO <sub>3</sub> %	Na <sub>2</sub> O %	K <sub>2</sub> O %	TiO <sub>2</sub> %	P <sub>2</sub> O <sub>5</sub> %	MnO %	SrO %
1	0,066	0,021	0,008	0,128	0,002	0,002	0,012	0,019	0,002	0,001	0,000	- <sup>a</sup>
2	0,015	0,008	0,003	0,066	0,005	0,030	0,003	0,001	0,002	0,004	0,002	0,000
3	0,082	0,021	0,023	0,139	0,027	0,020	0,003	0,001	0,005	0,001	0,000	-
4	0,098	0,008	0,007	0,015	0,016	0,001	0,008	0,008	0,006	0,003	0,001	0,001
5	0,008	0,006	0,002	0,027	0,006	0,014	0,001	0,001	0,000	0,001	0,000	0,000
6	0,085	0,030	0,005	0,175	0,006	0,019	0,018	0,011	0,006	0,001	0,000	0,000
7	0,016	0,004	0,003	0,062	0,013	0,001	0,005	0,000	0,000	0,001	0,001	0,000
8	0,064	0,001	0,002	0,007	0,005	0,007	0,000	0,002	0,003	0,001	0,003	0,000
9	0,010	0,001	0,003	0,062	0,000	0,007	0,000	0,001	0,003	0,003	0,000	0,000
10	0,050	0,024	0,001	0,120	0,031	0,010	0,014	0,001	0,002	0,010	0,000	-
11	0,005	0,046	0,017	0,224	0,006	0,040	0,001	0,007	0,005	0,003	0,002	-
12	0,022	0,006	0,004	0,079	0,010	0,020	0,003	0,002	0,006	0,000	0,000	0,001
13	0,028	0,010	0,001	0,083	0,006	0,007	0,002	0,001	0,001	0,001	0,001	0,000
14	0,058	0,003	0,003	0,026	0,004	0,014	0,000	0,001	0,009	0,001	0,000	0,000
15	0,056	0,035	0,018	0,199	0,022	0,030	0,011	0,003	0,003	0,002	0,002	0,000
16	0,022	0,014	0,002	0,108	0,008	0,003	0,006	0,003	0,001	0,004	0,001	0,000
104	0,102	0,035	0,040	0,135	0,010	0,029	0,005	0,019	0,007	0,004	0,001	0,000
106	0,083	0,007	0,011	0,128	0,001	0,025	0,004	0,002	-	-	-	-
108	0,020	0,000	0,000	0,060	0,010	0,010	0,000	0,000	-	0,000	-	-
109	0,034	0,000	0,003	0,053	0,008	0,012	-	0,007	-	-	-	-
E1	0,023	0,060	0,022	0,077	0,015	0,013	0,011	0,003	0,013	0,007	0,001	0,001
E4	0,079	0,020	0,003	0,066	0,007	0,026	0,006	0,004	0,002	0,000	0,000	0,004
E5	0,020	0,060	0,010	0,120	0,050	0,000	0,000	0,010	0,012	0,012	0,004	0,001
E6	0,024	0,017	0,011	0,189	0,004	0,015	0,004	0,000	0,001	0,004	0,001	-
E7	0,120	0,032	0,019	0,070	0,034	0,020	0,003	0,004	0,001	0,011	0,001	0,002
E8	0,019	0,021	0,017	0,091	0,021	0,002	0,011	0,001	0,004	0,002	0,000	0,000
E9	0,088	0,050	0,009	0,138	0,006	-	0,013	0,010	0,012	-	-	-
<b>Average</b>	0,049	0,033	0,011	0,101	0,018	0,012	0,006	0,004	0,006	0,005	0,001	0,002
<b>Max.</b>	0,120	0,060	0,022	0,189	0,050	0,026	0,013	0,019	0,013	0,012	0,004	0,004
<b>Min.</b>	0,019	0,000	0,000	0,060	0,004	0,000	0,000	0,000	0,000	0,000	0,000	0,000
<b>Range</b>	0,101	0,060	0,022	0,129	0,046	0,026	0,013	0,019	0,013	0,012	0,004	0,004
<b>Mean analysis</b>	20,91	5,09	3,03	65,95	1,37	2,21	0,21	0,50	0,31	0,24	0,10	0,05
<b>Limit value</b>	0,150	0,080	0,080	0,250	0,080	0,080	0,020	0,030	0,030	0,020	0,020	0,020

<sup>a</sup> “-” indicates that there was no result reported by the laboratory.

**Table 9 — Differences in concentrations for each pair of test sample**  
(Q-laboratories — Test sample: Sample JCA #2)

Laboratory ref.	SiO <sub>2</sub> %	Al <sub>2</sub> O <sub>3</sub> %	Fe <sub>2</sub> O <sub>3</sub> %	CaO %	MgO %	SO <sub>3</sub> <sup>a</sup> %	Na <sub>2</sub> O %	K <sub>2</sub> O %	TiO <sub>2</sub> %	P <sub>2</sub> O <sub>5</sub> %	MnO %	SrO %
1	0,014	0,011	0,002	0,077	0,002	0,006	0,000	0,003	0,001	0,000	0,000	- <sup>b</sup>
2	0,027	0,006	0,006	0,022	0,018	0,004	0,002	0,001	0,006	0,001	0,000	0,001
3	0,015	0,000	0,005	0,013	0,006	-	0,003	0,000	0,002	0,000	0,000	-
4	0,015	0,005	0,005	0,017	0,005	0,008	0,000	0,000	0,003	0,002	0,001	0,000
5	0,019	0,008	0,003	0,083	0,004	0,018	0,001	0,002	0,001	0,002	0,000	0,001
6	0,066	0,003	0,022	0,050	0,011	0,052	0,004	0,001	0,004	0,006	0,000	0,000
7	0,015	0,006	0,000	0,002	0,014	0,002	0,002	0,001	0,004	0,001	0,001	0,000
8	0,061	0,001	0,001	0,014	0,002	0,003	0,006	0,001	0,002	0,001	0,000	0,000
9	0,012	0,013	0,002	0,010	0,004	-	0,000	0,000	0,003	0,001	0,001	0,000
10	0,081	0,016	0,002	0,204	0,011	-	0,007	0,000	0,000	0,001	0,001	-
11	0,067	0,065	0,015	0,120	0,017	0,038	0,008	0,002	0,005	0,001	0,001	-
12	0,039	0,045	0,028	0,115	0,027	-	0,004	0,005	0,006	0,001	0,001	0,001
13	0,011	0,064	0,007	0,109	0,007	0,013	0,001	0,003	0,012	0,003	0,000	0,000
14	0,094	0,040	0,006	0,061	0,001	0,013	0,002	0,000	0,001	0,001	0,000	0,000
15	0,003	0,024	0,004	0,047	0,040	0,039	0,008	0,003	0,002	0,000	0,000	0,000
16	0,013	0,018	0,001	0,050	0,015	0,024	0,008	0,002	0,007	0,002	0,001	0,000
104	0,038	0,022	0,011	0,045	0,006	0,036	0,010	0,016	0,003	0,007	0,001	0,001
106	0,082	0,077	0,013	0,187	0,011	-	0,004	0,001	-	-	-	-
108	0,020	0,010	0,000	0,100	0,050	0,030	0,020	0,000	-	0,000	-	-
109	0,041	0,019	0,052	0,142	0,012	0,090	-	0,004	-	-	-	-
E1	0,045	0,063	0,025	0,121	0,002	0,179	0,008	0,005	0,007	0,007	0,001	0,001
E4	0,062	0,054	0,001	0,111	0,026	0,047	0,013	0,001	0,001	0,002	0,004	0,002
E5	0,040	0,030	0,010	0,120	0,100	0,030	0,015	0,000	0,003	0,010	0,001	0,002
E6	0,002	0,019	0,008	0,041	0,033	-	0,000	0,003	0,000	0,007	0,002	-
E7	0,118	0,052	0,001	0,179	0,008	0,013	0,003	0,002	0,003	0,005	0,001	0,001
E8	0,049	0,003	0,014	0,070	0,038	0,005	0,008	0,002	0,000	0,004	0,000	0,000
E9	0,063	0,025	0,006	0,082	0,008	-	-	0,001	0,016	-	-	-
<b>Average</b>	0,041	0,026	0,009	0,081	0,018	0,033	0,005	0,002	0,004	0,003	0,001	0,001
<b>Max.</b>	0,118	0,077	0,052	0,204	0,100	0,179	0,020	0,016	0,016	0,010	0,004	0,002
<b>Min.</b>	0,002	0,000	0,000	0,002	0,001	0,002	0,000	0,000	0,000	0,000	0,000	0,000
<b>Range</b>	0,116	0,077	0,052	0,202	0,099	0,177	0,020	0,016	0,016	0,010	0,004	0,002
<b>Mean analysis</b>	26,00	8,81	1,62	56,12	3,35	2,82	0,21	0,42	0,39	0,24	0,09	0,05
<b>Limit value</b>	0,150	0,120	0,080	0,250	0,080	-	0,020	0,020	0,020	0,020	0,020	0,020

NOTE Data in shaded cells represent results that did not satisfy the required criteria for repeatability specified for "expert" laboratories for the XRF method.

<sup>a</sup> SO<sub>3</sub> determination for sample JCA #2 is outside the scope of JIS R 5204.

<sup>b</sup> "-" indicates that there was no result reported by the laboratory.

### 5.3.2 Distribution of concentrations for test samples

Each concentration obtained by Q-laboratories for Sample JCA #1 and Sample JCA #2 is shown in Table 10 and Table 11. "Mean value" represents the average of two concentrations, and "Diff." represents the difference between the "Mean value" and the average, respectively. Data in parentheses are "outliers" by the Grubbs test, which was excluded from statistic calculation of the results.

The Grubbs test specified in 7.3.4 of ISO 5725-2:1994 was carried out when analysing results. "Outlier" means 5% "outlier" by the Grubbs test and "Outliers in Q-laboratory" are shown in the histograms. However, although both the minimum of K<sub>2</sub>O and the maximum of SrO for Sample JCA #2 were judged as "outliers", it was concluded that they were not "extreme results" and therefore, they were not excluded.

With regard to judgment of validation for results obtained by XRF analysis using validated calibration, it would be unlikely that the analytical accuracy of the results varies significantly in the same kind of sample without a failure in one of the processes of XRF analysis. For example, both JCA-CRM-1 and Sample JCA #1 are Portland cement, and both JCA-CRM-2 and Sample JCA #2 are Portland blast furnace slag cement.

It is normal practice that when there is a statistical “outlier” it is necessary to conduct an investigation to determine the cause.

The histograms of concentrations of test samples for all constituents are shown in Figure 1 to Figure 23. The data group shown by the shaded bars indicates the data of Q-laboratories, and the white bars indicate the data of the other laboratories (non-Q-laboratories). The average and two times the standard deviation ( $2\sigma$ ) shown in the histograms were calculated after excluding “outliers”.

The concentrations obtained by Q-laboratories were generally distributed between the average  $\pm 2\sigma$  for all constituents. On the other hand, the distribution of concentrations of non-Q-laboratories was wider than that of Q-laboratories, and there were some concentrations that were far from the average. As reported above, it is important for accurate analysis to use calibration equations validated in accordance with this XRF method.

**Table 10 — Concentrations for sample JCA #1 — Q-laboratories**

Laboratory ref.	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> %	
	Mean value <sup>a</sup>	Diff. b	Mean value <sup>a</sup>	Diff. b	Mean value <sup>a</sup>	Diff. b	Mean value <sup>a</sup>	Diff. b	Mean value <sup>a</sup>	Diff. b	Mean value <sup>a</sup>	Diff. b
1	20,93	-0,03	5,11	0,01	2,99	-0,04	65,97	0,08	1,36	0,00	2,23	0,02
2	20,85	-0,11	5,10	0,00	3,02	-0,01	65,95	0,06	1,36	0,00	2,19	-0,02
3	20,96	0,00	5,11	0,01	3,03	0,00	65,86	-0,03	1,34	-0,02	2,19	-0,02
4	20,88	-0,08	5,10	0,00	3,04	0,01	65,87	-0,02	1,36	0,00	2,25	0,04
5	20,90	-0,06	5,12	0,02	3,04	0,01	65,94	0,05	1,36	0,00	2,22	0,01
6	21,04	0,08	5,12	0,02	2,99	-0,04	65,91	0,02	1,34	-0,02	2,23	0,02
7	20,92	-0,04	5,10	0,00	3,03	0,00	65,76	-0,13	1,36	0,00	2,21	0,00
8	20,96	0,00	5,13	0,03	3,03	0,00	65,80	-0,09	1,38	0,02	2,21	0,00
9	20,83	-0,13	5,10	0,00	2,98	-0,05	65,89	0,00	1,36	0,00	2,23	0,02
10	20,98	0,02	5,08	-0,02	3,01	-0,02	66,10	0,21	1,36	0,00	2,22	0,01
11	21,01	0,05	5,12	0,02	3,05	0,02	65,89	0,00	1,36	0,00	(1,99) <sup>c</sup>	-
12	20,96	0,00	5,11	0,01	3,05	0,02	65,84	-0,05	1,34	-0,02	2,17	-0,04
13	21,08	0,12	5,12	0,02	3,06	0,03	65,68	-0,21	1,37	0,01	2,21	0,00
14	20,96	0,00	5,13	0,03	3,10	0,07	66,15	0,26	1,37	0,01	2,20	-0,01
15	21,07	0,11	5,12	0,02	3,05	0,02	65,86	-0,03	1,33	-0,03	2,16	-0,05
16	20,96	0,00	5,12	0,02	3,04	0,01	65,77	-0,12	1,38	0,02	2,21	0,00
104	20,95	-0,01	5,09	-0,01	3,00	-0,03	65,51	-0,38	1,37	0,01	2,15	-0,06
106	(20,47) <sup>c</sup>	-	5,05	-0,05	2,97	-0,06	(64,61) <sup>c</sup>	-	1,33	-0,03	2,17	-0,04
108	21,01	0,05	5,12	0,02	3,00	-0,03	65,88	-0,01	1,36	0,00	2,22	0,01
109	20,80	-0,16	5,06	-0,04	3,00	-0,03	65,88	-0,01	1,35	-0,01	2,11	-0,10
E1	20,89	-0,06	5,12	0,01	3,04	0,01	65,86	-0,03	1,36	0,00	2,30	0,09
E4	20,94	-0,01	5,10	-0,01	2,99	-0,03	65,71	-0,18	1,30	-0,06	2,21	0,00
E5	21,06	0,10	5,07	-0,03	3,02	-0,01	66,00	0,11	1,39	0,03	2,22	0,01
E6	21,10	0,14	5,10	-0,01	3,08	0,06	66,37	0,48	1,37	0,02	2,24	0,03
E7	20,86	-0,10	5,09	-0,01	3,08	0,05	65,83	-0,06	1,37	0,01	2,22	0,01
E8	20,92	-0,04	5,10	0,00	2,98	-0,04	65,91	0,02	1,37	0,01	2,22	0,01
E9	21,01	0,05	5,13	0,02	3,04	0,01	65,91	0,02	1,35	-0,01	-	-
<b>Average</b>	20,96		5,10		3,03		65,89		1,36		2,21	
<b>Max.</b>	21,10		5,13		3,10		66,37		1,39		2,30	
<b>Min.</b>	20,80		5,05		2,97		65,51		1,30		2,11	
<b>Range</b>	0,30		0,08		0,13		0,86		0,09		0,19	
<b>S.D.</b>	0,078		0,021		0,033		0,160		0,018		0,037	
<b>C.V.</b>	0,4		0,4		1,1		0,2		1,4		1,7	

Table 10 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %	
	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean Value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>	Mean value <sup>a</sup>	Diff. <sup>b</sup>
1	0,21	0,00	(0,45) <sup>c</sup>	-	0,31	0,00	0,24	0,00	0,10	0,00	-	-
2	0,21	0,00	0,50	0,00	0,32	0,01	0,24	0,00	0,10	0,00	0,05	0,00
3	0,19	-0,02	0,50	0,00	0,32	0,01	0,23	-0,01	0,09	-0,01	-	-
4	0,21	0,00	0,50	0,00	0,32	0,01	0,24	0,00	0,10	0,00	0,05	0,00
5	0,21	0,00	0,49	-0,01	0,32	0,01	0,24	0,00	0,10	0,00	0,05	0,00
6	0,23	0,02	0,52	0,02	0,31	0,00	0,24	0,00	0,09	-0,01	0,04	-0,01
7	0,20	-0,01	0,49	-0,01	0,32	0,01	0,24	0,00	0,10	0,00	0,05	0,00
8	0,19	-0,02	0,49	-0,01	0,32	0,01	0,24	0,00	0,09	-0,01	0,05	0,00
9	0,21	0,00	0,50	0,00	0,31	0,00	0,24	0,00	0,10	0,00	0,04	-0,01
10	0,18	-0,03	0,50	0,00	0,32	0,01	0,24	0,00	0,10	0,00	-	-
11	0,19	-0,02	0,52	0,02	0,32	0,01	0,24	0,00	0,10	0,00	-	-
12	0,21	0,00	0,48	-0,02	0,32	0,01	0,24	0,00	0,09	-0,01	0,05	0,00
13	0,21	0,00	0,49	-0,01	0,31	0,00	0,25	0,01	0,09	-0,01	0,05	0,00
14	0,21	0,00	0,49	-0,01	0,30	-0,01	0,25	0,01	0,10	0,00	0,05	0,00
15	0,18	-0,03	0,49	-0,01	0,31	0,00	0,24	0,00	0,10	0,00	0,05	0,00
16	0,21	0,00	0,50	0,00	0,32	0,01	0,24	0,00	0,09	-0,01	0,05	0,00
104	(0,13) <sup>c</sup>	-	0,49	-0,01	0,31	0,00	0,23	-0,01	0,09	-0,01	0,04	-0,01
106	0,20	-0,01	0,49	-0,01	-	-	-	-	-	-	-	-
108	(0,13) <sup>c</sup>	-	0,49	-0,01	-	-	0,24	0,00	-	-	-	-
109	-	-	0,50	0,00	-	-	-	-	-	-	-	-
E1	0,20	-0,01	0,49	0,00	0,32	0,01	0,24	0,00	0,10	0,00	0,05	0,00
E4	0,23	0,02	0,49	-0,01	0,31	0,00	0,24	0,00	0,09	0,00	0,05	0,01
E5	0,23	0,03	0,51	0,01	0,31	0,00	0,23	-0,01	0,10	0,00	0,05	0,00
E6	(0,10) <sup>c</sup>	-	0,50	0,00	0,31	0,00	0,27	0,03	0,09	-0,01	-	-
E7	0,21	0,00	0,50	0,00	0,32	0,01	0,24	0,00	0,10	0,00	0,06	0,01
E8	0,21	0,00	0,50	0,00	0,31	0,00	0,24	0,00	0,10	0,00	0,05	0,00
E9	0,26	0,05	0,51	0,01	0,30	-0,01	-	-	-	-	-	-
<b>Average</b>	0,21		0,50		0,31		0,24		0,10		0,05	
<b>Max.</b>	0,26		0,52		0,32		0,27		0,10		0,06	
<b>Min.</b>	0,18		0,48		0,30		0,23		0,09		0,04	
<b>Range</b>	0,08		0,04		0,02		0,04		0,01		0,02	
<b>S.D.</b>	0,019		0,009		0,007		0,008		0,005		0,005	
<b>C.V.</b>	8,9		1,8		2,1		3,4		4,9		10,8	

<sup>a</sup> "Mean value" is the mean value of the concentrations of a pair of analysis beads.

<sup>b</sup> "Diff." is the difference between the mean value of the concentrations of a pair of analysis beads and the average for all Q-laboratories.

<sup>c</sup> Concentrations in parentheses are the "outliers" by the Grubbs test.

Table 11 — Concentrations for Sample JCA #2 — Q-laboratories

Laboratory ref.	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> <sup>a</sup> %	
	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>
1	26,02	0,01	8,83	0,03	1,62	0,00	56,03	-0,06	3,34	0,02	2,90	0,04
2	25,83	-0,18	8,76	-0,04	1,63	0,01	56,14	0,05	3,31	-0,01	2,90	0,04
3	25,99	-0,02	8,82	0,02	1,56	-0,06	56,25	0,16	3,29	-0,03	-	-
4	26,00	-0,01	8,78	-0,02	1,65	0,03	55,90	-0,19	3,32	0,00	2,92	0,06
5	25,95	-0,06	8,80	0,00	1,62	0,00	56,16	0,07	3,31	-0,01	2,89	0,03
6	26,16	0,15	(8,98) <sup>d</sup>	-	1,63	0,01	56,20	0,11	3,38	0,06	2,83	-0,03
7	25,99	-0,02	8,82	0,02	1,61	-0,01	56,06	-0,03	3,35	0,03	2,95	0,09
8	26,04	0,03	8,77	-0,03	(1,51) <sup>d</sup>	-	55,63	-0,46	3,34	0,02	2,68	-0,18
9	25,91	-0,10	8,77	-0,03	1,63	0,01	56,01	-0,08	3,32	0,00	-	-
10	25,94	-0,07	8,77	-0,03	1,63	0,01	56,09	0,00	3,29	-0,03	-	-
11	25,91	-0,10	8,72	-0,08	1,61	-0,01	56,08	-0,01	3,28	-0,04	2,72	-0,14
12	26,03	0,02	8,79	-0,01	1,58	-0,04	55,95	-0,14	3,33	0,01	-	-
13	26,10	0,09	8,83	0,03	1,63	0,01	55,90	-0,19	3,32	0,00	2,96	0,10
14	26,06	0,05	8,81	0,01	1,64	0,02	56,11	0,02	3,31	-0,01	2,97	0,11
15	26,15	0,14	8,87	0,07	1,64	0,02	55,82	-0,27	3,30	-0,02	2,93	0,07
16	26,02	0,01	8,80	0,00	1,61	-0,01	56,21	0,12	3,32	0,00	2,93	0,07
104	25,98	-0,03	8,78	-0,02	1,63	0,01	56,08	-0,01	3,31	-0,01	(1,80) <sup>d</sup>	-
106	25,97	-0,04	8,80	0,00	1,57	-0,05	55,98	-0,11	3,28	-0,04	-	-
108	26,07	0,06	8,76	-0,04	1,63	0,01	56,22	0,13	3,32	0,00	2,88	0,02
109	26,15	0,14	8,85	0,05	1,66	0,04	56,50	0,41	3,35	0,03	(1,66) <sup>d</sup>	-
E1	25,95	-0,06	8,84	0,04	1,62	0,00	56,10	0,02	3,32	0,00	2,52	-0,34
E4	25,87	-0,14	8,80	0,00	1,60	-0,02	(55,31) <sup>d</sup>	-	(3,23) <sup>d</sup>	-	(3,75) <sup>d</sup>	-
E5	26,00	-0,01	8,75	-0,05	1,60	-0,02	56,11	0,02	3,32	0,00	(2,09) <sup>d</sup>	-
E6	26,07	0,06	8,79	-0,01	1,64	0,02	56,53	0,44	3,36	0,04	-	-
E7	25,95	-0,06	8,76	-0,04	1,63	0,01	55,93	-0,16	3,32	0,00	2,94	0,07
E8	26,03	0,02	8,81	0,02	1,63	0,01	55,94	-0,15	3,34	0,02	2,88	0,02
E9	26,09	0,08	8,87	0,07	1,58	-0,04	56,29	0,20	3,34	0,01	-	-
<b>Average</b>	26,01		8,80		1,62		56,09		3,32		2,86	
<b>Max.</b>	26,16		8,87		1,66		56,53		3,38		2,97	
<b>Min.</b>	25,83		8,72		1,56		55,63		3,28		2,52	
<b>Range</b>	0,33		0,15		0,10		0,90		0,10		0,45	
<b>S.D.</b>	0,083		0,037		0,025		0,192		0,024		0,121	
<b>C.V.</b>	0,3		0,4		1,5		0,3		0,7		4,2	

Table 11 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %	
	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>	Mean value <sup>b</sup>	Diff. <sup>c</sup>
1	0,25	0,03	0,40	-0,02	0,40	0,01	0,24	0,00	0,10	0,01	-	-
2	0,23	0,01	0,43	0,01	0,39	0,00	0,24	0,00	0,09	0,00	0,05	0,00
3	0,21	-0,01	0,43	0,01	0,40	0,01	0,24	0,00	0,10	0,01	-	-
4	0,22	0,00	0,42	0,00	0,39	0,00	0,24	0,00	0,09	0,00	0,05	0,00
5	0,22	0,00	0,43	0,01	0,39	0,00	0,24	0,00	0,09	0,00	0,05	0,00
6	0,19	-0,03	0,42	0,00	0,39	0,00	0,23	-0,01	0,09	0,00	0,05	0,00
7	0,21	-0,01	0,43	0,01	0,39	0,00	0,24	0,00	0,09	0,00	0,05	0,00
8	0,22	0,00	0,43	0,01	0,40	0,01	0,24	0,00	0,09	0,00	0,05	0,00
9	0,23	0,01	0,41	-0,01	0,40	0,01	0,23	-0,01	0,10	0,01	0,05	0,00
10	0,21	-0,01	0,43	0,01	0,40	0,01	0,23	-0,01	0,10	0,01	-	-
11	0,20	-0,02	0,42	0,00	0,38	-0,01	0,24	0,00	0,09	0,00	-	-
12	0,23	0,01	0,42	0,00	0,40	0,01	0,23	-0,01	0,09	0,00	0,06	0,01
13	0,22	0,00	0,43	0,01	0,40	0,01	0,25	0,01	0,08	-0,01	0,05	0,00
14	0,22	0,00	0,43	0,01	0,38	-0,01	0,25	0,01	0,09	0,00	0,05	0,00
15	0,20	-0,02	0,43	0,01	0,38	-0,01	0,25	0,01	0,09	0,00	0,05	0,00
16	0,22	0,00	0,42	0,00	0,38	-0,01	0,24	0,00	0,09	0,00	0,05	0,00
104	0,19	-0,03	0,42	0,00	0,39	0,00	0,23	-0,01	0,09	0,00	0,05	0,00
106	0,24	0,02	0,43	0,01	-	-	-	-	-	-	-	-
108	(0,15) <sup>d</sup>	-	0,43	0,01	-	-	0,23	-0,01	-	-	-	-
109	-	-	0,43	0,01	-	-	-	-	-	-	-	-
E1	0,21	-0,01	0,43	0,01	0,39	-0,01	0,25	0,01	0,09	-0,01	0,05	0,00
E4	0,23	0,01	0,42	-0,01	0,39	0,00	0,23	-0,01	0,10	0,01	0,05	0,00
E5	0,23	0,01	0,43	0,01	0,40	0,01	0,23	-0,01	0,09	0,00	0,05	0,00
E6	(0,10) <sup>d</sup>	-	0,43	0,01	0,38	-0,01	0,27	0,03	0,08	-0,01	-	-
E7	0,23	0,01	0,43	0,00	0,39	0,00	0,24	0,00	0,09	0,00	0,06	0,01
E8	0,22	0,00	0,42	0,00	0,40	0,00	0,23	-0,01	0,10	0,00	0,05	0,00
E9	-	-	0,42	0,00	0,43	0,03	-	-	-	-	-	-
<b>Average</b>	0,22		0,42		0,39		0,24		0,09		0,05	
<b>Max.</b>	0,25		0,43		0,43		0,27		0,10		0,06	
<b>Min.</b>	0,19		0,40		0,38		0,23		0,08		0,05	
<b>Range</b>	0,06		0,03		0,05		0,04		0,02		0,01	
<b>S.D.</b>	0,014		0,008		0,010		0,009		0,006		0,003	
<b>C.V.</b>	6,6		1,8		2,6		3,9		6,4		5,8	

<sup>a</sup> SO<sub>3</sub> for sample JCA #2 is outside the scope of JIS R 5204.

<sup>b</sup> "Mean value" is the mean value of the concentrations of a pair of analysis beads.

<sup>c</sup> "Diff." is the difference between the mean value of the concentrations of a pair of analysis beads and the average for all Q-laboratories.

<sup>d</sup> Concentrations in parentheses are the "outliers" by the Grubbs test.

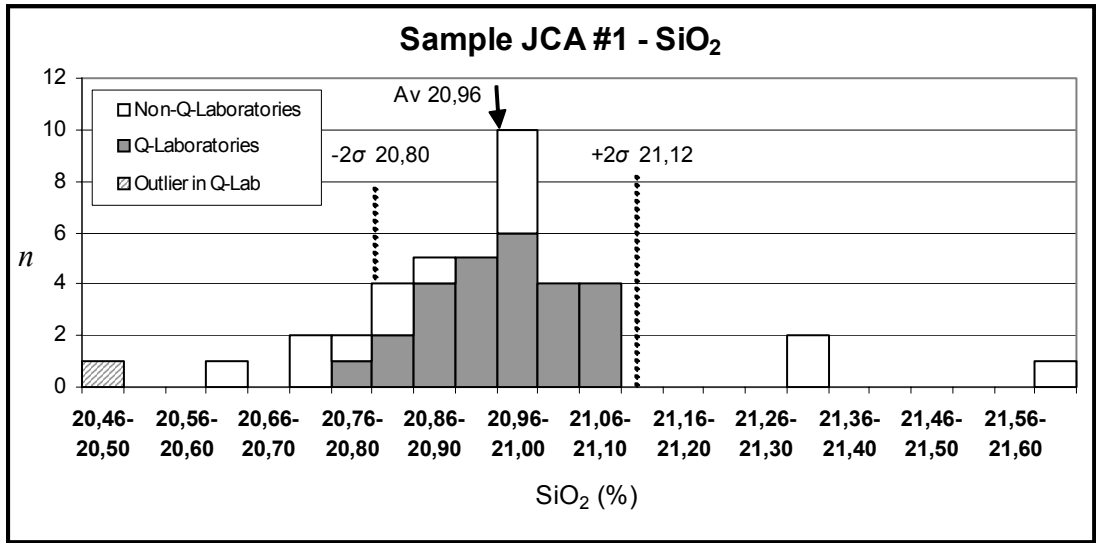


Figure 1 — The histogram of concentrations (Sample JCA #1, constituent SiO<sub>2</sub>)

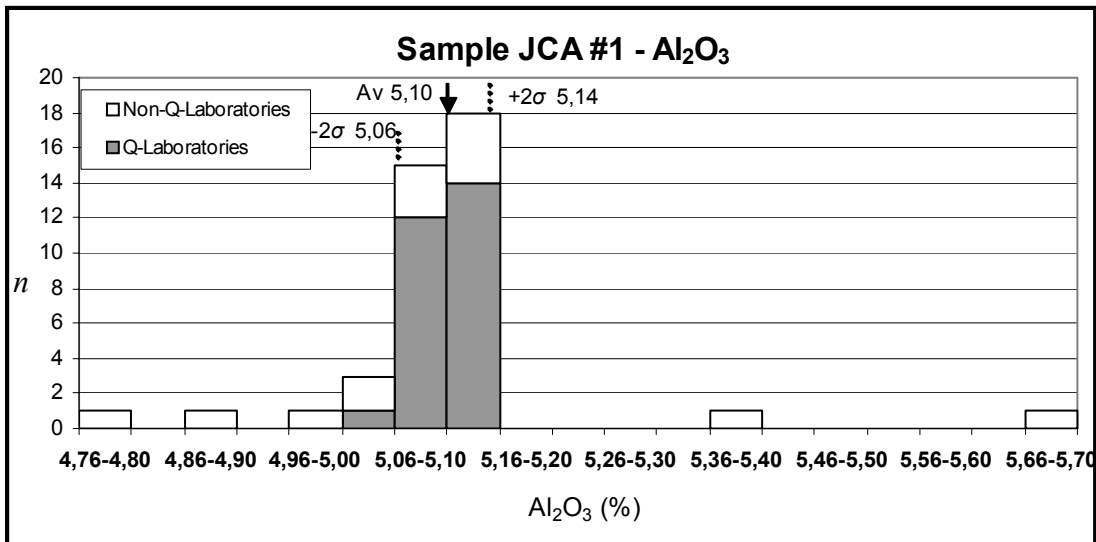


Figure 2 — The histogram of concentrations (Sample JCA #1, constituent Al<sub>2</sub>O<sub>3</sub>)

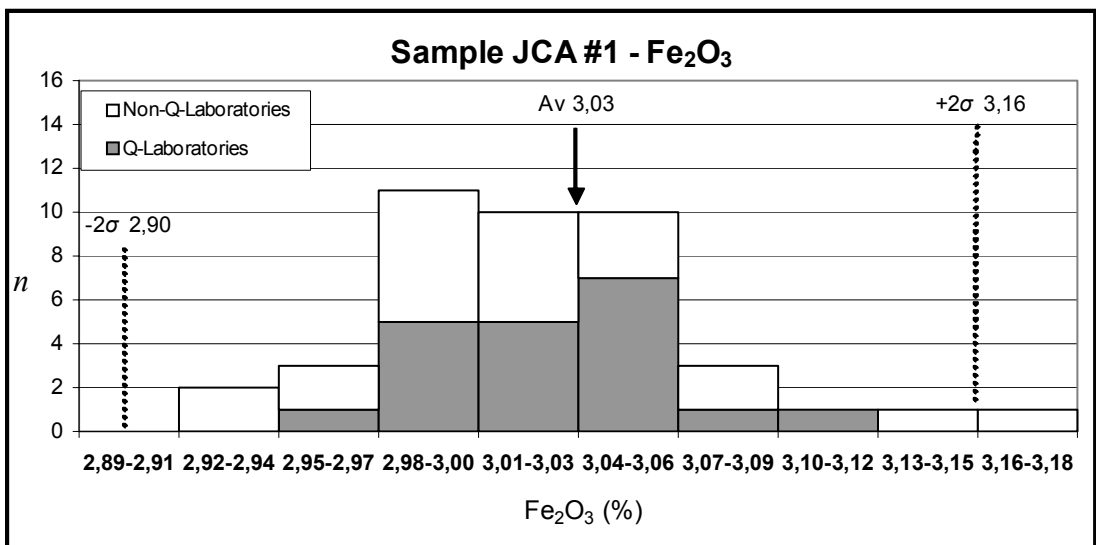


Figure 3 — The histogram of concentrations (Sample JCA #1, constituent Fe<sub>2</sub>O<sub>3</sub>)



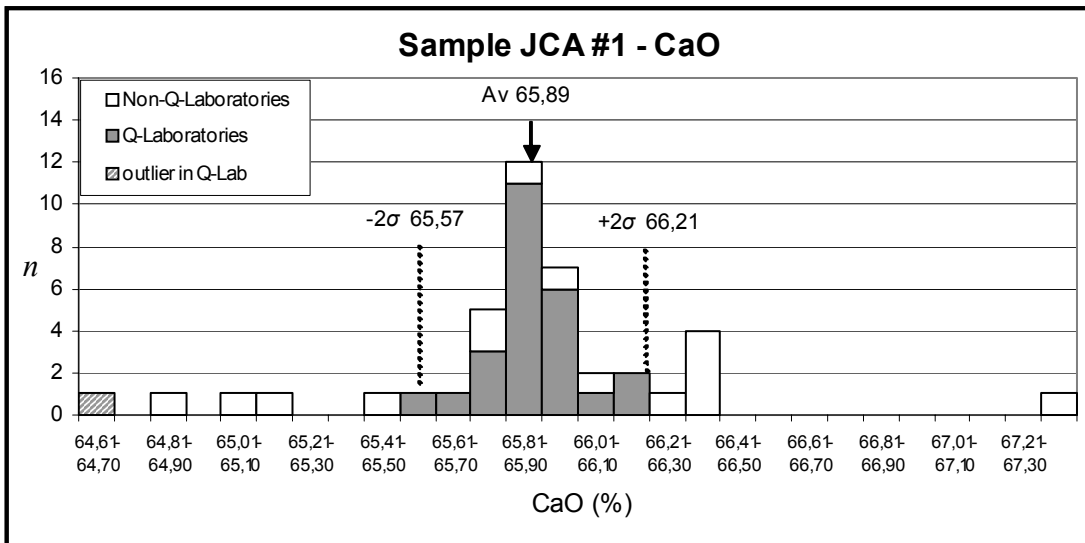


Figure 4 — The histogram of concentrations (Sample JCA #1, constituent CaO)

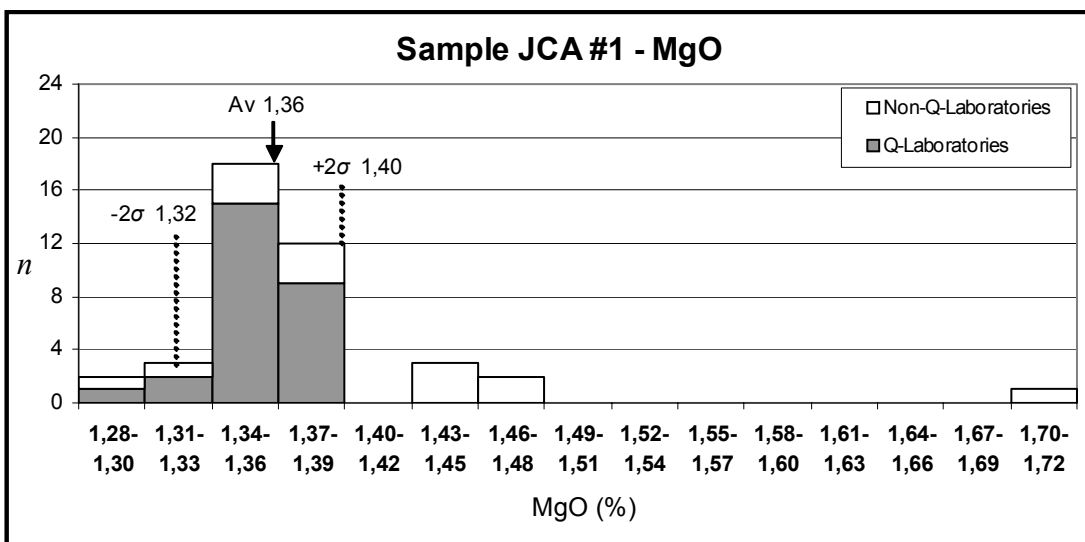


Figure 5 — The histogram of concentrations (Sample JCA #1, constituent MgO)

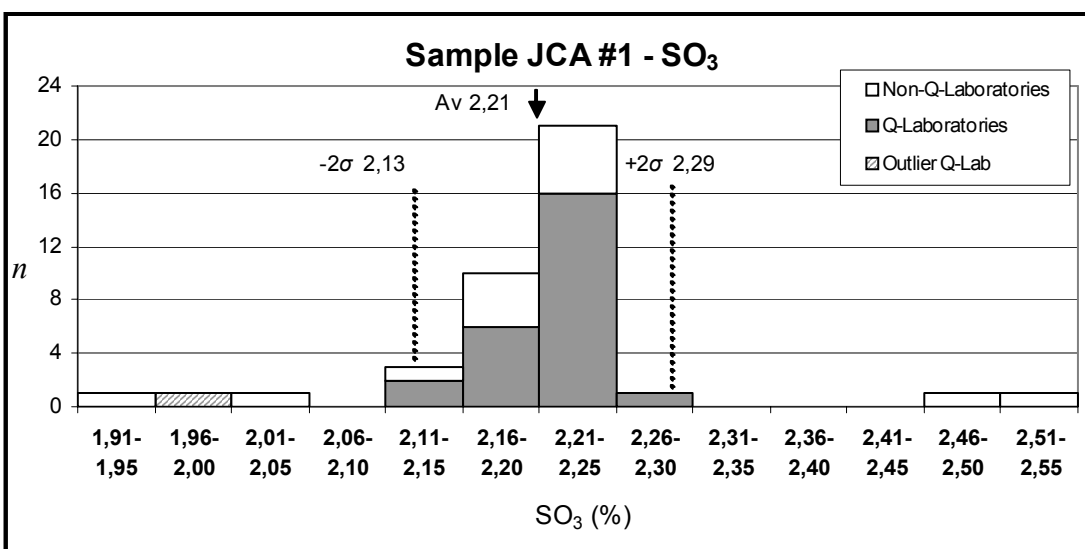


Figure 6 — The histogram of concentrations (Sample JCA #1, constituent SO<sub>3</sub>)

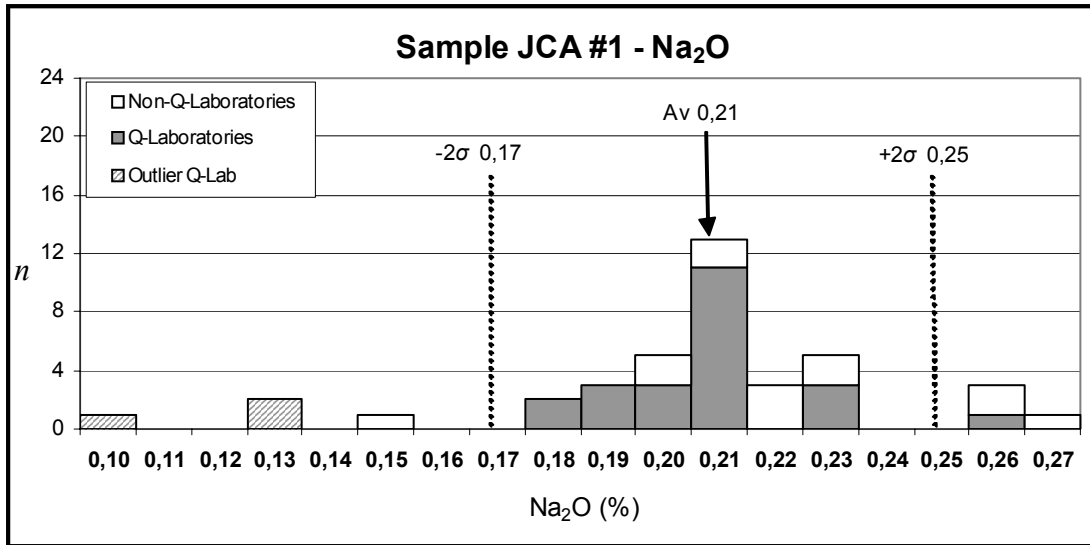


Figure 7 — The histogram of concentrations (Sample JCA #1, constituent Na<sub>2</sub>O)

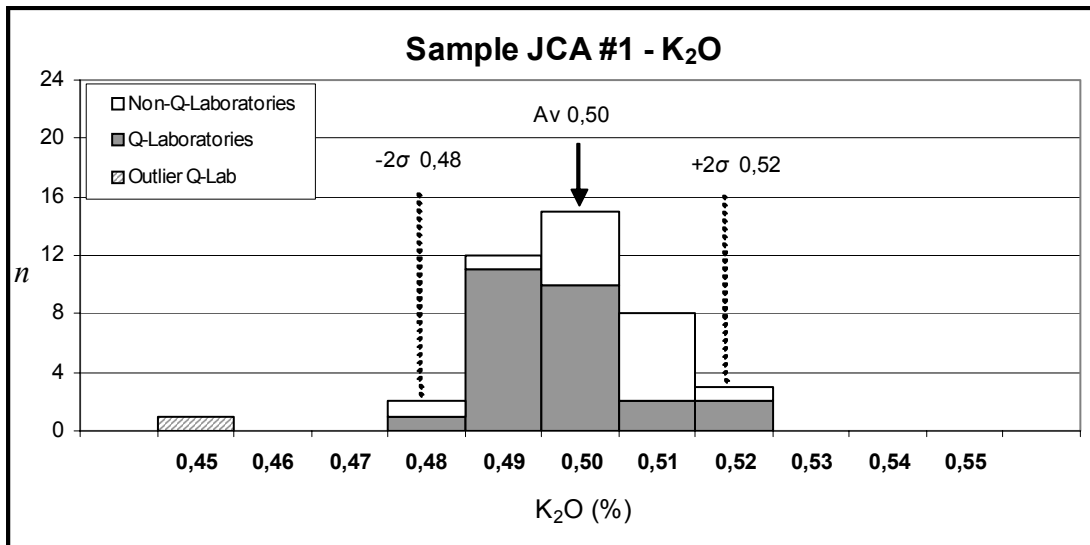


Figure 8 — The histogram of concentrations (Sample JCA #1, constituent K<sub>2</sub>O)

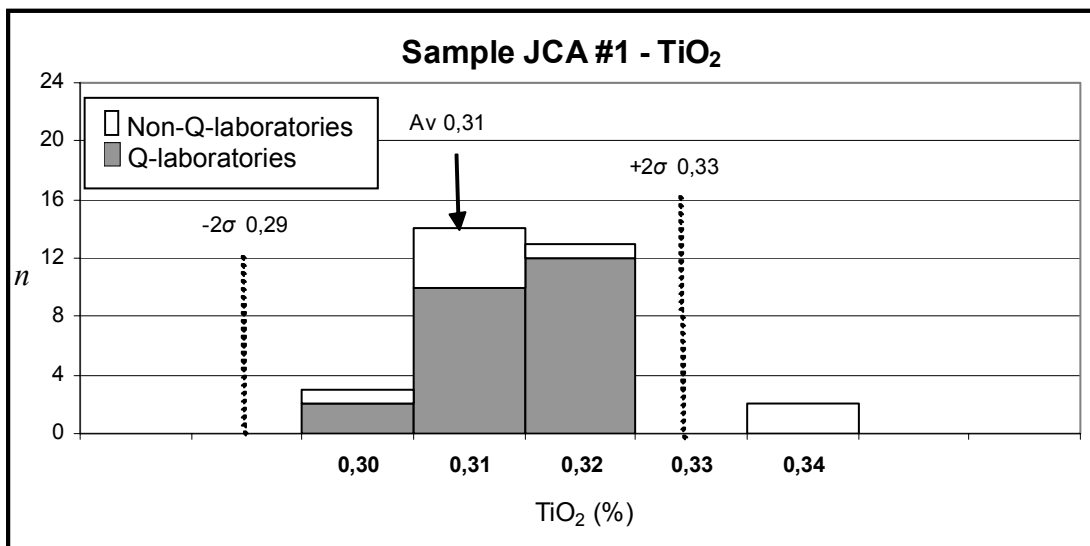


Figure 9 — The histogram of concentrations (Sample JCA #1, constituent TiO<sub>2</sub>)

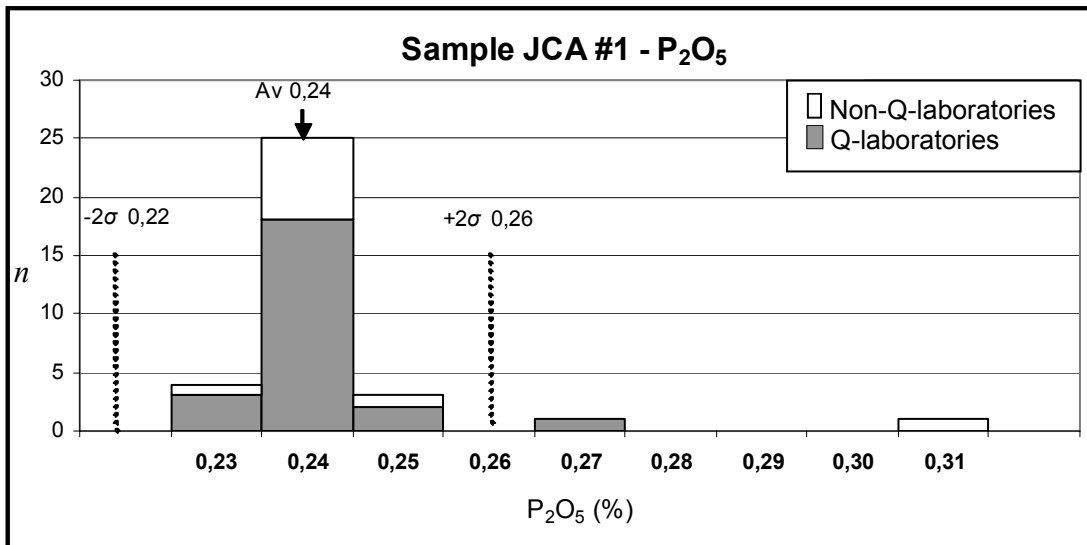


Figure 10 — The histogram of concentrations (Sample JCA #1, constituent P<sub>2</sub>O<sub>5</sub>)

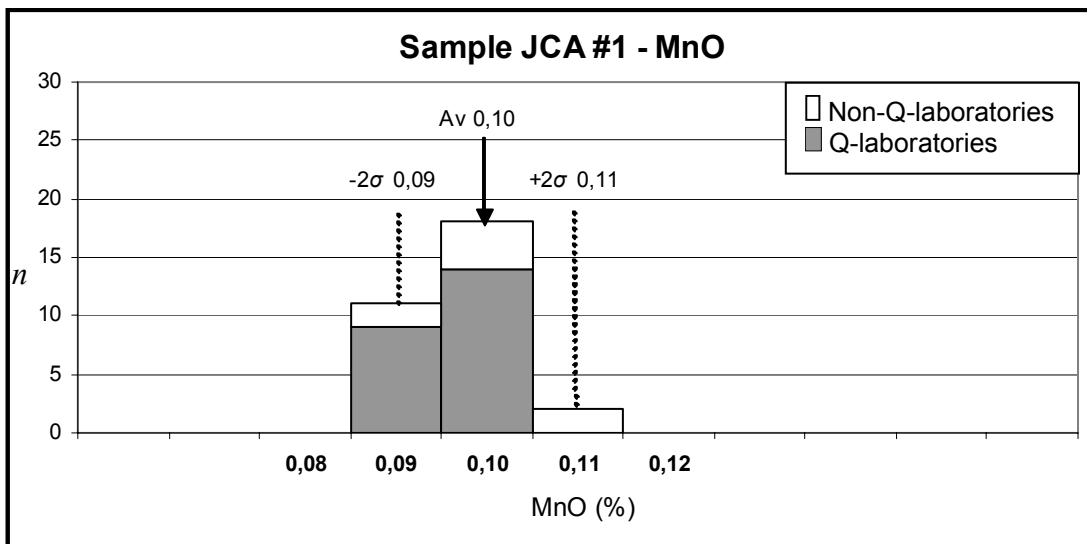


Figure 11 — The histogram of concentrations (Sample JCA #1 – constituent MnO)

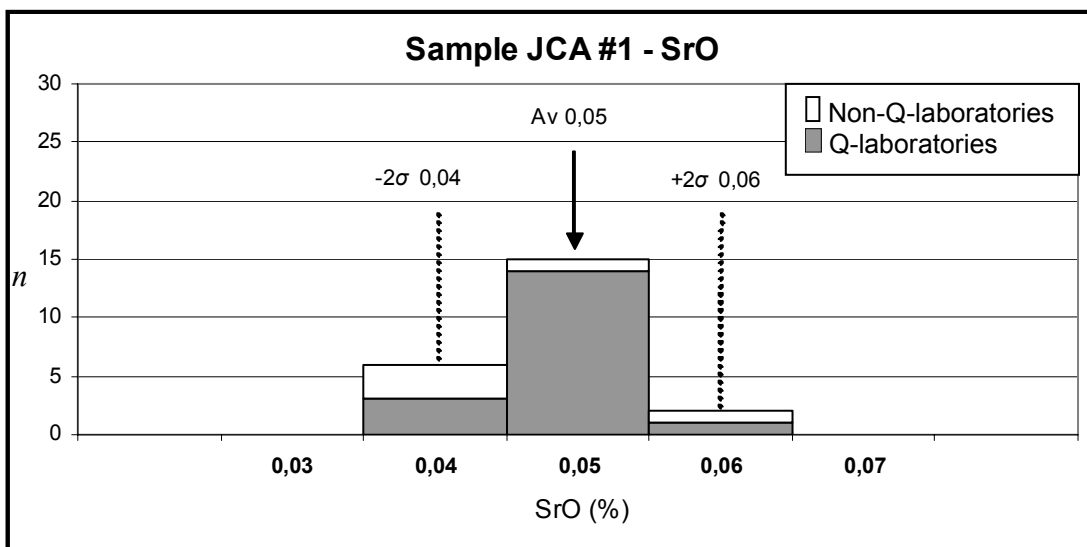


Figure 12 — The histogram of concentrations (Sample JCA #1, constituent SrO)

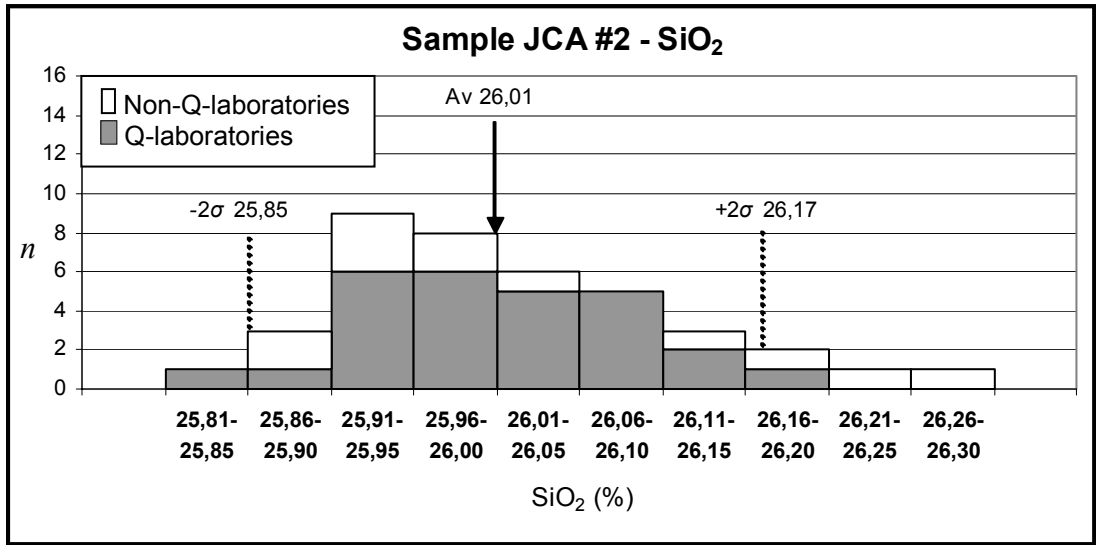


Figure 13 — The histogram of concentrations (Sample JCA #2, constituent SiO<sub>2</sub>)

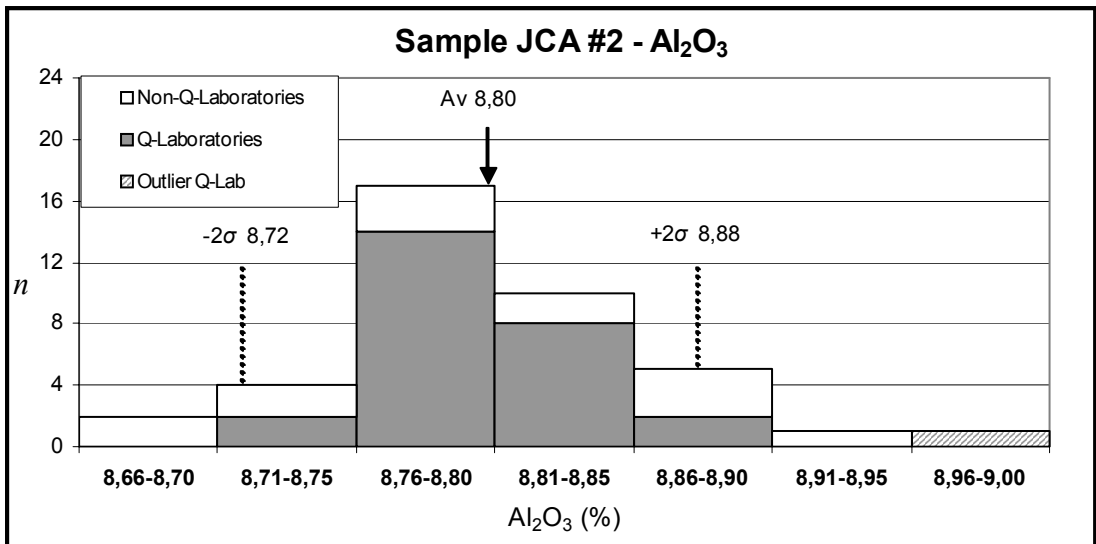


Figure 14 — The histogram of concentrations (Sample JCA #2, constituent Al<sub>2</sub>O<sub>3</sub>)

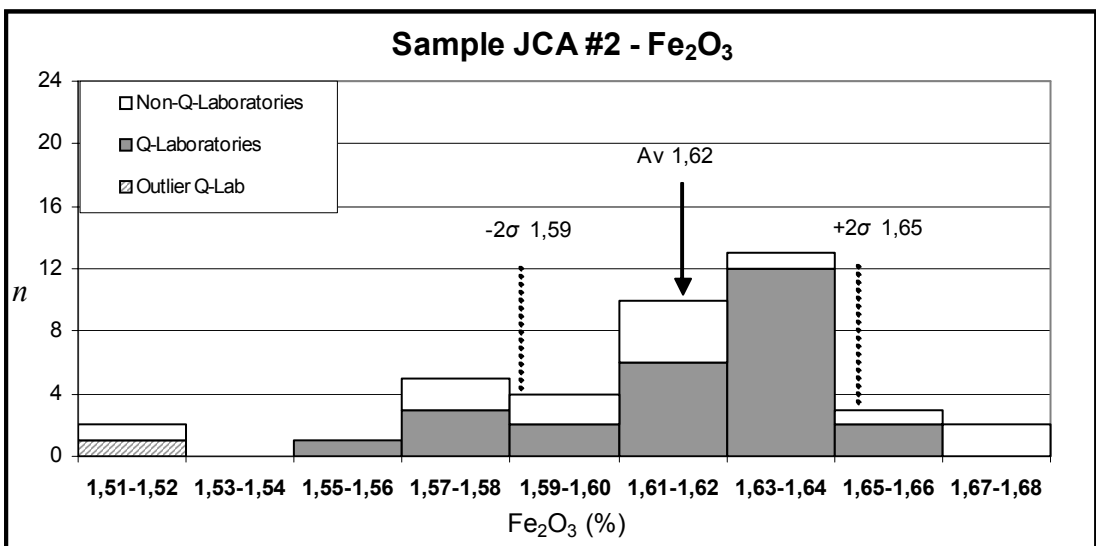


Figure 15 — The histogram of concentrations (Sample JCA #2, constituent Fe<sub>2</sub>O<sub>3</sub>)

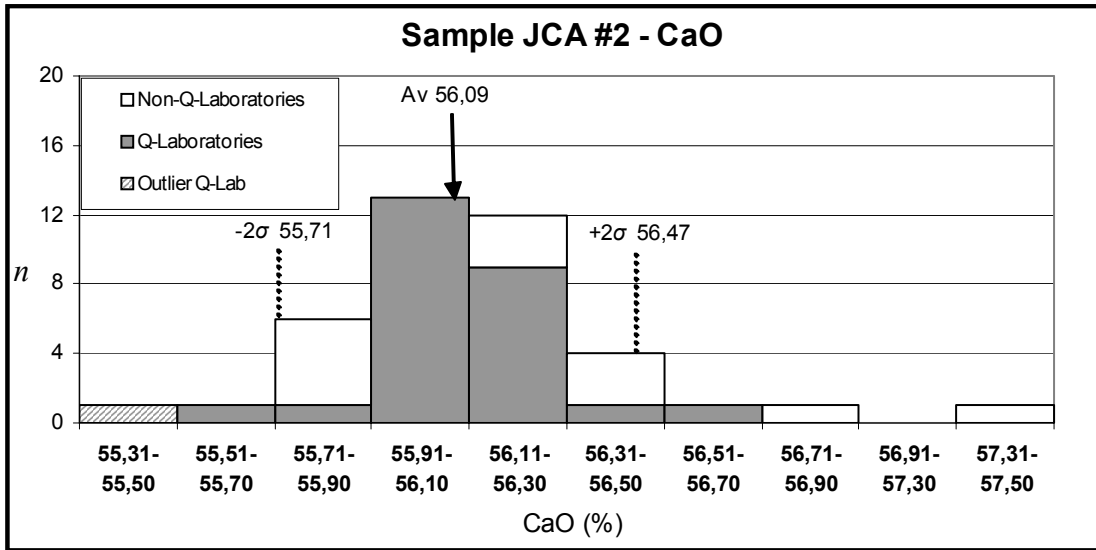


Figure 16 — The histogram of concentrations (Sample JCA #2, constituent CaO)

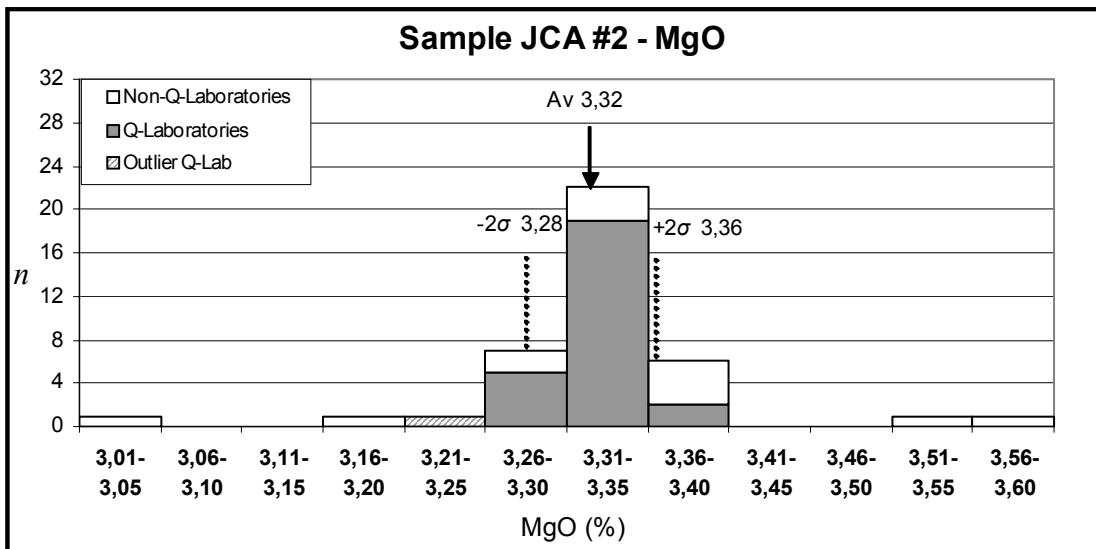


Figure 17 — The histogram of concentrations (Sample JCA #2, constituent MgO)

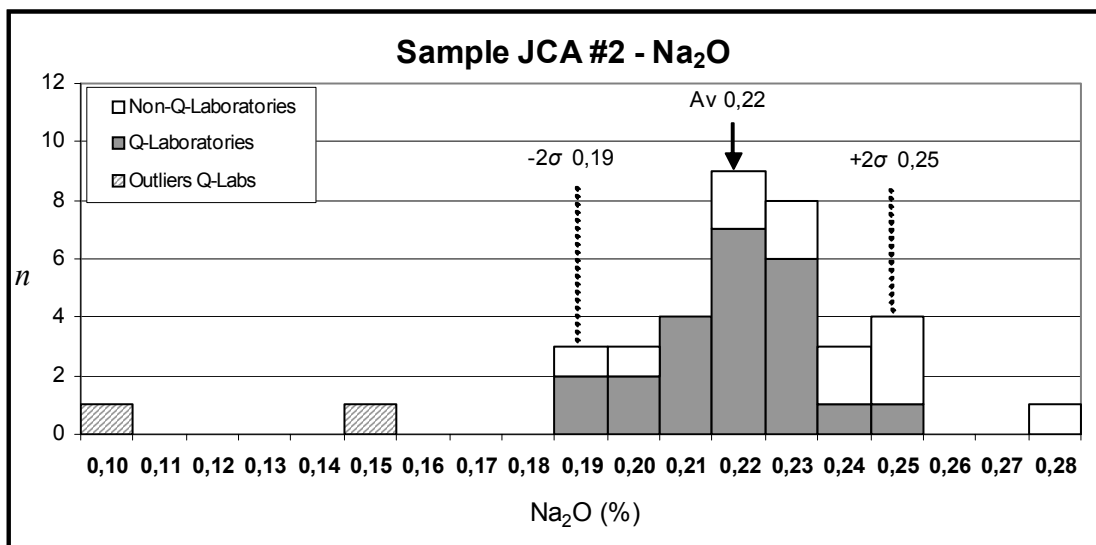


Figure 18 — The histogram of concentrations (Sample JCA #2, constituent Na<sub>2</sub>O)

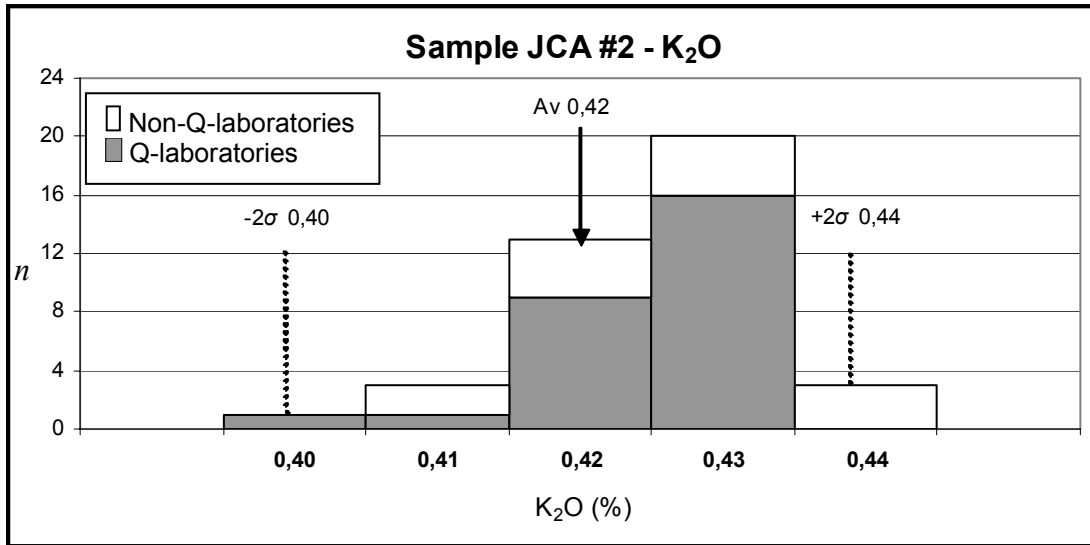


Figure 19 — The histogram of concentrations (Sample JCA #2, constituent K<sub>2</sub>O)

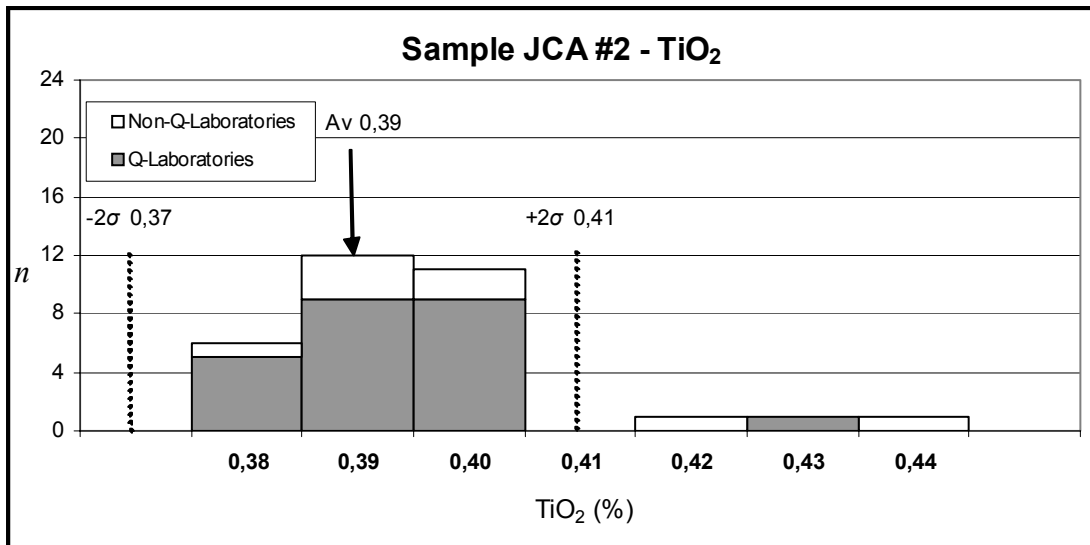


Figure 20 — The histogram of concentrations (Sample JCA #2, constituent TiO<sub>2</sub>)

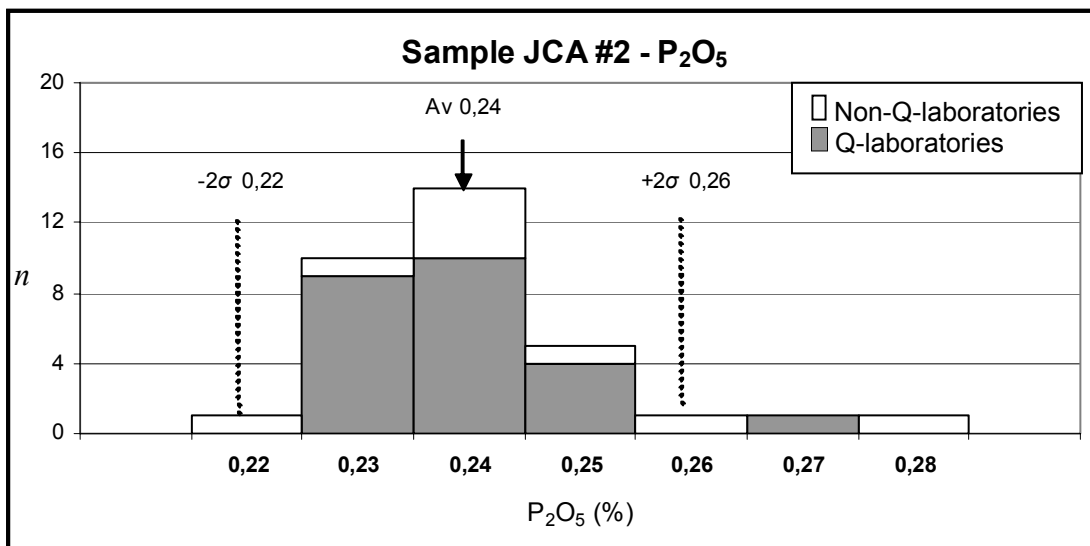


Figure 21 — The histogram of concentrations (Sample JCA #2, constituent P<sub>2</sub>O<sub>5</sub>)

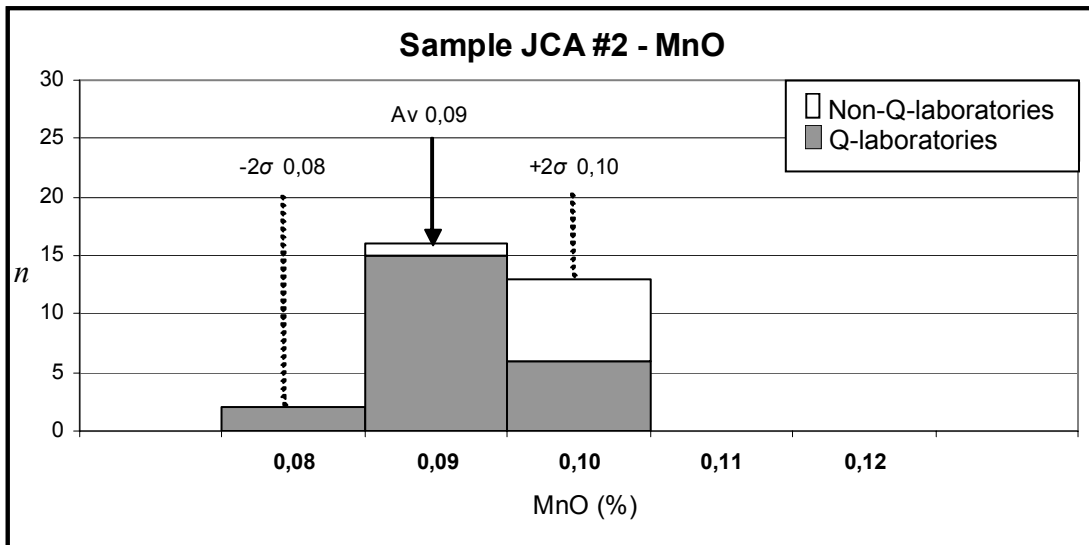


Figure 22 — The histogram of concentrations (Sample JCA #2, constituent MnO)

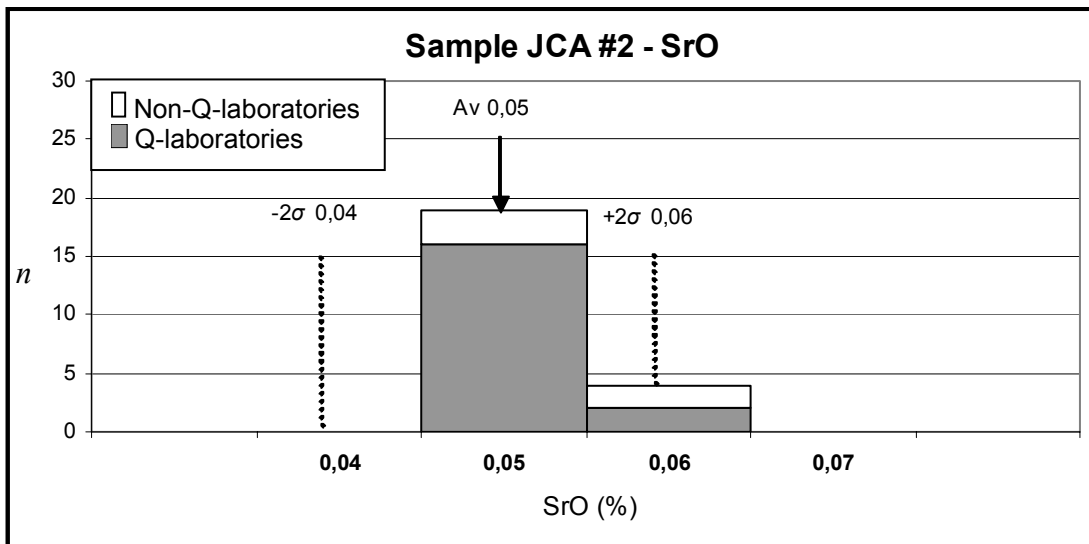


Figure 23 — The histogram of concentrations (Sample JCA #2, constituent SrO)

## 6 Conclusions

### 6.1 Result of test sample analyses

The average and the standard deviations of reproducibility of test samples obtained from the inter-laboratory testing by x-ray fluorescence are shown in Table 12.

For comparison, standard deviations of reproducibility obtained from the wet-chemistry methods in Inter-laboratory testing, 2004-OC in accordance with JIS R 5202 are also shown in Table 12.

Inter-laboratory testing, 2004-OC was conducted by the Japan Cement Association and the standard deviation of the reproducibility was calculated using only data from the laboratories of cement companies in Japan. Most of these laboratories participated in the inter-laboratory testing by x-ray fluorescence.

NOTE An "Inter-laboratory testing, xxxx-OC" has been conducted by the Japan Cement Association since 1948. "xxxx" stands for the year in which the inter-laboratory testing was conducted.

**Table 12 — Comparison between standard deviation obtained by Q-laboratories in this testing and that obtained from data of the wet method in Inter-laboratory testing, 2004-OC**

Constituent	Sample	Q-laboratories this inter-laboratory testing		Inter-laboratory testing 2004-OC	
		Average %	Reproducibility S.D. %	Reproducibility S.D. %	Number of laboratories
SiO <sub>2</sub>	Sample #1	20,96	0,078	0,129	22
	Sample #2	26,01	0,083		
Al <sub>2</sub> O <sub>3</sub>	Sample #1	5,10	0,021	0,068	22
	Sample #2	8,80	0,037		
Fe <sub>2</sub> O <sub>3</sub>	Sample #1	3,03	0,033	0,049	21
	Sample #2	1,62	0,025		
CaO	Sample #1	65,89	0,160	0,117	22
	Sample #2	56,09	0,192		
MgO	Sample #1	1,36	0,018	0,042	22
	Sample #2	3,32	0,024		
SO <sub>3</sub>	Sample #1	2,21	0,037	0,039	27
	Sample #2	(2,86) <sup>a</sup>	(0,121) <sup>a</sup>		
Na <sub>2</sub> O	Sample #1	0,21	0,019	0,014	23
	Sample #2	0,22	0,014		
K <sub>2</sub> O	Sample #1	0,50	0,009	0,009	23
	Sample #2	0,42	0,008		
TiO <sub>2</sub>	Sample #1	0,31	0,007	0,012	22
	Sample #2	0,39	0,010		
P <sub>2</sub> O <sub>5</sub>	Sample #1	0,24	0,008	0,027	22
	Sample #2	0,24	0,009		
MnO	Sample #1	0,10	0,005	0,007	22
	Sample #2	0,09	0,006		
SrO	Sample #1	0,05	0,005	-	-
	Sample #2	0,05	0,003		

<sup>a</sup> Concentrations in parentheses are the "outliers" by the Grubbs test.



The standard deviations of Q-laboratories are almost equal to or less than those of Inter-laboratory testing, 2004-OC, except for CaO. Therefore, the accuracy of XRF analysis according to the XRF method is considered to be generally equal to that of wet analysis.

For CaO, a few laboratories obtained results that are not within the average  $\pm 2$  times the standard deviation, even if the results are not "outliers". Factors affecting the determination of CaO should be investigated further.

As reported in 5.3.2, there are some "outliers", even in the analyses by Q-laboratories. The principle of the method assumes that extreme results should not arise, provided that the calibration used for sample analysis satisfied the criteria for both repeatability limits and accuracy limits. The possibility of error factors in these analyses should be investigated.

## 6.2 Factors affecting conformity with the validation criteria

The XRF method requires that, when analysing a sample by XRF analysis, it is necessary to satisfy the criteria for repeatability limits and accuracy limits for certified reference materials. This validation is essential for accurate analysis.

Some laboratories were unable to satisfy the validation criteria in this inter-laboratory testing.

In these cases, it is recommended that those laboratories re-check general matters for chemical analysis, such as weighing of samples, performance of spectrometer and general facilities for accurate XRF analysis.

The following matters should also be checked:

- a) bead preparation conditions, such as fusion temperature, flux-to-sample ratio;
- b) repeatability of bead preparation;
- c) procedure for preparing ignited sample;
- d) agreed basis for calculating results, e.g., as-received or loss-free;
- e) procedure for establishing calibration equations, such as range of contents or application of correction for inter-element effect;
- f) measurement conditions for light elements, especially Na<sub>2</sub>O, MgO and Al<sub>2</sub>O<sub>3</sub>.

## 6.3 Application to other international inter-laboratory testing

ISO 29581-2 is intended for use under everyday conditions in laboratories that operate to "good practice". Annex D sets out the results of some international round robins carried out by a large number of laboratories demonstrating the suitability of ISO 29581-2 as a means for comparing the everyday performance of laboratories.

## Annex A (informative)

### List of participating laboratories

#### A.1 Japanese laboratories:

Ube-Mitsubishi Cement Research Institute Corporation, Ube Center

Ube-Mitsubishi Cement Research Institute Corporation, Kurosaki Center

Ube-Mitsubishi Cement Research Institute Corporation, Saitama Center

Ube-Mitsubishi Cement Research Institute Corporation, Sendai Concrete Center

Nippon Steel Blast-Furnace Slag Cement Co., Ltd., Production and Technical Dept., Quality Assurance Group

Sumitomo Osaka Cement Co., Ltd., Production and Technical Dept., Analytical Center

Sumitomo Osaka Cement Co., Ltd., Cement/Concrete Research Laboratory, Cement Chemistry Research Group

Sumitomo Osaka Cement Co., Ltd., Cement/Concrete Research Laboratory, Cement Technology Group

Taiheiyo Cement Corporation, Ofunato Plant, Production Dept., Quality Assurance Section

Taiheiyo Cement Corporation, Kamiiso Plant, Production Dept., Quality Assurance Section

Taiheiyo Cement Corporation, Oita Plant(Saiki), Production Dept., Quality Assurance Section

Taiheiyo Consultant Co., Ltd., Quality Assurance Dept., Chemical Analysis Group

Chuken Consultant Co., Ltd., Kanto Branch, Technical Dev., Material Analytical Section

Tokuyama Corporation, Cement Manufacturing Dept., Technical Section 1

Tosoh Corporation, Cement and Energy Manufacturing Dept., Cement Testing Div.

Japan Cement Association, R & D Laboratory, Basic Research on Cement/Environment Group

#### A.2 ISO member laboratories – Outside Japan:

China, People's Republic of – China Building Materials Academy

Asia Cement Co., Ltd.

Hanil Cement Co., Ltd.

Hyundai Cement Co., Ltd., Danyang Plant

Hyundai Cement Co., Ltd., Yongwol Plant

Lafarge Halla Cement Corporation

	Ssangyong Cement Industrial Co., Ltd.
	Yongwol Plant
	Sungshin Cement Co., Ltd.
Korea, Republic of –	Tong Yang Cement Corporation, Samchok Plant
Lithuania, Republic of –	Prustitas Co., Ltd.
Philippines, Republic of the –	Cement Manufactures Association/APO Cement Corporation
	Union Cement Corporation, Lugait Plant
Vietnam, Socialist Republic of –	Butson Cement Company
	National Cement Association

### A.3 CEN member laboratories:

Italy –	Italcementi Group, Bergamo
France –	Three laboratories co-ordinated by ATILH, Paris
Germany –	VDZ, Research Institute of the Cement Industry, Duesseldorf
	HeidelbergCement Technology Center GmbH, Leimen
Belgium –	CRIC, Brussels
Turkey –	Turkish Cement Manufacturing Association, Ankara
United Kingdom –	Castle Cement Technical Centre, Clitheroe
Netherlands –	ENCI B.V. Vestiging, Maastricht
Spain –	IECA, Madrid
Czech Republic –	Research Institute for Binding Materials, Brno
Poland –	IMMB, Krakow

NOTE One CEN member laboratory was unable to meet the validation criteria and withdrew. It was subsequently discovered that the x-ray tube was unstable.

**Annex B**  
(informative)

**Individual results of all laboratories**

Tables B.1 to B.8 list the results of all laboratories participating in the test programme: Chemical analysis of cement by x-ray fluorescence.

**Table B.1 — Individual results for all laboratories — JCA-CRM-1**

Laboratory ref.	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> %	
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean
1	20,982 20,943	20,962	5,287 5,259	5,273	2,619 2,610	2,614	65,197 65,377	65,287	2,117 2,111	2,114	2,083 2,073	2,078
2	20,902 20,936	20,919	5,257 5,253	5,255	2,647 2,648	2,648	65,370 65,298	65,334	2,134 2,129	2,132	2,005 2,037	2,021
3	20,933 20,945	20,939	5,244 5,249	5,246	2,691 2,674	2,682	65,115 65,097	65,106	2,143 2,131	2,137	2,089 2,061	2,075
4	21,006 20,926	20,966	5,260 5,250	5,255	2,670 2,683	2,676	65,188 65,208	65,198	2,135 2,137	2,136	2,074 2,083	2,078
5	20,914 20,946	20,930	5,254 5,266	5,260	2,668 2,671	2,670	65,243 65,247	65,245	2,136 2,133	2,134	2,085 2,094	2,090
6	20,945 20,921	20,933	5,250 5,223	5,236	2,608 2,606	2,607	65,126 65,209	65,168	2,142 2,103	2,122	2,061 2,073	2,067
7	20,996 21,010	21,003	5,273 5,260	5,266	2,663 2,660	2,662	65,177 65,223	65,200	2,163 2,168	2,166	2,063 2,057	2,060
8	20,945 20,905	20,925	5,272 5,266	5,269	2,681 2,677	2,679	65,103 64,988	65,046	2,161 2,151	2,156	2,054 2,062	2,058
9	20,912 20,901	20,906	5,266 5,249	5,258	2,613 2,609	2,611	65,227 65,186	65,206	2,117 2,120	2,118	2,076 2,070	2,073
10	20,942 20,970	20,956	5,219 5,254	5,236	2,631 2,628	2,630	65,331 65,319	65,325	2,122 2,105	2,114	2,067 2,084	2,076
11	21,027 21,015	21,021	5,280 5,274	5,277	2,677 2,669	2,673	65,241 65,180	65,210	2,127 2,113	2,120	2,083 2,065	2,074
12	20,978 20,989	20,984	5,264 5,270	5,267	2,690 2,664	2,677	65,310 65,237	65,274	2,147 2,142	2,144	2,098 2,074	2,086
13	21,042 21,024	21,033	5,265 5,269	5,267	2,680 2,677	2,678	64,999 64,957	64,978	2,137 2,146	2,142	2,056 2,051	2,054
14	21,040 20,960	21,000	5,296 5,267	5,282	2,716 2,722	2,719	65,341 65,453	65,397	2,154 2,148	2,151	2,067 2,068	2,068
15	21,086 20,996	21,041	5,260 5,252	5,256	2,674 2,670	2,672	65,192 65,230	65,211	2,109 2,106	2,108	1,976 1,991	1,984
16	21,004 21,011	21,008	5,297 5,286	5,292	2,671 2,667	2,669	65,190 65,176	65,183	2,153 2,156	2,154	2,088 2,096	2,092
101	21,050 21,055	21,052	5,288 5,293	5,290	2,623 2,616	2,620	65,348 65,342	65,345	2,122 2,110	2,116	1,962 2,092	2,027
102	21,162 21,179	21,170	5,183 5,241	5,212	2,638 2,634	2,636	66,288 66,283	66,286	2,127 2,134	2,130	2,429 2,430	2,430
103	20,990 20,970	20,980	5,200 5,220	5,210	2,640 2,650	2,645	65,280 65,220	65,250	2,230 2,060	2,145	2,070 2,090	2,080
104	20,989 20,973	20,981	5,248 5,228	5,238	2,631 2,622	2,626	65,060 64,867	64,964	2,093 2,104	2,098	2,051 2,096	2,074
105	20,978 21,062	21,020	5,242 5,294	5,268	2,642 2,634	2,638	65,396 65,372	65,384	2,176 2,175	2,176	2,064 2,058	2,061

Table B.1 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %		Total
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	
1	0,272 0,257	0,264	0,541 0,548	0,544	0,344 0,344	0,344	0,287 0,286	0,286	0,069 0,069	0,069	- -	-	99,835
2	0,264 0,263	0,264	0,533 0,536	0,534	0,356 0,349	0,352	0,283 0,284	0,284	0,066 0,065	0,066	0,044 0,044	0,44	99,853
3	0,266 0,253	0,260	0,570 0,568	0,569	0,355 0,358	0,356	0,279 0,278	0,278	0,063 0,063	0,063	- -	-	99,711
4	0,260 0,258	0,259	0,560 0,564	0,562	0,358 0,354	0,356	0,288 0,286	0,287	0,063 0,063	0,063	0,043 0,043	0,043	99,879
5	0,262 0,263	0,262	0,560 0,563	0,562	0,357 0,355	0,356	0,283 0,284	0,284	0,064 0,064	0,064	0,044 0,044	0,044	99,901
6	0,265 0,276	0,270	0,581 0,588	0,584	0,341 0,349	0,345	0,287 0,285	0,286	0,066 0,064	0,065	0,042 0,042	0,042	99,725
7	0,253 0,255	0,254	0,566 0,564	0,565	0,359 0,354	0,356	0,282 0,282	0,282	0,065 0,064	0,064	0,044 0,044	0,044	99,922
8	0,244 0,251	0,248	0,562 0,561	0,562	0,352 0,344	0,348	0,283 0,282	0,282	0,061 0,061	0,061	0,043 0,043	0,043	99,677
9	0,264 0,265	0,264	0,575 0,574	0,574	0,345 0,347	0,346	0,285 0,286	0,286	0,069 0,069	0,069	0,041 0,041	0,041	99,752
10	0,232 0,239	0,236	0,568 0,567	0,568	0,347 0,350	0,348	0,281 0,281	0,281	0,069 0,069	0,069	- -	-	99,839
11	0,242 0,254	0,248	0,523 0,533	0,528	0,353 0,357	0,355	0,283 0,288	0,286	0,063 0,062	0,062	- -	-	99,854
12	0,264 0,271	0,268	0,572 0,570	0,571	0,346 0,357	0,352	0,285 0,285	0,285	0,063 0,066	0,064	0,043 0,044	0,044	100,016
13	0,264 0,266	0,265	0,559 0,559	0,559	0,354 0,358	0,356	0,291 0,291	0,291	0,064 0,063	0,064	0,044 0,044	0,044	99,731
14	0,267 0,269	0,268	0,586 0,568	0,577	0,341 0,328	0,334	0,302 0,292	0,297	0,064 0,065	0,064	0,045 0,045	0,045	100,202
15	0,274 0,272	0,273	0,560 0,559	0,560	0,354 0,348	0,351	0,291 0,291	0,291	0,064 0,065	0,064	0,043 0,042	0,042	99,853
16	0,263 0,255	0,259	0,577 0,576	0,576	0,351 0,356	0,354	0,284 0,282	0,283	0,063 0,063	0,063	0,043 0,043	0,043	99,976
101	0,229 0,223	0,226	0,569 0,573	0,571	0,347 0,344	0,346	0,288 0,285	0,286	- -	-	- -	-	99,879
102	- -	-	0,596 0,596	0,596	- -	-	- -	-	- -	-	- -	-	100,460
103	0,270 0,280	0,275	0,580 0,570	0,575	- -	-	- -	-	- -	-	- -	-	99,160
104	0,239 0,249	0,244	0,556 0,572	0,564	0,343 0,341	0,342	0,276 0,272	0,274	0,066 0,065	0,066	0,042 0,042	0,042	99,517
105	0,248 0,251	0,250	0,599 0,598	0,598	0,352 0,341	0,346	0,291 0,294	0,292	0,067 0,067	0,067	0,042 0,041	0,042	100,142

Table B.2 — Individual results for all laboratories — JCA-CRM-1

Laboratory ref.	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> %	
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean
106	20,890 21,008	20,949	5,251 5,265	5,258	2,673 2,675	2,674	65,088 65,178	65,133	2,123 2,125	2,124	2,058 2,072	2,065
107	21,055 21,061	21,058	5,526 5,315	5,420	2,687 2,695	2,691	64,449 64,494	64,472	2,167 2,134	2,150	2,055 2,023	2,039
108	20,91 20,90	20,905	5,25 5,26	5,255	2,62 2,61	2,615	65,18 65,16	65,170	2,11 2,10	2,105	2,07 2,06	2,065
109	20,992 20,960	20,976	5,256 5,265	5,260	2,636 2,622	2,629	65,555 65,439	65,497	2,109 2,112	2,110	1,939 1,954	1,946
110	20,852 20,974	20,913	5,202 5,301	5,252	2,581 2,640	2,610	65,154 65,113	65,134	2,302 2,041	2,172	1,925 2,061	1,993
111	20,94 20,90	20,920	4,97 5,00	4,985	2,62 2,63	2,625	64,67 64,68	64,675	2,39 2,37	2,380	2,00 2,00	2,000
112	20,95 21,06	21,005	5,86 5,87	5,865	2,58 2,58	2,580	64,78 64,76	64,770	2,10 2,01	2,055	1,81 1,80	1,805
113	22,960 22,990	22,975	5,260 5,230	5,245	2,650 2,640	2,645	65,210 65,360	65,285	2,070 1,980	2,025	2,080 2,050	2,065
114	21,33 21,98	21,655	5,09 5,27	5,180	2,94 2,84	2,890	65,45 66,07	65,760	2,16 1,85	2,005	2,30 2,17	2,235
E1	20,965 20,853	20,909	5,282 5,237	5,260	2,669 2,656	2,663	65,141 65,180	65,161	2,138 2,145	2,142	2,212 2,187	2,200
E2	20,790 20,803	20,797	5,269 5,322	5,296	2,601 2,609	2,605	65,080 64,919	65,000	2,104 2,123	2,114	2,078 2,057	2,068
E3	20,780 20,800	20,790	5,140 5,190	5,165	2,730 2,690	2,710	65,180 65,150	65,165	2,270 2,270	2,270	1,950 2,010	1,980
E4	20,947 20,913	20,930	5,269 5,281	5,275	2,658 2,649	2,654	65,025 64,987	65,006	2,174 2,168	2,171	2,033 2,036	2,035
E5	21,020 21,000	21,010	5,250 5,240	5,245	2,640 2,660	2,650	65,350 65,300	65,325	2,130 2,140	2,135	2,070 2,060	2,065
E6	20,963 20,927	20,945	5,213 5,252	5,233	2,680 2,683	2,682	65,112 65,205	65,159	2,151 2,154	2,153	2,104 2,146	2,125
E7	20,892 21,100	20,996	5,244 5,295	5,270	2,689 2,686	2,688	65,444 65,240	65,342	2,177 2,126	2,152	2,062 2,068	2,065
E8	20,852 20,937	20,895	5,250 5,286	5,268	2,576 2,578	2,577	65,140 65,126	65,133	2,142 2,138	2,140	2,062 2,069	2,066
E9	21,010 20,972	20,991	5,203 5,242	5,223	2,681 2,673	2,677	65,293 65,124	65,209	2,134 2,162	2,148	- -	-
E10	21,080 21,090	21,085	5,150 5,160	5,155	2,600 2,620	2,610	65,110 65,160	65,135	2,100 2,120	2,110	2,010 2,010	2,010
E11	20,753 20,756	20,755	5,263 5,268	5,266	2,670 2,663	2,667	65,528 65,518	65,523	2,157 2,178	2,168	1,989 1,991	1,990
E12	21,000 20,760	20,880	5,293 5,279	5,286	2,678 2,656	2,667	65,260 64,560	64,910	2,150 2,151	2,151	2,060 2,043	2,052

Table B.2 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %		Total
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	
106	0,282 0,265	0,274	0,569 0,566	0,568	- -	-	- -	-	- -	- -	- -	- -	99,045
107	0,247 0,252	0,250	0,563 0,557	0,560	- -	-	0,273 0,284	0,278	0,061 0,060	0,060	- -	- -	98,978
108	0,240 0,270	0,255	0,59 0,59	0,590	- -	-	0,28 0,28	0,280	- -	-	- -	- -	99,240
109	- -	-	0,569 0,571	0,570	- -	-	- -	-	- -	-	- -	- -	98,988
110	0,240 0,322	0,281	0,662 0,501	0,582	- -	-	0,276 0,298	0,287	- -	-	- -	- -	99,224
111	0,280 0,290	0,285	0,57 0,57	0,570	0,38 0,39	0,385	0,35 0,36	0,355	0,07 0,07	0,070	0,04 0,04	0,040	99,290
112	0,190 0,190	0,190	0,58 0,58	0,580	- -	-	- -	-	- -	-	- -	- -	98,850
113	0,260 0,250	0,255	0,580 0,580	0,580	0,350 0,350	0,350	0,280 0,290	0,285	0,070 0,070	0,070	0,040 0,040	0,040	101,820
114	0,710 0,710	0,710	0,54 0,54	0,540	- -	-	- -	-	- -	-	- -	- -	100,975
E1	0,253 0,262	0,258	0,565 0,563	0,564	0,351 0,357	0,354	0,292 0,292	0,292	0,062 0,062	0,062	0,044 0,044	0,044	99,906
E2	0,274 0,272	0,273	0,572 0,567	0,570	0,340 0,342	0,341	0,287 0,284	0,286	0,068 0,068	0,068	- -	- -	99,415
E3	0,260 0,260	0,260	0,550 0,550	0,550	0,350 0,350	0,350	0,300 0,290	0,295	0,070 0,070	0,070	0,050 0,050	0,050	99,655
E4	0,267 0,272	0,270	0,572 0,574	0,573	0,344 0,344	0,344	0,291 0,288	0,290	0,067 0,066	0,067	0,041 0,041	0,041	99,654
E5	0,270 0,260	0,265	0,570 0,580	0,575	0,340 0,350	0,345	0,260 0,290	0,275	0,070 0,070	0,070	0,040 0,040	0,040	100,000
E6	0,124 0,128	0,126	0,564 0,560	0,562	0,348 0,347	0,348	0,313 0,303	0,308	0,059 0,060	0,060	- -	- -	99,698
E7	0,270 0,278	0,274	0,561 0,567	0,564	0,361 0,351	0,356	0,281 0,286	0,284	0,063 0,062	0,063	0,054 0,053	0,054	100,105
E8	0,273 0,262	0,268	0,571 0,572	0,572	0,341 0,345	0,343	0,284 0,284	0,284	0,067 0,068	0,068	0,042 0,042	0,042	99,654
E9	0,251 0,260	0,256	0,562 0,563	0,563	0,332 0,343	0,338	- -	-	- -	-	- -	- -	97,403
E10	0,290 0,290	0,290	0,570 0,570	0,570	- -	-	- -	-	- -	-	- -	- -	98,965
E11	0,249 0,249	0,249	0,571 0,569	0,570	0,340 0,341	0,341	0,280 0,280	0,280	0,064 0,063	0,064	0,050 0,050	0,050	99,920
E12	0,263 0,243	0,253	0,572 0,561	0,566	0,355 0,348	0,352	0,288 0,281	0,285	0,071 0,070	0,071	- -	- -	99,471

Table B.3 — Individual results for all laboratories — JCA-CRM-2

Laboratory ref.	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> %	
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean
1	25,651	25,652	8,943	8,944	2,137	2,138	56,491	56,490	3,055	3,054	2,588	2,558
	25,652		8,944		2,140		56,489		3,053		2,557	
2	25,573	25,548	8,915	8,920	2,087	2,088	56,482	56,472	3,022	3,031	2,553	2,570
	25,522		8,925		2,088		56,462		3,040		2,586	
3	25,535	25,519	8,942	8,937	2,107	2,100	56,538	56,532	2,977	2,972	-	-
	25,503		8,932		2,094		56,525		2,968		-	
4	25,633	25,637	8,924	8,932	2,104	2,101	56,406	56,382	3,035	3,040	2,569	2,580
	25,641		8,940		2,098		56,359		3,045		2,590	
5	25,595	25,614	8,921	8,930	2,083	2,082	56,424	56,430	3,026	3,030	2,579	2,569
	25,633		8,940		2,082		56,436		3,035		2,559	
6	25,651	25,594	9,027	9,005	2,152	2,143	56,617	56,564	3,073	3,060	2,544	2,527
	25,538		8,983		2,134		56,512		3,048		2,510	
7	25,695	25,690	8,948	8,950	2,071	2,072	56,462	56,481	3,097	3,084	2,602	2,602
	25,686		8,951		2,072		56,500		3,071		2,603	
8	25,568	25,566	8,909	8,901	2,040	2,042	56,167	56,147	3,059	3,058	2,367	2,366
	25,563		8,893		2,043		56,127		3,056		2,366	
9	25,537	25,584	8,923	8,931	2,138	2,138	56,444	56,494	3,049	3,055	-	-
	25,631		8,939		2,139		56,545		3,061		-	
10	25,568	25,586	8,947	8,902	2,137	2,130	56,437	56,528	2,956	2,976	-	-
	25,603		8,856		2,122		56,620		2,996		-	
11	25,697	25,687	8,892	8,877	2,084	2,083	56,457	56,407	3,044	3,020	2,603	2,606
	25,677		8,862		2,082		56,357		2,997		2,608	
12	25,678	25,675	8,965	8,939	2,070	2,080	56,440	56,429	3,039	3,041	-	-
	25,672		8,913		2,090		56,418		3,043		-	
13	25,736	25,731	8,929	8,925	2,083	2,084	56,271	56,242	3,053	3,057	2,632	2,628
	25,726		8,921		2,086		56,213		3,061		2,624	
14	25,787	25,752	8,965	8,939	2,125	2,122	56,428	56,506	3,062	3,058	2,641	2,638
	25,716		8,913		2,119		56,584		3,053		2,635	
15	25,610	25,584	8,968	8,965	2,087	2,090	56,327	56,316	3,019	3,018	2,605	2,600
	25,558		8,962		2,092		56,306		3,018		2,596	
16	25,712	25,685	8,937	8,960	2,072	2,075	56,533	56,524	3,046	3,040	2,604	2,590
	25,658		8,983		2,078		56,514		3,035		2,577	
101	25,631	25,634	8,942	8,922	2,124	2,118	56,586	56,556	3,013	3,020	-	-
	25,636		8,903		2,113		56,526		3,026		-	
102	25,589	25,600	8,918	8,924	2,131	2,129	56,644	56,658	3,077	3,073	1,320	1,322
	25,611		8,929		2,127		56,673		3,069		1,323	
103	25,650	25,660	8,930	8,965	2,150	2,155	56,530	56,530	3,060	2,990	2,540	2,555
	25,670		9,000		2,160		56,530		2,920		2,570	
104	25,550	25,533	8,885	8,866	2,123	2,118	56,411	56,317	3,033	3,028	1,880	1,890
	25,516		8,846		2,113		56,223		3,024		1,900	
105	25,653	25,632	8,911	8,920	2,125	2,124	56,557	56,552	3,073	3,083	2,568	2,570
	25,610		8,930		2,123		56,547		3,093		2,571	



Table B.3 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %		Total
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	
1	0,273 0,268	0,270	0,309 0,315	0,312	0,505 0,504	0,504	0,074 0,074	0,074	0,162 0,162	0,162	- -	-	100,158
2	0,242 0,245	0,244	0,322 0,320	0,321	0,500 0,514	0,507	0,073 0,075	0,074	0,155 0,155	0,155	0,069 0,068	0,68	99,998
3	0,223 0,214	0,218	0,323 0,324	0,324	0,506 0,506	0,506	0,075 0,075	0,075	0,160 0,159	0,160	- -	-	97,343
4	0,240 0,237	0,238	0,320 0,317	0,318	0,506 0,506	0,506	0,076 0,075	0,076	0,151 0,154	0,152	0,065 0,065	0,065	100,027
5	0,241 0,240	0,240	0,320 0,321	0,320	0,504 0,502	0,503	0,075 0,075	0,075	0,155 0,155	0,155	0,069 0,069	0,069	100,017
6	0,246 0,234	0,240	0,320 0,313	0,316	0,515 0,508	0,512	0,074 0,072	0,073	0,155 0,155	0,155	0,066 0,066	0,066	100,255
7	0,231 0,231	0,231	0,322 0,323	0,322	0,502 0,504	0,503	0,074 0,073	0,074	0,154 0,154	0,154	0,068 0,068	0,068	100,231
8	0,234 0,234	0,234	0,323 0,323	0,323	0,496 0,503	0,500	0,075 0,076	0,076	0,157 0,158	0,158	0,063 0,063	0,063	99,434
9	0,252 0,254	0,253	0,310 0,312	0,311	0,504 0,500	0,502	0,074 0,074	0,074	0,163 0,162	0,162	0,065 0,065	0,065	97,569
10	0,232 0,221	0,226	0,324 0,326	0,325	0,508 0,505	0,506	0,074 0,074	0,074	0,158 0,159	0,158	- -	-	97,411
11	0,257 0,241	0,249	0,319 0,319	0,319	0,512 0,498	0,505	0,076 0,077	0,076	0,156 0,155	0,156	- -	-	99,985
12	0,236 0,250	0,243	0,330 0,326	0,328	0,504 0,510	0,507	0,076 0,076	0,076	0,157 0,156	0,156	0,063 0,064	0,064	97,538
13	0,241 0,243	0,242	0,320 0,320	0,320	0,503 0,508	0,506	0,080 0,080	0,080	0,152 0,152	0,152	0,069 0,069	0,069	100,036
14	0,252 0,244	0,248	0,329 0,325	0,327	0,492 0,478	0,485	0,094 0,079	0,086	0,153 0,156	0,154	0,070 0,071	0,070	100,385
15	0,253 0,247	0,250	0,320 0,322	0,321	0,521 0,518	0,520	0,081 0,082	0,082	0,155 0,155	0,155	0,065 0,065	0,065	99,966
16	0,244 0,239	0,242	0,310 0,312	0,311	0,504 0,501	0,502	0,075 0,075	0,075	0,155 0,154	0,154	0,066 0,067	0,066	100,224
101	0,217 0,200	0,208	0,323 0,324	0,324	0,506 0,505	0,506	0,074 0,074	0,074	- -	-	- -	-	97,362
102	- -	-	0,309 0,310	0,310	- -	-	- -	-	- -	-	- -	-	98,016
103	0,240 0,250	0,245	0,310 0,310	0,310	- -	-	- -	-	- -	-	- -	-	99,410
104	0,266 0,259	0,262	0,331 0,314	0,322	0,502 0,499	0,500	0,067 0,066	0,066	0,158 0,155	0,156	0,066 0,066	0,066	99,124
105	0,226 0,230	0,228	0,345 0,341	0,343	0,518 0,508	0,513	0,086 0,081	0,084	0,164 0,158	0,161	0,065 0,065	0,065	100,275

Table B.4 — Individual results for all laboratories — JCA-CRM-2

Laboratory ref.	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> %	
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean
106	25,547 25,490	25,518	8,962 8,917	8,940	2,047 2,090	2,068	56,510 56,617	56,564	3,009 3,024	3,016	- -	- -
107	25,510 25,631	25,570	8,944 8,930	8,937	2,033 2,081	2,057	56,456 56,468	56,462	2,885 2,870	2,878	- -	- -
108	25,870 25,620	25,745	8,980 8,920	8,950	2,130 2,130	2,130	56,770 56,520	56,645	3,050 3,030	3,040	2,570 2,540	2,555
109	25,752 25,698	25,725	8,996 8,973	8,984	2,154 2,141	2,148	56,542 56,485	56,514	3,076 3,074	3,075	2,454 2,430	2,442
110	25,663 25,641	25,652	8,940 8,821	8,880	2,082 2,064	2,073	56,482 56,620	56,551	3,054 3,091	3,072	1,910 1,932	1,921
111	25,280 25,340	25,310	8,650 8,600	8,625	2,110 2,100	2,105	56,340 56,270	56,305	3,230 3,260	3,245	1,260 1,280	1,270
112	- -	-	- -	-	- -	-	- -	-	- -	-	- -	- -
113	25,690 25,740	25,715	8,960 8,910	8,935	2,140 2,120	2,130	56,790 56,840	56,815	3,110 3,140	3,125	- -	- -
114	25,460 25,310	25,385	6,540 6,600	6,570	2,570 2,460	2,515	56,570 56,740	56,655	2,160 3,140	2,650	2,310 2,160	2,235
E1	25,667 25,635	25,651	8,914 8,919	8,917	2,082 2,079	2,081	56,470 56,398	56,434	3,030 3,040	3,035	2,385 2,384	2,385
E2	25,515 25,595	25,555	8,915 8,921	8,918	2,119 2,111	2,115	56,440 56,593	56,517	3,032 3,035	3,034	2,592 2,569	2,581
E3	25,330 25,370	25,350	8,700 8,730	8,715	2,130 2,100	2,115	56,330 56,370	56,350	3,210 3,200	3,205	2,540 2,500	2,520
E4	25,538 25,636	25,587	8,861 8,872	8,867	2,121 2,125	2,123	56,073 56,121	56,097	2,984 2,997	2,991	- -	- -
E5	25,630 25,670	25,650	8,940 8,920	8,930	2,100 2,100	2,100	56,210 56,250	56,230	3,030 3,030	3,030	- -	- -
E6	25,532 25,598	25,565	8,870 8,879	8,875	2,094 2,096	2,095	56,360 56,480	56,420	3,043 3,061	3,052	- -	- -
E7	25,769 25,808	25,789	8,930 8,881	8,906	2,094 2,095	2,095	56,416 56,491	56,454	3,059 3,025	3,042	2,698 2,716	2,618
E8	25,612 25,606	25,609	8,928 8,938	8,933	2,154 2,141	2,148	56,391 56,404	56,398	3,042 3,043	3,043	2,160 2,160	2,707
E9	25,724 25,639	25,682	8,919 8,869	8,894	2,091 2,116	2,104	56,434 56,643	56,539	3,041 3,075	3,058	- -	- -
E10	25,470 25,530	25,500	8,620 8,650	8,635	2,120 2,130	2,125	57,080 57,110	57,095	2,970 2,960	2,965	2,619 2,617	2,160
E11	25,519 25,472	25,496	8,989 8,996	8,993	2,137 2,137	2,137	57,040 57,038	57,039	3,125 3,089	3,107	2,503 2,504	2,504
E12	25,620 25,680	25,650	9,002 8,919	8,961	2,091 2,083	2,087	56,250 56,660	56,455	3,077 3,099	3,088	- -	- -

Table B.4 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %		Total
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	
106	0,253 0,251	0,252	0,328 0,329	0,328	- -	-	- -	-	- -	- -	- -	- -	96,686
107	0,252 0,261	0,256	0,332 0,337	0,334	- -	-	0,075 0,073	0,074	0,159 0,162	0,160	- -	- -	96,728
108	0,270 0,200	0,235	0,320 0,320	0,320	- -	-	0,080 0,070	0,075	- -	-	- -	- -	99,695
109	- -	-	0,307 0,317	0,312	- -	-	- -	-	- -	-	- -	- -	99,200
110	0,220 0,241	0,230	0,331 0,312	0,322	- -	-	0,086 0,078	0,082	- -	-	- -	- -	98,783
111	0,270 0,270	0,270	0,330 0,330	0,330	0,530 0,520	0,525	0,010 0,030	0,020	0,160 0,160	0,160	0,060 0,060	0,060	98,225
112	- -	-	- -	-	- -	-	- -	-	- -	-	- -	- -	-
113	0,240 0,230	0,235	0,330 0,320	0,325	0,510 0,500	0,505	0,080 0,080	0,080	0,160 0,160	0,160	0,060 0,060	0,060	98,085
114	0,660 0,660	0,660	0,280 0,270	0,275	- -	-	- -	-	- -	-	- -	- -	96,945
E1	0,249 0,248	0,249	0,323 0,326	0,325	0,498 0,504	0,501	0,075 0,080	0,078	0,156 0,156	0,156	0,068 0,068	0,068	99,877
E2	0,303 0,265	0,284	0,320 0,317	0,319	0,503 0,503	0,503	0,076 0,077	0,077	0,160 0,161	0,161	- -	- -	100,061
E3	0,240 0,240	0,240	0,310 0,310	0,310	0,490 0,490	0,490	0,080 0,080	0,080	0,180 0,180	0,180	0,080 0,080	0,080	99,635
E4	0,236 0,239	0,238	0,316 0,319	0,318	0,506 0,503	0,505	0,070 0,069	0,070	0,164 0,160	0,162	0,058 0,059	0,059	97,014
E5	0,220 0,240	0,230	0,310 0,320	0,315	0,500 0,510	0,505	0,070 0,070	0,070	0,160 0,160	0,160	0,070 0,080	0,075	97,295
E6	0,118 0,114	0,116	0,319 0,322	0,321	0,495 0,495	0,495	0,108 0,116	0,112	0,145 0,145	0,145	- -	- -	97,195
E7	0,256 0,240	0,248	0,317 0,318	0,318	0,497 0,502	0,500	0,075 0,077	0,076	0,156 0,156	0,156	0,082 0,080	0,081	100,280
E8	0,271 0,257	0,264	0,315 0,316	0,316	0,509 0,505	0,507	0,075 0,074	0,075	0,160 0,160	0,160	0,066 0,060	0,063	100,221
E9	- -	-	0,328 0,327	0,328	0,532 0,521	0,527	- -	-	- -	-	- -	- -	97,130
E10	0,260 0,260	0,260	0,340 0,340	0,340	- -	-	- -	-	- -	-	- -	- -	99,080
E11	0,238 0,228	0,233	0,329 0,329	0,329	0,503 0,505	0,504	0,079 0,080	0,080	0,157 0,157	0,157	0,075 0,075	0,075	100,652
E12	0,262 0,240	0,251	0,324 0,324	0,324	0,502 0,505	0,504	0,071 0,085	0,078	0,175 0,175	0,175	- -	- -	97,572

Table B.5 — Individual results for all laboratories — Sample JCA #1

Laboratory ref.	Loss on ignition	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> %	
		Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean
1	1,97	20,896	20,929	5,103	5,114	2,984	2,988	65,905	65,969	1,360	1,361	2,233	2,232
		20,962		5,124		2,992		66,033		1,362		2,231	
2	1,98	20,845	20,852	5,100	5,104	3,022	3,020	65,920	65,935	1,355	1,358	2,203	2,188
		20,860		5,108		3,019		65,986		1,360		2,173	
3	2,02	20,916	20,957	5,102	5,112	3,020	3,032	65,792	65,862	1,328	1,342	2,179	2,189
		20,998		5,123		3,043		65,931		1,355		2,199	
4	1,98	20,826	20,875	5,091	5,095	3,047	3,044	65,875	65,868	1,368	1,360	2,247	2,246
		20,924		5,099		3,040		65,860		1,352		2,246	
5	1,96	20,898	20,902	5,125	5,122	3,040	3,039	65,931	65,944	1,362	1,365	2,223	2,216
		20,906		5,119		3,038		65,958		1,368		2,209	
6	2,04	21,086	21,044	5,136	5,121	2,994	2,992	65,993	65,906	1,342	1,345	2,236	2,226
		21,001		5,106		2,989		65,818		1,348		2,217	
7	1,98	20,930	20,922	5,101	5,103	3,032	3,034	65,725	65,756	1,368	1,362	2,215	2,214
		20,914		5,105		3,035		65,787		1,355		2,214	
8	1,98	20,989	20,957	5,132	5,132	3,032	3,031	65,802	65,798	1,378	1,376	2,206	2,210
		20,925		5,131		3,030		65,795		1,373		2,213	
9	2,01	20,829	20,834	5,097	5,096	2,981	2,980	65,863	65,894	1,357	1,357	2,228	2,232
		20,839		5,096		2,978		65,925		1,357		2,235	
10	2,05	20,956	20,981	5,064	5,076	3,011	3,010	66,160	66,100	1,380	1,364	2,211	2,216
		21,006		5,088		3,010		66,040		1,349		2,221	
11	1,95	21,008	21,006	5,142	5,119	3,056	3,048	66,004	65,892	1,364	1,361	1,971	1,991
		21,003		5,096		3,039		65,780		1,358		2,011	
12	1,96	20,946	20,957	5,111	5,108	3,046	3,048	65,803	65,842	1,339	1,344	2,176	2,166
		20,968		5,105		3,050		65,882		1,349		2,156	
13	1,97	21,092	21,078	5,115	5,120	3,064	3,064	65,726	65,684	1,374	1,371	2,202	2,206
		21,064		5,125		3,063		65,643		1,368		2,209	
14	2,01	20,930	20,959	5,128	5,130	3,097	3,096	66,161	66,148	1,372	1,374	2,207	2,200
		20,988		5,131		3,094		66,135		1,376		2,193	
15	2,00	21,038	21,066	5,102	5,120	3,037	3,046	65,763	65,862	1,323	1,334	2,147	2,162
		21,094		5,137		3,055		65,962		1,345		2,177	
16	1,96	20,973	20,962	5,130	5,123	3,039	3,038	65,826	65,772	1,382	1,378	2,215	2,214
		20,951		5,116		3,037		65,718		1,374		2,212	
101	-	21,009	20,966	5,104	5,100	2,989	2,982	66,017	65,926	1,355	1,346	2,458	2,467
		20,924		5,095		2,976		65,836		1,338		2,476	
102	2,00	21,306	21,322	5,147	5,146	3,052	3,052	67,380	67,384	1,382	1,384	2,514	2,517
		21,338		5,145		3,053		67,387		1,386		2,520	
103	2,04	20,990	20,995	5,050	5,050	3,000	3,010	66,020	66,005	1,440	1,470	2,240	2,240
		21,000		5,050		3,020		65,990		1,500		2,240	
104	1,74	21,001	20,950	5,107	5,090	3,017	2,997	65,574	65,506	1,371	1,366	2,169	2,154
		20,899		5,072		2,977		65,439		1,361		2,140	
105	2,00	20,777	20,736	5,107	5,084	2,967	2,966	65,120	65,090	1,389	1,389	2,200	2,192
		20,694		5,062		2,965		65,061		1,389		2,185	

Table B.5 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %		Total
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	
1	0,214 0,202	0,208	0,463 0,444	0,454	0,308 0,310	0,309	0,241 0,242	0,242	0,097 0,097	0,097	- -	-	99,903
2	0,211 0,208	0,210	0,500 0,499	0,500	0,314 0,316	0,315	0,241 0,237	0,239	0,096 0,094	0,095	0,048 0,048	0,048	99,882
3	0,191 0,188	0,190	0,499 0,500	0,500	0,320 0,315	0,318	0,232 0,233	0,232	0,094 0,094	0,094	- -	-	99,828
4	0,213 0,205	0,209	0,496 0,504	0,500	0,320 0,326	0,323	0,239 0,242	0,240	0,095 0,096	0,096	0,048 0,047	0,048	99,904
5	0,210 0,211	0,210	0,491 0,490	0,490	0,316 0,316	0,316	0,238 0,239	0,238	0,096 0,096	0,096	0,049 0,049	0,049	99,987
6	0,236 0,218	0,227	0,521 0,510	0,516	0,317 0,311	0,314	0,244 0,243	0,244	0,092 0,092	0,092	0,045 0,045	0,045	100,072
7	0,205 0,200	0,202	0,494 0,494	0,494	0,319 0,319	0,319	0,238 0,237	0,238	0,096 0,097	0,096	0,048 0,048	0,048	99,788
8	0,193 0,193	0,193	0,495 0,493	0,494	0,318 0,315	0,316	0,237 0,238	0,238	0,092 0,095	0,094	0,046 0,046	0,046	99,885
9	0,209 0,209	0,209	0,504 0,505	0,504	0,307 0,310	0,308	0,238 0,241	0,240	0,097 0,097	0,097	0,044 0,044	0,044	99,795
10	0,170 0,170	0,170	0,499 0,499	0,500	0,317 0,317	0,316	0,247 0,237	0,242	0,097 0,097	0,097	- -	-	100,079
11	0,194 0,193	0,194	0,522 0,515	0,518	0,320 0,315	0,318	0,236 0,239	0,238	0,097 0,095	0,096	- -	-	99,781
12	0,205 0,208	0,206	0,484 0,486	0,485	0,317 0,323	0,320	0,235 0,235	0,235	0,091 0,091	0,091	0,053 0,054	0,054	99,856
13	0,212 0,214	0,213	0,493 0,494	0,494	0,313 0,312	0,312	0,246 0,245	0,246	0,094 0,095	0,094	0,049 0,049	0,049	99,931
14	0,213 0,213	0,213	0,493 0,492	0,492	0,300 0,309	0,304	0,246 0,247	0,246	0,095 0,095	0,095	0,050 0,050	0,050	100,307
15	0,187 0,176	0,182	0,490 0,493	0,492	0,311 0,314	0,312	0,244 0,246	0,245	0,097 0,095	0,096	0,047 0,047	0,047	99,964
16	0,205 0,211	0,208	0,503 0,506	0,504	0,319 0,318	0,318	0,240 0,236	0,238	0,093 0,094	0,094	0,048 0,048	0,048	99,897
101	0,162 0,142	0,152	0,500 0,499	0,500	0,311 0,308	0,310	0,239 0,235	0,237	- -	-	- -	-	99,986
102	- -	-	0,517 0,515	0,516	- -	-	- -	-	- -	-	- -	-	101,321
103	0,260 0,260	0,260	0,510 0,510	0,510	- -	-	- -	-	- -	-	- -	-	99,540
104	0,135 0,130	0,132	0,503 0,484	0,494	0,313 0,306	0,310	0,234 0,230	0,232	0,092 0,093	0,092	0,044 0,044	0,044	99,367
105	0,215 0,215	0,218	0,508 0,508	0,510	0,309 0,309	0,310	0,240 0,233	0,237	0,096 0,094	0,095	0,043 0,043	0,043	99,870

Table B.6 — Individual results for all laboratories — Sample JCA #1

Laboratory ref.	Loss on ignition	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> %	
		Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean
106	2,06	20,512 20,429	20,470	5,058 5,051	5,054	2,979 2,968	2,974	64,670 64,542	64,606	1,334 1,335	1,334	2,180 2,155	2,168
107	2,02	21,354 21,305	21,330	5,367 5,356	5,362	3,173 3,142	3,158	66,389 66,335	66,362	1,438 1,459	1,448	2,255 2,224	2,240
108	1,95	21,000 21,020	21,010	5,120 5,120	5,120	3,000 3,000	3,000	65,910 65,850	65,880	1,360 1,370	1,365	2,220 2,230	2,225
109	2,00	20,783 20,817	20,800	5,065 5,065	5,065	2,998 2,995	2,996	65,852 65,905	65,878	1,346 1,354	1,350	2,113 2,101	2,107
110	-	20,590 20,631	20,610	4,781 4,941	4,861	2,930 2,973	2,952	65,161 65,083	65,122	1,292 1,351	1,322	2,211 2,170	2,190
111	-	20,730 20,710	20,720	4,770 4,760	4,765	2,980 2,970	2,975	64,690 64,700	64,695	1,680 1,740	1,710	2,060 2,040	2,050
112	-	20,860 20,900	20,880	5,650 5,710	5,680	2,920 2,920	2,920	64,820 65,000	64,910	1,300 1,280	1,290	1,990 1,850	1,920
113	2,03	20,780 20,850	20,815	5,160 5,110	5,135	3,010 3,030	3,020	65,400 65,540	65,470	1,440 1,420	1,430	2,230 2,160	2,195
114	-	20,690 21,340	21,015	5,020 5,210	5,115	3,220 3,450	3,335	66,110 66,580	66,345	1,080 1,010	1,045	2,380 2,310	2,345
E1	-	20,882 20,905	20,894	5,147 5,087	5,117	3,029 3,050	3,040	65,821 65,898	65,860	1,353 1,368	1,361	2,308 2,295	2,302
E2	2,00	20,814 20,886	20,850	5,111 5,103	5,107	2,995 3,013	3,004	65,725 65,924	65,825	1,361 1,361	1,361	2,230 2,214	2,222
E3	-	20,950 21,020	20,985	5,040 5,030	5,035	3,120 3,130	3,125	66,280 66,180	66,230	1,450 1,460	1,455	2,110 2,110	2,110
E4	-	20,903 20,982	20,943	5,085 5,105	5,095	2,992 2,995	2,994	65,675 65,741	65,708	1,303 1,296	1,300	2,193 2,219	2,206
E5	1,96	21,070 21,050	21,060	5,100 5,040	5,070	3,010 3,020	3,015	65,940 66,060	66,000	1,410 1,360	1,385	2,220 2,220	2,220
E6	2,12	21,087 21,111	21,099	5,105 5,088	5,097	3,076 3,087	3,082	66,274 66,463	66,369	1,376 1,372	1,374	2,235 2,250	2,243
E7	2,02	20,918 20,798	20,858	5,076 5,108	5,092	3,088 3,069	3,079	65,865 65,793	65,828	1,385 1,351	1,368	2,228 2,208	2,218
E8	2,07	20,929 20,910	20,920	5,113 5,092	5,103	2,992 2,975	2,984	65,865 65,956	65,911	1,380 1,359	1,370	2,217 2,215	2,216
E9	1,94	21,054 20,966	21,010	5,152 5,102	5,127	3,031 3,040	3,036	65,981 65,843	65,912	1,344 1,350	1,347	- -	-
E10	-	20,600 20,630	20,615	5,000 5,000	5,000	2,960 2,970	2,965	65,680 65,720	65,700	1,370 1,370	1,370	2,220 2,220	2,220
E11	2,04	20,737 20,831	20,784	5,094 5,118	5,106	3,019 3,019	3,019	66,257 66,333	66,295	1,434 1,434	1,434	2,160 2,158	2,159
E12	1,99	21,050 20,860	20,955	5,118 5,089	5,104	3,037 3,029	3,033	65,980 65,460	65,720	1,357 1,354	1,356	2,221 2,191	2,206

Table B.6 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %		Total
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	
106	0,201 0,205	0,203	0,491 0,489	0,490	- -	-	- -	-	- -	- -	- -	- -	97,299
107	0,265 0,275	0,270	0,510 0,510	0,510	- -	-	0,237 0,237	0,237	0,081 0,091	0,086	- -	- -	101,003
108	0,130 0,130	0,130	0,490 0,490	0,490	- -	-	0,240 0,240	0,240	- -	-	- -	- -	99,460
109	- -	-	0,504 0,497	0,500	- -	-	- -	-	- -	-	- -	- -	98,696
110	0,243 0,220	0,232	0,490 0,511	0,500	- -	-	0,230 0,238	0,234	- -	-	- -	- -	98,023
111	0,250 0,260	0,255	0,500 0,500	0,500	0,350 0,340	0,345	0,320 0,300	0,310	0,100 0,100	0,100	0,040 0,040	0,040	98,465
112	0,230 0,230	0,230	0,510 0,510	0,510	- -	-	- -	-	- -	-	- -	- -	98,340
113	0,210 0,200	0,205	0,510 0,510	0,510	0,340 0,340	0,340	0,240 0,240	0,240	0,100 0,100	0,100	0,040 0,040	0,040	99,500
114	0,640 0,650	0,645	0,440 0,420	0,430	- -	-	- -	-	- -	-	- -	- -	100,275
E1	0,195 0,206	0,201	0,493 0,496	0,495	0,326 0,313	0,320	0,241 0,248	0,245	0,095 0,096	0,096	0,048 0,049	0,049	99,975
E2	0,208 0,207	0,208	0,498 0,499	0,499	0,312 0,311	0,312	0,240 0,236	0,238	0,097 0,097	0,097	- -	- -	99,721
E3	0,220 0,220	0,220	0,480 0,470	0,475	0,310 0,310	0,310	0,250 0,250	0,250	0,110 0,110	0,110	0,060 0,060	0,060	100,365
E4	0,234 0,228	0,231	0,490 0,494	0,492	0,305 0,307	0,306	0,238 0,238	0,238	0,092 0,092	0,092	0,052 0,056	0,054	99,658
E5	0,234 0,234	0,234	0,510 0,500	0,505	0,315 0,303	0,309	0,234 0,222	0,228	0,102 0,098	0,100	0,046 0,047	0,047	100,173
E6	0,105 0,101	0,103	0,496 0,497	0,496	0,313 0,315	0,314	0,273 0,269	0,271	0,090 0,091	0,090	- -	- -	100,538
E7	0,214 0,211	0,213	0,495 0,499	0,497	0,318 0,319	0,319	0,244 0,233	0,239	0,099 0,100	0,100	0,061 0,063	0,062	99,871
E8	0,204 0,215	0,210	0,501 0,502	0,502	0,309 0,305	0,307	0,240 0,238	0,239	0,096 0,096	0,096	0,045 0,045	0,045	99,900
E9	0,258 0,271	0,265	0,501 0,511	0,506	0,308 0,296	0,302	- -	-	- -	-	- -	- -	97,504
E10	0,220 0,210	0,215	0,510 0,510	0,510	- -	-	- -	-	- -	-	- -	- -	98,595
E11	0,202 0,201	0,202	0,496 0,497	0,497	0,302 0,303	0,303	0,237 0,235	0,236	0,093 0,093	0,093	0,054 0,054	0,054	100,181
E12	0,227 0,186	0,207	0,496 0,490	0,493	0,317 0,315	0,316	0,234 0,243	0,239	0,107 0,104	0,106	- -	- -	99,732

Table B.7 — Individual results for all laboratories — Sample JCA #2

Laboratory ref.	Loss on ignition	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> %	
		Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean
1	0,09	26,015	26,022	8,827	8,832	1,623	1,624	56,064	56,026	3,340	3,339	2,901	2,898
		26,029		8,838		1,625		55,987		3,338		2,895	
2	0,21	25,839	25,826	8,768	8,765	1,629	1,626	56,130	56,141	3,318	3,309	2,903	2,905
		25,812		8,762		1,623		56,152		3,300		2,907	
3	0,63	25,987	25,994	8,816	8,816	1,556	1,558	56,244	56,250	3,288	3,291	-	-
		26,002		8,816		1,561		56,257		3,294		-	
4	0,18	25,990	25,998	8,781	8,784	1,643	1,646	55,904	55,896	3,325	3,322	2,920	2,916
		26,005		8,786		1,648		55,887		3,320		2,912	
5	0,19	25,955	25,946	8,805	8,801	1,624	1,622	56,205	56,164	3,310	3,312	2,879	2,888
		25,936		8,797		1,621		56,122		3,314		2,897	
6	0,12	26,196	26,163	8,986	8,984	1,638	1,627	56,229	56,204	3,382	3,376	2,857	2,831
		26,130		8,983		1,616		56,179		3,371		2,805	
7	0,11	25,999	25,992	8,820	8,823	1,607	1,607	56,058	56,059	3,359	3,352	2,949	2,948
		25,984		8,826		1,607		56,060		3,345		2,947	
8	0,14	26,014	26,044	8,774	8,774	1,509	1,510	55,662	55,629	3,345	3,344	2,682	2,684
		26,075		8,775		1,510		55,636		3,343		2,685	
9	0,16	25,913	25,907	8,773	8,766	1,627	1,628	56,014	56,009	3,320	3,322	2,890	2,888
		25,901		8,760		1,629		56,004		3,324		2,887	
10	0,30	25,979	25,938	8,766	8,774	1,628	1,627	56,191	56,089	3,286	3,292	2,898	2,903
		25,898		8,782		1,626		55,987		3,297		2,908	
11	0,14	25,942	25,908	8,683	8,716	1,621	1,614	56,137	56,077	3,272	3,280	2,704	2,723
		25,875		8,748		1,606		56,017		3,289		2,742	
12	0,12	26,048	26,028	8,771	8,794	1,594	1,580	56,012	55,954	3,343	3,330	-	-
		26,009		8,816		1,566		55,897		3,316		-	
13	0,11	26,099	26,104	8,861	8,829	1,625	1,628	55,848	55,902	3,312	3,316	2,958	2,964
		26,110		8,797		1,632		55,957		3,319		2,971	
14	0,12	26,111	26,064	8,832	8,812	1,637	1,640	56,077	56,108	3,313	3,312	2,978	2,972
		26,017		8,792		1,643		56,138		3,312		2,965	
15	0,08	26,152	26,150	8,879	8,867	1,634	1,636	55,843	55,820	3,316	3,296	2,906	2,926
		26,149		8,855		1,638		55,796		3,276		2,945	
16	0,11	26,025	26,018	8,791	8,800	1,611	1,612	56,236	56,211	3,308	3,316	2,946	2,934
		26,012		8,809		1,612		56,186		3,323		2,922	
101	-	26,035	26,024	8,786	8,780	1,613	1,610	56,202	56,188	3,306	3,300	2,515	2,454
		26,012		8,773		1,608		56,175		3,295		2,392	
102	0,08	25,904	25,922	8,750	8,736	1,597	1,596	56,245	56,258	3,339	3,344	1,619	1,618
		25,941		8,721		1,596		56,270		3,348		1,617	
103	0,13	26,010	25,990	8,790	8,805	1,640	1,645	56,020	56,020	3,430	3,405	2,890	2,895
		25,970		8,820		1,650		56,020		3,380		2,900	
104	0,00	25,998	25,979	8,766	8,777	1,638	1,632	56,102	56,080	3,310	3,307	1,814	1,796
		25,960		8,788		1,627		56,057		3,304		1,778	
105	0,11	26,149	26,162	8,796	8,818	1,620	1,624	56,355	56,368	3,363	3,372	2,911	2,904
		26,174		8,841		1,628		56,380		3,380		2,897	



Table B.7 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %		Total
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	
1	0,254 0,254	0,254	0,400 0,397	0,398	0,398 0,397	0,398	0,237 0,237	0,237	0,098 0,098	0,098	- -	-	100,126
2	0,230 0,228	0,229	0,429 0,428	0,428	0,387 0,393	0,390	0,235 0,236	0,236	0,089 0,089	0,089	0,050 0,051	0,050	99,994
3	0,206 0,209	0,208	0,431 0,431	0,431	0,402 0,400	0,401	0,238 0,238	0,238	0,096 0,096	0,096	- -	-	97,283
4	0,218 0,218	0,218	0,417 0,417	0,417	0,390 0,393	0,392	0,242 0,240	0,241	0,087 0,086	0,086	0,049 0,049	0,049	99,965
5	0,216 0,215	0,216	0,432 0,430	0,431	0,387 0,388	0,388	0,239 0,237	0,238	0,088 0,088	0,088	0,051 0,050	0,050	100,144
6	0,195 0,191	0,193	0,423 0,424	0,424	0,393 0,389	0,391	0,234 0,228	0,231	0,090 0,090	0,090	0,051 0,051	0,051	100,565
7	0,212 0,210	0,211	0,431 0,432	0,432	0,393 0,389	0,391	0,238 0,237	0,238	0,086 0,087	0,086	0,050 0,050	0,050	100,189
8	0,223 0,217	0,220	0,426 0,425	0,426	0,401 0,403	0,402	0,237 0,238	0,238	0,094 0,094	0,094	0,050 0,050	0,050	99,415
9	0,230 0,230	0,230	0,413 0,413	0,413	0,396 0,399	0,398	0,234 0,233	0,234	0,098 0,099	0,098	0,052 0,052	0,052	99,945
10	0,206 0,213	0,210	0,429 0,429	0,429	0,400 0,400	0,400	0,234 0,235	0,234	0,095 0,096	0,096	- -	-	99,992
11	0,192 0,200	0,196	0,421 0,423	0,422	0,379 0,384	0,382	0,241 0,242	0,242	0,090 0,089	0,090	- -	-	99,650
12	0,225 0,229	0,227	0,414 0,419	0,416	0,398 0,392	0,395	0,230 0,231	0,230	0,086 0,085	0,086	0,058 0,057	0,058	97,098
13	0,216 0,217	0,216	0,428 0,431	0,430	0,408 0,396	0,402	0,244 0,247	0,246	0,084 0,084	0,084	0,051 0,051	0,051	100,172
14	0,216 0,214	0,215	0,433 0,433	0,433	0,380 0,379	0,380	0,248 0,247	0,248	0,086 0,086	0,086	0,051 0,051	0,051	100,321
15	0,196 0,204	0,200	0,431 0,434	0,432	0,384 0,382	0,383	0,246 0,246	0,246	0,088 0,088	0,088	0,048 0,048	0,048	100,092
16	0,213 0,221	0,217	0,422 0,424	0,423	0,378 0,385	0,382	0,241 0,239	0,240	0,088 0,087	0,088	0,049 0,049	0,049	100,290
101	0,197 0,190	0,194	0,426 0,430	0,428	0,395 0,395	0,395	0,238 0,238	0,238	- -	-	- -	-	99,611
102	- -	-	0,425 0,427	0,426	- -	-	- -	-	- -	-	- -	-	97,900
103	0,250 0,250	0,250	0,420 0,410	0,415	- -	-	- -	-	- -	-	- -	-	99,425
104	0,199 0,189	0,194	0,433 0,417	0,425	0,392 0,389	0,390	0,229 0,222	0,226	0,093 0,092	0,092	0,055 0,054	0,054	98,952
105	0,248 0,253	0,250	0,442 0,448	0,445	0,392 0,387	0,390	0,249 0,240	0,244	0,096 0,097	0,096	0,053 0,052	0,052	100,725

Table B.8 — Individual results for all laboratories — Sample JCA #2

Laboratory ref.	Loss on ignition	SiO <sub>2</sub> %		Al <sub>2</sub> O <sub>3</sub> %		Fe <sub>2</sub> O <sub>3</sub> %		CaO %		MgO %		SO <sub>3</sub> %	
		Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean
106	0,27	25,930 26,012	25,971	8,765 8,842	8,804	1,565 1,578	1,572	55,887 56,074	55,980	3,278 3,289	3,284	- -	-
107	0,09	26,254 26,264	26,259	8,888 8,878	8,883	1,503 1,531	1,517	56,852 56,832	56,842	3,031 3,001	3,016	- -	-
108	0,10	26,080 26,060	26,070	8,760 8,750	8,755	1,630 1,630	1,630	56,270 56,170	56,220	3,340 3,290	3,315	2,860 2,890	2,875
109	0,07	26,126 26,167	26,146	8,862 8,843	8,852	1,637 1,689	1,663	56,428 56,570	56,499	3,341 3,353	3,347	1,709 1,619	1,664
110	-	26,152 25,051	26,102	8,830 8,890	8,860	1,661 1,680	1,670	56,360 56,201	56,280	3,251 3,292	3,272	2,030 2,010	2,020
111	-	25,870 26,050	25,960	8,640 8,700	8,670	1,620 1,630	1,625	56,440 56,440	56,440	3,540 3,570	3,555	1,560 1,550	1,555
112	-	- -	-	- -	-	- -	-	- -	-	- -	-	- -	-
113	0,21	25,900 25,950	25,925	8,710 8,710	8,710	1,560 1,600	1,580	55,850 55,910	55,880	3,190 3,200	3,195	- -	-
114	-	26,610 27,590	27,100	6,730 6,880	6,805	2,160 2,100	2,130	55,150 56,170	55,660	4,370 4,180	4,275	2,550 2,420	2,485
E1	-	25,927 25,972	25,950	8,806 8,869	8,838	1,610 1,635	1,623	56,164 56,043	56,104	3,324 3,322	3,323	2,435 2,614	2,525
E2	0,15	25,872 25,869	25,871	8,791 8,788	8,790	1,596 1,604	1,600	55,957 55,974	55,966	3,315 3,317	3,316	2,911 2,886	2,899
E3	-	25,940 25,930	25,935	8,660 8,650	8,655	1,640 1,650	1,645	56,390 56,420	56,405	3,530 3,500	3,515	2,870 2,850	2,860
E4	-	25,839 25,901	25,870	8,772 8,826	8,799	1,598 1,597	1,598	55,365 55,254	55,310	3,215 3,241	3,228	3,775 3,728	3,752
E5	0,08	25,980 26,020	26,000	8,730 8,760	8,745	1,600 1,590	1,595	56,050 56,170	56,110	3,270 3,370	3,320	2,100 2,070	2,085
E6	0,23	26,069 26,067	26,068	8,799 8,780	8,790	1,639 1,647	1,643	56,508 56,549	56,528	3,348 3,381	3,365	- -	-
E7	0,15	26,004 25,886	25,945	8,729 8,781	8,755	1,629 1,630	1,630	55,838 56,017	55,928	3,320 3,328	3,324	2,942 2,929	2,936
E8	0,31	26,053 26,004	26,029	8,816 8,813	8,815	1,621 1,635	1,628	55,902 55,972	55,937	3,360 3,322	3,341	2,886 2,881	2,884
E9	0,07	26,124 26,061	26,093	8,853 8,878	8,866	1,584 1,578	1,581	56,326 56,244	56,285	3,341 3,333	3,337	- -	-
E10	-	26,240 26,250	26,245	8,890 8,900	8,895	1,620 1,610	1,615	55,810 55,770	55,790	3,340 3,340	3,340	2,610 2,610	2,610
E11	0,89	26,108 26,194	26,151	8,892 8,922	8,907	1,677 1,671	1,674	57,280 57,332	57,306	3,406 3,397	3,402	2,860 2,863	2,862
E12	0,20	25,740 26,000	25,870	8,944 8,751	8,848	1,557 1,580	1,569	55,550 55,980	55,765	3,359 3,364	3,362	- -	-

Table B.8 (continued)

Laboratory ref.	Na <sub>2</sub> O %		K <sub>2</sub> O %		TiO <sub>2</sub> %		P <sub>2</sub> O <sub>5</sub> %		MnO %		SrO %		Total
	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	Results	Mean	
106	0,243 0,239	0,241	0,433 0,432	0,432	- -	-	- -	-	- -	- -	- -	-	96,284
107	0,241 0,243	0,242	0,411 0,410	0,410	- -	-	0,049 0,049	0,049	0,100 0,098	0,099	- -	-	97,317
108	0,140 0,160	0,150	0,430 0,430	0,430	- -	-	0,230 0,230	0,230	- -	-	- -	-	99,675
109	- -	-	0,424 0,428	0,426	- -	-	- -	-	- -	-	- -	-	98,597
110	0,232 0,211	0,222	0,421 0,420	0,420	- -	-	0,243 0,253	0,248	- -	-	- -	-	99,094
111	0,230 0,250	0,240	0,440 0,450	0,445	0,440 0,430	0,435	0,270 0,300	0,285	0,100 0,090	0,095	0,050 0,050	0,050	99,355
112	- -	-	- -	-	- -	-	- -	-	- -	-	- -	-	-
113	0,280 0,270	0,275	0,430 0,430	0,430	0,400 0,400	0,400	0,240 0,230	0,235	0,100 0,100	0,100	0,050 0,050	0,050	96,780
114	0,640 0,650	0,645	0,360 0,360	0,360	- -	-	- -	-	- -	-	- -	-	99,460
E1	0,215 0,207	0,211	0,433 0,428	0,431	0,384 0,391	0,388	0,251 0,244	0,248	0,086 0,085	0,086	0,050 0,051	0,051	99,773
E2	0,228 0,233	0,231	0,420 0,425	0,423	0,390 0,391	0,391	0,230 0,236	0,233	0,094 0,096	0,095	- -	-	99,8121
E3	0,220 0,220	0,220	0,420 0,420	0,420	0,380 0,380	0,380	0,260 0,250	0,255	0,100 0,100	0,100	0,060 0,060	0,060	100,450
E4	0,219 0,232	0,226	0,416 0,417	0,417	0,394 0,395	0,395	0,228 0,230	0,229	0,100 0,104	0,102	0,051 0,053	0,052	99,975
E5	0,234 0,219	0,227	0,430 0,430	0,430	0,402 0,399	0,401	0,221 0,231	0,226	0,088 0,087	0,088	0,052 0,050	0,051	99,277
E6	0,101 0,101	0,101	0,429 0,432	0,430	0,379 0,379	0,379	0,262 0,269	0,265	0,082 0,080	0,081	- -	-	97,650
E7	0,227 0,224	0,226	0,430 0,428	0,429	0,390 0,387	0,389	0,241 0,246	0,244	0,087 0,086	0,087	0,058 0,059	0,059	99,948
E8	0,221 0,213	0,217	0,421 0,419	0,420	0,396 0,396	0,396	0,229 0,233	0,231	0,095 0,095	0,095	0,052 0,052	0,052	100,044
E9	- -	-	0,420 0,421	0,421	0,433 0,417	0,425	- -	-	- -	-	- -	-	97,007
E10	0,250 0,250	0,250	0,410 0,410	0,410	- -	-	- -	-	- -	-	- -	-	99,155
E11	0,205 0,197	0,201	0,444 0,443	0,444	0,400 0,400	0,400	0,237 0,236	0,237	0,089 0,089	0,089	0,058 0,059	0,059	101,730
E12	0,218 0,234	0,226	0,424 0,427	0,426	0,387 0,390	0,389	0,229 0,220	0,225	0,102 0,102	0,102	- -	-	96,779

## Annex C (informative)

### Questionnaire results

A questionnaire was sent to the participating laboratories and responses were received from 34 laboratories (including some responses where the questionnaire was only partially completed). The summarized results of the questionnaire are shown below, excluding items considered as having originated in individual equipment associated with the bead preparation conditions or measurement conditions.

#### C.1 Variety of fluxes

Flux used	Number of laboratories
Li <sub>2</sub> B <sub>4</sub> O <sub>7</sub> : 100 %	18
Li <sub>2</sub> B <sub>4</sub> O <sub>7</sub> : 90 %, LiF: 10 %	2
Li <sub>2</sub> B <sub>4</sub> O <sub>7</sub> : 90 %, LiNO <sub>3</sub> : 10 %	1
Li <sub>2</sub> B <sub>4</sub> O <sub>7</sub> : 84,9 %, LiF: 8,4 %, SrO: 4,6 %, V <sub>2</sub> O <sub>5</sub> : 2,1 %	1
Li <sub>2</sub> B <sub>4</sub> O <sub>7</sub> : 80 %, LiF: 20 %	1
Li <sub>2</sub> B <sub>4</sub> O <sub>7</sub> : 75 %, LiBO <sub>2</sub> : 25 %	1
Li <sub>2</sub> B <sub>4</sub> O <sub>7</sub> : 66,67 %, LiBO <sub>2</sub> : 32,83 %, LiBr: 0,50 %	1
Li <sub>2</sub> B <sub>4</sub> O <sub>7</sub> : 66 %, LiBO <sub>2</sub> : 34 %	5
Li <sub>2</sub> B <sub>4</sub> O <sub>7</sub> : 59 %, LiBO <sub>2</sub> : 30,6%, LiF: 10 %	1

#### C.2 Flux-to-sample ratio

Flux-to-sample ratio, by mass	< 1,0	1,0 to 1,9	2,0 to 2,9	3,0 to 3,9	4,0 to 4,9	5,0 to 5,9	6,0 to 6,9	7,0 to 7,9	8,0 to 8,9	9,0 to 9,9	10	15,7
Number of laboratories	2	0	2	4	10	4	5	2	1	2	1	1

#### C.3 Fusion temperature

Range of fusion temperature, °C	< 1 050	1 050 to 1 100	> 1 100
Laboratories	5	25	4

#### C.4 Background correction

Background correction	Applied	Not applied
Laboratories	4	22

**C.5 Correction for inter-element effect**

<b>Correction for inter-element effect</b>	Applied	Not applied
<b>Laboratories</b>	13	21

## Annex D (informative)

### Other international inter-laboratory round-robin analyses of cement

#### D.1 General

The ISO round robin was a method performance study conducted under close to optimum conditions with clear calibration and measurement guidelines. This is conducive to producing “best practice” values representative of the ideal situation.

However, ISO 29581-2 is intended for use under everyday conditions in laboratories that operate to “good practice”. In order to compare the performance of laboratories in the more general scenario, this Annex sets out the results of some international round robins carried out by a large number of laboratories. Generally around 60 laboratories participated in a range of standardized chemical and physical tests, although not all participated in all of the tests. Whilst most of the chemical analyses would have been undertaken using x-ray fluorescence methods, there is no record of which tests used pressed pellets or fused beads. Other wet chemical or other instrumental methods might equally have been used.

Clearly, these results are not directly comparable to the ISO round robin but they do put into context the performance criteria when applied to routine analyses. The criteria proposed in ISO 29581-2:—, Table 2, for “expert” and “normal” performance analyses are used to segregate other “outlier” results. Mean analyses and reproducibility standard deviations are calculated after excluding these “outliers”.

#### D.2 Accuracy limits for validation

The proposed values from ISO 29581-2:—, Table 2, are given in Table D.1.

**Table D.1 — Accuracy limits for validation of laboratory performance**

Content of element species % absolute	Accuracy limit: “normal” performance % absolute	Accuracy limit: “expert” performance % absolute
0 to 0,49	0,05	0,02
0,50 to 0,99	0,08	0,03
1,00 to 6,99	0,20	0,08
7,00 to 14,99	0,30	0,12
15,00 to 29,99	0,38	0,15
30,00 to 49,99	0,50	0,20
50,00 to 79,99	0,63	0,25
80,00 to 100	0,75	0,30

### D.3 Results of analyses

Results of analyses of Portland cement (CEM I), Portland-limestone cement (CEM II/A-LL) and Portland-slag cement (CEM II/A-S) carried out between April 2006 and January 2007 are summarized in Tables D.2 to D.4.

**Table D.2 — Analyses of Portland cement, CEM I — April 2006 round robin**

Parameter	SiO <sub>2</sub> %	Al <sub>2</sub> O <sub>3</sub> %	Fe <sub>2</sub> O <sub>3</sub> %	CaO %	MgO %	SO <sub>3</sub> %	Na <sub>2</sub> O %	K <sub>2</sub> O %	LOI <sup>a</sup> %
Reference analysis	20,57	5,11	3,27	62,06	2,68	3,59	0,25	1,28	0,97
Maximum	20,91	5,29	3,46	62,67	2,83	3,70	0,30	1,44	1,05
Minimum	20,21	4,94	3,10	61,47	2,48	3,43	0,21	1,10	0,87
S.D.	0,17	0,09	0,05	0,49	0,08	0,06	0,03	0,06	0,05
Number of laboratories	38	38	38	38	38	39	31	36	54
% rated "expert"	53	53	79	42	61	64	29	86	33
% rated "expert and normal"	82	84	95	71	79	82	58	100	67
% rated "outlier"	18	16	5	29	21	18	42	0	33

<sup>a</sup> Loss on ignition.

**Table D.3 — Analyses of Portland-limestone cement, CEM II/A-LL — October 2006 round robin**

Parameter	SiO <sub>2</sub> %	Al <sub>2</sub> O <sub>3</sub> %	Fe <sub>2</sub> O <sub>3</sub> %	CaO %	MgO %	SO <sub>3</sub> %	Na <sub>2</sub> O %	K <sub>2</sub> O %	LOI <sup>a</sup> %
Reference analysis	19,18	5,11	2,81	66,87	1,42	3,26	0,11	0,56	8,64
Maximum	19,54	5,28	2,96	67,38	1,62	3,46	0,15	0,64	8,86
Minimum	18,84	4,95	2,66	66,37	1,22	3,07	0,06	0,48	8,39
S.D.	0,17	0,07	0,07	0,50	0,09	0,10	0,02	0,03	0,09
Number of laboratories	36	36	36	36	36	36	28	35	53
% rated "expert"	47	64	78	53	58	50	50	66	66
% rated "expert and normal"	81	78	94	69	81	86	75	89	79
% rated "outlier"	19	22	6	31	19	14	25	11	21

<sup>a</sup> Loss on ignition.

**Table D.4 — Analyses of Portland-slag cement, CEM II/A-S — January 2007 round robin**

Parameter	SiO <sub>2</sub> %	Al <sub>2</sub> O <sub>3</sub> %	Fe <sub>2</sub> O <sub>3</sub> %	CaO %	MgO %	SO <sub>3</sub> %	Na <sub>2</sub> O %	K <sub>2</sub> O %	LOI <sup>a</sup> %
Reference analysis	22,79	6,17	2,89	58,51	3,52	3,33	0,25	1,30	1,46
Maximum	23,11	6,34	2,99	59,14	3,72	3,52	0,29	1,43	1,64
Minimum	22,46	6,00	2,70	58,00	3,39	3,13	0,22	1,22	1,27
S.D.	0,18	0,09	0,07	0,28	0,08	0,10	0,02	0,04	0,08
Number of laboratories	37	37	37	36	35	39	28	34	54
% rated "expert"	41	51	65	50	60	36	50	91	70
% rated "expert and normal"	70	86	89	83	83	72	71	94	87
% rated "outlier"	30	14	11	17	17	28	29	6	13

<sup>a</sup> Loss on ignition.

## D.4 Considerations

The results indicate that

- the ability to achieve the proposed analytical performance is not affected by cement type;
- a high proportion of laboratories were able to meet the performance associated with certain analytical constituents, e.g.  $\text{Fe}_2\text{O}_3$  and  $\text{K}_2\text{O}$ ;
- a lower proportion of laboratories were able to meet the performance associated with  $\text{Na}_2\text{O}$  (low concentration of a light element) and  $\text{CaO}$  (highest concentration).

These considerations suggest that the performance validation levels proposed in ISO 29581-2 for high and low constituent concentrations should be re-considered in relation to “normal” performance laboratories.



## Annex E (informative)

### Acknowledgements

We express our deep appreciation for the cooperation and understanding of the participating laboratories and all persons concerned with this inter-laboratory testing programme.

We are indebted to the Technical Committee on chemistry of cement, Japan Cement Association, for the initiation, management and first report of this programme.

Members of the committee as of April 2006 were:

#### Chairman

Shunsuke Hanehara	Taiheiyo Cement Corporation	(to 2005)
Hisashi Inokawa	Sumitomo Osaka Cement Co., Ltd.	(from May 2005)

#### Members

Masashi Osaki	Ube-Mitsubishi Cement Research Institute Corporation, Ube Center
Hiroshi Hirao	Taiheiyo Cement Corporation
Noriyuki Arano	Denki Kagaku Kogyo Kabushiki Kaisha
Daihachi Kitayama	Tokuyama Corporation
Kenichi Shimosaka	Ube-Mitsubishi Cement Research Institute Corporation, Saitama Center

#### Secretaries

Shigeru Takahashi	Japan Cement Association
Hiroyuki Anzai	Japan Cement Association
Naoki Aoki	Japan Cement Association

#### Other international inter-laboratory testing

We are grateful to the HeidelbergCement Technical Center for allowing us to include the data from their international cement testing performance reviews.

## Bibliography

- [1] ISO 680:1990, *Cement — Test methods — Chemical analysis*
- [2] ISO 5725-2:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*
- [3] ISO 29581-1, *Cement — Test methods — Part 1: Analysis by wet chemistry*
- [4] ISO 29581-2:—<sup>1)</sup>, *Methods of testing cement — Chemical analysis of cement — Part 2: Analysis by X-ray fluorescence*
- [5] EN 197-1:2000, *Cement — Part 1: Composition, specifications and conformity criteria for common cements*
- [6] EN 196-2, *Methods of testing cement — Part 2: Chemical analysis of cement*
- [7] Report of the Technical Committee on cement chemistry of Japan Cement Association: C10 — Report on the inter-laboratory testing of chemical analysis of cement by x-ray fluorescence, Tokyo, Japan, May 2006
- [8] JIS R 5204, *Chemical analysis method of cement by x-ray fluorescence*
- [9] JIS R 5211, *Portland blast-furnace slag cement*
- [10] World Cement Directory, 2002

---

1) To be published.



