
**Steel and iron — Determination of nitrogen
content — Thermal conductimetric method
after fusion in a current of inert gas**

*Aciers et fontes — Dosage de l'azote — Méthode par conductibilité
thermique après fusion sous un courant de gaz inerte*

This material is reproduced from ISO documents under International Organization for Standardization (ISO) Copyright License number IHS/ICC/1996. Not for resale. No part of these ISO documents may be reproduced in any form, electronic retrieval system or otherwise, except as allowed in the copyright law of the country of use, or with the prior written consent of ISO (Case postale 56, 1211 Geneva 20, Switzerland, Fax +41 22 734 10 79), IHS or the ISO Licensor's members.



Reference number
ISO 10720:1997(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 10720 was prepared by Technical Committee ISO/TC 17, *Steel*, Subcommittee SC 1, *Methods of determination of chemical composition*.

Annexes A to C of this International Standard are for information only.

© ISO 1997

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization
Case postale 56 • CH-1211 Genève 20 • Switzerland
Internet: central@iso.ch
X.400: c=ch; a=400net; p=iao; o=iso; s=central

Printed in Switzerland

Steel and iron — Determination of nitrogen content — Thermal conductimetric method after fusion in a current of inert gas

1 Scope

This International Standard specifies a thermal conductimetric method after fusion under inert gas for the determination of nitrogen in steel and iron.

The method is applicable to nitrogen contents between 0,000 8 % (m/m) and 0,5% (m/m).

2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 365-1:1984, *Laboratory glassware — Burettes — Part 1: General requirements.*

ISO 648:1977, *Laboratory glassware — One-mark pipettes.*

ISO 1042:—¹⁾, *Laboratory glassware — One-mark volumetric flasks.*

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods.*

ISO 5725-1:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions.*

ISO 5725-2:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method.*

ISO 5725-3:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 3: Intermediate measures of the precision of a standard measurement method.*

ISO 14284 :1996, *Steel and iron — Sampling and preparation of samples for the determination of chemical composition.*

3 Principle

Fusion of a test portion in a single-use graphite crucible under helium gas at a high temperature (e. g. 2 200 °C)
Extraction of the nitrogen in the form of molecular nitrogen in the stream of helium.

Separation from the other gaseous extracts and measurement by thermal conductimetric method.

4 Reagents and materials

During the analysis, unless otherwise stated, use only reagents of recognized analytical grade and only grade 2 water as specified in ISO 3696.

1) To be published. (Revision of ISO 1042:1983)

4.1 Water, prepare just before use.

4.2 Helium, high purity, total impurity content 0,000 5 % (m/m).

An oxidation reagent or catalyst [copper(II) oxide or platinum] tube heated to a temperature above 450 °C shall be used prior to a purifying unit, when the presence of organic contaminants is suspected in the helium.

4.3 Pure Iron, of known low nitrogen contents less than 0,001 % (m/m).

4.4 Copper (II) oxide, on granulated support.

4.5 Anhydrous magnesium perchlorate, $Mg(ClO_4)_2$, particle size from 1,2 mm to 2,0 mm, or anhydrous calcium sulfate, particle size from 0,60 mm to 0,85 mm.

4.6 Sodium hydroxide, on granulated support.

Particle size from 0,7 mm to 1,2 mm.

4.7 Appropriate solvent, suitable for washing greasy or dirty test samples, e.g. acetone.

4.8 Potassium nitrate, standard solution.

After drying at between 100 °C and 105 °C for 2 h and allowing to cool in a desiccator, weigh, to the nearest 0,1 mg, the masses of potassium nitrate [purity > 99,9 % (m/m)] indicated in table 1.

Dissolve the potassium nitrate in about 50 ml of water (4.1), transfer quantitatively to a 100 ml one-mark volumetric flask, dilute to the mark with water (4.1) and mix.

1 ml of each standard solution contains the mass of nitrogen indicated in table 1.

Table 1 — Standard solutions

| Name of the standard solution | Mass of potassium nitrate used | Corresponding concentration of nitrogen mg/ml |
|-------------------------------|--------------------------------|---|
| | g | |
| 4.8.1 | 9,022 8 | 12,5 |
| 4.8.2 | 7,218 2 | 10,0 |
| 4.8.3 | 5,413 8 | 7,5 |
| 4.8.4 | 3,609 1 | 5,0 |
| 4.8.5 | 1,804 6 | 2,50 |
| 4.8.6 | 0,902 3 | 1,25 |
| 4.8.7 | 0,360 9 | 0,50 |
| 4.8.8 | [4.8.5 × 1/10] ¹⁾ | 0,25 |
| 4.8.9 | [4.8.6 × 1/10] | 0,125 |
| 4.8.10 | [4.8.7 × 1/10] | 0,050 |

1) e.g. transfer 10,0 ml of the standard solution (4.8.5) into a 100 ml one-mark volumetric flask, dilute to the mark with water (4.1) and mix.

5 Apparatus

During the analysis, unless otherwise stated, use only ordinary laboratory apparatus.

All volumetric glassware shall be class A, in accordance with ISO 385-1, ISO 648 or ISO 1042 as appropriate.

The apparatus required for fusion of the test portion, separation and measurement of the nitrogen extracted may be obtained commercially from a number of manufacturers. Follow the manufacturer's instructions for the operation of the instrument.

Features of commercial instruments are given in annex A.

5.1 Graphite crucible, single-use.

Use high purity crucibles suitable for use with the apparatus.

5.2 Micropipette, 100 μ l and 200 μ l, limit of error shall be less than 1 μ l.

5.3 Nickel capsule.

For example, about 6 mm in diameter; 8 mm in height; 0,2 g in mass and 0,23 ml in volume, or about 6 mm in diameter; 12,5 mm in height; 0,5 g in mass and 0,35 ml in volume. In any case, the nitrogen content shall be less than 0,000 2 % (*m/m*).

5.4 Crucible tongs, for handling the crucibles used.

5.5 Glass-wool filters.

6 Sampling

Carry out sampling in accordance with ISO 14284 or appropriate national standards for steel and iron.

7 Procedure

WARNING — The risks involved when using an apparatus for fusing the test portion are mainly risks of burns. It is therefore essential to use crucible tongs (5.4) and appropriate containers for the used crucibles.

7.1 General instructions

Keep the glass-wool filters (5.5) clean. Using a certified reference material, verify the effectiveness of the installed reagents (4.4, 4.5 and 4.6) and change them if necessary.

In certain instruments, it is necessary to clean the sample introduction pipe in the furnace after each analysis in order to eliminate carbon deposits. If the electricity supply has been switched off for a long time, allow time for the instrument to stabilize as recommended by the manufacturer.

After changing the filters (5.5) and/or reagents (4.4, 4.5 and 4.6), or when the apparatus has been inoperative for a period, stabilize the instrument by carrying out trial analyses, the results of which are to be disregarded, then proceed with calibration as indicated in 7.5 before analysing the sample.

If the instrument used provides a direct reading in percentage of nitrogen, adjust the instrument reading for each calibration range as follows.

Read the content of a certified reference material of high nitrogen content at various power settings. The required heating power for the determination of test samples is that at which the reading levels off.

In order to determine a high alloy test sample a high alloy certified reference material shall be used to know the required heating power.

7.2 Test portion

Degrease the test sample by washing in a suitable solvent (4.7). Evaporate the last traces of the washing liquid by heating.

Weigh, to the nearest 1 mg, approximately 1,0 g of the test sample for nitrogen contents up to 0,1 % (*m/m*) and approximately 0,50 g for nitrogen contents greater than 0,1 % (*m/m*) (see note 1).

NOTE 1 The mass of the test portion may be dependent on the type of instrument used.

7.3 Blank test

Prior to the determination, carry out the following blank tests in duplicate.

7.3.1 Sample with nitrogen contents up to 0,10 % (*m/m*)

7.3.1.1 Using the micropipette (5.2), transfer 200 μ l of water (4.1) to a nickel capsule (5.3) and dry at 90 °C to 95 °C for 2 h. Treat the nickel capsule as specified in 7.4.1, and add the same quantity of the pure iron (4.3) in place of the test portion.

7.3.1.2 Obtain the reading of the blank tests and convert it to micrograms of nitrogen by means of the calibration graph (see 7.5).

The blank value is obtained by subtracting the mass of nitrogen in the pure iron used (4.3) from the mass of nitrogen in the blank tests.

The mean blank value (m_b) is calculated from the two blank values (see note 2).

NOTE 2 It is essential that neither the mean blank value nor the difference between the two blank values exceed 10 μ g of nitrogen. If these values are abnormally high, the source of contamination should be investigated and eliminated.

7.3.2 Sample with nitrogen contents between 0,10 % (*m/m*) and 0,50 % (*m/m*)

Using the micropipette (5.2), transfer 200 μ l of water (4.1) to a degassed graphite crucible (5.1) and dry at 90 °C to 95 °C for 2 h. Add the same quantity of the pure iron (4.3) instead of the test portion and proceed as specified in 7.3.1.2.

7.4 Determination

7.4.1 Sample with nitrogen contents up to 0,10 % (*m/m*)

7.4.1.1 Place a graphite crucible (5.1) in the furnace (see annex A) and then degas by heating at greater than 2 200 °C.

7.4.1.2 Flatten a nickel capsule (5.3) by pressing, insert it and add the test portion (see 7.2) to the degassed graphite crucible.

7.4.1.3 Operate the furnace in accordance with the manufacturer's instructions.

At the end of the fusion and measuring cycle, remove and discard the crucible, and record the analyser reading.

7.4.2 Sample with nitrogen contents between 0,10 % (*m/m*) and 0,50 % (*m/m*)

Place a graphite crucible (5.1) in the furnace (see annex A) and then degas by heating at greater than 2 200 °C.

Add the test portion (see 7.2) to the degassed graphite crucible (5.1) and continue as specified in 7.4.1.3.

7.5 Establishment of the calibration graph

7.5.1 Preparation of the calibration series

7.5.1.1 Sample with nitrogen contents up to 0,10 % (m/m)

Using the micropipette (5.2), transfer 200 μl of each of the potassium nitrate standard solutions (4.8) indicated in table 2, to the respective nickel capsule (5.3), and dry at 90 °C to 95 °C for 2 h.

7.5.1.2 Sample with nitrogen contents between 0,10 % (m/m) and 0,50 % (m/m)

Using the micropipette (5.2), transfer 200 μl of each of the potassium nitrate standard solutions (4.8) indicated in table 3, to the respective degassed graphite crucible (5.1), and dry at 90 °C to 95 °C for 2 h.

7.5.2 Measurements

7.5.2.1 Sample with nitrogen contents up to 0,10 % (m/m)

Treat the nickel capsule (5.3) containing potassium nitrate as specified in 7.4.1. Add the same quantity of the pure iron (4.3) in place of the test portion.

7.5.2.2 Sample with nitrogen contents between 0,10 % (m/m) and 0,50 % (m/m)

Add, to each dried graphite crucible, the same quantity of the pure iron (4.3) as that of the test portion used, and continue as specified in 7.4.1.3

7.5.3 Plotting the calibration graph

Obtain the net reading by subtracting the reading of the zero member (see tables 2 and 3) from that of each member of the calibration series.

Prepare a calibration graph by plotting the net reading against micrograms of nitrogen for each member of the calibration series.

Table 2 — Calibration solutions, nitrogen contents up to 0,10 % (m/m)

Test portion: 1,0 g — Standard solutions added: 200 μl

| Standard solution (4.8) used | Concentration of nitrogen | Mass of nitrogen taken in the nickel capsule or the graphite crucible | Nitrogen content in the test portion |
|---------------------------------|------------------------------|---|---|
| | mg/ml | μg | % (m/m) |
| water(4.1) | 0 ¹⁾ | 0 | 0 |
| 4.8.10 | 0,050 | 10 | 0,001 0 |
| 4.8.9 | 0,125 | 25 | 0,002 5 |
| 4.8.8 | 0,250 | 50 | 0,005 0 |
| 4.8.7 | 0,500 | 100 | 0,010 |
| 4.8.6 | 1,25 | 250 | 0,025 |
| 4.8.5 | 2,50 | 500 | 0,050 |
| 4.8.4 | 5,00 | 1 000 | 0,100 |
| 1) Zero member | | | |

Table 3 — Calibration solutions, nitrogen contents between 0,10 % (m/m) and 0,50 % (m/m)

Test portion: 0,5 g — Standard solutions added: 200 µl

| Standard solution (4.8) used | Concentration of nitrogen | Mass of nitrogen taken in the nickel capsule or the graphite crucible | Nitrogen content in the test portion |
|---------------------------------|------------------------------|---|---|
| | mg/ml | µg | % (m/m) |
| water(4.1) | 0 ¹⁾ | 0 | 0 |
| 4.8.5 | 2,5 | 500 | 0,100 |
| 4.8.4 | 5,0 | 1 000 | 0,200 |
| 4.8.3 | 7,5 | 1 500 | 0,300 |
| 4.8.2 | 10,0 | 2 000 | 0,400 |
| 4.8.1 | 12,5 | 2 500 | 0,500 |

1) Zero member

8 Expression of results

8.1 Method of calculation

Convert the analyser reading for the test portion to micrograms of nitrogen (m_0) by means of the calibration graph (see 7.5).

The nitrogen content, w_N , expressed as a percentage by mass, is given by the equation:

$$w_N = \frac{(m_0 - m_1)}{m \times 10^6} \times 100$$

$$= \frac{(m_0 - m_1)}{10^4 m}$$

where

m_0 is the mass, expressed in micrograms, of nitrogen in the test portion;

m_1 is the mass, expressed in micrograms, of nitrogen in the blank test (see 7.3);

m is the mass, in grams, of the test portion (see 7.2).

8.2 Precision

A planned trial of this method was carried out by 14 laboratories, at eleven levels of nitrogen, each laboratory making three determinations (see notes 3 and 4) of nitrogen at each level.

NOTES

3 Two of the three determinations were carried out under repeatability conditions as defined in ISO 5725-1; i.e. one operator, same apparatus, identical operating conditions, same calibration, and a minimum period of time.

4 The third determination was carried out at a different time (on a different day) by the same operator as in note 3, using the same apparatus with a new calibration.

The test samples used are listed in annex B.1.

The results obtained were treated statistically in accordance with ISO 5725, Parts 1, 2 and 3.

The data obtained showed a logarithmic relationship between nitrogen content and repeatability (r) and reproducibility (R and R_w) of the test results (see note 5) as summarized in table 4. The graphical representation of the data is shown in annex C.

Table 4 — Results for repeatability and reproducibility limits

| Nitrogen content % (m/m) | Repeatability limit r | Reproducibility limits | |
|-----------------------------|-------------------------------|---------------------------|----------|
| | | R | R_w |
| 0,000 8 | 0,000 24 | 0,000 39 | 0,000 27 |
| 0,001 0 | 0,000 27 | 0,000 45 | 0,000 30 |
| 0,002 0 | 0,000 36 | 0,000 71 | 0,000 44 |
| 0,005 0 | 0,000 54 | 0,001 30 | 0,000 71 |
| 0,010 0 | 0,000 73 | 0,002 07 | 0,001 03 |
| 0,020 0 | 0,000 98 | 0,003 28 | 0,001 49 |
| 0,050 0 | 0,001 46 | 0,006 03 | 0,002 42 |
| 0,100 | 0,001 97 | 0,009 56 | 0,003 50 |
| 0,200 | 0,003 07 | 0,014 4 | 0,006 26 |
| 0,500 | 0,005 54 | 0,024 9 | 0,013 5 |

NOTE 5 From the two values obtained on day 1, the repeatability limit (r) and reproducibility limit (R) were calculated using the procedure specified in ISO 5725-2. From the first value obtained on day 1 and the value obtained on day 2, the within-laboratory reproducibility limit (R_w) was calculated using the procedure given in ISO 5725-3.

9 Test report

The test report shall include the following information:

- all information necessary for the identification of the sample, the laboratory and the date of analysis;
- the method used by reference to this International Standard;
- the results, and the form in which they are expressed;
- any unusual features noted during the determination;
- any operation not specified in this International Standard, or any optional operation which may have influenced the results.

Annex A

(informative)

Features of commercial resistive electrode furnaces and nitrogen analysers

A.1 The helium source is fitted with a fine adjustment valve and a pressure gauge. The pressure control valve is used to check the helium inlet pressure in the furnace in accordance with the manufacturer's instructions; this is usually 28 kN/m².

A.2 The purifying apparatus contains sodium hydroxide-impregnated attapulgite, and magnesium perchlorate in a dehydration tube.

A.3 Flowmeter for measuring the flow of helium in the range 0 to 4 l/min.

A.4 Resistive electrode furnace, as follows:

A.4.1 The furnace used for fusion of the test portion by the Joule effect is composed of two solid copper or copper alloy electrodes which fit together tightly while providing an adequate volume to accommodate a graphite crucible. The graphite crucible is used as an electrical connection between the two electrodes.

Tightness is generally ensured by an O-ring.

The electrodes are generally cooled down by water circulation so that the O-rings are not damaged during the fusion of the test portion.

A.4.2 A transformer supplies the necessary amperage for fusion to be performed satisfactorily.

A.4.3 The graphite crucible containing the test portion, and a nickel capsule, if required, is placed on the lower electrode to ensure a good electrical connection.

A.4.4 The electrode diameter, the geometrical form of the furnace and the transformer output are determined by the apparatus manufacturer.

A.4.5 The temperature reached during fusion is dependent partly on the parameters in A.4.4 and partly on the metal properties, on the test portion shape and mass, and sometimes on the crucible geometry.

A.5 Thermal conductivity gas analyser (catharometer), as follows:

A.5.1 In most current apparatus, the gaseous fusion emissions are transferred into the analyser by a continuous helium flow.

An apparatus, after an oxidation furnace, in which reagents (4.4, 4.5 and 4.6) are installed makes it possible to convert carbon monoxide and hydrogen into carbon dioxide and water and absorb them.

The helium-nitrogen stream flow is led to the catharometer. The difference in thermal conductivity of the pure gas and of the mixture is recorded and integrated over a pre-programmed time interval.

Signal amplification and conversion with digital display make it possible to obtain the percentage nitrogen concentration.

A.5.2 Electronic controls are used to set the instrument to zero, to compensate for the blank value, to adjust the calibration curve slope, and to correct non-linear responses.

Provision is generally incorporated in the analyser to take into account the mass of the reference sample or test portion, and to automatically correct readings.

Some equipment may also be fitted with integrated automatic scales to weigh the test portion and to transfer the corresponding value into the analyser.

Annex B (informative)

Additional information on the international cooperative tests

Table 4 was derived from the results of two international analytical trials. The first one was carried out in 1991 on three steel samples in three countries involving 10 laboratories and the second one was carried out in 1993 on six steel samples and two iron samples in four countries involving 14 laboratories.

The results of the trials were reported in document ISO/TC 17/SC 1 N 928, 1992-02-14 and N 1018, 1994-03-20. The graphical representation of the precision data is given in annex C.

The test samples used and the results obtained are listed in tables B.1 and B.2.

Table B.1 — Test samples used in the interlaboratory tests


| Sample | Chemical composition, % (m/m) | | | | | | | |
|-------------------------------------|-------------------------------|-------|-------|---------|---------|---------|-------|-----------------------------|
| | N | C | Si | Mn | Ni | Cr | Ti | Others |
| ECRM 097-1 (Pure iron) | 0,000 7 | | | 0,006 4 | 0,002 5 | 0,001 6 | | |
| ECRM 285-1 (High alloy steel) | 0,002 3 | 0,003 | | 0,013 | 18,46 | 0,034 | 0,74 | Mo 5,07 |
| NIST 7g (Cast iron) | 0,004 | 2,69 | 2,41 | 0,612 | 0,120 | 0,048 | | |
| ECRM 077-2 (Mild steel) | 0,005 4 | 0,151 | 0,293 | 1,28 | | | | |
| ECRM 182-1 (Unalloyed steel) | 0,010 2 | 0,79 | 0,368 | 0,389 | 0,152 | 0,591 | | |
| ECRM 281-1 (High alloy steel) | 0,023 | 0,048 | 0,929 | 0,786 | 9,37 | 18,17 | 0,216 | |
| ECRM 227-1 (High alloy steel) | 0,040 | 0,950 | 0,272 | 0,236 | 0,114 | 4,25 | | Mo 2,64 V 2,44 W 3,03 |
| JK 8F (High alloy steel) | 0,071 5 | 0,038 | 0,474 | 1,552 | 11,02 | 16,91 | | Mo 2,775 Co 0,125 |
| BAM 230-1 (Alloyed steel) | 0,159 8 | 0,077 | 0,524 | 8,45 | 5,55 | 18,05 | | |
| NIST 346a (Heat resisting steel) | 0,415 | 0,502 | 0,219 | 9,16 | 3,43 | 21,08 | | |
| DAIDO (Heat resisting steel) | 0,450 | 0,5 | 0,1 | 9 | 4 | 21 | | |

Table B.2 — The results obtained in interlaboratory tests

| Sample | Nitrogen content | | Precision data | | | |
|---|------------------|-----------------|-----------------|---|---------------------------|----------------------|
| | Certified | Found | | Repeat- ability limit <i>r</i> | Reproducibility limits | |
| | | $\bar{w}_{N,1}$ | $\bar{w}_{N,2}$ | | <i>R</i> | <i>R_w</i> |
| ECRM 097-1 (Pure iron) | 0,000 7 | 0,000 78 | 0,000 75 | 0,000 23 | 0,000 44 | 0,000 30 |
| ECRM 285-1 (High alloy steel) | 0,002 3 | 0,002 3 | 0,002 3 | 0,000 46 | 0,000 81 | 0,000 53 |
| NIST 7g (Cast iron) | 0,004 | 0,005 0 | 0,005 0 | 0,000 63 | 0,001 5 | 0,000 41 |
| ECRM 077-2 (Mild steel) | 0,005 4 | 0,005 4 | 0,005 5 | 0,000 47 | 0,000 98 | 0,000 97 |
| ECRM 182-1 (Unalloyed steel) | 0,010 2 | 0,009 7 | 0,009 8 | 0,000 56 | 0,001 7 | 0,000 63 |
| ECRM 281-1 (High alloy steel) | 0,023 | 0,022 | 0,022 | 0,001 4 | 0,003 5 | 0,002 1 |
| ECRM 227-1 (High alloy steel) | 0,040 | 0,039 | 0,039 | 0,000 7 | 0,005 3 | 0,003 5 |
| JK 8F (High alloy steel) | 0,071 5 | 0,069 | 0,069 | 0,002 6 | 0,008 6 | 0,002 1 |
| BAM 230-1 (Alloyed steel) | 0,159 8 | 0,153 3 | 0,154 0 | 0,002 3 | 0,009 0 | 0,003 7 |
| NIST 346a (Heat resisting steel) | 0,415 | 0,413 | 0,413 | 0,005 3 | 0,035 | 0,011 |
| DAIDO (Heat resisting steel) | 0,450 | 0,454 | 0,455 | 0,009 3 | 0,036 | 0,021 |
| $\bar{w}_{N,1}$: general average on one day $\bar{w}_{N,2}$: general average over several days | | | | | | |

Annex C (informative)

Graphical representation of precision data

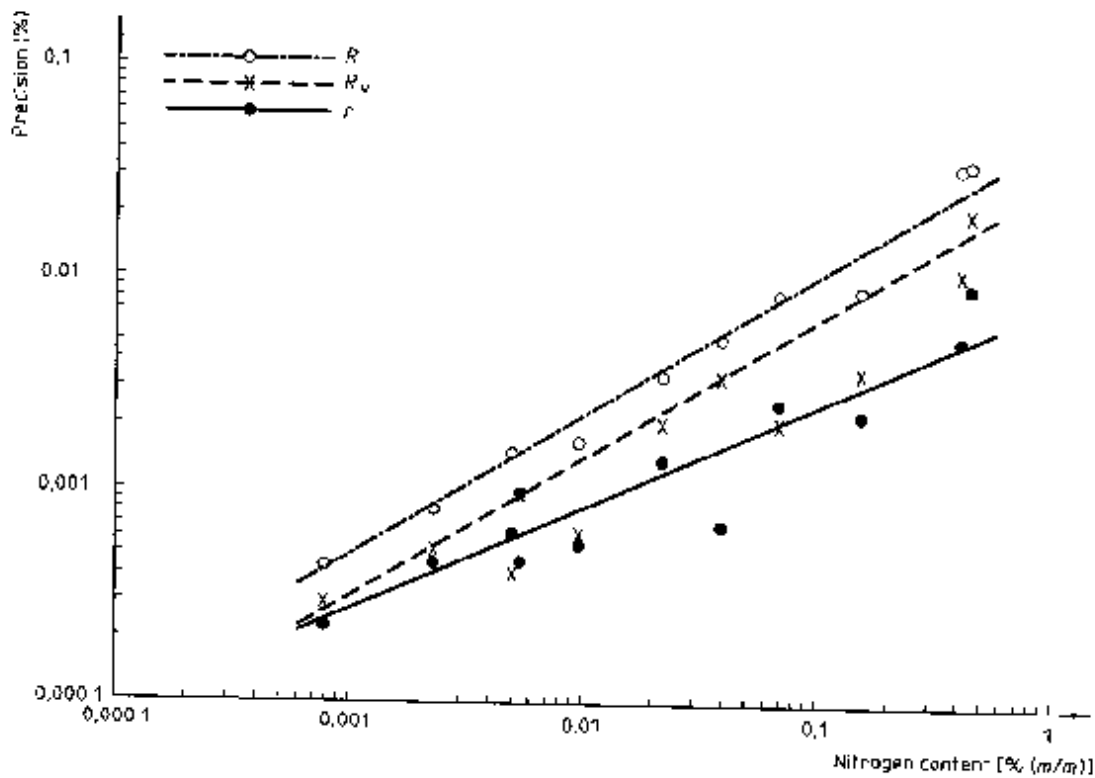

Nitrogen contents up to 0,1 % (m/m)

$$\lg r = 0,433\ 4 \lg \bar{w}_{N,1} - 2,271\ 4$$

$$\lg R = 0,665\ 3 \lg \bar{w}_{N,1} - 1,354\ 0$$

$$\lg R_w = 0,532\ 6 \lg \bar{w}_{N,2} - 1,922\ 9$$

Nitrogen contents between 0,1 % (m/m) and 0,5 % (m/m)

$$\lg r = 0,642\ 4 \lg \bar{w}_{N,1} - 2,063\ 1$$

$$\lg R = 0,594\ 8 \lg \bar{w}_{N,1} - 1,424\ 7$$

$$\lg R_w = 0,838\ 8 \lg \bar{w}_{N,2} - 1,617\ 1$$

where

$\bar{w}_{N,1}$ is the average nitrogen content, expressed as a percentage by mass, obtained within a day;

$\bar{w}_{N,2}$ is the average nitrogen content, expressed as a percentage by mass, obtained between days.

Figure C.1 — Logarithmic relationship between nitrogen content (\bar{w}_N) and repeatability limit (r) or reproducibility limits (R and R_w)

ICS 77.080.01

Descriptors: steels, iron and steel products, chemical analysis, determination of content, nitrogen, conductimetric methods.

Price based on 11 pages
