
**Non-destructive testing — Infrared
thermography — Vocabulary**

Essais non destructifs — Thermographie infrarouge — Vocabulaire



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



COPYRIGHT PROTECTED DOCUMENT

© ISO 2013

The reproduction of the terms and definitions contained in this International Standard is permitted in teaching manuals, instruction booklets, technical publications and journals for strictly educational or implementation purposes. The conditions for such reproduction are: that no modifications are made to the terms and definitions; that such reproduction is not permitted for dictionaries or similar publications offered for sale; and that this International Standard is referenced as the source document.

With the sole exceptions noted above, no other part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents	Page
Foreword	iv
Introduction	v
Scope	1
1 Terms and definitions	1
Bibliography	26
Alphabetical index	27

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2. www.iso.org/directives

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received. www.iso.org/patents

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 135, *Non-destructive testing*, Subcommittee SC 8, *Infrared thermography for non-destructive testing*.

Introduction

This International Standard is a compilation of terms and definitions to provide a precise understanding or interpretation of infrared thermography and thermal/infrared non-destructive testing. These serve to secure the foundation of infrared thermography technology growth within the academic and industrial communities.

Non-destructive testing — Infrared thermography — Vocabulary

Scope

This International Standard defines terms used in infrared thermography for non-destructive testing and forms a common basis for standard general use.

1 Terms and definitions

1.1

absorptivity

α

absorptance

absorptance coefficient

proportion (as a fraction of 1) of the radiant energy impinging on a material's surface that is absorbed by the material

NOTE 1 Absorptivity is dimensionless.

NOTE 2 For a blackbody, this is unity (1,0). Technically, absorptivity is the internal absorptance per path length. In thermography, the two terms, absorptivity and absorptance, are often used interchangeably.

NOTE 3 Absorptance is the ratio between the radiation energy absorbed by a body and the total radiation incident on the body.

NOTE 4 Absorptivity can vary with wavelength and be quoted for a specified band width or a specific wavelength. See 1.136, Spectral absorption coefficient.

1.2

active thermography

infrared thermographic examination of materials and objects which requires additional thermal stimulation

NOTE The thermal stimulation can be optical, sonic (ultrasonic), inductive, microwave or use any other form of energy.

1.3

ambient operating range

range of ambient temperatures over which an instrument is designed to operate within reported performance specifications

1.4

ambient temperature

temperature of the air in the vicinity of a test object (target)

NOTE "Ambient temperature" is not to be confused with "reflected ambient temperature", which is a term often used to mean "reflected apparent temperature".

1.5

ambient temperature compensation

correction built into infrared instruments to provide automatic compensation of temperature readings affected by the ambient temperature

1.6
angular subtense
angular diameter of an optical system or subsystem

NOTE 1 Angular subtense is expressed in angular degrees or milliradians.

NOTE 2 In infrared thermography, the angle over which a sensing instrument collects radiant energy.

1.7
anomalous thermal image
observed thermal pattern of a structure that is not in accordance with the expected (reference) thermal pattern

1.8
anomaly
irregularity or abnormality in a system

EXAMPLE An irregularity, such as an anomalous thermal pattern or any indication that deviates from what is normally expected in the absence of any anomaly.

1.9
anti-reflectance coating
coating of infrared optical elements (lenses, windows) used to increase the sensitivity of a specified wavelength range through minimization or suppression of reflections causing signal loss

1.10
apparent temperature
uncompensated reading from an infrared thermography camera containing all radiation incident on the detector, regardless of its source

[ISO 18434-1:2008^[6], 3.1]

1.11
area effect
change in infrared radiometer output depending on the area of the measuring target

1.12
artefact
<1> product of artificial character due to an extraneous agency
<2> error caused by an uncompensated anomaly

EXAMPLE In thermography, an emissivity artefact simulates apparent variation of surface temperature.

1.13
atmospheric absorption
absorption of specific wavelengths of solar radiation, due largely to moisture, atmospheric gases and pollutants

1.14
atmospheric temperature
temperature of the atmosphere between the infrared camera and the object

1.15
atmospheric window
<infrared> any spectral interval within the infrared spectrum in which the atmosphere transmits radiant energy well (atmospheric absorption is minimal)

EXAMPLE Atmospheric windows are roughly defined to lie in the wavelength ranges:

- a) 0,78 μm to 2,0 μm in the near infrared (NIR);
- b) 2,0 μm to 5,5 μm in the mid-wave infrared (MWIR);
- c) 7,5 μm to 14,0 μm in the long-wave infrared (LWIR).

1.16

attenuating medium
material or other medium that attenuates infrared radiation emitted from a source

EXAMPLE Attenuating media include windows, filters, atmospheres, external optics.

1.17

blackbody
ideal perfect emitter and absorber of thermal radiation at all wavelengths

NOTE A blackbody is described by Planck's law. In its classical form, Planck's law describes the spectral distribution of the radiant energy emitted by a blackbody.

1.17.1

blackbody equivalent temperature
apparent temperature of a test object that is equal to the temperature of a blackbody emitting the same amount of radiant energy

1.17.2

blackbody radiator
radiator with the effective emissivity ε close to unity ($\varepsilon \geq 0,98$ across all relevant wavelengths)

1.17.3

blackbody reference
calibrated, traceable device used to check the calibration of infrared imaging radiometers or infrared thermometers

1.17.4

blackbody simulator
device whose radiation is close to that of a blackbody at the same temperature

EXAMPLE A cavity or a flat plate with a structured or coated surface characterized by a stable and uniform temperature and with emissivity close to 1.

1.18

centre wavelength
wavelength in the middle of the spectral sensitivity band of an infrared detector

1.19

cooled sensor
sensor that needs cooling to improve sensitivity to infrared radiant energy by reducing thermal noise influence

1.20

detecting element
sensitive part of a detector which is directly affected by the quantity to be measured

EXAMPLE For temperature-sensing devices: a thermocouple junction; resistive element; photoelectric, pyroelectric or quantum sensor.

1.21

differential blackbody
device for establishing two parallel isothermal planar zones of different temperatures and with effective emissivities close to 1,0

1.22

diffraction limit
limit of geometric diffraction of optical systems

1.23

diffuse reflector

lambertian reflector

surface that reflects incident radiation equally in all directions

NOTE 1 A lambertian diffuser is a surface that reflects a portion of the incident radiation in such a manner that the reflected radiation is equal in all directions, such as a gold perfect sphere.

NOTE 2 A mirror is not a diffuse reflector.

1.24

edge effect

(1) effect caused by measurement error mainly at the edge due to solid displacement or deformation by variable loading in thermoelastic stress measurement

(2) change in thermal properties at the edge of a target object as a result of different thermal conduction and convection properties

EXAMPLE Effect caused by measurement error at an edge due to solid displacement or deformation by variable loading in thermoelastic stress measurement.

1.25

effective emissivity

ε^*

measured emissivity value of a particular target surface under existing measurement conditions (rather than the generic tabulated value for the same material) that can be used to correct specific temperature readings

NOTE 1 Effective emissivity is also called emittance; however, the latter term is not preferred because it has been used to describe radiant exitance.

NOTE 2 Effective emissivity is context dependent, and is not purely a property of a material.

1.26

effective number of pixels

spatial resolution of a measured infrared image

NOTE The effective number of pixels is determined for a scanning infrared thermographic instrument according to the scanning pitch, and for an infrared thermographic instrument with an array sensor according to the number of pixels of the detector.

1.27

EMI/RFI noise

disturbance to electrical signals caused by electromagnetic interference (EMI) or radio frequency interference (RFI)

NOTE In infrared thermography, EMI/RFI noise can cause patterns to appear on the display and is sometimes due to poor grounding or earthing.

1.28

emissivity

ε

ratio of the radiance of a target surface to that of a blackbody at the same temperature and over the same spectral interval

1.29

emittance

ratio of the radiant flux emitted by a real target and that emitted by a blackbody at the same temperature and under the same conditions

NOTE 1 The total radiance, R^0 , is obtained by an integration of the monochromatic radiance between wavelengths zero and infinity.

$$R^0 = \int_0^{\infty} \frac{2\pi hc^2 \lambda^{-5}}{\exp\left(\frac{hc}{k\lambda T}\right) - 1} d\lambda = \frac{\sigma}{\pi} T^4$$

where

c is the speed of light in a vacuum;

h is the Planck constant;

k is the Boltzmann constant;

T is the thermodynamic temperature;

σ is the Stefan-Boltzmann constant, in watts per square metre per kelvin to the power four, given by

$$\sigma = \frac{2\pi k^4}{15c^2 h^3} = 5,67 \times 10^{-8}$$

Radiance and emittance being connected, the total emittance, M^0 , is given by

$$M^0 = \pi R^0 = \sigma T^4$$

NOTE 2 In thermography, the terms “radiance” and “emittance” are technically often used interchangeably.

NOTE 3 Refer to ISO 80000-7

1.30

environmental rating

rating assigned to an operating unit (typically an electrical or mechanical enclosure) to indicate the limits of the environmental conditions under which the unit functions reliably and within reported performance specifications

1.31

extended source

source of infrared radiation whose image fills completely or a larger part of the field of view of the infrared camera

1.32

field of view

field of vision

FOV

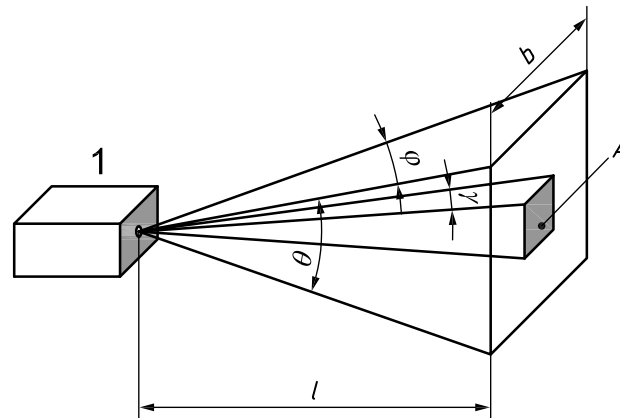
angular subtense over which an instrument integrates total incoming radiant energy

NOTE 1 Angular subtense is expressed in angular degrees or radians per side if rectangular or square and in angular degrees or radians if circular.

NOTE 2 In infrared thermometers, field of view defines the target spot size; in a scanning/staring imager, it defines the scan angle or picture size or a total field of view (TFOV).

NOTE 3 The field of view is the angular extent of the observable world that is seen at any given moment.

See Figure 1.



Key

- 1 detector
- A minimum detecting size
- b view
- l working distance
- γ instantaneous view angle (scanning type); spatial resolution (2D sensor type)
- θ vertical view angle
- φ horizontal view angle

Figure 1 — Field of view

1.33

fill factor

(focal plane arrays) ratio of the total surface of sensitive detector elements to the total area of the detector

1.34

filter

(infrared thermography) optical element, usually transmissive, which is used to limit spectral sensitivity of infrared detectors

1.35

fixed pattern noise

FPN

non-temporal variations between pixels that are exposed to the same scene radiation

NOTE These variations can be caused by non-linearities in the detector, non-perfections in gain and offset maps, and slow temporal changes that are too slow for the eye or brain to interpret as a temporal change. In uncooled detectors, the slow temporal term is, most of the time, the dominant term of the spatial noise equivalent temperature difference.

1.36

focal plane array

FPA

type of infrared detector which involves a one- or two-dimensional array consisting of many individual sensing elements (called "pixels")

NOTE Detector arrays are typically placed at the focal plane of an instrument. In thermography, rectangular or square FPAs are used in "staring" (non-scanning) infrared imagers. These are called IRFPA imagers.

1.37

focal point

(infrared thermography) image point conjugate to an infinitely distant object point on the optical axis

NOTE In infrared thermometers, this is where the spot size is the smallest. In scanning or staring imagers, this point corresponds to the minimum instantaneous field of view (IFOV).

1.38

foreground temperature

temperature of the scene behind and surrounding the instrument, as viewed from the target

NOTE 1 This is often referred to as 'Instrument background temperature' or as 'Observer background temperature'

NOTE 2 See ambient temperature.

1.39

frame averaging

addition of images and the division of their total for signal to noise ratio (signal level to noise level) improvement

1.40

frame repetition rate

number of full fields of view scanned per second

1.41

frame time

time needed to obtain signal information in all field elements, or pixels)

1.42

grey body

object whose emissivity is constant (less than 1) in a particular spectral range

1.43

image display tone

grey shade or colour hue on a thermogram

1.44

image processing

converting an image to digital form and further enhancing the image to prepare it for computer or visual analysis

NOTE For an infrared image or thermogram, image processing can include temperature scaling, spot temperature measurements, thermal profiles, image manipulation, subtraction, and storage.

1.45

imaging line scanner

line scanner

line-scanning (one-dimensional) device which images perpendicularly to a scan direction to produce a two-dimensional image of a scene

1.46

imaging radiometer

infrared thermal imager or point infrared sensor that can provide thermal images from which quantitative temperature measurements are possible

1.46.1

infrared camera

infrared thermography camera

IRT camera

instrument that collects the infrared radiant energy from a target and produces an image in monochrome (black and white) or colour, where the grey shades or colour hues are related to target apparent temperature distribution.

NOTE Such images are sometimes called infrared thermograms.

1.46.2

infrared imaging system
infrared thermal imager

instrument that converts spatial variations of surface infrared radiation to grey tones or colours corresponding to radiation power (temperature)

NOTE See infrared camera.

1.46.3

infrared thermographic instrument

instrument that converts infrared radiant energy to a temperature and displays a thermogram

1.47

indium antimonide

InSb

InSb is a narrow-gap semiconductor with an energy band gap of 0,17 eV at 300 K and spectral sensitivity in the range of 1 μm to 5 μm ; it is widely used as the sensor in infrared thermal imaging systems

NOTE Such detectors typically require cooling while in operation.

1.48

infrared

infrared radiation

IR

optical radiation for which the wavelengths are longer than those for visible radiation

NOTE 1 For infrared radiation, the range between 780 nm and 1 mm is commonly subdivided into:

— IR-A: 780 nm to 1 400 nm;

— IR-B: 1,4 μm to 3 μm ;

— IR-C: 3 μm to 1 mm.

[IEC 60050-845:1987^[7]]

NOTE 2 The range of infrared emitted by the source and which reaches the lens should be considered in the design of an infrared-absorbing material.

1.49

infrared bolometer

sensor that provides a signal; it employs an electrical conductance

1.49.1

infrared thermistor bolometer

thermistor configured so as to collect radiant infrared energy

1.49.2

infrared thermister bolometer

type of thermal infrared detector

1.50

infrared calibration source

blackbody simulator or other target of known temperature and effective emissivity used as a calibration reference

1.51

infrared detector

sensor which converts absorbed infrared radiation into an electrical signal

1.52

infrared fibre optic

flexible fibre made of a material that transmits infrared energy, used for non-contact temperature measurements in cases where there is no direct sight between the instrument and the target

1.53

infrared fibre optics

fibre optics which transmit infrared radiation

1.54

infrared focal plane array

IRFPA

one- or two-dimensional array of individual infrared sensing elements, typically used as a detector in infrared imaging instruments

1.55

infrared image

image that shows distribution of infrared radiant energy with colour hues or grey shades

1.56

infrared-imaging line scanner

infrared (one-dimensional) line-scanning device which images perpendicularly to a scan direction to produce a two-dimensional thermogram of a scene

1.57

infrared optical element

element that collects, transmits, restricts, refracts or reflects infrared energy as part of an infrared sensing or imaging instrument

1.58

infrared radiant energy

energy that is radiated and propagated as infrared, an electromagnetic wave whose wavelength is longer than visible light and shorter than 1 mm

1.59

infrared radiation thermometer

infrared non-imaging device allowing non-contact temperature measurement by sensing thermal radiation emitted by a target (target emissivity is to be known for measuring the “true” temperature)

1.60

infrared radiometer

equipment that measures infrared radiant energy

NOTE An infrared camera is a type of infrared radiometer.

1.61

infrared reflector

material with an excellent reflectance in the infrared region, close to 1,00

EXAMPLE Polished gold is an excellent infrared reflector commonly used in first surface mirrors.

1.62

infrared sensing device

instrument intended for the analysis of objects by the capture of their infrared radiation

EXAMPLE Infrared cameras, both imaging and staring, and infrared thermometers are the most typical infrared sensing devices.

1.63

infrared thermal detector

detector that absorbs infrared radiation and produces an electrical signal following changes of its temperature

EXAMPLE Measuring signals are changed to electrical resistance (bolometer), the thermal voltage (thermal element) and electrical polarization.

1.64

infrared thermographic testing

thermographic testing

inspection of materials and products using infrared thermography

1.65

infrared thermography

thermography infrared

IR thermography

technique allowing imaging of objects by sensing their emitted infrared (thermal) radiation

1.66

instantaneous field of view

IFOV

angular subtense energy or the angular projection of the detector element at the target plane

NOTE 1 The angular subtense is expressed in angular degrees or radians per side if rectangular, and angular degrees or radians if round.

NOTE 2 In infrared thermometers, instantaneous field of view defines the target spot size; in a line scanner or imager it represents a single resolution element in a scan line or a thermogram being a measure of spatial resolution.

NOTE 3 The instantaneous field of view is equivalent to the horizontal and vertical fields of view of an individual detector. For small detectors, the detector angular subtenses or projections α and β are defined by $\alpha = af/f$ and $\beta = bf/f$, where a and b are horizontal and vertical dimensions of the detector, and f is the effective focal length of the optics.

NOTE 4 Instantaneous field of view can be expressed as a solid angle in units of π .

NOTE 5 IFOVs may be different in the vertical (VIFOV) and horizontal (HIFOV) directions.

1.67

irradiance

radiant flux (power) per area incident on a given surface

NOTE Irradiance is expressed in watts per metre squared.

1.68

isotherm

zone marking an interval of equal apparent temperature in a thermogram

NOTE As an image enhancement feature, it replaces certain colours in the scale with a contrasting colour.

1.69

laser pyrometer

infrared radiation thermometer that projects a laser beam on to a target and uses the reflected laser energy to calculate the target effective emissivity and automatically correct the target temperature (assuming that the target is a diffuse reflector)

NOTE Laser pyrometers are not to be confused with laser-aiming infrared thermometers, where the laser is used to indicate a measured area.

1.70

limiting resolution

highest spatial frequency of a target that an imaging sensor is able to resolve

1.71

line scan rate

number of target lines scanned by an infrared scanner or imager in 1 s

1.72

load frequency range

range of load frequencies used in elastic stress measurement

1.73

lock-in technique

technique allowing for the extraction of a signal of known carrier wave from an extremely noisy environment. This signal can be, but should not be, restricted to temperature.

NOTE A common application is for non-destructive evaluation.

1.74

long-wave infrared

LWIR

wavelength range 7 μm to 14 μm , in which certain infrared instruments operate

1.75

measurement spatial resolution

IFOV_{meas}

MFOV

smallest target spot size on which an infrared camera can fulfil measurement, expressed in terms of angular subtense

NOTE 1 The angular subtense is expressed in milliradians.

NOTE 2 The slit response function (SRF) test and the hole response function (HRF) are used to measure IFOV_{meas}

1.76

mercury cadmium telluride

MCT

HgCdTe

material sensitive to infrared radiation in the spectral range of 1,5 μm to 14 μm and widely used as a detector in infrared imagers, especially in the 8-14 μm range.)

NOTE Such detectors typically require cooling while in operation.

1.77

mid-wave infrared

middle-wave infrared

MWIR

wavelength range 3 μm to 5 μm , in which certain infrared instruments operate

1.78

minimum detectable dimension

MDD

dimension or length of the smallest object that can be measured

1.79

minimum detectable temperature difference

MDTD

measure of the combined ability of an infrared imaging system and a human observer to detect a target at a particular temperature of unknown location against a vast uniform background having another temperature, the target being displayed on a monitor for a limited time

NOTE For a given target size, the MDTD is the minimum temperature difference between the target and its background at which the observer can detect the target. The standard target is a circle whose size is given by its angular subtense, and both the target and the background are isothermal black bodies.

1.80

minimum resolvable temperature difference

MRTD

measure of the ability of an infrared imaging system and the human observer to recognize periodic bar targets on a display

See Figure 2.

NOTE The MRTD is the minimum temperature difference between a standard periodic test pattern (7:1 aspect ratio, four bars) and the blackbody background at which an observer can resolve the pattern as the four-bar pattern.

1.81

modulation transfer function

MTF

measure of the ability of an imaging system to reproduce an image of a target

NOTE A formalized procedure is used to measure the modulation transfer function. It assesses the spatial resolution of a scanning or imaging system as a function of distance to the target.

1.82

motion compensation

correction of the measurement error caused by displacement or transformation of the measuring object

1.83

multi-element sensor

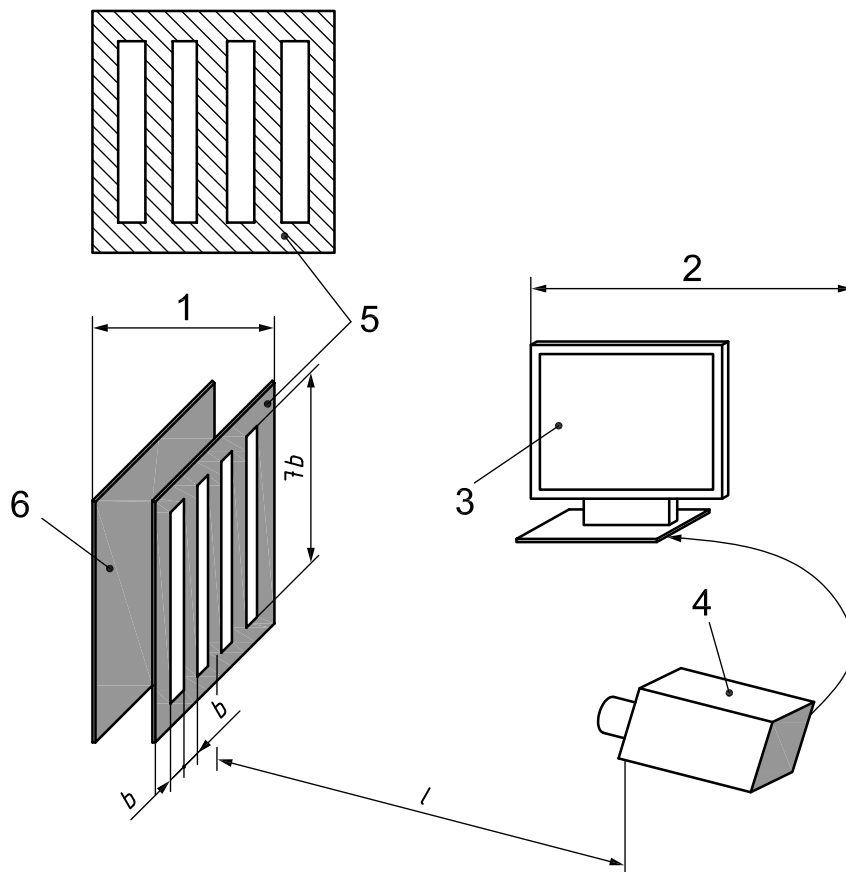
sensor that arranges infrared detectors in one dimension or two dimensions

1.84

near infrared

NIR

wavelength range 0,75 μm to 1,9 μm , in which certain infrared instruments operate

**Key**

- 1 test target
- 2 infrared imaging system
- 3 display
- 4 detector
- 5 near plate with rectangular slot
- 6 far plate
- b slot width
- l working distance

Figure 2 — Minimum resolvable temperature difference

1.85

noise equivalent temperature difference
NETD

target-to-background temperature difference between a blackbody target and its blackbody background at which the signal-to-noise ratio for a particular infrared instrument is equal to unity

NOTE Noise equivalent temperature difference is the result of both temporal and spatial noise, expressed in equivalence of temperature.

1.86

non-contact style

method for measuring temperature without a contact between the object and the sensor, typically, by object thermal radiation

1.87

non-grey body

object whose spectral radiation is not constant at all wavelengths unlike a grey body and a blackbody

NOTE 1 Such an object can be partially transparent to infrared radiation; also called a “coloured body” or “real body”.

NOTE 2 Almost all real objects are non-grey bodies in that their emissivity properties vary with temperature and wavelength; most have zero transmissivity. A non-grey body is also known as a “selective radiator”.

EXAMPLE Glass and plastics films.

1.88

non-uniformity correction

NUC

camera software-initiated picture correction for compensation of various sensitivities of individual sensing elements in array detectors (FPA-cameras), as well as other disturbances of an optical or geometric nature

NOTE Some cameras perform a “manual non-uniformity correction” where the lens cap is put in front of the lens while the NUC is performed.

1.89

number of pixels

number of units of picture elements (pixel) that compose a thermal image or infrared image displayed on a monitor

1.90

object plane resolution

dimension in the object plane that corresponds to the product of the system instantaneous field of view and the specified distance between the infrared instrument and the object

1.91

observer background radiation

total radiation emitted by background objects and reflected from a target

1.92

opaque

impervious to radiant energy

NOTE In thermography, opaque materials do not transmit thermal infrared energy ($\tau = 0$).

1.93

passive thermography

thermographic technique for inspecting objects or installations by measuring their emitted thermal radiation, without using any additional energy source for thermal stimulation

1.94

peak hold

feature of an instrument whereby an output signal is maintained at the peak instantaneous measurement for a specified duration

1.95

permissible uncertainty

uncertainty value specified in the technical documentation, at which the blackbody radiator is considered fit for its intended use

NOTE Degrees Celsius or kelvin are used as temperature units.

1.96

phase adjustment

{infrared thermography} adjustment of the phase of a “signal that is synchronized to heat or load to the measuring object” and “actual temperature change”

1.97

photodetector
 photonic detector
 quantum detector

infrared detector whose operating principle is based on using the internal or external photoeffect (in the capture of incoming photons)

NOTE These detectors are characterized by fast response (of the order of microseconds), a limited spectral response, and usually their need for cooling while in operation. They are widely used in infrared imagers and thermometers.

1.98

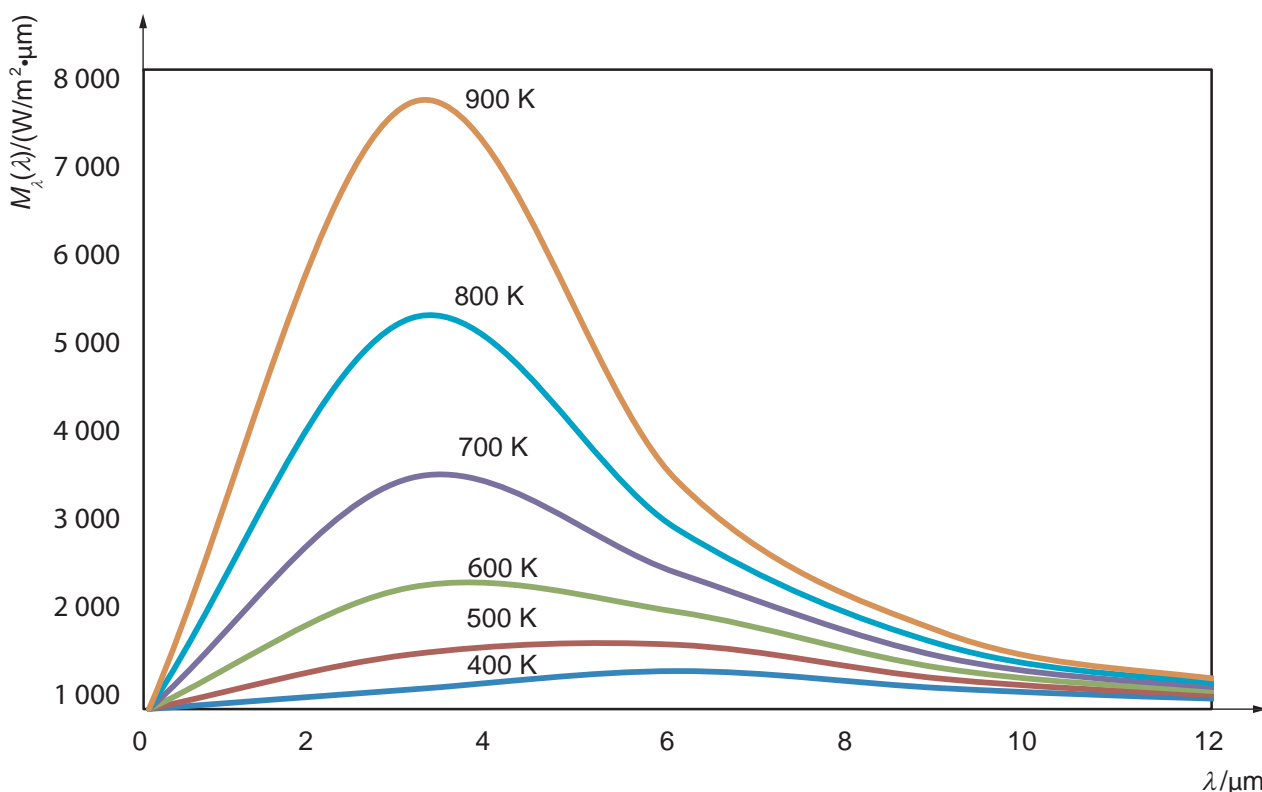
Planck's law

law establishing the spectral radiance of unpolarised electromagnetic radiation at all wavelengths emitted by a black bod, at an absolute temperature $T(K)$

See Figure 3.

NOTE This law was formulated by Max Planck in 1900.

EXAMPLE For the purposes of thermography, Planck's law is best shown by a set of curves of spectral radiant exitance against wavelength.

**Key**

$M_{\lambda}(\lambda)$ spectral radiant exitance
 λ wavelength

Figure 3 — Blackbody curves at various temperatures

1.99

point source

source whose linear dimensions are very small compared to the distance between the source and the infrared instrument

NOTE The irradiance varies inversely with the square of the distance, a unique property of point sources.

1.100

pulsed phase thermography

PPT

processing technique used in pulsed thermography and in which data are analysed in the frequency domain rather than in the time domain

NOTE Phase data are often of particular interest.

1.101

pulsed thermography

active infrared thermographic inspection technique, in which a test sample is stimulated with a pulse of energy and recorded infrared image sequences are analysed to enhance defect "visibility" and to characterize defect parameters

1.102

pyroelectric detector

type of thermal infrared detector that operates as a current source, with its output being proportional to the rate of a detector temperature change

1.103

pyroelectric vidicon

PEV

pyrovidicon

video camera tube whose receiving element is fabricated of a pyroelectric material and which is sensitive to wavelengths from about 2 μm to 20 μm ; used in infrared thermal viewers

NOTE At the time of publication, these devices are becoming obsolete.

1.104

pyrometer

instrument used to infrared thermometer

EXAMPLE Radiation or brightness pyrometers measure visible energy and relate it to brightness or colour temperature. Infrared pyrometers measure infrared radiation and relate it to the target surface temperature.

1.105

qualitative infrared examination

qualitative thermography

technique which relies on the analysis of thermal patterns to reveal the existence and locate the position of anomalies

1.106

quantitative infrared examination

quantitative thermography

technique which uses quantitative temperature measurement to determine the seriousness of an anomaly, in order to establish repair priorities

1.107

quantum well infrared photodetector

QWIP detector

special type of infrared detector which uses the effect of photo-excitation of electrons (holes) between the base and the first excitation levels in the conduction (valence) band of so-called quantum wells

NOTE Special cases are QWIPs.

1.108

radiance

L

thermal flux per projected area per solid angle leaving a source or, in general, any reference surface

NOTE At a point on a surface of a source and in a given direction.

$$L = \frac{dI}{dA} \frac{1}{\cos \alpha}$$

where

dI is the radiant intensity emitted from an element of the surface with area dA ;

α is the angle between the normal to the surface and the given direction.

[ISO 80000-7:2008^[5], 7.15]

1.109

radiant exitance

radiosity

M

total infrared energy (radiant flux) leaving a target surface

NOTE 1 Radiant exitance includes radiated, reflected and transmitted components. Only the radiated component is related to the target surface temperature.

NOTE 2 At a point on a surface,

$$M = \frac{d\Phi}{dA}$$

where $d\Phi$ is the radiant flux leaving the element of the surface with area dA .

[ISO 80000-7:2008^[5], 7.18]

1.110

radiation reference source

blackbody-like or other target of a known temperature and effective emissivity used as a reference to obtain optimum measurement accuracy, ideally, traceable to relevant national or International Standards

1.111

radiation thermometer

radiometer

instrument for non-contact temperature measurement by object thermal radiation

NOTE Instrument calibration and material emissivity values are required to convert apparent temperatures into "true" temperatures

1.112

radiometric temperature measurement

measurement made by using an infrared system which converts radiant energy into temperature

NOTE Radiometric data should be corrected for emissivity, atmosphere transmission, and reflected apparent temperature.

1.113

ratio pyrometer

bi-colour pyrometer

infrared thermometer that uses the ratio of incoming infrared radiant energy in two separated wavelengths in order to determine target temperature independently of its emissivity

NOTE A ratio pyrometer assumes "grey body" conditions and is normally limited to relatively hot targets (above 300 °C).

1.114

recognition

ability to differentiate between different types of thermal patterns such as board-stock, picture-framed and amorphous

NOTE Recognition of thermal anomalies can be accomplished when their dimensions are at least several times greater than a pixel size on a test object.

1.115

reflected apparent temperature

T_{refl}

apparent temperature of other objects that are reflected by the target into the infrared thermography camera

[ISO 18434-1:2008^[6], 3.12]

NOTE 1 This is one of the most important definitions in thermography because it is the temperature of the sink for the thermal energy radiated by the target. Making an erroneous assumption about this leads to considerable errors in estimation of the target temperature.

NOTE 2 Reflected apparent temperature was previously known as “reflected ambient temperature”, “reflected temperature” or sometimes just “ambient temperature”.

1.116

reflection coefficient

ρ

(infrared thermography) ratio of reflected radiation energy from a body to the total radiation incident on the body

NOTE The reflection coefficient is dimensionless and quantifies the reflection capability of a body.

1.116.1

reflectivity

reflectance

ratio of the total reflected energy from a surface to total incident energy on that surface

NOTE 1 $\rho = 1 - \varepsilon - \tau$ [where ε is emissivity; τ is transmittance]; for a [perfect] mirror, reflectivity approaches 1,0; for a blackbody, $\rho = 0$.

NOTE 2 Technically, reflectivity is the ratio of the intensity of the reflected radiation to the total radiation; reflectance is the ratio of the reflected flux to the incident flux.

[ISO 18434-1:2008^[6], 3.11]

NOTE 3 “Reflectivity”, “reflectance”, and “reflection coefficient” are often used interchangeably.

NOTE 4 [Expressed mathematically]:

$$\rho = \frac{\Phi_r}{\Phi_m}$$

where

Φ_r is the reflected radiant flux or the reflected luminous flux;

Φ_m is the radiant flux or luminous flux of the incident radiation.

[ISO 80000-7:2008^[5], 7-22.2]

1.117

short-wave infrared

SWIR

wavelength range 1 μm to 3 μm , in which certain infrared instruments operate

1.118
single element sensor
sensor that consists of one infrared detector

1.119
slit response function
SRF
measure of the measurement spatial resolution (IFOV_{meas} or MFOV) of a scanning infrared

1.120
spatial frequency
measure of details in terms of equivalent, uniformly spaced, cyclical patterns

NOTE 1 In an object or image plane, spatial frequency can be expressed in cycles per millimetre or line pairs per millimetre.

NOTE 2 In an imaging system, spatial frequency can be expressed in terms of cycles per milliradian or line pairs per milliradian.

1.121
spatial measurement resolution
measurement-spot size in terms of working distance which is connected to SRF, HRF, etc.

NOTE 1 In an infrared radiation thermometer, spatial measurement resolution is expressed in milliradians or as a ratio of the target-spot size (containing 95 % of the radiant energy, according to common usage) to the working distance. In scanners, cameras, and imagers, spatial measurement resolution is most often expressed in milliradians.

NOTE 2 Adapted from ISO 18434-1:2008^[6], 3.14.

1.122
spectral absorption coefficient
 α_λ
wavelength-dependent absorption coefficient

NOTE Linear absorption coefficient:

$$\alpha(\lambda) = \frac{1}{\Phi_\lambda(\lambda)} \frac{d\Phi_\lambda(\lambda)}{dl}$$

where $d\Phi/\Phi$ is the relative decrease, caused by absorption, in the spectral radiant flux Φ of a collimated beam of electromagnetic radiation corresponding to the wavelength λ during traversal of an infinitesimal layer of a medium and dl is the length traversed.

[ISO 80000-7:2008^[5], 7-25.2]

1.123
spectral emissivity
 ε_λ
wavelength-dependent emissivity

NOTE [Expressed mathematically]:

$$\varepsilon(\lambda) = \frac{M_\lambda(\lambda)}{M_{b,\lambda}(\lambda)}$$

where

$M_\lambda(\lambda)$ is the spectral radiant exitance of a thermal radiator;

$M_{b,\lambda}(\lambda)$ is the spectral radiant exitance of a blackbody at the same temperature.

[ISO 80000-7:2008^[5], 7-21.2]

1.124
spectral reflection coefficient

ρ_{λ}
wavelength-dependent reflection coefficient

1.125
spectral response
spectral wavelength interval over which an instrument or sensor responds to infrared radiant energy

NOTE 1 Spectral response is expressed in micrometres.

NOTE 2 Spectral response can be plotted on a spectral response curve of a particular infrared detector (infrared camera).

1.126
spectral transmission coefficient

τ_{λ}
wavelength-dependent transmission coefficient

1.127
specular reflector
smooth surface that reflects most (total) incident radiant energy at an angle complementary (equal about the normal) to the angle of incidence

EXAMPLE A mirror.

1.128
spherical aberration
lens geometry-dependent display fault of a lens

EXAMPLE For lenses whose surfaces can be described by spherical segments, axis far boundary radiation is not displayed exactly at the focal point or a point in the picture level.

1.129
spot
instantaneous area (quantified by its diameter, unless otherwise specified) at the target plane that is being measured by an instrument

NOTE In infrared thermometry, a spot is specified by most manufacturers to contain 95 % of the radiant energy emitted by an infinitely large target of the same temperature and emissivity.

1.130
spot radiometer
non-imaging device that senses infrared radiation and that can be calibrated in temperature of thermal flux power density

1.131
standard large aperture radiator
standard (reference) radiator, with angular dimensions several times greater than the elementary field of view of a given thermographic instrument

1.132
standard radiator
radiator which simulates a blackbody

1.133
standard slit pattern
slit pattern introduced into a standard specimen used for the estimation of minimum resolvable temperature difference

1.134

storage operating range

temperature extremes over which an instrument can be stored and, subsequently, operated within reported performance specifications

1.135

stress resolution

resolution of stress achieved by measuring thermoelastic stresses

NOTE Stress resolution is applied to temperature resolution of an infrared instrument.

1.136

surface-modifying material

tape, spray or paint used to modify (enhance) emissivity of test samples

1.137

target background

set of objects and the atmosphere in the vicinity of a test object that is observed by an infrared camera and which can affect the thermal pattern of the test object

1.138

target plane

plane perpendicular to the sight direction of a radiation thermometer that is in focus for that instrument

1.139

target size

diameter of a circle in the target plane of a radiation thermometer that is centred on its sight direction and which contains 99 % of the input radiant power received by that instrument

1.140

temperature difference imaging technique

signal-processing method to obtain a picture of the change of the sum of principal stresses, consisting of measuring temperature distribution images during the maximum temperature period and the minimum temperature period, and making an overall "temperature range image" from the images

NOTE Range means the total amplitude.

1.141

temperature drift

reading change (error) in time when observing a target with non-varying temperature, which can be caused by a combination of ambient factors and variation in voltage and instrument characteristics

1.142

temperature maintenance instability

instability of a blackbody radiator temperature, i.e. standard deviation of blackbody radiator temperature values measured every 10 s to 15 s during 15 min to 20 min with reference to their arithmetic mean value during the same period

1.143

temperature resolution

minimum simulated or actual change in the target temperature that produces a temperature signal identified by an observer (typically, at the signal-to-noise ratio equal to unity)

NOTE This is equivalent to NETD. See NETD.

1.144

thermal anomaly

surface thermal pattern which deviates from a reference (expected) thermal pattern

1.145

thermal contrast

degree of detectable temperature difference between adjacent areas or objects having unequal temperatures at a particular moment

NOTE Thermal contrast is a processing technique used to enhance target visibility. In its simplest form, a thermal contrast is computed by calculating the difference between the temperature of the target and the temperature of a (sound) reference area.

1.146

thermal diffusivity

α

ratio of conductivity, χ , to the product of density, ρ , and specific heat, c_p

$$\alpha = \frac{\chi}{\rho c_p}$$

NOTE 1 Thermal diffusivity is expressed in metres squared per second.

NOTE 2 Thermal diffusivity is the ability of a material to diffuse thermal energy after a change in heat input. A body with a high diffusivity reaches a uniform temperature distribution faster than a body with a lower diffusivity.

1.147

thermal effusivity

thermal inertia

e

measure of the resistance of a material to a temperature change

NOTE 1 Expressed mathematically

$$e = (\chi \rho c_p)^{1/2}$$

where

χ is the thermal conductivity;

ρ is the bulk density;

c_p is the specific heat capacity.

NOTE 2 Thermal effusivity is expressed in watts squared root second per square metre kelvin.

1.148

thermal pattern

area on an infrared thermogram of a particular shape and amplitude

NOTE A thermal pattern is often used to identify thermal anomalies.

1.149

thermal radiation

mode of energy flow that occurs by emission and absorption of electromagnetic radiation, propagating at the speed of light

NOTE Unlike conductive and convective heat flow, thermal radiation is capable of propagating across a vacuum, a form of heat transfer which allows IRT to work since infrared energy travels from the target to the detector by radiation.

1.150

thermal resolution

smallest apparent temperature difference between two blackbodies that can be measured by an infrared sensing device

1.151

thermal test object

device producing a special thermal pattern of a specific spatial frequency, shape or temperature on a uniformly radiating background with known temperature and emissivity of both the object and the background

1.152

thermal tomography

processing technique used in pulsed thermography and in which data are analysed by reference to a particular instant of interest such as the time of maximum thermal contrast

1.153

thermal wave imaging

active infrared thermographic inspection technique, in which a test sample is stimulated with periodical pulses of thermal energy and recorded infrared image sequences are analysed to enhance defect “visibility” and characterize defect parameters

NOTE Sometimes this term is applied to pulsed infrared thermographic non-destructive testing.

1.154

thermistor

temperature detector, usually a semiconductor, whose resistivity changes predictably with increasing temperature

1.155

thermoelastic coefficient

proportional coefficient of “temperature change” and “product of object temperature and change of the sum of principal stresses by thermoelastic effect”

NOTE The thermoelastic coefficient, k_t , in reciprocal pascals, is material constant and is given by the equation.

$$k_t = \frac{\alpha_l}{\rho c_p}$$

where

α_l	is the coefficient of linear thermal expansion, in reciprocal kelvins;
ρ	is the material density, in kilograms per metre cubed;
c_p	is the specific heat at constant pressure, in joules per kilogram per kelvin.

1.156

thermoelastic effect

phenomenon in which temperature changes with adiabatic elastic deformation of an object

NOTE Temperature generally decreases with tension and increases with compression. Temperature change, ΔT , in kelvins, is proportional to the change in the sum of principal stresses:

$$\Delta T = -k_t T \Delta \sigma$$

where

k_t	is the thermoelastic coefficient, in reciprocal pascals;
T	is the object temperature, in kelvins;
$\Delta \sigma$	is the change in the sum of principal stresses, in pascals.

1.157

thermoelastic apparatus (stress measuring)

instrument that measures stress distribution in a measuring object based on the thermoelastic effect

1.158

thermoelastic method (stress measuring)

method that measures distribution of surface temperature change in a measurement object using the thermoelastic effect with an infrared thermography instrument and converts and displays the distribution of the sum of principal stress change

1.159

thermogram

thermal map or image of a target where the grey tones or colour hues represent the distribution of infrared thermal radiant energy over the surface of the target

[ISO 18434-1:2008^[6], 3.17]

1.160

thermographic signal reconstruction

TSR

signal-processing technique for reconstructing and improving time-resolved thermal images, used in pulsed thermography material testing and based on polynomial fitting of the temperature decay

1.161

thermology

(medical applications) thermography

1.162

thermometer

device used to measure temperature

1.163

thermopile

device constructed from thermocouples in series to add the thermoelectric voltage

NOTE A radiation thermopile has junctions arranged so as to collect infrared radiant energy from a target, i.e. it is a type of thermal infrared detector.

1.164

total field of view

TFOV

total solid angle scanned view, usually rectangular in cross-section, in imagers

1.165

transfer calibration

technique for correcting a temperature measurement or a thermogram for various errors by placing a radiation reference adjacent to the target

1.166

transfer standard

precision radiometric measurement instrument whose calibration is traceable to national or international standards which is used to calibrate radiation reference sources

1.167

transmission coefficient

ratio of the radiation energy transmitted through a body to the total incident radiation

1.168

transmissivity

τ

transmittance

proportion of infrared radiant energy impinging on an object surface, for any given spectral interval, that is transmitted through the object

NOTE 1

$$\tau = 1 - \varepsilon - \rho$$

where

τ is transmissivity;

ε is emissivity;

ρ is reflectivity.

[ISO 18434-1:2008^[6], 3.18]

NOTE 2 “Transmissivity” and “reflectance” are often used interchangeably.

NOTE 3 Transmissivity is that fraction of incident radiation transmitted by matter.

$$\tau = \frac{\Phi_t}{\Phi_m}$$

where

Φ_t is the transmitted radiant flux or luminous flux;

Φ_m is the radiant flux or luminous flux of the incident radiation.

(Adapted from ISO 80000-7:2008^[5], 7-47.3.)

EXAMPLE For a blackbody, $\tau = 0$.

1.169

transmitting medium

composition of the measurement path between a target and a measuring instrument through which radiant energy propagates

NOTE The transmitting medium can be a vacuum, gaseous (such as air), solid, liquid or any combination of these.

1.170

vibrothermography

thermographic technique for examining an object where temperature differences are produced by mechanical vibrations

Bibliography

- [1] ISO 6781:1983, *Thermal insulation — Qualitative detection of thermal irregularities in building envelopes — Infrared method*
- [2] ISO 10241-1, *Terminological entries in standards — Part 1: General requirements and examples of presentation*
- [3] ISO 9712:2005, *Non-destructive testing — Qualification and certification of personnel*
- [4] ISO 80000-5, *Quantities and units — Part 5: Thermodynamics*
- [5] ISO 80000-7:2008, *Quantities and units — Part 7: Light*
- [6] ISO 18434-1:2008, *Condition monitoring and diagnostics of machines — Thermography — Part 1: General procedures*
- [7] IEC 60050-845:1987, *International electrotechnical vocabulary — Lighting*
- [8] OIML TC 11/SC 3¹⁾, *Standard black body radiator for the temperature range from –50 °C to 2 500 °C*
- [9] OIML R 141, *Procedure for calibration and verification of the main characteristics of thermographic instruments*
- [10] ASTM C1060-90(2003), *Standard practice for thermographic inspection of insulation installations in envelope cavities of frame buildings*
- [11] ASTM C1153-97(2003)e1, *Standard practice for location of wet insulation in roofing systems using infrared imaging*
- [12] ASTM E1543-00(2000), *Standard test method for noise equivalent temperature difference of thermal imaging systems*
- [13] ASTM E1897-97(2002)e1, *Standard test methods for measuring and compensating for transmittance of an attenuating medium using infrared imaging radiometers*
- [14] ASTM E1933-99a(2005)e1, *Standard test methods for measuring and compensating for emissivity using infrared imaging radiometers*
- [15] ASTM E1934-99a(2005)e1, *Standard guide for examining electrical and mechanical equipment with infrared thermography*
- [16] JIS Z 2300:2009, *Terms and definitions of non-destructive testing*
- [17] JIS Z 8710:1993, *Temperature measurement — General requirement*

1) In preparation.

Alphabetical index

- A**
- absorptance 1.1
 - absorptance coefficient 1.1
 - absorptivity 1.1
 - active thermography 1.2
 - ambient operating range 1.3
 - ambient temperature 1.4
 - ambient temperature compensation 1.5
 - angular subtense 1.6
 - anomalous thermal image 1.7
 - anomaly 1.8
 - anti-reflectance coating 1.9
 - apparent temperature 1.10
 - area effect 1.11
 - artefact 1.12
 - atmospheric absorption 1.13
 - atmospheric temperature 1.14
 - atmospheric window 1.15
 - attenuating medium 1.16
- B**
- bi-colour pyrometer 1.113
 - blackbody 1.17
 - blackbody equivalent temperature 1.17.1
 - blackbody radiator 1.17.2
 - blackbody reference 1.17.3
 - blackbody simulator 1.17.4
- C**
- centre wavelength 1.18
 - cooled sensor 1.19
- D**
- detecting element 1.20
 - differential blackbody 1.21
 - diffraction limit 1.22
 - diffuse reflector 1.23
- E**
- edge effect 1.24
 - effective emissivity 1.25
 - effective number of pixels 1.26
 - EMI/RFI noise 1.27
 - emissivity 1.28
 - emittance 1.29
 - environmental rating 1.30
 - extended source 1.31
- F**
- field of view 1.32
 - field of vision 1.32
 - fill factor 1.33
 - filter 1.34
 - fixed pattern noise 1.35
 - focal plane array 1.36
 - focal point 1.37
 - foreground temperature 1.38
 - FOV 1.32
 - FPA 1.36
 - FPN 1.35
 - frame averaging 1.39
 - frame repetition rate 1.40
 - frame time 1.41
- G**
- grey body 1.42
- H**
- HgCdTe 1.76
- I**
- IFOV 1.66
 - IFOV_{meas} 1.75
 - image display tone 1.43
 - image processing 1.44
 - imaging line scanner 1.45
 - imaging radiometer 1.46
 - indium antimonide 1.47
 - infrared 1.48
 - infrared bolometer 1.49
 - infrared calibration source 1.50
 - infrared camera 1.46.1
 - infrared detector 1.51
 - infrared fibre optic 1.52
 - infrared fibre optics 1.53
 - infrared focal plane array 1.54
 - infrared image 1.55
 - infrared imaging system 1.46.2
 - infrared optical element 1.57
 - infrared radiant energy 1.58
 - infrared radiation 1.48
 - infrared radiation thermometer 1.59
 - infrared radiometer 1.60
 - infrared reflector 1.61
 - infrared sensing device 1.62
 - infrared thermal detector 1.63
 - infrared thermal imager 1.46.2,
 - infrared thermister bolometer 1.49.2
 - infrared thermistor bolometer 1.49.1
- infrared thermographic instrument** 1.46.3
- infrared thermographic testing** 1.64
- infrared thermography** 1.65
- infrared thermography camera** 1.46.1
- infrared-imaging line scanner** 1.56
- InSb** 1.47
- instantaneous field of view** 1.66
- IR** 1.48
- IR thermography** 1.65
- IRFPA** 1.54
- irradiance** 1.67
- IRT camera** 1.46.1
- isotherm** 1.68
- L**
- lambertian reflector 1.23
 - laser pyrometer 1.69
 - limiting resolution 1.70
 - line scan rate 1.71
 - line scanner 1.45
 - load frequency range 1.72
 - lock-in technique 1.73
 - long-wave infrared 1.74
 - LWIR 1.74
- M**
- MCT 1.76
 - MDD 1.78
 - MDTD 1.79
 - measurement spatial resolution 1.75
 - mercury cadmium telluride 1.76
 - MFOV 1.75
 - middle-wave infrared 1.77
 - mid-wave infrared 1.77
 - minimum detectable dimension 1.78
 - minimum detectable temperature difference 1.79
 - minimum resolvable temperature difference 1.80
 - modulation transfer function 1.81
 - motion compensation 1.82
 - MRTD 1.80
 - MTF 1.81
 - multi-element sensor 1.83
 - MWIR 1.77
- N**
- near infrared 1.84
 - NETD 1.85

NIR 1.84
 noise equivalent temperature
 difference 1.85
 non-contact style 1.86
 non-grey body 1.87
 non-uniformity correction 1.88
 NUC 1.88
 number of pixels 1.89

O

object plane resolution 1.90
 observer background
 radiation 1.91
 opaque 1.92

P

passive thermography 1.93
 peak hold 1.94
 permissible uncertainty 1.95
 PEV 1.103
 phase adjustment 1.96
 photodetector 1.97
 photonic detector 1.97
 Planck's law 1.98
 point source 1.99
 PPT 1.100
 pulsed phase thermography 1.100
 pulsed thermography 1.101
 pyroelectric detector 1.102
 pyroelectric vidicon 1.103
 pyrometer 1.104
 pyrovidicon 1.103

Q

qualitative infrared
 examination 1.105
 qualitative thermography 1.105
 quantitative infrared
 examination 1.106
 quantitative thermography 1.106
 quantum detector 1.97
 quantum well infrared
 photodetector 1.107
 QWIP detector 1.107

R

radiance 1.108
 radiant exitance 1.109
 radiation reference source 1.110
 radiation thermometer 1.111
 radiometer 1.111
 radiometric temperature
 measurement 1.112
 radiosity 1.109
 ratio pyrometer 1.113

recognition 1.114
 reflectance 1.116.1
 reflected apparent
 temperature 1.115
 reflection coefficient 1.116
 reflectivity 1.116.1

S

short-wave infrared 1.117
 single element sensor 1.118
 slit response function 1.119
 spatial frequency 1.120
 spatial measurement
 resolution 1.121
 spectral absorption
 coefficient 1.122
 spectral emissivity 1.123
 spectral reflection
 coefficient 1.124
 spectral response 1.125
 spectral transmission
 coefficient 1.126
 specular reflector 1.127
 spherical aberration 1.128
 spot 1.129
 spot radiometer 1.130
 SRF 1.119
 standard large aperture
 radiator 1.131
 standard radiator 1.132
 standard slit pattern 1.133
 storage operating range 1.134
 stress resolution 1.135
 surface-modifying material 1.136
 SWIR 1.117

T

target background 1.137
 target plane 1.138
 target size 1.139
 temperature difference imaging
 technique 1.140
 temperature drift 1.141
 temperature maintenance
 instability 1.142
 temperature resolution 1.143
 TFOV 1.164
 thermal anomaly 1.144
 thermal contrast 1.145
 thermal diffusivity 1.146
 thermal effusivity 1.147
 thermal inertia 1.147
 thermal pattern 1.148
 thermal radiation 1.149
 thermal resolution 1.150
 thermal test object 1.151
 thermal tomography 1.152
 thermal wave imaging 1.153
 thermistor 1.154

thermoelastic apparatus (stress-
 measuring) 1.157
 thermoelastic coefficient 1.155
 thermoelastic effect 1.156
 thermoelastic method (stress
 measurement) 1.158
 thermogram 1.159
 thermographic signal
 reconstruction 1.160
 thermographic testing 1.64
 thermography infrared 1.65
 thermology 1.161
 thermometer 1.162
 thermopile 1.163
 total field of view 1.164
 transfer calibration 1.165
 transfer standard 1.166
 transmission coefficient 1.167
 transmissivity 1.168
 transmittance 1.168
 transmitting medium 1.169
 TSR 1.160

V

vibrothermography 1.170

