



INTERNATIONAL STANDARD ISO 11564:1998
TECHNICAL CORRIGENDUM 1

Published 2000-04-01

INTERNATIONAL ORGANIZATION FOR STANDARDIZATION • МЕЖДУНАРОДНАЯ ОРГАНИЗАЦИЯ ПО СТАНДАРТИЗАЦИИ • ORGANISATION INTERNATIONALE DE NORMALISATION

Stationary source emissions — Determination of the mass concentration of nitrogen oxides — Naphthylethylenediamine photometric method

TECHNICAL CORRIGENDUM 1

Emissions de sources fixes — Détermination de la concentration en masse des oxydes d'azote — Méthode photométrique à la naphtyléthylène diamine (NEDA)

RECTIFICATIF TECHNIQUE 1

Technical Corrigendum 1 to International Standard ISO 11564:1998 was prepared by Technical Committee ISO/TC 146, *Air quality*, Subcommittee SC 1, *Stationary source emissions*.

Page 1

1 Scope

In the second paragraph after the note, change "... for a sample gas volume of 1000 ml." to read "... for a sample gas volume of 500 ml."

Replace the existing Figure 6 with the Figure 6 shown below, in which the curves designating 1 cm pathlength and 5 cm pathlength have been interchanged.

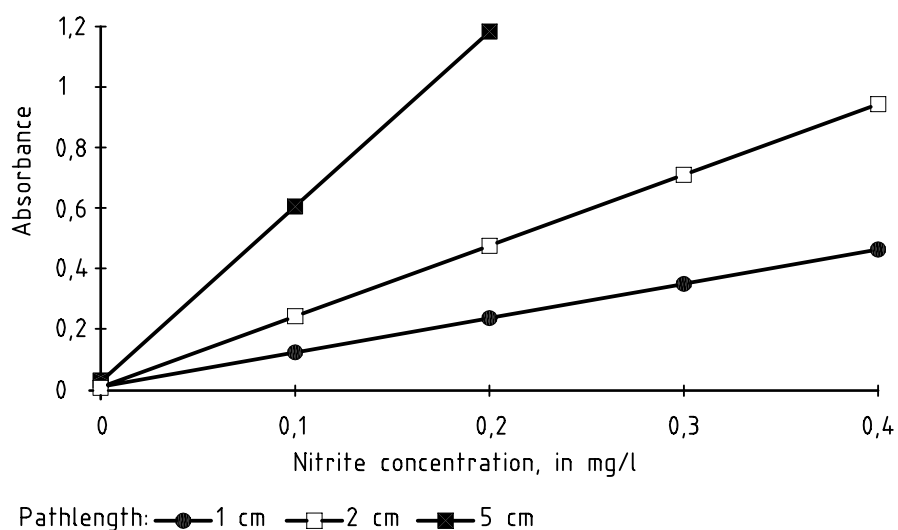


Figure 6 — Calibration curve for nitrogen oxides (example)