

---

---

**Olive oils and olive-pomace oils —  
Determination of aliphatic alcohols  
content by capillary gas chromatography**

*Huiles d'olive et huiles de grignons d'olive — Détermination de la teneur  
en alcools aliphatiques par chromatographie en phase gazeuse sur  
colonne capillaire*



**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2010

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

Foreword .....	iv
Introduction.....	v
1 Scope .....	1
2 Normative references .....	1
3 Terms and definitions .....	1
4 Principle.....	1
5 Reagents.....	1
6 Apparatus .....	2
7 Sampling.....	3
8 Preparation of the test sample .....	3
9 Procedure .....	4
9.1 Preparation of the unsaponifiable matter .....	4
9.2 Separation of alcoholic fractions.....	4
9.3 Preparation of the trimethylsilyl ethers.....	5
9.4 Gas chromatographic analysis .....	6
10 Precision.....	7
10.1 Interlaboratory test.....	7
10.2 Repeatability .....	7
10.3 Reproducibility .....	7
11 Test report.....	8
Annex A (informative) Determination of the linear velocity of the gas .....	9
Annex B (informative) Results of an interlaboratory test .....	10
Bibliography.....	11

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 12871 was prepared by Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 11, *Animal and vegetable fats and oils*.

.....

## Introduction

As part of the *Trade standard applying to olive oils and olive-pomace oils*, the International Olive Oil Council (IOOC) — now known as the International Olive Council (IOC) — published COI/T.20/Doc. 26:2003<sup>[4]</sup>. COI/T.20/Doc. 26 was applicable to olive and olive-pomace oils and was used to distinguish between lampante virgin olive oils and crude olive-pomace oils. Olive pomace is the residual paste which still contains a variable amount of water and oil after pressing or centrifuging.

In 2008, the IOC submitted the document to ISO/TC 34/SC 11 for adoption as an International Standard.

© ISO 2010. All rights reserved.

.....

# Olive oils and olive-pomace oils — Determination of aliphatic alcohols content by capillary gas chromatography

## 1 Scope

This International Standard specifies a procedure for the determination of the content, as a mass fraction expressed as milligrams per kilogram, of aliphatic alcohols in olive oils and olive-pomace oils.

NOTE This International Standard is based on COI/T.20/Doc. 26:2003<sup>[4]</sup>.

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 661, *Animal and vegetable fats and oils — Preparation of test sample*

## 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

### 3.1

#### aliphatic alcohols content

sum of the aliphatic alcohols with carbon number  $C_{22}$ ,  $C_{24}$ ,  $C_{26}$ , and  $C_{28}$ , as a mass fraction, determined according to the method specified in this International Standard

## 4 Principle

The oil, to which 1-eicosanol has been added as an internal standard, is saponified with ethanolic potassium hydroxide and the unsaponifiable matter extracted with diethyl ether. The alcoholic fraction is separated from the unsaponifiable matter by chromatography on a basic silica gel plate; the alcohols recovered from the silica gel are transformed into trimethylsilyl ethers (TMSE) and analysed by capillary gas chromatography.

## 5 Reagents

**WARNING — Comply with any local regulations which specify the handling of hazardous substances. Technical, organizational and personal safety measures shall be followed.**

During the analysis, unless otherwise stated, use only reagents of recognized analytical grade, and distilled or demineralized water or water of equivalent purity.

### 5.1 Potassium hydroxide, ethanolic solution, $c(\text{KOH}) \approx 2 \text{ mol/l}$ .

Dissolve, while cooling, 130 g potassium hydroxide [ $w(\text{KOH}) = 85 \%$  mass fraction minimum] in 200 ml water and make up to 1 l with ethanol. Store the solution in a well-stoppered opaque glass bottle.

## ISO 12871:2010(E)

**5.2 Potassium hydroxide**, ethanolic solution,  $c(\text{KOH}) \approx 0,2 \text{ mol/l}$ .

Dissolve 13 g potassium hydroxide in 20 ml water and make up to 1 l with ethanol.

**5.3 Diethyl ether**.

**5.4 Anhydrous sodium sulfate**.

**5.5 Glass plates**, coated with silica gel, without fluorescence indicator, 0,25 mm thick.

Suitable ready-for-use products are available commercially.

**5.6 Benzene**, chromatography grade.

**5.7 Acetone**, chromatography grade.

**5.8 Hexane**, chromatography grade.

**5.9 Diethyl ether**, chromatography grade.

**5.10 Chloroform**, chromatography grade.

**5.11 Reference solution for thin-layer chromatography**: 1-eicosanol, 0,5 g/100 ml solution in chloroform, or a fraction of alcohols obtained as indicated in 9.2 from the unsaponifiable matter of an olive-pomace oil.

**5.12 2',7'-Dichlorofluorescein in ethanol**, 0,2 g/100 ml solution. Make slightly basic by adding a few drops of alcoholic potassium hydroxide solution (5.1).

**5.13 Anhydrous pyridine**, chromatography grade.

**5.14 Hexamethyldisilazane (HMDS)**.

**5.15 Trimethylchlorosilane (TMCS)**.

**5.16 Standard solutions of trimethylsilyl ethers (TMSE)**, of aliphatic alcohols from  $\text{C}_{20}$  to  $\text{C}_{28}$ . Prepare from mixtures of pure alcohols immediately prior to use.

**5.17 Internal standard solution**: solution of 1-eicosanol in chloroform, mass concentration 0,1 g/100 ml.

**5.18 Carrier gas**: hydrogen or helium, gas chromatography grade.

**5.19 Auxiliary gas**: nitrogen, gas chromatography grade.

## 6 Apparatus

Usual laboratory equipment and in particular the following.

**6.1 Round-bottomed flask**, of capacity 250 ml, fitted with a reflux condenser having ground-glass joints.

**6.2 Separating funnel**, of capacity 500 ml.

**6.3 Round-bottomed flasks**, of capacity 250 ml.

**6.4 Chromatographic chamber for thin-layer chromatography**, suitable for glass plates of dimensions 20 cm  $\times$  20 cm.

**6.5 Ultraviolet lamp**, of wavelength 366 nm or 254 nm.



**6.6 Microsyringes**, of capacities 100 µl and 500 µl.

**6.7 Cylindrical filter funnel** with a G3 porous septum (porosity 15 µm to 40 µm), of approximate dimensions: diameter 2 cm and depth 5 cm, with an attachment suitable for filtration under vacuum and a 12/21 male ground-glass joint.

**6.8 Vacuum conical flask**, of capacity 50 ml, with a 12/21 female ground-glass joint which can be fitted to the filter funnel (6.7).

**6.9 Test-tube**, of capacity 10 ml, with a tapering bottom and a sealing stopper.

**6.10 Gas chromatograph**, suitable for use with capillary columns, equipped with the components specified in 6.10.1 to 6.10.4.

**6.10.1 Column oven**, capable of maintaining a temperature to within  $\pm 1$  °C.

**6.10.2 Split injection unit**, temperature-adjustable, with a persilylated glass vaporizing element, or an on-column unit.

**6.10.3 Flame ionization detector**.

**6.10.4 Integration system**.

**6.11 Fused silica capillary column**, of length 20 m to 30 m, internal diameter 0,25 mm to 0,32 mm, with SE-52 or SE-54<sup>1)</sup> liquid phase or equivalent, with a film thickness between 0,10 µm and 0,30 µm.

**6.12 Microsyringe for gas chromatography**, of capacity 10 µl, with hardened needle.

**6.13 Analytical balance**, sensitive to 1 mg (with 0,1 mg display).

**6.14 Desiccator**, with calcium chloride as desiccant.

**6.15 Drying oven**.

## 7 Sampling

Sampling is not part of the method specified in this International Standard. A recommended sampling method is given in ISO 5555<sup>[1]</sup>.

It is important that the laboratory receive a truly representative sample which has not been damaged or changed during transport or storage.

## 8 Preparation of the test sample

Prepare the test sample in accordance with ISO 661.

---

1) SE-52 and SE-54 are examples of suitable products available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of these products.

## 9 Procedure

### 9.1 Preparation of the unsaponifiable matter

**9.1.1** Using a 500 µl microsyringe (6.6), transfer to a 250 ml round-bottomed flask (6.1) a volume of internal standard solution (5.17) containing a quantity of 1-eicosanol approximately equal to 10 % of the content of aliphatic alcohols in the test portion. For example, to 5 g of sample, add 250 µl of the internal standard solution for olive oil and 1 500 µl for olive-pomace oil.

Evaporate to dryness under a stream of nitrogen, then weigh (6.13) accurately 5,000 g of the dry filtered sample into the same flask.

**9.1.2** Add 50 ml of 2 mol/l ethanolic potassium hydroxide solution (5.1), fit the reflux condenser and boil gently on a steam bath, stirring continuously throughout the heating process until saponification has taken place, i.e. until the solution becomes clear. Continue heating for a further 20 min and then add 50 ml of water through the condenser. The condenser is then disconnected and the flask cooled to approximately 30 °C.

**9.1.3** Transfer the contents of the flask quantitatively to a 500 ml separating funnel (6.2), progressively adding portions of about 50 ml water. Add approximately 80 ml of diethyl ether (5.9), shake vigorously for approximately 30 s, and allow to settle.

NOTE Emulsions are broken by spraying small quantities of diethyl ether or methanol into the funnel.

Separate off the lower aqueous phase, collecting it in a second separating funnel. Two further extractions are performed in the same manner on the aqueous phase, using 60 ml to 70 ml diethyl ether each time.

**9.1.4** The diethyl ether extracts are combined in a separating funnel and washed with water (50 ml at a time) until the washing water gives a neutral reaction against phenolphthalein.

Discard the washing water, dry with anhydrous sodium sulfate (5.4) and filter into a 250 ml round-bottomed flask (6.3) that has previously been weighed, and wash the funnel and filter with small quantities of diethyl ether which are added to the total.

**9.1.5** Distil the ether down to a few millilitres, then bring to dryness under a slight vacuum or under a stream of nitrogen, completing the drying process in an oven (6.15) maintained at 103 °C for approximately 10 min; weigh (6.13) after cooling in a desiccator (6.14).

### 9.2 Separation of alcoholic fractions

**9.2.1** Prepare basic TLC plates by immersing the silica gel plates (5.5) completely in an 0,2 mol/l potassium hydroxide solution (5.2) for 10 s, leaving them to dry for 2 h under an extractor hood and finally placing them in an oven (6.15) at 100 °C for 1 h.

NOTE When basic silica gel plates are used to separate the alcoholic fraction, there is no need to treat the unsaponifiable matter with alumina. It follows that all acid compounds (fatty acids and others) are retained at the origin, thereby producing both aliphatic alcohol and terpenic alcohol bands, which are both separated distinctly from the sterol band.

Remove the plate from the oven and keep in a desiccator (6.14) until required for use (plates treated in this way shall be used within 15 days).

**9.2.2** Place a hexane-diethyl ether mixture (volume fraction of hexane 65 ml/100 ml and of diethyl ether 35 ml/100 ml) in the plate development chamber to a depth of approximately 1 cm.

In particular cases, use a benzene-acetone eluent mixture (volume fraction of benzene 95 ml/100 ml and of acetone 5 ml/100 ml) to obtain distinct band separation.

Close the chamber using an appropriate cover and leave for half an hour to allow equilibration between vapour and liquid. Strips of filter paper partially immersed in the eluent may be affixed to the inside surfaces of

the chamber to reduce the development time by approximately one-third and obtain a more uniform and regular elution of the components.

Use fresh developing solution for each analysis in order to obtain reproducible developing conditions.

**9.2.3** Prepare a solution of approximately 50 mg/ml unsaponifiable matter (9.1.5) in chloroform and streak 0,3 ml of the solution as a uniform strip of minimum thickness, using a 100 µl microsyringe (6.6), at approximately 2 cm from the bottom of a TLC plate. Aligned with the origin, 2 µl to 3 µl of the aliphatic alcohols reference solution (5.11) are spotted for the identification of the aliphatic alcohols band after development has been completed.

**9.2.4** Place the plate inside the development chamber (see 9.2.2). The ambient temperature shall be maintained between 15 °C and 20 °C. Immediately close the chamber with the cover and allow to elute until the solvent front reaches approximately 1 cm from the upper edge of the plate.

Remove the plate from the development chamber and either evaporate the solvent under a hot air stream or leave the plate for a while under the extractor hood.

**9.2.5** Spray the plate lightly and evenly with the solution of 2',7'-dichlorofluorescein (5.12) when the plate is placed under ultraviolet light (6.5) for observation. Identify the aliphatic alcohols band by aligning against the stain obtained from the reference solution: using a black pencil, outline both the band of aliphatic alcohols and the band immediately above that, which is the terpenic alcohols band.

**NOTE** The aliphatic alcohols band and the terpenic alcohols band are grouped together because of the possible migration of some aliphatic alcohols into the triterpenic alcohols band.

**9.2.6** Using a metal spatula, scrape off the silica gel in the marked area. Place the finely comminuted material into the filter funnel (6.7). Add 10 ml of boiling chloroform, mix carefully with the metal spatula and filter under vacuum, collecting the filtrate in a conical flask (6.8) attached to the filter funnel.

Wash the residue in the flask three times with diethyl ether (5.3), using approximately 10 ml each time, collecting the filtrate in the flask attached to the funnel. Evaporate the filtrate to a volume of 4 ml to 5 ml, transfer the residual solution to a previously weighed 10 ml test-tube (6.9), evaporate to dryness by heating under a gentle stream of nitrogen, make up again using a few drops of acetone, evaporate again to dryness, place in an oven (6.15) at 103 °C for approximately 10 min, then allow to cool in a desiccator (6.14) and weigh (6.13).

The residue inside the test-tube is composed of the alcoholic fraction.

### 9.3 Preparation of the trimethylsilyl ethers

**9.3.1** The reagent for silylation, consisting of pyridine (5.13), hexamethyldisilazane (HMDS, 5.14), trimethylchlorosilane (TMCS, 5.15), volume fractions: 9 ml/13 ml; 3 ml/13 ml; 1 ml/13 ml, respectively, in the proportion of 50 µl for each milligram of aliphatic alcohols, is added to the test-tube containing the alcoholic fraction (9.2.6), avoiding all absorption of moisture.

**NOTE** Ready-for-use solutions are available commercially. Other silylating reagents such as bis-trimethylsilyl, trifluoroacetamide + 1 % trimethyl chlorosilane, which has to be diluted with an equal volume of anhydrous pyridine, are also available.

The slight opalescence which may form is normal and does not cause any interference. The formation of a white floc or the appearance of a pink colour are indicative of the presence of moisture or deterioration of the reagent. If these occur, the test shall be repeated.

**9.3.2** Stopper the test-tube, shake carefully (without overturning) until the aliphatic alcohols are completely dissolved. Stand for at least 15 min at ambient temperature and then centrifuge for a few minutes. The clear solution is ready for gas chromatographic analysis.

## 9.4 Gas chromatographic analysis

### 9.4.1 Preliminary operations and column packing

**9.4.1.1** Fit the column (6.11) in the gas chromatograph (6.10), attaching the inlet end to the injector connected to the splitting system (6.10.2) and the outlet end to the detector (6.10.3). Carry out a general check of the gas chromatography assembly (tightness of gas fittings, efficiency of the detector, efficiency of the splitting system and of the recording system, etc.).

**9.4.1.2** Condition the column on the first time of use. Circulate a little carrier gas through the capillary column, then switch on the gas chromatography assembly and heat gradually until a temperature of not less than 20 °C above the operating temperature is reached. Maintain that temperature for not less than 2 h. Then bring the assembly to operating conditions [by regulation of gas flow, split flame ignition, connection to the electronic recorder, adjustment of the temperature of the capillary column oven (6.10.1), the detector and the injector, etc.] and adjust the signal to a sensitivity that is at least twice as high as that planned for the analysis. The base line shall be linear, with no peaks of any kind, and shall not drift. A negative straight-line drift indicates leakage from the column connections; a positive drift indicates inadequate conditioning of the column.

The conditioning temperature shall be at least 20 °C less than the maximum temperature planned for the liquid phase employed.

### 9.4.2 Operating conditions

**9.4.2.1** The following operating conditions are recommended for a chromatographic system with a split injection unit:

- a) column temperature: the initial temperature is set to 180 °C for 8 min, then programmed to increase at a rate of 5 °C/min to 260°C, and the final temperature is maintained for a further 15 min at 260 °C;
- b) temperature of injector: 280 °C;
- c) temperature of detector: 290 °C;
- d) linear velocity of carrier gas: helium 20 cm/s to 35 cm/s, hydrogen 30 cm/s to 50 cm/s;
- e) splitting ratio: 1:50 to 1:100;
- f) injection quantity: 0,5 µl to 1 µl of TMSE solution.

The above conditions may be modified according to the characteristics of the column and of the gas chromatograph to obtain chromatograms satisfying the following conditions (see also Figure A.1):

- 1) the retention time for C<sub>26</sub> alcohol shall be (18 ± 5) min;
- 2) the peak of the C<sub>22</sub> alcohol shall be (80 ± 20) % of the full-scale value for olive oil and (40 ± 20) % of the full-scale value for olive-pomace oil.

**9.4.2.2** The above requirements are checked by repeated injection of the standard TMSE mixture of alcohols and the operating conditions are adjusted to yield the best possible results.

**9.4.2.3** The parameters for the integration of peaks shall be set so that a correct appraisal of the areas of the peaks considered is obtained.

### 9.4.3 Analytical procedure

**9.4.3.1** Using the 10 µl microsyringe (6.12), draw in 1 µl of hexane followed by 0,5 µl of air and subsequently 0,5 µl to 1 µl of the sample solution; raise the plunger of the syringe further so the needle is emptied. Push the needle through the membrane of the injection unit and, after 1 s to 2 s, inject rapidly; slowly remove the needle after approximately 5 s.

**9.4.3.2** Recording is effected until the TMSE of the aliphatic alcohols present have been eluted completely. The base line shall always correspond to the requirements of 9.4.1.2.

#### 9.4.4 Peak identification

The individual peaks are identified according to their retention times and by comparison with the standard TMSE mixture analysed under the same conditions.

A chromatogram of the alcoholic fraction of a virgin olive oil is shown in Figure A.1.

#### 9.4.5 Quantitative evaluation

**9.4.5.1** The peak areas of 1-eicosanol and of the aliphatic alcohols C<sub>22</sub>, C<sub>24</sub>, C<sub>26</sub>, and C<sub>28</sub> are calculated by electronic integration.

**9.4.5.2** The content of each aliphatic alcohol *i*, *w<sub>i</sub>*, as a mass fraction expressed in milligrams per kilogram of oil, is calculated as follows:

$$w_i = \frac{A_i m_s \times 1\,000}{A_s m}$$

where

*A<sub>i</sub>* is the peak area due to alcohol *i*;

*A<sub>s</sub>* is the peak area of 1-eicosanol;

*m<sub>s</sub>* is the mass, in milligrams, of 1-eicosanol;

*m* is the mass, in grams, of the test portion.

## 10 Precision

### 10.1 Interlaboratory test

Details of an interlaboratory test on the precision of the method are summarized in Annex B. The values derived from this interlaboratory test may not be applicable to concentration ranges and matrices other than those given.

### 10.2 Repeatability

The absolute difference between two independent single test results, obtained with the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, should, in not more than 5 % of cases, exceed the values of the repeatability limit, *r*, given in Table B.1.

### 10.3 Reproducibility

The absolute difference between two single test results, obtained with the same method on identical test material in different laboratories by different operators using different equipment, should, in not more than 5 % of cases, exceed the values of the repeatability limit, *R*, given in Table B.1.

## 11 Test report

The test report shall include at least the following information:

- a) all information necessary for the complete identification of the sample;
- b) the sampling method used, if known;
- c) the test method used, with reference to this International Standard (ISO 12871:2010);
- d) the result(s) obtained;
- e) if the repeatability has been checked, the final quoted result obtained;
- f) any operating details not specified in this International Standard, or regarded as optional, together with details of any incidents which may have influenced the test result(s).

## Annex A (informative)

### Determination of the linear velocity of the gas

Inject 1  $\mu\text{l}$  to 3  $\mu\text{l}$  of methane or propane into the gas chromatograph under normal operating conditions and measure, using a stopwatch, the time,  $t$ , taken for the methane or propane to flow through the column from the instant of injection to the instant the peak elutes.


The linear velocity,  $v$ , in centimetres per second, is given by:

$$v = \frac{L}{t}$$

where

$L$  is the length, in centimetres, of the column;

$t$  is the measured time, in seconds.

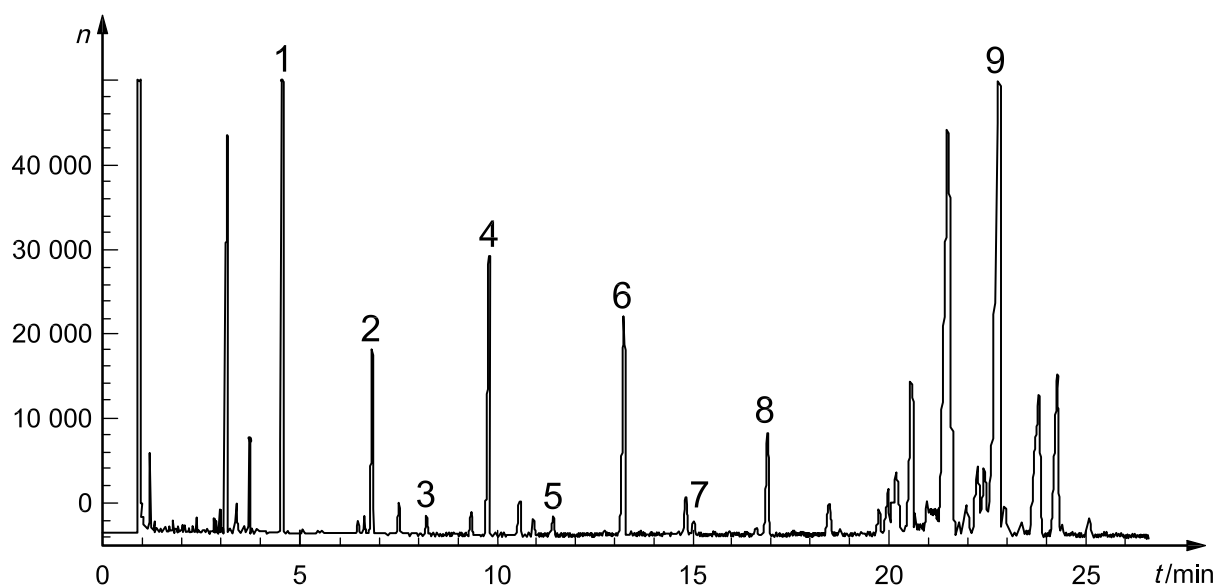

#### Key

1 eicosanol	6 hexacosanol
2 docosanol	7 heptacosanol
3 tricosanol	8 octacosanol
4 tetracosanol	9 triterpenic alcohols and methyl sterols
5 pentacosanol	
$n$ counts	$t$ time

**Figure A.1 — Chromatogram of the alcoholic fraction of virgin olive oil**

## Annex B (informative)

### Results of an interlaboratory test

Precision data for the method have been derived from the results of an international collaborative trial.

A total of 15 laboratories — holding IOC recognition — from seven countries took part in the collaborative test organized in May-June 2003. The trial was coordinated by the Instituto de la Grasa [Fats and Oils Institute], Seville, Spain.

The results of the collaborative test were subjected to statistical analysis in accordance with the recommendations of the Collaborative Study Guidelines<sup>[5]</sup>, which are identical to ISO 5725-1<sup>[2]</sup> and ISO 5725-2<sup>[3]</sup>. Outliers were examined by applying the tests of Cochran and Grubbs to the laboratory results for each determination (replicates a and b) and each sample.

The test was performed on five samples of lampante virgin olive oil and crude olive-pomace oil obtained on centrifuging the pomace from two-phase decanters (COPO) and blends thereof (see Table B.1). For the results, see Table B.2.

**Table B.1 — Compositions of samples**

Sample	Lampante virgin olive oil % volume fraction	Crude olive-pomace oil % volume fraction
A	100	—
B	85	15
C	75	25
D	60	40
E	—	100

**Table B.2 — Statistical results for the total aliphatic alcohols content ( $C_{22} + C_{24} + C_{26} + C_{28}$ )**

Parameter	Sample				
	A	B	C	D	E
<b>No. participating laboratories, <math>n_p</math></b>	15	15	15	15	15
<b>No. laboratories retained after eliminating outliers, <math>n_p</math></b>	12	14	14	14	14
<b>No. test results in all laboratories, <math>n_t</math></b>	24	28	28	28	28
<b>Mean content, <math>w_p</math>, mg/kg</b>	245	363	440	541	997
<b>Repeatability standard deviation, <math>s_p</math>, mg/kg</b>	6	10	10	13	19
<b>Coefficient of variation of repeatability, <math>C_{V,r}</math>, %</b>	2,4	2,8	2,3	2,4	1,9
<b>Repeatability limit, <math>r</math>, mg/kg</b>	16	28	29	36	54
<b>Reproducibility standard deviation, <math>s_R</math>, mg/kg</b>	17	28	58	54	71
<b>Coefficient of variation of reproducibility, <math>C_{V,R}</math>, %</b>	6,9	7,6	13,1	9,9	7,1
<b>Reproducibility limit, <math>R</math>, mg/kg</b>	47	78	161	150	198



## Bibliography

- [1] ISO 5555, *Animal and vegetable fats and oils — Sampling*
- [2] ISO 5725-1, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions*
- [3] ISO 5725-2, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*
- [4] COI/T.20/Doc. 26:2003, *Method of analysis — Determination of aliphatic alcohols content by capillary gas chromatography*
- [5] AOAC. International guidelines for collaborative study procedures to validate characteristics of a method of analysis. *J. AOAC Int.* 1995, **78**, 143A-160A

.....

---

---

**ICS 67.200.10**

Price based on 11 pages