
**Water quality — Determination of the
acute toxicity of waste water to zebrafish
eggs (*Danio rerio*)**

*Qualité de l'eau — Détermination de la toxicité aiguë des eaux
résiduelles vis-à-vis des œufs de poisson-zèbre (*Danio rerio*)*



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



COPYRIGHT PROTECTED DOCUMENT

© ISO 2007

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Interferences	2
5 Principle	3
6 Reagents	3
7 Apparatus	3
8 Procedure	4
9 Determination of toxicological endpoints	7
10 Validity criteria	8
11 Determination of LID_{egg}	9
12 Expression of results	9
13 Test report	9
14 Reproducibility	9
Annex A (informative) Scheme for layout and distribution of eggs in microplates	11
Bibliography	12

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 15088 was prepared by Technical Committee ISO/TC 147, *Water quality*, Subcommittee SC 5, *Biological methods*.

Introduction

Fish play a major role in the aquatic food web. They are high-order consumers (often final consumers) and have important functions of regulation in aquatic ecosystems. They are a confirmed part within test concepts regarding aquatic organisms from different trophic levels.

The eggs of the zebrafish (*Danio rerio* Hamilton-Buchanan) are used as test material. The zebrafish belongs to the family of Cyprinidae (carp-related fish) within the class of Osteichthyes (teleost fish). Zebrafish are easy to keep and produce transparent, nonadhesive eggs (diameter about 1 mm) throughout the whole year. Their embryonic development is well described. The zebrafish is one of the most important model fish in research on the developmental biology of vertebrates and is recommended as a test fish, i.e. in the OECD Guidelines 203, 204 and 210.

The development of fertilized fish eggs can be affected by water constituents and effluents. Death of embryos and certain defined disturbances of embryonic development, which finally lead to death, are considered effects.

Water quality — Determination of the acute toxicity of waste water to zebrafish eggs (*Danio rerio*)

WARNING — Persons using this International Standard shall be familiar with normal laboratory practice. This International Standard does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

IMPORTANT — It is absolutely essential that tests conducted according to this International Standard be carried out by suitably qualified staff. When applying this International Standard, it is necessary in each case to determine if and to what extent additional conditions should be established.

1 Scope

This International Standard specifies a method for the determination of degrees of dilution or of concentrations as a measure of the acute toxic effect of waste water to fish eggs within 48 h. This International Standard is also applicable to treated municipal waste water and industrial effluents.

NOTE This International Standard has been elaborated as a substitute for the acute fish toxicity test. Applied to waste water, it gives the same or similar results as achieved from the acute fish toxicity test (e.g. ISO 7346-1 or ISO 7346-2). If used for single substances, different sensitivities from both test systems are possible.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 5667-16, *Water quality — Sampling — Part 16: Guidance on biotesting of samples*

ISO 5814, *Water quality — Determination of dissolved oxygen — Electrochemical probe method*

ISO 7346-1, *Water quality — Determination of the acute lethal toxicity of substances to a freshwater fish (Brachydanio rerio Hamilton-Buchanan (Teleostei, Cyprinidae)) — Part 1: Static method*

ISO 7346-2, *Water quality — Determination of the acute lethal toxicity of substances to a freshwater fish (Brachydanio rerio Hamilton-Buchanan (Teleostei, Cyprinidae)) — Part 2: Semi-static method*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

control

dilution water with fertilized fish eggs

3.2
dilution level

D
reciprocal value of the volume fraction of waste water in dilution water in which the test is conducted

EXAMPLE 250 ml of waste water in a total volume of 1 000 ml (volume fraction of 25 %) represents dilution level $D = 4$.

NOTE See ISO 5667-16.

3.3
EC₅₀

concentration at which there is an effect on 50 % of the organisms in line with the test criterion

NOTE In this International Standard, LC₅₀ is the lethal concentration at which 50 % of the organisms are dead.

3.4
fish egg

generally used term for all development stages of an egg cell (inside the chorion) within this International Standard

NOTE If necessary, the following qualifiers for this term are used: “not fertilized”, immediately after spawning; “freshly fertilized”, between 4-cell stage and 128-cell stage; “embryo”, if the developing embryo is visible inside the egg before hatching.

3.5
lowest ineffective dilution
dilution factor
LID

lowest ineffective dilution tested, expressed as dilution level D (3.2), at which no inhibition, or only effects not exceeding the test-specific variability, are observed

3.6
LID_{egg}

lowest ineffective dilution within a test batch in which at least 90 % of the fish eggs do not show any effect according to this International Standard

NOTE See Clauses 11 and 12 and Figure 2.

3.7
test batch

defined dilutions with fertilized fish eggs

4 Interferences

The differentiation of eggs can be difficult in the case of heavily coloured and/or turbid waste water. In such cases, the following modified preparation order is used before starting the exposure:

- spawning;
- differentiation into fertilized and unfertilized eggs (8.2.2);
- transfer into dilution water (7.10, crystallization bowls);
- transfer into microplates without previous exposure.

While transferring into microplates, the error in dilution caused by adherent water should be kept as small as possible.

5 Principle

In a dilution series, waste water graduated to integral volume ratio is mixed with dilution water giving defined dilution levels, D . After exposure of fertilized fish eggs to the test batches for 48 h using microplates, the dilution limit in which no acute toxic effect occurs is determined (LID). At 26 °C, the embryos hatch after 72 h to 96 h. The test duration is 48 h. As a positive control, a solution of 3,7 mg/l of the reference substance, 3,4-dichloroaniline, is tested with 10 fertilized eggs (8.3).

This International Standard may also be used to calculate dose-response-based EC_{50} values as percentages of waste water without changing the test design.

6 Reagents

As far as available, use only reagent grade chemicals.

6.1 Water, deionized or of equivalent purity (conductivity < 10 μ S/cm).

6.2 Hydrochloric acid, e.g. $c(\text{HCl}) = 0,1$ mol/l.

6.3 Sodium hydroxide solution, e.g. $c(\text{NaOH}) = 0,1$ mol/l.

6.4 Reference substance 3,4-dichloroaniline, stock solution, $\rho(\text{C}_6\text{H}_5\text{Cl}_2\text{N}) = 100$ mg/l.

Stir 0,05 g of dichloroaniline in 500 ml of dilution water (6.5) for 24 h. Adjust the pH to 7,0.

Kept dark in a refrigerator, this stock solution may be stored for up to 6 months. A concentration of 3,7 mg/l is used as positive control, (8.3).

6.5 Dilution water

Use standard dilution water as specified in ISO 7346-1 and ISO 7346-2.

— 294,0 mg/l of calcium chloride dihydrate, $\text{CaCl}_2 \cdot 2 \text{H}_2\text{O}$;

— 123,3 mg/l of magnesium sulfate heptahydrate, $\text{MgSO}_4 \cdot 7 \text{H}_2\text{O}$;

— 63,0 mg/l of sodium hydrogen carbonate, NaHCO_3 ;

— 5,5 mg/l of potassium chloride, KCl.

Before adding the reference substance (6.4) or waste water samples to be tested, the dilution water shall be equilibrated with air to 100 % oxygen saturation at $26 \text{ °C} \pm 1 \text{ °C}$.

7 Apparatus

7.1 Inverse microscope and/or binocular, with a minimum magnification of 30 \times .

7.2 Exposure vessels, with a volume of 2,5 ml to 5 ml, plain ground, i.e. polystyrene one-way microplates (24 wells).

7.3 Self-adhesive foil, to cover the microplates.

7.4 Temperature-controlled incubator or climatization of the room to $26 \text{ °C} \pm 1 \text{ °C}$, controlled illumination during the keeping of parental fish and exposure of eggs.

- 7.5 pH-meter.
- 7.6 Oxygen probe, see ISO 5814.
- 7.7 Spawning dishes of inert plastic or glass to sample the eggs during spawning.
- 7.8 Artificial plants of glass or plastic.
- 7.9 Pipette, for transfer of the eggs.
- 7.10 Crystallization dishes or bowls.
- 7.11 Glassware to prepare the concentration levels and dilution water.
 - 7.11.1 Volumetric flasks.
 - 7.11.2 Graduated cylinders.
 - 7.11.3 Graduated pipettes.
 - 7.11.4 Petri dishes.
 - 7.11.5 Beaker, e.g. 150 ml.
- 7.12 Aquaria to keep the adult fish.
- 7.13 Laboratory thermometer.

8 Procedure

8.1 Keeping of fish and production of eggs

8.1.1 General

For the production of eggs, use only apparently healthy spawners free from externally visible diseases and aged between 6 months and 24 months.

Do not treat parental test fish with any pharmaceuticals (acute or prophylactic) during the 6 months immediately before spawning.

8.1.2 Aquaria

Keep spawners in aquaria in which sufficient space for swimming is available (i.e. 1 l per fish).

8.1.3 Water for fish keeping and breeding

Use standardized dilution water (6.5).

The oxygen saturation should be at least 80 %, the temperature $26\text{ }^{\circ}\text{C} \pm 1\text{ }^{\circ}\text{C}$. For keeping and breeding, suitable drinking water (e.g. free from disinfectants) may be used alternatively.

8.1.4 Food

Fish should be fed with commercially available dried food for aquarium fish.

Supplemental feeding with for example living food (*Artemia spec.–nauplia*, *Daphnia* in appropriate size) is recommended.

Overfeeding should be avoided.

Eggs of *Artemia spec.* can be purchased from the aquarist trade. Breeding conditions are generally given in the manufacturer's instructions. Before feeding the fish, rinse *Artemia-nauplia* thoroughly with water to remove salt.

8.1.5 Light conditions

The photoperiod is constantly adjusted throughout the year, i.e. 16/8 h (light/dark) or 12/12 h.

NOTE Any physiological tolerable light conditions and photoperiods are acceptable.

8.2 Providing eggs for the test

8.2.1 General

Mating and spawning usually take place within 30 min after starting the light period. A ratio for males to females of 2:1 is recommended and has been proved successful.

Adult zebrafish are known to feed upon their own spawned eggs. Therefore, spawning dishes covered with a grid of stainless steel are placed in the aquaria, thus allowing the eggs to be sampled without interference from the adults. As a supporting tactile stimulus to initiate spawning, artificial plants of plastic or glass (7.8) should be fixed to the grid covering the spawning dishes.

Insert spawning dishes (7.7) into the aquaria immediately before activation of light to ensure that the development stage of fertilized eggs is within the range of the 4-cell stage to 128-cell stage.

Other procedures to achieve fertilized eggs are permissible as long as criteria for the starting conditions (4-cell stage to 128-cell stage) are met.

Remove spawning dishes about 30 min after activation of light and before feeding.

The transparent eggs can easily be identified by putting the spawning dish on a black pad and using transverse light for investigation.

The fertilization rate should be more than 50 %. An approximation of the fertilization rate may be accepted (8.2.2).

8.2.2 Differentiation of eggs

To differentiate the eggs, use a microscope or a binocular. Freshly spawned eggs show the following structures: the perivitelline space containing the yolk is surrounded by the egg membrane; the germinal disc is formed at the animalic pole (upper side of the yolk). After fertilization of the eggs, the first cell division proceeds after about 15 min at 26 °C. Subsequently, the germinal disc is divided synchronously into 4, 8, 16 and 32 blastomeres (discoidal groove, see Figure 1). From the 4-cell stage onwards, fertilized eggs can be distinguished clearly and definitely from non-fertilized eggs.

Use only fertilized eggs from the 4-cell stage to the 128-cell stage for the test.

Differentiate eggs within the first hour after spawning.

Separate and reject eggs with conspicuous anomalies in cell division (asymmetries, vesicles) or damaged membranes.

NOTE Diminutive, completely white eggs are oocytes denatured in the females' bodies before spawning.




Figure 1 — Relevant development stages for the differentiation of eggs

8.3 Test procedure

Consider the general recommendations on biotesting and handling of samples as specified in ISO 5667-16.

Determine the pH and oxygen concentration of the original sample.

Adjust the pH of the waste water to $7,0 \pm 0,2$ by the addition of hydrochloric acid (6.2) or sodium hydroxide solution (6.3) respectively, using beakers.

Make sure that the volume of the acid or base required for neutralisation is as small as possible.

Avoid surpassing the neutral point.

Neutralization should be omitted if the effect of the pH is to be reflected in the test result or if physical modification or chemicals reactions (e.g. precipitation) are observed due to pH adjustment. Following Table 1, prepare a set of dilutions from 1 volume of waste water and the appropriate volume of dilution water.

Table 1 — Dilution levels, *D*

Multiple of dilution water <i>X</i>	Dilution level <i>D</i>	Portion of sample in <i>D</i> %
0	1	100,00
1	2	50,00
2	3	33,00
3	4	25,00
5	6	16,67
7	8	12,50
11	12	8,33
15	16	6,25
23	24	4,17
31	32	3,13

Ensure that O₂ concentration does not fall below 4 mg/l O₂ (about 50 % saturation) in each dilution. If aeration is necessary, the O₂ concentration should not exceed the corresponding saturation value.

To start the exposure as soon as possible, immediately transfer about 40 eggs into the prepared dilution (preferably in glass crystallization dishes of 100 ml). Subsequently differentiate eggs into fertilized and unfertilized. Transfer only fertilized eggs separately into each well of the microplate, such that each well contains one egg in a constant volume of test concentration (i.e. 2 ml in a 24-well microplate).

For each dilution, incubate at least 10 fertilized eggs. If incubation is carried out with 24-well microplates, it is possible to arrange two dilution levels on one microplate.

Use the remaining four wells on this microplate for microplate control, placing one fertilized egg per well and filling with dilution water.

In the same way, prepare a negative dilution water control consisting of at least 10 fertilized eggs (see Annex A).

With each dilution series, measure a positive control with 3,7 mg/l of reference substance 3,4-dichloroaniline, also consisting of at least 10 fertilized eggs.

Cover the microplates with self-adhesive foil and incubate at $26\text{ °C} \pm 1\text{ °C}$ for 48 h.

After incubation, examine the eggs/embryos and record the results.

9 Determination of toxicological endpoints

9.1 General

After 48 h of incubation, investigate, determine and record the following toxicological endpoints.

9.2 Number of coagulated eggs

Even without magnification, coagulated eggs can be clearly identified. They are opaque and seem to be dark when observed through the microscope.


9.3 Tail detachment

It should be verified if the embryo's tail has been detached from the yolk sac due to its growth in length. The detachment should have developed at least as shown in Figure 2. If not, record as "no detachment".

9.4 Heartbeat

In Figure 2, “a” shows the location of the heart.

Record if a heartbeat is detected or not.



Key

- a heart
- b detached tail

Figure 2 — Embryos of zebrafish after 24 h and 48 h

Acute toxicity can be assumed if detachment of embryonic tail has not proceeded, and heartbeat cannot be detected; also, coagulated eggs indicate lethality. Supplementary investigations have shown that embryos do not hatch if one of the described effects has been detected.

After 48 h, an embryo is defined as dead, if

- it is coagulated, or
- it does not show tail detachment (if, after 48 h, embryonic tail is not more detached than after 24 h, it is defined as “not detached”, see Figure 2), or
- a heartbeat is not detectable.

10 Validity criteria

The test is valid if

- at least 90 % of the embryos in the negative dilution water control survive after the 48 h incubation time, and
- the results of the positive control are within the defined range (3,7 mg/l of reference substance should cause an effect > 10 %, see 8.3).

As a positive control, a defined concentration of reference substance (3,7 mg/l of 3,4-dichloroaniline) should be tested with 10 fertilized eggs (8.3) in parallel when the test is carried out.

11 Determination of LID_{egg}

Summarize the number of dead eggs for each test batch after 48 h (9.2). If one of the criteria described in 9.4 is fulfilled, the egg is considered dead.

The test result is the lowest tested value for D (LID) in which at least 90 % of the eggs have survived. This dilution level is specified as the result.

If more than one egg dies in a microplate control, the respective microplate should be excluded from calculation.

Mortality in microplate controls has not been considered within validity criteria. They give some indication of unsuitable microplates. Normally, mortality in microplate controls does not occur (< 0,1 %). If so, plausibility has to be checked. In case of doubt, the microplate is excluded from the evaluation of the test result.

12 Expression of results

Values for LID are reported as integral numbers.

EXAMPLE LID_{egg} = 2

It is generally possible to calculate EC₅₀ values from dilution series of different volume fractions of waste water. In this case, ISO/TS 20281 should be taken into account.

13 Test report

This clause specifies which information shall be included in the test report. It is required that information is given on at least the following aspects of the test:

- a) a reference to this International Standard (ISO 15088);
- b) identification of the method;
- c) identity of waste water;
- d) pH and oxygen concentration in milligrams per litre (or percentage saturation) of the original sample and the dilutions, if necessary, at the beginning of test;
- e) report of test results according to Clause 12;
- f) any deviation from the test protocol and report of all marginal conditions of relevance according to the test result.

14 Reproducibility

An interlaboratory trial based on the method described in this International Standard was carried out in 2000. Results with the reference substance 3,4-dichloroaniline and the percentage of mortality at a given concentration (3,7 mg/l of 3,4-dichloroaniline) are given in Table 2. Additional information referring to the test procedure and comparisons between the acute fish test and the fish egg test are given in a validation document, which is available under http://www.gdch.de/strukturen/fg/wasser/publikat/vali/vdok_t6.pdf¹⁾.

1) At the time of publication, this document is available in German only. An English translation is in progress.

Table 2 — Interlaboratory test results for EC₅₀ of 3,4-dichloroaniline and mortality at 3,7 mg/l of 3,4-dichloroaniline

Parameter	<i>l</i>	<i>n</i>	<i>o</i> %	\bar{x}	<i>s_R</i>	CV _{<i>R</i>} %	<i>s_r</i>	CV _{<i>r</i>} %
A	15	43	8,5	3,31 mg/l	0,455 mg/l	13,8	0,289 mg/l	8,7
B	16	46	0,0	68,0 %	24,0 %	35,0	16,9 %	25,0

where


l is the number of laboratories;
n is the number of valid measured values;
o is the percentage of outliers;
 \bar{x} is the overall mean;
s_R is the reproducibility standard deviation;
 CV_{*R*} is the reproducibility variation coefficient;
s_r is the repeatability standard deviation;
 CV_{*r*} is the repeatability variation coefficient.

Parameter:

A EC₅₀ of 3,4-DCA (mg/l).
 B Mortality at 3,7 mg/l 3,4-DCA (%).

Annex A
(informative)

Scheme for layout and distribution of eggs in microplates

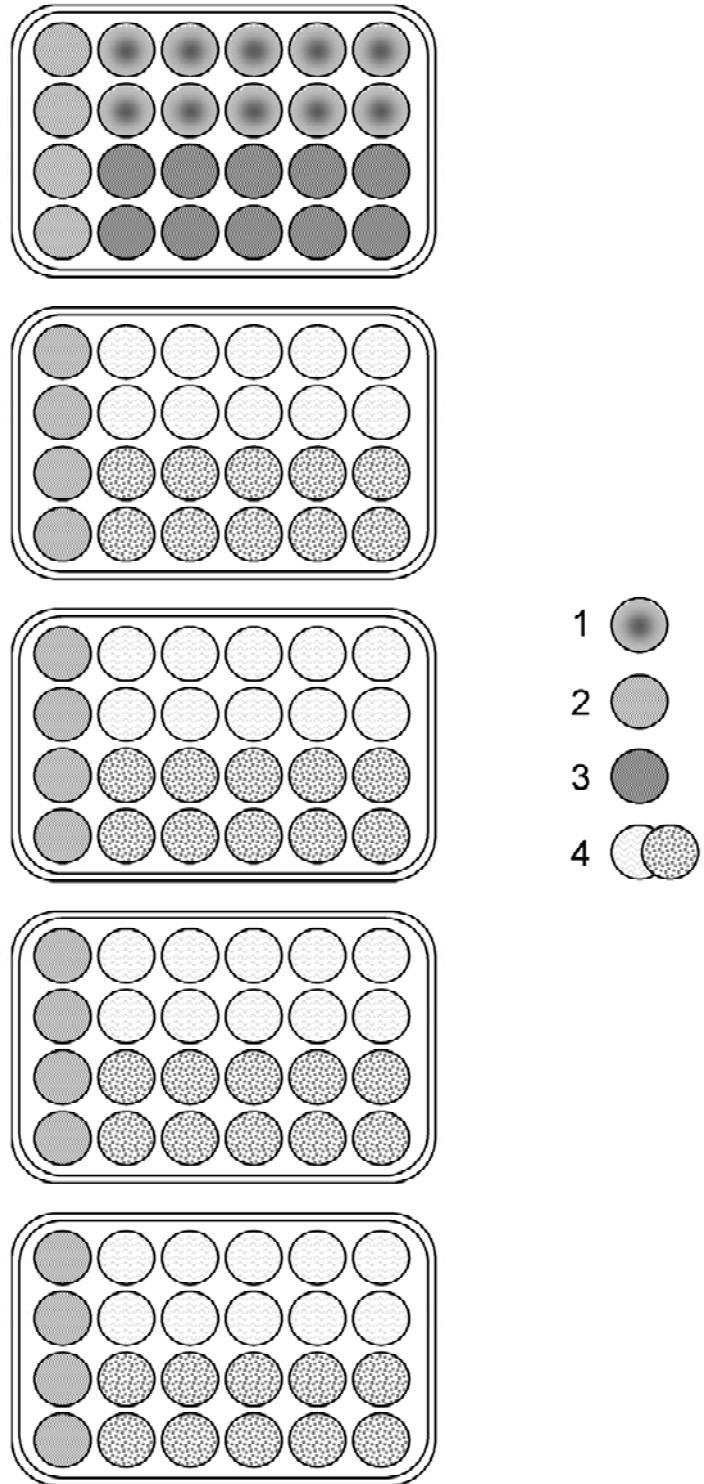

Key

- 1 positive control (3,7 mg/l 3,4-DCA)
- 2 microplate control
- 3 negative dilution water control
- 4 dilution level

Figure A.1 — Scheme for layout and distribution of eggs in microplates

Bibliography

- [1] ISO/TS 20281, *Water quality — Guidance on statistical interpretation of ecotoxicity data*
- [2] DETRICH, H.W., WESTERFIELD, M., ZON, L.I. The zebrafish – biology. *Methods in Cell Biology*, **59**, Academic Press, San Diego, London, Boston, New York, Sydney, Tokyo, Toronto, 1999, 391 pp.
- [3] FRICCIUS, T., SCHULTE, C., ENSENBACH, U., SEEL, P. and NAGEL, R. Der Embryotest mit dem Zebrafisch – eine neue Möglichkeit zur Prüfung und Bewertung der Toxizität von Abwasserproben. *Vom Wasser*, **84**, 1995, pp. 407-418
- [4] FUßMANN, G. and NAGEL, R. *Laborvergleichsversuche — Embryotest mit dem Zebrafisch Brachydanio rerio*. UBA-FB 98-009, 1997
- [5] HISAOKA, K.K. and FIRLIT, C.F. Further studies on the embryonic development of the zebrafish, *Brachydanio rerio* (Hamilton Buchanan). *J. Morphol.*, **107**, 1960, pp. 205-225
- [6] HISAOKA, K.K. and BATTLE, H.J. The normal developmental stages of the zebrafish, *Brachydanio rerio* (Hamilton Buchanan). *J. Morphol.*, **102**, 1958, pp. 311-328
- [7] KIMMEL, C.B., BALLARD, W.W., KIMMEL, S.R., ULLMAN, B. and SCHILLING, T.F. Stages of Embryonic Development of the Zebrafish. *Developmental Dynamics*, **203**, No. 3, 1995, pp. 253-310
- [8] NAGEL, R. and ISBERNER, K. Testing of chemicals with fish – a critical evaluation of tests with special regard to zebrafish. In: *Fish Ecotoxicology* (eds. BRAUNBECK, T., HINTON, D.E. and STREIT, B.), Birkhäuser Verlag, Basel, Switzerland, 1998, pp. 338-352
- [9] SCHIRONE, R.C. and GROSS, L. Effect of temperature on early embryological development of the zebrafish, *Brachydanio rerio*. *J. exp. Zool.*, **169**, 1963, pp. 43-52
- [10] SCHULTE, C. and NAGEL, R. Testing Acute Toxicity in the Embryo of Zebrafish, *Brachydanio rerio*, as an Alternative to the Acute Fish Test: Preliminary results. *ATLA*, **22**, 1994, pp. 12-19
- [11] WESTERFIELD, M. *The zebrafish book. Guide for the laboratory use of zebrafish (Danio rerio)*. 3rd edn., Univ. of Oregon Press, Eugene, 1995
- [12] OECD Guideline 203, *Fish — Acute toxicity test*
- [13] OECD Guideline 204, *Fish — Prolonged toxicity test: 14-day study*
- [14] OECD Guideline 210, *Fish — Early-life stage toxicity test*

Copyright International Organization for Standardization

ICS 13.060.70

Price based on 12 pages