
**Cosmetics — Analytical methods —
Nitrosamines: Detection and
determination of N-nitrosodiethanolamine
(NDELA) in cosmetics by HPLC-MS-MS**

Cosmétiques — Méthodes analytiques — Nitrosamines: Recherche et dosage des N-nitrosodiéthanolamines (NDELA) dans les produits cosmétiques par CLHP-SM-SM



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



COPYRIGHT PROTECTED DOCUMENT

© ISO 2008

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 15819 was prepared by Technical Committee ISO/TC 217, *Cosmetics*.

Introduction

Human exposure to N-nitrosamines can occur through diverse sources such as environment, food or personal care products. As a result of their perceived carcinogenic potential on several animal species, minimization of exposure to N-nitrosamines is recognised as important to the preservation of human health. Among N-nitrosamines, N-nitrosodiethanolamine (NDELA) has been recognised as a potential contaminant of cosmetics.

In this context, several analytical methods have been developed to detect and determine its presence in cosmetics – such as gas chromatography/thermal energy analysis, high performance liquid chromatography (HPLC) coupled either with photolysis and colorimetric quantification or with mass spectrometry (MS) determination. This latter method uses advanced technology to ensure the maximum specificity towards NDELA, to minimize the risk of artifactual formation of the analyte of interest and to allow precise quantification.

This analytical method uses high performance liquid chromatography coupled with mass spectrometry to separate and detect trace levels of NDELA from a cosmetic ingredient or product matrix with maximum specificity for NDELA.

Cosmetics — Analytical methods — Nitrosamines: Detection and determination of N-nitrosodiethanolamine (NDELA) in cosmetics by HPLC-MS-MS

1 Scope

This International Standard describes a method for the detection and quantification of NDELA in cosmetics and raw materials used in cosmetics.

This method is not applicable to the detection and/or quantification of nitrosamines other than NDELA nor to the detection and/or quantification of NDELA in products other than cosmetics or raw materials used in cosmetics.

If a product has a possibility of either NDELA contamination from ingredients or NDELA formation by the composition of ingredients, the method shall be applied for quantitative determination of NDELA. Accordingly the method would not be applied in routine testing of cosmetic products. Because of the large variety of cosmetic products within this field of application, this method might need to be adapted for certain matrices.

Therefore, International Standards dedicated to alternative methods for testing nitrosamines in cosmetic products are being developed separately. Other methods can be employed provided that they are verified as to their detection of NDELA and validated in terms of recovery and quantification of the analyte.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods*

3 Principle

Extraction of the nitrosamine NDELA in cosmetic samples is carried out with water in the presence of deuterated d8-NDELA used as internal standard. Clean-up is performed either using solid phase extraction (SPE clean-up, see 6.3.1) with a C18 cartridge or liquid-liquid extraction using dichloromethane (DCM clean-up, see 6.3.2) when the samples are not dispersible in water. The extracts are analysed by HPLC-MS-MS (high performance liquid chromatography coupled with tandem mass spectrometric detection).

NDELA quantification is done by comparing the ratio of the major fragment ions of NDELA and d8-NDELA with the calibration curve.

Confirmation of the presence of NDELA is carried out by using the molecular ion and two diagnostic ions.

4 Reagents

During the analysis, unless otherwise stated, use only reagents of recognized analytical grade and only distilled water or water of grade 1 in accordance with ISO 3696:1987. Solvent shall be of quality for HPLC analysis.

- 4.1 **Methanol** (MeOH), HPLC grade.
- 4.2 **Ethanol** (EtOH), HPLC grade.
- 4.3 **Dichloromethane**, HPLC grade.
- 4.4 **N-nitrosodiethanolamine**, with known purity greater than 95 %.
- 4.5 **d8-N-nitrosodiethanolamine**, with known purity greater than 95 %.
- 4.6 **Ammonium acetate** (NH₄Ac), analytical grade.
- 4.7 **1 mol/l ammonium acetate solution**, formed by dissolving 77,08 g of NH₄Ac in 1,0 l water.
- 4.8 **Eluent A: 2 mmol NH₄Ac in water**, formed by taking 2 ml of 1 mol/l NH₄Ac (4.7) and making up to 1 l with water.
- 4.9 **Eluent B: 2 mmol NH₄Ac in 90 % MeOH/water**, formed by taking 2 ml of 1 mol/l NH₄Ac (4.7) and adding 900 ml MeOH and 98 ml water.

5 Apparatus

Use standard laboratory glassware and equipment, with the addition of:

- 5.1 **Vortex mixer**.
- 5.2 **Sample processing station**, in SPE application (such as Vacmaster^{®1)} sample processing station, IST).
- 5.3 **Centrifuge**, capable of reaching not less than 20 000 G.
- 5.4 **Solid phase extraction columns**, e.g. Bakerbond^{®1)} C18 – 6 ml, 500 mg reversed phase octadecylsilane bonded to silicagel, 40 APD, 60 Å.
- 5.5 **HPLC-MS-MS equipment** consisting of:
 - 5.5.1 **High performance liquid chromatography apparatus**, consisting of an eluent reservoir, a pump, an injection system, a data processor, e.g. an integrator with plotter, coupled with tandem mass spectrometry using electrospray ionization.

1) Vacmaster[®], Bakerbond[®] and Spherisorb[®] are examples of suitable products available commercially. This information is given for the convenience of users of this International Standard and does not constitute an endorsement by ISO of these products.

5.5.2 Analytical reversed phase HPLC separating column, C18, e.g. Spherisorb® ODS II¹⁾ protected with a guard column, the dimensions of which are:

separating column

- length: 150 mm
- internal diameter: 4,6 mm
- size of spherical particles: 5 µm

guard column

- length: 10 mm
- internal diameter: 4,6 mm
- size of spherical particles: 5 µm

6 Sample preparation and conservation

6.1 General

WARNING — Most N-nitrosamines are potent carcinogens and every possible precaution shall be taken to avoid human exposure.

All operations involving handling of N-nitrosamines or their solutions should take place in an adequately ventilated fume hood or glove box.

NOTE Rubber surgical gloves, which are frequently employed, do not provide complete protection. They should be removed and disposed of immediately after use and not worn for long periods.

Thought should be given to safe disposal of any solution of material containing N-nitrosamines.

N-Nitrosodiethanolamine shall be stored in the absence of light between 2 °C and 8 °C.

UV degrades N-nitrosamines, so all solutions (standards/extracts) shall be stored in such a way that deterioration and change in composition are prevented.

Injection for analysis shall be made within 30 min of preparation of the extract sample.

6.2 Standards preparation

6.2.1 Prepare stock solutions (A) of NDELA containing 1,016 mg/ml in ethanol and store them in the absence of light at –20 °C.

6.2.2 Prepare stock solutions (d8A) of d8-NDELA containing 1,016 mg/ml in ethanol and store them in the absence of light at –20 °C.

6.2.3 Prepare working solutions (B, C, D, E and F) by sequential 10-fold dilutions of the 1,016 mg/ml solution. All solutions shall be stored in the absence of light between 2 °C and 8 °C.

Working solutions	Stock or working solution volume	Water volume	Final concentration	Stability
Working solution B	100 µl of A	900 µl	0,101 645 mg/ml	1 day
Working solution C	100 µl of B	900 µl	10,164 5 µg/ml	1 day
Working solution D	100 µl of C	900 µl	1,016 45 µg/ml	1 day
Working solution E	100 µl of D	900 µl	101,645 ng/ml	1 day
Working solution F	100 µl of E	900 µl	10,164 5 ng/ml	1 day

6.2.4 Prepare d8 working solutions (d8B, d8C, d8D and d8E) by sequential 10-fold dilutions of the 1,016 mg/ml solution. All solutions shall be stored in the absence of light between 2 °C and 8 °C.

d8 working solutions	Stock or working solution volume	Water volume	Final concentration	Stability
Working solution d8B	1 ml of d8A	9 ml	0,101 645 mg/ml	1 day
Working solution d8C	1 ml of d8B	9 ml	10,164 5 µg/ml	1 day
Working solution d8D	1 ml of d8C	9 ml	1,016 45 µg/ml	1 day
Working solution d8E	1 ml of d8D	9 ml	101,645 ng/ml	1 day

6.2.5 Prepare standard solutions by dilutions of the working solutions. A standard curve from 1,0 ng/ml to 80 ng/ml is made. The internal standard d8-NDELA was at 20 ng/ml in each solution. All solutions shall be stored in the absence of light between 2 °C and 8 °C.

Standard solutions	Working solution volume	Working solution d8E	H ₂ O volume	Final concentration	Stability
Standard solution 1	800 µl of E	200 µl	–	81,32 ng/ml	1 day
Standard solution 2	400 µl of E	200 µl	400 µl	40,66 ng/ml	1 day
Standard solution 3	200 µl of E	200 µl	600 µl	20,33 ng/ml	1 day
Standard solution 4	100 µl of E	200 µl	700 µl	10,16 ng/ml	1 day
Standard solution 5	100 µl of F	200 µl	700 µl	1,02 ng/ml	1 day

6.3 Sample preparation

6.3.1 SPE clean-up

Weigh about 1,0 g of the sample (note the exact mass), add 400 µl of d8D working solution and adjust to 20,0 ml with water. Shake for 15 min. Centrifuge for 10 min if necessary.

Condition the solid phase extraction C18 column with 3 ml of methanol followed by 3 ml of water with a flow-rate of approximately 3,0 ml/min. Do not allow the column to dry out.

Load 5 ml of the SE preparation to the above solid phase extraction C18 column and discard the first 3 ml of solution. Collect the following 2 ml (with a flow-rate of approximately 3,0 ml/min) into a vial.

If necessary, filter the collected solution through an appropriate filter.

6.3.2 Alternative sample preparation for samples non dispersible in water (DCM clean-up)

Weigh about 0,2 g of the sample (note the exact mass) into a centrifuge tube, add 800 µl of working solution d8E and shake for 1 min. Add 4 ml of dichloromethane and shake for 1 min. Add 3,2 ml of water and shake for 5 min.

Centrifuge at 20 000 G for 5 min.

A portion of the upper aqueous layer is used for chromatographic analysis.

7 Procedure

7.1 General

With both types of sample preparation, the final extract is analysed for NDELA by HPLC-MS-MS.

7.2 Chromatographic conditions

Mobile phase: Eluent A – 2 mmol NH₄Ac in water (4.8)

Eluent B – 2 mmol NH₄Ac in 90 % MeOH/water (4.9)

Gradient:

Interval min	% A	% B
0 – 7	70	30
7 – 10	70→0	30→100
10 – 17	0	100
17 – 20	0→70	100→30
20 – 30	70	30

Flow: 0,2 ml/min

Injection volume: 20 µl

Temperature column oven: 30 °C

Run injection: Every run consists of five calibration points, five sample extracts and one control sample (a standard solution). At least after every four runs (20 sample extracts) a new calibration curve is made.

The acquisition window is from 7 min to 11 min.

7.3 LC-MS-MS condition

Electrospray, positive mode.

EXAMPLE Suitable parameters for quadrupole mass-spectrometer (such as QUATTRO ULTIMA®)

Source settings

Capillary voltage 3,50 kV

ISO 15819:2008(E)

Cone voltage	20 V
Capillary temperature	120 °C
Desolvation temperature	350 °C
Cone gas flow	93 l/h (N ₂)
Desolvation gas flow	398 l/h (N ₂)
Analyser settings	
Low Mass LM 1 resolution	13,5
High Mass HM 1 resolution	13,5
Collision	8
Low Mass LM 2 resolution	13,5
High Mass HM 2 resolution	13,5
Multiplier	650 V

Characteristic ions 134,9 (M+H), 104 and 74 (daughter ions) identify the presence of NDELA in the sample.

NDELA quantification is made by using the ratio of the intensity of the two major fragment ions 104 (from NDELA) and 111 (from d8-NDELA).

8 Calculation of results

8.1 Determination of the *R* value

For each injection (calibration point, sample extract and control sample) an *R* value is determined, being defined as the intensity ratio between the intensity from ion 104 resulting from the fragmentation of the NDELA M+H ion and ion 111 resulting from the fragmentation of the d8-NDELA M+H ion (see, for example, Figure A.2).

These *R* values are used for the determination of the calibration curve and of concentration *c* as indicated in 8.4.

8.2 Calibration curve

Prepare a calibration curve by plotting the concentration of NDELA standards (see 6.2.5) against their *R* value.

For quantification the calibration curve shall have a correlation coefficient better than or equal to 0,990.

8.3 Experimental conditions for validity of the measurement

The relative intensities of the two detected ions (104 and 74) from sample preparations, expressed as a percentage of the intensity of the most intense ion, shall correspond to those of the calibration standard solutions, at comparable concentrations, measured under the same conditions, within the tolerances listed in Table 1.

Validity is checked for each sample preparation measurement which gives an NDELA concentration above the limit of detection.

Table 1 — Maximum permitted tolerances for relative ion intensities

Relative intensity (% of base ion intensity)	Relative range of the response
> 50 %	± 20 %
> 20 % to 50 %	± 25 %
> 10 % to 20 %	± 30 %
≤ 10 %	± 50 %

8.4 Calculation of concentrations

Determine the concentrations, c , of the extracted samples in ng/ml by using their R values to read them directly from the calibration curve. These determined values, in ng/ml, of the concentrations correspond to the mass fractions, w , in ng/g of NDELA in the extracted samples.

NDELA concentrations of unknown samples are calculated using the following equations:

— for the SPE clean-up: $W = w \times [(m + 19)/m]$

— for the DCM clean-up: $W = w \times [(m + 4)/m]$

where

W is the mass fraction of NDELA in the product in micrograms per kilogram;

w is the mass fraction of NDELA determined in the extracts in nanograms per gram;

m is the mass of cosmetic product in grams.


9 Test report

The test report shall contain at least the following information:

- a) all information necessary for the identification of the sample;
- b) a reference to this International Standard, i.e. ISO 15819:2008;
- c) date and type of sampling (if known);
- d) date of receipt of the laboratory sample;
- e) date of test;
- f) the results and the units in which the results have been expressed;
- g) the method of clean-up used;
- h) any particular points observed in the course of the test;
- i) any operations not specified in the method or regarded as optional which might have affected the results.

Annex A (informative)

Examples of a calibration curve and of chromatograms

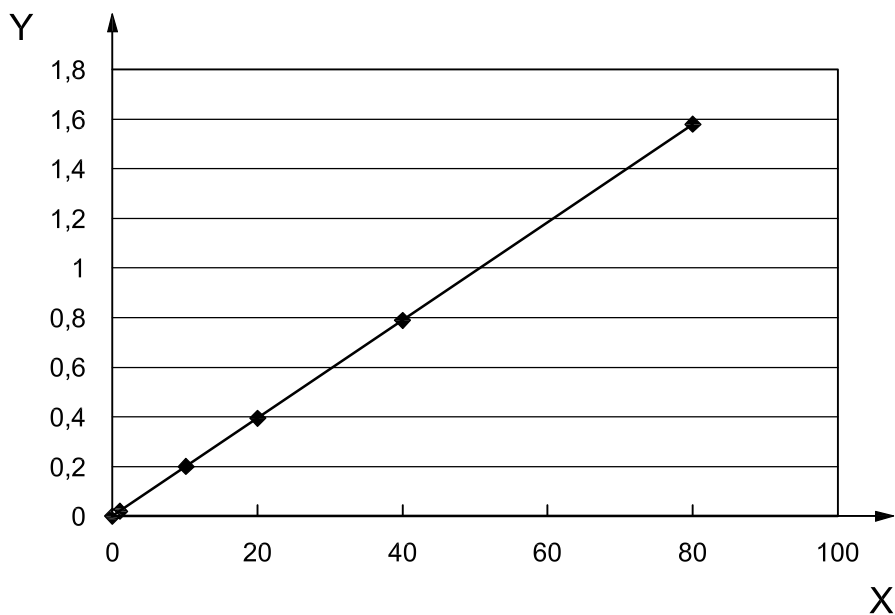

Key

- X concentration (ng/ml)
- Y response

Figure A.1 — Example of a calibration curve for NDELA

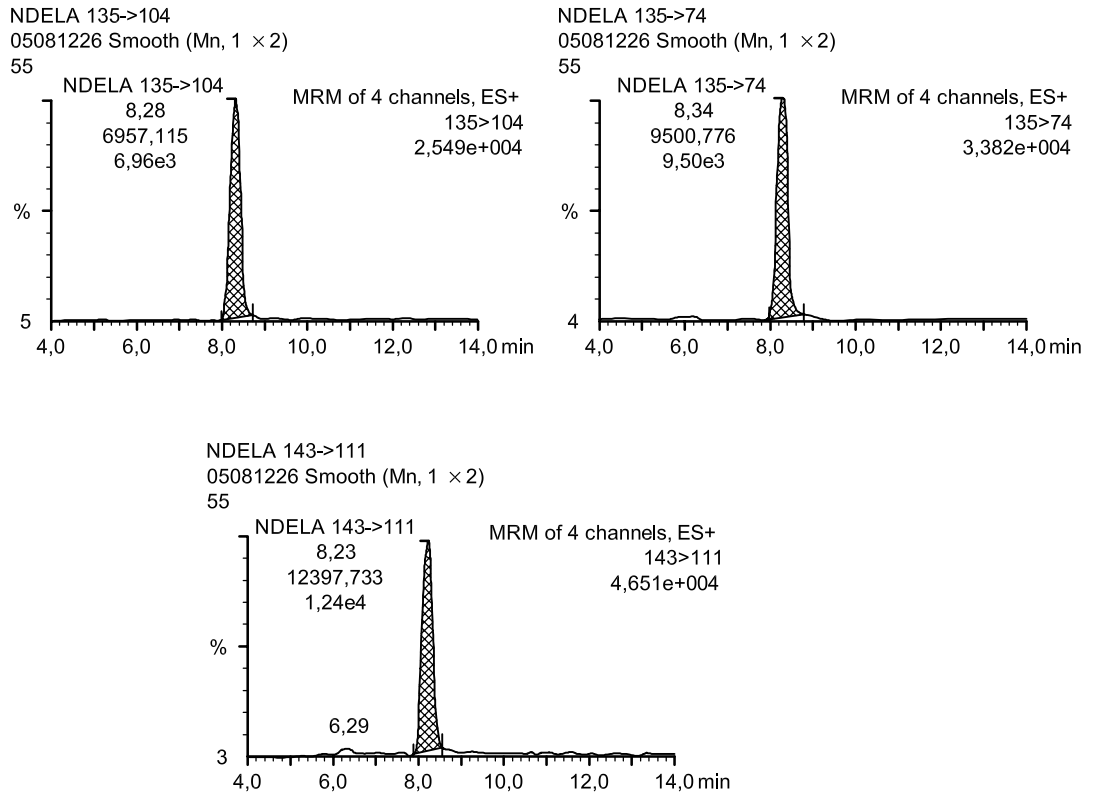


Figure A.2 — Examples of chromatograms

