
**Milk and milk products — Determination
of lactose content by high-performance
liquid chromatography (Reference
method)**

*Lait et produits laitiers — Détermination de la teneur en lactose par
chromatographie liquide haute performance (Méthode de référence)*

www.iso.org



Reference numbers
ISO 22662:2007(E)
IDF 198:2007(E)

© ISO and IDF 2007

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. Neither the ISO Central Secretariat nor the IDF accepts any liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies and IDF national committees. In the unlikely event that a problem relating to it is found, please inform the ISO Central Secretariat at the address given below.



COPYRIGHT PROTECTED DOCUMENT

© ISO and IDF 2007

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO or IDF at the respective address below.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

International Dairy Federation
Diamant Building • Boulevard Auguste Reyers 80 • B-1030 Brussels
Tel. + 32 2 733 98 88
Fax + 32 2 733 04 13
E-mail info@fil-idf.org
Web www.fil-idf.org

Published in Switzerland

Contents

Page

Foreword.....	iv
Foreword.....	v
1 Scope	1
2 Normative references	1
3 Terms and definitions.....	1
4 Principle.....	1
5 Reagents	1
6 Apparatus	2
7 Sampling.....	3
8 Preparation of test sample.....	3
9 Procedure	4
9.1 Preparation of the standard solution.....	4
9.2 Preparation of test portion.....	4
9.3 Preparation of filtrate.....	4
9.4 HPLC determination	5
10 Calculation and expression of results.....	6
10.1 Calculation.....	6
10.2 Expression of results	6
11 Precision.....	7
11.1 Interlaboratory test	7
11.2 Repeatability.....	7
11.3 Reproducibility.....	7
12 Test report	7
Annex A (informative) Results of interlaboratory test.....	8
Bibliography	10

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 22662|IDF 198 was prepared by Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 5, *Milk and milk products*, and the International Dairy Federation (IDF). It is being published jointly by ISO and IDF.

Foreword

IDF (the International Dairy Federation) is a worldwide federation of the dairy sector with a National Committee in every member country. Every National Committee has the right to be represented on the IDF Standing Committees carrying out the technical work. IDF collaborates with ISO in the development of standard methods of analysis and sampling for milk and milk products.

Draft International Standards adopted by the Action Teams and Standing Committees are circulated to the National Committees for voting. Publication as an International Standard requires approval by at least 50 % of the IDF National Committees casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. IDF shall not be held responsible for identifying any or all such patent rights.

ISO 22662|IDF 198 was prepared by the International Dairy Federation (IDF) and Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 5, *Milk and milk products*. It is being published jointly by IDF and ISO.

All work was carried out by the Joint ISO-IDF Action Team on *Lactose & lactate determination* of the Standing Committee on *Main components in milk* under the aegis of its project leader, Mr. R. Kouaouci (CA).

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100

Milk and milk products — Determination of lactose content by high-performance liquid chromatography (Reference method)

1 Scope

This International Standard specifies the reference method for the determination of lactose content of raw milk, heat-treated milks, dried milk and raw and pasteurized cream.

The method is not applicable to fermented milks and milks to which oligosaccharides have been added.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 648, *Laboratory glassware — One-mark pipettes*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

lactose content

mass fraction of substances determined by the procedure specified in this International Standard

NOTE The mass fraction can be expressed as a percentage.

4 Principle

An internal standard [D(+)-melezitose] is added to a weighed volume of milk and to lactose standards. A chemical reagent (Biggs-Szijarto solution) is added to precipitate out the fat and the protein component fractions of milk. The sample is filtered twice prior to injection, first through paper filter and then through a 0,45 µm nylon filter. The lactose and the internal standard are separated by a cation exchange column in the lead form and detected by a differential refractometer detector or other suitable detector. As mobile phase, HPLC grade water is used.

5 Reagents

Use only reagents of recognized analytical grade, unless otherwise specified.

5.1 Degassed HPLC grade water.

Filter the water, conforming to the requirements of ISO 3696, Grade 1, obtained from the water purification unit (6.9) using the solvent filtration unit (6.10). To improve the pump performance and to obtain a stable baseline, degas the mobile phase daily by selecting one of the available techniques such as sparging with helium, sonication, vacuum or in-line degassing system.

5.2 D(+)-Melezitose hydrate solution, $c(C_{18}H_{32}O_{16} \cdot H_2O) = 50 \text{ mg/ml}$.

Dissolve an amount of D(+)-melezitose hydrate in water (5.1) to give a final concentration equivalent to 50 mg/ml of the anhydrous form.

The D(+)-melezitose solution can be stored at 4 °C for no longer than 1 week.

5.3 α -Lactose monohydrate, $C_{12}H_{22}O_{11} \cdot H_2O$.

Before use, dry the α -lactose monohydrate at 70 °C for 4 h. Cool it to room temperature in a desiccator.

NOTE After drying, the lactose remains in the monohydrate form.

5.4 Biggs-Szijarto solution.

Dissolve 25 g of zinc acetate dihydrate, $Zn(CH_3COO)_2 \cdot 2H_2O$ and 12,5 g of phosphotungstic acid monohydrate ($W_{12}O_{36} \cdot H_3PO_4 \cdot H_2O$) in about 100 ml of HPLC grade water (5.1) in a 200 ml one-mark volumetric flask.

Add 20 ml of glacial acetic acid (CH_3COOH). Dilute to the 200 ml mark with HPLC grade water (5.1) and mix. After use, the solution may be stored at 4 °C for no longer than 1 week.

SAFETY PRECAUTIONS — Follow prevailing health and safety guidelines for the storage and handling of these chemicals.

6 Apparatus

Usual laboratory equipment and, in particular, the following.

6.1 HPLC ion exchange resin column, of length 300 mm, of internal diameter 7,8 mm, with 8 % cross-linked copolymer, based on polystyrene-divinylbenzene cation exchange resin, packed in the lead form.

6.2 Guard column.

In order to prolong ion exchange resin column life, replace the guard column after about 200 injections.

6.3 Micro-guard holder.

6.4 Column heater, capable of maintaining a constant temperature of $85 \text{ °C} \pm 1 \text{ °C}$.

6.5 HPLC pump, capable of maintaining a flow rate of between 0 ml/min and 10 ml/min.

6.6 HPLC autosampler.

NOTE Manual injection can also be used.

6.7 Differential refractometer detector, highly sensitive.

NOTE Other detectors, e.g. an evaporative light scattering detector, can also be used.

6.8 Software, capable of: automating injections, performing data acquisition, processing, and managing chromatographic information.

6.9 Water purification unit, capable of providing water complying with grade 1 requirements of ISO 3696, with a resistivity of between 10 M Ω -cm and 18 M Ω -cm.

6.10 Solvent filtration unit, including a vacuum source, with a membrane filter of 0,45 μ m pore size and of diameter 47 mm.

6.11 Analytical balance, capable of weighing to the nearest 1 mg, with a readability of 0,1 mg.

6.12 Water bath, capable of maintaining a temperature of between 38 °C and 40 °C.

6.13 Accurate dispenser, accurate automatic pipette, or one-mark pipettes conforming to the requirements of ISO 648, Class A, of capacity 2 ml.

6.14 Filter funnel, of diameter 75 mm.

6.15 Filter paper, of diameter 110 mm, Whatman¹⁾ No 1 or equivalent.

6.16 Nylon syringe filter, of porosity 0,45 μ m.

NOTE An in-line filter of the same porosity may also be used.

6.17 Syringe, with Luer-lock, of capacity 5 ml.

6.18 HPLC vials, with caps.

6.19 One-mark volumetric flasks, of capacity 10 ml \pm 0,02 ml.

NOTE Flasks with a capacity of more than 10 ml can also be used by taking into account the concentration factor.

7 Sampling

A representative sample should have been sent to the laboratory. It should not have been damaged or changed during transport or storage.

Sampling is not part of the method specified in this International Standard. A recommended sampling method is given in ISO 707|IDF 50.

8 Preparation of test sample

For fluid milk and cream, warm the test sample in the water bath (6.12) to between 38 °C and 40 °C. Gently mix the test sample by repeatedly inverting the bottle. Cool the sample quickly to 20 °C \pm 1 °C while gently mixing the sample immediately prior to weighing the test portion (9.2).

1) Whatman is an example of a suitable product available commercially. This information is given for the convenience of users of this International Standard and does not constitute an endorsement by ISO or by IDF of this product.

9 Procedure

9.1 Preparation of the standard solution

9.1.1 In a 10 ml one-mark volumetric flask (6.19), weigh, to the nearest 1 mg, the appropriate amount of α -lactose monohydrate (5.3) to give the equivalent of a 20 mg/ml anhydrous α -lactose solution.

9.1.2 Dissolve the α -lactose monohydrate (9.1.1) in about 5 ml of HPLC grade water (5.1). Add 2 ml of D(+)-melezitose solution (5.2), used as internal standard, to the flask. Make up to the mark with HPLC grade water (5.1) and mix by inverting the flask. Express the final α -lactose concentration in milligrams of the anhydrous form per millilitre.

9.1.3 Filter the standard solution through a pleated filter paper (6.15) using a filter funnel (6.14). Aspirate the filtrate into a syringe (6.17). Screw the nylon syringe filter (6.16) to the syringe and then transfer each filtrate into an HPLC vial (6.18). Inject each standard solution twice in accordance with the requirements of 9.4.2.

The standard solution thus prepared can provide three sets of calibration solutions. Use each set once only to calibrate the HPLC column. Store non-used sets of lactose standard solution at 4 °C for no longer than 1 week. Before use, bring all refrigerated standard solutions to approximately 20 °C.

In order to monitor the calibration, inject the standard solution as unknown sample at the beginning and at the end of the set of the test portions.

9.2 Preparation of test portion

9.2.1 Fluid milk test sample

Weigh, to the nearest 1 mg, about 3 ml of prepared test sample (see Clause 8) into a 10 ml one-mark volumetric flask (6.19). Proceed as in 9.3.

9.2.2 Milk powder test sample

Weigh, to the nearest 1 mg, about 0,300 g of test sample into a 10 ml one-mark volumetric flask (6.19). Add about 5 ml of HPLC grade water (5.1) pre-warmed to between 50 °C and 60 °C. Mix thoroughly until the solution becomes homogenous. Allow the test solution thus obtained to cool to 20 °C \pm 1 °C. Proceed as in 9.3.

9.2.3 Cream test sample

Weigh, to the nearest 1 mg, about 1 g of prepared test sample (see Clause 8) into a 10 ml one-mark volumetric flask (6.19). Proceed as in 9.3.

9.3 Preparation of filtrate

Add 2 ml of D(+)-melezitose internal standard solution (5.2) and 1,2 ml of Biggs-Szijarto solution (5.4) to the content of the flask obtained in accordance with the procedures of 9.2.1, 9.2.2 or 9.2.3, as appropriate. Dilute to the mark with HPLC grade water (5.1).

Gently mix the contents by inverting the flask five times. Allow to stand at room temperature for 10 min. Repeat the mixing and standing process two more times.

Filter the contents of the flask through a pleated filter paper (6.15) using a filter funnel (6.14). Collect the filtrate with a syringe (6.17). Screw the nylon syringe filter (6.16) to the syringe and then transfer the filtrate into a HPLC vial (6.18). Inject the test solution in accordance with the requirements of 9.4.2.

NOTE The filtration step through the filter paper can be replaced by centrifugation of the test sample.

9.4 HPLC determination

9.4.1 Preliminary preparation of HPLC

In order to get a stable baseline, turn on the detector (6.7) at least 24 h before starting the analysis. Set the internal temperature at 35 °C. Set the HPLC pump (6.5) to deliver a flow rate of 0,2 ml/min for at least 20 min while the column heater (6.4) is set to room temperature.

Increase the column heater temperature to 85 °C. When that temperature is reached, gradually increase the flow rate from 0,2 ml/min to 0,6 ml/min. Allow the system to equilibrate at a flow rate of 0,6 ml/min and at 85 °C for 2 h or until a stable baseline is obtained.

NOTE Checking and recording the pressure of the system from day to day can help to detect whether abnormal pressure changes occur.

9.4.2 Chromatographic conditions

The chromatographic conditions are as follows:

Condition	Details
Mobile phase	degassed HPLC grade water
Internal detector temperature	35 °C
Guard column temperature	ambient temperature
Column temperature	85 °C
Flow rate	0,6 ml/min
Volume to be injected	20 µl
Run time	15 min
Retention time of D(+)-melezitose	9 min ± 1 min
Retention time of lactose	11 min ± 1 min

Carefully choose the acquisition and integration parameters such as sensitivity, scale factor, time constant, peak width and threshold. See Figure 1 for an example of a chromatogram.

Measure the column efficiency, also called theoretical plate count, N , at least once per week. A decrease in N is related to the band spreading of the peak which is often due to a loss in column performance. Calculate N by using the following equation:

$$N = 5,54 \times \left(\frac{t_R}{w} \right)^2$$


where

t_R is the retention time, in minutes, of the lactose peak;

w is the width of the lactose peak, equivalent to time difference in minutes, at 50 % of its height.

When the theoretical plate count decreases by more than 25 % compared to the original measurement, a replacement of the column is recommended.

NOTE In most cases, a used column performing with low efficiency can be restored to its original form by back washing with an appropriate regenerating solvent described in the manufacturer's documentation.

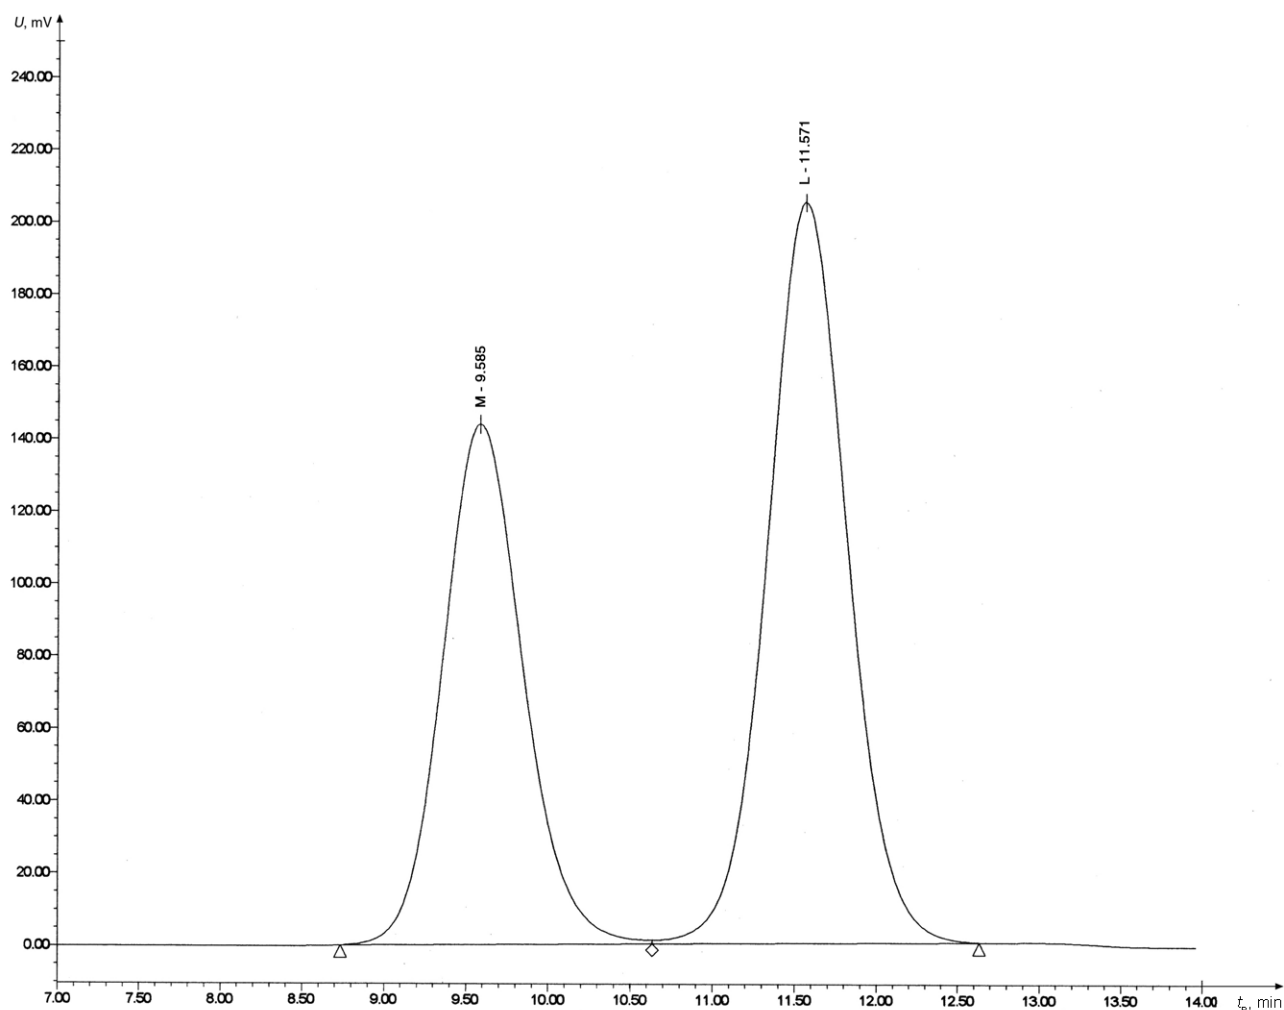

Key

- M D(+)-melezitose
- L α -lactose
- t_R retention time
- U potential difference

Figure 1 — Example of a chromatogram from a raw milk sample containing the internal standard

10 Calculation and expression of results

10.1 Calculation

A computer performs the calculations as follows:

First, the software (6.8) generates a curve by plotting the response ratio of the lactose standard peak area, A_S , to that of the internal standard, A_{IS} , multiplied by the internal standard concentration, c_{IS} , i.e. $(A_S/A_{IS}) \times c_{IS}$, against lactose concentration, c_l . The curve fit is linear through the origin.

To quantify an unknown test sample, the software divides the concentration derived from the calibration curve by the mass of the test sample to calculate the anhydrous lactose mass fraction expressed as a percentage.

10.2 Expression of results

Express the test results to three decimal places.

11 Precision

11.1 Interlaboratory test

Details of the interlaboratory test on the precision of the method are summarized in Annex A.

The values derived from this interlaboratory test may not be applicable to concentration ranges and matrices other than those given.

11.2 Repeatability

The absolute difference between two independent single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, will in not more than 5 % of cases be greater than:

- a) for fluid milk: 0,06 %;
- b) for cream: 0,06 %;
- c) for milk powder: 0,37 %.

11.3 Reproducibility

The absolute difference between two single test results, obtained using the same method on identical test material in different laboratories with different operators using different equipment, will in not more than 5 % of cases be greater than:

- a) for fluid milk: 0,13 %;
- b) for cream: 0,38 %;
- c) for milk powder: 2,94 %.

12 Test report

The test report shall specify:

- a) all the information required for the complete identification of the sample;
- b) the sample method used, if known;
- c) the method used, with reference to this International Standard;
- d) all operating details not specified in this International Standard, or regarded as optional, together with details of any incident which may have influenced the results;
- e) the test result(s) obtained and, if the repeatability has been checked, the final quoted result obtained.

Annex A (informative)

Results of interlaboratory test

An international collaborative test involving eight laboratories from five countries was carried out on 18 samples (six of fluid milk, six of cream and six of milk powder), all obtained from three dairy plants in Québec, Canada. The test was organized by the Programme des Analyses des Troupeaux Laitiers du Québec.

The results obtained were subjected to statistical analysis in accordance with ISO 5725-1 and ISO 5725-2 to give the precision data shown in Tables A.1 to A.3. All values expressed as percentages, except coefficients of variation, are mass fractions.

Table A.1 — Fluid milk results

	Test sample						Mean
	1	2	3	4	5	6	
No. of participating laboratories after eliminating outliers	8	8	7	8	7	8	
Mean lactose mass fraction, %	4,530	4,466	4,718	4,644	4,364	4,551	
Repeatability standard deviation, s_r, %	0,025	0,023	0,017	0,035	0,011	0,018	0,022
Repeatability limit, $r = 2,8s_r$, %	0,071	0,065	0,047	0,098	0,031	0,051	0,061
Coefficient of variation of repeatability, %	0,559	0,523	0,360	0,751	0,258	0,397	0,474
Reproducibility standard deviation, s_R, %	0,042	0,056	0,044	0,046	0,030	0,058	0,046
Reproducibility limit, $R = 2,8s_R$, %	0,118	0,156	0,123	0,128	0,085	0,162	0,129
Coefficient of variation of reproducibility, %	0,931	1,249	0,929	0,986	0,692	1,273	1,010

Table A.2 — Cream results

	Test sample						Mean
	1	2	3	4	5	6	
No. of participating laboratories after eliminating outliers	8	8	7	8	6	6	
Mean lactose mass fraction, %	1,461	3,822	3,686	2,886	3,256	3,103	
Repeatability standard deviation, s_r, %	0,030	0,015	0,025	0,032	0,009	0,007	0,020
Repeatability limit, $r = 2,8s_r$, %	0,084	0,041	0,069	0,090	0,026	0,020	0,055
Coefficient of variation of repeatability, %	2,066	0,381	0,672	1,117	0,283	0,224	0,790
Reproducibility standard deviation, s_R, %	0,171	0,108	0,136	0,118	0,134	0,136	0,134
Reproducibility limit, $R = 2,8s_R$, %	0,479	0,302	0,380	0,331	0,375	0,382	0,375
Coefficient of variation of reproducibility, %	11,721	2,824	3,686	4,090	4,113	4,397	5,139

Table A.3 — Milk powder results

	Test sample						Mean
	1	2	3	4	5	6	
No. of participating laboratories after eliminating outliers^a	6	7	7	6	6	7	
Mean lactose mass fraction, %	48,721	36,348	35,087	52,306	46,460	48,171	
Repeatability standard deviation, s_r, %	0,110	0,040	0,111	0,260	0,157	0,118	0,133
Repeatability limit, $r = 2,8s_r$, %	0,308	0,111	0,312	0,729	0,440	0,331	0,372
Coefficient of variation of repeatability, %	0,226	0,109	0,318	0,497	0,339	0,245	0,289
Reproducibility standard deviation, s_R, %	1,130	0,801	0,773	0,709	1,461	1,419	1,049
Reproducibility limit, $R = 2,8s_R$, %	3,165	2,241	2,1663	1,986	4,091	3,974	2,937
Coefficient of variation of reproducibility, %	2,322	2,202	2,202	1,356	3,145	2,946	2,362
^a Only seven laboratories provided results for the tests on milk powder.							

Bibliography

- [1] ISO 707|IDF 50, *Milk and milk products — Guidance on sampling*
- [2] ISO 5725-1, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions*
- [3] ISO 5725-2, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*
- [4] BIGGS D.A., SZIJARTO, L. Method for routine determination of lactose in milk, *J. Dairy Sci.* 1963, **46**, pp. 1196-200
- [5] HARVEY, J. A high performance liquid chromatography method for lactose determination in milk. *Austral. J. Dairy Technol.* 1988, **43**, pp. 19–20
- [6] BRONS, C., OLIEMAN, C. Study of the high-performance liquid chromatographic separation of reducing sugars, applied to the determination of lactose in milk. *J. Chromatogr.* 1983, **259**, pp. 79–86
- [7] KOOPS, J., OLIEMAN, C. Routine testing of farm milk with the Milko-Scan 203.3. Comparative evaluation of polarimetry, HPLC, enzymatic assay and reductometry for the determination of lactose. Calibration for infra-red analysis of lactose. Calculation of total solids from infra-red measurements, *Neth. Milk Dairy J.* 1985, **39**, pp. 89–106

1

ISO 22662:2007(E)
IDF 198:2007(E)

ICS 67.100.01

Price based on 10 pages